# **FCC SAR Test Report**

Product Name: Moticam X<sup>2</sup> Smart Camera

Model No. : Moticam X<sup>2</sup>

FCC ID : PVEMOTICAMX2

Applicant: Motic China Group Co., Ltd

Address: MOTIC BLDG, TORCH HI-TECH INDUSTRIAL DEV

**ZONE XIAMEN FUJIAN,361006,CN** 

Date of Receipt: Nov. 11, 2014

Date of Test : Nov. 11, 2014

Issued Date : Dec. 12, 2014

Report No. : 14B0296R-HP-US-P03V01

Report Version: V1.3



The test results relate only to the samples tested.

The test report shall not be reproduced except in full without the written approval of QuieTek Corporation.



# Test Report Certification

Issued Date: Dec. 12, 2014

Report No.: 14B0296R-HP-US-P03V01

# QuieTek

Product Name : Moticam X<sup>2</sup>Smart Camera

Applicant : Motic China Group Co., Ltd

: MOTIC BLDG, TORCH HI-TECH INDUSTRIAL DEV ZONE Address

XIAMEN FUJIAN,361006,CN

Manufacturer : Motic China Group Co., Ltd

: MOTIC BLDG, TORCH HI-TECH INDUSTRIAL DEV ZONE

Address XIAMEN FUJIAN,361006,CN

Model No. : Moticam X<sup>2</sup>

FCC ID : PVEMOTICAMX2

Brand Name : Motic

EUT Voltage : DC 5V

Applicable Standard : FCC KDB Publication 447498 D01v05r02

FCC KDB Publication 865664 D01v01r03 FCC KDB Publication 248227 D01v01r02

Test Result : Max. SAR Measurement (1g)

0.067 W/kg for Head; 0.128 W/kg for Body

Performed Location : Suzhou EMC Laboratory

No.99 Hongye Rd., Suzhou Industrial Park Loufeng Hi-Tech

Development Zone., Suzhou, China

TEL: +86-512-6251-5088 / FAX: +86-512-6251-5098

FCC Registration Number: 800392

Documented By : Alice Ni

Reviewed By : Drewn Cas

Approved By : Telf Chen



## **Laboratory Information**

We, **QuieTek Corporation**, are an independent EMC and safety consultancy that was established the whole facility in our laboratories. The test facility has been accredited/accepted(audited or listed) by the following related bodies in compliance with ISO 17025, EN 45001 and specified testing scope:

Taiwan R.O.C. : BSMI, NCC, TAF

**CNAS** 

Germany : TUV Rheinland

Norway : Nemko, DNV

USA : FCC Japan : VCCI

China

The related certificate for our laboratories about the test site and management system can be downloaded from QuieTek Corporation's Web Site: <a href="http://www.quietek.com/tw/ctg/cts/accreditations.htm">http://www.quietek.com/tw/ctg/cts/accreditations.htm</a>
The address and introduction of QuieTek Corporation's laboratories can be founded in our Web site:

The address and introduction of QuieTek Corporation's laboratories can be founded in our Web site: <a href="http://www.quietek.com/">http://www.quietek.com/</a>

If you have any comments, Please don't hesitate to contact us. Our contact information is as below:

#### **HsinChu Testing Laboratory:**

#### **LinKou Testing Laboratory:**

No.5-22, Ruishukeng, Linkou Dist., New Taipei City 24451, Taiwan, R.O.C.

#### Suzhou Testing Laboratory:

No.99 Hongye Rd., Suzhou Industrial Park Loufeng Hi-Tech Development Zone., SuZhou, China



## TABLE OF CONTENTS

Descrip	otion	Page
1. Ge	neral Information	7
1.1.	EUT Description	7
1.2.	Test Environment	8
1.3.	EUT Antenna Locations	8
1.4.	Simultaneous Transmission Configurations	9
1.5.	SAR Test Exclusions Applied	9
1.6.	Power Reduction for SAR	9
1.7.	Guidance Documents	9
2. SA	R Measurement System	10
2.1.	DASY5 System Description	10
2.1	.1. Applications	11
2.1	2. Area Scans	11
2.1	.3. Zoom Scan (Cube Scan Averaging)	11
2.1	.4. Uncertainty of Inter-/Extrapolation and Averaging	11
2.2.	DASY5 E-Field Probe	12
2.2	.1. Isotropic E-Field Probe Specification	12
2.3.	Boundary Detection Unit and Probe Mounting Device	13
2.4.	DATA Acquisition Electronics (DAE) and Measurement Server	13
2.5.	Robot	
2.6.	Light Beam Unit	
2.7.	Device Holder	
2.8.	SAM Twin Phantom	15
3. Tis	sue Simulating Liquid	16
3.1.	The composition of the tissue simulating liquid	16
3.2.	Tissue Calibration Result	16
3.3.	Tissue Dielectric Parameters for Head and Body Phantoms	17
4. SA	R Measurement Procedure	18
4.1.	SAR System Validation	18
4.1	.1. Validation Dipoles	18
4.1	2. Validation Result	19
4.2.	SAR Measurement Procedure	20
5. SA	R Exposure Limits	21



6.	Test Equipment List	22
7.	Measurement Uncertainty	23
8.	Conducted Power Measurement	25
9.	Test Results	26
9	9.1. Test Results	26
9	9.2. SAR Test Notes	27
Αp	pendix A. SAR System Validation Data	28
Ap	pendix B. SAR measurement Data	30
Αp	pendix C. Test Setup Photographs & EUT Photographs	36
Αp	pendix D. Probe Calibration Data	45
Αp	pendix E. Dipole Calibration Data	56
Ap	pendix F. DAE Calibration Data	64



**History of This Test Report** 

REPORT NO.	VERSION	DESCRIPTION	ISSUED DATE
14B0296R-HP-US-P03V01	V1.0	Initial Issued Report	Nov. 18, 2014
14B0296R-HP-US-P03V01	V1.1	Modified the power and some mistakes of the report.	Nov. 27, 2014
14B0296R-HP-US-P03V01	V1.2	Modified the power and some mistakes of the report.	Dec. 04, 2014
14B0296R-HP-US-P03V01	V1.3	Added the test photos for head	Dec. 12, 2014



## 1. General Information

## 1.1. EUT Description

Product Name	Moticam X <sup>2</sup> Smart Camera
Model No.	Moticam X <sup>2</sup>
Product Category	prototype
Device Category	Mobile
Wi-Fi	
Wi Fi Fraguency	802.11b/g/n(20): 2412 ~ 2462 MHz
Wi-Fi Frequency	802.11n(40): 2422~2452 MHz
Type of modulation	802.11b: DSSS; 802.11g/n: OFDM
	802.11b: 11 Mbps
Data Rate	802.11g/n(20): 54 Mbps
	802.11n(40): up to 150 Mbps
Antenna Gain	2.5dBi

Note: The device should be fixed on a microscope during the normal operation. Though it is a mobile device, but people would be very close to the microscope, in other words, the WIFI camera, so we still test it as a portable device according to KDB 447498 D01v05r02.





## 1.2. Test Environment

Ambient conditions in the laboratory:

Items	Required	Actual
Temperature (°C)	18-25	21.5± 2
Humidity (%RH)	30-70	52

## 1.3. EUT Antenna Locations



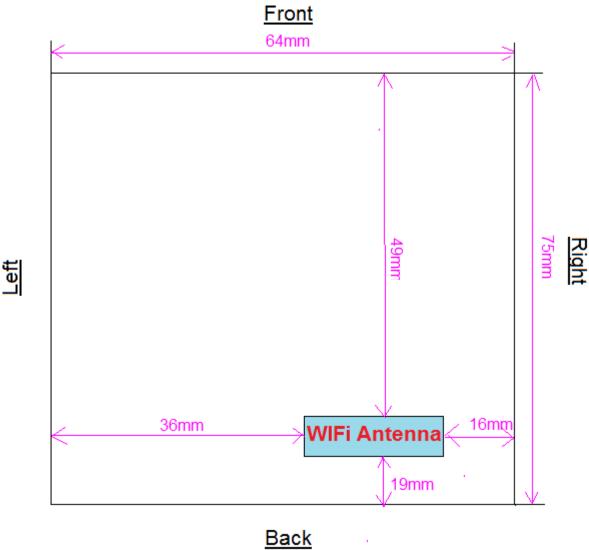



## 1.4. Simultaneous Transmission Configurations

There is only one antenna, so simultaneous transmission is not available.

## 1.5. SAR Test Exclusions Applied

Wi-Fi

Per FCC KDB 447498 D05v01r02, the SAR exclusion threshold for distances<50mm is defined by the following equation:

$$\frac{Max\ Power\ of\ Channel\ (mW)}{Test\ Separation\ Dist\ (mm)}*\sqrt{Frequency(GHz)} \leq 3.0$$

Based on the maximum power of WIFI, the test exclution distance should be:

Exclusion distance >  $(63.10 \text{mW} * \sqrt{2.437}) / 3=32.83 \text{mm}$ , so the distance between the antenna to the edge which is over 32.83 mm can meet the SAR exclution refer to KDB 447498 D01v05r02

#### 1.6. Power Reduction for SAR

There is no power reduction used for any band/mode implemented in this device for SAR purposes.


#### 1.7. Guidance Documents

- 1) FCC KDB Publication 447498 D01v05r02 (General SAR Guidance)
- 2) FCC KDB Publication 865664 D01v01r03(SAR measurement 100 MHz to 6 GHz)
- 3) FCC KDB Publication 248227 D01v01r02 (SAR Considerations for 802.11 Devices)



## 2. SAR Measurement System

## 2.1. DASY5 System Description

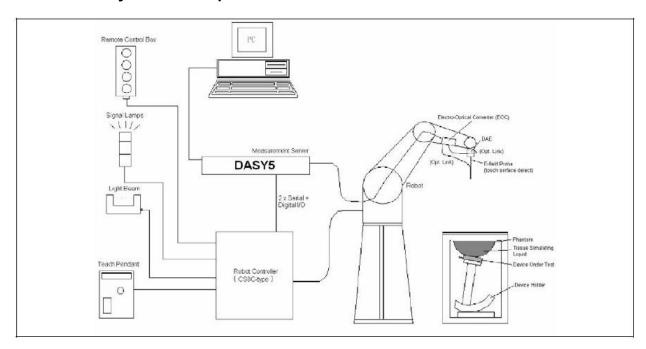

The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running WinXP and the DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.



## 2.1.1. Applications

Predefined procedures and evaluations for automated compliance testing with all worldwide standards, e.g., IEEE 1528, OET 65, IEC 62209-1, IEC 62209-2, EN 50360, EN 50383 and others.

#### 2.1.2. Area Scans

Area scans are defined prior to the measurement process being executed with a user defined variable spacing between each measurement point (integral) allowing low uncertainty measurements to be conducted. Scans defined for FCC applications utilize a 10mm<sup>2</sup> step integral, with 1mm interpolation used to locate the peak SAR area used for zoom scan assessments.

When an Area Scan has measured all reachable points, it computes the field maxima found in the scanned area, within a range of the global maximum. The range (in dB) is specified in the standards for compliance testing. For example, a 2 dB range is required in IEEE 1528-2003 and IEC 62209 standards, whereby 3 dB is a requirement when compliance is assessed in accordance with the ARIB standard (Japan).

## 2.1.3. Zoom Scan (Cube Scan Averaging)

Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. A density of 1000 kg/m³ is used to represent the head and body tissue density and not the phantom liquid density, in order to be consistent with the definition of the liquid dielectric properties, i.e. the side length of the 1 g cube is 10mm, with the side length of the 10 g cube 21,5mm.

The zoom scan integer steps can be user defined so as to reduce uncertainty, but normal practice for typical test applications utilize a physical step of 7x7x7 (5mmx5mmx5mm) providing a volume of 30mm in the X & Y axis, and 30mm in the Z axis.

## 2.1.4. Uncertainty of Inter-/Extrapolation and Averaging

In order to evaluate the uncertainty of the interpolation, extrapolation and averaged SAR calculation algorithms of the Postprocessor, DASY5 allows the generation of measurement grids which are artificially predefined by analytically based test functions. Therefore, the grids of area scans and zoom scans can be filled with uncertainty test data, according to the SAR benchmark functions of IEEE 1528. The three analytical functions shown in equations as below are used to describe the possible range of the expected SAR distributions for the tested handsets. The field gradients are covered by the spatially flat distribution f1, the spatially steep distribution f3 and f2 accounts for H-field cancellation on the phantom/tissue surface.

Page: 11 of 68



$$f_1(x, y, z) = Ae^{-\frac{z}{2a}}\cos^2\left(\frac{\pi}{2}\frac{\sqrt{x'^2 + y'^2}}{5a}\right)$$

$$f_2(x, y, z) = Ae^{-\frac{z}{a}}\frac{a^2}{a^2 + x'^2}\left(3 - e^{-\frac{2z}{a}}\right)\cos^2\left(\frac{\pi}{2}\frac{y'}{3a}\right)$$

$$f_3(x, y, z) = A\frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2}\left(e^{-\frac{2z}{a}} + \frac{a^2}{2(a+2z)^2}\right)$$

#### 2.2. DASY5 E-Field Probe

The SAR measurement is conducted with the dosimetric probe manufactured by SPEAG. The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency.

SPEAG conducts the probe calibration in compliance with international and national standards (e.g. IEEE 1528, EN 62209-1, IEC 62209, etc.) under ISO 17025. The calibration data are in Appendix D.

## 2.2.1. Isotropic E-Field Probe Specification

Model	EX3DV4		
Construction	Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g.,		
	DGBE)		
Frequency	10 MHz to 6 GHz		
	Linearity: ± 0.2 dB (30 MHz to 6 GHz)		
Directivity	± 0.3 dB in HSL (rotation around probe axis)		
	± 0.5 dB in tissue material (rotation normal to		
	probe axis)		
Dynamic Range	10 μW/g to 100 mW/g		
	Linearity: ± 0.2 dB (noise: typically < 1 μW/g)		
Dimensions	Overall length: 330 mm (Tip: 20 mm)		
	Tip diameter: 2.5 mm (Body: 12 mm)		
	Typical distance from probe tip to dipole centers:		
	1 mm		
Application	High precision dosimetric measurements in any exposure scenario		
	(e.g., very strong gradient fields). Only probe which enables		
	compliance testing for frequencies up to 6 GHz with precision of better		
	30%.		



## 2.3. Boundary Detection Unit and Probe Mounting Device

The DASY probes use a precise connector and an additional holder for the probe, consisting of a plastic tube and a flexible silicon ring to center the probe. The connector at the DAE is flexibly mounted and held in the default position with magnets and springs. Two switching systems in the connector mount detect frontal and lateral probe collisions and trigger the necessary software response.



## 2.4. DATA Acquisition Electronics (DAE) and Measurement Server

The data acquisition electronics (DAE) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit.

Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.



The DASY5 measurement server is based on a PC/104 CPU board with a 400MHz intel ULV Celeron, 128MB chipdisk and 128MB RAM. The necessary circuits for communication with the DAE electronics box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY5 I/O board, which is directly connected to the PC/104 bus of the CPU board.





#### 2.5. Robot

The DASY5 system uses the high precision robots TX90 XL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY5 system, the CS8C robot controller version from Stäubli is used.

The XL robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ➢ 6-axis controller



#### 2.6. Light Beam Unit

The light beam switch allows automatic "tooling" of the probe. During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, such that the robot coordinates are valid for the probe tip.

The repeatability of this process is better than 0.1 mm. If a position has been taught with an aligned probe, the same position will be reached with another aligned probe within 0.1 mm, even if the other probe has different dimensions. During probe rotations, the probe tip will keep its actual position.





#### 2.7. Device Holder

The DASY5 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY5 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity  $\epsilon r = 3$  and loss tangent  $\delta = 0.02$ . The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



#### 2.8. SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- Left head
- Right head
- Flat phantom



The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.



## 3. Tissue Simulating Liquid

## 3.1. The composition of the tissue simulating liquid

INGREDIENT	2450MHz	2450MHz
(% Weight)	Head	Body
Water	46.7	73.2
Salt	0.00	0.04
Sugar	0.00	0.00
HEC	0.00	0.00
Preventol	0.00	0.00
DGBE	53.3	26.7
Triton X-100	0.00	0.00

## 3.2. Tissue Calibration Result

The dielectric parameters of the liquids were verified prior to the SAR evaluation using DASY5 Dielectric Probe Kit and Agilent Vector Network Analyzer E5071C

Head Tissue Simulant Measurement							
Frequency	ncy Dielectric Parameters		Tissue Temp.				
[MHz]	Description	ε <sub>r</sub>	σ [s/m]	[°C]			
	Reference result	39.20	1.80	N/A			
2450MHz	± 5% window	37.24 to 41.16	1.62 to 1.98	IN/A			
	11-11-2014	39.24	1.82	21.0			
	Reference result	39.22	1.79	N/A			
2437MHz	± 5% window	37.26 to 41.18	1.70 to 1.88	IN/A			
	11-11-2014	39.30	1.80	21.0			

## **Body Tissue Simulant Measurement**

Frequency	Description	Dielectric Pa	Tissue Temp.	
[MHz]	Description	ε <sub>r</sub>	σ [s/m]	[°C]
2450MHz	Reference result ± 5% window	52.7 50.07 to 55.34	1.95 1.85 to 2.05	N/A
	11-11-2014	51.24	1.96	21.0
2437MHz	Reference result ± 5% window	52.72 50.08 to 55.35	1.94 1.84 to 2.03	N/A
	11-11-2014	51.31	1.94	21.0

Page: 16 of 68



## 3.3. Tissue Dielectric Parameters for Head and Body Phantoms

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in P1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations described in Reference [12] and extrapolated according to the head parameters specified in P1528.

Target Frequency	Head		Во	dy
(MHz)	€ <sub>r</sub>	σ (S/m)	$\epsilon_{r}$	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800 – 2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00


( $\varepsilon_r$  = relative permittivity,  $\sigma$  = conductivity and  $\rho$  = 1000 kg/m³)



## 4. SAR Measurement Procedure

## 4.1. SAR System Validation

## 4.1.1. Validation Dipoles



The dipoles used is based on the IEEE-1528 standard, and is complied with mechanical and electrical specifications in line with the requirements of both IEEE and FCC Supplement C. the table below provides details for the mechanical and electrical specifications for the dipoles.

Frequency	L (mm)	h (mm)	d (mm)
2450MHz	53.5	30.4	3.6



## 4.1.2. Validation Result

## System Performance Check at 2450MHz for Head

Validation Dipole: D2450V2-SN 839

Frequency [MHz]	Description	SAR [w/kg] 1g	SAR [w/kg] 10g	Tissue Temp. [°C]
2450 MHz	Reference result ± 10% window	52.0 46.8 to 57.2	24.3 21.87 to 26.73	N/A
	11-11-2014	55.20	24.96	21.0

Note: All SAR values are normalized to 1W forward power.

## System Performance Check at 2450MHz for Body

Validation Dipole: D2450V2, SN: 839

Frequency [MHz]	Description	SAR [w/kg] 1g	SAR [w/kg] 10g	Tissue Temp. [°C]
2450 MHz	Reference result ± 10% window	49.9 44.91 to 54.89	23.1 20.79 to 25.41	N/A
	11-11-2014	49.20	22.28	21.0

Note: All SAR values are normalized to 1W forward power.



#### 4.2. SAR Measurement Procedure

The DASY5 calculates SAR using the following equation,

$$SAR = \frac{\sigma |E|^2}{\rho}$$

σ: represents the simulated tissue conductivity

p: represents the tissue density

The EUT is set to transmit at the required power in line with product specification, at each frequency relating to the LOW, Tablet PC, and HIGH channel settings.

Pre-scans are made on the device to establish the location for the transmitting antenna, using a large area scan in either air or tissue simulation fluid.

The EUT is placed against the Universal Phantom where the maximum area scan dimensions are larger than the physical size of the resonating antenna. When the scan size is not large enough to cover the peak SAR distribution, it is modified by either extending the area scan size in both the X and Y directions, or the device is shifted within the predefined area.

The area scan is then run to establish the peak SAR location (interpolated resolution set at 1mm<sup>2</sup>) which is then used to orient the center of the zoom scan. The zoom scan is then executed and the 1g and 10g averages are derived from the zoom scan volume (interpolated resolution set at 1mm<sup>3</sup>).



## 5. SAR Exposure Limits

SAR assessments have been made in line with the requirements of IEEE-1528, FCC Supplement C, and comply with ANSI/IEEE C95.1-1992 "Uncontrolled Environments" limits. These limits apply to a location which is deemed as "Uncontrolled Environment" which can be described as a situation where the general public may be exposed to an RF source with no prior knowledge or control over their exposure.

## Limits for General Population/Uncontrolled Exposure (W/kg)

Type Exposure	Uncontrolled
	Environment Limit
Spatial Peak SAR (1g cube tissue for brain or body)	1.60 W/kg
Spatial Average SAR (whole body)	0.08 W/kg
Spatial Peak SAR (10g for hands, feet, ankles and wrist)	4.00 W/kg



# 6. Test Equipment List

Instrument	Manufacturer	Model No.	Serial No.	Cali. Due Date
Stäubli Robot TX60L	Stäubli	TX60L	F10/5C90A1/A/01	N/A
Controller	Stäubli	SP1	S-0034	N/A
Dipole Validation Kits	Speag	D2450V2	839	2016.02.24
SAM Twin Phantom	Speag	SAM	TP-1561/1562	N/A
Device Holder	Speag	SD 000 H01 HA	N/A	N/A
Data	Speag	DAE4	1220	2015.01.21
Acquisition Electronic				
E-Field Probe	Speag	EX3DV4	3710	2015.03.03
SAR Software	Speag	DASY5	V5.2 Build 162	N/A
Power Amplifier	Mini-Circuit	ZVA-183-S+	N657400950	N/A
Directional Coupler	Agilent	778D	20160	N/A
Universal Radio	R&S	CMU 200	117088	2015.03.28
Communication Tester				
Vector Network	Agilent	E5071C	MY48367267	2015.03.28
Signal Generator	Agilent	E4438C	MY49070163	2015.03.28
Power Meter	Anritsu	ML2495A	0905006	2015.11.01
Wide Bandwidth	Anritsu	MA2411B	0846014	2015.11.01
Sensor				



# 7. Measurement Uncertainty

		DASY	5 Und	ertair	ity			
Measurement uncertainty	for 300 M	Hz to 3 (	GHz aver	aged ove	er 1 gram	/ 10 gram.		
Error Description	Uncert.	Prob.	Div.	(Ci)	(Ci)	Std.	Std.	(Vi)
	value	Dist.		1g	10g	Unc.	Unc.	Veff
						(1g)	(10g)	
Measurement System		-						
Probe Calibration	±6.0%	N	1	1	1	±6.0%	±6.0%	∞
Axial Isotropy	±4.7%	R	√3	0.7	0.7	±1.9%	±1.9%	∞
Hemispherical Isotropy	±9.6%	R	√3	0.7	0.7	±3.9%	±3.9%	∞
Boundary Effects	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Linearity	±4.7%	R	√3	1	1	±2.7%	±2.7%	8
System Detection Limits	±1.0%	R	√3	1	1	±0.6%	±0.6%	∞
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%	∞
Response Time	±0.8%	R	√3	1	1	±0.5%	±0.5%	8
Integration Time	±2.6%	R	√3	1	1	±1.5%	±1.5%	8
RF Ambient Noise	±3.0%	R	√3	1	1	±1.7%	±1.7%	∞
RF Ambient Reflections	±3.0%	R	√3	1	1	±1.7%	±1.7%	8
Probe Positioner	±0.4%	R	√3	1	1	±0.2%	±0.2%	8
Probe Positioning	±2.9%	R	√3	1	1	±1.7%	±1.7%	∞
Max. SAR Eval.	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	8
Test Sample Related								
Device Positioning	±2.9%	N	1	1	1	±2.9%	±2.9%	145
Device Holder	±3.6%	N	1	1	1	±3.6%	±3.6%	5
Power Drift	±5.0%	R	√3	1	1	±2.9%	±2.9%	8
Phantom and Setup				·				
Phantom Uncertainty	±4.0%	R	√3	1	1	±2.3%	±2.3%	8
Liquid Conductivity	LE 00/	В	/2	0.64	0.42	±1.8%	14.20/	
(target)	±5.0%	R	√3	0.64	0.43	±1.0%	±1.2%	∞
Liquid Conductivity	±2.5%	N	1	0.64	0.43	±1.6%	±1.1%	∞
(meas.)	12.5 /6	IN	l	0.04	0.43	±1.0 /0	±1.170	~
Liquid Permittivity	±5.0%	R	√3	0.6	0.49	±1.7%	±1.4%	∞
(target)	±0.0 /0	1	γJ	0.0	0.70	±1.7 /0	±1.₹/0	
Liquid Permittivity	±2.5%	N	1	0.6	0.49	±1.5%	±1.2%	∞
(meas.)	070	.,	'	0.0	0.40	21.070	±1.270	
Combined Std. Uncertain	inty					±11.0%	±10.8%	387
Expanded STD Uncertain	inty					±22.0%	±21.5%	

Page: 23 of 68



		DASY	5 Unc	ertain	ty			
Measurement uncertainty	for 3 GHz	to 6 GH	z average	ed over 1	gram / 10	0 gram.		
Error Description	Uncert.	Prob.	Div.	(Ci)	(Ci)	Std.	Std.	(Vi)
	value	Dist.		1g	10g	Unc.	Unc.	<b>V</b> eff
						(1g)	(10g)	
Measurement System								
Probe Calibration	±6.55%	N	1	1	1	±6.55%	±6.55%	∞
Axial Isotropy	±4.7%	R	√3	0.7	0.7	±1.9%	±1.9%	∞
Hemispherical Isotropy	±9.6%	R	√3	0.7	0.7	±3.9%	±3.9%	∞
Boundary Effects	±2.0%	R	√3	1	1	±1.2%	±1.2%	∞
Linearity	±4.7%	R	√3	1	1	±2.7%	±2.7%	∞
System Detection Limits	±1.0%	R	√3	1	1	±0.6%	±0.6%	∞
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%	∞
Response Time	±0.8%	R	√3	1	1	±0.5%	±0.5%	∞
Integration Time	±2.6%	R	√3	1	1	±1.5%	±1.5%	∞
RF Ambient Noise	±3.0%	R	√3	1	1	±1.7%	±1.7%	∞
RF Ambient Reflections	±3.0%	R	√3	1	1	±1.7%	±1.7%	∞
Probe Positioner	±0.8%	R	√3	1	1	±0.5%	±0.5%	∞
Probe Positioning	±9.9%	R	√3	1	1	±5.7%	±5.7%	∞
Max. SAR Eval.	±4.0%	R	√3	1	1	±2.3%	±2.3%	∞
Test Sample Related			•			1		
Device Positioning	±2.9%	N	1	1	1	±2.9%	±2.9%	145
Device Holder	±3.6%	N	1	1	1	±3.6%	±3.6%	5
Power Drift	±5.0%	R	√3	1	1	±2.9%	±2.9%	∞
Phantom and Setup		i.				1		
Phantom Uncertainty	±4.0%	R	√3	1	1	±2.3%	±2.3%	∞
Liquid Conductivity	. 5.00/	Б	lo.	0.04	0.40	.4.00/	.4.00/	
(target)	±5.0%	R	√3	0.64	0.43	±1.8%	±1.2%	∞
Liquid Conductivity	10.50/	N	4	0.64	0.42	14.60/	.4.40/	
(meas.)	±2.5%	N	1	0.64	0.43	±1.6%	±1.1%	∞
Liquid Permittivity	±5.0%	R	√3	0.6	0.49	±1.7%	±1.4%	8
(target)	10.0 /0	13	γu	0.0	0.48	±1.7 /0	⊥1.→/0	
Liquid Permittivity	±2.5%	N	1	0.6	0.49	±1.5%	±1.2%	∞
(meas.)	0 /0		•	0.0	J10	±1.070	±1.2/0	
Combined Std. Uncerta	inty					±12.8%	±12.6%	330
Expanded STD Uncertain	inty					±25.6%	±25.2%	



## 8. Conducted Power Measurement

## WLAN output power

Test Mode	Channel No.	Frequency (MHz)	Average Power (dBm)	Max. Average Power (dBm)	Scaling Factor
	01	2412	17.36	18.0	1.159
802.11b	06	2437	17.46	18.0	1.132
	11	2462	17.12	18.0	1.225
	01	2412	16.53	17.0	1.114
802.11g	06	2437	16.83	17.0	1.040
	11	2462	16.79	17.0	1.050
	01	2412	15.16	16.0	1.213
802.11n (20MHz)	06	2437	15.64	16.0	1.086
	11	2462	15.23	16.0	1.194
	03	2422	15.34	16.0	1.164
802.11n (40MHz)	06	2437	15.74	16.0	1.062
	09	2452	15.66	16.0	1.081

Note 1: Justification for reduced test configurations for Wi-Fi channels per KDB Publication 248227 D01v01r02.

2: For 2.4 GHz, highest average RF output power channel for the lowest data rate for IEEE 802.11b were selected for SAR evaluation. Other IEEE 802.11 modes (including 802.11g/n) were not investigated since the average output powers over all channels and data rates were not more than 0.25 dB higher than the tested channel in the lowest data rate of IEEE 802.11b mode.

3: When the maximum extrapolated peak SAR of the zoom scan for the maximum output channel is <1.6 W/kg and the reported 1g averaged SAR is <0.8 W/kg, SAR testing on other channels is not required. Otherwise, the other default (or corresponding required) test channels were additionally tested using the lowest data rate.



## 9. Test Results

## 9.1. Test Results

SAR MEASUREMENT	
Ambient Temperature (°C): 21.5 ± 2	Relative Humidity (%): 52
Liquid Temperature (°C) : 21.0 ± 2	Depth of Liquid (cm):>15
Description Matter and VO Occupation	

Product: Moticam X2 Smart Camera

Test Mode: 802.11b for Head

Test Position	Antenna	Frequency		Frame	Power	SAR 1g	Scaling	Scaled	Limit
Body at 0mm	Position	Channel	MHz	Power (dBm)	Drift (<±0.2)	(W/kg)	Factor	SAR 1g (W/kg)	(W/kg)
Back	Fixed	01	2412	17.36			1.159		1.6
Back	Fixed	06	2437	17.46	0.01	0.046	1.132	0.052	1.6
Back	Fixed	11	2462	17.12		1	1.225		1.6
Right	Fixed	06	2437	17.46	0.02	0.059	1.132	0.067	1.6
Bottom	Fixed	06	2437	17.46	0.10	0.035	1.132	0.040	1.6

Note: when the 1-g SAR is ≤ 0.8 W/kg, testing for low and high channel is optional, refer to KDB 447498.

SAR MEASUREMENT	
Ambient Temperature (°C): 21.5 ± 2	Relative Humidity (%): 52
Liquid Temperature (°C): 21.0 ± 2	Depth of Liquid (cm):>15
Product: Moticam X2 Smart Camera	

Test Mode: 802.11b for Body

Test Position	Antenna	Frequency		Frame	Power	SAR 1g	Scaling	Scaled	Limit
Body at 0mm	Position	Channel	MHz	Power	Drift	(W/kg)	Factor	SAR 1g	(W/kg)
Body at onim	1 0010011	Chamile	IVII IZ	(dBm)	(<±0.2)	(VV/Ng)	1 40101	(W/kg)	(VV/Ng)
Back	Fixed	01	2412	17.36		-	1.159		1.6
Back	Fixed	06	2437	17.46	-0.17	0.099	1.132	0.112	1.6
Back	Fixed	11	2462	17.12		1	1.225		1.6
Right	Fixed	06	2437	17.46	-0.09	0.113	1.132	0.128	1.6
Bottom	Fixed	06	2437	17.46	-0.18	0.056	1.132	0.063	1.6

Note: when the 1-g SAR is  $\leq$  0.8 W/kg, testing for low and high channel is optional, refer to KDB 447498.



#### 9.2. SAR Test Notes

#### General Notes:

- 1. Batteries are fully charged at the beginning of the SAR measurements.
- 2. Liquid tissue depth was at least 15.0 cm for all frequencies.
- 3. The manufacturer has confirmed that the device(s) tested have the same physical, mechanical and thermal characteristics and are within operational tolerances expected for production units.
- 4. SAR results were scaled to the maximum allowed power to demonstrate compliance per FCC KDB Publication 447498 D01v05r02.
- 5. Head SAR was also tested at body phantom with a test distance of 0mm for back, right side and bottom sides according to the exclusion guidance of KDB 447498D01v05r02.

#### WLAN Notes:

- 1. Justification for reduced test configurations for Wi-Fi channels per KDB Publication 248227 D01v01r02 and April 2010 FCC/TCB Meeting Notes for 2.4 GHz Wi-Fi: Highest average RF output power channel for the lowest data rate was selected for SAR evaluation in 802.11b. Other IEEE 802.11 modes (including 802.11g/n) were not investigated since the average output powers over all channels and data rates were not more than 0.25 dB higher than the tested channel in the lowest data rate of IEEE 802.11b mode.
- 2. When the maximum extrapolated peak SAR of the zoom scan for the maximum output channel is <1.6 W/kg and the reported 1g averaged SAR is <0.8 W/kg, SAR testing on other default channels is not required.



## Appendix A. SAR System Validation Data

Date/Time: 11-11-2014

Test Laboratory: QuieTek Lab System Check Head 2450MHz

DUT: Dipole 2450 MHz D2450V2; Type: D2450V2


Communication System: UID 0, CW; Communication System Band: Exported from older format (data unavailable - please correct).; Duty Cycle: 1:1; Frequency: 2450 MHz; Medium parameters used: f = 2450 MHz;  $\sigma$  = 1.82 S/m;  $\epsilon$ r = 39.24;  $\rho$  = 1000 kg/m3; Phantom section: Flat Section; Input Power=250mW Ambient temperature (°C): 21.5, Liquid temperature (°C): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(7.04, 7.04, 7.04); Calibrated: 04/03/2014;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 22/01/2014
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Configuration/Head 2450MHz/Area Scan (6x10x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 14.2 W/kg

Configuration/Head 2450MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm, Reference Value = 90.828 V/m; Power Drift = 0.12 dB
Peak SAR (extrapolated) = 29.8 W/kg

**SAR(1 g) = 13.8 W/kg; SAR(10 g) = 6.24 W/kg** Maximum value of SAR (measured) = 15.7 W/kg

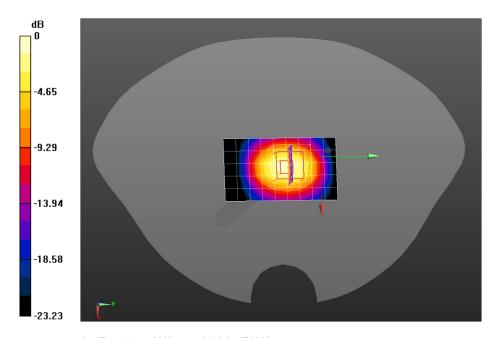

0 dB = 15.7 W/kg = 11.96 dBW/kg



Date/Time: 11-11-2014

Test Laboratory: QuieTek Lab System Check Body 2450MHz

#### DUT: Dipole 2450 MHz D2450V2; Type: D2450V2

Communication System: UID 0, CW; Communication System Band: D2450(2450MHz); Duty Cycle: 1:1;

Frequency: 2450 MHz; Medium parameters used: f = 2450 MHz;  $\sigma = 1.96$  S/m;  $\epsilon r = 51.24$ ;  $\rho = 1000$  kg/m3;

Phantom section: Flat Section; Input Power=250mW

Ambient temperature ( $^{\circ}$ ): 21.5, Liquid temperature ( $^{\circ}$ ): 21.0


DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(6.88, 6.88, 6.88); Calibrated: 04/03/2014;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 22/01/2014
- Phantom: SAM2; Type: SAM; Serial: TP1562
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Configuration/System Check Body 2450MHz/Area Scan (7x11x1): Measurement grid: dx=10mm, dy=10mm, Maximum value of SAR (measured) = 13.2 W/kg

Configuration/System Check Body 2450MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm, Reference Value = 82.154 V/m; Power Drift = 0.04 dB
Peak SAR (extrapolated) = 25.9 W/kg

SAR(1 g) = 12.3 W/kg; SAR(10 g) = 5.57 W/kg Maximum value of SAR (measured) = 14.1 W/kg

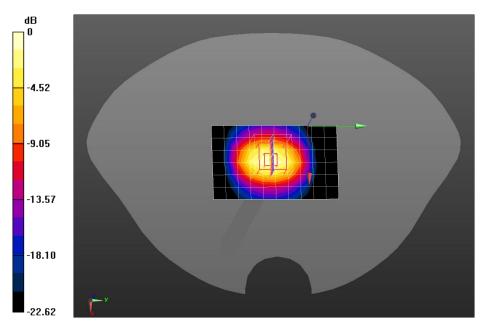

0 dB = 14.1 W/kg = 11.49 dBW/kg



## Appendix B. SAR measurement Data

SAR for Head

Date/Time: 11-11-2014

Test Laboratory: QuieTek Lab 802.11b 2437MHz Back

**DUT: Moticam X2 Smart Camera; Type: Moticam X2** 

Communication System: UID 0, Wi-Fi (0); Communication System Band: 802.11b; Duty Cycle: 1:1.0;

Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz;  $\sigma = 1.8$  S/m;  $\epsilon r = 39.3$ ;  $\rho = 1000$  kg/m3;

Phantom section: Flat Section

Ambient temperature ( $^{\circ}$ C): 21.5, Liquid temperature ( $^{\circ}$ C): 21.0

DASY5 Configuration:

Probe: EX3DV4 - SN3710; ConvF(7.04, 7.04, 7.04); Calibrated: 04/03/2014;

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1220; Calibrated: 22/01/2014

Phantom: SAM2; Type: SAM; Serial: TP1562


Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Configuration/802.11b 2437MHz Back/Area Scan (7x9x1): Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.0407 W/kg

Configuration/802.11b 2437MHz Back/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 2.906 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 0.132 W/kg

SAR(1 g) = 0.046 W/kg; SAR(10 g) = 0.026 W/kg Maximum value of SAR (measured) = 0.0450 W/kg

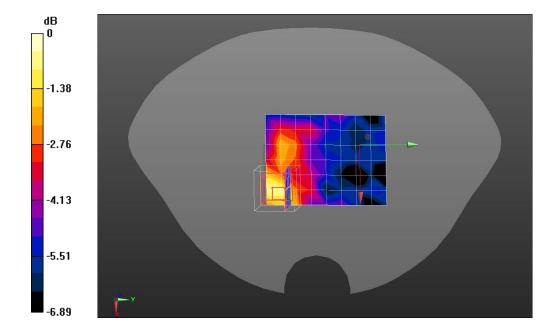

Page: 30 of 68



0 dB = 0.0450 W/kg = -13.47 dBW/kg



Date/Time: 11-11-2014

Test Laboratory: QuieTek Lab 802.11b 2437MHz Right side

DUT: Moticam X2 Smart Camera; Type: Moticam X2

Communication System: UID 0, Wi-Fi (0); Communication System Band: 802.11b; Duty Cycle: 1:1.0;

Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz;  $\sigma = 1.8$  S/m;  $\epsilon r = 39.3$ ;  $\rho = 1000$  kg/m3;

Phantom section: Flat Section

Ambient temperature ( $^{\circ}$ ): 21.5, Liquid temperature ( $^{\circ}$ ): 21.0


DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(7.04, 7.04, 7.04); Calibrated: 04/03/2014;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 22/01/2014
- Phantom: SAM2; Type: SAM; Serial: TP1562
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Configuration/802.11b 2437MHz Back/Area Scan (7x9x1): Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.0493 W/kg

Configuration/802.11b 2437MHz Back/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 2.889 V/m; Power Drift = 0.02 dB
Peak SAR (extrapolated) = 0.150 W/kg

SAR(1 g) = 0.059 W/kg; SAR(10 g) = 0.032 W/kg Maximum value of SAR (measured) = 0.0624 W/kg

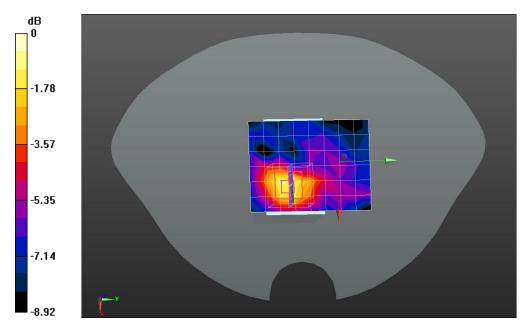

0 dB = 0.0624 W/kg = -12.05 dBW/kg



Date/Time: 11-11-2014

Test Laboratory: QuieTek Lab 802.11b 2437MHz Bottom

#### DUT: Moticam X2 Smart Camera; Type: Moticam X2

Communication System: UID 0, Wi-Fi (0); Communication System Band: 802.11b; Duty Cycle: 1:1.0;

Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz;  $\sigma = 1.8$  S/m;  $\epsilon r = 39.3$ ;  $\rho = 1000$  kg/m3;

Phantom section: Flat Section

Ambient temperature ( $^{\circ}$ C): 21.5, Liquid temperature ( $^{\circ}$ C): 21.0


DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(7.04, 7.04, 7.04); Calibrated: 04/03/2014;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 22/01/2014
- Phantom: SAM2; Type: SAM; Serial: TP1562
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Configuration/802.11b 2437MHz Back/Area Scan (7x9x1): Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.0330 W/kg

Configuration/802.11b 2437MHz Back/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 2.916 V/m; Power Drift = 0.10 dB
Peak SAR (extrapolated) = 0.0710 W/kg

SAR(1 g) = 0.035 W/kg; SAR(10 g) = 0.021 W/kg Maximum value of SAR (measured) = 0.0386 W/kg

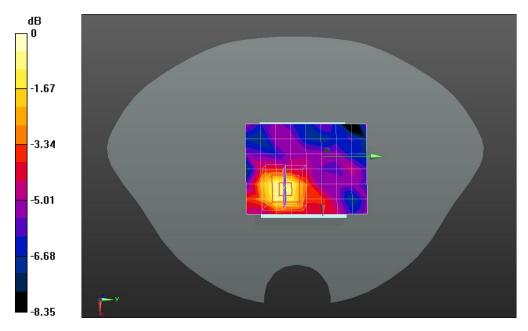

0 dB = 0.0386 W/kg = -14.13 dBW/kg



SAR for Body

Date/Time: 11-11-2014

Test Laboratory: QuieTek Lab 802.11b 2437MHz Back face

**DUT: Moticam X2 Smart Camera; Type: Moticam X2** 

Communication System: UID 0, Wi-Fi (0); Communication System Band: 802.11b; Duty Cycle: 1:1.0;

Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz;  $\sigma = 1.94$  S/m;  $\epsilon r = 51.31$ ;  $\rho = 1000$  kg/m3;

Phantom section: Flat Section

Ambient temperature ( $^{\circ}$ C): 21.5, Liquid temperature ( $^{\circ}$ C): 21.0

**DASY5** Configuration:


- Probe: EX3DV4 SN3710; ConvF(6.88, 6.88, 6.88); Calibrated: 04/03/2014;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 22/01/2014
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Configuration/802.11b 2437MHz Back face/Area Scan (7x9x1): Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.0871 W/kg

Configuration/802.11b 2437MHz Back face/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 5.403 V/m; Power Drift = -0.17 dB

Peak SAR (extrapolated) = 0.227 W/kg

**SAR(1 g) = 0.099 W/kg; SAR(10 g) = 0.034 W/kg** Maximum value of SAR (measured) = 0.133 W/kg

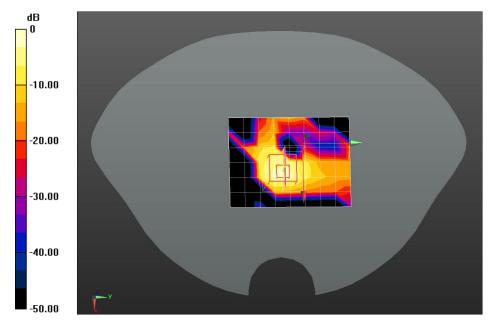

0 dB = 0.133 W/kg = -8.76 dBW/kg



Date/Time: 11-11-2014

Test Laboratory: QuieTek Lab 802.11b 2437MHz Right face

DUT: Moticam X2 Smart Camera; Type: Moticam X2

Communication System: UID 0, Wi-Fi (0); Communication System Band: 802.11b; Duty Cycle: 1:1.0;

Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz;  $\sigma = 1.94$  S/m;  $\epsilon r = 51.31$ ;  $\rho = 1000$  kg/m3;

Phantom section: Flat Section

Ambient temperature ( $^{\circ}$ ): 21.5, Liquid temperature ( $^{\circ}$ ): 21.0

DASY5 Configuration:


- Probe: EX3DV4 SN3710; ConvF(6.88, 6.88, 6.88); Calibrated: 04/03/2014;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 22/01/2014
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Configuration/802.11b 2437MHz Right face/Area Scan (7x9x1): Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 0.0969 W/kg

Configuration/802.11b 2437MHz Right face/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 5.768 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 0.262 W/kg


SAR(1 g) = 0.113 W/kg; SAR(10 g) = 0.039 W/kg Maximum value of SAR (measured) = 0.151 W/kg

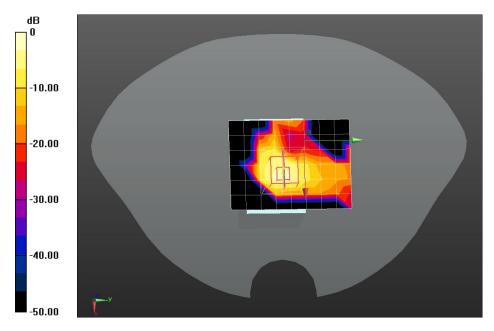

0 dB = 0.151 W/kg = -8.21 dBW/kg



## **Z-Axis Plot**

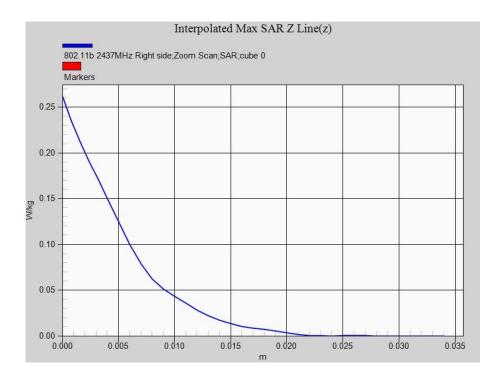



Date/Time: 11-11-2014

Test Laboratory: QuieTek Lab 802.11b 2437MHz Bottom face

#### DUT: Moticam X2 Smart Camera; Type: Moticam X2

Communication System: UID 0, Wi-Fi (0); Communication System Band: 802.11b; Duty Cycle: 1:1.0;

Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz;  $\sigma = 1.94$  S/m;  $\epsilon r = 51.31$ ;  $\rho = 1000$  kg/m3;

Phantom section: Flat Section

Ambient temperature ( $^{\circ}$ C): 21.5, Liquid temperature ( $^{\circ}$ C): 21.0

DASY5 Configuration:


- Probe: EX3DV4 SN3710; ConvF(6.88, 6.88, 6.88); Calibrated: 04/03/2014;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 22/01/2014
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

# Configuration/802.11b 2437MHz Bottom face/Area Scan (7x9x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 0.0512 W/kg

Configuration/802.11b 2437MHz Bottom face/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 4.122 V/m; Power Drift = -0.18 dB
Peak SAR (extrapolated) = 0.123 W/kg

SAR(1 g) = 0.056 W/kg; SAR(10 g) = 0.020 W/kg Maximum value of SAR (measured) = 0.0710 W/kg

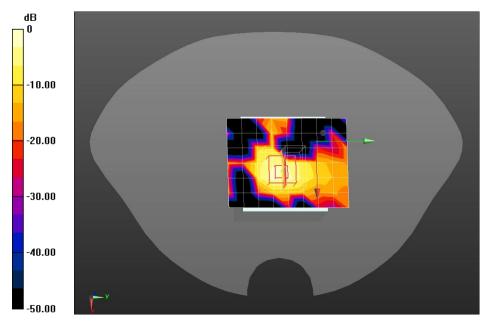

0 dB = 0.0710 W/kg = -11.49 dBW/kg



# Appendix C. Test Setup Photographs & EUT Photographs

# **Antenna to Antenna/User Separation Distances**


# Top of EUT Front 64mm 75mm WIFI Antenna 16mm

# <u>Back</u>

Antenna-to-user	WIFI Antenna for Head/ Body
separation distances:	Moticam X2 Smart Camera -Bottom face: 20mm from WIFI Antenna
	Moticam X2 Smart Camera -Edges with the following configurations
	Top: 35mm from WIFI Antenna
	Left: 36mm from WIFI Antenna
	Right: 16mm from WIFI Antenna
	Front: 49mm from WIFI Antenna
	Back: 19mm from WIFI Antenna





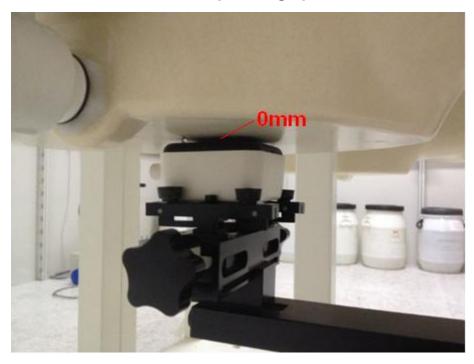


WIFI SAR Bottom face 0mm for Head




WIFI SAR Right face 0mm for Head



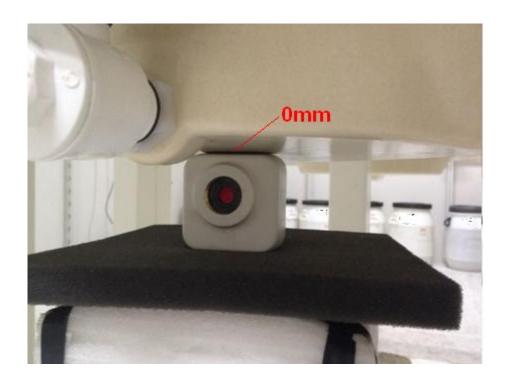


WIFI SAR Back face 0mm for Head

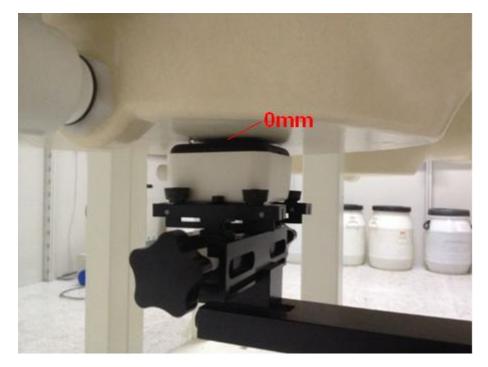


WIFI SAR Bottom face 0mm for Body



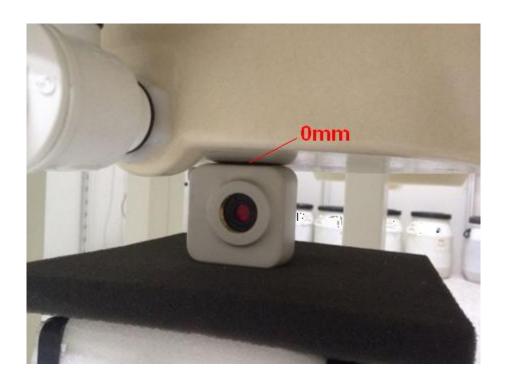

WIFI SAR Right face 0mm for Body

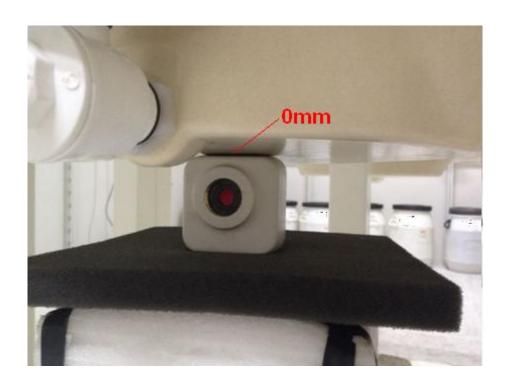


WIFI SAR Back face 0mm for Body



# Depth of the liquid in the phantom – Zoom in


Note: The position used in the measurements were according to IEEE 1528 - 2003

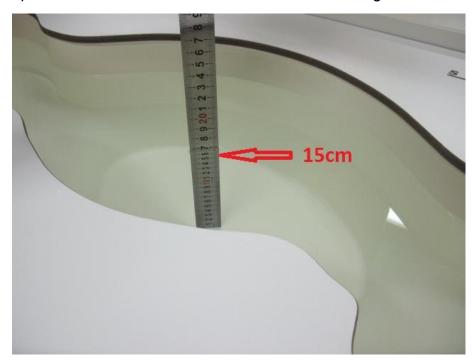



# **EUT Photographs**

## (1) EUT Photo

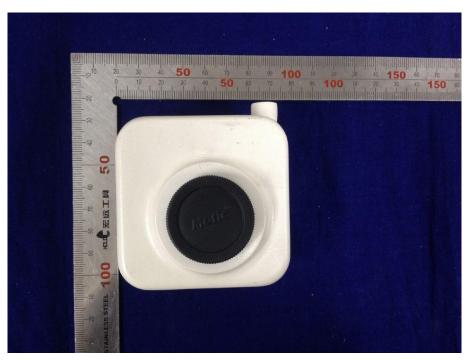


## (2) EUT Photo






# (3) EUT Photo

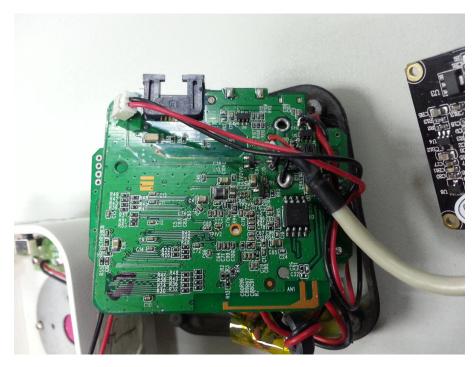

# (4) EUT Photo

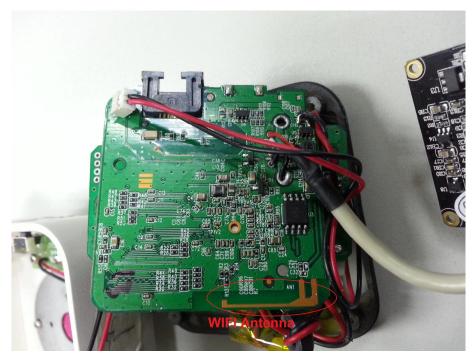

Report No.: 14B0296R-HP-US-P03V01



## **Appendix D. Probe Calibration Data**

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Quietek (Auden)

Certificate No: EX3-3710 Mar14

#### CALIBRATION CERTIFICATE

Object EX3DV4 - SN:3710

QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5, Calibration procedure(s)

QA CAL-25.v6

Calibration procedure for dosimetric E-field probes

March 4, 2014 Calibration date:

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	04-Apr-13 (No. 217-01733)	Apr-14
Power sensor E4412A	MY41498087	04-Apr-13 (No. 217-01733)	Apr-14
Reference 3 dB Attenuator	SN: S5054 (3c)	04-Apr-13 (No. 217-01737)	Apr-14
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-13 (No. 217-01735)	Apr-14
Reference 30 dB Attenuator	SN: S5129 (30b)	04-Apr-13 (No. 217-01738)	Apr-14
Reference Probe ES3DV2	SN: 3013	30-Dec-13 (No. ES3-3013_Dec13)	Dec-14
DAE4	SN: 660	13-Dec-13 (No. DAE4-660_Dec13)	Dec-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

Function Jeton Kastrati Laboratory Technician Calibrated by: Katja Pokovic Technical Manager Approved by: Issued: March 4, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Page 1 of 11

Certificate No: EX3-3710\_Mar14

Report No.: 14B0296R-HP-US-P03V01



#### Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

tissue simulating liquid TSL NORMx,y,z sensitivity in free space ConvF sensitivity in TSL / NORMx,y,z DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters A, B, C, D

Polarization φ φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
  b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close
- proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E2-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx, y, z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: EX3-3710 Mar14 Page 2 of 11



EX3DV4 - SN:3710 March 4, 2014

# Probe EX3DV4

SN:3710

Manufactured: July 21, 2009 Calibrated:

March 4, 2014

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: EX3-3710\_Mar14

Page 3 of 11



EX3DV4-SN:3710 March 4, 2014

#### DASY/EASY - Parameters of Probe: EX3DV4 - SN:3710

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) <sup>2</sup> ) <sup>A</sup>	0.51	0.56	0.44	± 10.1 %
DCP (mV) <sup>B</sup>	100.3	97.6	101.3	

#### Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc <sup>b</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	137.9	±3.5 %
		Y	0.0	0.0	1.0		136.7	
		Z	0.0	0.0	1.0		139.8	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: EX3-3710\_Mar14

Page 4 of 11

A The uncertainties of NormX,Y,Z do not affect the E2-field uncertainty inside TSL (see Pages 5 and 6).

Numerical linearization parameter: uncertainty not required.

Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the



EX3DV4-SN:3710 March 4, 2014

#### DASY/EASY - Parameters of Probe: EX3DV4 - SN:3710

#### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
450	43.5	0.87	10.42	10.42	10.42	0.17	2.22	± 13.3 %
750	41.9	0.89	9.76	9.76	9.76	0.62	0.69	± 12.0 %
835	41.5	0.90	9.56	9.56	9.56	0.57	0.69	± 12.0 %
900	41.5	0.97	9.42	9.42	9.42	0.53	0.72	± 12.0 %
1810	40.0	1.40	7.74	7.74	7.74	0.41	0.94	± 12.0 %
1900	40.0	1.40	7.72	7.72	7.72	0.49	0.85	± 12.0 %
2450	39.2	1.80	7.04	7.04	7.04	0.39	1.03	± 12.0 %
2600	39.0	1.96	6.87	6.87	6.87	0.60	0.80	± 12.0 %
3500	37.9	2.91	6.82	6.82	6.82	0.55	0.88	± 13.1 %
5200	36.0	4.66	4.91	4.91	4.91	0.40	1.80	± 13.1 %
5500	35.6	4.96	4.63	4.63	4.63	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.43	4.43	4.43	0.40	1.80	± 13.1 %

Certificate No: EX3-3710\_Mar14

<sup>&</sup>lt;sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Fat frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip disposer from the boundary.

diameter from the boundary.



March 4, 2014 EX3DV4-SN:3710

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3710

#### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
450	56.7	0.94	10.53	10.53	10.53	0.10	1.00	± 13.3 %
750	55.5	0.96	9.28	9.28	9.28	0.39	0.93	± 12.0 %
835	55.2	0.97	9.22	9.22	9.22	0.65	0.72	± 12.0 %
900	55.0	1.05	9.04	9.04	9.04	0.75	0.67	± 12.0 %
1810	53.3	1.52	7.36	7.36	7.36	0.80	0.62	± 12.0 %
1900	53.3	1.52	7.25	7.25	7.25	0.55	0.76	± 12.0 %
2450	52.7	1.95	6.88	6.88	6.88	0.80	0.58	± 12.0 %
2600	52.5	2.16	6.67	6.67	6.67	0.80	0.50	± 12.0 %
3500	51.3	3.31	6.29	6.29	6.29	0.44	1.02	± 13.1 %
5200	49.0	5.30	4.22	4.22	4.22	0.50	1.90	± 13.1 %
5500	48.6	5.65	3.91	3.91	3.91	0.50	1.90	± 13.1 %
5800	48.2	6.00	4.00	4.00	4.00	0.50	1.90	± 13.1 %

Certificate No: EX3-3710\_Mar14

 $<sup>^{\</sup>rm C}$  Frequency validity of  $\pm$  100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to  $\pm$  50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


F At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than  $\pm$  1% for frequencies below 3 GHz and below  $\pm$  2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



EX3DV4-SN:3710 March 4, 2014

# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

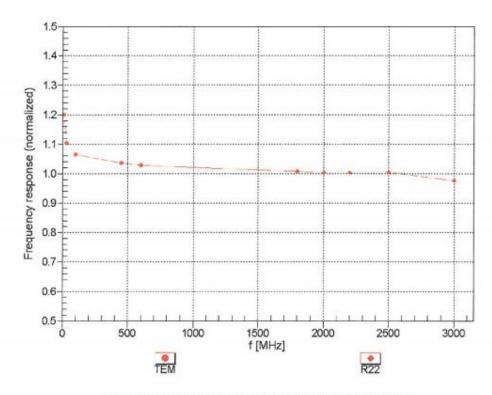

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: EX3-3710\_Mar14

Page 7 of 11





EX3DV4- SN:3710 March 4, 2014


# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$



MHz,TEM f=1800 MHz,R22





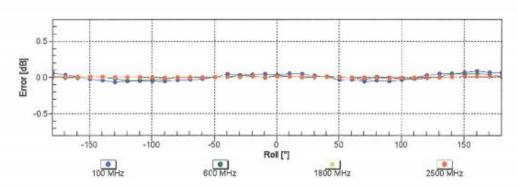

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Certificate No: EX3-3710\_Mar14


Page 8 of 11



EX3DV4- SN:3710 March 4, 2014

## Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f<sub>eval</sub>= 1900 MHz)

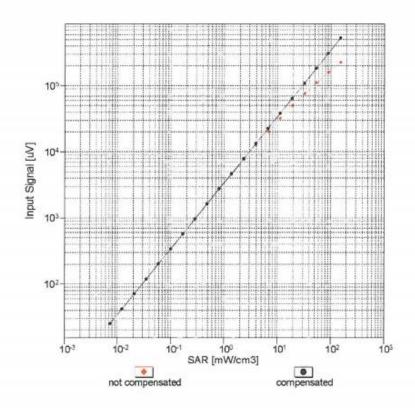

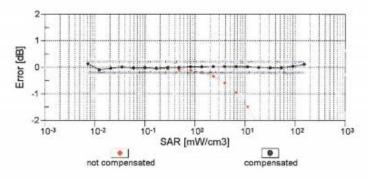


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: EX3-3710\_Mar14

Page 9 of 11



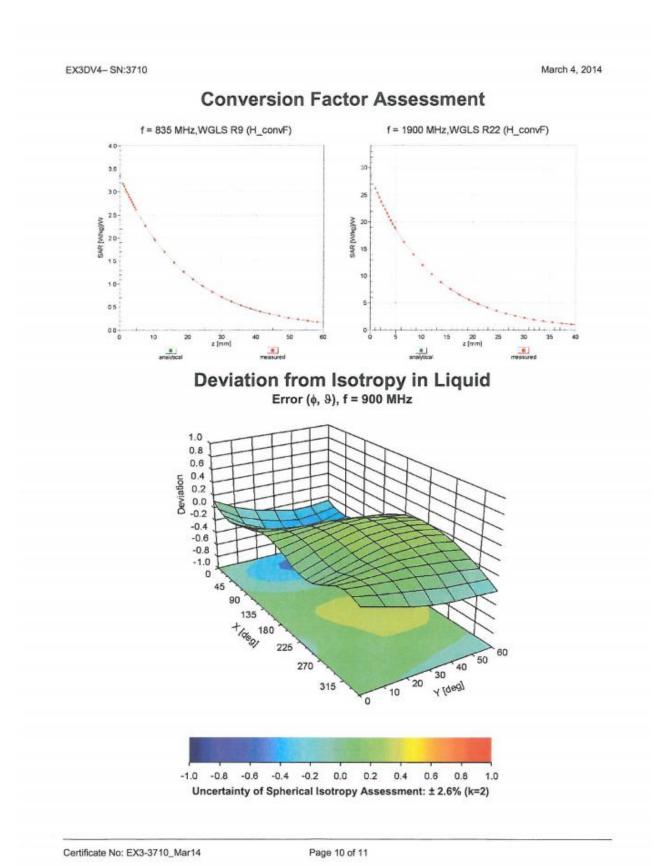



EX3DV4- SN:3710 March 4, 2014

# DASY/EASY - Parameters of Probe: EX3DV4 - SN:3710

#### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-19.6
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

Certificate No: EX3-3710\_Mar14

Page 11 of 11



# **Appendix E. Dipole Calibration Data**

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





C

Accreditation No.: SCS 108


Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

CALIBRATION (	CERTIFICATI		
Object	D2450V2 - SN: 8	839	
Calibration procedure(s)	QA CAL-05.v9 Calibration proce	edure for dipole validation kits ab	ove 700 MHz
Calibration date:	February 24, 20	14	
		tional standards, which realize the physical u probability are given on the following pages a	
All calibrations have been condu		bry facility: environment temperature (22 $\pm$ 3)°	C and humidity < 70%.
All calibrations have been conducation Equipment used (M&			
	TE critical for calibration)	Cal Date (Certificate No.)  09-Oct-13 (No. 217-01827)	Scheduled Calibration Oct-14
All calibrations have been conducted that calibration Equipment used (M&Primary Standards Power meter EPM-442A	TE critical for calibration)	Cal Date (Certificate No.)	Scheduled Calibration
All calibrations have been conducted (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317	Cal Date (Certificate No.) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01827) 09-Oct-13 (No. 217-01828)	Scheduled Calibration Oct-14
All calibrations have been conductable.  Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)	Cal Date (Certificate No.)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01828)  04-Apr-13 (No. 217-01736)	Scheduled Calibration Oct-14 Oct-14 Oct-14 Apr-14
Calibrations have been conductable Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.3 / 06327	Cal Date (Certificate No.)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01828)  04-Apr-13 (No. 217-01736)  04-Apr-13 (No. 217-01739)	Scheduled Calibration Oct-14 Oct-14 Oct-14 Apr-14 Apr-14
All calibrations have been conductable.  Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)	Cal Date (Certificate No.)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01828)  04-Apr-13 (No. 217-01736)	Scheduled Calibration Oct-14 Oct-14 Oct-14 Apr-14
Calibrations have been conductable Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.3 / 06327  SN: 3205	Cal Date (Certificate No.)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01828)  04-Apr-13 (No. 217-01736)  04-Apr-13 (No. 217-01739)  30-Dec-13 (No. ES3-3205_Dec13)	Scheduled Calibration Oct-14 Oct-14 Oct-14 Apr-14 Apr-14 Dec-14
All calibrations have been conductable Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.3 / 06327  SN: 3205  SN: 601	Cal Date (Certificate No.)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01828)  04-Apr-13 (No. 217-01736)  04-Apr-13 (No. 217-01739)  30-Dec-13 (No. ES3-3205_Dec13)  25-Apr-13 (No. DAE4-601_Apr13)	Scheduled Calibration Oct-14 Oct-14 Oct-14 Apr-14 Apr-14 Dec-14 Apr-14
All calibrations have been conductable Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	ID #  GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601  ID #	Cal Date (Certificate No.)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01828)  04-Apr-13 (No. 217-01736)  04-Apr-13 (No. 217-01739)  30-Dec-13 (No. ES3-3205_Dec13)  25-Apr-13 (No. DAE4-601_Apr13)  Check Date (in house)	Scheduled Calibration Oct-14 Oct-14 Oct-14 Apr-14 Apr-14 Dec-14 Apr-14 Scheduled Check
All calibrations have been conductable Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	ID #  GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601  ID #  100005	Cal Date (Certificate No.)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01828)  04-Apr-13 (No. 217-01736)  04-Apr-13 (No. 217-01739)  30-Dec-13 (No. ES3-3205_Dec13)  25-Apr-13 (No. DAE4-601_Apr13)  Check Date (in house)  04-Aug-99 (in house check Oct-13)	Scheduled Calibration Oct-14 Oct-14 Oct-14 Apr-14 Apr-14 Dec-14 Apr-14 Scheduled Check In house check: Oct-16
All calibrations have been conductable Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	ID #  GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601  ID #  100005 US37390585 S4206	Cal Date (Certificate No.)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01827)  09-Oct-13 (No. 217-01828)  04-Apr-13 (No. 217-01736)  04-Apr-13 (No. 217-01739)  30-Dec-13 (No. ES3-3205_Dec13)  25-Apr-13 (No. DAE4-601_Apr13)  Check Date (in house)  04-Aug-99 (in house check Oct-13)  18-Oct-01 (in house check Oct-13)	Scheduled Calibration Oct-14 Oct-14 Oct-14 Apr-14 Apr-14 Dec-14 Apr-14 Scheduled Check In house check: Oct-16 In house check: Oct-14

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D2450V2-839\_Feb14 Page 1 of 8





#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

Multilateral Agreement for the recognition of calibration certificates

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-839\_Feb14 Page 2 of 8



#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

#### **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.1 ± 6 %	1.86 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.3 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.0 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.15 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.3 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	50.7 ± 6 %	2.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.8 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	49.9 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.86 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.1 W/kg ± 16.5 % (k=2)

Certificate No: D2450V2-839\_Feb14

Page 3 of 8



#### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	$54.5 \Omega + 2.4 j\Omega$
Return Loss	- 26.2 dB

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	$50.6 \Omega + 4.3 j\Omega$
Return Loss	- 27.4 dB

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.159 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	July 20, 2009

Certificate No: D2450V2-839\_Feb14



#### DASY5 Validation Report for Head TSL

Date: 24.02.2014

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 839

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 1.86 \text{ S/m}$ ;  $\varepsilon_r = 38.1$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

#### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 99.591 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 27.9 W/kg

SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.15 W/kgMaximum value of SAR (measured) = 17.0 W/kg




0 dB = 17.0 W/kg = 12.30 dBW/kg

Certificate No: D2450V2-839\_Feb14



#### Impedance Measurement Plot for Head TSL

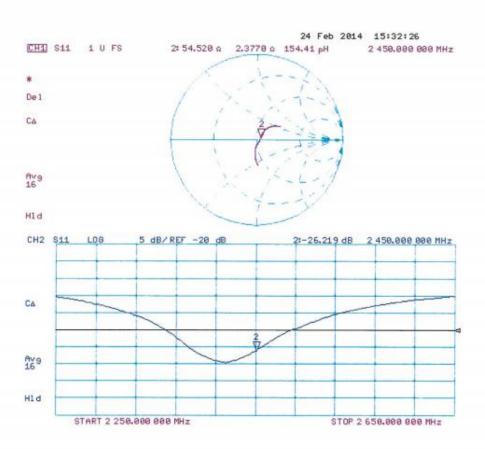

Certificate No: D2450V2-839\_Feb14

Page 6 of 8



#### DASY5 Validation Report for Body TSL

Date: 24.02.2014

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 839

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 2.02 \text{ S/m}$ ;  $\varepsilon_r = 50.7$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.35, 4.35, 4.35); Calibrated: 30.12.2013;

· Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 25.04.2013

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

#### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.267 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 27.1 W/kg

SAR(1 g) = 12.8 W/kg; SAR(10 g) = 5.86 W/kg

Maximum value of SAR (measured) = 17.0 W/kg

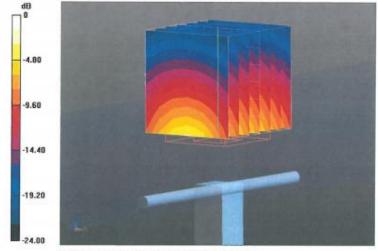


0 dB = 17.0 W/kg = 12.30 dBW/kg

Certificate No: D2450V2-839\_Feb14



#### Impedance Measurement Plot for Body TSL

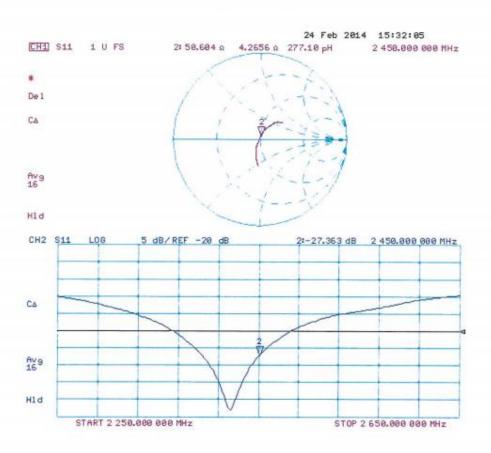

Certificate No: D2450V2-839\_Feb14

Page 8 of 8



## **Appendix F. DAE Calibration Data**

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service sulsse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Quietek-CN (Auden)

Certificate No: DAE4-1220\_Jan14

Accreditation No.: SCS 108

CALIBI	RATION	CERTII	-ICATE

Object DAE4 - SD 000 D04 BM - SN: 1220

Calibration procedure(s) QA CAL-06.v26

Calibration procedure for the data acquisition electronics (DAE)

Calibration date: January 22, 2014

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).

The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	01-Oct-13 (No:13976)	Oct-14
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	07-Jan-14 (in house check)	In house check: Jan-15
AUTO DAE Calibration Offit	00 0110 000 101 1001	or carrier (in ricode directly	III HOUSE CHECK GUIT 15

Calibrated by:

Name R.Mayoraz Function Technician Signature

Approved by:

Fin Bomholt

Deputy Technical Manager

Issued: January 22, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: DAE4-1220\_Jan14

Page 1 of 5



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

#### Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

#### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-1220\_Jan14

Page 2 of 5



# DC Voltage Measurement A/D - Converter Resolution nominal

High Range:  $1LSB = 6.1\mu V$ , full range = -100...+300 mVLow Range: 1LSB = 61nV, full range = -1......+3mVDASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Υ	Z
High Range	405.217 ± 0.02% (k=2)	404.944 ± 0.02% (k=2)	404.170 ± 0.02% (k=2)
Low Range	3.97747 ± 1.50% (k=2)	3.99640 ± 1.50% (k=2)	3.98639 ± 1.50% (k=2)

#### **Connector Angle**

Connector Angle to be used in DASY system	176.5 ° ± 1 °
---	---------------

Certificate No: DAE4-1220\_Jan14

Page 3 of 5



#### Appendix

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	199996.00	0.76	0.00
Channel X + Input	20002.66	1.98	0.01
Channel X - Input	-19998.07	2.88	-0.01
Channel Y + Input	199996.91	1.60	0.00
Channel Y + Input	20001.20	0.56	0.00
Channel Y - Input	-20001.74	-0.74	0.00
Channel Z + Input	199994.91	-0.44	-0.00
Channel Z + Input	20000.27	-0.23	-0.00
Channel Z - Input	-20001.65	-0.63	0.00

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2001.09	0.27	0.01
Channel X + Input	202.00	0.81	0.40
Channel X - Input	-197.89	0.69	-0.35
Channel Y + Input	2000.99	0.22	0.01
Channel Y + Input	200.07	-1.02	-0.50
Channel Y - Input	-201.19	-2.34	1.18
Channel Z + Input	2000.92	0.16	0.01
Channel Z + Input	200.20	-0.82	-0.41
Channel Z - Input	-199.32	-0.45	0.23

#### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	10.55	8.63
	- 200	-6.76	-8.77
Channel Y	200	-9.89	-10.34
	- 200	7.59	7.71
Channel Z	200	12.72	12.38
	- 200	-13.94	-14.25

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	1.02	-3.16
Channel Y	200	8.35	-	2.35
Channel Z	200	10.56	5.06	-

Certificate No: DAE4-1220\_Jan14

Page 4 of 5



#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15888	15493
Channel Y	16012	15900
Channel Z	15706	16099

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	1.13	-0.62	2.79	0.50
Channel Y	-0.89	-2.63	0.76	0.48
Channel Z	-0.60	-2.36	0.94	0.50

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1220\_Jan14