


1. Set-Up for Tune-Up and Adjustment of Transmitter

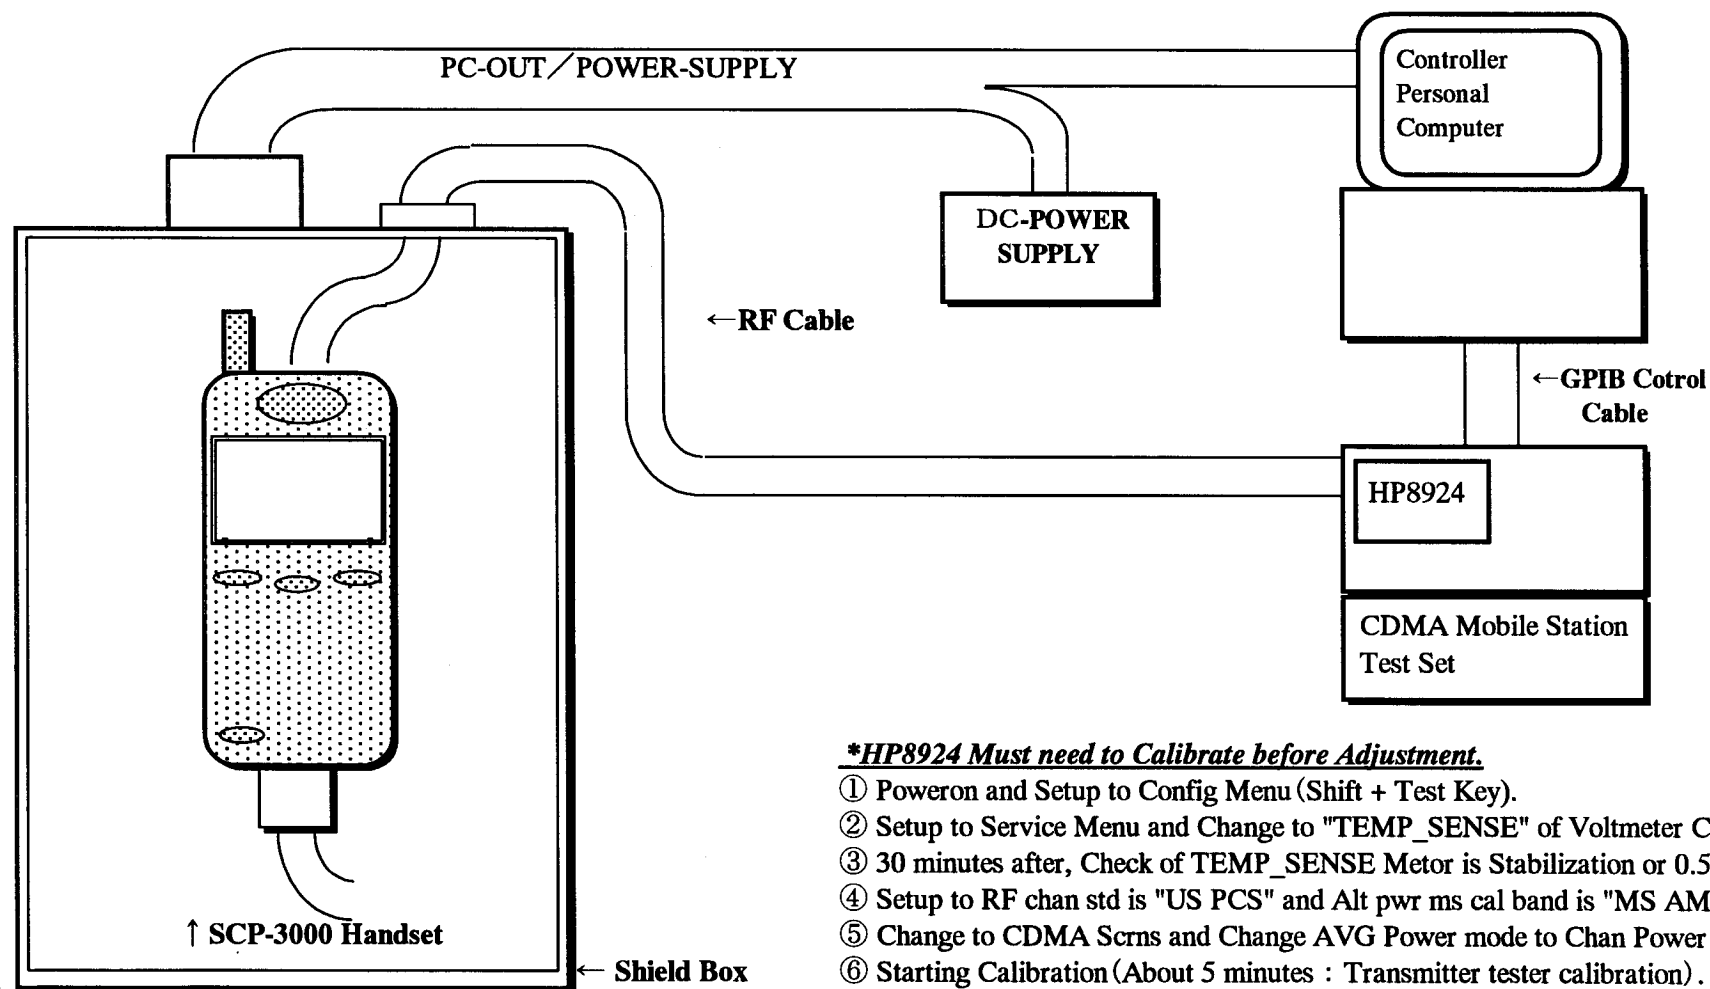




***HP8924 Must need to Calibrate before Adjustment.**

- ① Poweron and Setup to Config Menu (Shift + Test Key).
- ② Setup to Service Menu and Change to "TEMP_SENSE" of Voltmeter Connection .
- ③ 30 minutes after, Check of TEMP_SENSE Meter is Stabilization or 0.5V (=50°C).
- ④ Setup to RF chan std is "US PCS" and Alt pwr ms cal band is "MS AMPS".
- ⑤ Change to CDMA Scrns and Change AVG Power mode to Chan Power mode.
- ⑥ Starting Calibration (About 5 minutes : Transmitter tester calibration).
- ⑦ Next time, Return to Config Menu and Starting Rfgen Lvl Calibration (few Seconds).

*** Added HP Documents of calibration Nextpage.**

2. Alignment Procedure

(1) Adjustment Procedure

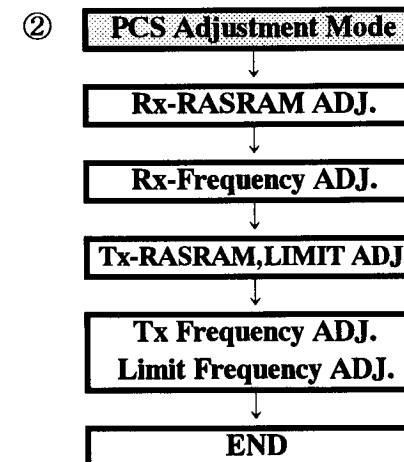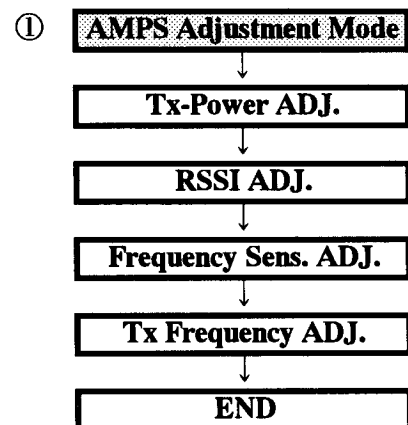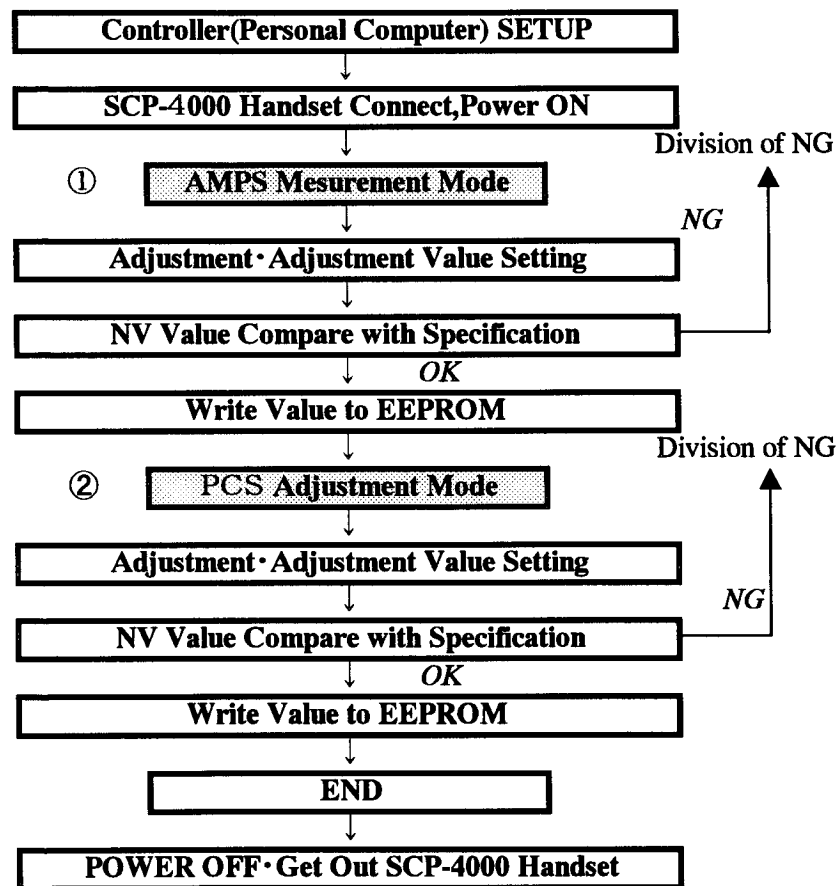

(2) Measurement Procedure

