

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

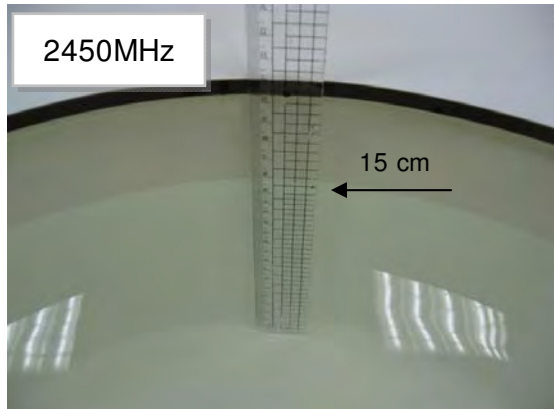


Fig.2.1

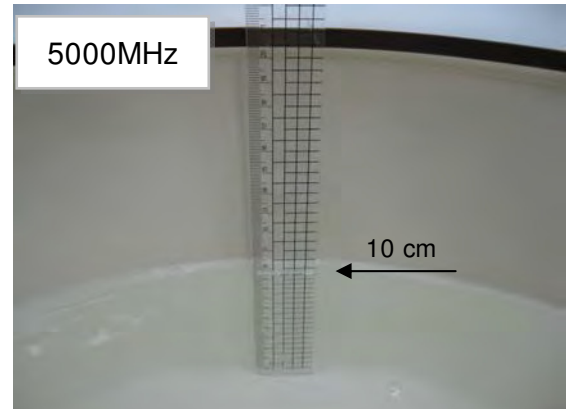


Fig.2.2

Body - distance between flat phantom and EUT is 0 mm

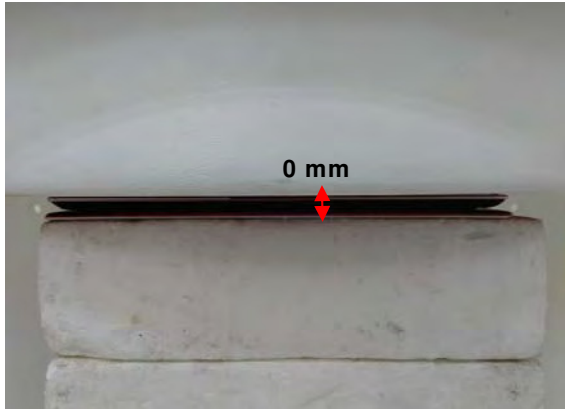


Fig.3 EUT Back side_Tablet mode to flat phantom

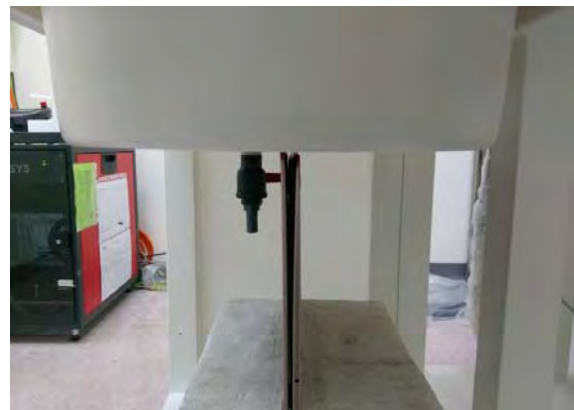
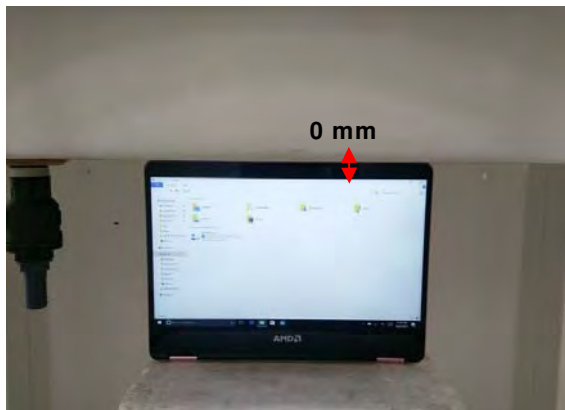


Fig.4 EUT Top side_Tablet mode to flat phantom

12. Photographs of the EUT

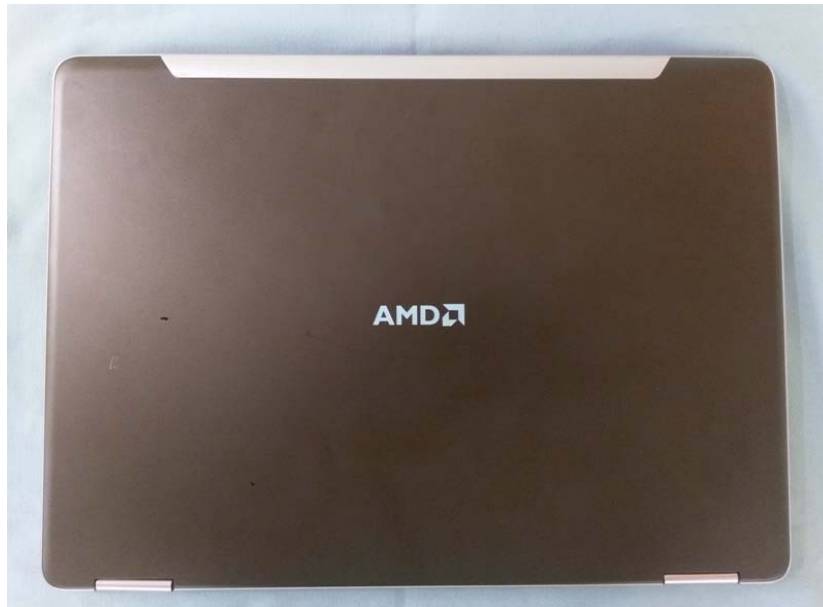


Fig.5 Front view of EUT



Fig.6 Back view of EUT

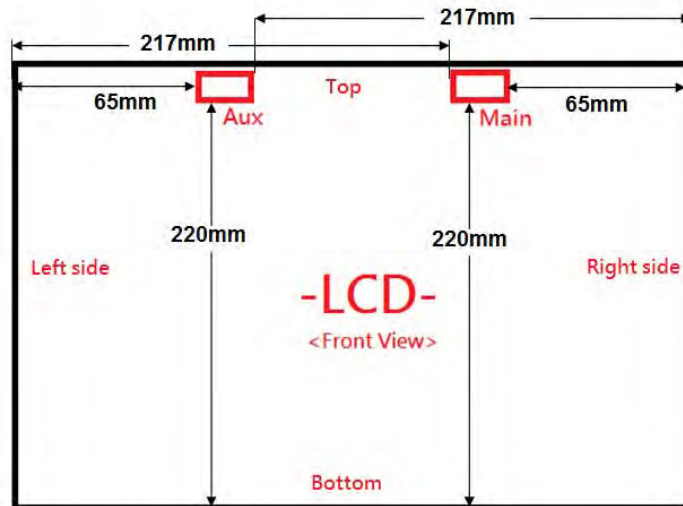


Fig.7 Antenna location of tablet mode (front view)



Fig.8 Antenna location of tablet mode (cross section view)

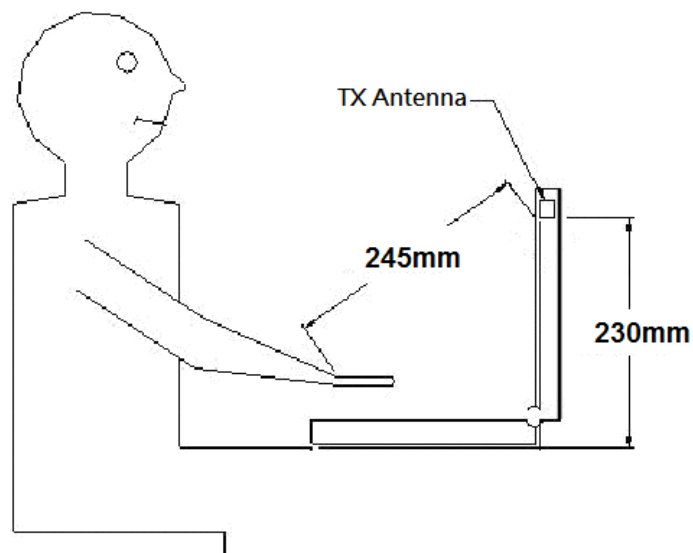


Fig.9 Antenna location of laptop mode
- End of Report -