

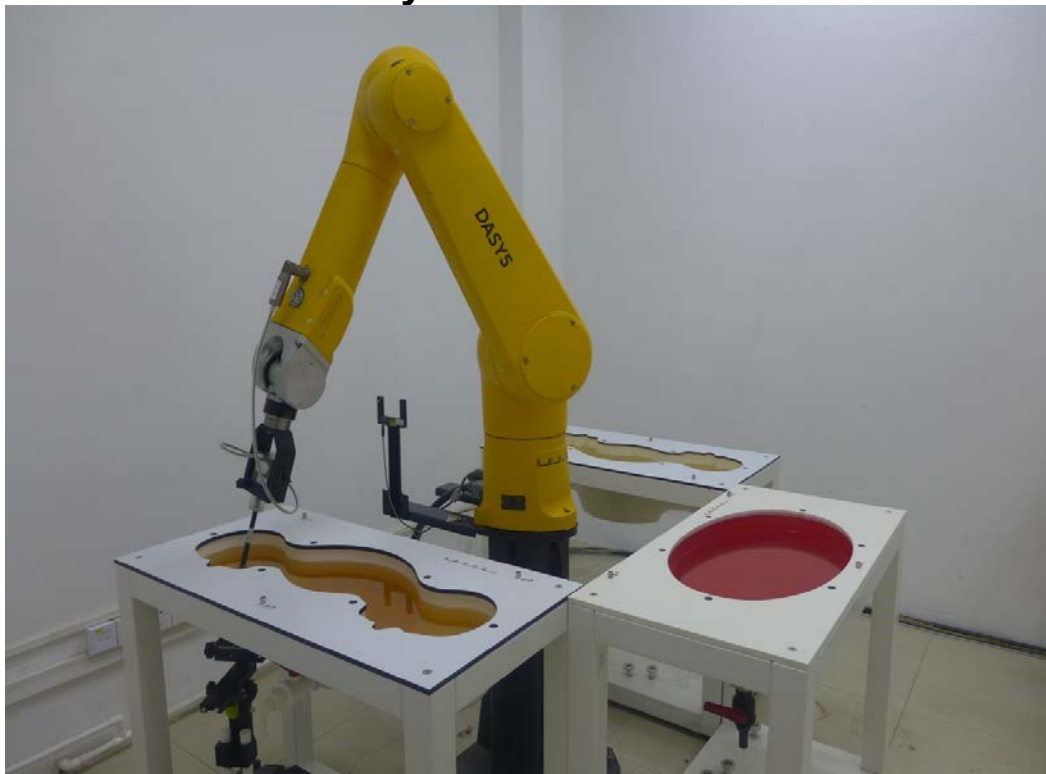


Appendix D

Photographs

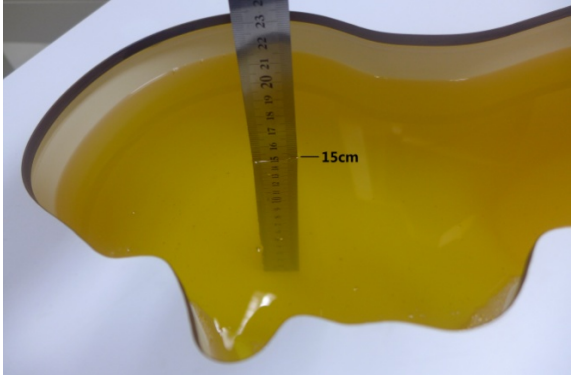
1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



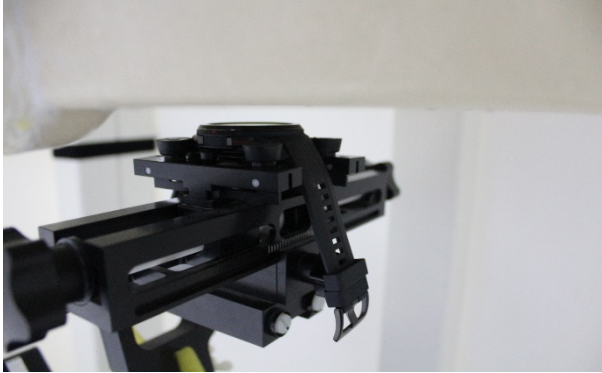
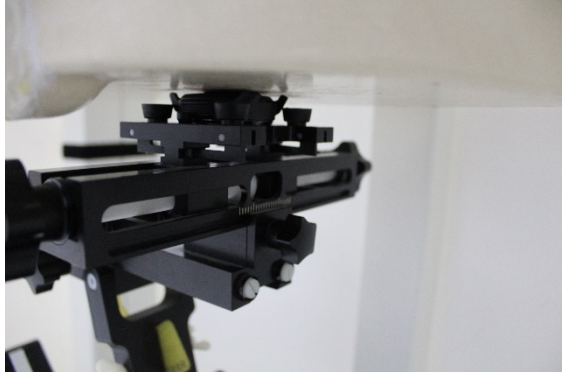


2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2450	NA
	NA



3. Photographs of EUT test position

Photo 2: Next to the mouth	Photo 3: Extremity
 A close-up photograph of a black mechanical device, likely a testing fixture, positioned next to a white, curved surface that resembles a mouth. The device has various components, including a central vertical rod and a horizontal arm.	 A close-up photograph of the same black mechanical device, showing a different angle that highlights its extremity. The device is positioned against a white, curved surface.



4. EUT Constructional Details

Photo 4: Front View	Photo 5: Back View
