

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.88 S/m; perm = 39.7; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 06/14/2023; Ambient Temp: 21.1°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7308; ConvF:(7.91,7.91,7.91); Calibrated: 2023-02-13

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn467; Calibrated: 2023-02-15

Phantom: Twin-SAM V4.0; Serial: 1275

Measurement SW: DASY Module SAR V16.2.0.1425

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.6 W/kg

SAR(1 g) = 5.20 W/kg; SAR(10 g) = 2.42 W/kg

Deviation (1 g) = -4.06%; Deviation (10 g) = -5.10%;

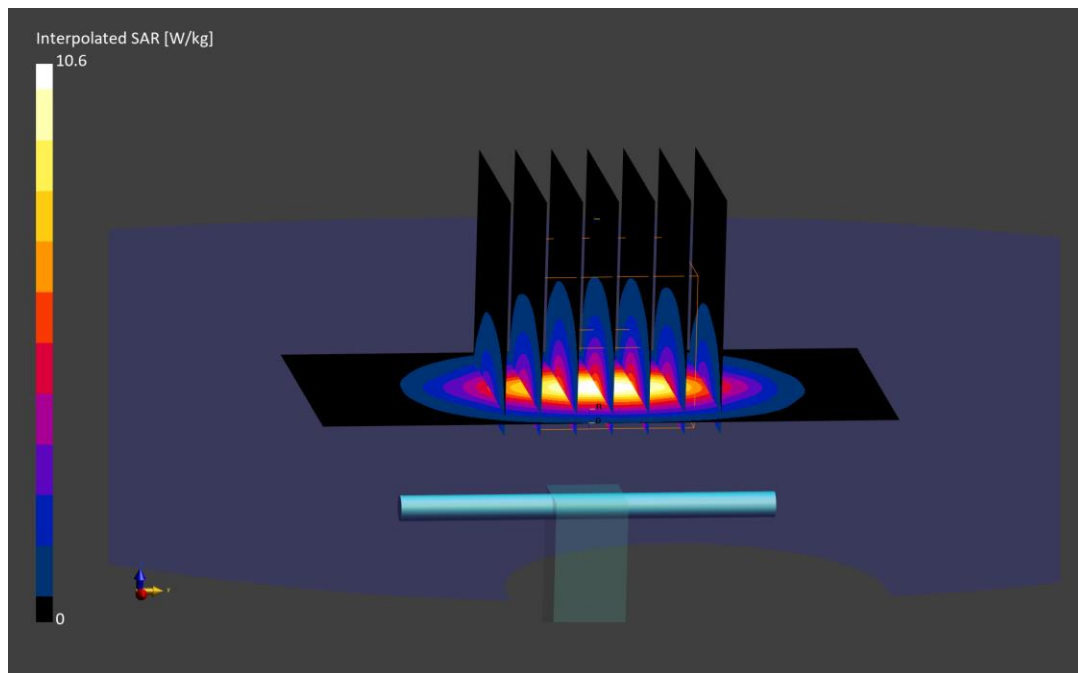

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5250.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5250.0 MHz; cond = 4.73 S/m; perm = 35.2; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2023; Ambient Temp: 22.0°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7420; ConvF:(5.22,5.22,5.22); Calibrated: 2022-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1333; Calibrated: 2022-10-13

Phantom: Twin-SAM V8.0; Serial: 1736

Measurement SW: DASY Module SAR V16.2.0.1425

5250 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.8 W/kg

SAR(1 g) = 4.04 W/kg; SAR(10 g) = 1.14 W/kg

Deviation (1 g) = 0.37%; Deviation (10 g) = -0.44%;

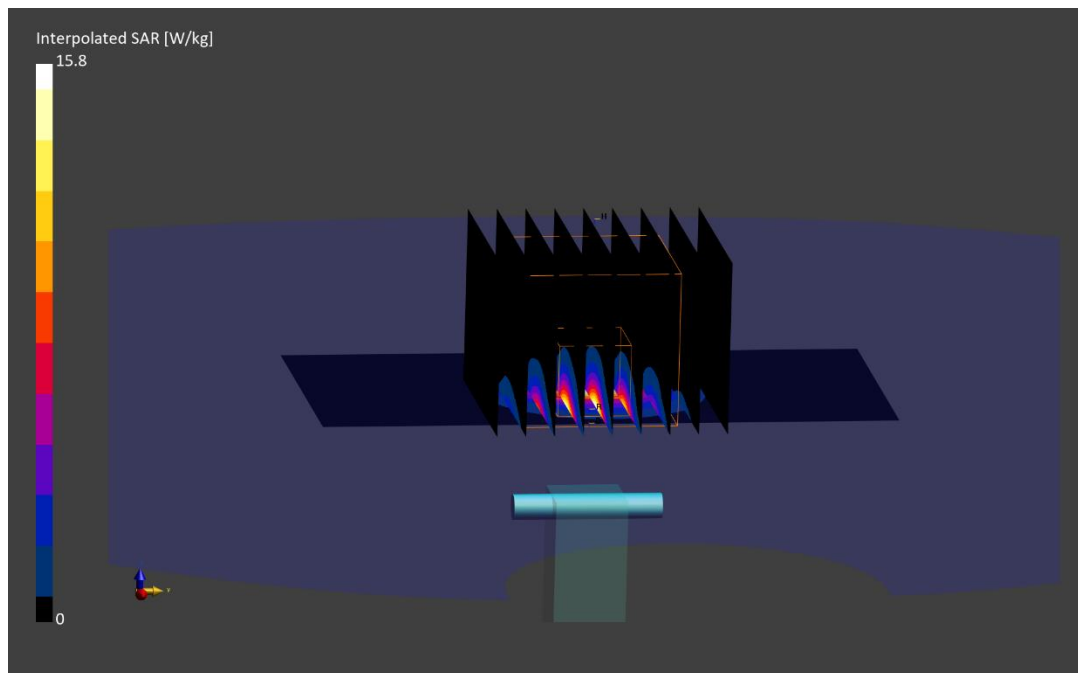

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5250.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5250.0 MHz; cond = 4.49 S/m; perm = 35.6; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/18/2023; Ambient Temp: 22.50°C; Tissue Temp: 20.70°C

Probe: EX3DV4 - SN7420; ConvF:(5.22,5.22,5.22); Calibrated: 2022-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1333; Calibrated: 2022-10-13

Phantom: Twin-SAM V8.0; Serial: 1736

Measurement SW: DASY Module SAR V16.2.0.1425

5250 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.6 W/kg

SAR(1 g) = 3.85 W/kg; SAR(10 g) = 1.10 W/kg

Deviation (1 g) = -4.35%; Deviation (10 g) = -3.93%;

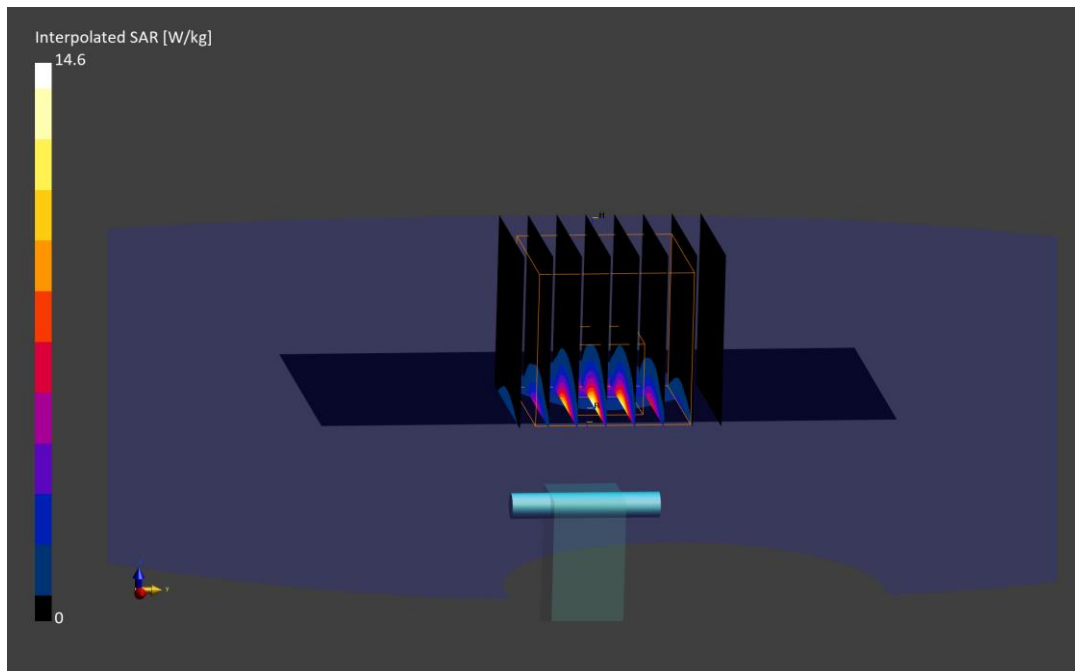

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5600.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5600.0 MHz; cond = 5.12 S/m; perm = 34.5; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2023; Ambient Temp: 22.0°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7420; ConvF:(4.63,4.63,4.63); Calibrated: 2022-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1333; Calibrated: 2022-10-13

Phantom: Twin-SAM V8.0; Serial: 1736

Measurement SW: DASY Module SAR V16.2.0.1425

5600 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.9 W/kg

SAR(1 g) = 4.28 W/kg; SAR(10 g) = 1.20 W/kg

Deviation (1 g) = 2.27%; Deviation (10 g) = 1.27%;

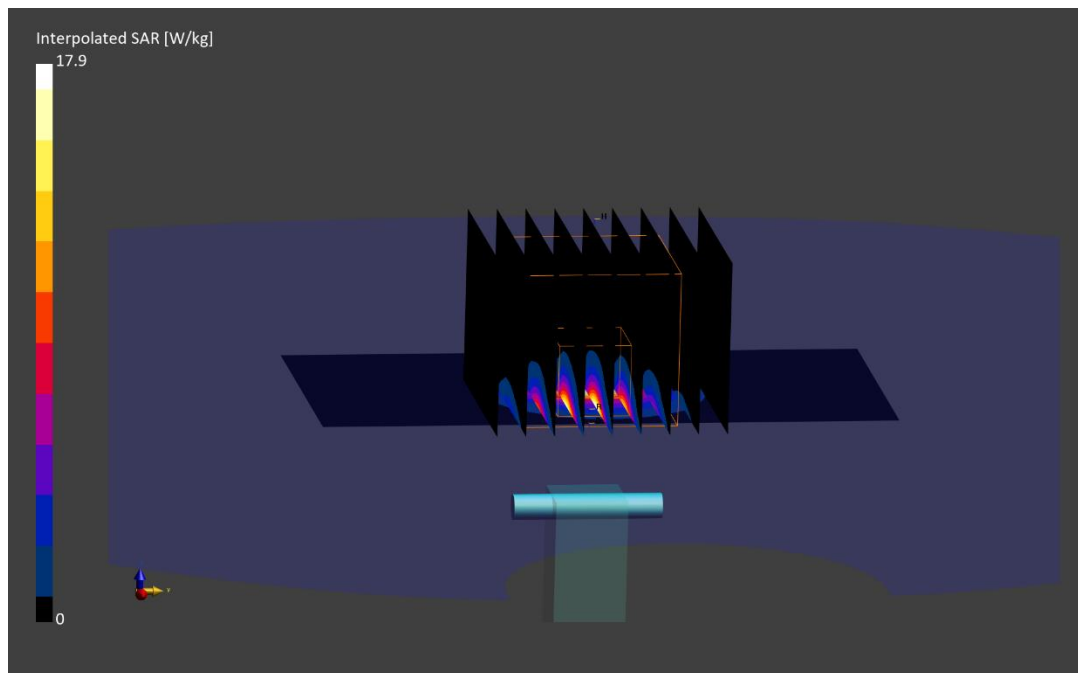

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5600.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5600.0 MHz; cond = 4.87 S/m; perm = 35.0; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/18/2023; Ambient Temp: 22.50°C; Tissue Temp: 20.70°C

Probe: EX3DV4 - SN7420; ConvF:(4.63,4.63,4.63); Calibrated: 2022-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1333; Calibrated: 2022-10-13

Phantom: Twin-SAM V8.0; Serial: 1736

Measurement SW: DASY Module SAR V16.2.0.1425

5600 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.0 W/kg

SAR(1 g) = 4.26 W/kg; SAR(10 g) = 1.21 W/kg

Deviation (1 g) = 1.79%; Deviation (10 g) = 2.11%;

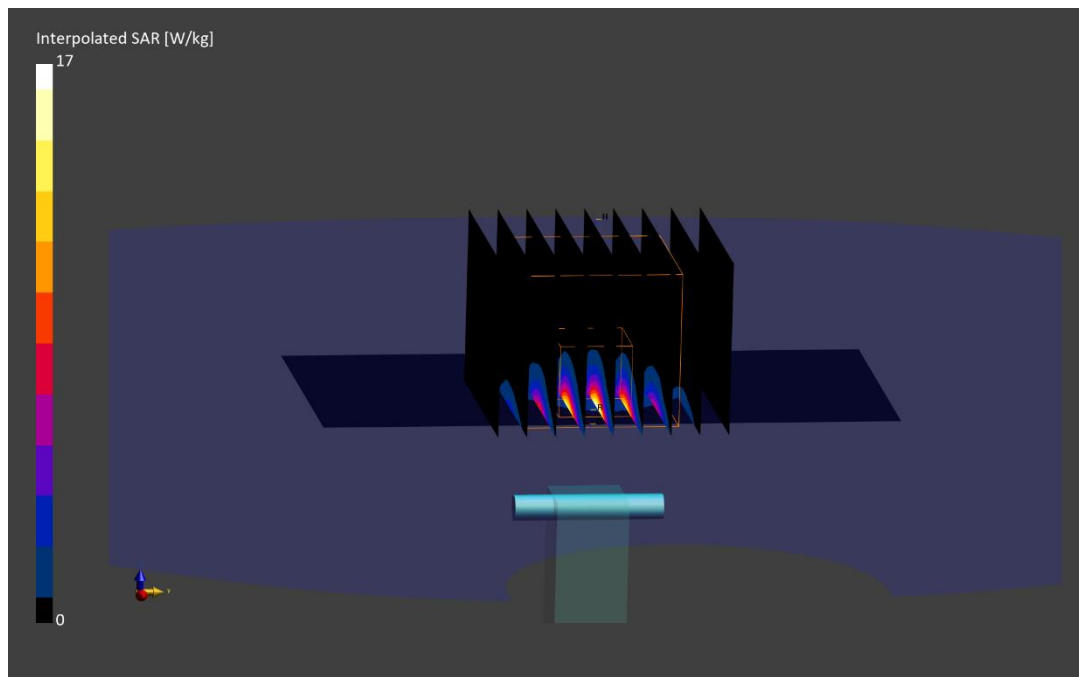

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5750.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5750.0 MHz; cond = 5.31 S/m; perm = 34.2; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2023; Ambient Temp: 22.0°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7420; ConvF:(4.8,4.8,4.8); Calibrated: 2022-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1333; Calibrated: 2022-10-13

Phantom: Twin-SAM V8.0; Serial: 1736

Measurement SW: DASY Module SAR V16.2.0.1425

5750 MHz System Verification at 17 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.5 W/kg

SAR(1 g) = 3.83 W/kg; SAR(10 g) = 1.08 W/kg

Deviation (1 g) = -4.84%; Deviation (10 g) = -4.85%;

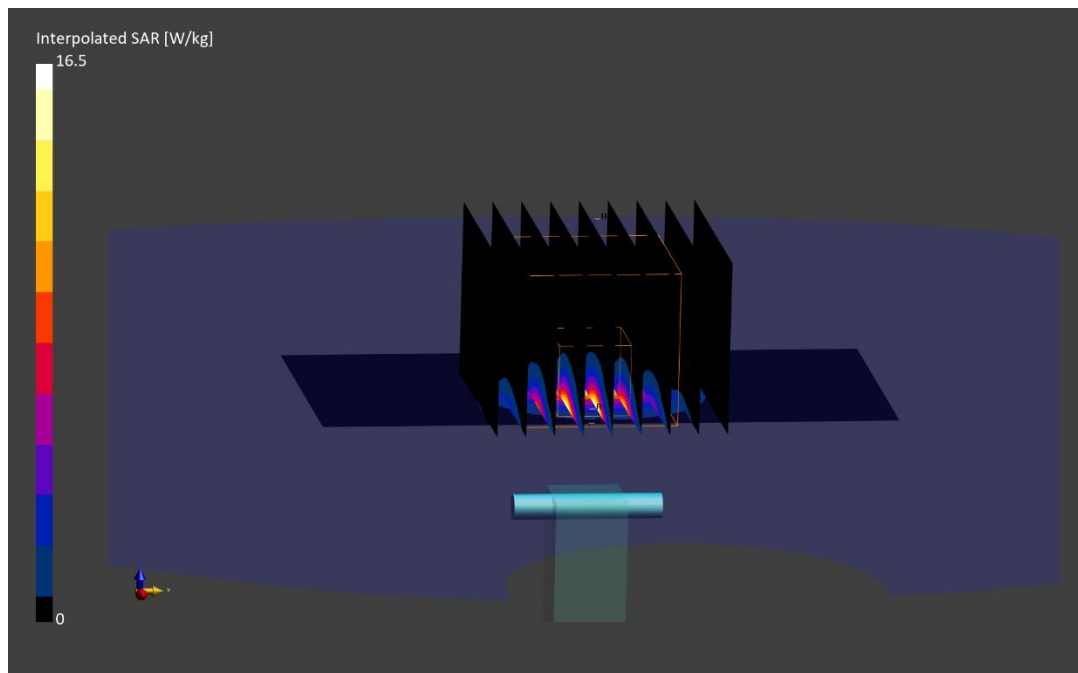

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5750.0 MHz

Medium: 5200-5800 Head; Medium parameters used:

f = 5750.0 MHz; cond = 5.05 S/m; perm = 34.8; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 07/18/2023; Ambient Temp: 22.50°C; Tissue Temp: 20.70°C

Probe: EX3DV4 - SN7420; ConvF:(4.8,4.8,4.8); Calibrated: 2022-10-20

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1333; Calibrated: 2022-10-13

Phantom: Twin-SAM V8.0; Serial: 1736

Measurement SW: DASY Module SAR V16.2.0.1425

5750 MHz System Verification at 17 dBm (50 mW)

Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.0 W/kg

SAR(1 g) = 3.81 W/kg; SAR(10 g) = 1.08 W/kg

Deviation (1 g) = -5.34%; Deviation (10 g) = -4.85%;

