



## Appendix A: Measurement Plots

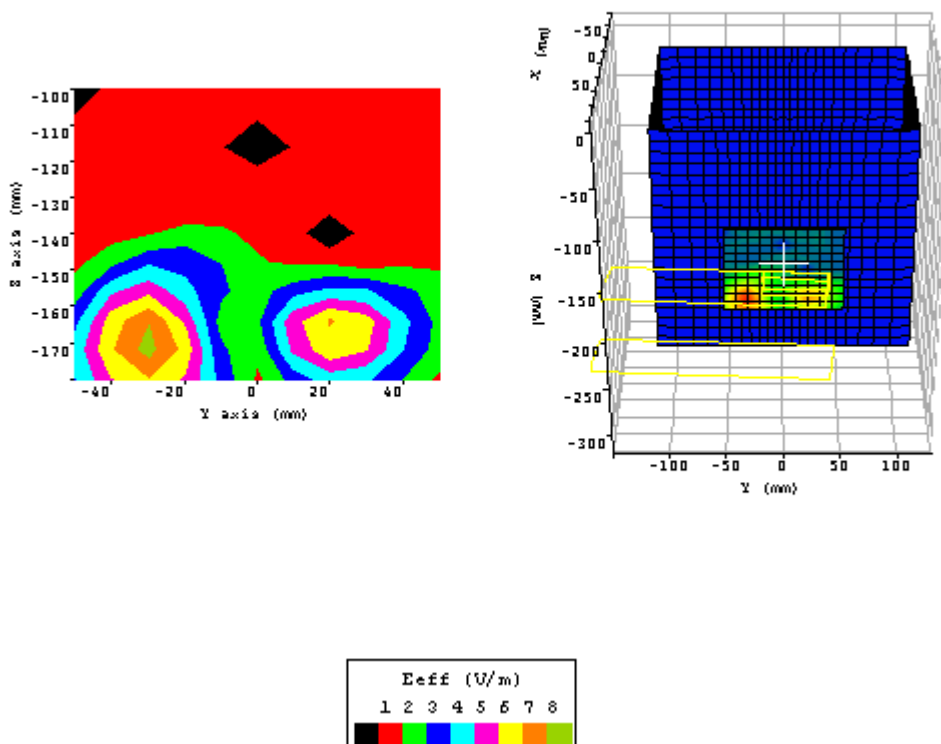

Plot 1.	
Date:	04/08/2003
Temperature Air / Liquid:	21.0°C / 21.0°C
Liquid mass density ( $\rho$ ):	1
DCP <sup>1</sup>	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	$\epsilon_r$ : 51.62 $\sigma$ : 1.961
Transmit Antenna / Test Position	Right / bystander 5mm
Device Frequency	2437 MHz
Maximum 1 gram SAR:	0.166W/Kg
Maximum 10 gram SAR:	0.076/Kg
Power reference start:	0.032W/Kg
Power reference end	0.032W/Kg
Power reference change <sup>2</sup>	-0.00%

<sup>1</sup> DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.


<sup>2</sup> The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

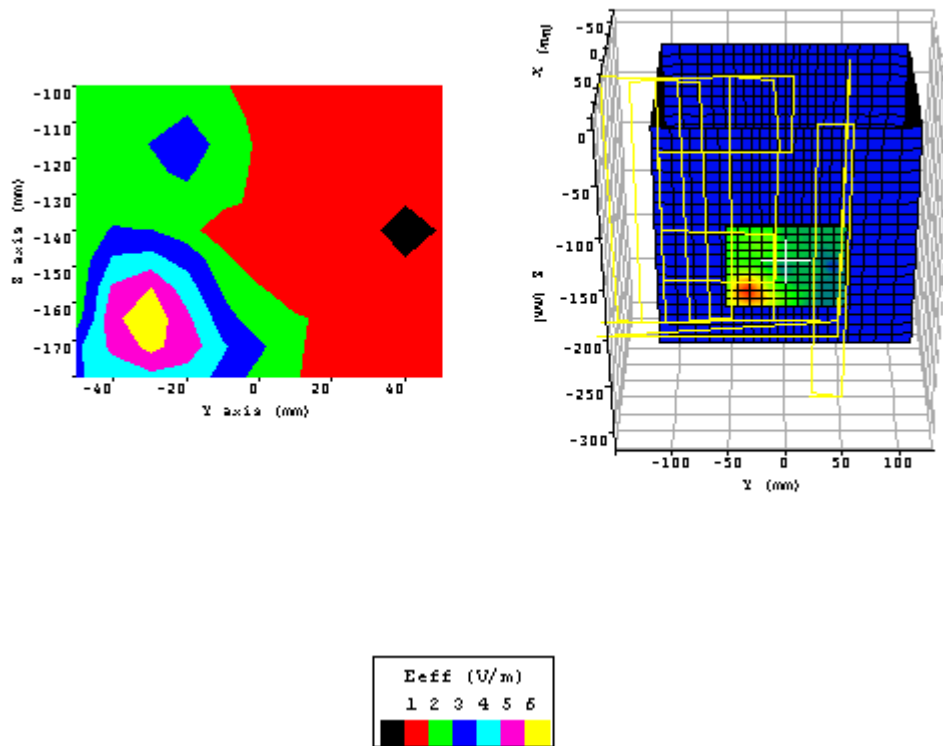

Plot 2.	
Date:	04/08/2003
Temperature Air / Liquid:	22.0°C / 21.0°C
Liquid mass density ( $\rho$ ):	1
DCP <sup>1</sup>	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	$\epsilon_r$ : 51.62 $\sigma$ : 1.961
Transmit Antenna / Test Position	Right / lap
Device Frequency	2437 MHz
Maximum 1 gram SAR:	0.131W/Kg
Maximum 10 gram SAR:	0.063/Kg
Power reference start:	0.028W/Kg
Power reference end	0.028W/Kg
Power reference change <sup>2</sup>	-0.00%

<sup>1</sup> DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.


<sup>2</sup> The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

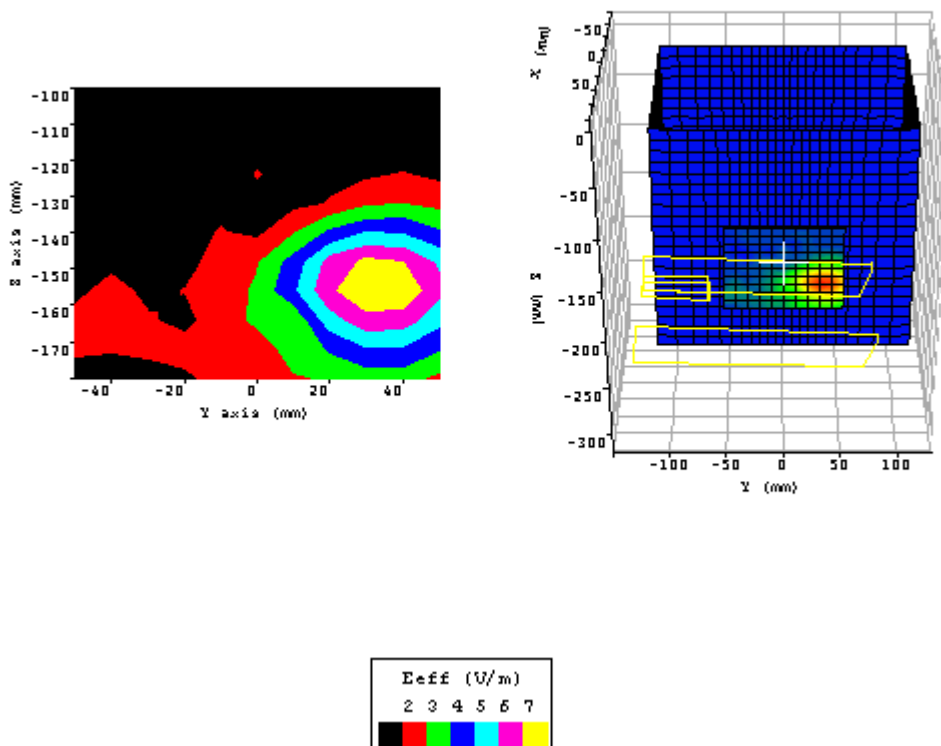

Plot 3.	
Date:	04/08/2003
Temperature Air / Liquid:	22.0°C / 22.0°C
Liquid mass density ( $\rho$ ):	1
DCP <sup>1</sup>	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	$\epsilon_r$ : 51.62 $\sigma$ : 1.961
Transmit Antenna / Test Position	Left / bystander 5mm
Device Frequency	2437 MHz
Maximum 1 gram SAR:	0.143W/Kg
Maximum 10 gram SAR:	0.072W/Kg
Power reference start:	0.029W/Kg
Power reference end	0.029W/Kg
Power reference change <sup>2</sup>	-0.00%

<sup>1</sup> DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.


<sup>2</sup> The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

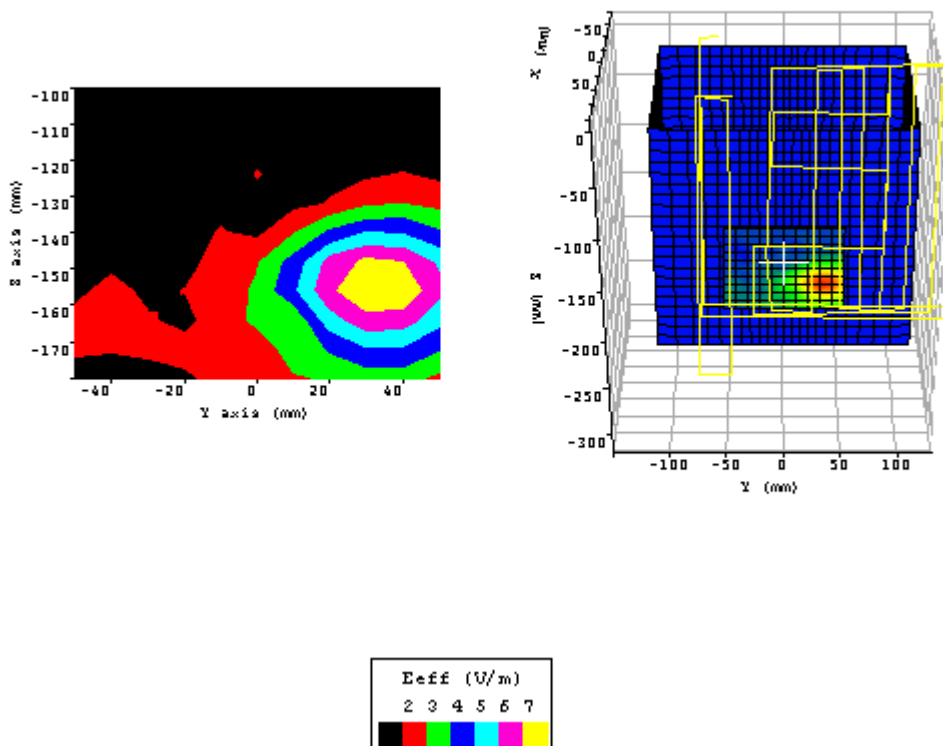

Plot 4.		
Date:	04/08/2003	
Temperature Air / Liquid:	22.0°C / 22.0°C	
Liquid mass density ( $\rho$ ):	1	
DCP <sup>1</sup>	20	
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386	
Probe S/N:0123 liquid/air conversion Factor	0.816	
Simulated tissue dielectric parameters:	$\epsilon_r$ : 51.62	$\sigma$ : 1.961
Transmit Antenna / Test Position	Left / lap	
Device Frequency	2437 MHz	
Maximum 1 gram SAR:	0.054W/Kg	
Maximum 10 gram SAR:	0.030W/Kg	
Power reference start:	0.010W/Kg	
Power reference end	0.010W/Kg	
Power reference change <sup>2</sup>	-0.00%	

<sup>1</sup> DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.


<sup>2</sup> The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

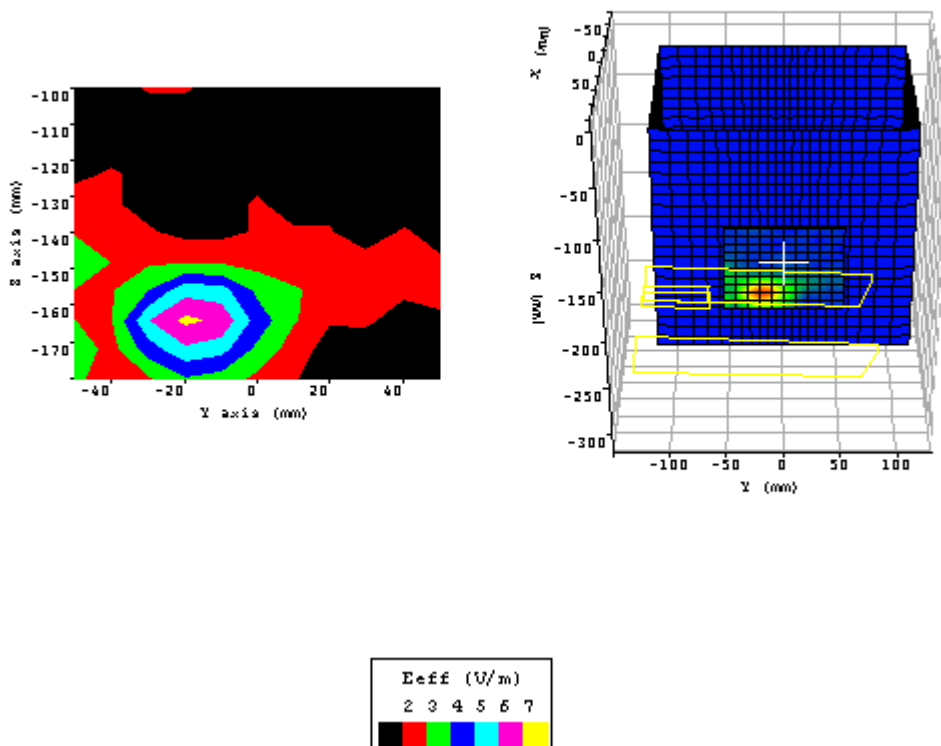

Plot 5.	
Date:	04/08/2003
Temperature Air / Liquid:	22.0°C / 21.0°C
Liquid mass density ( $\rho$ ):	1
DCP <sup>1</sup>	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	$\epsilon_r$ : 51.13 $\sigma$ : 1.951
Transmit Antenna / Test Position	Right / bystander 5mm
Device Frequency	2412 MHz
Maximum 1 gram SAR:	0.135W/Kg
Maximum 10 gram SAR:	0.061W/Kg
Power reference start:	0.032W/Kg
Power reference end	0.032W/Kg
Power reference change <sup>2</sup>	0.00%

<sup>1</sup> DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.

<sup>2</sup> The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

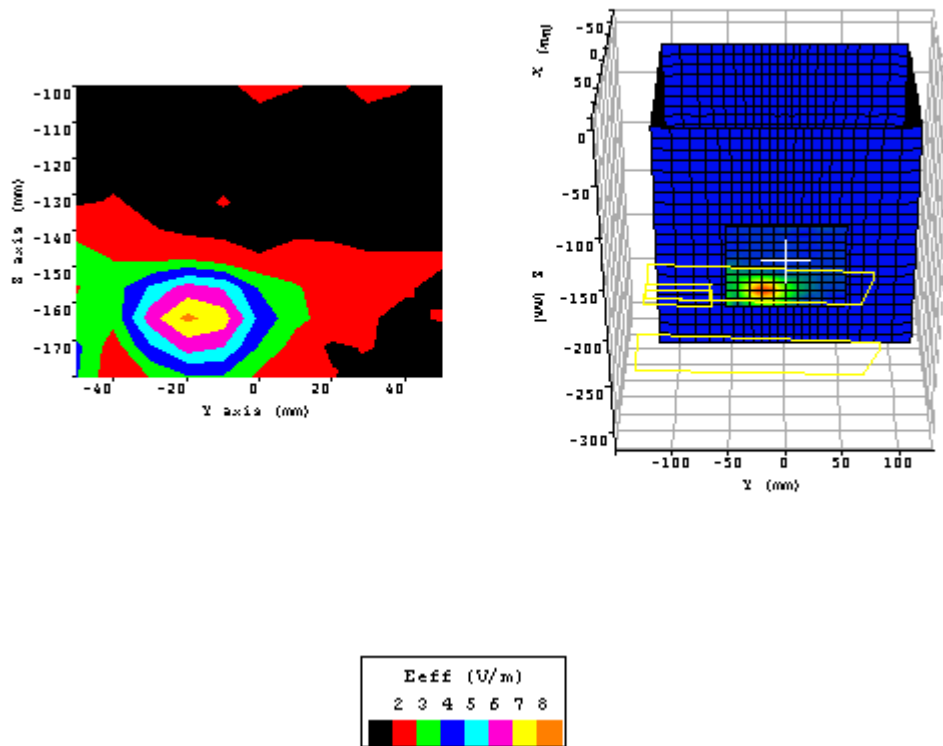

Plot 6.	
Date:	04/08/2003
Temperature Air / Liquid:	22.0°C / 21.0°C
Liquid mass density ( $\rho$ ):	1
DCP <sup>1</sup>	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	$\epsilon_r$ : 51.15 $\sigma$ : 1.961
Transmit Antenna / Test Position	Right / bystander 5mm
Device Frequency	2462 MHz
Maximum 1 gram SAR:	0.180W/Kg
Maximum 10 gram SAR:	0.078W/Kg
Power reference start:	0.036W/Kg
Power reference end	0.036W/Kg
Power reference change <sup>2</sup>	0.00%

<sup>1</sup> DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.

<sup>2</sup> The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.