

EXHIBIT A- RADIATED SPURIOUS EMISSION DATA

Note : Transmit frequency is ignore ,mark →

30M-1G

BLE-Horizontal-TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.59.38

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

RÉmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_30MHz-1GHz

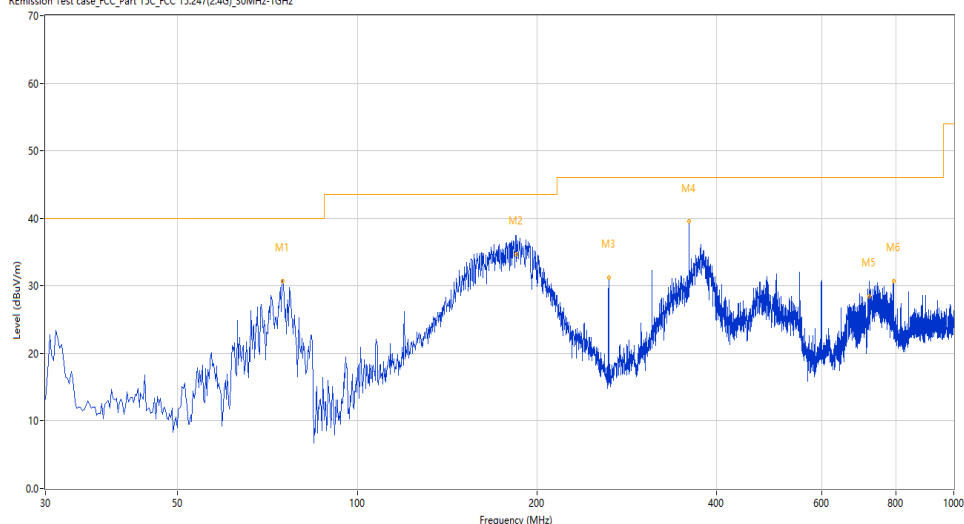

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	75.064	37.52	-30.92	40.0	2.48	Peak	359.10	246	Horizontal	Pass
1*	75.064	30.74	-30.92	40.0	9.26	QP	359.10	246	Horizontal	Pass
2	184.832	38.11	-27.54	43.5	5.39	Peak	2.10	185	Horizontal	Pass
2*	184.832	34.71	-27.54	43.5	8.79	QP	2.10	185	Horizontal	Pass
3	263.999	32.38	-23.84	46.0	13.62	Peak	62.60	135	Horizontal	Pass
3*	263.999	31.24	-23.84	46.0	14.76	QP	62.60	135	Horizontal	Pass
4	359.999	40.60	-21.87	46.0	5.40	Peak	105.40	100	Horizontal	Pass
4*	359.999	39.62	-21.87	46.0	6.38	QP	105.40	100	Horizontal	Pass
5	720.989	31.84	-12.84	46.0	14.16	Peak	319.80	113	Horizontal	Pass
5*	720.989	28.42	-12.84	46.0	17.58	QP	319.80	113	Horizontal	Pass
6	791.998	34.09	-11.86	46.0	11.91	Peak	103.50	104	Horizontal	Pass
6*	791.998	30.75	-11.86	46.0	15.25	QP	103.50	104	Horizontal	Pass

BLE-Vertical-TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.44.57

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_30MHz-1GHz

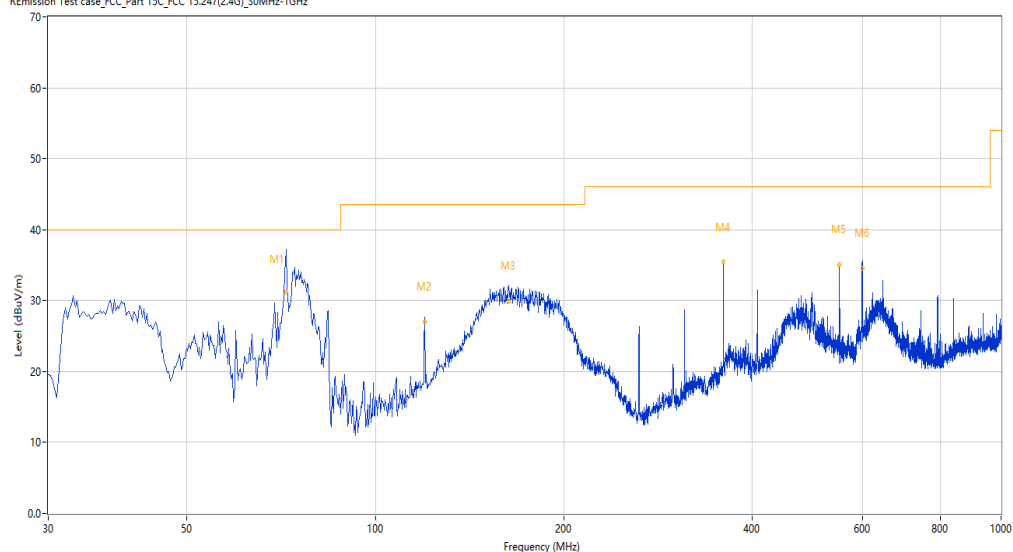

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	72.000	39.19	-30.00	40.0	0.81	Peak	0.00	100	Vertical	Pass
1*	72.000	31.24	-30.00	40.0	8.76	QP	0.00	100	Vertical	Pass
2	120.000	28.22	-28.11	43.5	15.28	Peak	83.10	108	Vertical	Pass
2*	120.000	27.05	-28.11	43.5	16.45	QP	83.10	108	Vertical	Pass
3	163.396	32.94	-29.06	43.5	10.56	Peak	160.40	100	Vertical	Pass
3*	163.396	29.94	-29.06	43.5	13.56	QP	160.40	100	Vertical	Pass
4	359.999	38.52	-21.87	46.0	7.48	Peak	47.00	131	Vertical	Pass
4*	359.999	35.52	-21.87	46.0	10.48	QP	47.00	131	Vertical	Pass
5	551.999	36.18	-16.99	46.0	9.82	Peak	236.40	115	Vertical	Pass
5*	551.999	35.06	-16.99	46.0	10.94	QP	236.40	115	Vertical	Pass
6	599.998	36.26	-14.77	46.0	9.74	Peak	0.00	100	Vertical	Pass
6*	599.998	34.49	-14.77	46.0	11.51	QP	0.00	100	Vertical	Pass

1-18G

BLE-Low channel-Horizontal-TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.19.55

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_1GHz-7GHz RSE

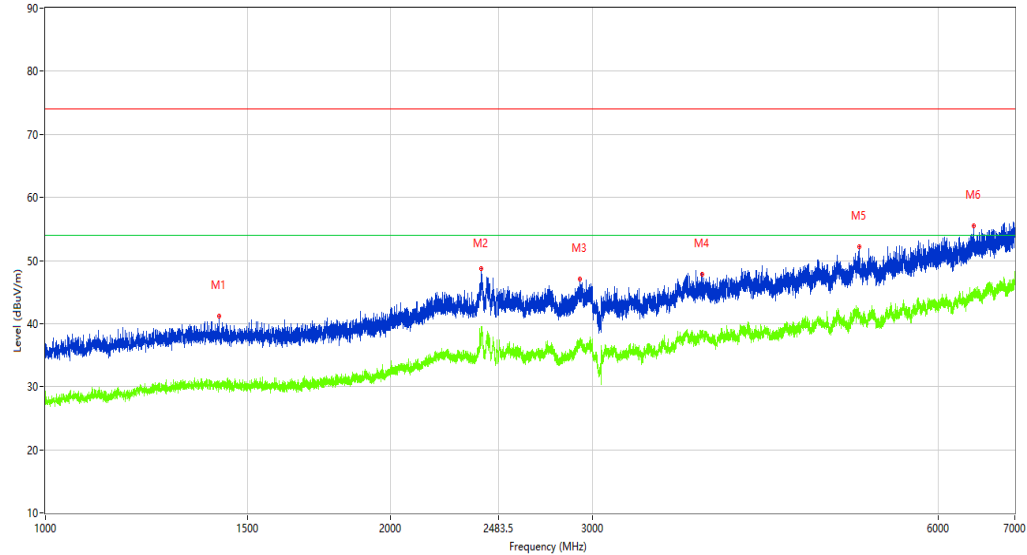

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	1416.250	41.22	-13.50	74.0	32.78	Peak	179.80	100	Horizontal	Pass
1**	1416.250	29.86	-13.50	54.0	24.14	AV	179.80	100	Horizontal	Pass
2	2399.250	48.75	-4.93	74.0	25.25	Peak	0.00	100	Horizontal	Pass
2**	2399.250	38.79	-4.93	54.0	15.21	AV	0.00	100	Horizontal	Pass
3	2923.250	47.01	-5.29	74.0	26.99	Peak	0.00	100	Horizontal	Pass
3**	2923.250	36.97	-5.29	54.0	17.03	AV	0.00	100	Horizontal	Pass
4	3737.000	47.79	-2.78	74.0	26.21	Peak	360.00	100	Horizontal	Pass
4**	3737.000	37.26	-2.78	54.0	16.74	AV	360.00	100	Horizontal	Pass
5	5121.500	52.23	0.10	74.0	21.77	Peak	253.20	100	Horizontal	Pass
5**	5121.500	40.33	0.10	54.0	13.67	AV	253.20	100	Horizontal	Pass
6	6447.500	55.57	3.06	74.0	18.43	Peak	236.50	100	Horizontal	Pass
6**	6447.500	45.18	3.06	54.0	8.82	AV	236.50	100	Horizontal	Pass

Test result

Project Number: Certification

Test Time: 2024-11-12_15.40.26

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247_7GHz-18GHz

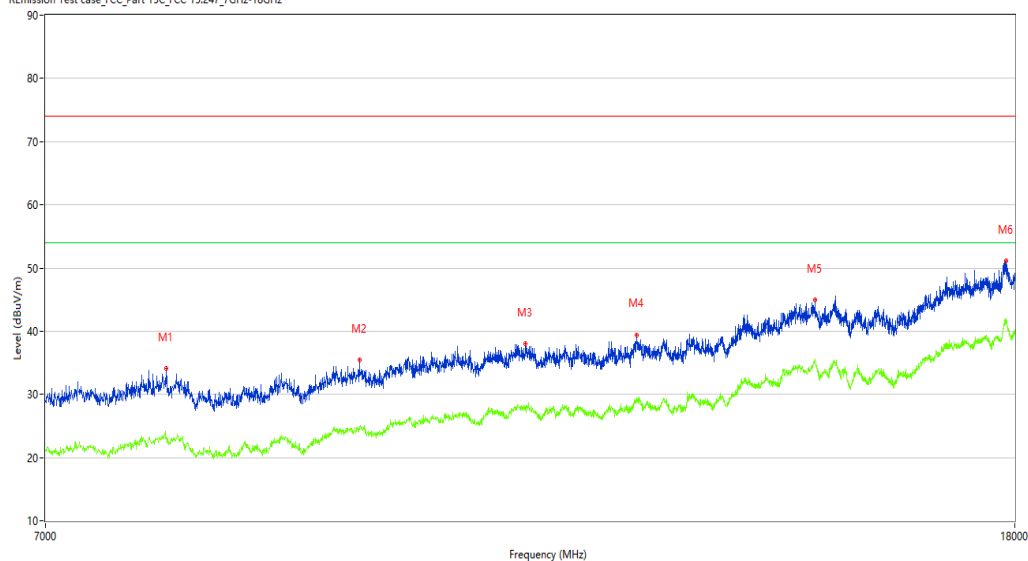

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	7874.500	34.11	0.95	74.0	39.89	Peak	217.80	100	Horizontal	Pass
1**	7874.500	23.21	0.95	54.0	30.79	AV	217.80	100	Horizontal	Pass
2	9505.250	35.51	2.48	74.0	38.49	Peak	292.50	100	Horizontal	Pass
2**	9505.250	24.88	2.48	54.0	29.12	AV	292.50	100	Horizontal	Pass
3	11174.500	38.02	4.08	74.0	35.98	Peak	359.10	100	Horizontal	Pass
3**	11174.500	28.07	4.08	54.0	25.93	AV	359.10	100	Horizontal	Pass
4	12450.500	39.45	4.88	74.0	34.55	Peak	128.50	100	Horizontal	Pass
4**	12450.500	29.33	4.88	54.0	24.67	AV	128.50	100	Horizontal	Pass
5	14815.500	44.92	11.67	74.0	29.08	Peak	109.90	100	Horizontal	Pass
5**	14815.500	35.20	11.67	54.0	18.80	AV	109.90	100	Horizontal	Pass
6	17846.000	51.10	15.96	74.0	22.90	Peak	92.40	100	Horizontal	Pass
6**	17846.000	41.57	15.96	54.0	12.43	AV	92.40	100	Horizontal	Pass

BLE-Low channel-Vertical-TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.16.48

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_1GHz-7GHz RSE

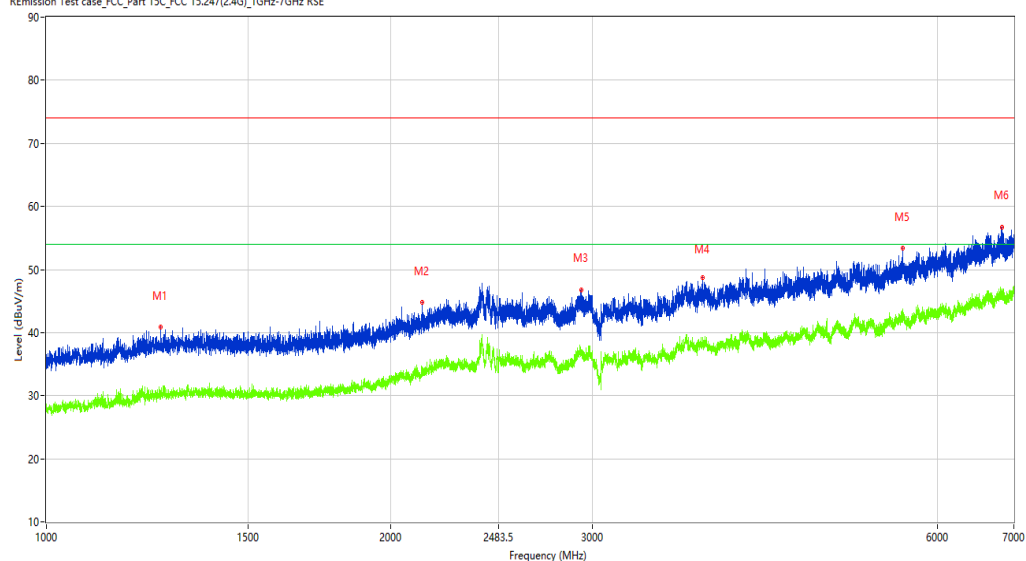

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	1258.250	40.91	-14.04	74.0	33.09	Peak	0.00	100	Vertical	Pass
1**	1258.250	30.86	-14.04	54.0	23.14	AV	0.00	100	Vertical	Pass
2	2128.750	44.82	-10.23	74.0	29.18	Peak	251.90	100	Vertical	Pass
2**	2128.750	33.59	-10.23	54.0	20.41	AV	251.90	100	Vertical	Pass
3	2930.500	46.82	-5.26	74.0	27.18	Peak	282.80	100	Vertical	Pass
3**	2930.500	36.77	-5.26	54.0	17.23	AV	282.80	100	Vertical	Pass
4	3742.000	48.78	-2.59	74.0	25.22	Peak	298.70	100	Vertical	Pass
4**	3742.000	38.34	-2.59	54.0	15.66	AV	298.70	100	Vertical	Pass
5	5598.000	53.32	1.01	74.0	20.68	Peak	280.00	100	Vertical	Pass
5**	5598.000	42.58	1.01	54.0	11.42	AV	280.00	100	Vertical	Pass
6	6836.500	56.66	4.02	74.0	17.34	Peak	315.40	100	Vertical	Pass
6**	6836.500	46.46	4.02	54.0	7.54	AV	315.40	100	Vertical	Pass

Test result

Project Number: Certification

Test Time: 2024-11-12_15.30.00

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+


Work Addition: TX

Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

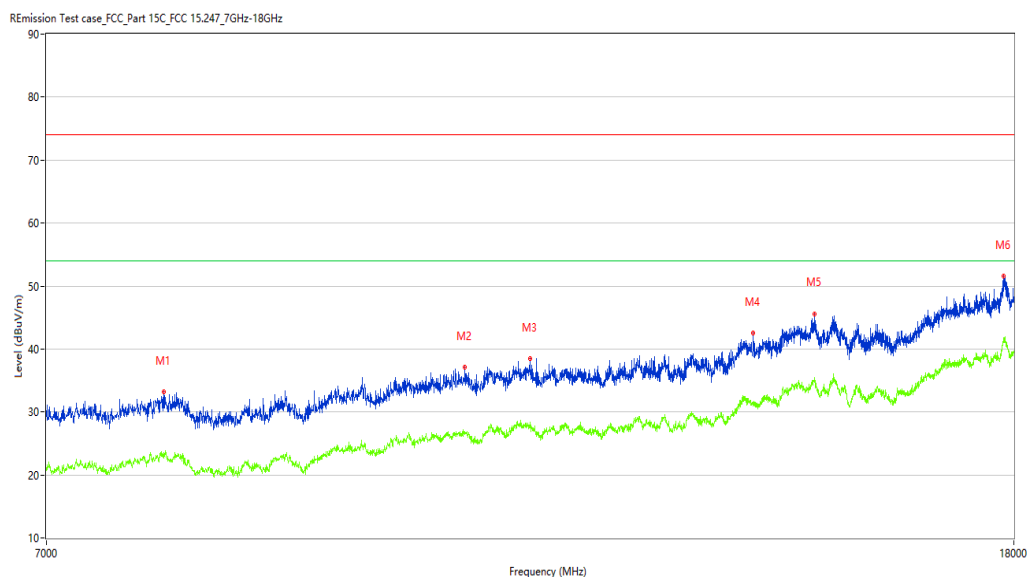

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	7847.000	33.15	1.03	74.0	40.85	Peak	38.50	100	Vertical	Pass
1**	7847.000	23.37	1.03	54.0	30.63	AV	38.50	100	Vertical	Pass
2	10531.000	37.06	4.06	74.0	36.94	Peak	0.00	100	Vertical	Pass
2**	10531.000	26.50	4.06	54.0	27.50	AV	0.00	100	Vertical	Pass
3	11224.001	38.51	4.27	74.0	35.49	Peak	38.50	100	Vertical	Pass
3**	11224.001	28.31	4.27	54.0	25.69	AV	38.50	100	Vertical	Pass
4	13954.750	42.50	8.49	74.0	31.50	Peak	307.90	100	Vertical	Pass
4**	13954.750	30.88	8.49	54.0	23.12	AV	307.90	100	Vertical	Pass
5	14821.000	45.62	11.44	74.0	28.38	Peak	290.40	100	Vertical	Pass
5**	14821.000	35.43	11.44	54.0	18.57	AV	290.40	100	Vertical	Pass
6	17826.750	51.51	15.60	74.0	22.49	Peak	0.00	100	Vertical	Pass
6**	17826.750	41.74	15.60	54.0	12.26	AV	0.00	100	Vertical	Pass

BLE-Middle channel-Horizontal-TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.30.16

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

R/Emission Test case_FCC_Part 15C_FCC 15.247(2.4G)_1GHz-7GHz RSE

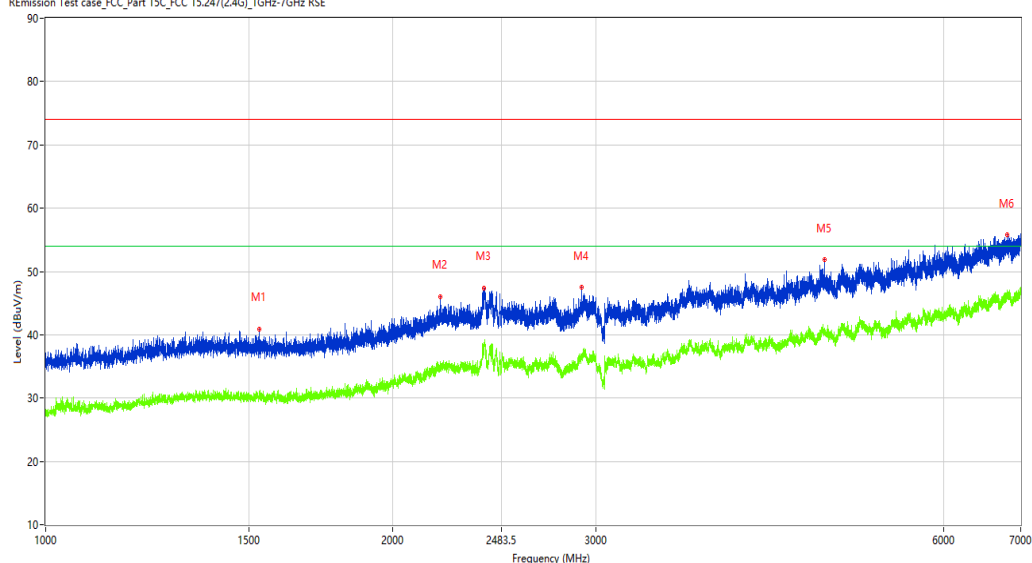

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	1531.500	40.96	-13.80	74.0	33.04	Peak	0.00	100	Horizontal	Pass
1**	1531.500	30.54	-13.80	54.0	23.46	AV	0.00	100	Horizontal	Pass
2	2199.500	45.94	-8.55	74.0	28.06	Peak	169.80	100	Horizontal	Pass
2**	2199.500	35.23	-8.55	54.0	18.77	AV	169.80	100	Horizontal	Pass
3	2400.000	47.44	-4.93	74.0	26.56	Peak	281.40	100	Horizontal	Pass
3**	2400.000	38.76	-4.93	54.0	15.24	AV	281.40	100	Horizontal	Pass
4	2912.250	47.47	-5.06	74.0	26.53	Peak	136.60	100	Horizontal	Pass
4**	2912.250	36.74	-5.06	54.0	17.26	AV	136.60	100	Horizontal	Pass
5	4731.000	51.83	-0.60	74.0	22.17	Peak	334.00	100	Horizontal	Pass
5**	4731.000	40.68	-0.60	54.0	13.32	AV	334.00	100	Horizontal	Pass
6	6818.500	55.78	4.26	74.0	18.22	Peak	249.90	100	Horizontal	Pass
6**	6818.500	46.04	4.26	54.0	7.96	AV	249.90	100	Horizontal	Pass

Test result

Project Number: Certification

Test Time: 2024-11-12_15.41.55

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247_7GHz-18GHz

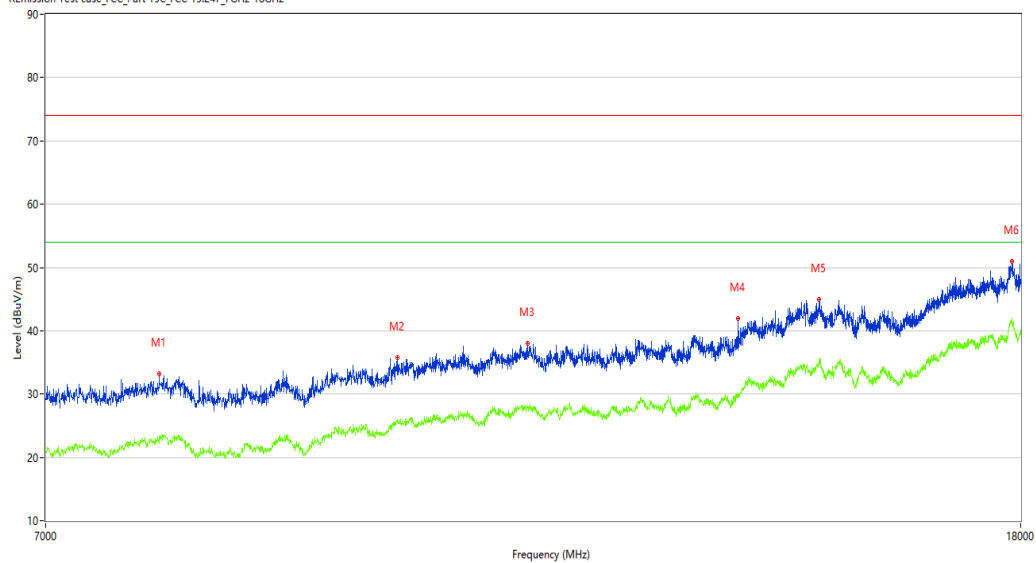

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	7814.000	33.15	0.52	74.0	40.85	Peak	52.00	100	Horizontal	Pass
1**	7814.000	22.96	0.52	54.0	31.04	AV	52.00	100	Horizontal	Pass
2	9840.750	35.78	3.06	74.0	38.22	Peak	126.80	100	Horizontal	Pass
2**	9840.750	25.64	3.06	54.0	28.36	AV	126.80	100	Horizontal	Pass
3	11160.750	37.99	4.08	74.0	36.01	Peak	198.00	100	Horizontal	Pass
3**	11160.750	28.01	4.08	54.0	25.99	AV	198.00	100	Horizontal	Pass
4	13693.500	41.92	7.14	74.0	32.08	Peak	215.90	100	Horizontal	Pass
4**	13693.500	29.75	7.14	54.0	24.25	AV	215.90	100	Horizontal	Pass
5	14801.750	44.98	11.27	74.0	29.02	Peak	271.40	100	Horizontal	Pass
5**	14801.750	34.51	11.27	54.0	19.49	AV	271.40	100	Horizontal	Pass
6	17848.750	50.91	15.91	74.0	23.09	Peak	87.30	100	Horizontal	Pass
6**	17848.750	41.88	15.91	54.0	12.12	AV	87.30	100	Horizontal	Pass

BLE-Middle channel-Vertical-TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.41.02

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_1GHz-7GHz RSE

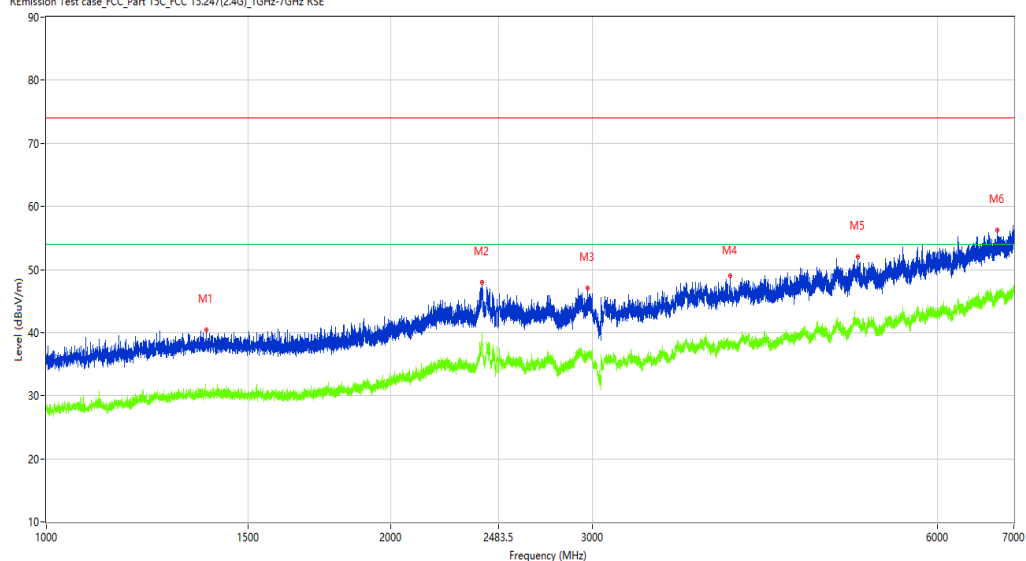

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	1379.500	40.43	-13.51	74.0	33.57	Peak	360.00	100	Vertical	Pass
1**	1379.500	30.53	-13.51	54.0	23.47	AV	360.00	100	Vertical	Pass
2	2403.000	47.91	-4.93	74.0	26.09	Peak	34.00	100	Vertical	Pass
2**	2403.000	38.09	-4.93	54.0	15.91	AV	34.00	100	Vertical	Pass
3	2970.750	47.09	-4.69	74.0	26.91	Peak	147.40	100	Vertical	Pass
3**	2970.750	36.30	-4.69	54.0	17.70	AV	147.40	100	Vertical	Pass
4	3958.000	49.06	-2.41	74.0	24.94	Peak	0.00	100	Vertical	Pass
4**	3958.000	38.22	-2.41	54.0	15.78	AV	0.00	100	Vertical	Pass
5	5113.500	51.99	0.24	74.0	22.01	Peak	78.10	100	Vertical	Pass
5**	5113.500	41.94	0.24	54.0	12.06	AV	78.10	100	Vertical	Pass
6	6768.000	56.25	3.69	74.0	17.75	Peak	145.40	100	Vertical	Pass
6**	6768.000	45.88	3.69	54.0	8.12	AV	145.40	100	Vertical	Pass

Test result

Project Number: Certification

Test Time: 2024-11-12_15.27.12

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

R Emission Test case_FCC_Part 15C_FCC 15.247_7GHz-18GHz

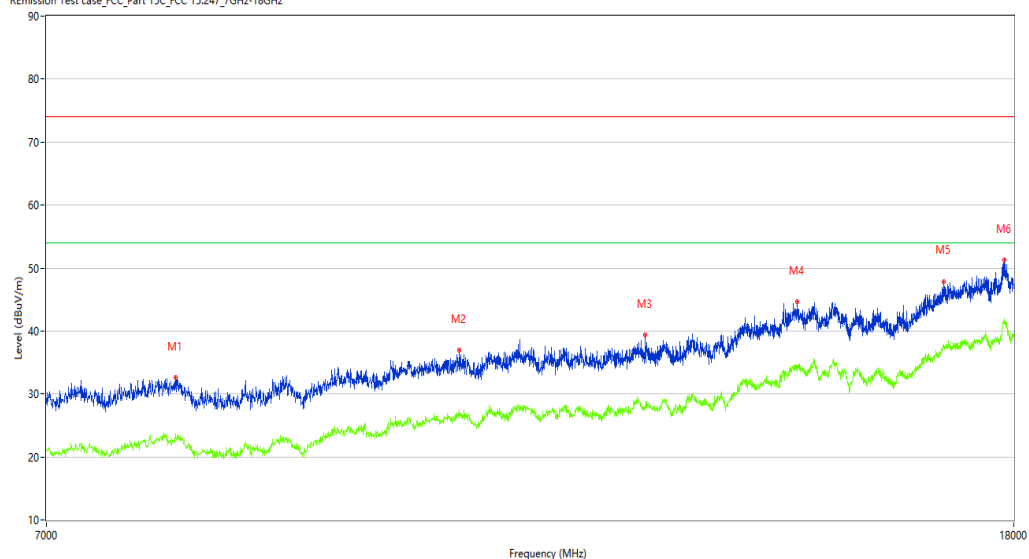

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	7940.500	32.63	0.60	74.0	41.37	Peak	216.60	100	Vertical	Pass
1**	7940.500	23.69	0.60	54.0	30.31	AV	216.60	100	Vertical	Pass
2	10473.250	36.90	3.87	74.0	37.10	Peak	360.00	100	Vertical	Pass
2**	10473.250	27.49	3.87	54.0	26.51	AV	360.00	100	Vertical	Pass
3	12563.250	39.44	4.60	74.0	34.56	Peak	253.10	100	Vertical	Pass
3**	12563.250	28.28	4.60	54.0	25.72	AV	253.10	100	Vertical	Pass
4	14570.750	44.58	9.57	74.0	29.42	Peak	253.10	100	Vertical	Pass
4**	14570.750	33.48	9.57	54.0	20.52	AV	253.10	100	Vertical	Pass
5	16809.250	47.88	12.50	74.0	26.12	Peak	142.50	100	Vertical	Pass
5**	16809.250	37.43	12.50	54.0	16.57	AV	142.50	100	Vertical	Pass
6	17829.501	51.29	15.63	74.0	22.71	Peak	253.10	100	Vertical	Pass
6**	17829.501	41.31	15.63	54.0	12.69	AV	253.10	100	Vertical	Pass

BLE-High channel-Horizontal-TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.26.24

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

R Emission Test case_FCC_Part 15C_FCC 15.247(2.4G)_1GHz-7GHz RSE

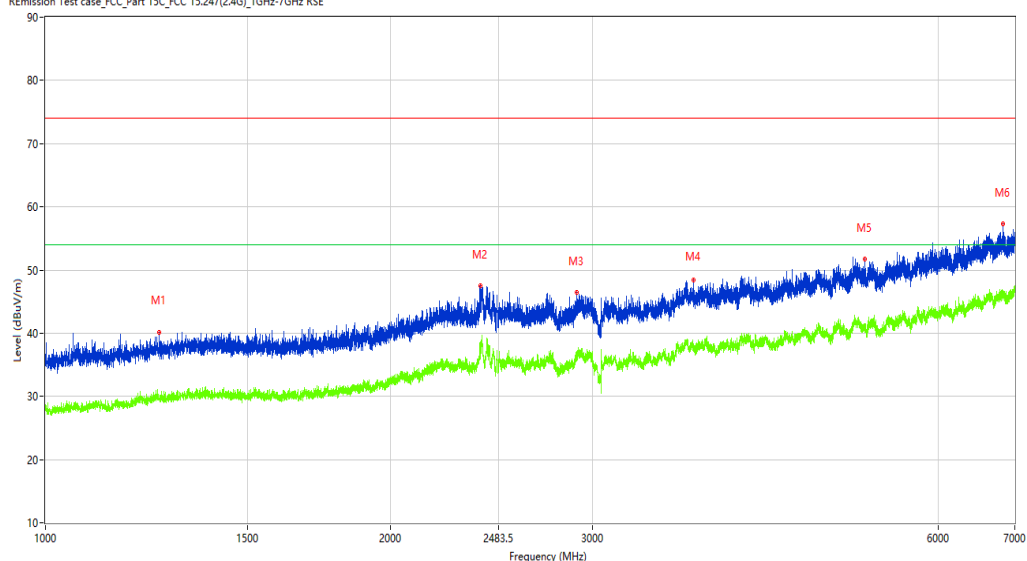

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	1256.250	40.20	-14.08	74.0	33.80	Peak	83.10	100	Horizontal	Pass
1**	1256.250	29.68	-14.08	54.0	24.32	AV	83.10	100	Horizontal	Pass
2	2392.500	47.49	-4.88	74.0	26.51	Peak	99.40	100	Horizontal	Pass
2**	2392.500	38.62	-4.88	54.0	15.38	AV	99.40	100	Horizontal	Pass
3	2903.500	46.47	-5.08	74.0	27.53	Peak	68.50	100	Horizontal	Pass
3**	2903.500	36.50	-5.08	54.0	17.50	AV	68.50	100	Horizontal	Pass
4	3671.500	48.35	-3.14	74.0	25.65	Peak	353.00	100	Horizontal	Pass
4**	3671.500	37.70	-3.14	54.0	16.30	AV	353.00	100	Horizontal	Pass
5	5181.000	51.67	-0.60	74.0	22.33	Peak	197.40	100	Horizontal	Pass
5**	5181.000	41.35	-0.60	54.0	12.65	AV	197.40	100	Horizontal	Pass
6	6830.500	57.38	4.17	74.0	16.62	Peak	267.40	100	Horizontal	Pass
6**	6830.500	45.96	4.17	54.0	8.04	AV	267.40	100	Horizontal	Pass

Test result

Project Number: Certification

Test Time: 2024-11-12_15.36.08

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247_7GHz-18GHz

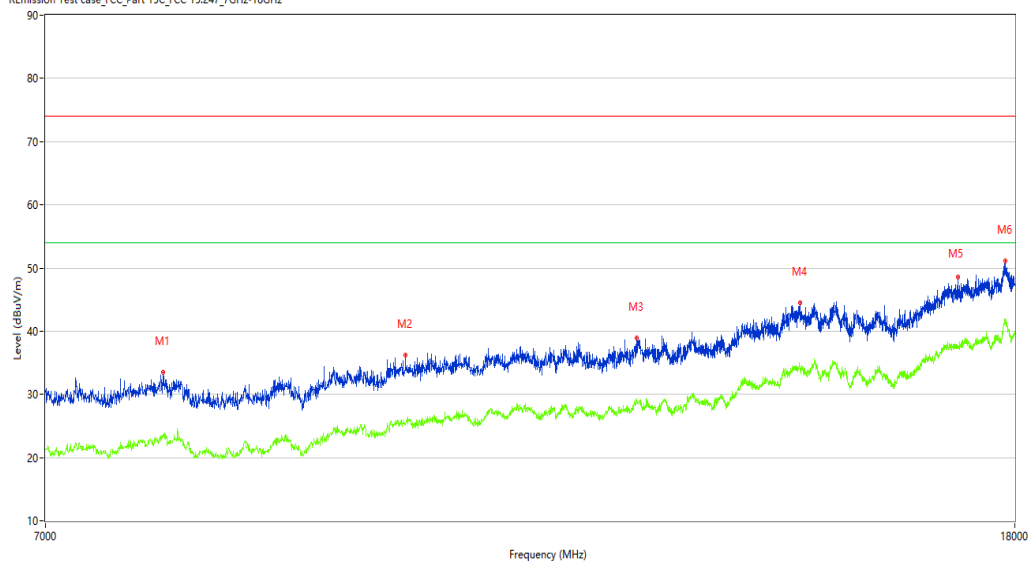

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	7852.500	33.51	1.06	74.0	40.49	Peak	320.00	100	Horizontal	Pass
1**	7852.500	23.28	1.06	54.0	30.72	AV	320.00	100	Horizontal	Pass
2	9939.750	36.21	3.32	74.0	37.79	Peak	0.00	100	Horizontal	Pass
2**	9939.750	25.17	3.32	54.0	28.83	AV	0.00	100	Horizontal	Pass
3	12455.999	38.85	5.00	74.0	35.15	Peak	301.80	100	Horizontal	Pass
3**	12455.999	29.25	5.00	54.0	24.75	AV	301.80	100	Horizontal	Pass
4	14598.250	44.49	10.65	74.0	29.51	Peak	171.50	100	Horizontal	Pass
4**	14598.250	34.43	10.65	54.0	19.57	AV	171.50	100	Horizontal	Pass
5	17026.500	48.56	13.41	74.0	25.44	Peak	283.20	100	Horizontal	Pass
5**	17026.500	37.63	13.41	54.0	16.37	AV	283.20	100	Horizontal	Pass
6	17829.501	51.09	15.63	74.0	22.91	Peak	0.00	100	Horizontal	Pass
6**	17829.501	41.89	15.63	54.0	12.11	AV	0.00	100	Horizontal	Pass

BLE-High channel-Vertical-TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.36.53

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_1GHz-7GHz RSE

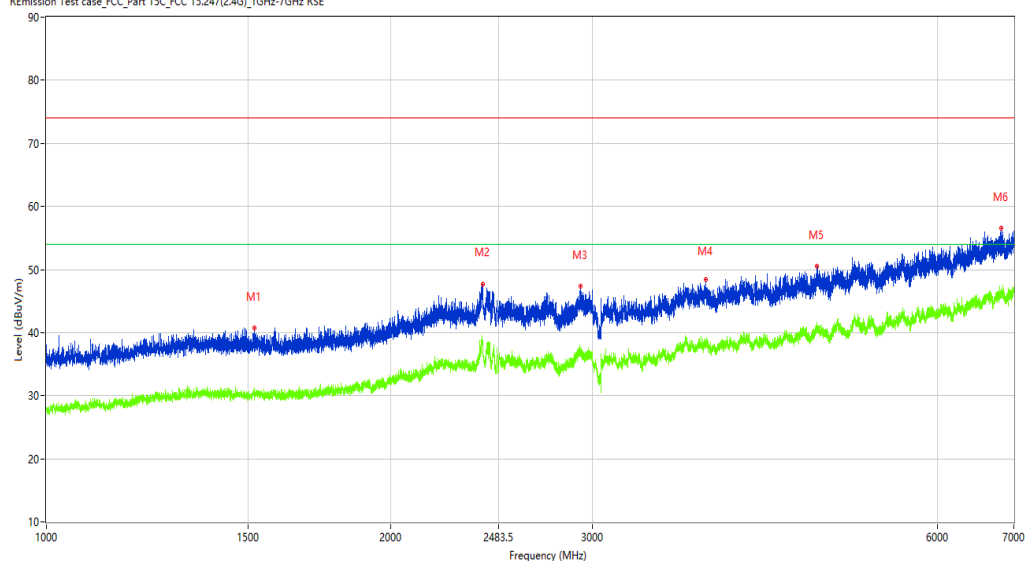

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	1520.000	40.68	-13.78	74.0	33.32	Peak	116.50	100	Vertical	Pass
1**	1520.000	31.20	-13.78	54.0	22.80	AV	116.50	100	Vertical	Pass
2	2404.250	47.72	-5.01	74.0	26.28	Peak	189.80	100	Vertical	Pass
2**	2404.250	38.27	-5.01	54.0	15.73	AV	189.80	100	Vertical	Pass
3	2928.500	47.30	-5.32	74.0	26.70	Peak	219.20	100	Vertical	Pass
3**	2928.500	36.22	-5.32	54.0	17.78	AV	219.20	100	Vertical	Pass
4	3766.000	48.40	-2.62	74.0	25.60	Peak	0.00	100	Vertical	Pass
4**	3766.000	38.05	-2.62	54.0	15.95	AV	0.00	100	Vertical	Pass
5	4709.500	50.52	-0.79	74.0	23.48	Peak	198.50	100	Vertical	Pass
5**	4709.500	40.78	-0.79	54.0	13.22	AV	198.50	100	Vertical	Pass
6	6827.000	56.49	4.24	74.0	17.51	Peak	315.00	100	Vertical	Pass
6**	6827.000	45.96	4.24	54.0	8.04	AV	315.00	100	Vertical	Pass

Test result

Project Number: Certification

Test Time: 2024-11-12_15.17.43

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+


Work Addition: TX

Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

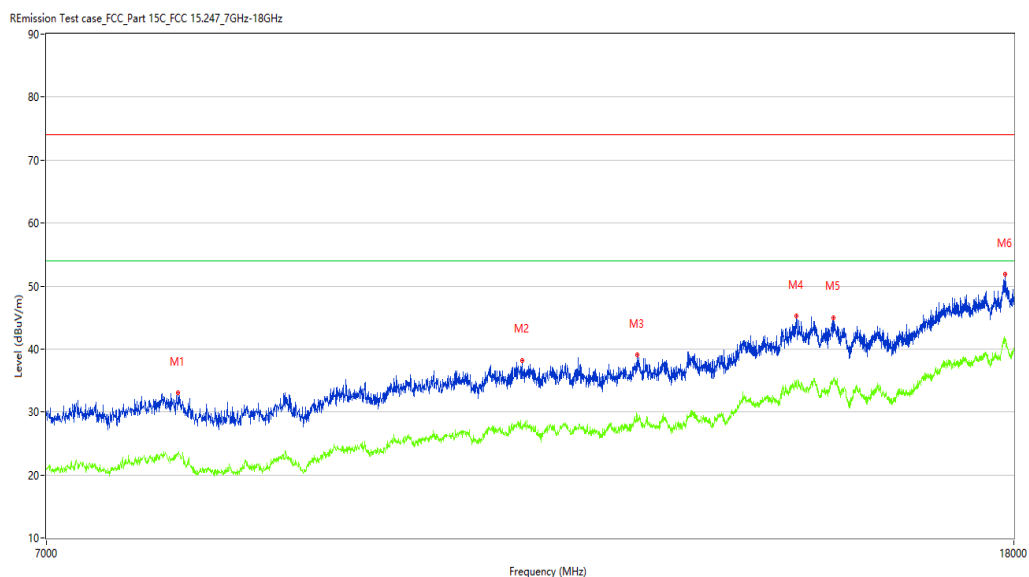

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	7959.750	33.09	1.13	74.0	40.91	Peak	0.00	100	Vertical	Pass
1**	7959.750	22.94	1.13	54.0	31.06	AV	0.00	100	Vertical	Pass
2	11136.000	38.10	4.14	74.0	35.90	Peak	360.00	100	Vertical	Pass
2**	11136.000	27.77	4.14	54.0	26.23	AV	360.00	100	Vertical	Pass
3	12461.500	39.08	5.03	74.0	34.92	Peak	160.30	100	Vertical	Pass
3**	12461.500	28.96	5.03	54.0	25.04	AV	160.30	100	Vertical	Pass
4	14559.750	45.20	9.77	74.0	28.80	Peak	160.30	100	Vertical	Pass
4**	14559.750	34.73	9.77	54.0	19.27	AV	160.30	100	Vertical	Pass
5	15096.001	44.89	10.09	74.0	29.11	Peak	319.90	100	Vertical	Pass
5**	15096.001	34.96	10.09	54.0	19.04	AV	319.90	100	Vertical	Pass
6	17843.249	51.92	15.69	74.0	22.08	Peak	160.30	100	Vertical	Pass
6**	17843.249	41.26	15.69	54.0	12.74	AV	160.30	100	Vertical	Pass

BLE-Bandedge -Low channel- Horizontal -TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.21.41

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_bandedge 2400

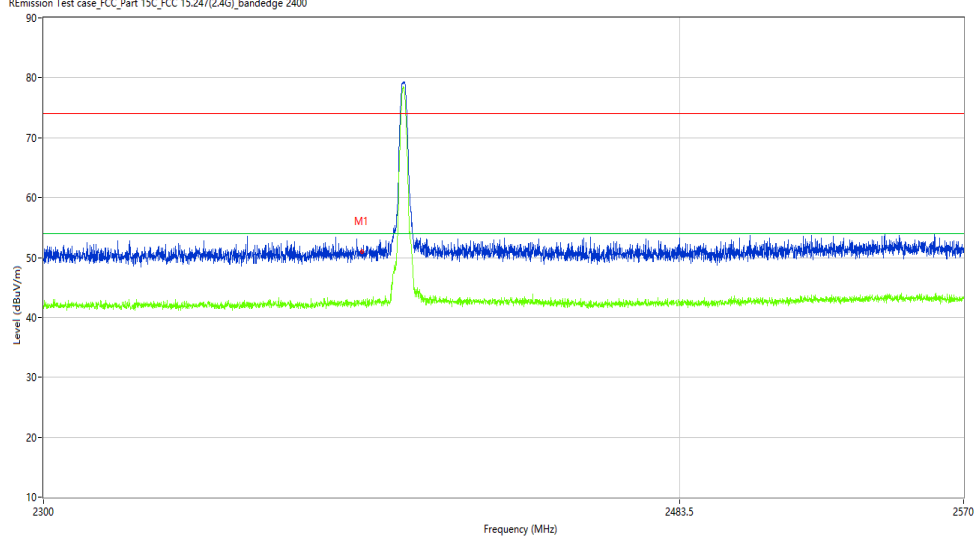

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	2390.000	51.05	-10.74	74.0	22.95	Peak	330.84	100	H	Pass
1**	2390.000	42.32	-10.74	54.0	11.68	AV	330.84	100	H	Pass

BLE-Bandedge -Low channel- Vertical -TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.15.13

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_bandedge 2400

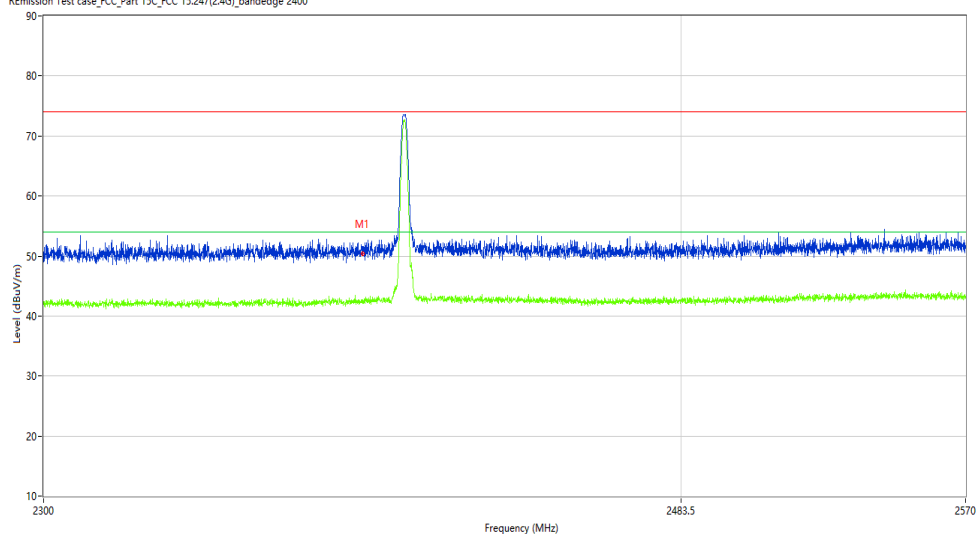

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	2390.000	50.41	-10.74	74.0	23.59	Peak	359.04	100	V	Pass
1**	2390.000	42.18	-10.74	54.0	11.82	AV	359.04	100	V	Pass

BLE-Bandedge -High channel- Horizontal –TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.25.09

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_bandedge 2400

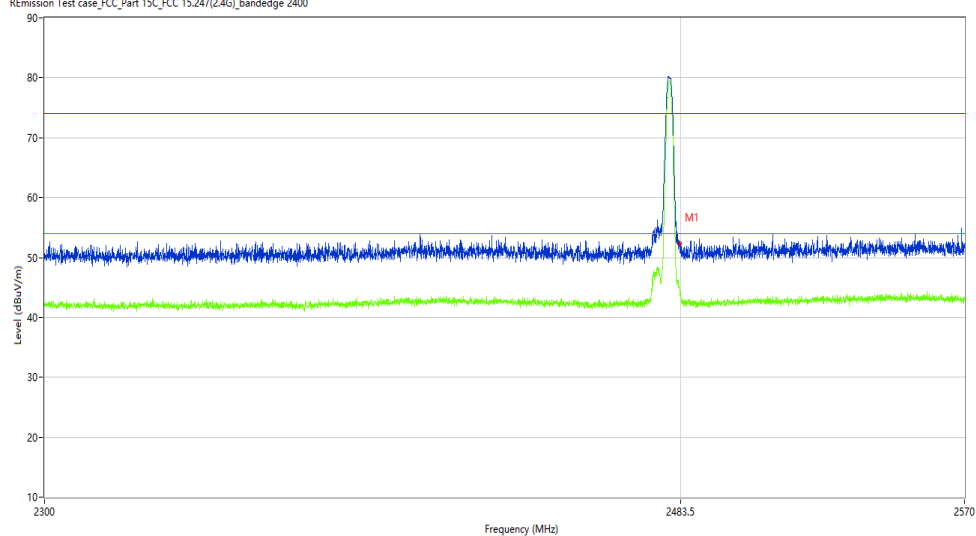

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	2483.500	51.84	-10.74	74.0	22.16	Peak	196.42	100	H	Pass
1**	2483.500	42.49	-10.74	54.0	11.51	AV	196.42	100	H	Pass

BLE-Bandedge -High channel- Vertical –TX

Test result

Project Number: Certification

Test Time: 2024-11-12_14.39.25

EUT Name: Blood Glucose Meter

Test Engineer: CJY

Manufacturer: N.A

Test Standard: FCC

Model: 1018U+

Work Addition: TX


Temp.(oC): 25.1

Load: Full load

Hum.: 47%RH

Remark: DR-RF01-H24110002-01#02

REmission Test case_FCC_Part 15C_FCC 15.247(2.4G)_bandedge 2400

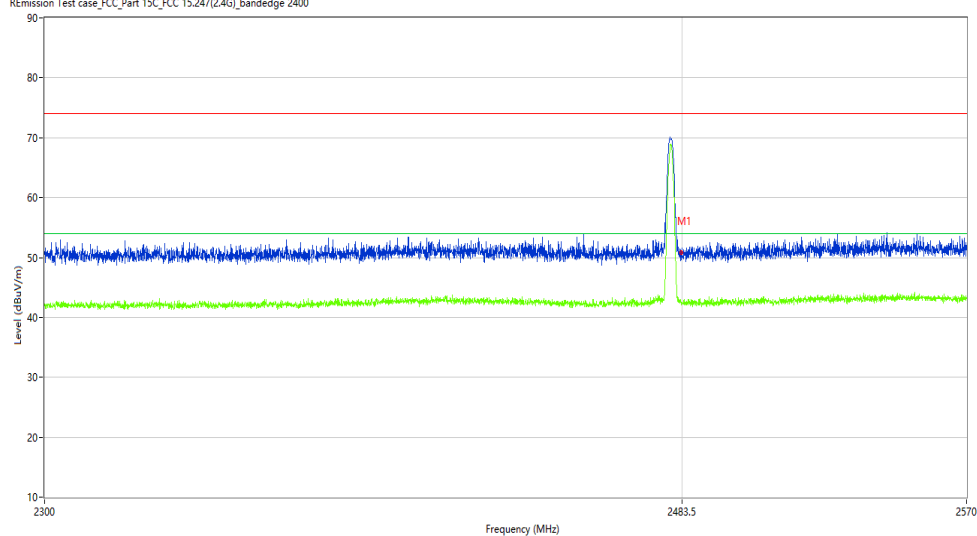

No.	Frequency (MHz)	Results (dBuV/m)	Factor (dB/m)	Limit (dBuV/m)	Margin (dB)	Detector	Table (Degree)	Height (cm)	Antenna	Verdict
1	2483.500	50.68	-10.74	74.0	23.32	Peak	91.46	100	V	Pass
1**	2483.500	42.54	-10.74	54.0	11.46	AV	91.46	100	V	Pass