ResMed SPECIFICATION	FCC & IC Labelling submission	ResMed Confidential Proprietary Information, not to be reproduced or made available to third parties without prior consent from ResMed and not to be used in any unauthorised way. © ResMed Ltd	SPEC NO.	eLB0925-070
			REV	2.0
			PAGE	1 OF 1

Mark Bertinetti
24 July 2014

Common labels/moulded in artwork

BRAND
ResMed branding
chrome or colour foiled
on front of product

"BF APPLIED PART"
Body Fibrillation Icon
& Text
Moulded into plastic case
using an insert
near rear Outlet

R370-407

"REFER TO MANUAL" Label
Man reading book Icon & Text
White pre-printed label stuck next to
power connector on rear of chassis

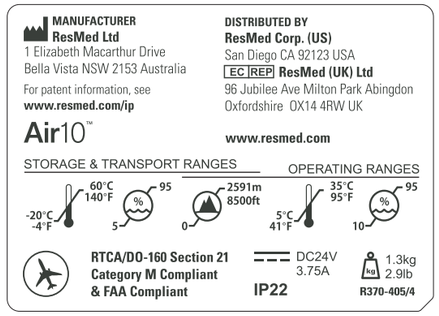

REGULATORY Label
White pre-printed label
stuck on bottom of chassis

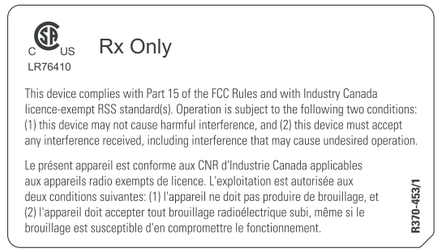

FCC & IC Compliance Labels
White pre-printed label
stuck on bottom of chassis

Product Specific Labels

37015 AirSense10 CPAP - USA

R370-7204

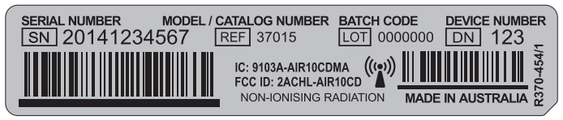

37020 AirSense10 Elite - USA

R370-7205

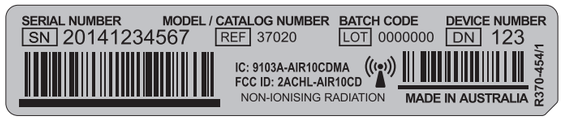

37028 AirSense10 AutoSet - USA

R370-7206

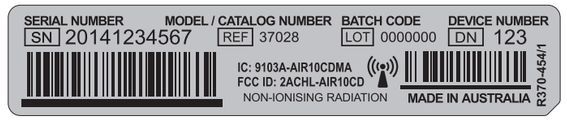

37036 AirSense10 AutoSet FH - USA

R370-7207

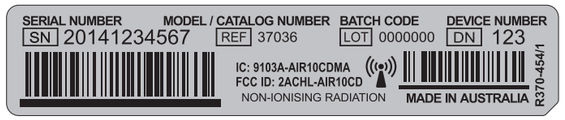

37043 AirSense10 ASV - USA

R370-7210

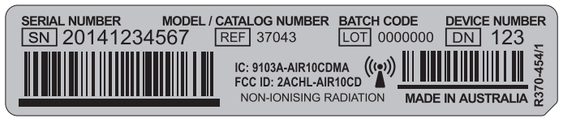

37046 AirSense10 S - USA

R370-7208

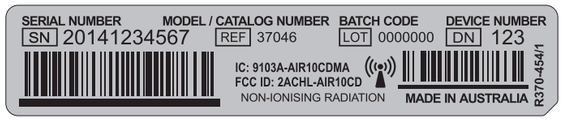

37051 AirSense10 VAuto - USA

R370-7209

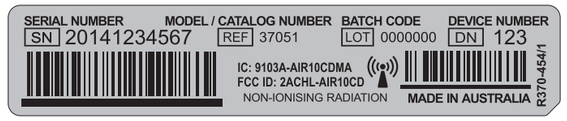

PRODUCT NAME PLAQUES
Foiled product variant badges
"permanently" attached to front of product

SERIAL NUMBER LABELS
Thermally printed labels
attached to rear of product

Figure 1 Front of CPAP

Figure 2 Back of CPAP

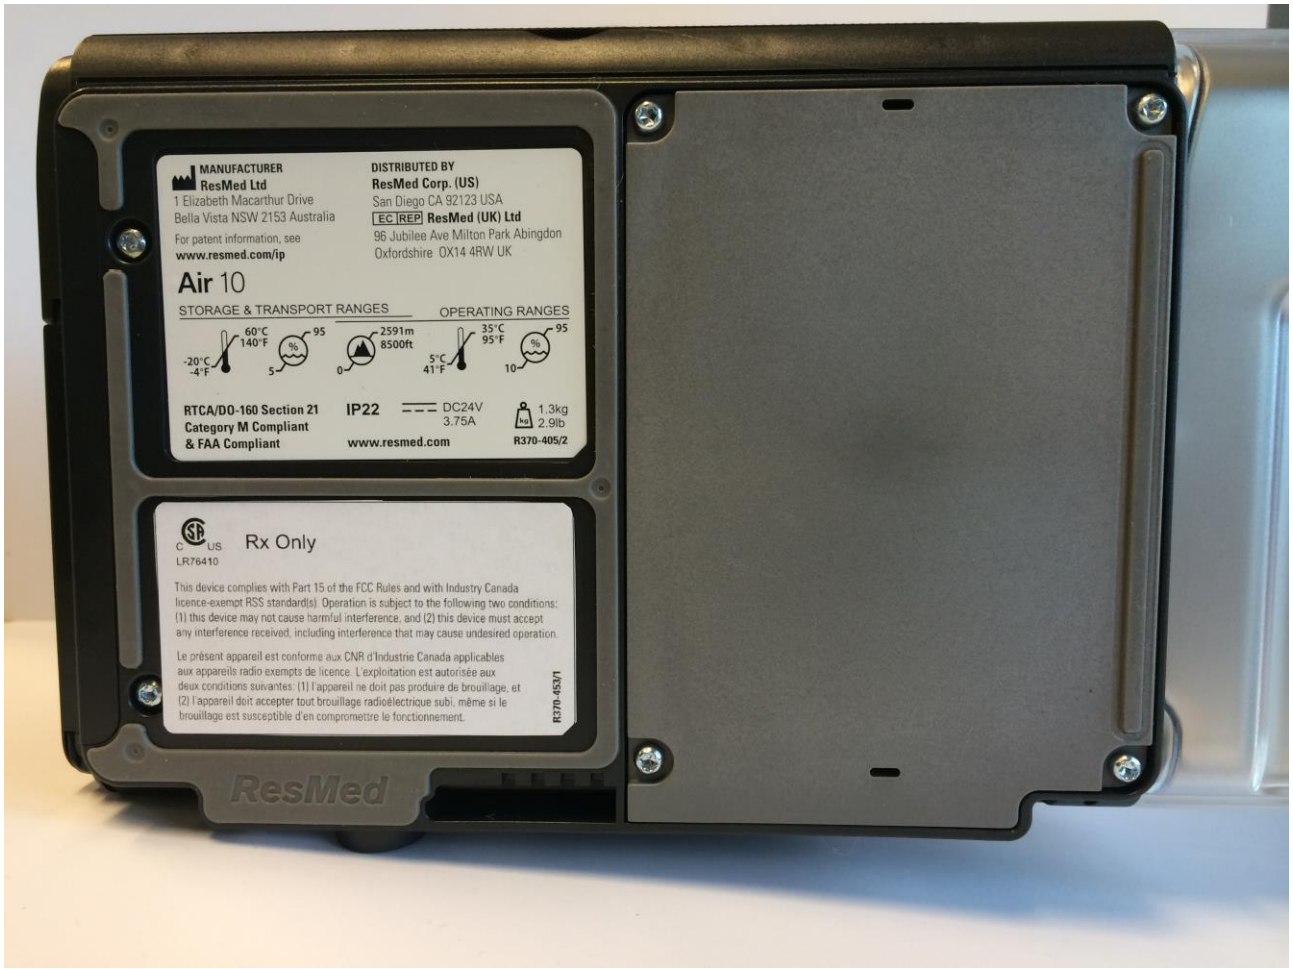

Figure 3 Underneath of CPAP