

5.6 Measurement Uncertainty

Measurement Uncertainty according to IEEE 1528							
Error Description	Uncertainty Value	Probability Distribution	Div.	c _i (1g)	c _i (10g)	Std. Unc. 1g	Std. Unc. 10g
Measurement System							
Probe Calibration	±6.55%	N	1	1	1	±6.55%	±6.55%
Axial Isotropy	±4.7%	R	$\sqrt{3}$	0.7	0.7	±1.9%	±1.9%
Hemispherical Isotropy	±9.6%	R	$\sqrt{3}$	0.7	0.7	±3.9%	±3.9%
Linearity	±4.7%	R	$\sqrt{3}$	1	1	±2.7%	±2.7%
Modulation Response	±2.4%	R	$\sqrt{3}$	1	1	±1.4%	±1.4%
System Detection Limits	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%
Boundary effects	±2.0%	R	$\sqrt{3}$	1	1	±1.2%	±1.2%
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%
Response Time	±0.8%	R	$\sqrt{3}$	1	1	±0.5%	±0.5%
Integration Time	±2.6%	R	$\sqrt{3}$	1	1	±1.5%	±1.5%
RF Ambient Noise	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%
RF Ambient Reflections	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%
Probe Positioner	±0.8%	R	$\sqrt{3}$	1	1	±0.5%	±0.5%
Probe Positioning	±6.7%	R	$\sqrt{3}$	1	1	±3.9%	±3.9%
Post processing	±4.0%	R	$\sqrt{3}$	1	1	±2.3%	±2.3%
Test Sample Related							
Device Holder	±3.6%	N	1	1	1	±3.6%	±3.6%
Test Sample Positioning	±2.9%	N	1	1	1	±2.9%	±2.9%
Power Scaling	±0%	R	$\sqrt{3}$	1	1	±0%	±0%
Power Drift	±5.0%	R	$\sqrt{3}$	1	1	±2.9%	±2.9%
Phantom and Setup Related							
Phantom Uncertainty	±7.9%	R	$\sqrt{3}$	1	1	±4.6%	±4.6%
SAR correction	±1.9%	R	$\sqrt{3}$	1	0.84	±1.1%	±0.9%
Liquid conductivity (measured)	±2.5%	N	1	0.78	0.71	±2.0%	±1.8%
Liquid permittivity (measured)	±2.5%	N	1	0.26	0.26	±0.1%	±0.1%
Temperature uncertainty - Conductivity	±5.2%	R	$\sqrt{3}$	0.78	0.71	±2.3%	±2.1%
Temperature uncertainty - Permittivity	±0.8%	R	$\sqrt{3}$	0.23	0.26	±0.1%	±0.1%
Combined Standard Uncertainty						±12.8%	±12.7%
Expanded Standard Uncertainty						±25.6%	±25.4%

Measurement Uncertainty according to EN 62209-1							
Error Description	Uncertainty Value	Probability Distribution	Div.	c _i (1g)	c _i (10g)	Std. Unc. 1g	Std. Unc. 10g
Measurement System							
Probe Calibration	±6.0%	N	1	1	1	±6.0%	±6.0%
Axial Isotropy	±4.7%	R	$\sqrt{3}$	0.7	0.7	±1.9%	±1.9%
Hemispherical Isotropy	±9.6%	R	$\sqrt{3}$	0.7	0.7	±3.9%	±3.9%
Boundary effects	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%
Linearity	±4.7%	R	$\sqrt{3}$	1	1	±2.7%	±2.7%
System Detection Limits	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%
Response Time	±0.8%	R	$\sqrt{3}$	1	1	±0.5%	±0.5%
Integration Time	±2.6%	R	$\sqrt{3}$	1	1	±1.5%	±1.5%
RF Ambient Noise	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%
RF Ambient Reflections	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%
Probe Positioner	±0.4%	R	$\sqrt{3}$	1	1	±0.2%	±0.2%
Probe Positioning	±2.9%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%
Max. SAR Evaluation	±2.0%	R	$\sqrt{3}$	1	1	±1.2%	±1.2%
Test Sample Related							
Device Positioning	±2.9%	N	1	1	1	±2.9%	±2.9%
Device Holder	±3.6%	N	1	1	1	±3.6%	±3.6%
Power Drift	±5.0%	R	$\sqrt{3}$	1	1	±2.9%	±2.9%
Power Scaling	±0%	R	$\sqrt{3}$	1	1	±0.0%	±0.0%
Phantom and Setup Related							
Phantom Uncertainty	±6.1%	R	$\sqrt{3}$	1	1	±3.5%	±3.5%
SAR correction	±1.9%	R	$\sqrt{3}$	1	0.84	±1.1%	±0.9%
Liquid conductivity (measured)	±2.5%	N	1	0.78	0.71	±2.0%	±1.8%
Liquid permittivity (measured)	±2.5%	N	1	0.26	0.26	±0.6%	±0.7%
Temperature uncertainty - Conductivity	±5.2%	R	$\sqrt{3}$	0.78	0.71	±2.3%	±2.1%
Temperature uncertainty - Permittivity	±0.8%	R	$\sqrt{3}$	0.23	0.26	±0.1%	±0.1%
Combined Standard Uncertainty						±11.4%	±11.3%
Expanded Standard Uncertainty						±22.9%	±22.7%

Measurement Uncertainty according to EN 62209-2							
Error Description	Uncertainty Value	Probability Distribution	Div.	c _i (1g)	c _i (10g)	Std. Unc. 1g	Std. Unc. 10g
Measurement System							
Probe Calibration	±6.55%	N	1	1	1	±6.55%	±6.55%
Axial Isotropy	±4.7%	R	$\sqrt{3}$	0.7	0.7	±1.9%	±1.9%
Hemispherical Isotropy	±9.6%	R	$\sqrt{3}$	0.7	0.7	±3.9%	±3.9%
Linearity	±4.7%	R	$\sqrt{3}$	1	1	±2.7%	±2.7%
Modulation Response	±2.4%	R	$\sqrt{3}$	1	1	±1.4%	±1.4%
System Detection Limits	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%
Boundary effects	±2.0%	R	$\sqrt{3}$	1	1	±1.2%	±1.2%
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%
Response Time	±0.8%	R	$\sqrt{3}$	1	1	±0.5%	±0.5%
Integration Time	±2.6%	R	$\sqrt{3}$	1	1	±1.5%	±1.5%
RF Ambient Noise	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%
RF Ambient Reflections	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%
Probe Positioner	±0.8%	R	$\sqrt{3}$	1	1	±0.5%	±0.5%
Probe Positioning	±6.7%	R	$\sqrt{3}$	1	1	±3.9%	±3.9%
Post processing	±4.0%	R	$\sqrt{3}$	1	1	±2.3%	±2.3%
Test Sample Related							
Device Holder	±3.6%	N	1	1	1	±3.6%	±3.6%
Test Sample Positioning	±2.9%	N	1	1	1	±2.9%	±2.9%
Power Scaling	±0%	R	$\sqrt{3}$	1	1	±0%	±0%
Power Drift	±5.0%	R	$\sqrt{3}$	1	1	±2.9%	±2.9%
Phantom and Setup Related							
Phantom Uncertainty	±7.9%	R	$\sqrt{3}$	1	1	±4.6%	±4.6%
SAR correction	±1.9%	R	$\sqrt{3}$	1	0.84	±1.1%	±0.9%
Liquid conductivity (measured)	±2.5%	N	1	0.78	0.71	±2.0%	±1.8%
Liquid permittivity (measured)	±2.5%	N	1	0.26	0.26	±0.1%	±0.1%
Temperature uncertainty - Conductivity	±5.2%	R	$\sqrt{3}$	0.78	0.71	±2.3%	±2.1%
Temperature uncertainty - Permittivity	±0.8%	R	$\sqrt{3}$	0.23	0.26	±0.1%	±0.1%
Combined Standard Uncertainty						±12.8%	±12.7%
Expanded Standard Uncertainty						±25.6%	±25.4%

6 Test Conditions and Results

6.1 Recipes for Tissue Simulating Liquids

Body Tissue Simulating Liquids					
Ingredient	M 450-B weight (%)	M 900-B weight (%)	M 1800-B weight (%)	M 1950-A weight (%)	M 2450-B weight (%)
Water	46.21	50.75	70.17	69.79	68.64
Sugar	51.17	48.21	-	-	-
Cellulose	0.18	-	-	-	-
Salt	2.34	-	0.39	0.2	-
Preventol	0.08	0.1	-	-	-
DGBE	-	-	29.44	30	31.37
Head Tissue Simulating Liquids					
Ingredient	HSL 450-A weight (%)	HSL 900-B weight (%)	HSL 1800-F weight (%)	HSL 1950-B weight (%)	HSL 2450-B weight (%)
Water	38.91	40.29	55.24	55.41	55
Sugar	56.93	57.9	-	-	-
Cellulose	0.25	0.24	-	-	-
Salt	3.79	1.38	0.31	0.08	-
Preventol	0.12	0.18	-	-	-
DGBE	-	-	44.45	44.51	45

Water: deionized water, resistivity $\geq 16 \text{ M}\Omega$

Sugar: refined white sugar

Salt: pure NaCl

Cellulose: Hydroxyethyl-cellulose

Preservative: Preventol D-7

DGBE: Diethylenglycol-monobuthyl ether

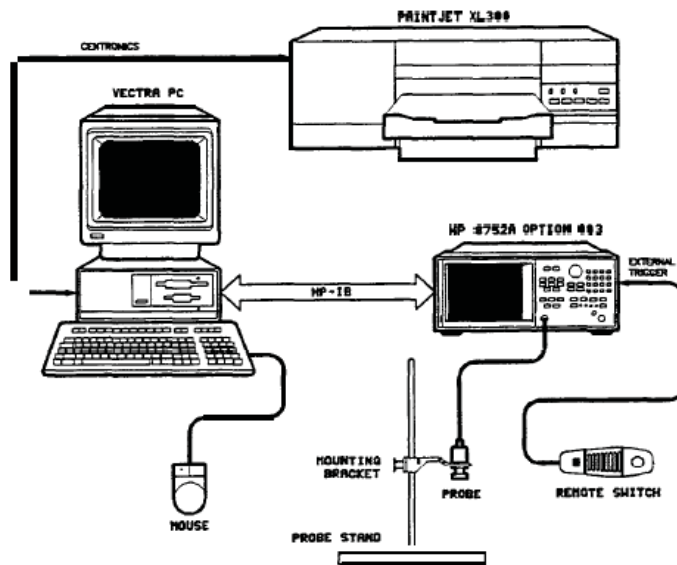
The parameters for the different frequencies are defined in the corresponding compliance standards (e.g., IEEE 1528-2003, IEC 62209-1)

The HBBL3-6GHz and MBBL 3-6 GHz liquids are direct from Speag.

6.2 Test Conditions and Results – Tissue Validation

Tissue Validation acc. to 865664 D01 SAR Measurement 100 MHz to 6 GHz / ISED RSS-102					Verdict: PASS
Test according to measurement reference		Reference Method			
		865664 D01 SAR Measurement 100 MHz to 6 GHz			
Target Values					
Frequency [MHz]	Head		Body		Permitted tolerance [%]
	Relative dielectric constant ϵ_r	Conductivity σ [S/m]	Relative dielectric constant ϵ_r	Conductivity σ [S/m]	
150	52.3	0.76	61.9	0.80	$\leq \pm 5$
300	45.3	0.87	58.2	0.92	$\leq \pm 5$
450	43.5	0.87	56.7	0.94	$\leq \pm 5$
835	41.5	0.90	55.2	0.97	$\leq \pm 5$
900	41.5	0.97	55.0	1.05	$\leq \pm 5$
915	41.5	0.98	55.0	1.06	$\leq \pm 5$
1450	40.5	1.20	54.0	1.30	$\leq \pm 5$
1610	40.3	1.29	53.8	1.40	$\leq \pm 5$
1800 – 2000	40.0	1.40	53.3	1.52	$\leq \pm 5$
2450	39.2	1.80	52.7	1.95	$\leq \pm 5$
3000	38.5	2.40	52.0	2.73	$\leq \pm 5$
5200	36.0	4.66	49.0	5.30	$\leq \pm 5$
5500	35.6	4.96	48.6	5.65	$\leq \pm 5$
5800	35.3	5.27	48.2	6.00	$\leq \pm 5$

Test setup



Test procedure

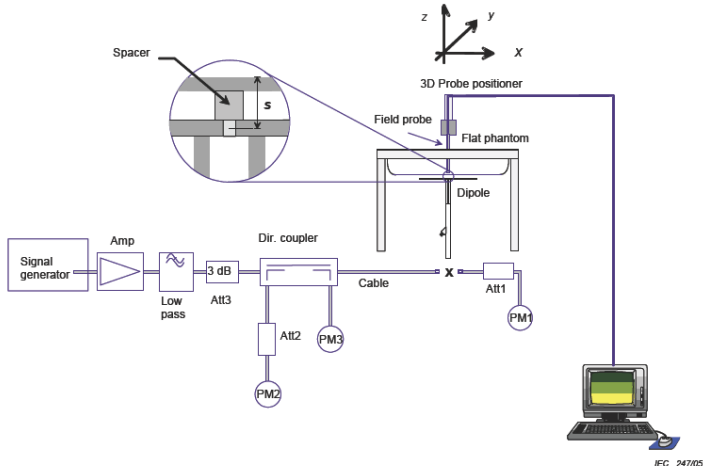
1. The dielectric probe kit is calibrated using the standards air, short circuit and deionized water
2. The tissue simulating liquid is measured using the dielectric probe
3. Target values are compared to the measurement values and deviations are determined

Test results

Frequency [MHz]	Tissue	Measured ϵ_r	Target ϵ_r	Delta ϵ_r [%]	Measured σ [S/m]	Target σ [S/m]	Delta σ [%]
2450	Body	50.455	52.7	-4.26	2.016	1.95	3.38
2402	Body	50.650	52.7	-3.89	1.939	1.95	-0.56
2441	Body	50.563	52.7	-4.06	1.999	1.95	2.51
2480	Body	50.360	52.7	-4.44	2.040	1.95	4.62

Comments: * Measured radio frequencies

6.3 Test Conditions and Results – System Validation

System Validation acc. to 865664 D01 SAR Measurement 100 MHz to 6 GHz / ISED RSS-102				Verdict: PASS
Test according to measurement reference	Reference Method			
	865664 D01 SAR Measurement 100 MHz to 6 GHz / IEEE 1528			
Test frequency range	Tested frequencies			
	2450 MHz			
Test mode	unmodulated CW			
Target Values				
Frequency [MHz]	Target SAR value [W/kg (1g)]		Permitted tolerance [%]	
2450	12.5 @ 250mW		≤ ±10	
The target reference values are taken from the calibration sheets (see annex)				
Test setup				
				
Test procedure				
1. The dipole antenna input power is set to 250mW 2. The reference dipole is positioned under the phantom 3. With the dipole antenna powered the SAR value is measured 4. The measured SAR values are compared to the target SAR values				
Test results				
Frequency [MHz]	Input power [mW]	Measured SAR value [W/kg (1g)]	Target SAR value [W/kg (1g)]	Delta [%]
2450	250	13.7	12.5	8.26
Comments:				

6.4 Test Conditions and Results – Standalone SAR Measurement

Standalone SAR acc. to 865664 D01 SAR Measurement 100 MHz to 6 GHz / ISED RSS-102								Verdict: PASS
Test according to measurement reference			Reference Method					
			865664 D01 SAR Measurement 100 MHz to 6 GHz ISED RSS-102 Issue 5					
Room temperature			22.0 – 22.6 °C					
Liquid depth			15.5 cm					
Environment			general public					
Limits								
Region			Occupational SAR values [W/kg]		General public SAR values [W/kg]			
Whole body average SAR			0.4		0.08			
Localized SAR (Head and trunk) SAR averaging mass = 1g			8		1.6			
Localized SAR (Limbs) SAR averaging mass = 10g			20		4			
Test results								
Mode	Position	Channel	Frequency [MHz]	Drift [dB]	Scaling Factor*	Measured SAR [W/kg (1g)]	Reported SAR [W/kg (1g)] **	SAR Limit [W/kg (1g)]
BT-TX	FRONT 0mm	39	2441	0.16	1.58	0.038	0.06	1.6
Comments:*tune up limit power (mW) / measured conducted power (mW) = scaling factor								
** attached measurement plot: highest SAR value for the communication system								

According to KDB 865664 D02 v01r02 only the SAR plots for the highest SAR results for each EUT configuration and operating condition are given in the “SAR Results” part of the report.

6.5 Test Conditions and Results – Multi-transmitter SAR Result

No multi-transmitter evaluation

ANNEX A Calibration Documents



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Eurofins**

Certificate No: **DAE3-522_Sep16**

CALIBRATION CERTIFICATE

Object **DAE3 - SD 000 D03 AA - SN: 522**

Calibration procedure(s) **QA CAL-06.v29**
Calibration procedure for the data acquisition electronics (DAE)

Calibration date: **September 28, 2016**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	09-Sep-16 (No:19065)	Sep-17
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit Calibrator Box V2.1	SE UWS 053 AA 1001	05-Jan-16 (in house check)	In house check: Jan-17
	SE UMS 006 AA 1002	05-Jan-16 (in house check)	In house check: Jan-17

Calibrated by: Name **Eric Hainfeld** Function **Technician**

Signature

Approved by: **Fin Bornholt** Deputy Technical Manager

Issued: September 28, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary

DAE data acquisition electronics
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
 - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
 - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
 - *Input Offset Measurement:* Output voltage and statistical results over a large number of zero voltage measurements.
 - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
 - *Power consumption:* Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 μ V , full range = -100...+300 mV

Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	404.445 $\pm$ 0.02% (k=2)	404.110 $\pm$ 0.02% (k=2)	404.959 $\pm$ 0.02% (k=2)
Low Range	3.95998 $\pm$ 1.50% (k=2)	3.93992 $\pm$ 1.50% (k=2)	3.99728 $\pm$ 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	56.0 ° $\pm$ 1 °
---	------------------

Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	199998.65	1.51	0.00
Channel X + Input	20003.67	1.49	0.01
Channel X - Input	-19998.57	1.81	-0.01
Channel Y + Input	199997.59	-0.07	-0.00
Channel Y + Input	20000.66	-1.46	-0.01
Channel Y - Input	-19999.61	0.87	-0.00
Channel Z + Input	199997.76	0.55	0.00
Channel Z + Input	19999.68	-2.27	-0.01
Channel Z - Input	-20000.13	0.36	-0.00

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2002.77	0.92	0.05
Channel X + Input	202.84	0.66	0.33
Channel X - Input	-196.58	1.09	-0.55
Channel Y + Input	2002.44	0.71	0.04
Channel Y + Input	202.20	0.08	0.04
Channel Y - Input	-198.06	-0.28	0.14
Channel Z + Input	2002.08	0.42	0.02
Channel Z + Input	200.37	-1.61	-0.80
Channel Z - Input	-199.14	-1.33	0.67

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	-3.54	-5.21
	- 200	6.25	4.83
Channel Y	200	-0.35	-0.64
	- 200	-0.21	-0.07
Channel Z	200	15.29	15.53
	- 200	-18.32	-18.03

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	0.24	-4.36
Channel Y	200	7.55	-	0.52
Channel Z	200	9.68	4.92	-

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15770	16653
Channel Y	15724	15421
Channel Z	16050	15178

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M Ω

	Average (μ V)	min. Offset (μ V)	max. Offset (μ V)	Std. Deviation (μ V)
Channel X	1.44	-0.31	2.82	0.59
Channel Y	-0.40	-1.67	0.99	0.60
Channel Z	0.67	-1.25	2.04	0.58

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)



Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

**CUSTOMER
COPY**

DAE REPAIR REPORT – SPEAG Production Center

PRODUCT		DAE4 - Data Acquisition Electronics		
SERIAL Nr.:		522	IN DATE: 16-Sep-2016	
CUSTOMER:		Eurofins		
DAE REPAIR				
MATERIAL	WORK DESCRIPTION		WORKING TIME (h)	
Emergency stop:	fixed ☐	exchanged ☐	6 new magnets ☐	hours
DAE Connector:	fixed ☐	exchanged ☐	 ☐	hours
DAE Battery Cover:	fixed ☐	exchanged ☐	 ☐	hours
AD Converter Print:	fixed ☐	exchanged ☒	 ☐	1.00 hours
Battery Connector:	fixed ☐	exchanged ☐	 ☐	hours
Battery Con. PCB:	fixed ☐	exchanged ☐	 ☐	hours
DAE 3 - 4 upgrade	fixed ☐	installed ☐	 ☐	hours
Input PCB:	fixed ☐	exchanged ☐	 ☐	hours
DAE Bottom Cover	fixed ☐	exchanged ☐	 ☐	hours
Analysis:				1.50 hours
Final Assembly:				hours
Total hours				2.50 hours
COMMENTS:				
This DAE was returned for calibration. It failed the receiving inspection test. The input range of the Y channel (4.104) is too high (tolerance 3.9 - 4.1). The linearity of the channel wasn't affected. To re-establish full functionality of this DAE the ADC printed circuit board has been replaced. After this repair the DAE will get newly calibrated.				
CONDUCTED BY:		APPROVED BY:		
 DATE: 26-Sep-2016		 DATE: 26-Sep-2016		
REPAIR COST:				
MATERIAL COST:		USD	Euro	
free		☒	☐	
REPAIR:		☒	☐	
TOTAL COST:		QUOTATION #:		
free		-		
APPROVED BY:				
 DATE: 26-Sep-2016				



Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Eurofins**

Certificate No: **EX3-3893_Sep16**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3893**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,
 QA CAL-25.v6
 Calibration procedure for dosimetric E-field probes**

Calibration date: **September 23, 2016**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	06-Apr-16 (No. 217-02288/02289)	Apr-17
Power sensor NRP-Z91	SN: 103244	06-Apr-16 (No. 217-02288)	Apr-17
Power sensor NRP-Z91	SN: 103245	06-Apr-16 (No. 217-02289)	Apr-17
Reference 20 dB Attenuator	SN: S5277 (20x)	05-Apr-16 (No. 217-02293)	Apr-17
Reference Probe ES3DV2	SN: 3013	31-Dec-15 (No. ES3-3013_Dec15)	Dec-16
DAE4	SN: 660	23-Dec-15 (No. DAE4-660_Dec15)	Dec-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Calibrated by:	Name Michael Weber	Function Laboratory Technician	Signature
Approved by:	Katja Pokovic	Technical Manager	
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			Issued: September 28, 2016



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E^2 -field uncertainty inside TSL (see below *ConvF*).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * *frequency_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * *ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).