

#### WLAN2450\_CH1 Left Tilt

Date: 8/8/2019 Electronics: DAE4 Sn771 Medium: head 2450 MHz Medium parameters use: f = 2412 MHz;  $\sigma = 1.772$  mho/m;  $\epsilon r = 38.66$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature: 22.5°C, Liquid Temperature: 22.3°C Communication System: WLan 2450 Frequency: 2412 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(6.95, 6.95, 6.95)

Area Scan (81x131x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Maximum value of SAR (interpolated) = 1.97 W/kg

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 7.443 V/m; Power Drift = 0.09 dB Peak SAR (extrapolated) = 2.40 W/kg SAR(1 g) = 0.913 W/kg; SAR(10 g) = 0.349 W/kg Maximum value of SAR (measured) = 1.57 W/kg

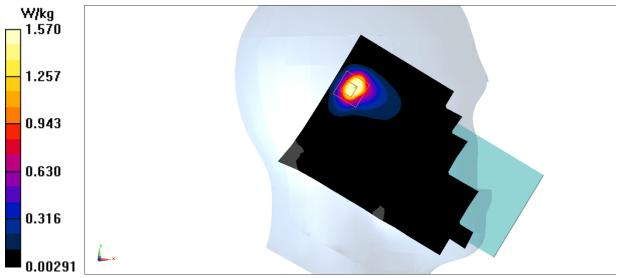


Fig.19 2450 MHz



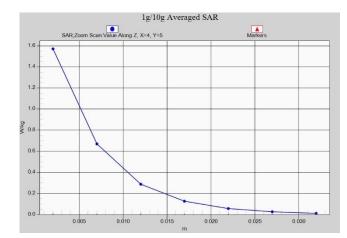


Fig. 19-1 Z-Scan at power reference point (2450 MHz)



#### WLAN2450\_CH1 Top

Date: 8/8/2019 Electronics: DAE4 Sn771 Medium: Body 2450 MHz Medium parameters used (interpolated): f = 2412 MHz;  $\sigma = 1.913$  mho/m;  $\epsilon_r = 53.38$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature: 22.5°C, Liquid Temperature: 22.3°C Communication System: WLAN2450 2412 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(7.13, 7.13, 7.13)

**Area Scan (71x121x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm Maximum value of SAR (interpolated) = 0.923 W/kg

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 12.57 V/m; Power Drift = 0.13 dB Peak SAR (extrapolated) = 1.22 W/kg SAR(1 g) = 0.591 W/kg; SAR(10 g) = 0.253 W/kg Maximum value of SAR (measured) = 0.915 W/kg

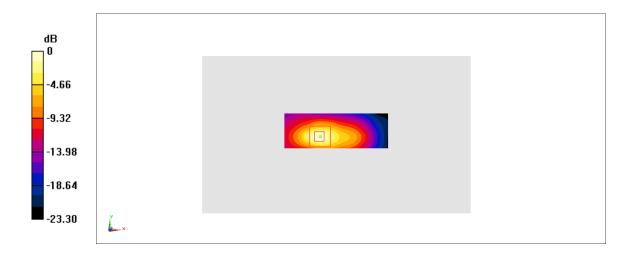


Fig.20 2450 MHz



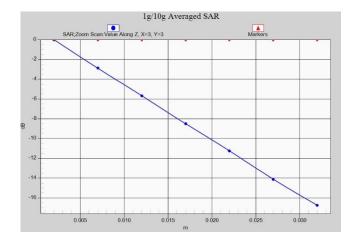


Fig. 20-1 Z-Scan at power reference point (2450 MHz)





## ANNEX B System Verification Results

#### 835 MHz

Date: 8/5/2019 Electronics: DAE4 Sn771 Medium: Head 835 MHz Medium parameters used: f = 835 MHz;  $\sigma = 0.906$  mho/m;  $\varepsilon_r = 41.52$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature: 22.5°C Liquid Temperature: 22.3°C Communication System: CW Frequency: 835 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(9.09,9.09,9.09) **System Validation /Area Scan (81x191x1):** Interpolated grid: dx=1.000 mm, dy=1.000 mm Reference Value = 64.02 V/m; Power Drift = -0.05 **Fast SAR: SAR(1 g) = 2.3 W/kg; SAR(10 g) = 1.51 W/kg** Maximum value of SAR (interpolated) = 3.8 W/kg

System Validation /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value =64.02 V/m; Power Drift = -0.05 dB Peak SAR (extrapolated) = 4.04 W/kg SAR(1 g) = 2.31 W/kg; SAR(10 g) = 1.5 W/kg Maximum value of SAR (measured) = 3.6 W/kg

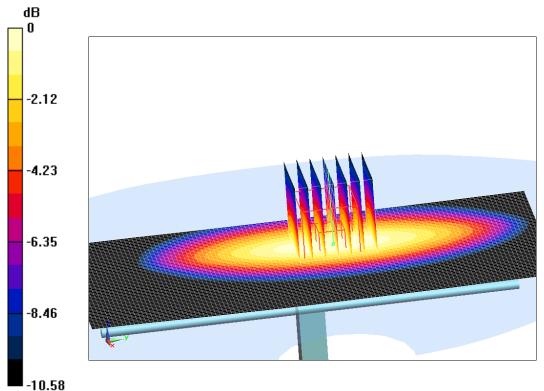



#### Fig.B.1 validation 835 MHz 250mW





Date: 8/5/2019Electronics: DAE4 Sn771 Medium: Body 835 MHz Medium parameters used: f = 835 MHz;  $\sigma = 0.97$  mho/m;  $\varepsilon_r = 55.12$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature: 22.5°C Liquid Temperature: 22.3°C Communication System: CW Frequency: 835 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(9.47,9.47,9.47)


System Validation /Area Scan (81x191x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Reference Value = 59.12 V/m; Power Drift = -0.09

**Fast SAR: SAR(1 g) = 2.34 W/kg; SAR(10 g) = 1.53 W/kg** Maximum value of SAR (interpolated) = 3.56 W/kg

System Validation /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value =59.12 V/m; Power Drift = -0.09 dB Peak SAR (extrapolated) = 3.74 W/kg SAR(1 g) = 2.35 W/kg; SAR(10 g) = 1.54 W/kg Maximum value of SAR (measured) = 3.18 W/kg

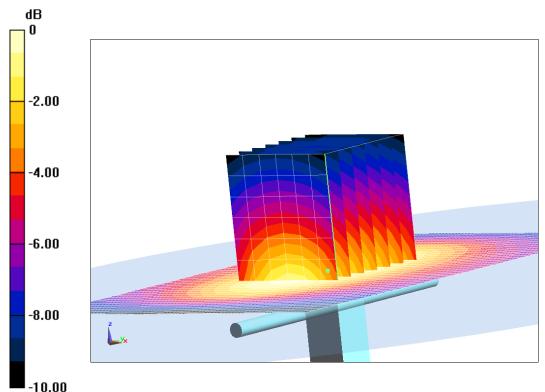








Date: 8/6/2019 Electronics: DAE4 Sn771 Medium: Head 1900 MHz Medium parameters used: f = 1900 MHz;  $\sigma$  =1.4 mho/m;  $\epsilon_r$  = 39.37;  $\rho$  = 1000 kg/m<sup>3</sup> Ambient Temperature: 22.5°C Liquid Temperature: 22.3°C Communication System: CW Frequency: 1900 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(7.73,7.73,7.73)


System Validation /Area Scan (81x191x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Reference Value = 106.13 V/m; Power Drift = 0.02


Fast SAR: SAR(1 g) = 9.83 W/kg; SAR(10 g) = 5.21 W/kg Maximum value of SAR (interpolated) = 14.63 W/kg

System Validation /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value =106.13 V/m; Power Drift = 0.02 dB Peak SAR (extrapolated) = 18.05 W/kg SAR(1 g) = 9.8 W/kg; SAR(10 g) = 5.28 W/kg

Maximum value of SAR (measured) = 15.1 W/kg

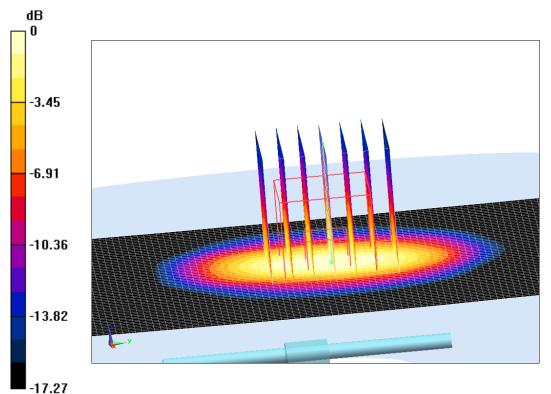








Date: 8/6/2019 Electronics: DAE4 Sn771 Medium: Body 1900 MHz Medium parameters used: f = 1900 MHz;  $\sigma$  =1.513 mho/m;  $\epsilon_r$  = 53.91;  $\rho$  = 1000 kg/m<sup>3</sup> Ambient Temperature: 22.5°C Liquid Temperature: 22.3°C Communication System: CW Frequency: 1900 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(7.53,7.53,7.53)

System Validation /Area Scan (81x191x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Reference Value = 102.83 V/m; Power Drift = 0.07


Fast SAR: SAR(1 g) = 9.97 W/kg; SAR(10 g) = 5.3 W/kg Maximum value of SAR (interpolated) = 17.67 W/kg

System Validation /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value =102.83 V/m; Power Drift = 0.07 dB Peak SAR (extrapolated) = 17.4 W/kg SAR(1 g) = 10.14 W/kg; SAR(10 g) = 5.38 W/kg

Maximum value of SAR (measured) = 14.16 W/kg

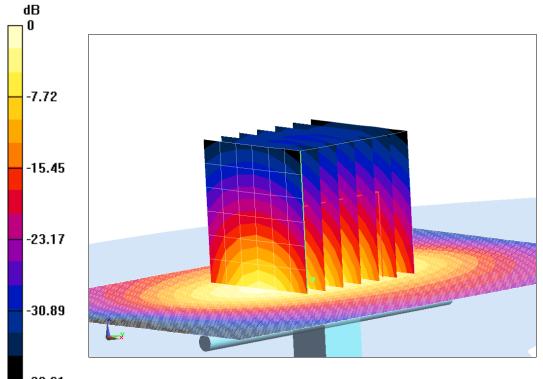





#### Fig.B.4 validation 1900 MHz 250mW





Date: 8/7/2019Electronics: DAE4 Sn771 Medium: Head 2450 MHz Medium parameters used: f = 2450 MHz;  $\sigma = 1.797$  mho/m;  $\epsilon_r = 38.65$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature: 22.5°C Liquid Temperature: 22.3°C Communication System: CW Frequency: 2450 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(6.95,6.95,6.95)


System Validation /Area Scan (81x191x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Reference Value = 114.63 V/m; Power Drift = -0.08

Fast SAR: SAR(1 g) = 13.05 W/kg; SAR(10 g) = 6.13 W/kgMaximum value of SAR (interpolated) = 21.64 W/kg

System Validation /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value =114.63 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 26.89 W/kg SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.28 W/kg Maximum value of SAR (measured) = 21.45 W/kg

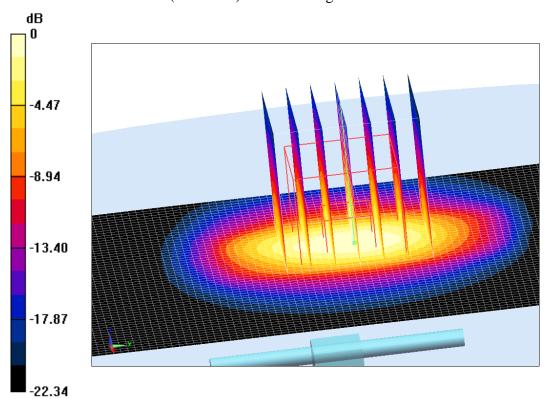







Date: 8/7/2019 Electronics: DAE4 Sn771 Medium: Body 2450 MHz Medium parameters used: f = 2450 MHz;  $\sigma = 1.939$  mho/m;  $\epsilon_r = 53.13$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature: 22.5°C Liquid Temperature: 22.3°C Communication System: CW Frequency: 2450 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(7.13,7.13,7.13)


System Validation /Area Scan (81x191x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Reference Value = 104.23 V/m; Power Drift = 0.05


Fast SAR: SAR(1 g) = 12.45 W/kg; SAR(10 g) = 5.85 W/kg Maximum value of SAR (interpolated) = 25.73 W/kg

System Validation /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value =104.23 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 25.46 W/kg

SAR(1 g) = 12.43 W/kg; SAR(10 g) = 5.85 W/kg

Maximum value of SAR (measured) = 19.82 W/kg

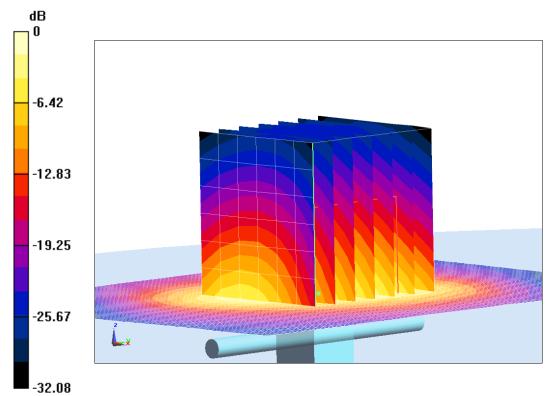









Date: 8/8/2019 Electronics: DAE4 Sn771 Medium: Head 2600 MHz Medium parameters used: f = 2600 MHz;  $\sigma = 1.942$  mho/m;  $\epsilon_r = 38.63$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature: 22.5°C Liquid Temperature: 22.3°C Communication System: CW Frequency: 2600 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(6.92,6.92,6.92)


System Validation /Area Scan (81x191x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Reference Value = 111.47 V/m; Power Drift = 0.06 Fast SAR: SAR(1 g) = 14.33 W/kg; SAR(10 g) = 6.33 W/kg

Maximum value of SAR (interpolated) = 24.84 W/kg

System Validation /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value =111.47 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 31.96 W/kg SAR(1 g) = 14.3 W/kg; SAR(10 g) = 6.47 W/kg Maximum value of SAR (measured) = 25.43 W/kg

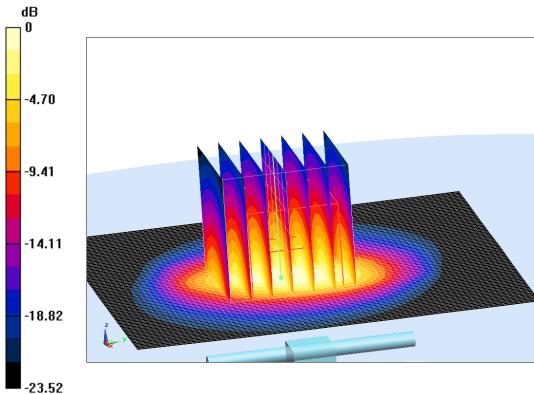








Date: 8/8/2019 Electronics: DAE4 Sn771 Medium: Body 2600 MHz Medium parameters used: f = 2600 MHz;  $\sigma = 2.175$  mho/m;  $\epsilon_r = 51.64$ ;  $\rho = 1000$  kg/m<sup>3</sup> Ambient Temperature: 22.5°C Liquid Temperature: 22.3°C Communication System: CW Frequency: 2600 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN7514 ConvF(7.06,7.06)


System Validation /Area Scan (81x191x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Reference Value = 105.84 V/m; Power Drift = -0.04


Fast SAR: SAR(1 g) = 13.79 W/kg; SAR(10 g) = 6.2 W/kg Maximum value of SAR (interpolated) = 29.42 W/kg

System Validation /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value =105.84 V/m; Power Drift = -0.04 dB Peak SAR (extrapolated) = 30.08 W/kg SAR(1 g) = 14.08 W/kg; SAR(10 g) = 6.26 W/kg

Maximum value of SAR (measured) = 23.24 W/kg

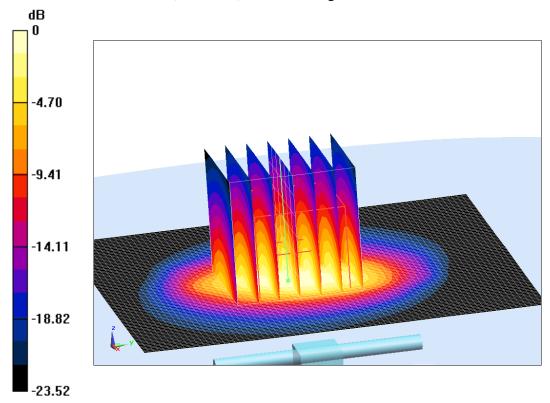







The SAR system verification must be required that the area scan estimated 1-g SAR is within 3% of the zoom scan 1-g SAR.

Date	Band	Position	Area scan (1g)	Zoom scan (1g)	Drift (%)
2019-8-5	835	Head	2.3	2.31	-0.43
	835	Body	2.34	2.35	-0.42
2019-8-6	1900	Head	9.83	9.8	0.31
	1900	Body	9.97	10.14	-1.68
2019-8-7	2450	Head	13.05	13.1	-0.38
	2450	Body	12.45	12.43	0.16
2019-8-8	2600	Head	14.33	14.3	0.21
	2600	Body	13.79	14.08	-2.06


#### Table B.1 Comparison between area scan and zoom scan for system verification



## ANNEX C SAR Measurement Setup

#### C.1 Measurement Set-up

The Dasy4 or DASY5 system for performing compliance tests is illustrated above graphically. This system consists of the following items:

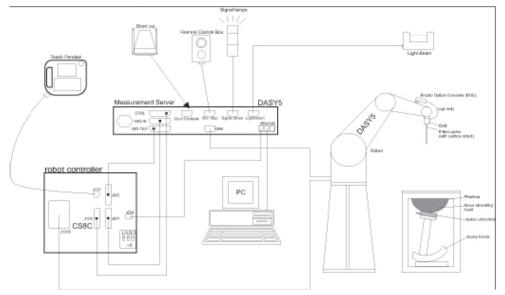

Picture C.1SAR Lab Test Measurement Set-up

- A standard high precision 6-axis robot (StäubliTX=RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- An isotropic field probe optimized and calibrated for the targeted measurement.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running WinXP and the DASY4 or DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as
- warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.



#### No.I19Z61624-SEM03 Page 124 of 217

#### C.2 Dasy4 or DASY5 E-field Probe System

The SAR measurements were conducted with the dosimetric probe designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multifiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY4 or DASY5 software reads the reflection durning a software approach and looks for the maximum using 2<sup>nd</sup> ord curve fitting. The approach is stopped at reaching the maximum.

#### **Probe Specifications:**

Model:	ES3DV3, EX3DV4		
Frequency	10MHz — 6.0GHz(EX3DV4)		
Range:	10MHz — 4GHz(ES3DV3)		
Calibration:	In head and body simulating tissue at		
	Frequencies from 835 up to 5800MHz		
Linearity:	± 0.2 dB(30 MHz to 6 GHz) for EX3DV4		
± 0.2 dB(30 MHz to 4 GHz) for ES3DV3			
DynamicRange: 10 mW/kg — 100W/kg			
Probe Length:	330 mm		
Probe Tip			
Length:	20 mm		
<b>Body Diameter:</b>	12 mm		
Tip Diameter:	2.5 mm (3.9 mm for ES3DV3)		
Tip-Center:	1 mm (2.0mm for ES3DV3)		
Application:SAR Dosimetry Testing			
	Compliance tests of mobile phones		
	Dosimetry in strong gradient fields		
Picture C.3E-field Probe			



Picture C.2Near-field Probe



#### C.3 E-field Probe Calibration

Each E-Probe/Probe Amplifier combination has unique calibration parameters. A TEM cell calibration procedure is conducted to determine the proper amplifier settings to enter in the probe parameters. The amplifier settings are determined for a given frequency by subjecting the probe to a known E-field density (1 mW/cm<sup>2</sup>) using an RF Signal generator, TEM cell, and RF Power Meter.

The free space E-field from amplified probe outputs is determined in a test chamber. This calibration can be performed in a TEM cell if the frequency is below 1 GHz and inn a waveguide or other methodologies above 1 GHz for free space. For the free space calibration, the probe is placed ©Copyright. All rights reserved by CTTL.



#### No.I19Z61624-SEM03 Page 125 of 217

in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees until the three channels show the maximum reading. The power density readings equates to 1 mW/cm<sup>2</sup>.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The E-field in the medium correlates with the temperature rise in the dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$SAR = C \frac{\Delta T}{\Delta t}$$

Where:

 $\Delta t$  = Exposure time (30 seconds), C = Heat capacity of tissue (brain or muscle),  $\Delta T$  = Temperature increase due to RF exposure.

$$SAR = \frac{\left|E\right|^2 \cdot \sigma}{\rho}$$

Where:  $\sigma$  = Simulated tissue conductivity,  $\rho$  = Tissue density (kg/m<sup>3</sup>).

#### C.4 Other Test Equipment

#### C.4.1 Data Acquisition Electronics(DAE)

The data acquisition electronics consist of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder with a control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information, as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE is 200 MOhm; the inputs are symmetrical and floating. Common mode rejection is above 80 dB.



PictureC.4: DAE

#### No.I19Z61624-SEM03 Page 126 of 217



#### C.4.2 Robot

The SPEAG DASY system uses the high precision robots (DASY4: RX90XL; DASY5: RX160L) type from Stäubli SA (France). For the 6-axis controller system, the robot controller version from Stäubli is used. The Stäubli robot series have many features that are important for our application:

- High precision (repeatability 0.02mm)
- High reliability (industrial design)
- > Low maintenance costs (virtually maintenance free due to direct drive gears; no belt drives)
- Jerk-free straight movements (brushless synchron motors; no stepper motors)
- Low ELF interference (motor control fields shielded via the closed metallic construction shields)



Picture C.5DASY 4



Picture C.6DASY 5

#### C.4.3 Measurement Server

The Measurement server is based on a PC/104 CPU broad with CPU (dasy4: 166 MHz, Intel Pentium; DASY5: 400 MHz, Intel Celeron), chipdisk (DASY4: 32 MB; DASY5: 128MB), RAM (DASY4: 64 MB, DASY5: 128MB). The necessary circuits for communication with the DAE electronic box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY I/O broad, which is directly connected to the PC/104 bus of the CPU broad.

The measurement server performs all real-time data evaluation of field measurements and surface detection, controls robot movements and handles safety operation. The PC operating system cannot interfere with these time critical processes. All connections are supervised by a watchdog, and disconnection of any of the cables to the measurement server will automatically disarm the robot and disable all program-controlled robot movements. Furthermore, the measurement server is equipped with an expansion port which is reserved for future applications. Please note that this expansion port does not have a standardized pinout, and therefore only devices provided by SPEAG can be connected. Devices from any other supplier could seriously damage the measurement server.







No.I19Z61624-SEM03 Page 127 of 217

Picture C.7 Server for DASY 4

#### Picture C.8 Server for DASY 5

#### C.4.4 Device Holder for Phantom

The SAR in the phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source at 5mm distance, a positioning uncertainty of  $\pm 0.5$ mm would produce a SAR uncertainty of  $\pm 20\%$ . Accurate device positioning is therefore crucial for accurate and repeatable measurements. The positions in which the devices must be measured are defined by the standards.


The DASY device holder is designed to cope with the different positions given in the standard. It has two scales for device rotation (with respect to the body axis) and device inclination (with respect to the line between the ear reference points). The rotation centers for both scales are the ear reference point (ERP). Thus the device needs no repositioning when changing the angles. The DASY device holder is constructed of low-loss POM material having the following dielectric parameters: relative permittivity  $\mathcal{E}$ =3 and loss tangent  $\mathcal{E}$ =0.02. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.

<Laptop Extension Kit>

The extension is lightweight and made of POM, acrylic glass and foam. It fits easily on the upper part of the Mounting Device in place of the phone positioner. The extension is fully compatible with the Twin-SAM and ELI phantoms.



**Picture C.9-1: Device Holder** 



Picture C.9-2: Laptop Extension Kit



#### No.I19Z61624-SEM03 Page 128 of 217

#### C.4.5 Phantom

The SAM Twin Phantom V4.0 is constructed of a fiberglass shell integrated in a table. The shape of the shell is based on data from an anatomical study designed to

Represent the 90<sup>th</sup> percentile of the population. The phantom enables the dissymmetric evaluation of SAR for both left and right handed handset usage, as well as body-worn usage using the flat phantom region. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. The shell phantom has a 2mm shell thickness (except the ear region where shell thickness increases to 6 mm).

Shell Thickness:2±0. 2 mmFilling Volume:Approx. 25 litersDimensions:810 x 1000 x 500 mm (H x L x W)Available:Special




Picture C.10: SAM Twin Phantom




## ANNEX D Position of the wireless device in relation to the phantom

#### **D.1 General considerations**

This standard specifies two handset test positions against the head phantom – the "cheek" position and the "tilt" position.

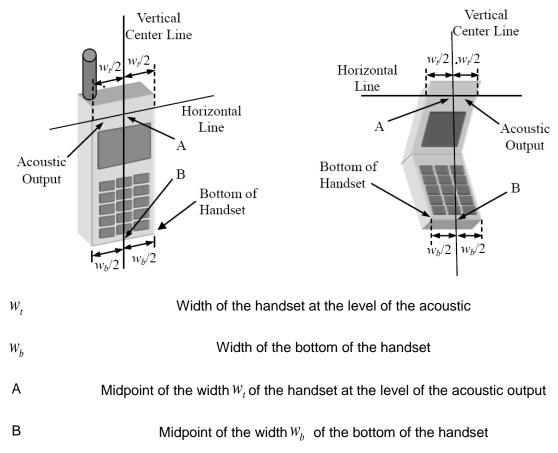


Picture D.1-a Typical "fixed" case handset Picture D.1-b Typical "clam-shell" case handset

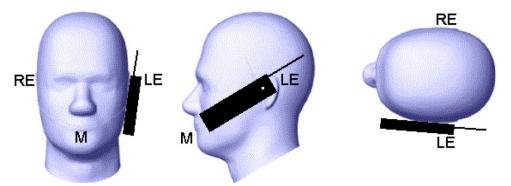

Picture D.2 Cheek position of the wireless device on the left side of SAM




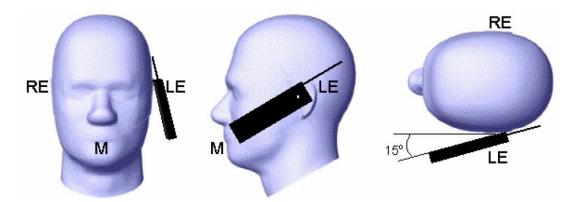

Picture D.3 Tilt position of the wireless device on the left side of SAM

#### D.2 Body-worn device

A typical example of a body-worn device is a mobile phone, wireless enabled PDA or other battery operated wireless device with the ability to transmit while mounted on a person's body using a carry accessory approved by the wireless device manufacturer.

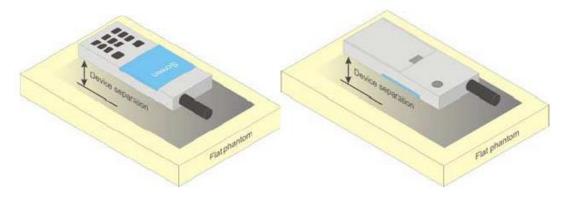


Picture D.4Test positions for body-worn devices

#### D.3 Desktop device

A typical example of a desktop device is a wireless enabled desktop computer placed on a table or desk when used.

The DUT shall be positioned at the distance and in the orientation to the phantom that corresponds to the intended use as specified by the manufacturer in the user instructions. For devices that employ an external antenna with variable positions, tests shall be performed for all antenna positions specified. Picture8.5 show positions for desktop device SAR tests. If the intended use is not specified, the device shall be tested directly against the flat phantom.

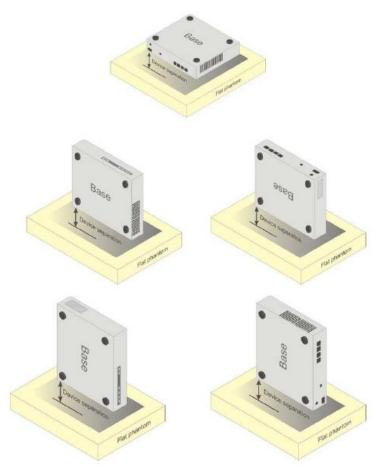

Picture D.5 Test positions for desktop devices



**D.4 DUT Setup Photos** 

Picture D.6



## ANNEX E Equivalent Media Recipes

The liquid used for the frequency range of 800-3000 MHz consisted of water, sugar, salt, preventol, glycol monobutyl and Cellulose. The liquid has been previously proven to be suited for worst-case. The Table E.1 shows the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the IEEE 1528 and IEC 62209.

		. Composit			Equivale	nt matter		
Frequency	835Head	835Body	1900	1900	2450	2450	5800	5800
(MHz)	osoneau		Head	Body	Head	Body	Head	Body
Ingredients (% by weight)								
Water	41.45	52.5	55.242	69.91	58.79	72.60	65.53	65.53
Sugar	56.0	45.0	١	١	١	١	١	١
Salt	1.45	1.4	0.306	0.13	0.06	0.18	١	١
Preventol	0.1	0.1	١	١	١	١	١	١
Cellulose	1.0	1.0	١	١	١	١	١	١
Glycol	``	,	44.450	00.00	44.45	07.00		,
Monobutyl		١	44.452	29.96	41.15	27.22	١	١
Diethylenglycol	``	``	\ \	N	``	N	17.04	17.04
monohexylether	Λ	١	١	١	۸	١	17.24	17.24
Triton X-100	\	\	١	١	١	١	17.24	17.24
Dielectric	ε=41.5		ε=40.0	c-E2 2	c=20.2	c=E0.7	c=25.2	ε=48.2
Parameters		ε=55.2		ε=53.3	ε=39.2	ε=52.7	ε=35.3	
Target Value	σ=0.90	σ=0.97	σ=1.40	σ=1.52	σ=1.80	σ=1.95	σ=5.27	σ=6.00
	•		•		•		•	-

Note: There are a little adjustment respectively for 750, 1750, 2600, 5200, 5300 and 5600 based on the recipe of closest frequency in table E.1.



## ANNEX F System Validation

The SAR system must be validated against its performance specifications before it is deployed. When SAR probes, system components or software are changed, upgraded or recalibrated, these must be validated with the SAR system(s) that operates with such components.

Probe SN.	Liquid name	Validation date	Frequency point	Status (OK or Not)
7514	Head 750MHz	Sep.10,2018	750 MHz	ÔK
7514	Head 850MHz	Sep.10,2018	835 MHz	ОК
7514	Head 900MHz	Sep.10,2018	900 MHz	OK
7514	Head 1750MHz	Sep.10,2018	1750 MHz	OK
7514	Head 1810MHz	Sep.10,2018	1810 MHz	OK
7514	Head 1900MHz	Sep.11,2018	1900 MHz	OK
7514	Head 2000MHz	Sep.11,2018	2000 MHz	OK
7514	Head 2100MHz	Sep.11,2018	2100 MHz	OK
7514	Head 2300MHz	Sep.11,2018	2300 MHz	OK
7514	Head 2450MHz	Sep.11,2018	2450 MHz	OK
7514	Head 2600MHz	Sep.12,2018	2600 MHz	OK
7514	Head 3500MHz	Sep.12,2018	3500 MHz	OK
7514	Head 3700MHz	Sep.12,2018	3700 MHz	OK
7514	Head 5200MHz	Sep.12,2018	5250 MHz	OK
7514	Head 5500MHz	Sep.12,2018	5600 MHz	OK
7514	Head 5800MHz	Sep.12,2018	5800 MHz	OK
7514	Body 750MHz	Sep.12,2018	750 MHz	OK
7514	Body 850MHz	Sep.9,2018	835 MHz	OK
7514	Body 900MHz	Sep.9,2018	900 MHz	OK
7514	Body 1750MHz	Sep.9,2018	1750 MHz	OK
7514	Body 1810MHz	Sep.9,2018	1810 MHz	OK
7514	Body 1900MHz	Sep.9,2018	1900 MHz	OK
7514	Body 2000MHz	Sep.13,2018	2000 MHz	OK
7514	Body 2100MHz	Sep.13,2018	2100 MHz	OK
7514	Body 2300MHz	Sep.13,2018	2300 MHz	OK
7514	Body 2450MHz	Sep.13,2018	2450 MHz	OK
7514	Body 2600MHz	Sep.13,2018	2600 MHz	OK
7514	Body 3500MHz	Sep.8,2018	3500 MHz	OK
7514	Body 3700MHz	Sep.8,2018	3700 MHz	OK
7514	Body 5200MHz	Sep.8,2018	5250 MHz	OK
7514	Body 5500MHz	Sep.8,2018	5600 MHz	OK
7514	Body 5800MHz	Sep.8,2018	5800 MHz	OK

Table F.1: System Validation for 7514



## ANNEX G Probe Calibration Certificate

#### **Probe 7514 Calibration Certificate**

Calibration Laborato Chmid & Partner Engineering AG Eughausstrasse 43, 8004 Zur		S C S	Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
ccredited by the Swiss Accredi he Swiss Accreditation Servi	Steaments and an end of the second second		reditation No.: SCS 0108
lient CTTL-BJ (Aud			EX3-7514_Aug18
CALIBRATION	CERTIFICATE		
Dbject	EX3DV4 - SN:751	4	
Calibration procedure(s)	QA CAL-25.v6	A CAL-12.v9, QA CAL-14.v4, QA lure for dosimetric E-field probes	CAL-23.v5,
Calibration date:	August 27, 2018		
The measurements and the und	certainties with confidence pro	al standards, which realize the physical units bability are given on the following pages and a facility: environment temperature $(22 \pm 3)^{\circ}C$ a	are part of the certificate.
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards	certainties with confidence pro lucted in the closed laboratory &TE critical for calibration)	bability are given on the following pages and a facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.)	are part of the certificate.
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP	certainties with confidence pro lucted in the closed laboratory &TE critical for calibration) ID SN: 104778	bability are given on the following pages and a facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 04-Apr-18 (No. 217-02672/02673)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91	certainties with confidence pro lucted in the closed laboratory &TE critical for calibration) ID SN: 104778 SN: 103244	bability are given on the following pages and a facility: environment temperature (22 ± 3)°C a         Cal Date (Certificate No.)         04-Apr-18 (No. 217-02672/02673)         04-Apr-18 (No. 217-02672)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91	certainties with confidence pro lucted in the closed laboratory &TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245	bability are given on the following pages and a facility: environment temperature (22 ± 3)°C a           Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672)/02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator	Certainties with confidence pro- lucted in the closed laboratory &TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: S5277 (20x)	bability are given on the following pages and a facility: environment temperature (22 ± 3)°C a           Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)           04-Apr-18 (No. 217-02673)           04-Apr-18 (No. 217-02673)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Apr-19 Apr-19
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference Probe ES3DV2	certainties with confidence pro lucted in the closed laboratory &TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245	bability are given on the following pages and a facility: environment temperature (22 ± 3)°C a           Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672)/02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4	Certainties with confidence pro- lucted in the closed laboratory &TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: S5277 (20x) SN: 3013	Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672)/02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)           04-Apr-18 (No. 217-02673)           04-Apr-18 (No. 217-02673)           04-Apr-17 (No. ES3-3013_Dec17)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Apr-19 Apr-19 Dec-18
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	Certainties with confidence pro- lucted in the closed laboratory &TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: S5277 (20x) SN: 3013 SN: 660	Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672)           04-Apr-17 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-17 (No. ES3-3013_Dec17)           21-Dec-17 (No. DAE4-660_Dec17)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Apr-19 Dec-18 Dec-18
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power meter E4419B	Certainties with confidence pro- lucted in the closed laboratory &TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 3013245 SN: 3013 SN: 660 ID	Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672)           04-Apr-17 (No. DAE1-060_Dec17)           21-Dec-17 (No. DAE4-660_Dec17)           Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Apr-19 Dec-18 Dec-18 Dec-18 Scheduled Check
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A	certainties with confidence producted in the closed laboratory           &TE critical for calibration)           ID           SN: 104778           SN: 103244           SN: 103245           SN: 3013           SN: 660           ID           SN: 6841293874           SN: 3N: 3010210	Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672)           04-Apr-17 (No. DAE4-660_Dec17)           21-Dec-17 (No. DAE4-660_Dec17)           Check Date (in house)           06-Apr-16 (in house check Jun-18)           06-Apr-16 (in house check Jun-18)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Apr-19 Dec-18 Dec-18 Scheduled Check In house check: Jun-20 In house check: Jun-20
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power meter E4419B Power sensor E4412A RF generator HP 8648C	certainties with confidence producted in the closed laboratory           &TE critical for calibration)           ID           SN: 104778           SN: 103244           SN: 103245           SN: 3013           SN: 660           ID           SN: 6841293874           SN: MY41498087           SN: 000110210           SN: US3642U01700	Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)           04-Apr-17 (No. DAE4-660_Dec17)           21-Dec-17 (No. DAE4-660_Dec17)           Check Date (in house)           06-Apr-16 (in house check Jun-18)           06-Apr-16 (in house check Jun-18)           04-Apr-16 (in house check Jun-18)           04-Apr-16 (in house check Jun-18)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Apr-19 Dec-18 Dec-18 Scheduled Check In house check: Jun-20 In house check: Jun-20 In house check: Jun-20 In house check: Jun-20
The measurements and the uno	certainties with confidence producted in the closed laboratory           &TE critical for calibration)           ID           SN: 104778           SN: 103244           SN: 103245           SN: 3013           SN: 660           ID           SN: 6841293874           SN: 3N: 3010210	Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672)           04-Apr-17 (No. DAE4-660_Dec17)           21-Dec-17 (No. DAE4-660_Dec17)           Check Date (in house)           06-Apr-16 (in house check Jun-18)           06-Apr-16 (in house check Jun-18)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Apr-19 Dec-18 Dec-18 Scheduled Check In house check: Jun-20 In house check: Jun-20
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power meter E4419B Power sensor E4412A RF generator HP 8648C	certainties with confidence producted in the closed laboratory           &TE critical for calibration)           ID           SN: 104778           SN: 103244           SN: 103245           SN: 3013           SN: 660           ID           SN: 6841293874           SN: MY41498087           SN: 000110210           SN: US3642U01700	Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)           04-Apr-17 (No. DAE4-660_Dec17)           21-Dec-17 (No. DAE4-660_Dec17)           Check Date (in house)           06-Apr-16 (in house check Jun-18)           06-Apr-16 (in house check Jun-18)           04-Apr-16 (in house check Jun-18)           04-Apr-16 (in house check Jun-18)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Apr-19 Dec-18 Dec-18 Scheduled Check In house check: Jun-20 In house check: Jun-20 In house check: Jun-20 In house check: Jun-20
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A RF generator HP 8648C Network Analyzer E8358A	certainties with confidence producted in the closed laboratory           &TE critical for calibration)           ID           SN: 104778           SN: 103244           SN: 103245           SN: 3013           SN: 660           ID           SN: GB41293874           SN: 00110210           SN: US3642U01700           SN: US41080477	Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02682)           30-Dec-17 (No. ES3-3013_Dec17)           21-Dec-17 (No. DAE4-660_Dec17)           Check Date (in house)           06-Apr-16 (in house check Jun-18)           06-Apr-16 (in house check Jun-18)           06-Apr-16 (in house check Jun-18)           04-Aug-99 (in house check Jun-18)           31-Mar-14 (in house check Oct-17)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Dec-18 Dec-18 Dec-18 Scheduled Check In house check: Jun-20 In house check: Oct-18
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power meter E4419B Power sensor E4412A RF generator HP 8648C	ID           ID           SN: 104778           SN: 103244           SN: 103245           SN: 3013           SN: 660           ID           SN: 660           SN: 00110210           SN: 00110210           SN: US3642U01700           SN: US41080477	Cal Date (Certificate No.)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672/02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02673)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02672)           04-Apr-18 (No. 217-02682)           30-Dec-17 (No. DAE4-660_Dec17)           21-Dec-17 (No. DAE4-660_Dec17)           Check Date (in house)           06-Apr-16 (in house check Jun-18)           06-Apr-16 (in house check Jun-18)           04-Aug-99 (in house check Jun-18)           04-Aug-99 (in house check Jun-18)           31-Mar-14 (in house check Oct-17)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Dec-18 Dec-18 Dec-18 Scheduled Check In house check: Jun-20 In house check: Oct-18
The measurements and the une All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power meter E44198 Power sensor E4412A RF generator HP 8648C Network Analyzer E8358A Calibrated by:	Certainties with confidence pro- lucted in the closed laboratory &TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 30132 SN: 3013 SN: 660 ID SN: GB41293874 SN: MY41498087 SN: 00110210 SN: US3642U01700 SN: US3642U01700 SN: US3642U01700 SN: US41080477 Name Jeton Kastrati	Cal Date (Certificate No.)         04-Apr-18 (No. 217-02672/02673)         04-Apr-18 (No. 217-02672)         04-Apr-18 (No. 217-02672)         04-Apr-18 (No. 217-02672)         04-Apr-18 (No. 217-02673)         04-Apr-18 (No. 217-02672)         04-Apr-18 (No. 217-02673)         04-Apr-18 (No. 217-02672)         04-Apr-17 (No. DAE4-660_Dec17)         21-Dec-17 (No. DAE4-660_Dec17)         Check Date (in house)         06-Apr-16 (in house check Jun-18)         06-Apr-16 (in house check Jun-18)         04-Aug-99 (in house check Oct-17)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-19 Apr-19 Apr-19 Dec-18 Dec-18 Dec-18 Scheduled Check In house check: Jun-20 In house check: Cot-18



#### No.I19Z61624-SEM03 Page 135 of 217

#### Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst S Service suisse d'étalonnage С

Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization 9	9 rotation around an axis that is in the plane normal to probe axis (at measurement center),
	i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

**Connector Angle** 

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement
- Techniques", June 2013 IEC 62209-1, ", "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from handb) held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices c) used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Methods Applied and Interpretation of Parameters:

- NORMx, y,z: Assessed for E-field polarization  $\vartheta = 0$  (f  $\leq 900$  MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: EX3-7514\_Aug18

Page 2 of 39



EX3DV4 - SN:7514

August 27, 2018

# Probe EX3DV4

## SN:7514

Manufactured: Calibrated: November 13, 2017 August 27, 2018

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: EX3-7514\_Aug18

Page 3 of 39

©Copyright. All rights reserved by CTTL.