

Specific Absorption Rate (SAR) Test Report

for
ZyXEL Communications Corporation
on the
CardBus 11Mbps Wireless LAN Card
Model Number: ZyAIR B-122



Test Report: EME-031071
Date of Report: Sep. 24, 2003
Date of test: Sep. 23, 2003

Total No of Pages Contained in this Report: 70



0597
ILAC MRA

Accredited for testing to FCC Part 15

| | |
|----------------------------|--|
| Tested by: Kevin Chen |  |
| Reviewed by: Elton Chen |  |

Review Date: Sep. 25, 2003

All services undertaken are subject to the following general policy: Reports are submitted for exclusive use of the client to whom they are addressed. Their significance is subject to the adequacy and representative character of the samples and to the comprehensiveness of the tests, examinations or surveys made. This report shall not be reproduced except in full, without written consent of Intertek Testing Services, Taiwan Ltd.

Table of Contents

| | |
|---|----|
| 1.0 Job Description | 4 |
| 1.1 Client Information..... | 4 |
| 1.2 Equipment under test (EUT)..... | 4 |
| 1.3 Test plan reference | 5 |
| 1.4 System test configuration..... | 5 |
| 1.4.1 System block diagram & Support equipment | 5 |
| 1.4.2 Test Position..... | 6 |
| 1.4.3 Test Condition | 6 |
| 1.5 Modifications required for compliance..... | 7 |
| 1.6 Additions, deviations and exclusions from standards | 7 |
| 2.0 SAR Evaluation | 8 |
| 2.1 SAR Limits | 8 |
| 2.2 Configuration Photographs | 9 |
| 2.3 SAR measurement system | 13 |
| 2.4 SAR measurement system validation | 14 |
| 2.5 Test Result..... | 15 |
| 3.0 Test Equipment | 17 |
| 3.1 Equipment List..... | 17 |
| 3.2 Body Tissue Simulating Liquid for evaluation test | 18 |
| 3.3 Head Tissue Simulating Liquid for System performance Check test | 18 |
| 3.4 E-Field Probe Calibration | 18 |
| 3.5 Measurement Uncertainty | 19 |
| 3.6 Measurement Traceability..... | 20 |
| 4.0 WARNING LABEL INFORMATION - USA | 21 |
| REFERENCES | 22 |
| DOCUMENT HISTORY | 23 |
| APPENDIX A - SAR Evaluation Data..... | 24 |
| APPENDIX B – 2450MHz body liquid Calibration Data | 45 |
| APPENDIX C - E-Field Probe Certificate and Calibration Data | 50 |

STATEMENT OF COMPLIANCE

The ZyXEL sample device, model # ZyAIR B-122 was evaluated in accordance with the requirements for compliance testing defined in FCC OET Bulletin 65, Supplement C (Edition 01-01). Testing was performed at the Intertek Testing Services facility in Hsinchu, Taiwan.

For the evaluation, the dosimetric assessment system INDEXSAR SARA2 was used. The phantom employed was the box phantom of 2mm thick in one wall. The total uncertainty for the evaluation of the spatial peak SAR values averaged over a cube of 1g tissue mass had been assessed for this system to be $\pm 20.6\%$.

The device was tested at their maximum output power declared by the ZyXEL.

In summary, the maximum spatial peak SAR value for the sample device averaged over 1g was found to be:

| Phantom | Position | SAR _{1g} , mW/g |
|----------------------------|---|--------------------------|
| 2mm thick box phantom wall | The EUT inserted into the left side of notebook PC, with EUT perpendicular to the phantom, 0 mm separatio | 0.180 mW/g. |

In conclusion, the tested Sample device was found to be in compliance with the requirements defined in OET Bulletin 65, Supplement C (Edition 01-01) for body configurations.

1.0 Job Description

1.1 Client Information

The ZyAIR B-122 has been tested at the request of:

Company: ZyXEL Communications Corporation
No. 6, Innovation Rd II, Science-Based Industrial Park,
Hsin-Chu, Taiwan

1.2 Equipment under test (EUT)

Product Descriptions:

| | | | |
|-----------------------|---|--------------------|--------------------------|
| Equipment | CardBus 11Mbps Wireless LAN Card | | |
| Trade Name | ZyXEL | Model No: | ZyAIR B-122 |
| FCC ID | I88B122 | S/N No. | Not Labeled |
| Category | Portable | RF Exposure | Uncontrolled Environment |
| Frequency Band | 2412 – 2462 MHz | System | DSSS |

| EUT Antenna Description | | | |
|--------------------------------|-------------|----------------------|---------|
| Type | Ceramic | Configuration | Fixed |
| Dimensions | 116 x 54 mm | Gain | 2.5 dBi |
| Location | Embedded | | |

Use of Product : Wireless Data Communication

Manufacturer: ZyXEL

Production is planned: ☒ Yes, ☐ No

EUT receive date: Sep. 1/, 2003

EUT received condition: Good operating condition prototype

Test start date: Sep. 23, 2003

Test end date: Sep. 23, 2003

1.3 Test plan reference

FCC Rule: Part 2.1093, FCC's OET Bulletin 65, Supplement C (Edition 01-01)

1.4 System test configuration

1.4.1 System block diagram & Support equipment

| Support Equipment | | | |
|-------------------|-----------|--------------|-----------|
| Item # | Equipment | Model No. | S/N |
| 1 | Notebook | PS240T-00UHT | 92043590J |



1.4.2 Test Position

See the photographs as section 2.2

1.4.3 Test Condition

During tests the worst-case data (max RF coupling) was determined with following conditions:

| | | | | |
|---|-----------------------------------|---|---|-----------------------------|
| Usage | Operates with a portable computer | Distance between antenna axis at the joint and the liquid surface: | Laptop is touching the Phantom in bottom side, perpendicular to phantom 15mm separating, perpendicular to phantom 0mm positions | |
| Simulating human Head/ Body/Hand | Body | EUT Battery | Device is powered from host computer through battery. | |
| Conducted output Power | Channel | Frequency MHz | Before SAR Test (dBm) | After SAR Test (dBm) |
| | Low Channel - 1 | 2412 | 14.93 | 14.95 |
| | Mid Channel - 6 | 2437 | 15.13 | 15.22 |
| | High Channel- 11 | 2462 | 15.33 | 15.30 |

The spatial peak SAR values were assessed for lowest, middle and highest operating channels, defined by the manufacturer.

The conducted output power was measured before and after the test using a diode detector, oscilloscope and signal generator.

Settle the EUT into Notebook, run the test program “ZDconfig”, under windows Os, provided by manufacturer. The EUT was transmitted continuously during all the test.

The EUT was transmitted continuously during the test.

After verifying the maximum output power, we found the maximum output power was occurred at 11Mbps data rate.

All the test data were performed under the above transmission rate.



FCC ID. : I88B122

Report No.: EME-031071

Page 7 of 70

1.5 Modifications required for compliance

Intertek Testing Services implemented no modifications.

1.6 Additions, deviations and exclusions from standards

The phantom employed was the box phantom of 2mm thick in vertical wall.

2.0 SAR Evaluation

2.1 SAR Limits

The following FCC limits for SAR apply to devices operate in General Population/Uncontrolled Exposure environment:

| EXPOSURE (General Population/Uncontrolled Exposure environment) | SAR (W/kg) |
|--|-----------------------|
| Average over the whole body | 0.08 |
| Spatial Peak (1g) | 1.60 |
| Spatial Peak for hands, wrists, feet and ankles (10g) | 4.00 |

2.2 Configuration Photographs

SAR Measurement Test Setup

Test System



SAR Measurement Test Setup

Bottom side of Laptop facing phantom touching



Bottom side of Laptop facing phantom touching – Zoom In




**SAR Measurement Test Setup
EUT perpendicular to phantom, 0 mm separation**



EUT perpendicular to phantom, 0 mm separation – Zoom In



SAR Measurement Test Setup
EUT perpendicular to phantom, 15 mm separation

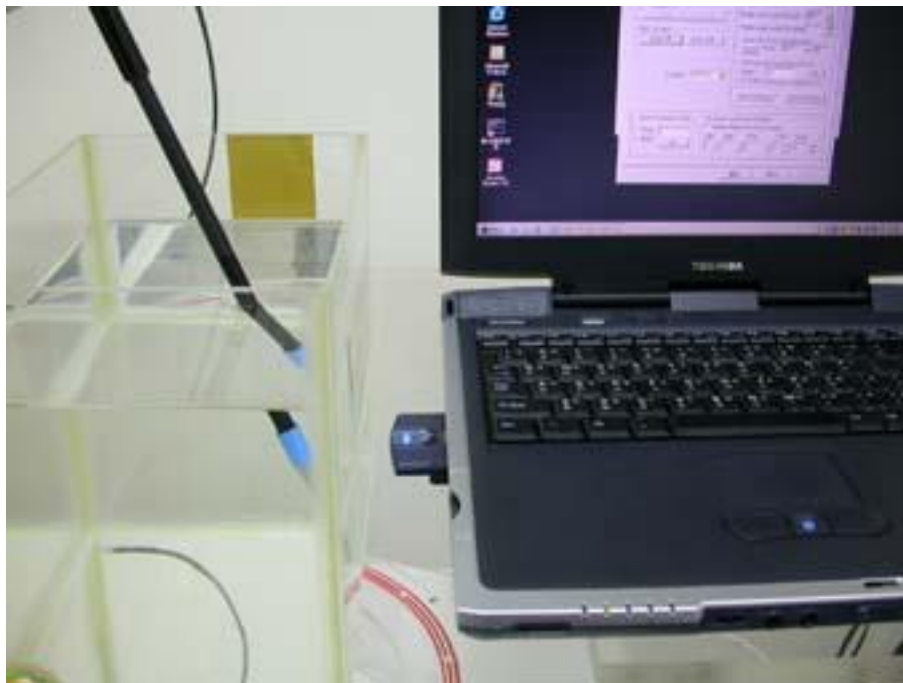

EUT perpendicular to phantom, 15 mm separation– Zoom In



2.3 SAR measurement system

Robot system specification

The SAR measurement system being used is the IndexSAR SARA2 system, which consists of a Mitsubishi RV-E2 6-axis robot arm and controller, IndexSAR probe and amplifier and SAM phantom Head Shape. The robot is used to articulate the probe to programmed positions inside the phantom head to obtain the SAR readings from the DUT.

The system is controlled remotely from a PC, which contains the software to control the robot and data acquisition equipment. The software also displays the data obtained from test scans.

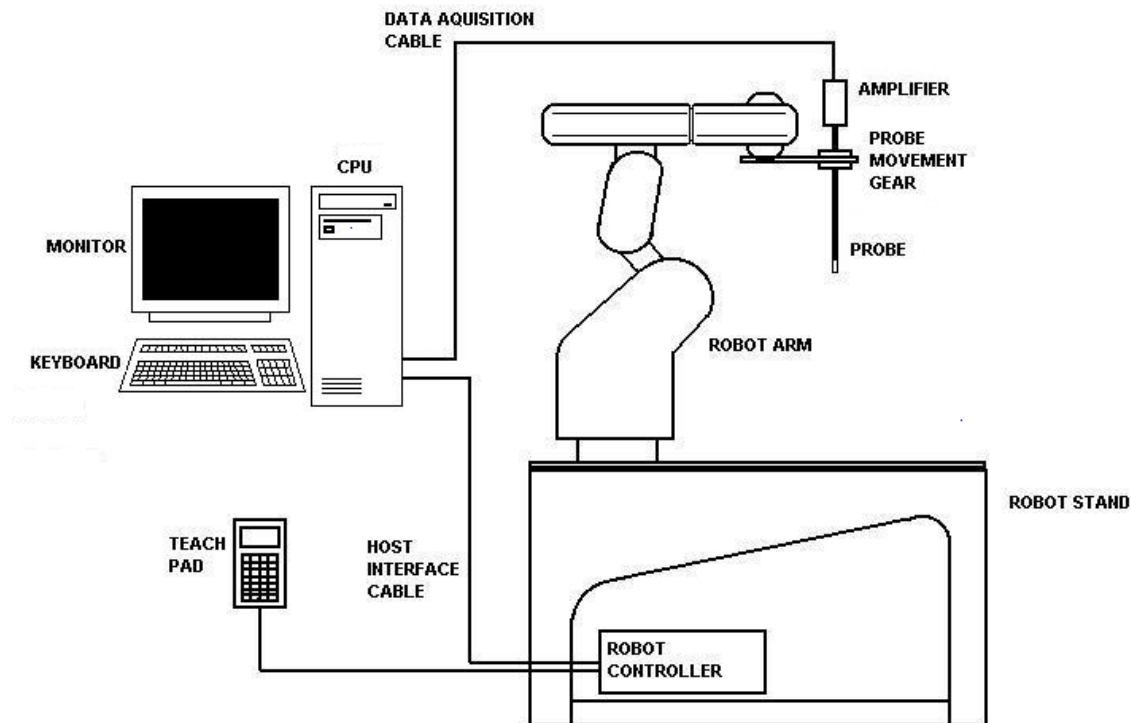


Figure 1: Schematic diagram of the SAR measurement system

The position and digitised shape of the phantom heads are made available to the software for accurate positioning of the probe and reduction of set-up time.

The SAM phantom heads are individually digitised using a Mitutoyo CMM machine to a precision of 0.02mm. The data is then converted into a shape format for the software, providing an accurate description of the phantom shell.

In operation, the system first does an area (2D) scan at a fixed depth within the liquid from the inside wall of the phantom. When the maximum SAR point has been found, the system will then carry out a 3D scan centred at that point to determine volume averaged SAR level.

2.4 SAR measurement system validation

Prior to the assessment, the system was verified to the $\pm 10\%$ of the specifications by using the system validation equipments. The validation was performed at 2450 MHz on the bottom side of box phantom.

Procedures

The SAR evaluation was performed with the following procedures:

- a. The SAR distribution was measured at the exposed side of the bottom of the box phantom and was measured at a distance of 8 mm from the inner surface of the shell. The feed power was 1/4W.
- b. The dimension for this cube is 32 mm x 32 mm x 34 mm was assessed by measuring 5 x 5 x 7 points. On the basis of this data set, the spatial peak SAR value was evaluated with the following procedure:
 - i) The data at the surface were extrapolated, since the center of the dipoles is 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measurement point is 5 mm. The extrapolation was based on a least square algorithm. A polynomial of the fourth order was calculated through the points in Z-axes. This polynomial was then used to evaluate the points between the surface and the probe tip.
 - ii) The maximum interpolated value was searched with a straightforward algorithm. Around this maximum, the SAR values averaged over the spatial volumes (1g or 10g) were computed using the 3-D spline interpolation algorithm. The 3-D spline is composed of three one-dimensional splines with the “Not a knot” condition (in x, y and z directions). The volume was integrated with the trapezoidal algorithm. 1000 points (10 x 10 x 10) were interpolated to calculate the average.
 - iii) All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.

| System Validation (2450 MHz Head) | | | | | |
|-----------------------------------|----------------|---------------------------------|-----------------------------------|--------------------------|-------------|
| Frequency MHz | Operating Mode | Target SAR _{1g} (mW/g) | Measured SAR _{1g} (mW/g) | Deviation ($\pm 10\%$) | Plot Number |
| 2450 | CW | 52.4 | 55.79 | 6.47% | 1 |

| System performance check (2450 MHz Head) | | | | | |
|--|----------------|---------------------------------|-----------------------------------|--------------------------|-------------|
| Frequency MHz | Operating Mode | Target SAR _{1g} (mW/g) | Measured SAR _{1g} (mW/g) | Deviation ($\pm 10\%$) | Plot Number |
| 2450 | CW | 52.4 | 49.78 | -5% | 2 |

2.5 Test Result

The results on the following page(s) were obtained when the device was tested in the condition described in this report. Detailed measurement data and plots, which reveal information about the location of the maximum SAR with respect to the device, are reported in Appendix A.

Measurement Results

| | | | |
|-------------------------------------|-------------------|------------------------------------|-------------|
| Trade Name: | ZyXEL | Model No.: | ZyAIR B-122 |
| Serial No.: | Not Labeled | Test Engineer: | Kevin Chen |
| TEST CONDITIONS | | | |
| Ambient Temperature | 23 °C | Relative Humidity | 50 % |
| Test Signal Source | Test Mode | Signal Modulation | DSSS |
| Output Power Before SAR Test | See page 6 | Output Power After SAR Test | See page 6 |
| Test Duration | 22 min. each scan | Number of Battery Change | 1 |

| EUT Position | | | | | | |
|----------------------|-----------------------|---------------------|--------------------------|----------------------|---|--------------------|
| Channel (MHz) | Operating Mode | Crest Factor | Description | Distance (mm) | Measured SAR_{1g} (mW/g) | Plot Number |
| 2437 | DSSS | 1 | Bottom of NoteBook PC | 0 | 0.093 | 3 |
| 2412 | DSSS | 1 | Bottom of NoteBook PC | 0 | 0.095 | 4 |
| 2462 | DSSS | 1 | Bottom of Note Book PC | 0 | 0.111 | 5 |
| 2437 | DSSS | 1 | Perpendicular to phantom | 15 | 0.032 | 6 |
| 2412 | DSSS | 1 | Perpendicular to phantom | 15 | 0.030 | 7 |
| 2462 | DSSS | 1 | Perpendicular to phantom | 15 | 0.040 | 8 |
| 2437 | DSSS | 1 | Perpendicular to phantom | 0 | 0.148 | 9 |
| 2412 | DSSS | 1 | Perpendicular to phantom | 0 | 0.142 | 10 |
| 2462 | DSSS | 1 | Perpendicular to phantom | 0 | 0.180 | 11 |

Note: The distance from bottom of EUT to flat phantom is 13 mm.

3.0 Test Equipment

3.1 Equipment List

The Specific Absorption Rate (SAR) tests were performed with the INDEXSAR SARA2 SYSTEM.

The following major equipment/components were used for the SAR evaluations:

| SAR Measurement System | | | |
|--|---|--------------------------|----------------|
| EQUIPMENT | SPECIFICATIONS | S/N # | LAST CAL. DATE |
| Balanced Validation dipole | 2450MHz | 0048 | N/A |
| Controller | Mitsubishi CR-E116 | F1008007 | N/A |
| Robot | Mitsubishi RV-E2 | EA009002 | N/A |
| | Repeatability: ± 0.04 mm; Number of Axes: 6 | | |
| E-Field Probe | IXP-050 | 0136 | 09/10/2003 |
| | Frequency Range: Probe outer diameter: 5.2 mm; Length: 350 mm; Distance between the probe tip and the dipole center: 2.7 mm | | |
| Data Acquisition | SARA2 | N/A | N/A |
| | Processor: Pentium 4; Clock speed: 1.5GHz; OS: Windows XP; I/O: two RS232; Software: SARA2 ver. 0.421N | | |
| Phantom | 2mm wall thickness box phantom | N/A | N/A |
| | Shell Material: clear Perspex; Thickness: 2 ± 0.1 mm; Capacity: 152.5 x 215.5 x 200 (W x L x D) mm ³ ; Dielectric constant: less than 2.85 above 500MHz; | | |
| Device holder | Material: clear Perspex; Dielectric constant: less than 2.85 above 500MHz | N/A | N/A |
| Simulated Tissue | Mixture | N/A | N/A |
| | Please see section 3.2 for details | | |
| RF Power Meter | Boonton 4231A with 51011-EMC power sensor | 79401-32482 | 03/21/2003 |
| | Frequency Range: 0.03 to 8 GHz, <24dBm | | |
| RF Power Amplifier | INDEXSAR VTL5400 | 0302 | 01/23/2003 |
| | 10MHz to 2.5GHz, Gain >30dB | | |
| Directional Coupler | INDEXSAR VDC0830-20 | 0302 | 05/19/2003 |
| | 0.8 to 3 GHz, Max. Power<500W | | |
| Vector Network Analyzer | HP 8753B HP 85046A | 2807J04037 2729A01958 | 07/04/2003 |
| | 300k to 3GHz | | |
| Signal Generator | R&S SMR27 | 100036 | 09/19/2003 |
| | 10M to 27GHz, <120dBuV | | |
| Crystal Detector | Agilent 8472B | MY42240243 | N/A |
| | 10MHz to 18GHz | | |
| Two Channel Digital Storage Oscilloscope | Tektronix TDS1012 | C031679 | Aug. 16, 2003 |

3.2 Body Tissue Simulating Liquid for evaluation test

The dielectric parameters were verified prior to assessment using the HP 85046A dielectric probe kit and the HP 8753B network Analyzer. The dielectric parameters were:

| Frequency (MHz) | Temp. (°C) | e _r / Relative Permittivity | | | s / Conductivity (mho/m) | | | ρ *(kg/m ³) |
|-----------------|------------|--|--------|--------|--------------------------|--------|--------|-------------------------|
| 2450 | 22.5 | measured | target | Δ(±5%) | measured | target | Δ(±5%) | 1000 |
| | | 51.15 | 52.7 | -2.9% | 1.952 | 1.95 | 0.10% | |

* Worst-case assumption

Test data is included in Appendix B.

3.3 Head Tissue Simulating Liquid for System performance Check test

The dielectric parameters were verified prior to assessment using the HP 85046A dielectric probe kit and the HP 8753B network Analyzer. The dielectric parameters were:

| Frequency (MHz) | Temp. (°C) | e _r / Relative Permittivity | | | s / Conductivity (mho/m) | | | ρ *(kg/m ³) |
|-----------------|------------|--|--------|--------|--------------------------|--------|--------|-------------------------|
| 2450 | 23.5 | measured | target | Δ(±5%) | measured | target | Δ(±5%) | 1000 |
| | | 38.398 | 39.2 | -2.05% | 1.779 | 1.80 | -1.17 | |

* Worst-case assumption

3.4 E-Field Probe Calibration

Probe calibration factors are included in Appendix C.

3.5 Measurement Uncertainty

The uncertainty budget has been determined for the INDEXSAR SARA2 measurement system according to IEEE P1528 documents [3] and is given in the following table. The extended uncertainty (95% confidence level) was assessed to be 20.6 %

| Uncertainty Component | Sec. | (dB) | Tol.(+/-) | (%) | Prob. Dist. | Divisor (descript) | Divisor (value) | c1 | Standard Uncertainty (%) |
|---|---------|------|-----------|-------|-------------|--------------------|-----------------|------|--------------------------|
| Measurement System | | | | | | | | | |
| Probe Calibration | E 2.1 | | | 2.5 | N | 1 or k | 1 | 1 | 2.50 |
| Axial Isotropy | E 2.2 | 0.25 | 5.93 | 5.93 | R | $\sqrt{3}$ | 1.73 | 0 | 0.00 |
| Hemispherical Isotropy | E 2.2 | 0.45 | 10.92 | 10.92 | R | $\sqrt{3}$ | 1.73 | 1 | 6.30 |
| Boundary effects | E 2.3 | | 4 | 4.00 | R | $\sqrt{3}$ | 1.73 | 1 | 2.31 |
| Linearity | E 2.4 | 0.04 | 0.93 | 0.93 | R | $\sqrt{3}$ | 1.73 | 1 | 0.53 |
| System Detection Limits | E 2.5 | | 1 | 1.00 | R | $\sqrt{3}$ | 1.73 | 1 | 0.58 |
| Readout Electronics | E 2.6 | | 1 | 1.00 | N | 1 or k | 1.00 | 1 | 1.00 |
| Response time | E 2.7 | | 0 | 0.00 | R | $\sqrt{3}$ | 1.73 | 1 | 0.00 |
| Integration time | E 2.8 | | 1.4 | 1.40 | R | $\sqrt{3}$ | 1.73 | 1 | 0.81 |
| RF Ambient Conditions | E 6.1 | | 3 | 3.00 | R | $\sqrt{3}$ | 1.73 | 1 | 1.73 |
| Probe Positioner Mechanical Tolerance | E 6.2 | | 0.6 | 0.60 | R | $\sqrt{3}$ | 1.73 | 1 | 0.35 |
| Probe Position wrt. Phantom Shell | E 6.3 | | 3 | 3.00 | R | $\sqrt{3}$ | 1.73 | 1 | 1.73 |
| SAR Evaluation Algorithms | E 5 | | 8 | 8.00 | R | $\sqrt{3}$ | 1.73 | 1 | 4.62 |
| Test Sample Related | | | | | | | | | |
| Test Sample Positioning | E 4.2 | | 2 | 2.00 | N | 1 | 1.00 | 1 | 2.00 |
| Device Holder Uncertainty | E 4.1 | | 2 | 2.00 | N | 1 | 1.00 | 1 | 2.00 |
| Output Power Variation | E 6.6.2 | | 5 | 5.00 | R | $\sqrt{3}$ | 1.73 | 1 | 2.89 |
| Phantom and tissue Parameters | | | | | | | | | |
| Phantom Uncertainty (shape and thickness) | E 3.1 | | 4 | 4.00 | R | $\sqrt{3}$ | 1.73 | 1 | 2.31 |
| Liquid conductivity (Deviation from target) | E 3.2 | | 5 | 5.00 | R | $\sqrt{3}$ | 1.73 | 0.64 | 1.85 |
| Liquid conductivity (Meas. Uncertainty) | E 3.3 | | 1.1 | 1.10 | N | 1 | 1.00 | 0.64 | 0.70 |
| Liquid permittivity (Deviation from target) | E 3.2 | | 5 | 5.00 | R | $\sqrt{3}$ | 1.73 | 0.6 | 1.73 |
| Liquid permittivity (Meas. Uncertainty) | E 3.3 | | 1.1 | 1.10 | N | 1 | 1.00 | 0.6 | 0.66 |
| Combined standard uncertainty | | | | | RSS | | | | 10.5 |



FCC ID. : I88B122

Report No.: EME-031071

Page 20 of 70

3.6 Measurement Traceability

All measurements described in this report are traceable to Chinese National Laboratory Accreditation (CNLA) standards or appropriate national standards.



FCC ID. : I88B122

Report No.: EME-031071

Page 21 of 70

4.0 WARNING LABEL INFORMATION - USA

See user manual.

REFERENCES

- [1] ANSI, *ANSI/IEEE C95.1-1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3kHz to 300 GHz*, The Institute of electrical and Electronics Engineers, Inc., New York, NY 10017, 1999

- [2] Federal Communications Commission, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", OET Bulletin 65, FCC, Washington, D.C. 20554, 1997

- [3] IEEE Standards Coordinating Committee 34, "*DRAFT* Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Measurement Techniques", IEEE Std 1528-200X, Draft CD 1.2 – April 21, 2003

DOCUMENT HISTORY

| Revision/ Job Number | Writer Initials | Date | Change |
|-------------------------|--------------------|---------------|-------------------|
| N/A | J.C. | Sep. 24, 2003 | Original document |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |

APPENDIX A - SAR Evaluation Data

Power drift is the measurement of power drift of the device over one complete SAR scan.


To assess the drift of the power of the device under test, a SAR measurement was made in the middle of the zoom scan volume at the start of the scan and a measurement at this point was then also made after the measurement scan. The difference between the two measurements should be less than 5%.

Plot #1

| | | | |
|-----------------------|----------------|------------------------|-----------|
| Date: | 2003/3/7 | Position: | Bottom |
| Filename: | 2450val3-7.txt | Phantom: | Box1.csv |
| Device Tested: | SARA2 system | Head Rotation: | 0 |
| Antenna: | 2450dipole | Test Frequency: | 2450MHz |
| Shape File: | none.csv | Power Level: | 24dBm /CW |

| | | | | |
|----------------------------|---------------------|----------|----------|----------|
| Probe: | 0114 | | | |
| Cal File: | SN0114_2450_CW_HEAD | | | |
| Cal Factors: | | X | Y | Z |
| | Air | 532 | 494 | 450 |
| | DCP | 20 | 20 | 20 |
| | Lin | .495 | .495 | .495 |
| Amp Gain: | 2 | | | |
| Averaging: | 1 | | | |
| Batteries Replaced: | N/A | | | |

| | |
|-------------------------------|--------------|
| Liquid: | 15.1cm |
| Type: | 2450MHz Head |
| Conductivity: | 1.790 |
| Relative Permittivity: | 38.050 |
| Liquid Temp (deg C): | 23 |
| Ambient Temp (deg C): | 22.1 |
| Ambient RH (%): | 63 |
| Density (kg/m3): | 1000 |
| Software Version: | 0.421N |
| Crest Factor = 1 | |

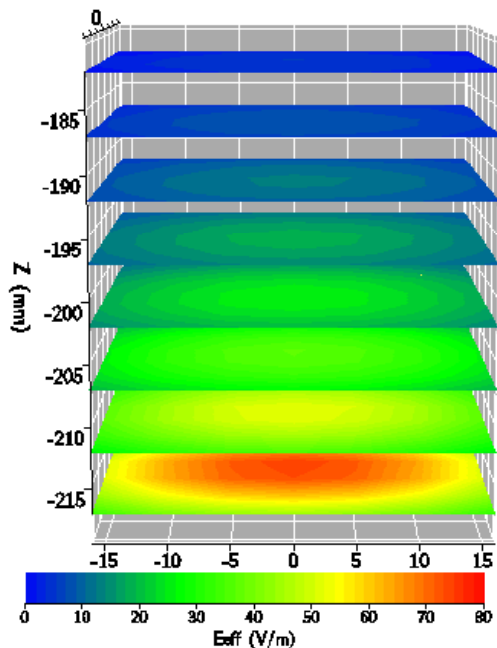

ZOOM SCAN RESULTS:

| | | |
|-------------------------|-------------------|-----------------|
| Spot SAR (W/kg): | Start Scan | End Scan |
| | | |

Change during Scan (%)

Max E-field (V/m): 76.33

| | | |
|-----------------------|-----------|------------|
| Max SAR (W/kg) | 1g | 10g |
| | 13.9475 | 6.54 |

| | | | |
|------------------------------|----------|----------|----------|
| Location of Max (mm): | X | Y | Z |
| | 2.7 | 1.4 | -223.0 |

Normalized to an input power of 1W
Averaged over 1 cm³ (1g) of tissue
55.79 W/kg

Plot #2

| | | | |
|-----------------------|------------------------|------------------------|---------------|
| Date / Time: | 17/09/2003 | Position: | bottom of box |
| Filename: | 2450 performance-2.txt | Phantom: | HeadBox1.csv |
| Device Tested: | 2450 performance check | Head Rotation: | 0 |
| Antenna: | dipole antenna | Test Frequency: | 2450MHz |
| Shape File: | none.csv | Power Level: | 24dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_HEAD | Type: | 2450MHz Head |
| Cal Factors: | | Conductivity: | 1.7788 |
| | | Relative Permittivity: | 38.3985 |
| | | Liquid Temp (deg C): | 23.5 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | - | Software Version: | 0.421N |
| | | Crest Factor: | 1 |

The figure displays a 3D surface plot of the electric field (E-field) distribution within a rectangular volume. The vertical axis is labeled 'Z (mm)' and ranges from -190 to -210. The horizontal axes are labeled 'X (mm)' and 'Y (mm)', both ranging from -15 to 15. A color bar at the bottom indicates the E-field magnitude in V/m, with a scale from 0 (blue) to 80 (red). The plot shows a high-intensity region (red/orange) centered around Z = -205 mm, Y = 0 mm, and X = 0 mm, with the intensity decreasing towards the edges (blue/green).

ZOOM SCAN RESULTS:

Spot SAR

(W/kg):

| Start Scan | End Scan |
|------------|----------|
| | |

Change during

Scan (%)

Max E-field

(V/m):

71.99

Max SAR (W/kg)

| 1g | 10g |
|--------|-------|
| 12.445 | 5.911 |

Location of Max

(mm):

| X | Y | Z |
|-----|-----|--------|
| 1.3 | 0.0 | -222.5 |

Normalized to an input power of 1W


Averaged over 1 cm³ (1g) of tissue

49.78 W/kg

Plot #3 (1/2)

| | | | |
|-----------------------|--------------------|------------------------|--------------|
| Date / Time: | 2003/9/23 | Position: | bottom 0mm |
| Filename: | b-122-2437bot0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2437MHz |
| Shape File: | 122bottom.csv | Power Level: | 15.13dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_BODY | Type: | 2450MHz Body |
| Cal Factors: | | Conductivity: | 1.95229 |
| | | Relative Permittivity: | 51.1547 |
| | | Liquid Temp (deg C): | 22.8 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | 1 | Software Version: | 0.421N |
| | | Crest Factor: | 1 |

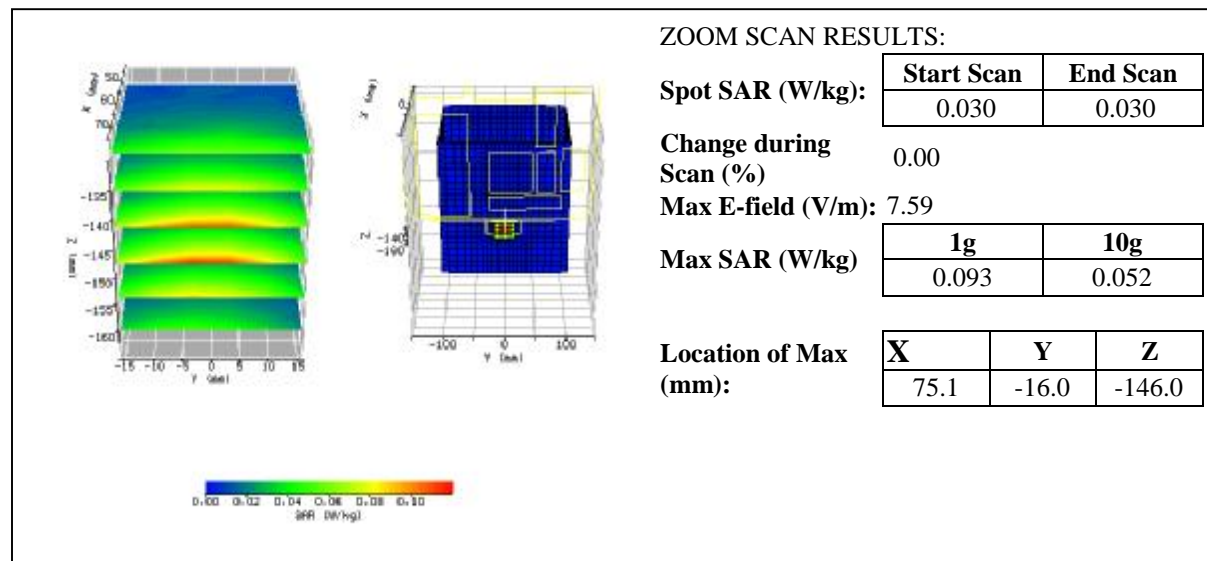


Plot #3 (2/2)

| | | | |
|-----------------------|--------------------|------------------------|--------------|
| Date / Time: | 2003/9/23 | Position: | bottom 0mm |
| Filename: | b-122-2437bot0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2437MHz |
| Shape File: | 122bottom.csv | Power Level: | 15.13dBm |

AREA SCAN:

Scan Extent:

| | Min | Max | Steps |
|----------|--------|--------|-------|
| Y | -35.0 | 35.0 | 7.0 |
| Z | -170.0 | -120.0 | 5.0 |

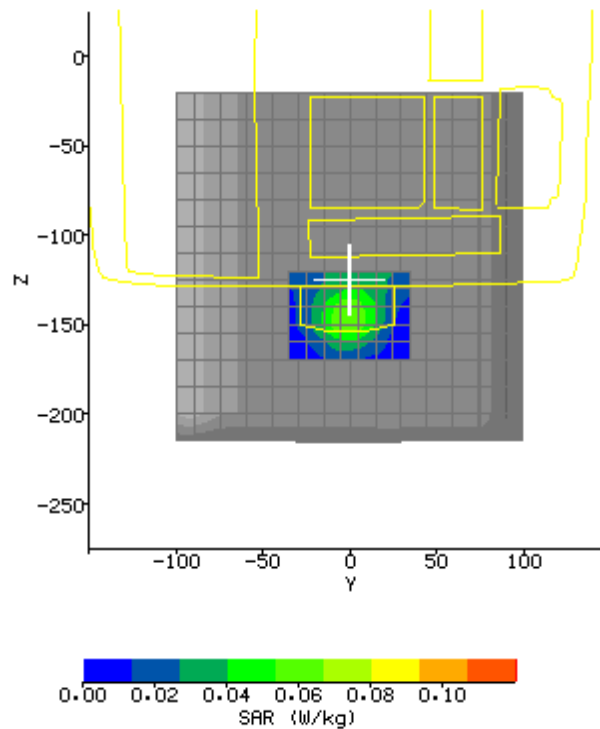

Plot #4 (1/2)

| | | | |
|-----------------------|--------------------|------------------------|--------------|
| Date / Time: | 2003/9/23 | Position: | bottom 0mm |
| Filename: | b-122-2412bot0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2412MHz |
| Shape File: | 122bottom.csv | Power Level: | 14.93dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_BODY | Type: | 2450MHz Body |
| Cal Factors: | | Conductivity: | 1.95229 |
| | | Relative Permittivity: | 51.1547 |
| | | Liquid Temp (deg C): | 22.8 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | 1 | Software Version: | 0.421N |
| | | Crest Factor: | 1 |

The figure displays two 3D surface plots of Specific Absorption Rate (SAR) distribution. The left plot shows a color-coded SAR distribution on a rectangular volume, with axes X (mm) from -15 to 10, Y (mm) from -100 to 100, and Z (mm) from -180 to 50. The right plot shows a similar distribution on a different volume. A color bar at the bottom indicates SAR values from 0.00 to 0.10 W/kg.

ZOOM SCAN RESULTS:

Spot SAR (W/kg):

| Start Scan | End Scan |
|------------|----------|
| 0.025 | 0.026 |

Change during Scan (%) 2.56

Max E-field (V/m): 7.73

Max SAR (W/kg)

| 1g | 10g |
|-------|-------|
| 0.095 | 0.052 |

Location of Max (mm):

| X | Y | Z |
|------|-------|--------|
| 75.1 | -17.0 | -145.0 |


Plot #4 (2/2)

| | | | |
|-----------------------|--------------------|------------------------|--------------|
| Date / Time: | 2003/9/23 | Position: | bottom 0mm |
| Filename: | b-122-2412bot0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2412MHz |
| Shape File: | 122bottom.csv | Power Level: | 14.93dBm |

AREA SCAN:

Scan Extent:


| | Min | Max | Steps |
|----------|--------|--------|-------|
| Y | -35.0 | 35.0 | 7.0 |
| Z | -170.0 | -120.0 | 5.0 |

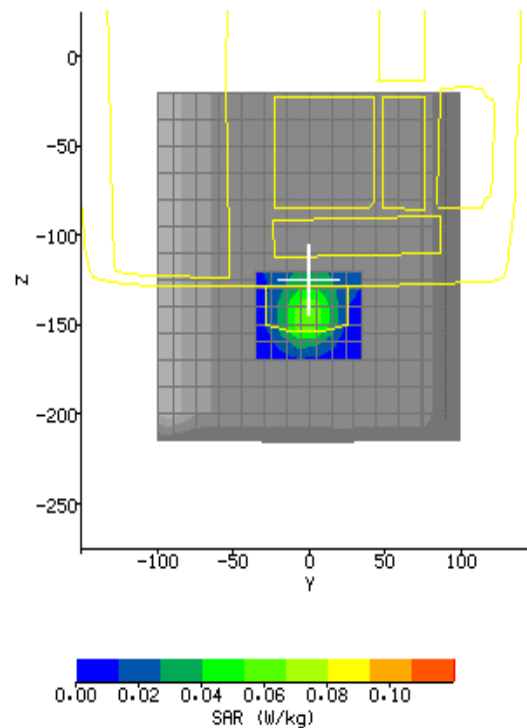

Plot #5 (1/2)

| | | | |
|-----------------------|--------------------|------------------------|--------------|
| Date / Time: | 2003/9/23 | Position: | bottom 0mm |
| Filename: | b-122-2462bot0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2462MHz |
| Shape File: | 122bottom.csv | Power Level: | 15.33dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_BODY | Type: | 2450MHz Body |
| Cal Factors: | | Conductivity: | 1.95229 |
| | | Relative Permittivity: | 51.1547 |
| | | Liquid Temp (deg C): | 22.8 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | 1 | Software Version: | 0.421N |
| | | Crest Factor: | 1 |

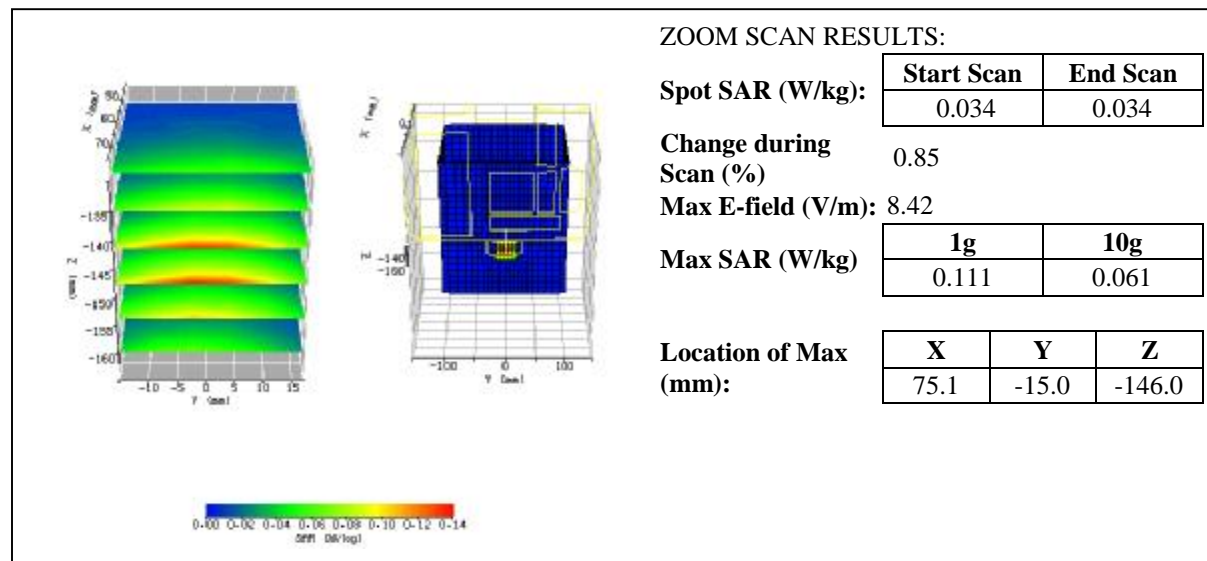


Plot #5 (2/2)

| | | | |
|-----------------------|--------------------|------------------------|--------------|
| Date / Time: | 2003/9/23 | Position: | bottom 0mm |
| Filename: | b-122-2462bot0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2462MHz |
| Shape File: | 122bottom.csv | Power Level: | 15.33dBm |

AREA SCAN:

Scan Extent:


| | Min | Max | Steps |
|----------|--------|--------|-------|
| Y | -35.0 | 35.0 | 7.0 |
| Z | -170.0 | -120.0 | 5.0 |

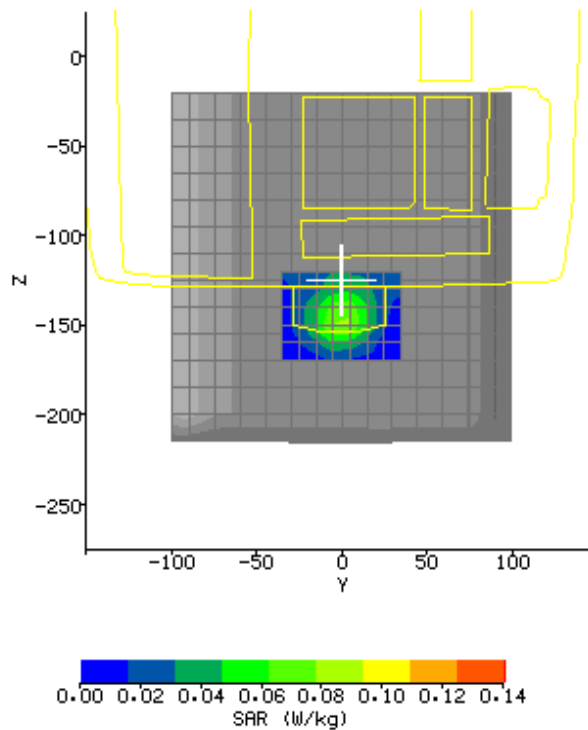

Plot #6 (1/2)

| | | | |
|-----------------------|---------------------|------------------------|--------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 15mm |
| Filename: | b-122-2437per15.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2437MHz |
| Shape File: | 122left.csv | Power Level: | 15.13dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_BODY | Type: | 2450MHz Body |
| Cal Factors: | | Conductivity: | 1.95229 |
| | | Relative Permittivity: | 51.1547 |
| | | Liquid Temp (deg C): | 22.8 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | 1 | Software Version: | 0.421N |
| | | Crest Factor: | 1 |

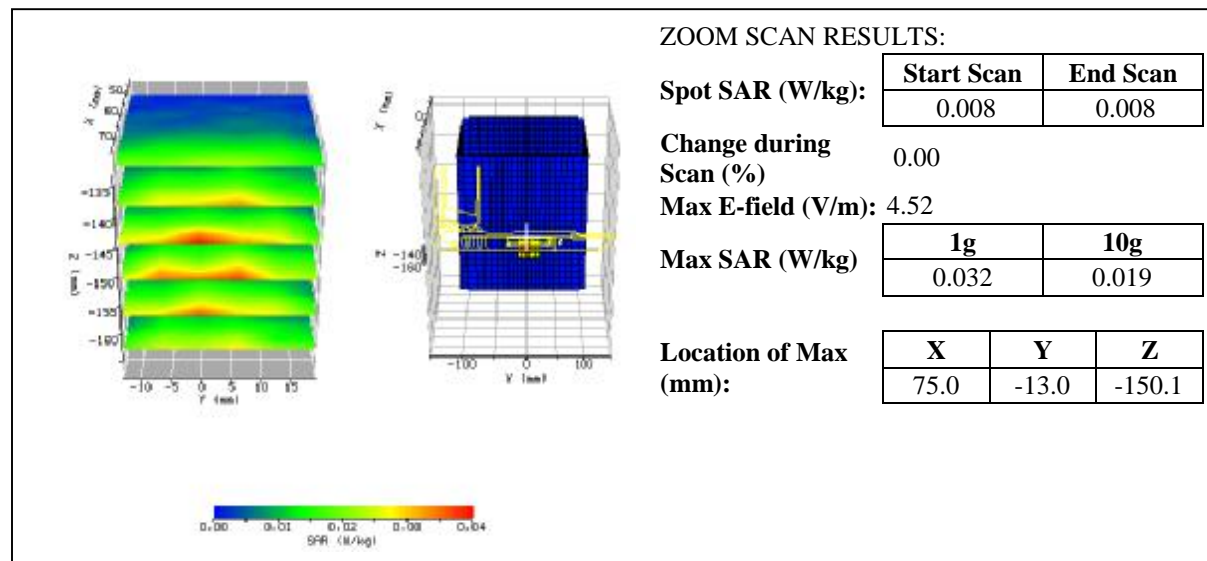


Plot #6 (2/2)

| | | | |
|-----------------------|---------------------|------------------------|--------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 15mm |
| Filename: | b-122-2437per15.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2437MHz |
| Shape File: | 122left.csv | Power Level: | 15.13dBm |

AREA SCAN:

Scan Extent:


| | Min | Max | Steps |
|----------|--------|--------|-------|
| Y | -30.0 | 30.0 | 6.0 |
| Z | -170.0 | -130.0 | 4.0 |

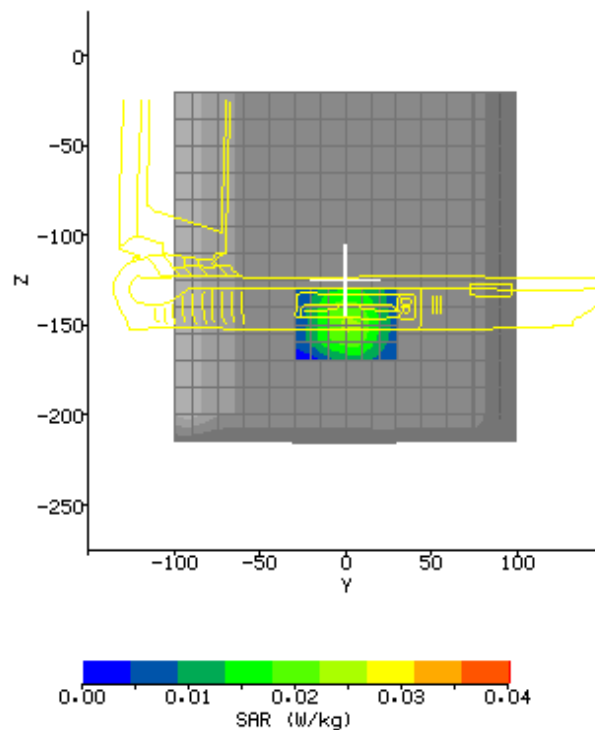

Plot #7 (1/2)

| | | | |
|-----------------------|---------------------|------------------------|--------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 15mm |
| Filename: | b-122-2412per15.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2412MHz |
| Shape File: | 122left.csv | Power Level: | 14.93dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_BODY | Type: | 2450MHz Body |
| Cal Factors: | | Conductivity: | 1.95229 |
| | | Relative Permittivity: | 51.1547 |
| | | Liquid Temp (deg C): | 22.8 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | 1 | Software Version: | 0.421N |
| | | Crest Factor: | 1 |

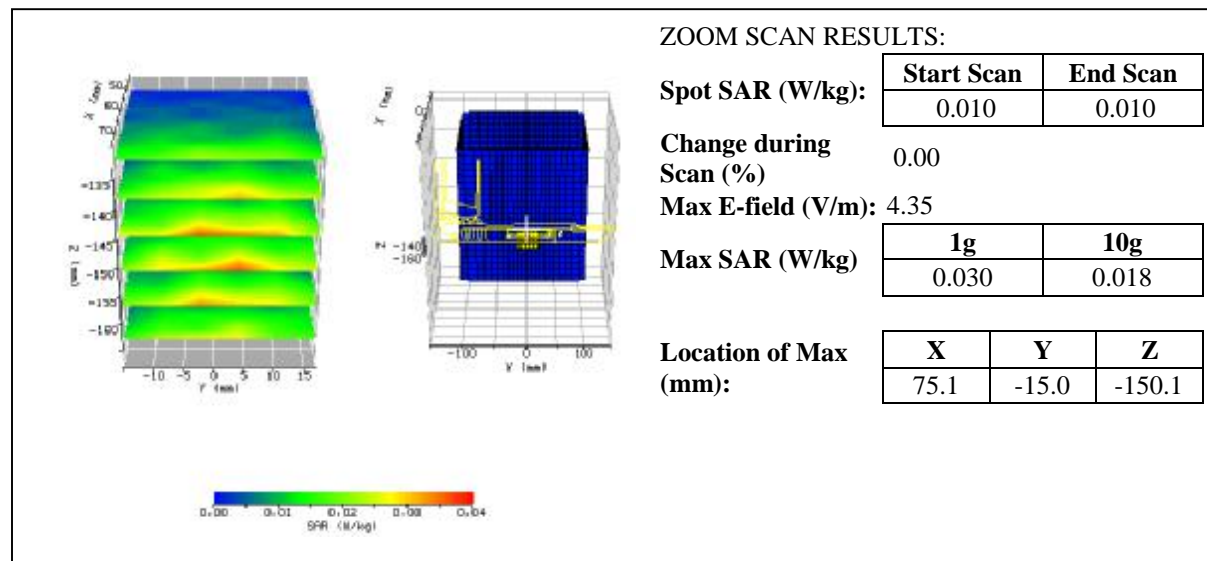


Plot #7 (2/2)

| | | | |
|-----------------------|---------------------|------------------------|--------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 15mm |
| Filename: | b-122-2412per15.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2412MHz |
| Shape File: | 122left.csv | Power Level: | 14.93dBm |

AREA SCAN:

Scan Extent:


| | Min | Max | Steps |
|----------|--------|--------|-------|
| Y | -30.0 | 30.0 | 6.0 |
| Z | -170.0 | -130.0 | 4.0 |

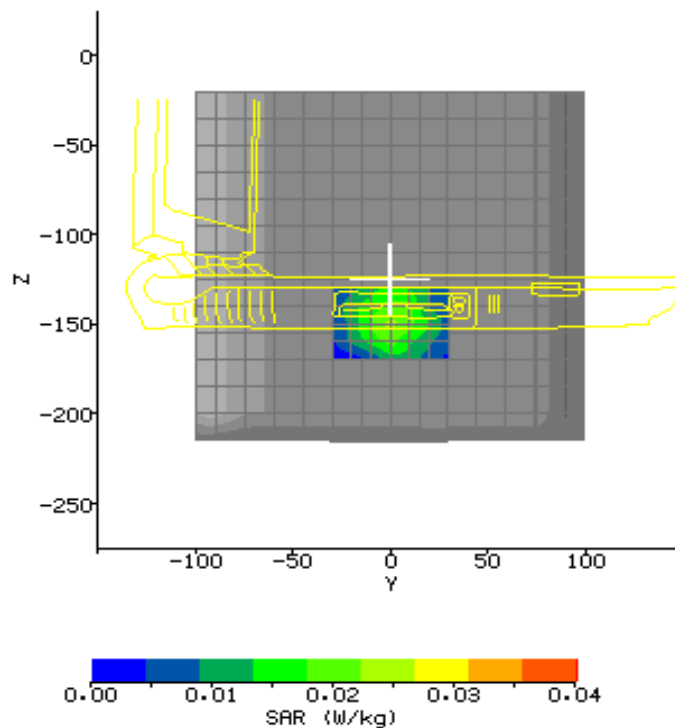

Plot #8 (1/2)

| | | | |
|-----------------------|---------------------|------------------------|--------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 15mm |
| Filename: | b-122-2462per15.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2462MHz |
| Shape File: | 122left.csv | Power Level: | 15.33dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_BODY | Type: | 2450MHz Body |
| Cal Factors: | | Conductivity: | 1.95229 |
| | | Relative Permittivity: | 51.1547 |
| | | Liquid Temp (deg C): | 22.8 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | 1 | Software Version: | 0.421N |
| | | Crest Factor: | 1 |

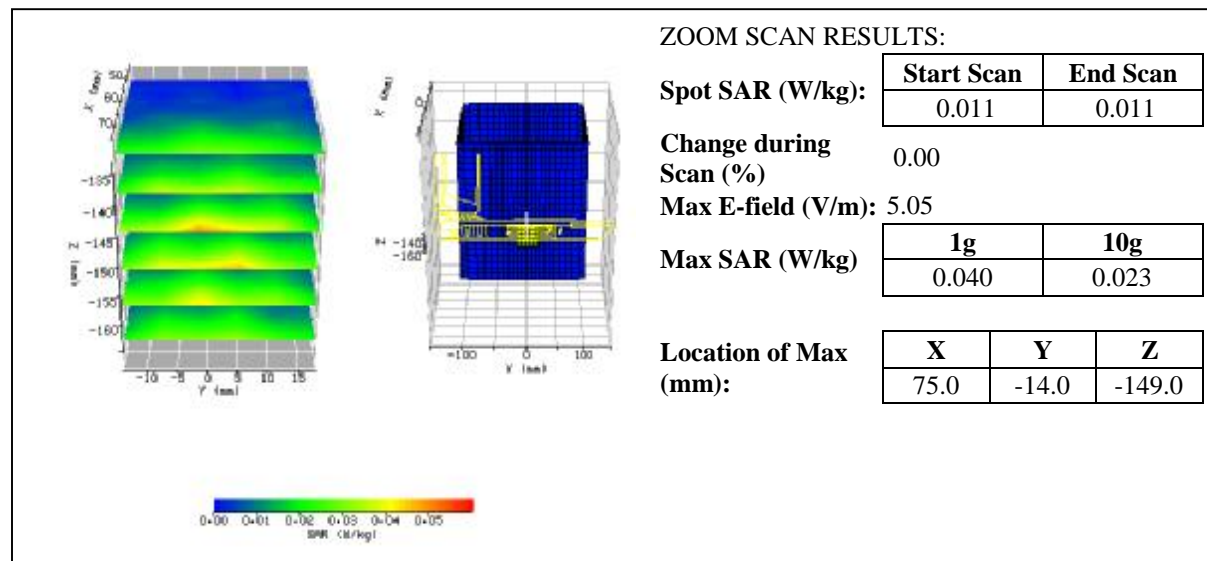


Plot #8 (2/2)

| | | | |
|-----------------------|---------------------|------------------------|--------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 15mm |
| Filename: | b-122-2462per15.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2462MHz |
| Shape File: | 122left.csv | Power Level: | 15.33dBm |

AREA SCAN:

Scan Extent:


| | Min | Max | Steps |
|---|--------|--------|-------|
| Y | -30.0 | 30.0 | 6.0 |
| Z | -170.0 | -130.0 | 4.0 |

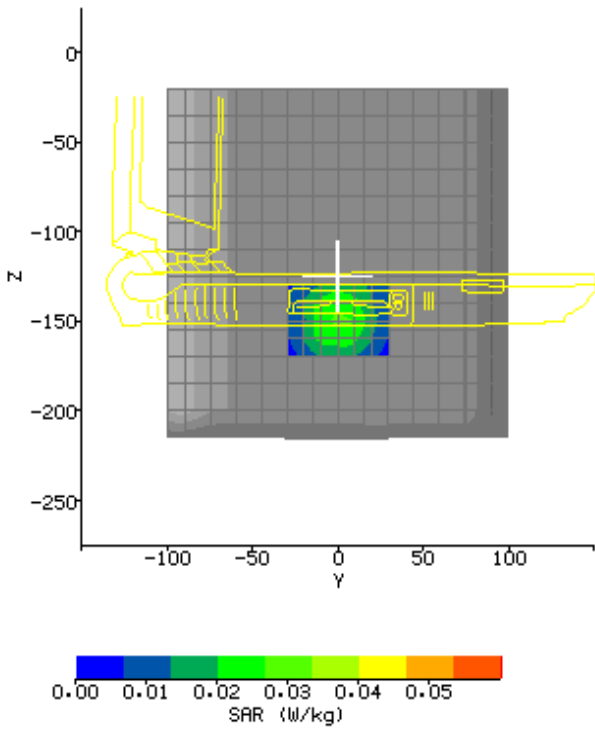

Plot #9 (1/2)

| | | | |
|-----------------------|--------------------|------------------------|-------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 0mm |
| Filename: | b-122-2437per0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2437MHz |
| Shape File: | 122left.csv | Power Level: | 15.13dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_BODY | Type: | 2450MHz Body |
| Cal Factors: | | Conductivity: | 1.95229 |
| | | Relative Permittivity: | 51.1547 |
| | | Liquid Temp (deg C): | 22.8 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | 1 | Software Version: | 0.421N |

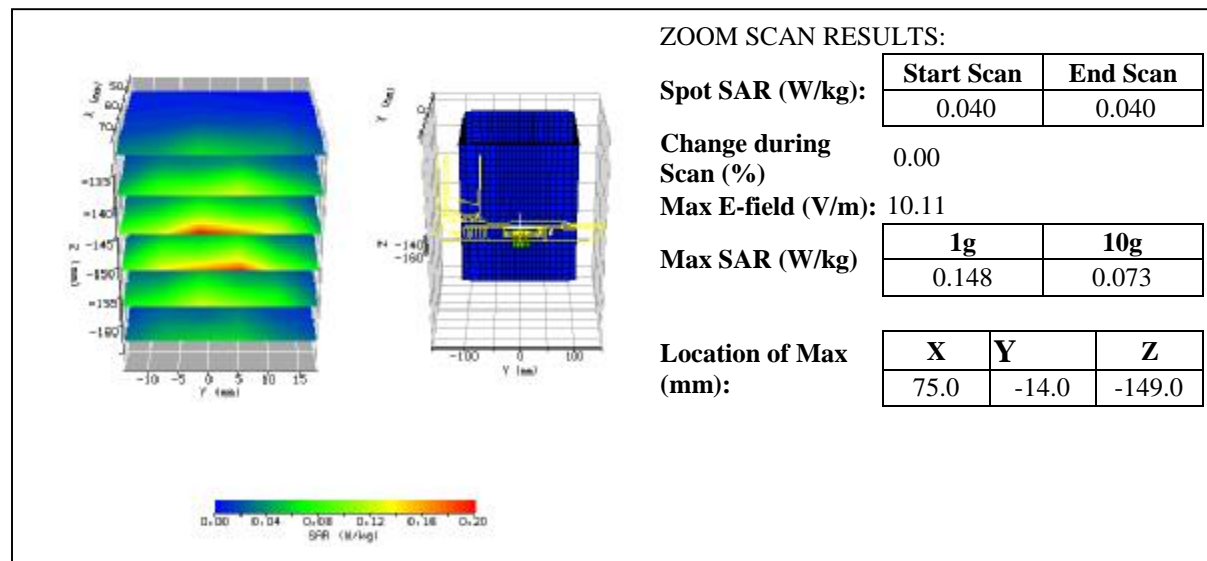


Plot #9 (2/2)

| | | | |
|-----------------------|--------------------|------------------------|-------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 0mm |
| Filename: | b-122-2437per0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2437MHz |
| Shape File: | 122left.csv | Power Level: | 15.13dBm |

AREA SCAN:

Scan Extent:


| | Min | Max | Steps |
|----------|--------|--------|-------|
| Y | -30.0 | 30.0 | 6.0 |
| Z | -170.0 | -130.0 | 4.0 |

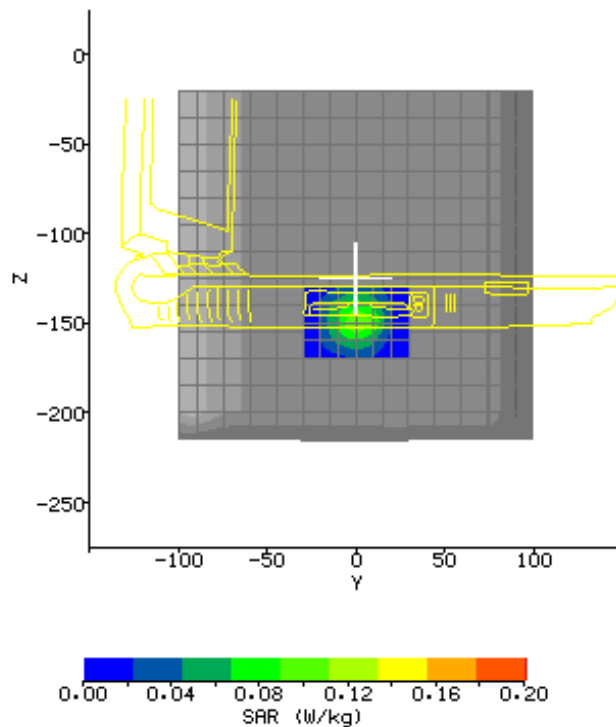

Plot #10 (1/2)

| | | | |
|-----------------------|--------------------|------------------------|-------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 0mm |
| Filename: | b-122-2412per0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2412MHz |
| Shape File: | 122left.csv | Power Level: | 14.93dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_BODY | Type: | 2450MHz Body |
| Cal Factors: | | Conductivity: | 1.95229 |
| | | Relative Permittivity: | 51.1547 |
| | | Liquid Temp (deg C): | 22.8 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | 1 | Software Version: | 0.421N |
| | | Crest Factor= | 1 |

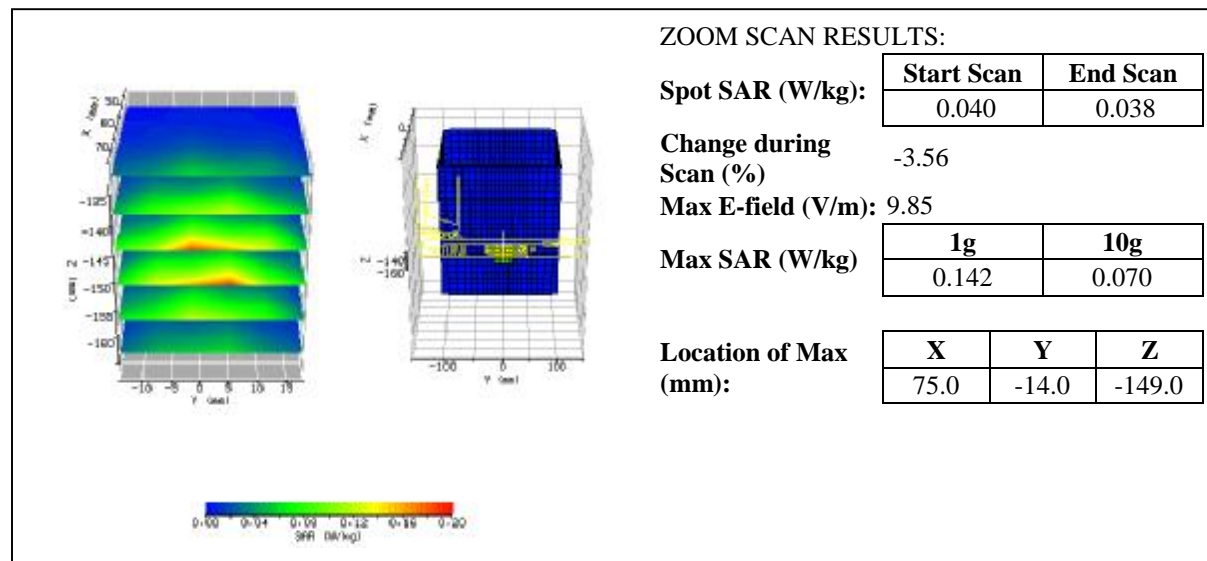


Plot #10 (2/2)

| | | | |
|-----------------------|--------------------|------------------------|-------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 0mm |
| Filename: | b-122-2412per0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2412MHz |
| Shape File: | 122left.csv | Power Level: | 14.93dBm |

AREA SCAN:

Scan Extent:


| | Min | Max | Steps |
|----------|--------|--------|-------|
| Y | -30.0 | 30.0 | 6.0 |
| Z | -170.0 | -130.0 | 4.0 |

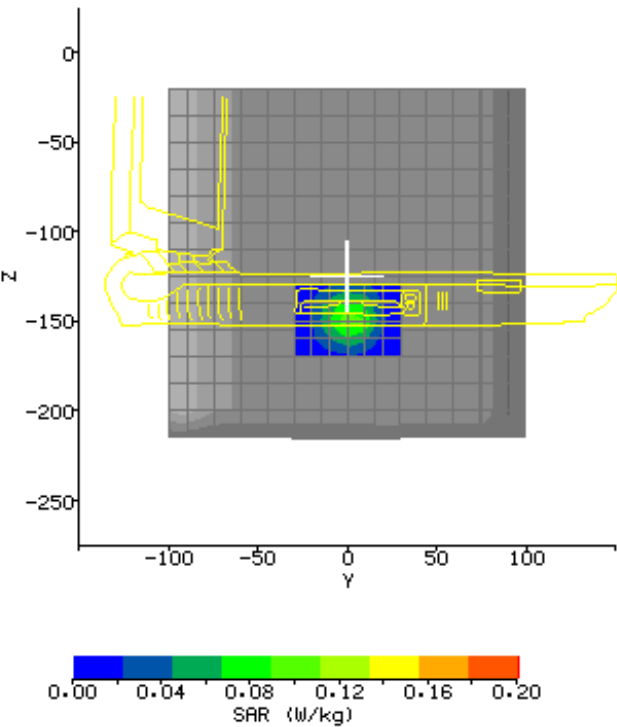

Plot #11 (1/2)

| | | | |
|-----------------------|--------------------|------------------------|-------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 0mm |
| Filename: | b-122-2462per0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2462MHz |
| Shape File: | 122left.csv | Power Level: | 15.33dBm |

| | | | |
|----------------------------|---------------------|-------------------------------|--------------|
| Probe: | 0136 | Liquid: | 15.5cm |
| Cal File: | SN0136_2450_CW_BODY | Type: | 2450MHz Body |
| Cal Factors: | | Conductivity: | 1.95229 |
| | | Relative Permittivity: | 51.1547 |
| | | Liquid Temp (deg C): | 22.8 |
| | | Ambient Temp (deg C): | 23 |
| Amp Gain: | 2 | Ambient RH (%): | 50 |
| Averaging: | 1 | Density (kg/m3): | 1000 |
| Batteries Replaced: | 1 | Software Version: | 0.421N |

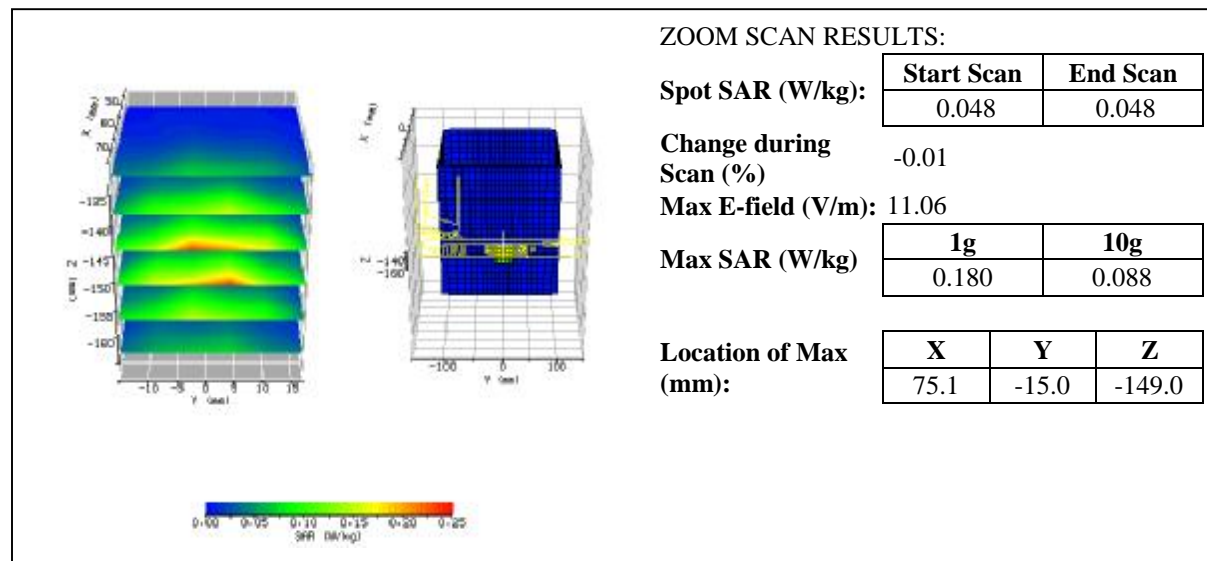


Plot #11 (2/2)

| | | | |
|-----------------------|--------------------|------------------------|-------------------|
| Date / Time: | 2003/9/23 | Position: | perpendicular 0mm |
| Filename: | b-122-2462per0.txt | Phantom: | HeadBox1.csv |
| Device Tested: | ZyAIR B-122 | Head Rotation: | 0 |
| Antenna: | Ceramic | Test Frequency: | 2462MHz |
| Shape File: | 122left.csv | Power Level: | 15.33dBm |

AREA SCAN:


Scan Extent:

| | Min | Max | Steps |
|----------|--------|--------|-------|
| Y | -30.0 | 30.0 | 6.0 |
| Z | -170.0 | -130.0 | 4.0 |

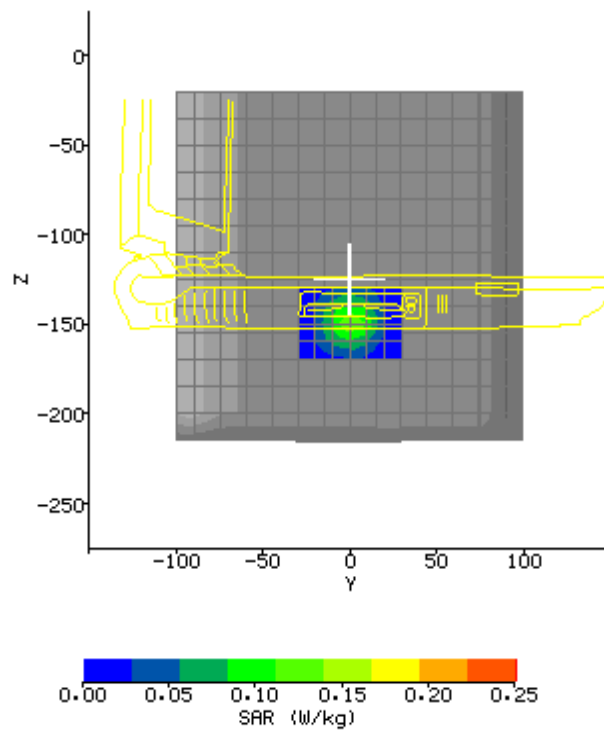


APPENDIX B – 2450MHz body liquid Calibration Data

| Date: 23 Sep. 2003 | Temperature:22.5°C | Type:2450MHz/body (FCC) | Tested by: Kevin |
|------------------------------------|--------------------|---|------------------|
| 2410, 50.5461637144, -2.0154744203 | | 2450, 51.1546861107, -1.9522934902 | |
| 2411, 50.5182646199, -2.0177380403 | | 2451, 51.1603419606, -1.9540475153 | |
| 2412, 50.455642907, -2.0130190975 | | 2452, 51.1986427605, -1.9614249412 | |
| 2413, 50.523758025, -2.0080668361 | | 2453, 51.2256013652, -1.9595758662 | |
| 2414, 50.5009028244, -2.0111139484 | | 2454, 51.2563104777, -1.9608064518 | |
| 2415, 50.5016207218, -1.9983672986 | | 2455, 51.3047196667, -1.9624285369 | |
| 2416, 50.4707402331, -1.9971879665 | | 2456, 51.2877418897, -1.9696394201 | |
| 2417, 50.5030911885, -1.9971326231 | | 2457, 51.3455995022, -1.970326476 | |
| 2418, 50.5296835511, -1.9993513784 | | 2458, 51.3198779435, -1.9702798189 | |
| 2419, 50.5082616489, -1.9881839715 | | 2459, 51.358923221, -1.9725006217 | |
| 2420, 50.5110599479, -1.9906577426 | | 2460, 51.3840932028, -1.9702317657 | |
| 2421, 50.5259298428, -1.9838111234 | | 2461, 51.4135855942, -1.9780302297 | |
| 2422, 50.5253773418, -1.9864108025 | | 2462, 51.4572035483, -1.9841790126 | |
| 2423, 50.5514286533, -1.9806004513 | | 2463, 51.4736652802, -1.986668944 | |
| 2424, 50.5620087971, -1.9774308466 | | 2464, 51.4603829208, -1.9924019822 | |
| 2425, 50.5567500421, -1.9725405196 | | 2465, 51.5051669823, -1.992990205 | |
| 2426, 50.5511601679, -1.9717491366 | | 2466, 51.4852268866, -1.9862598974 | |
| 2427, 50.5636458222, -1.9654683305 | | 2467, 51.5699090833, -2.001261124 | |
| 2428, 50.6203544608, -1.964925314 | | 2468, 51.572352744, -2.0085375044 | |
| 2429, 50.621646019, -1.9639689564 | | 2469, 51.565522828, -2.0073562786 | |
| 2430, 50.6774592621, -1.9586479117 | | 2470, 51.5514651739, -2.008567638 | |
| 2431, 50.6890338061, -1.9581888833 | | 2471, 51.6109612245, -2.0163871076 | |
| 2432, 50.6877404552, -1.9581082096 | | 2472, 51.5805941624, -2.0220455621 | |
| 2433, 50.7039560273, -1.9511250653 | | 2473, 51.6317560976, -2.0256682404 | |
| 2434, 50.7009804402, -1.9543809047 | | 2474, 51.6026935319, -2.0219768126 | |
| 2435, 50.7583242302, -1.9525657078 | | 2475, 51.6693812404, -2.0358685895 | |
| 2436, 50.7774191322, -1.9550525613 | | 2476, 51.715334044, -2.035333953 | |
| 2437, 50.7931079647, -1.9546745227 | | 2477, 51.7177845957, -2.0378834 | |
| 2438, 50.844106081, -1.949233922 | | 2478, 51.708654741, -2.0457699168 | |
| 2439, 50.8652541494, -1.9514933214 | | 2479, 51.6978230532, -2.0515309153 | |
| 2440, 50.8925937131, -1.9498449766 | | 2480, 51.7212113857, -2.0533418455 | |
| 2441, 50.9106256988, -1.9493719349 | | 2481, 51.7305123016, -2.0681996158 | |
| 2442, 50.9124813911, -1.9558182996 | | 2482, 51.6848010929, -2.0602313134 | |
| 2443, 50.957178675, -1.9518552696 | | 2483, 51.7564620287, -2.068629867 | |
| 2444, 50.9789312172, -1.9478314726 | | 2484, 51.8003708703, -2.0771380294 | |
| 2445, 51.008191062, -1.9500872835 | | 2485, 51.7799579277, -2.0786870005 | |
| 2446, 51.0188668037, -1.9495628072 | | 2486, 51.7749876473, -2.083657993 | |
| 2447, 51.077040652, -1.9512422002 | | 2487, 51.7738553283, -2.0910191602 | |
| 2448, 51.0826879171, -1.9486645579 | | 2488, 51.7858878174, -2.0872875866 | |
| 2449, 51.1352815872, -1.9536023362 | | 2489, 51.778274655, -2.1033458369 | |
| | | 2490, 51.7973567737, -2.1002439783 | |


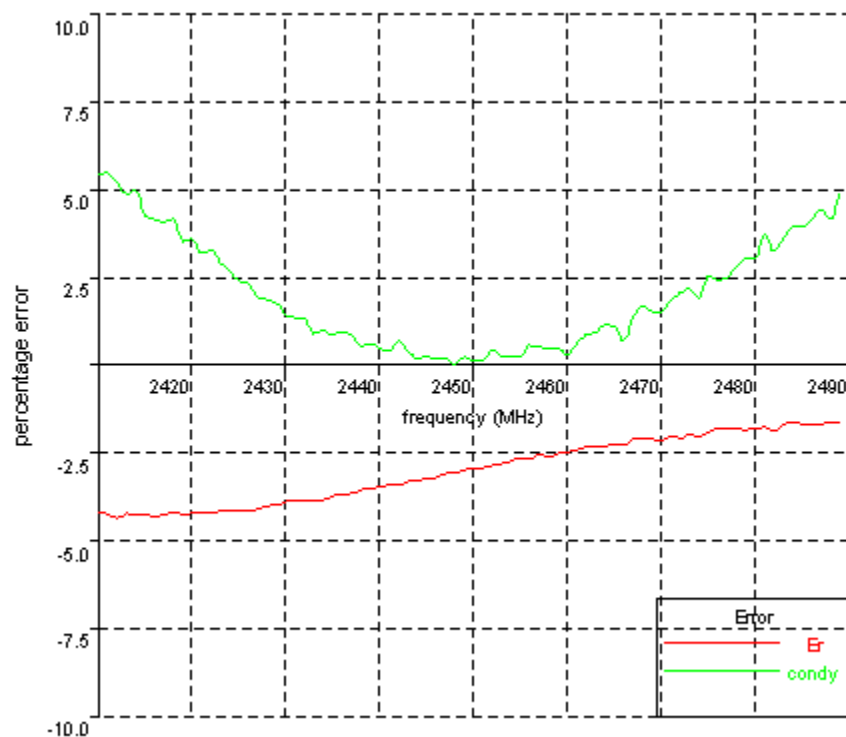




Photographs

External photo

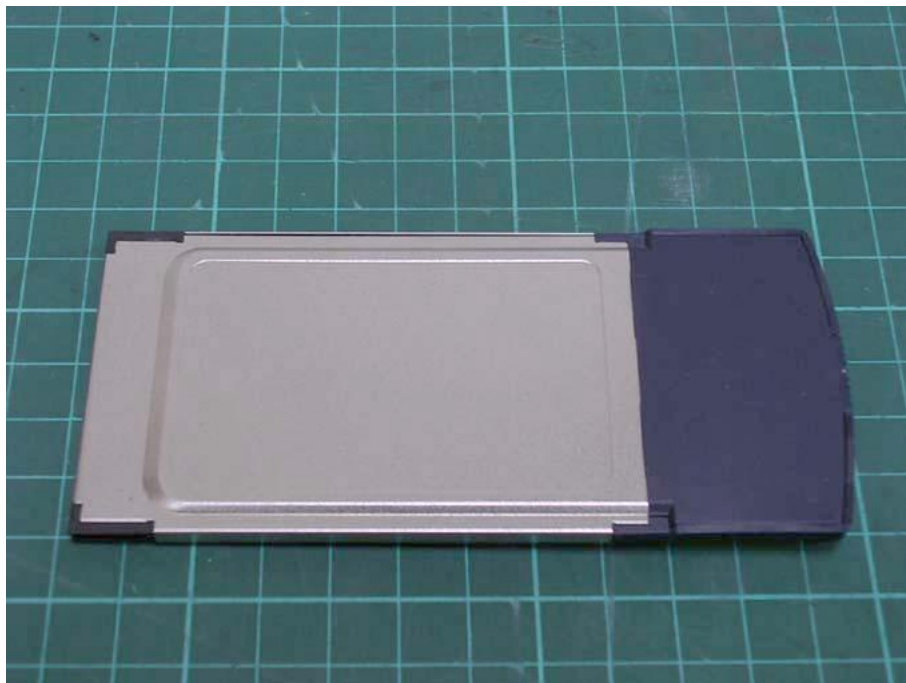

Internal photo

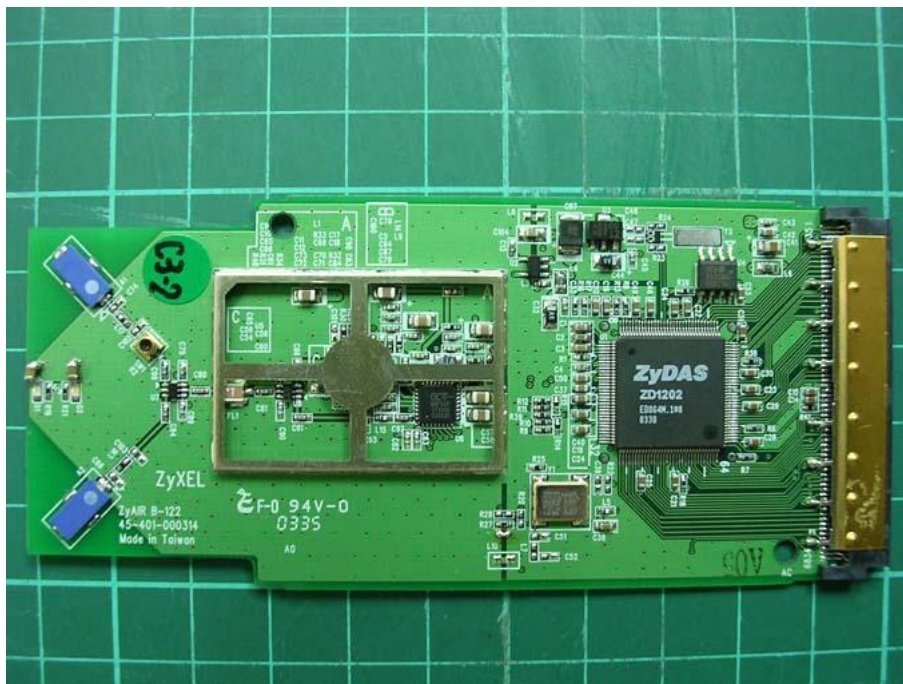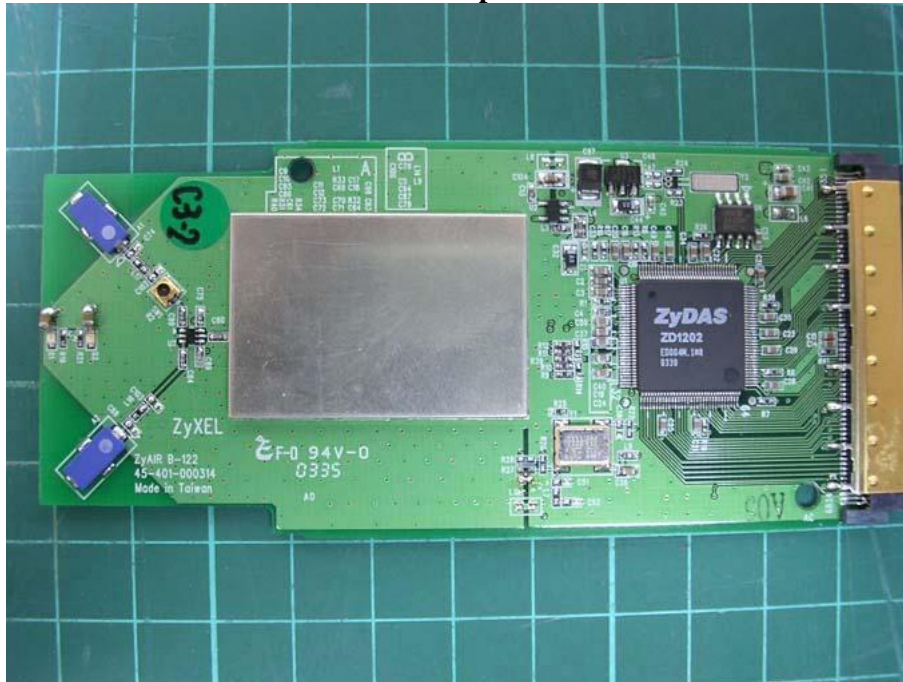

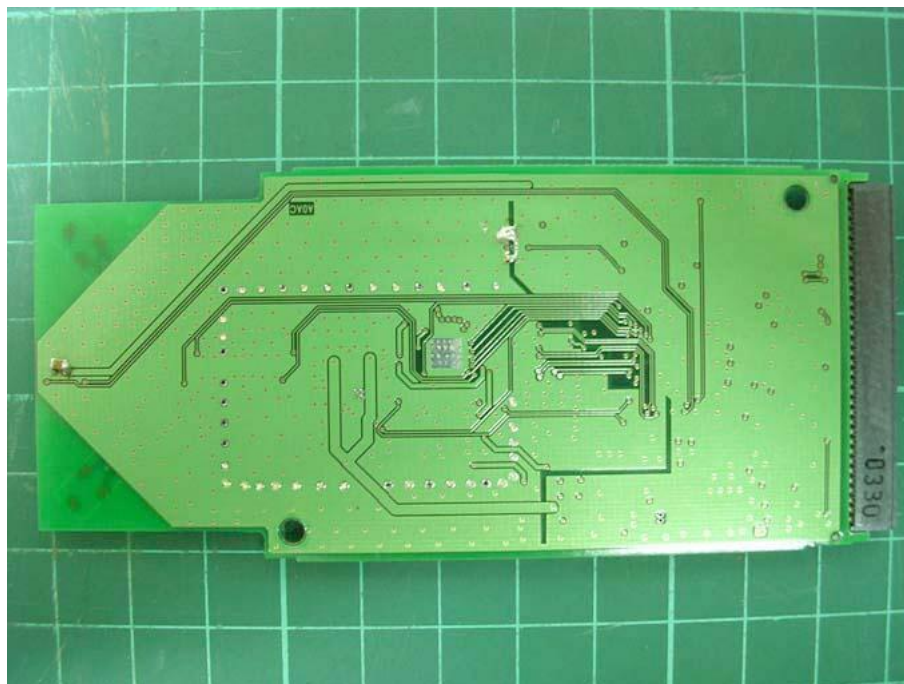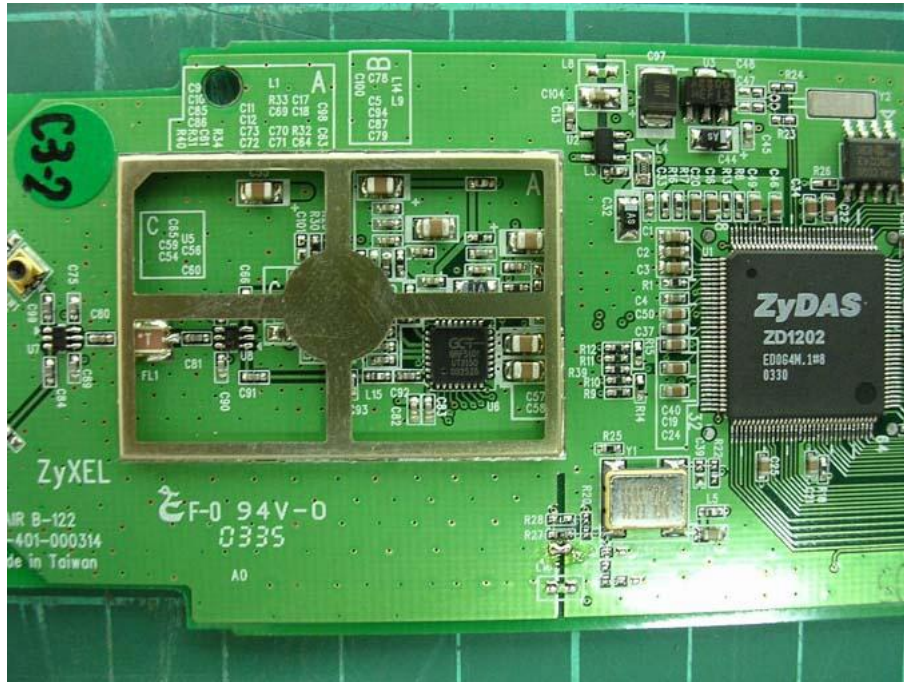



FCC ID. : I88B122

Report No.: EME-031071

Page 50 of 70

APPENDIX C - E-Field Probe Certificate and Calibration Data
Validation dipole certificate and performance measurements



Type: **IXP-050**

Manufacturer: **IndexSAR, UK**

Serial Number: **0136**

Place of Calibration: **IndexSAR, UK**

IndexSAR Limited hereby declares that the IXP-050 Probe named above has been calibrated for conformity to the IEEE 1528 and CENELEC En 50361 standards on the date shown below.

Date of Initial Calibration: **10th September 2003**

The probe named above will require a calibration check on the date shown below.

Next Calibration Date: **September 2004**

The calibration was carried out using the methods described in the calibration document.
Where applicable, the standards used in the calibration process are traceable to the UK's National Physical Laboratory.

Calibrated By:

A handwritten signature in blue ink, appearing to read "K. M. Ladbey".

Approved By:

A handwritten signature in black ink, appearing to read "M. J. Mann".

Please keep this certificate with the calibration document. When the probe is sent for a calibration check, please include the calibration document.



IMMERSIBLE SAR PROBE

CALIBRATION REPORT

Part Number: IXP – 050

S/N 0136

10th September 2003



Indexsar Limited
Oakfield House
Cudworth Lane
Newdigate
Surrey RH5 5DR
Tel: +44 (0) 1306 631 233
Fax: +44 (0) 1306 631 834
e-mail: enquiries@indexsar.com

INTRODUCTION

This Report presents measured calibration data for a particular Indexsar SAR probe (S/N 0136) and describes the procedures used for characterisation and calibration.

Indexsar probes are characterised using procedures that, where applicable, follow the recommendations of CENELEC [1] and IEEE [2] standards. The procedures incorporate techniques for probe linearisation, isotropy assessment and determination of liquid factors (conversion factors). Calibrations are determined by comparing probe readings with analytical computations in canonical test geometries (waveguides) using normalised power inputs.

Each step of the calibration procedure and the equipment used is described in the sections below.

CALIBRATION PROCEDURE

1. Equipment Used

For the first part of the characterisation procedure, the probe is placed in an isotropy measurement jig as pictured in Figure 1. In this position the probe can be rotated about its axis by a non-metallic belt driven by a stepper motor.

The probe is attached via its amplifier and an optical cable to a PC. A schematic representation of the test geometry is illustrated in Figure 2.

A balanced dipole (900 MHz) is inserted horizontally into the bracket attached to a second belt (Figure 1). The dipole can also be rotated about its axis. A cable connects the dipole to a signal generator, via a directional coupler and power meter. The signal generator feeds an RF amplifier at constant power, the output of which is monitored using the power meter. The probe is positioned so that its sensors line up with the rotation center of the source dipole. By recording output voltage measurements of each channel as both the probe and the dipole are rotated, data are obtained from which the spherical isotropy of the probe can be optimised and its magnitude determined.

The calibration process requires E-field measurements to be taken in air, in 900 MHz simulated brain liquid and at other frequencies/liquids as appropriate.

2. Linearising probe output

The probe channel output signals are linearised in the manner set out in Refs [1] and [2]. The following equation is utilized for each channel:

$$U_{lin} = U_{o/p} + U_{o/p}^2 / DCP \quad (1)$$

where U_{lin} is the linearised signal, $U_{o/p}$ is the raw output signal in voltage units and DCP is the diode compression potential in similar voltage units.

DCP is determined from fitting equation (1) to measurements of U_{lin} versus source feed power over the full dynamic range of the probe. The DCP is a characteristic of the schottky diodes used as the sensors. For the IXP-050 probes with CW signals the DCP values are typically 0.10V (or 20 in the voltage units used by Indexsar software, which are V*200).

3. Selecting channel sensitivity factors to optimise isotropic response

The basic measurements obtained using the calibration jig (Fig 1) represent the output from each diode sensor as a function of the presentation angle of the source (probe and dipole rotation angles). The directionality of the orthogonally-arranged sensors can be checked by analysing the data using dedicated Indexsar software, which displays the data in 3D format as in Figure 3. The left-hand side of this diagram shows the individual channel outputs after linearisation (see above). The program uses these data to balance the channel outputs and then applies an optimisation process, which makes fine adjustments to the channel factors for optimum isotropic response.

The next stage of the process is to calibrate the Indexsar probe to a W&G EMR300 E-field meter in air. The principal reasons for this are to obtain conversion factors applicable should the probe be used in air and to provide an overall measure of the probe sensitivity.

A multiplier is applied to factors to bring the magnitudes of the average E-field measurements as close as possible to those of the W&G probe.

The following equation is used (where linearised output voltages are in units of V*200):

$$E_{air}^2 \text{ (V/m)} = U_{linx} * \text{Air Factor}_x + U_{liny} * \text{Air Factor}_y + U_{linz} * \text{Air Factor}_z \quad (2)$$

It should be noted that the air factors are not separately used for normal SAR testing. The IXP-050 probes are optimised for use in tissue-simulating liquids and do not behave isotropically in air.

4. 900 MHz Liquid Calibration

Conversion factors for use when the probes are immersed in tissue-simulant liquids at 900 MHz are determined either using a waveguide or by comparison to a reference probe that has been calibrated by NPL. Waveguide procedures are described later. The summary sheet indicates the method used for the probe S/N 0136.

The conversion factor, referred to as the 'liquid factor' is also applied to the measurements of each channel. The following equation is used (where output voltages are in units of V*200):

$$E_{liq}^2 \text{ (V/m)} = U_{linx} * \text{Air Factor}_x * \text{Liq Factor}_x + U_{liny} * \text{Air Factor}_y * \text{Liq Factor}_y + U_{linz} * \text{Air Factor}_z * \text{Liq Factor}_z \quad (3)$$

A 3D representation of the spherical isotropy for probe S/N 0136 using these factors is shown in Figure 3.

The rotational isotropy can also be determined from the calibration jig measurements and is reported as the 900MHz isotropy in the summary table. Note that waveguide measurements can also be used to determine rotational isotropy (Fig. 5).

The design of the cells used for determining probe conversion factors are waveguide cells is shown in Figure 4. The cells consist of a coax to waveguide transition and an open-ended section of waveguide containing a dielectric separator. Each waveguide cell stands in the upright position and is filled with liquid within 10 mm of the open end. The separator provides a liquid seal and is designed for a good

electrical transition from air filled guide to liquid filled guide. The choice of cell depends on the portion of the frequency band to be examined and the choice of liquid used. The depth of liquid ensures there is negligible radiation from the waveguide open top and that the probe calibration is not influenced by reflections from nearby objects. The return loss at the coaxial connector of the filled waveguide cell is measured initially using a network analyser and this information is used subsequently in the calibration procedure. The probe is positioned in the centre of the waveguide and is adjusted vertically or rotated using stepper motor arrangements. The signal generator is connected to the waveguide cell and the power is monitored with a coupler and a power meter. A fuller description of the waveguide method is given below.

The liquid dielectric parameters used for the probe calibrations are listed in the Tables below. The final calibration factors for the probe are listed in the summary chart.

WAVEGUIDE MEASUREMENT PROCEDURE

The calibration method is based on setting up a calculable specific absorption rate (SAR) in a vertically-mounted WG8 (R22) waveguide section [1]. The waveguide has an air-filled, launcher section and a liquid-filled section separated by a matching window that is designed to minimise reflections at the liquid interface. A TE_{01} mode is launched into the waveguide by means of a N-type-to-waveguide adapter. The power delivered to the liquid section is calculated from the forward power and reflection coefficient measured at the input to the waveguide. At the centre of the cross-section of the waveguide, the local spot SAR in the liquid as a function of distance from the window is given by functions set out in IEEE1528 as below:

Because of the low cutoff frequency, the field inside the liquid nearly propagates as a TEM wave. The depth of the medium (greater than three penetration depths) ensures that reflections at the upper surface of the liquid are negligible. The power absorbed in the liquid is determined by measuring the waveguide forward and reflected power. Equation (4) shows the relationship between the SAR at the cross-sectional center of the lossy waveguide and the longitudinal distance (z) from the dielectric separator

$$SAR(z) = \frac{4(P_f - P_b)}{rabd} e^{-2z/d} \quad (4)$$

where the density r is conventionally assumed to be 1000 kg/m^3 , ab is the cross-sectional area of the waveguide, P_f and P_b are the forward and reflected power inside the lossless section of the waveguide, respectively. The penetration depth d , which is the reciprocal of the waveguide-mode attenuation coefficient, is determined from a scan along the z -axis and compared with the theoretical value determined from Equation (5) using the measured dielectric properties of the lossy liquid.

$$d = \left[\text{Re} \left\{ \sqrt{(p/a)^2 + jwm_o(s + jwe_o e_r)} \right\} \right]^{-1} \quad (5)$$

Table A.1 of [1] can be used for designing calibration waveguides with a return loss greater than 30 dB at the most important frequencies used for personal wireless communications. Values for the penetration depth for these specific fixtures and tissue-simulating mixtures are also listed in Table A.1.

According to [1], this calibration technique provides excellent accuracy, with standard uncertainty of less than 3.6% depending on the frequency and medium. The calibration itself is reduced to power measurements traceable to a standard calibration procedure. The practical limitation to the frequency

band of 800 to 2500 MHz because of the waveguide size is not severe in the context of compliance testing.

CALIBRATION FACTORS MEASURED FOR PROBE S/N 0136

The probe was calibrated at 900, 1800, 1900 and 2450MHz MHz in liquid samples representing both brain liquid and body fluid at these frequencies. The calibration was for CW signals only, and the axis of the probe was parallel to the direction of propagation of the incident field i.e. end-on to the incident radiation. The axial isotropy of the probe was measured by rotating the probe about its axis in 10 degree steps through 360 degrees in this orientation.

The reference point for the calibration is in the centre of the probe's cross-section at a distance of 2.7 m from the probe tip in the direction of the probe amplifier. A value of 2.7 mm should be used for the tip to sensor offset distance in the software.

It is important that the diode compression point and air factors used in the software are the same as those quoted in the results tables, as these are used to convert the diode output voltages to a SAR value.

DIELECTRIC PROPERTIES OF LIQUIDS

The dielectric properties of the brain and body tissue-simulant liquids employed for calibration are listed in the tables below. The measurements were performed prior to each waveguide test using an Indexsar DiLine measurement kit, which uses the TEM method as recommended in [2].

AMBIENT CONDITIONS

Measurements were made in the open laboratory at $22 \pm 2.0^{\circ}\text{C}$. The temperature of the liquids in the waveguide used was measured using a mercury thermometer.

RESPONSE TO MODULATED SIGNALS

To measure the response of the probe and amplifier to modulated signals, the probe is held vertically in a liquid-filled waveguide.

An RF amplifier is allowed to warm up and stabilise before use. A spectrum analyser is used to demonstrate that the peak power of the RF amplifier for the CW signals and the pulsed signals are within 0.1dB of each other when the signal generator is switched from CW to modulated output. Subsequently, the power levels recorded are read from a power meter when a CW signal is being transmitted.

The test sequence involves manually stepping the power up in regular (e.g. 2 dB) steps from the lowest power that gives a measurable reading on the SAR probe up to the maximum that the amplifiers can deliver.

At each power level, the individual channel outputs from the SAR probe are recorded at CW and then recorded again with the modulation setting. The results are entered into a spreadsheet. Using the spreadsheets, the modulated power is calculated by applying a factor to the measured CW power (e.g. for GSM, this factor is 9.03dB). This process is repeated 3 times with the response maximised for each channel sensor in turn.

The probe channel output signals are linearised in the manner set out in Section 1 above using equation (1) with the DCPs determined from the linearisation procedure. Calibration factors for the probe are used to determine the E-field values corresponding to the probe readings using equation (3). SAR is determined from the equation

$$\text{SAR (W/kg)} = E_{\text{liq}}^2 \text{ (V/m)} * \sigma \text{ (S/m)} / 1000 \quad (6)$$


Where σ is the conductivity of the simulant liquid employed.

Using the spreadsheet data, the DCP value for linearising each of the individual channels (X, Y and Z) is assessed separately. The corresponding DCP values are listed in the summary page of the calibration factors for each probe.

Figure 7 shows the linearised probe response to GSM signals, Figure 8 the response to GPRS signals (GSM with 2 timeslots) and Figure 9 the response to CDMA IS-95A and W-CDMA signals.

Additional tests have shown that the modulation response is similar at 1800MHz and is not affected by the orientation between the source and the probe.

SUMMARY OF CALIBRATION FACTORS FOR PROBE IXP-050 S/N 0136

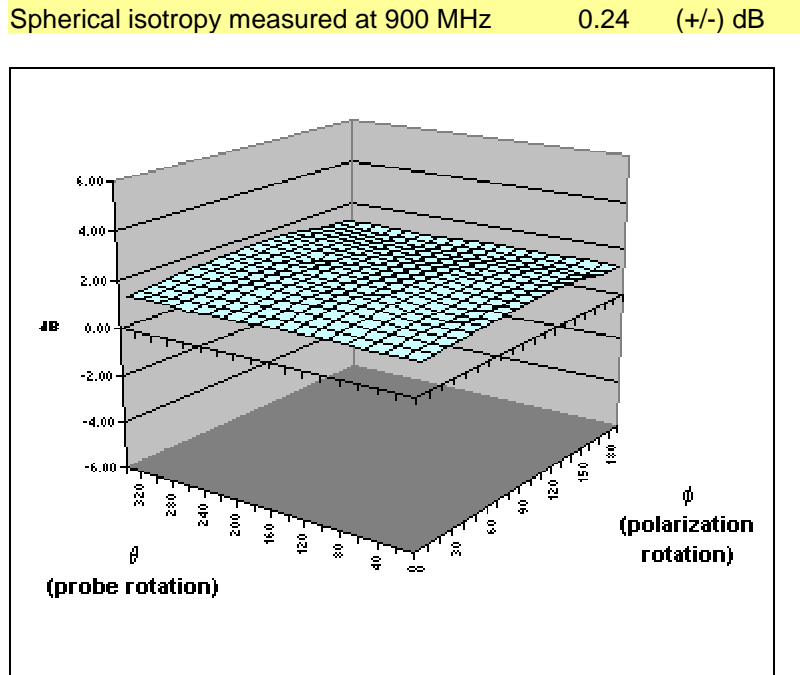

| | | | | |
|-------------|-----|-----|------|---------|
| | X | Y | Z | |
| Air factors | 490 | 405 | 405 | (V*200) |
| DCPs | 20 | 20 | 20 | (V*200) |
| DSSS | 20 | 20 | 20 | (V*200) |
| GSM | 8 | 9.5 | 11.2 | (V*200) |
| CDMA | 20 | 20 | 20 | (V*200) |

| f (MHz) | Axial isotropy (+/- dB) | | SAR conversion factors (liq/air) | | Notes |
|---------|----------------------------|------|-------------------------------------|-------|-------|
| | BRAIN | BODY | BRAIN | BODY | |
| 450 | | | | | |
| 835 | 0.05 | 0.04 | 0.257 | 0.272 | 1,2,3 |
| 900 | 0.05 | 0.04 | 0.261 | 0.282 | 1,2,3 |
| 1800 | 0.06 | 0.06 | 0.315 | 0.339 | 1,2,3 |
| 1900 | 0.06 | 0.06 | 0.327 | 0.351 | 1,2,3 |
| 2450 | 0.05 | 0.10 | 0.453 | 0.486 | 1,2,3 |

Notes

1) Calibrations done at 22C +/- 2C

2) Waveguide calibration

3) Checked using box-phantom validation test

(the graph shows a simple, spreadsheet representation of surface shown in 3D in Figure 3 below)

PROBE SPECIFICATIONS

Indexsar probe 0136, along with its calibration, is compared with CENELEC and IEEE standards recommendations (Refs [1] and [2]) in the Tables below. A listing of relevant specifications is contained in the tables below:

| Dimensions | S/N 0136 | CENELEC [1] | IEEE [2] |
|--|----------|-------------|----------|
| Overall length (mm) | 350 | | |
| Tip length (mm) | 10 | | |
| Body diameter (mm) | 12 | | |
| Tip diameter (mm) | 5.2 | 8 | 8 |
| Distance from probe tip to dipole centers (mm) | 2.7 | | |

| Dynamic range | S/N 0136 | CENELEC [1] | IEEE [2] |
|-------------------------------|----------|-------------|----------|
| Minimum (W/kg) | 0.01 | <0.02 | 0.01 |
| Maximum (W/kg) | >35 | >100 | 100 |
| N.B. only measured to 35 W/kg | | | |

| Linearity of response | S/N 0136 | CENELEC [1] | IEEE [2] |
|-------------------------------------|----------|-------------|----------|
| Over range 0.01 – 100 W/kg (+/- dB) | 0.125 | 0.50 | 0.25 |

| Isotropy (measured at 900MHz) | S/N 0136 | CENELEC [1] | IEEE [2] |
|--|-------------------------------|-------------|----------|
| Axial rotation with probe normal to source (+/- dB) at 835, 900, 1800, 1900 and 2450 MHz | Max. 0.10 (see summary table) | 0.5 | 0.25 |
| Spherical isotropy covering all orientations to source (+/- dB) | 0.24 | 1.0 | 0.50 |

| | |
|---------------------|--|
| Construction | Each probe contains three orthogonal dipole sensors arranged on a triangular prism core, protected against static charges by built-in shielding, and covered at the tip by PEEK cylindrical enclosure material. No adhesives are used in the immersed section. Outer case materials are PEEK and heat-shrink sleeving. |
| Chemical resistance | Tested to be resistant to glycol and alcohol containing simulant liquids but probes should be removed, cleaned and dried when not in use. |

REFERENCES

[1] CENELEC, EN 50361, July 2001. Basic Standard for the measurement of specific absorption rate related to human exposure to electromagnetic fields from mobile phones.

[2] IEEE 1528, Recommended practice for determining the spatial-peak specific absorption rate (SAR) in the human body due to wireless communications devices: Experimental techniques.

[3] Calibration report on SAR probe IXP-050 S/N 0071 from National Physical Laboratory. Test Report EF07/2002/03/IndexSAR. Dated 20 February 2002.

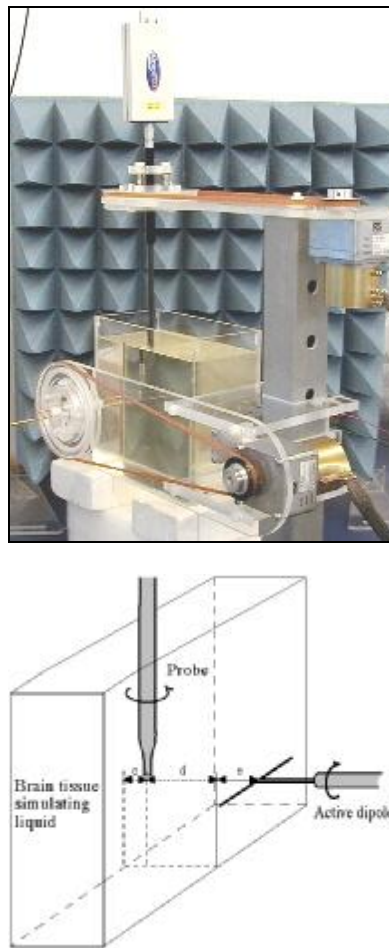


Figure 1. Spherical isotropy jig showing probe, dipole and box filled with simulated brain liquid (see Ref [2], Section A.5.2.1)

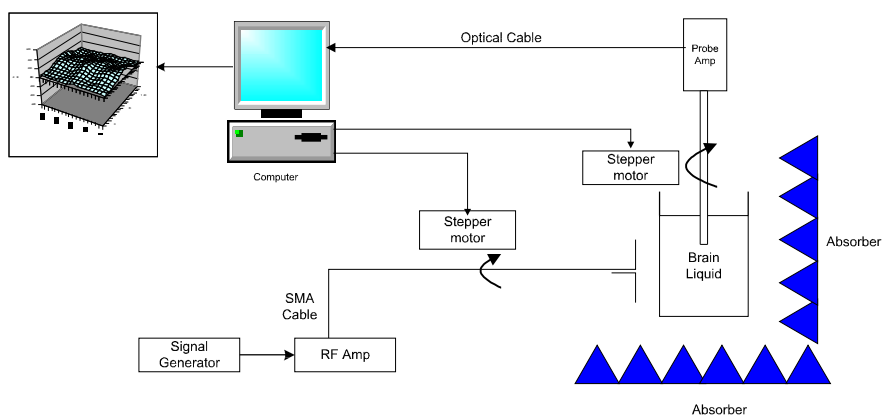


Figure 2. Schematic diagram of the test geometry used for isotropy determination

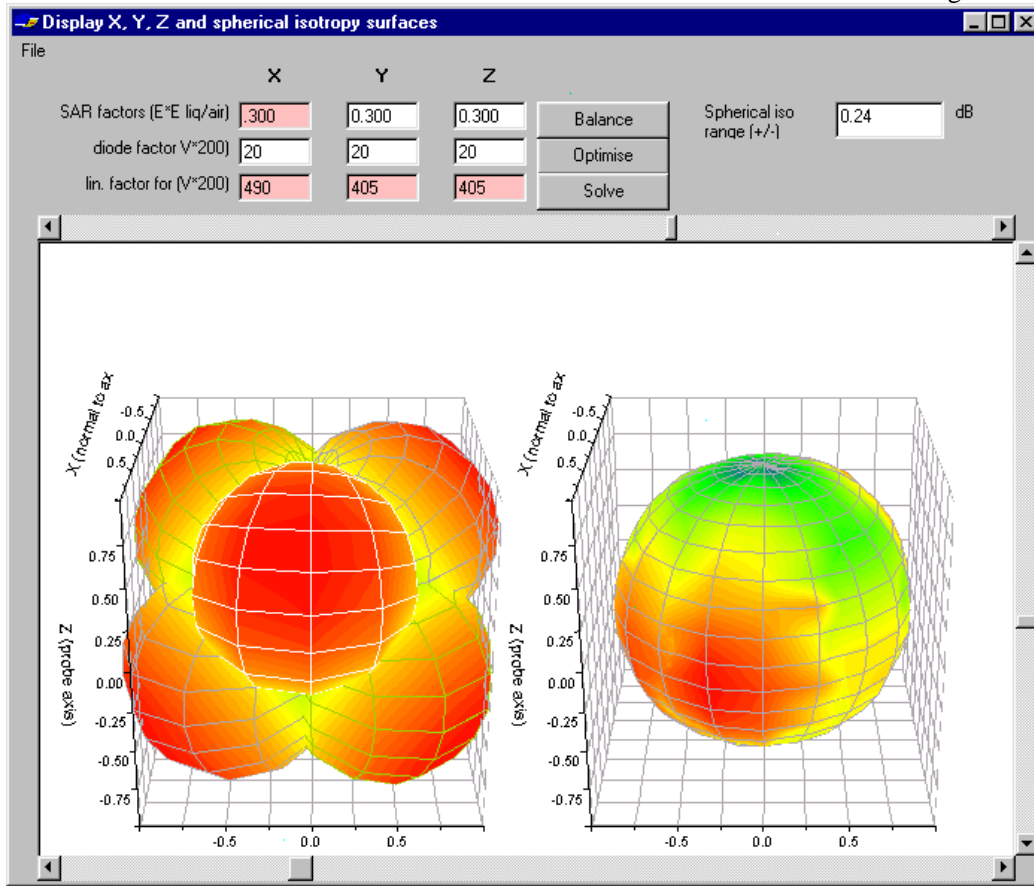


Figure 3. Graphical representation of the probe response to fields applied from each direction. The diagram on the left shows the individual response characteristics of each of the three channels and the diagram on the right shows the resulting probe sensitivity in each direction. The colour range in the figure images the lowest values as blue and the maximum values as red. For the probe S/N 0136, this range is (+/-) 0.24 dB. The probe is more sensitive to fields parallel to the axis and less sensitive to fields normal to the probe axis.

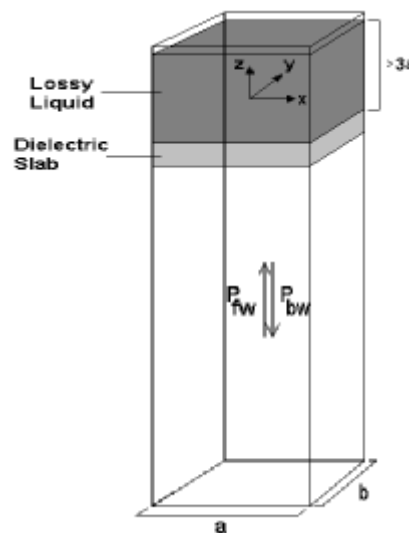


Figure 4. Geometry used for waveguide calibration (after Ref [2]. Section A.3.2.2)

IXP-050 S/N 0136

18-Aug-03

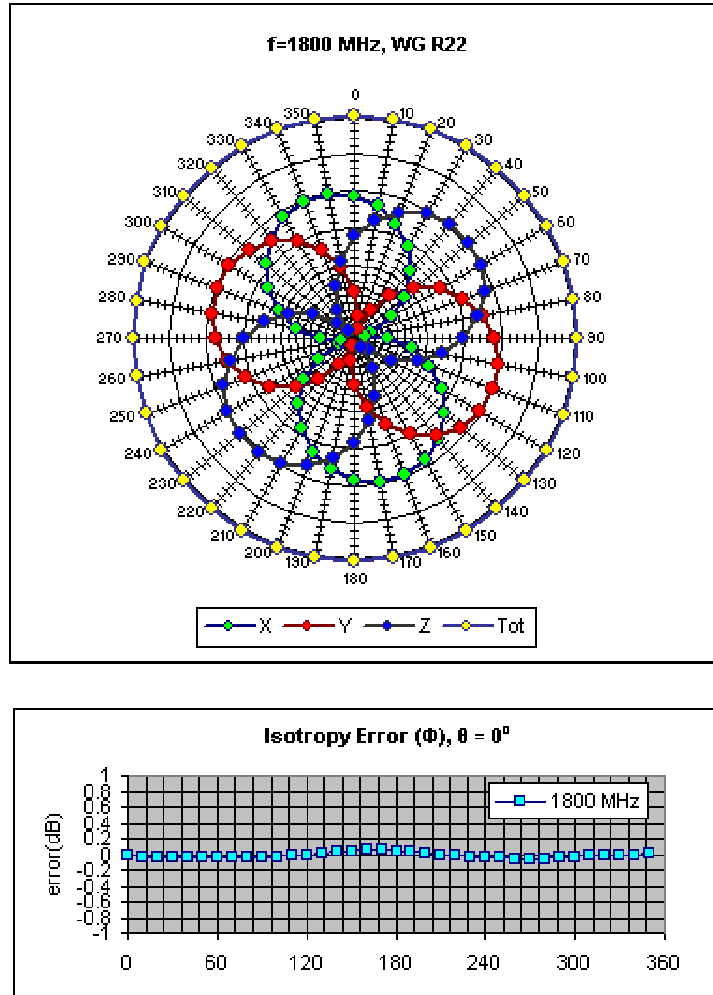


Figure 5. Example of the rotational isotropy of probe S/N 0136 obtained by rotating the probe in a liquid-filled waveguide at 2450 MHz. Similar distributions are obtained at the other test frequencies (1800 and 1900 MHz) both in brain liquids and body fluids (see summary table)

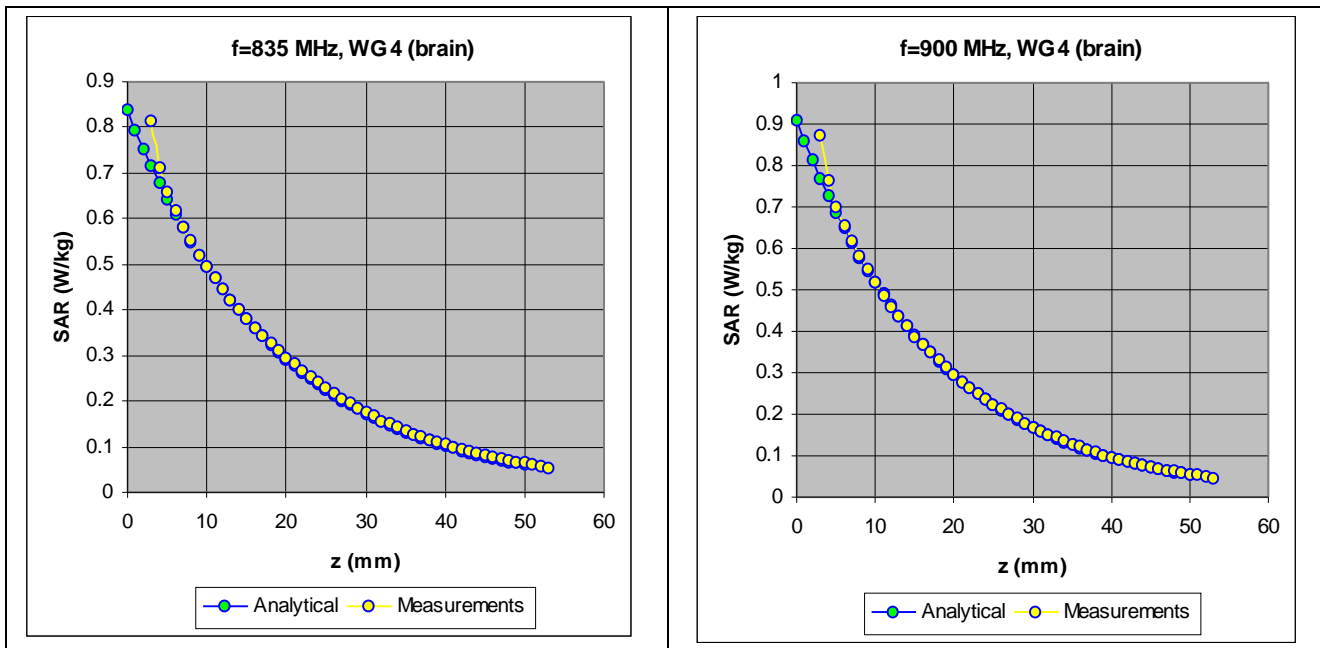


Figure 6. The measured SAR decay function along the centreline of the WG4 waveguide with conversion factors adjusted to fit to the theoretical function for the particular dimension, frequency, power and liquid properties employed.

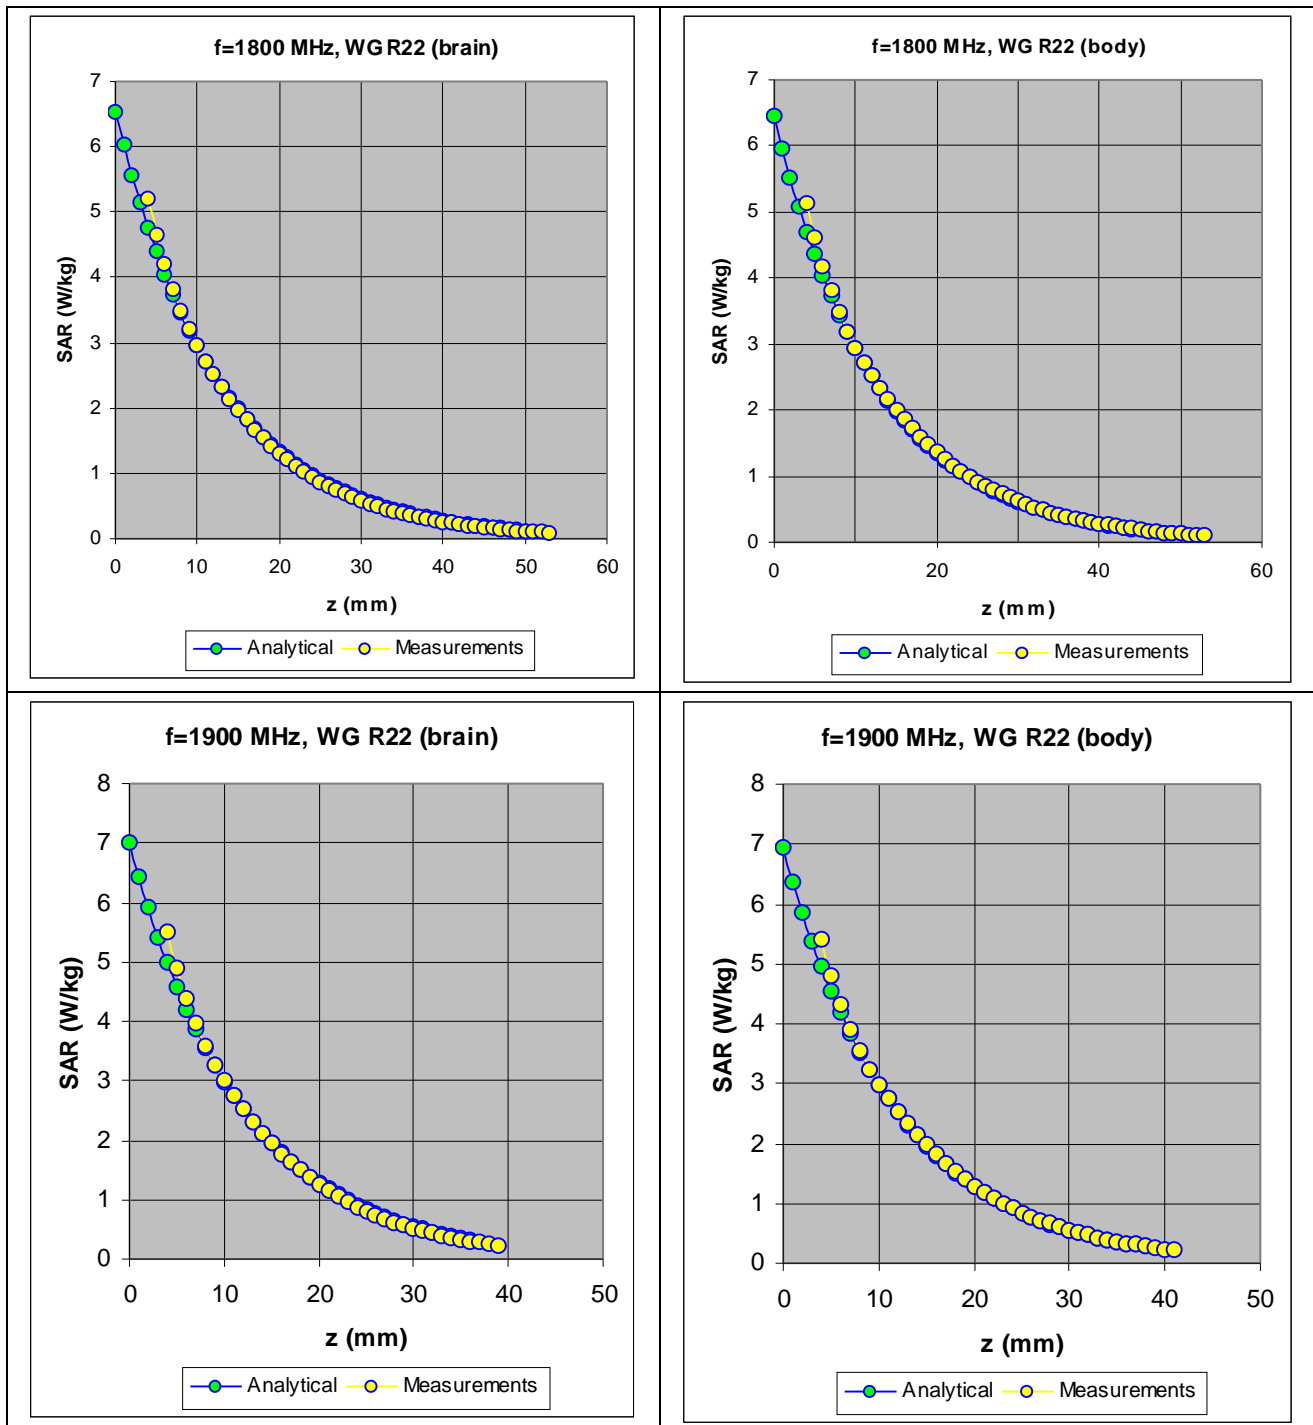


Figure 7. The measured SAR decay function along the centreline of the R22 waveguide with conversion factors adjusted to fit to the theoretical function for the particular dimension, frequency, power and liquid properties employed.

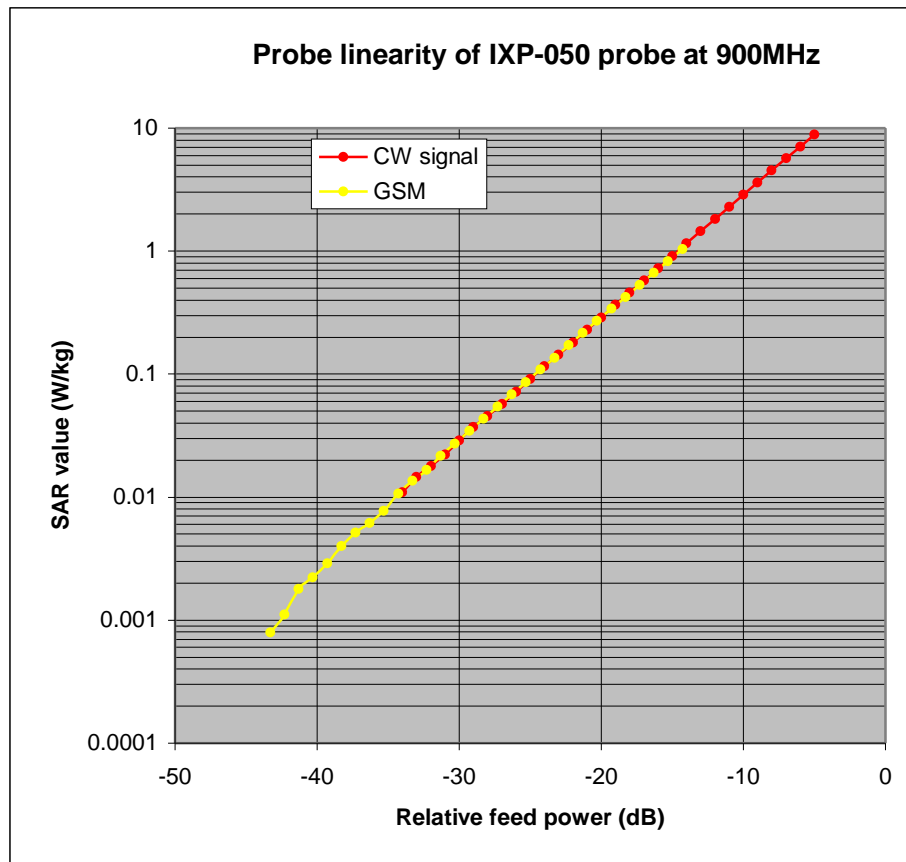


Figure 8. The GSM response of an IXP-050 probe at 900MHz.

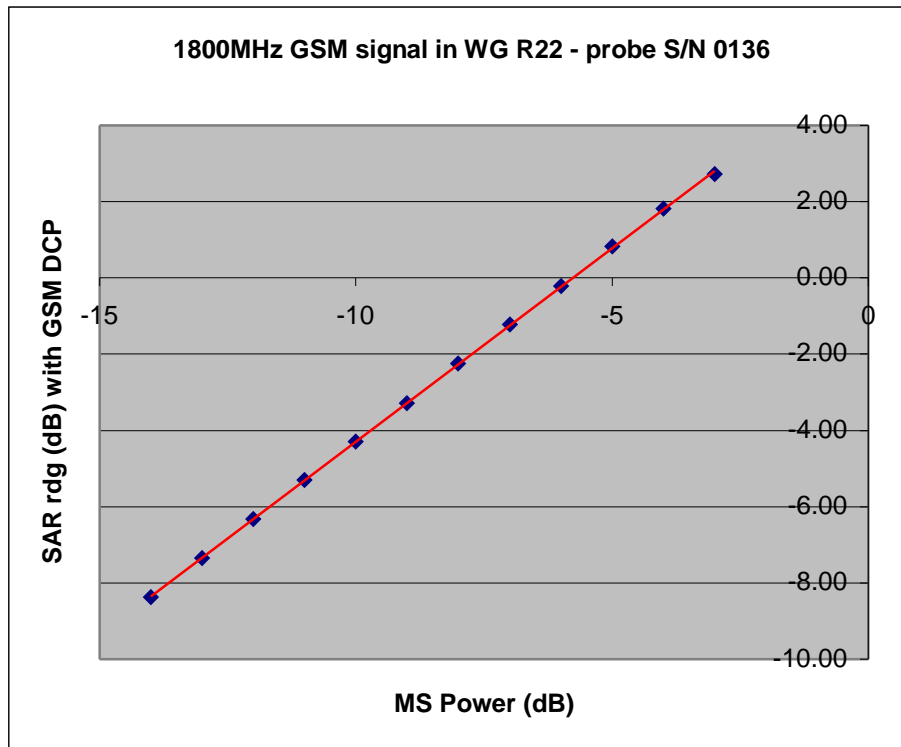


Figure 8a. The actual GSM response of IXP-050 probe S/N 0136 at 1800MHz

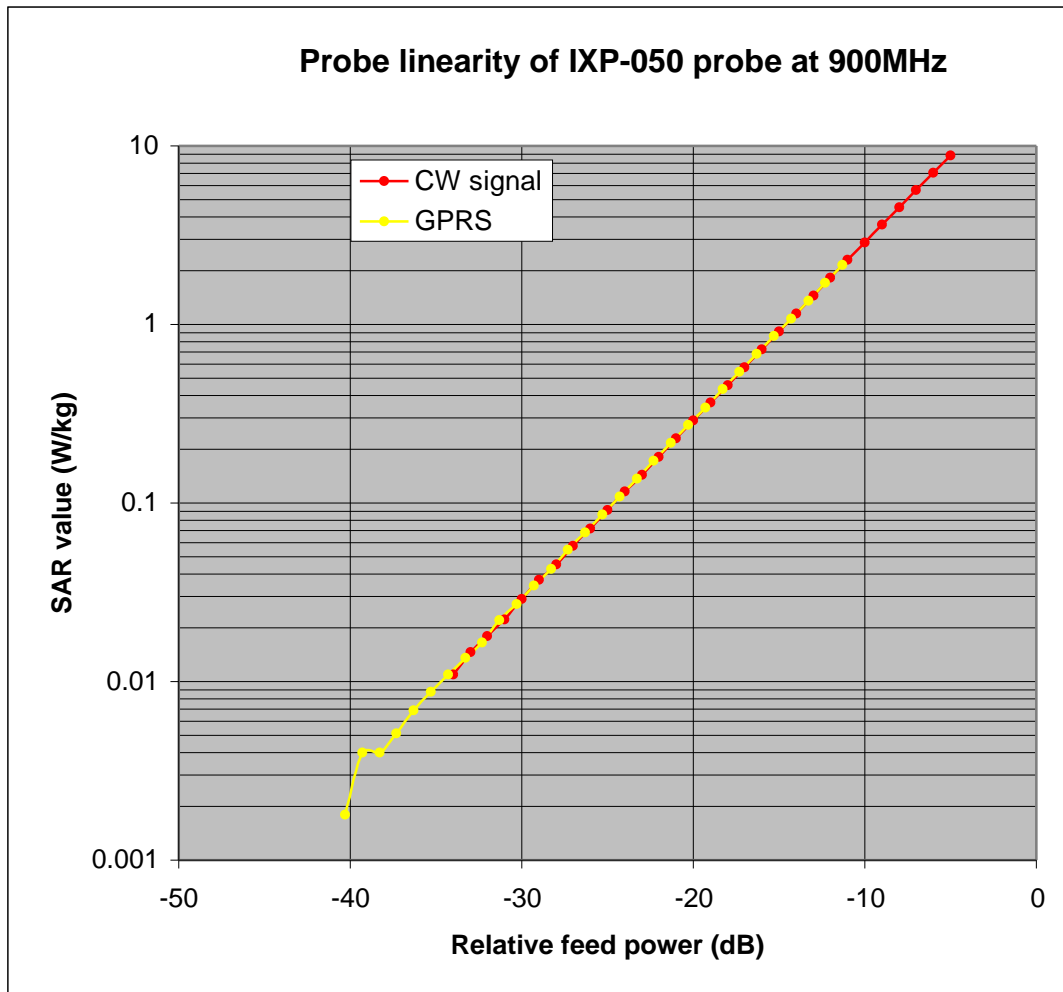
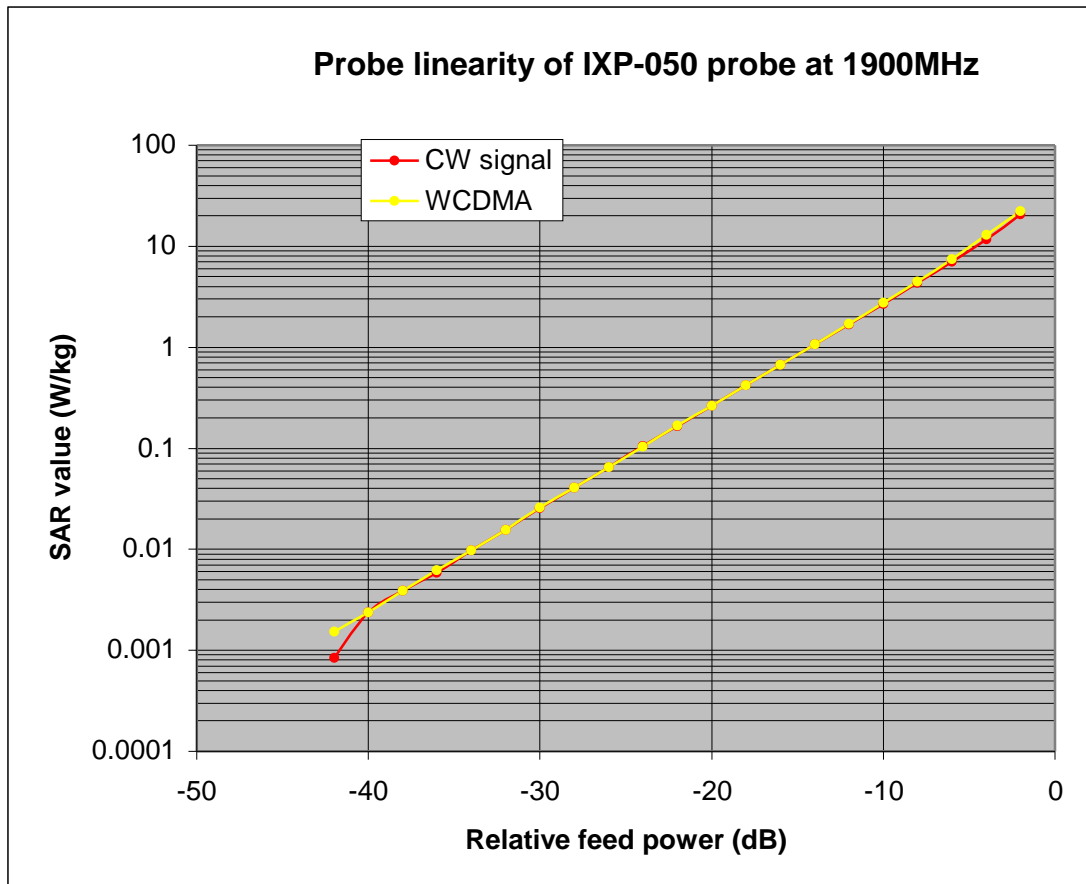


Figure 9. The GPRS response of an IXP-050 probe at 900MHz.



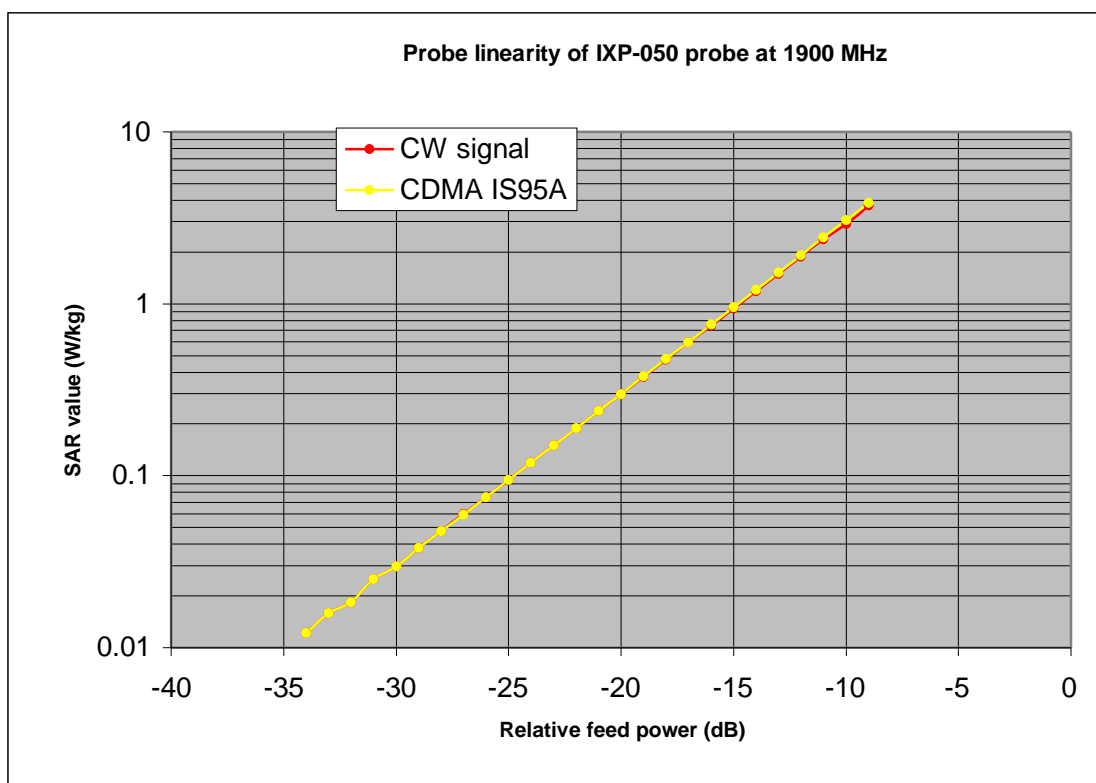


Figure 10. The CDMA response of an IXP-050 probe at 1900MHz.

Table indicating the dielectric parameters of the liquids used for calibrations at each frequency

| <i>Liquid used</i> | <i>Relative permittivity (measured)</i> | <i>Conductivity (S/m) (measured)</i> |
|---------------------------|--|---|
| 835 MHz BRAIN | 43.18 | 0.935 |
| 835 MHz BODY | 59.19 | 0.992 |
| 900 MHz BRAIN | 42.47 | 0.998 |
| 900 MHz BODY | 58.7 | 1.056 |
| 1800 MHz BRAIN | 38.72 | 1.34 |
| 1800 MHz BODY | 52.5 | 1.53 |
| 1900 MHz BRAIN | 38.31 | 1.43 |
| 1900 MHz BODY | 52.06 | 1.64 |
| 2450 MHz BRAIN | 38.9 | 1.87 |
| 2450 MHz BODY | 52.59 | 2.08 |