

System Check_Head_2000MHz

DUT: D2000V2 - SN1010

Communication System: CW; Frequency: 2000.000 MHz

Medium: HSL_2000_240325 Medium parameters used: $f = 2000.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 39.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.68, 7.84, 7.84); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 1.96 W/kg; SAR (10g) = 0.997 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.96 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 10.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.6 %

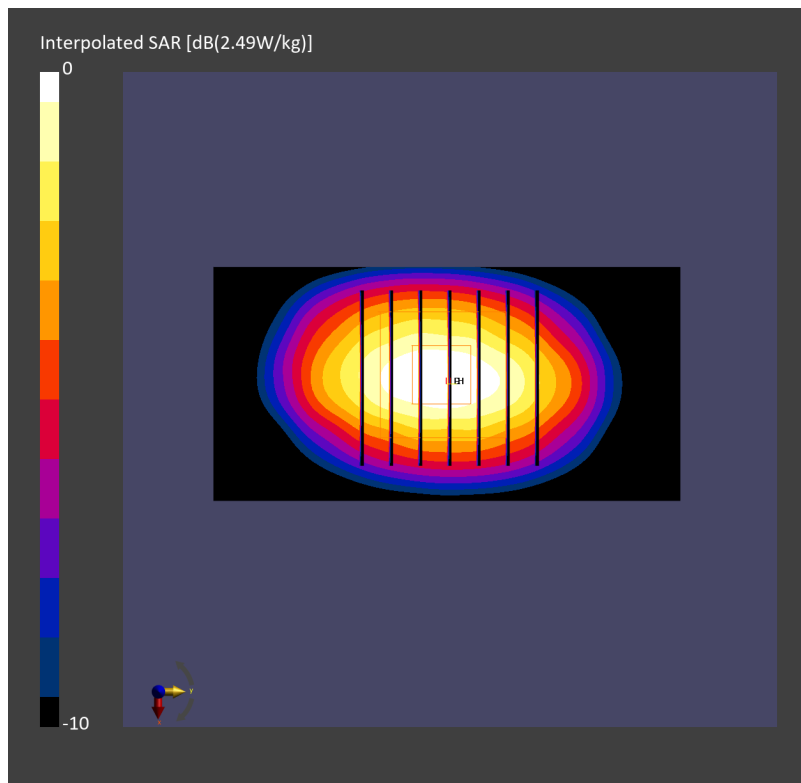

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240216 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.890$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.84, 9.84, 9.84); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.412 W/kg; SAR (10g) = 0.275 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.412 W/kg; SAR (8g) = 0.285 W/kg; SAR (10g) = 0.270 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.6 %

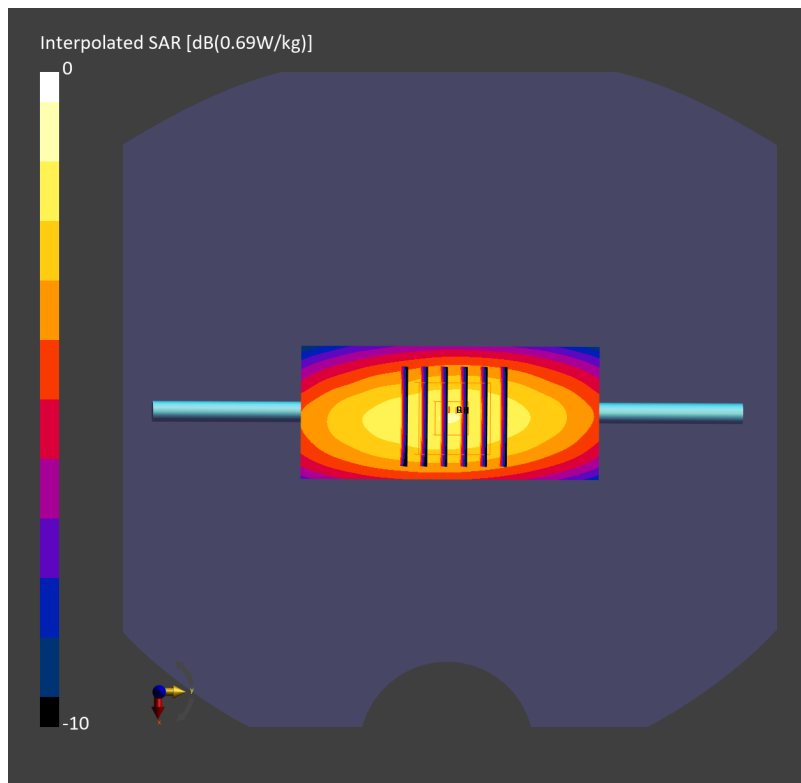

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240221 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.892$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.84, 9.84, 9.84); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.388 W/kg; SAR (10g) = 0.259 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 0.407 W/kg; SAR (8g) = 0.282 W/kg; SAR (10g) = 0.268 W/kg

Smallest distance from peaks to all points 3 dB below = 22.1 mm

Ratio of SAR at M2 to SAR at M1 = 82.6 %

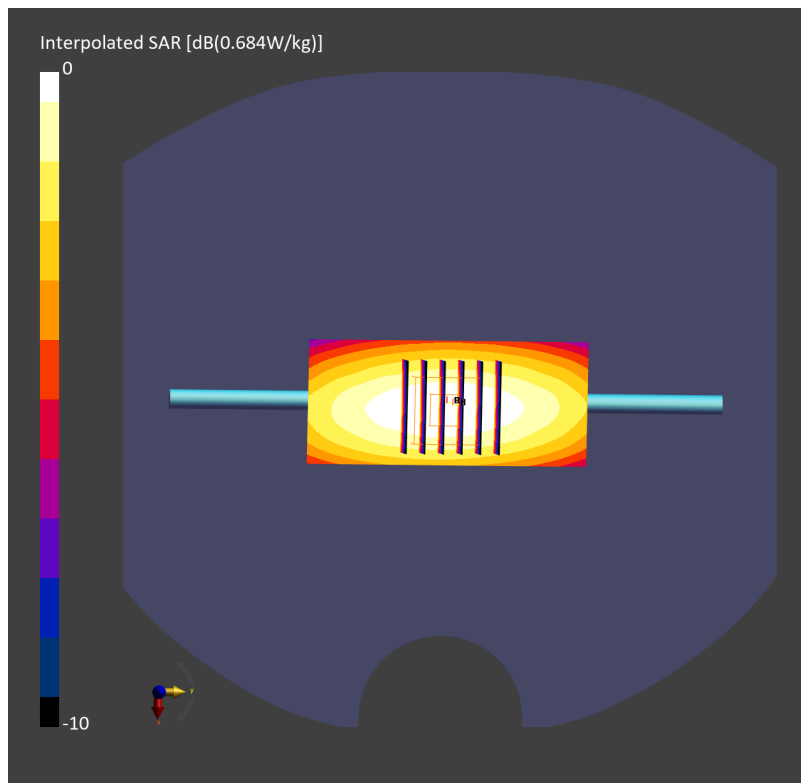

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240226 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.898$ S/m; $\epsilon_r = 42.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.45, 9.55, 9.92); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.422 W/kg; SAR (10g) = 0.282 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.421 W/kg; SAR (8g) = 0.298 W/kg; SAR (10g) = 0.284 W/kg

Smallest distance from peaks to all points 3 dB below = 19.7 mm

Ratio of SAR at M2 to SAR at M1 = 89.3 %

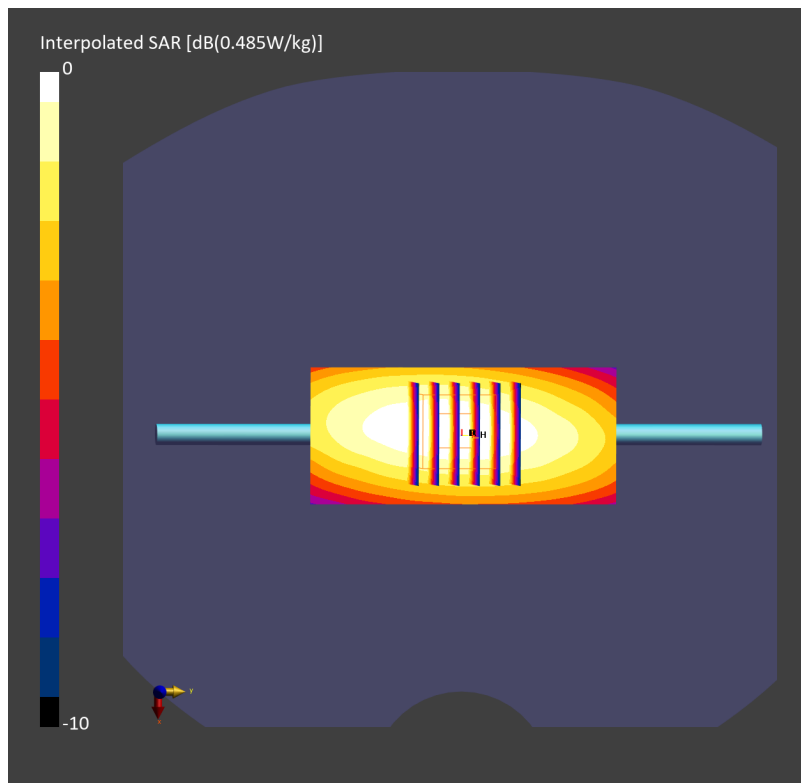

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240228 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.896$ S/m; $\epsilon_r = 43.1$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.45, 9.55, 9.92); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.421 W/kg; SAR (10g) = 0.282 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 0.421 W/kg; SAR (8g) = 0.295 W/kg; SAR (10g) = 0.280 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 89.3 %

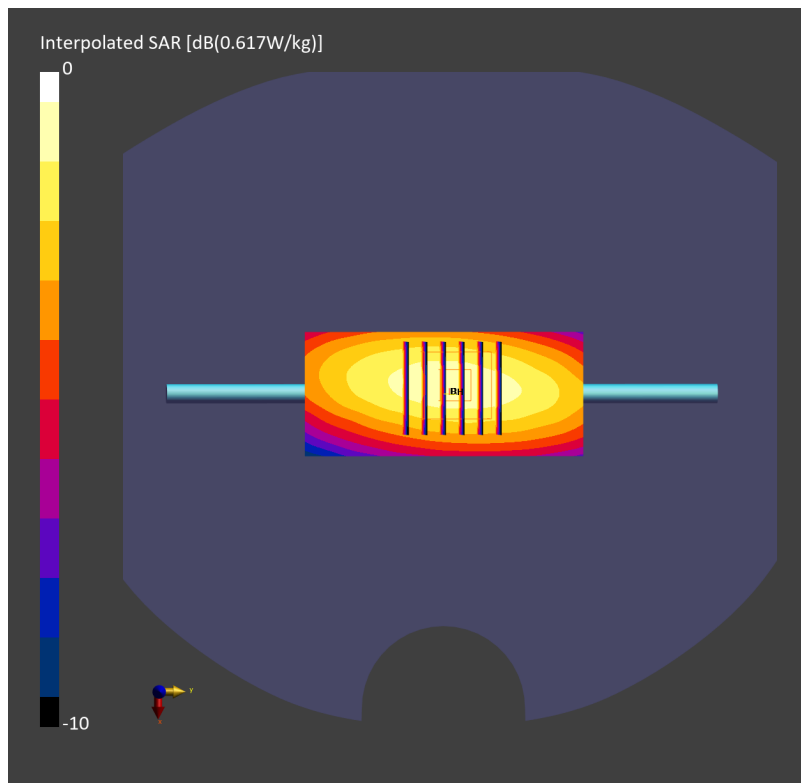

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240302 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.895$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.45, 9.55, 9.92); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.425 W/kg; SAR (10g) = 0.284 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.424 W/kg; SAR (8g) = 0.301 W/kg; SAR (10g) = 0.287 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

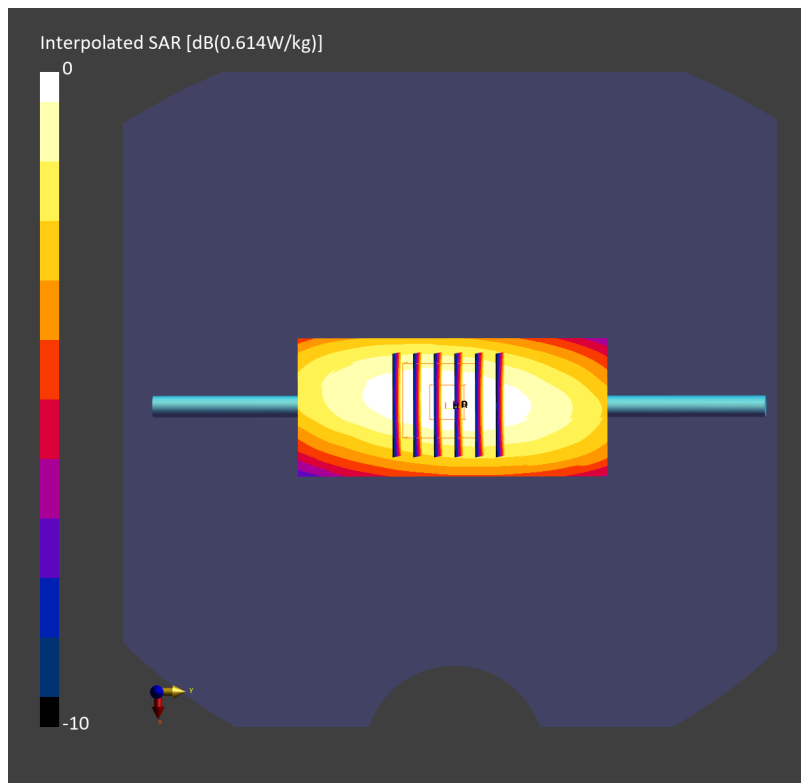

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240305 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.897$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.45, 9.55, 9.92); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.399 W/kg; SAR (10g) = 0.268 W/kg;


Pin=17dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.06 dB

SAR (1g) = 0.398 W/kg; SAR (8g) = 0.279 W/kg; SAR (10g) = 0.265 W/kg

Smallest distance from peaks to all points 3 dB below = 18.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.9 %

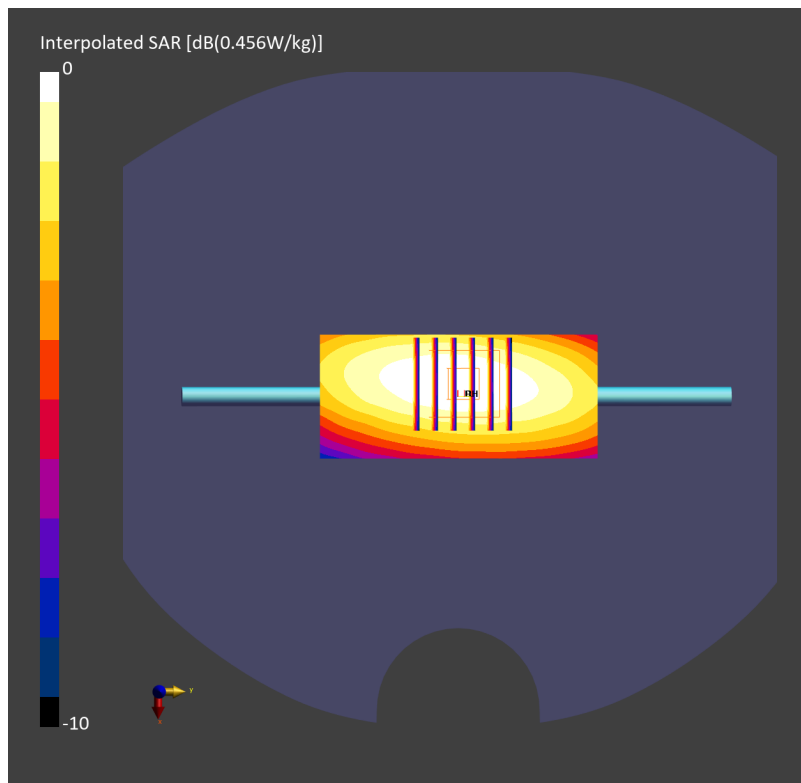

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240305 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.893$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.84, 9.84, 9.84); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.421 W/kg; SAR (10g) = 0.280 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.422 W/kg; SAR (8g) = 0.289 W/kg; SAR (10g) = 0.274 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 83.1 %

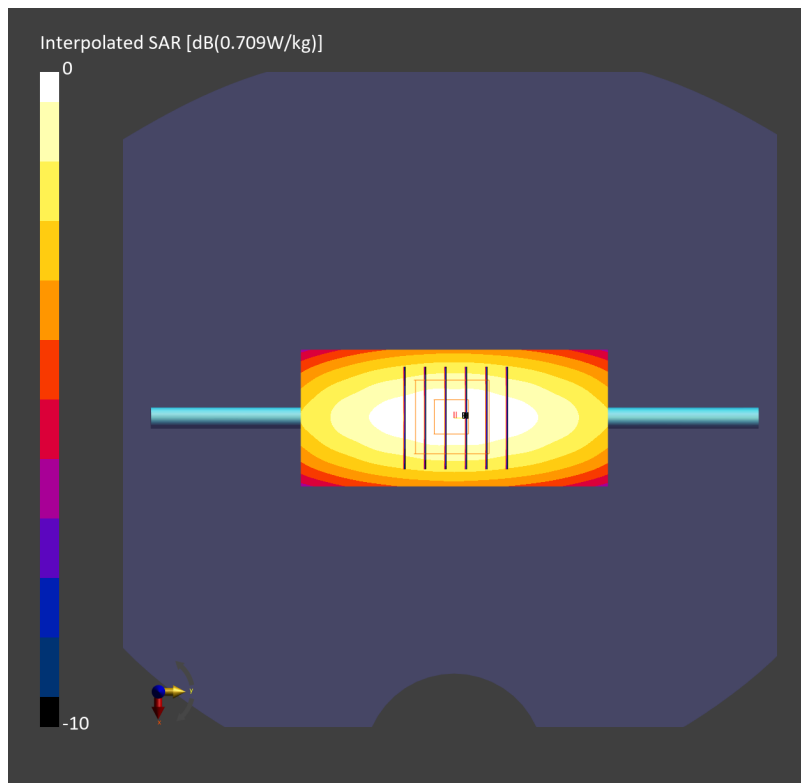

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240306 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.896$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.84, 9.84, 9.84); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.421 W/kg; SAR (10g) = 0.280 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 0.423 W/kg; SAR (8g) = 0.292 W/kg; SAR (10g) = 0.277 W/kg

Smallest distance from peaks to all points 3 dB below = 22.2 mm

Ratio of SAR at M2 to SAR at M1 = 84.4 %

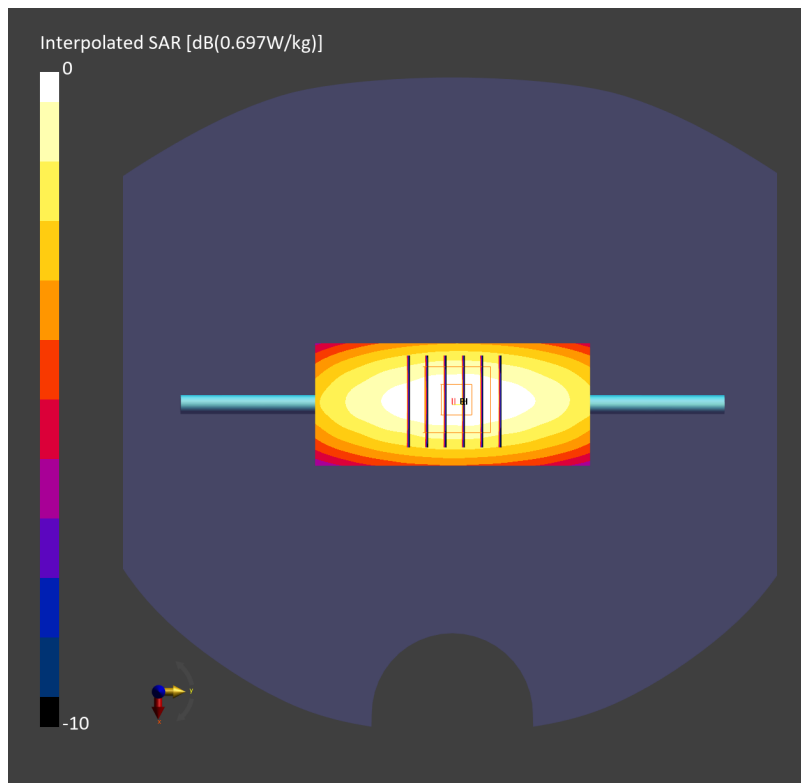

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240307 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.877$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.45, 9.55, 9.92); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.406 W/kg; SAR (10g) = 0.271 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 0.401 W/kg; SAR (8g) = 0.282 W/kg; SAR (10g) = 0.268 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.3 %

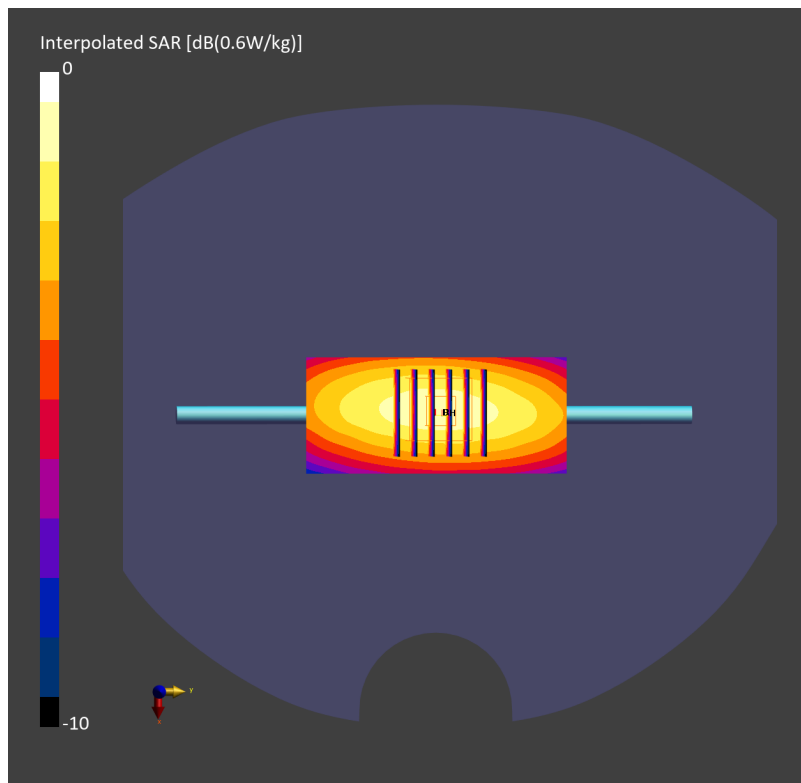

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240310 Medium parameters used: $f=750.000$ MHz; $\sigma=0.884$ S/m; $\epsilon_r=42.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.45, 9.55, 9.92); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.393 W/kg; SAR (10g) = 0.261 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.06 dB

SAR (1g) = 0.402 W/kg; SAR (8g) = 0.283 W/kg; SAR (10g) = 0.269 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

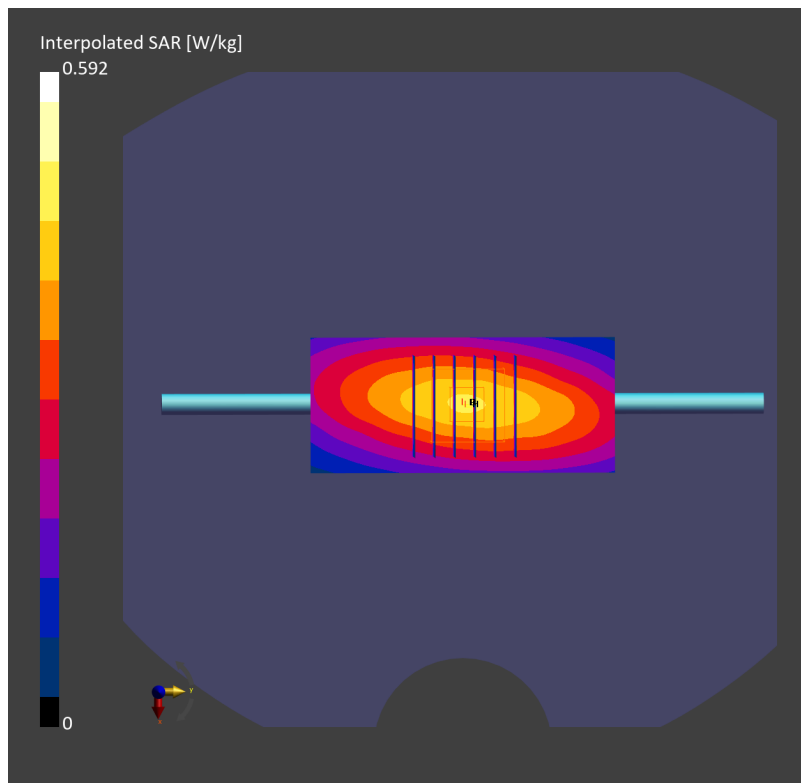

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240310 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.886$ S/m; $\epsilon_r = 43.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.84, 9.84, 9.84); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.403 W/kg; SAR (10g) = 0.267 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.04 dB

SAR (1g) = 0.397 W/kg; SAR (8g) = 0.275 W/kg; SAR (10g) = 0.260 W/kg

Smallest distance from peaks to all points 3 dB below = 16.1 mm

Ratio of SAR at M2 to SAR at M1 = 83.3 %

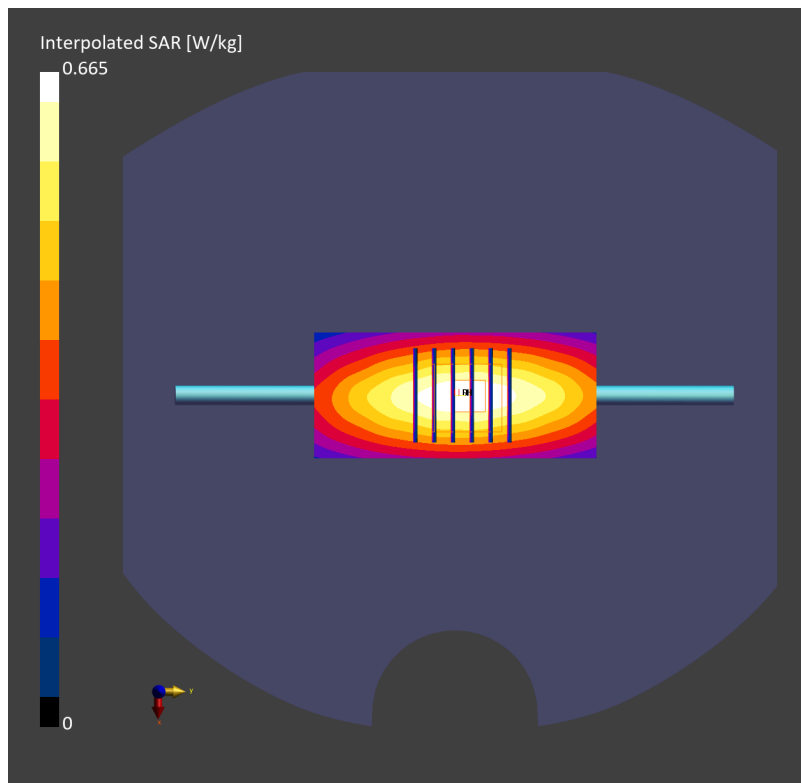

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240311 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.890$ S/m; $\epsilon_r = 42.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(8.42, 8.24, 8.07); Calibrated: 2023-11-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2023-12-06
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2127; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.401 W/kg; SAR (10g) = 0.268 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.404 W/kg; SAR (8g) = 0.286 W/kg; SAR (10g) = 0.272 W/kg

Smallest distance from peaks to all points 3 dB below = 22.1 mm

Ratio of SAR at M2 to SAR at M1 = 93.1 %

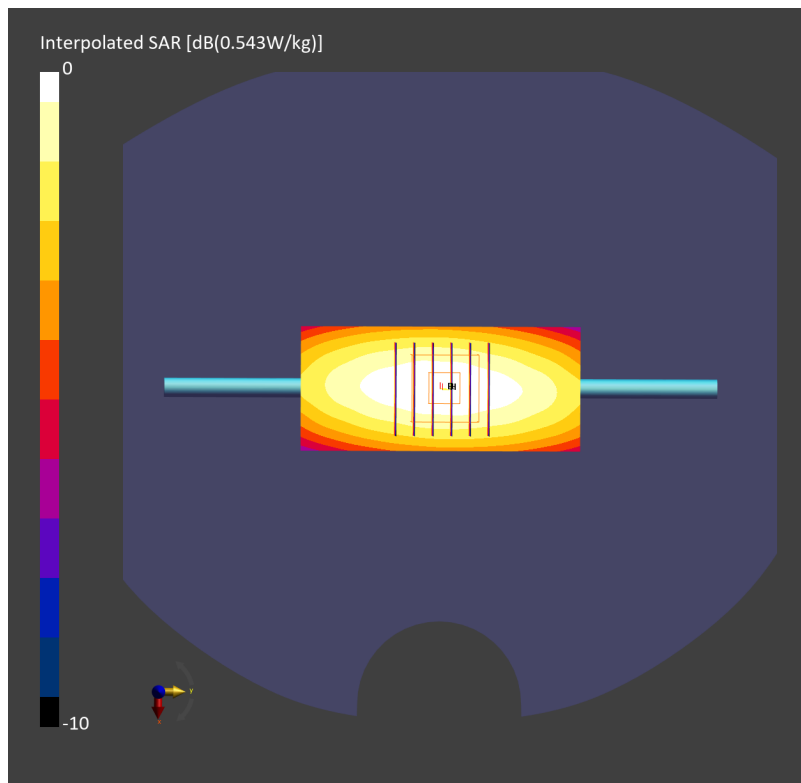

System Check_Head_750MHz

DUT: D750V3 - SN1107

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL_750_240317 Medium parameters used: $f = 750.000$ MHz; $\sigma = 0.889$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.45, 9.55, 9.92); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.416 W/kg; SAR (10g) = 0.278 W/kg;


Pin=17dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 0.413 W/kg; SAR (8g) = 0.289 W/kg; SAR (10g) = 0.274 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.7 %

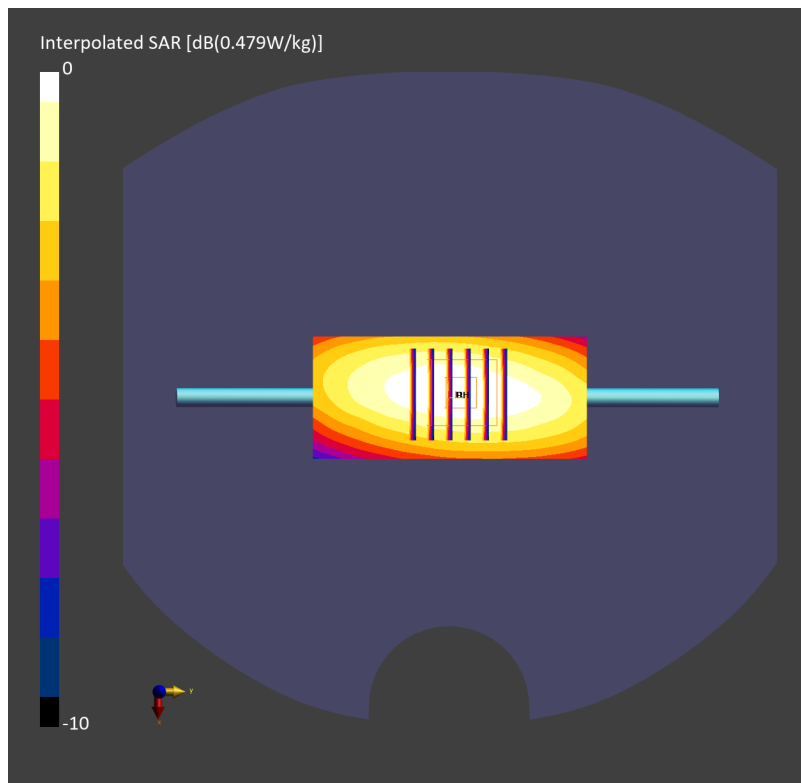

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240214 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.924$ S/m; $\epsilon_r = 42.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.48, 9.48, 9.48); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.525 W/kg; SAR (10g) = 0.346 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 0.526 W/kg; SAR (8g) = 0.359 W/kg; SAR (10g) = 0.340 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

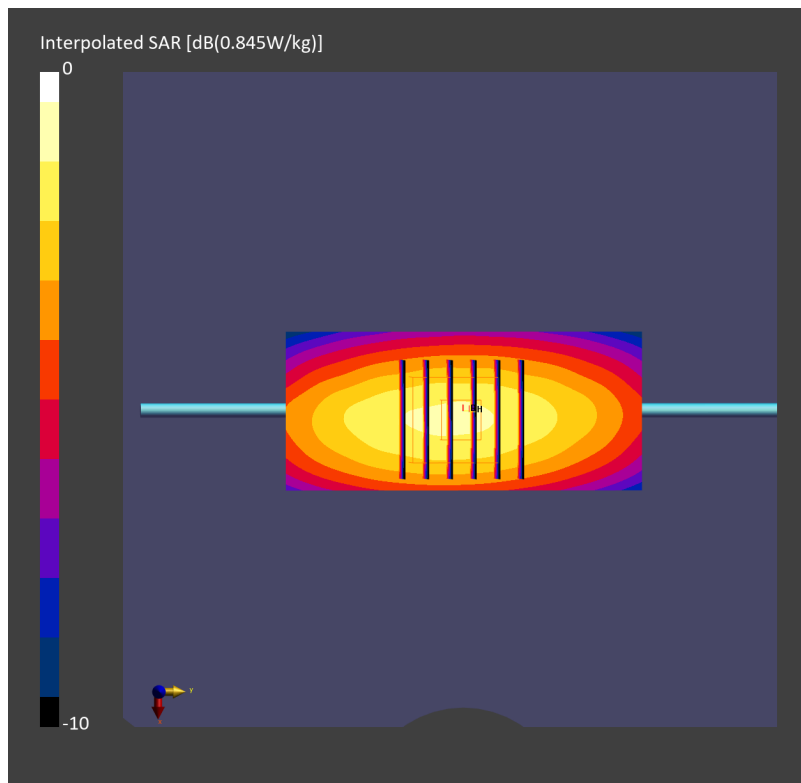

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240218 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.923$ S/m; $\epsilon_r = 41.4$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.48, 9.48, 9.48); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.530 W/kg; SAR (10g) = 0.349 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.09 dB

SAR (1g) = 0.521 W/kg; SAR (8g) = 0.356 W/kg; SAR (10g) = 0.337 W/kg

Smallest distance from peaks to all points 3 dB below = 16.4 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

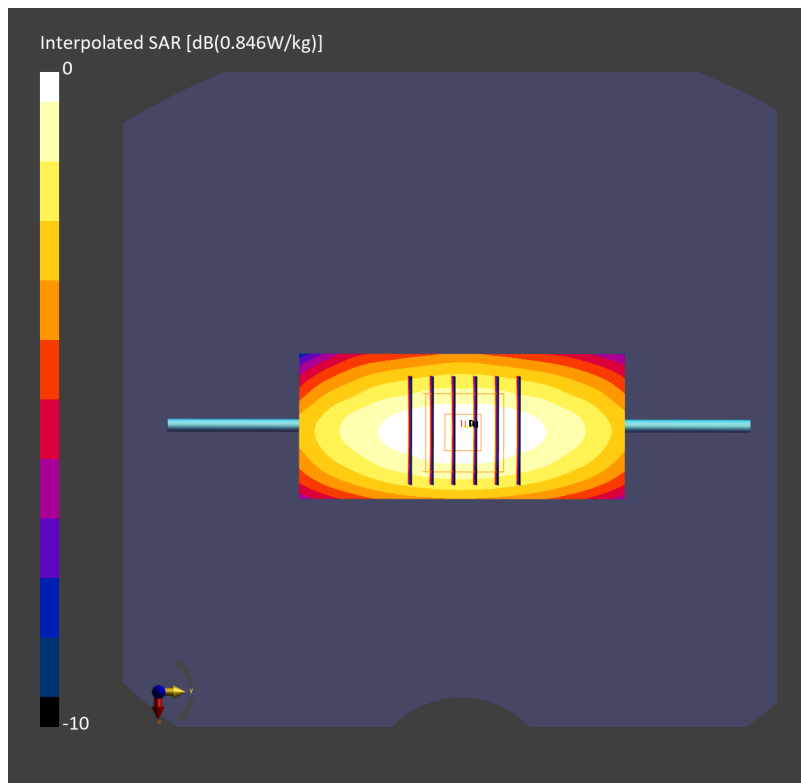

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240301 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.930$ S/m; $\epsilon_r = 42.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.49, 9.77, 9.84); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.499 W/kg; SAR (10g) = 0.329 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.500 W/kg; SAR (8g) = 0.349 W/kg; SAR (10g) = 0.331 W/kg

Smallest distance from peaks to all points 3 dB below = 18.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.9 %

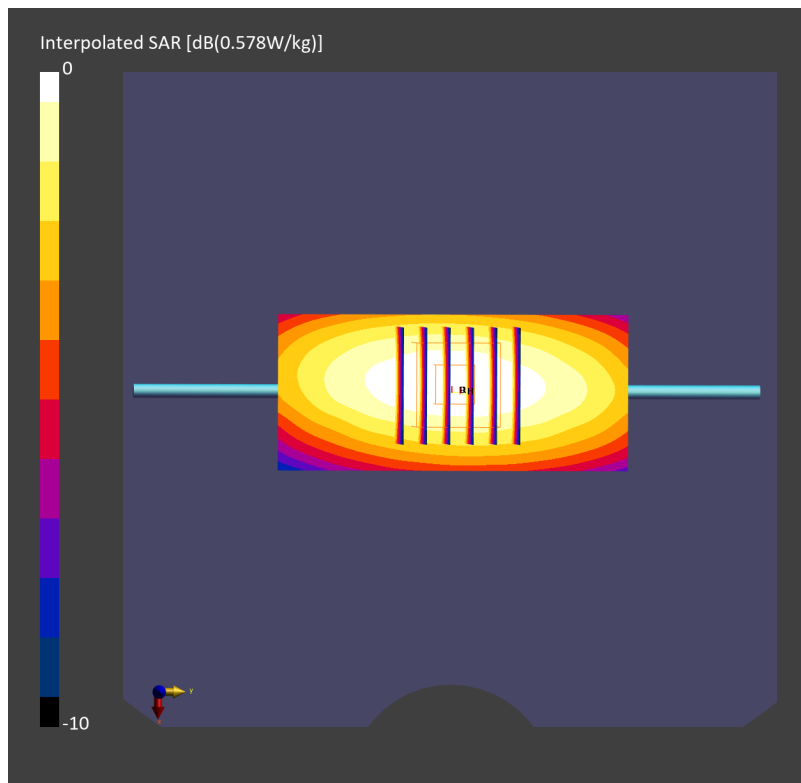

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240302 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.936$ S/m; $\epsilon_r = 42.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.48, 9.48, 9.48); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.515 W/kg; SAR (10g) = 0.338 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.513 W/kg; SAR (8g) = 0.352 W/kg; SAR (10g) = 0.333 W/kg

Smallest distance from peaks to all points 3 dB below = 18.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

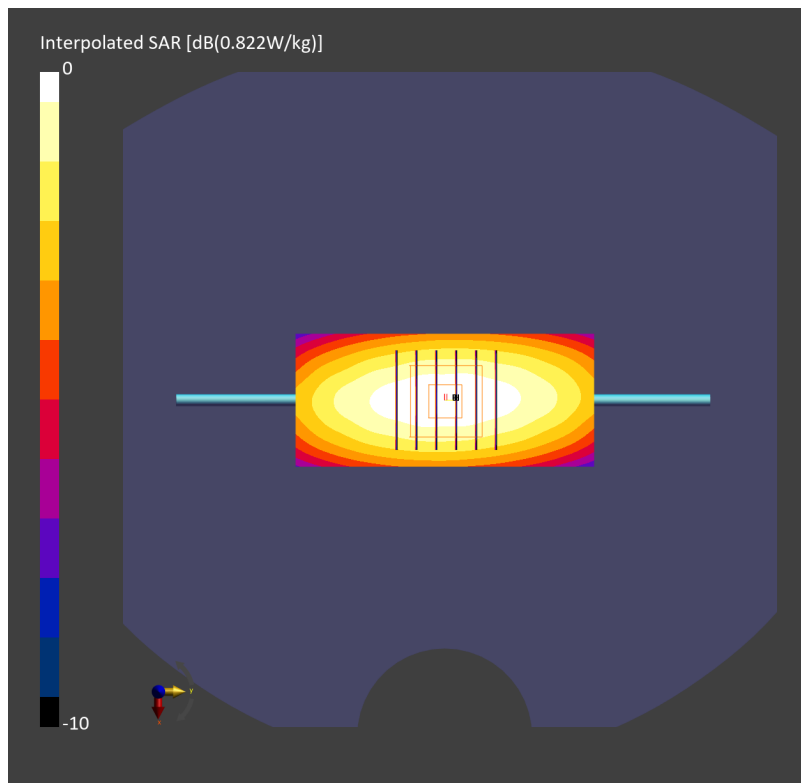

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240304 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.928$ S/m; $\epsilon_r = 42.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.48, 9.48, 9.48); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.515 W/kg; SAR (10g) = 0.340 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.518 W/kg; SAR (8g) = 0.357 W/kg; SAR (10g) = 0.338 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 85.5 %

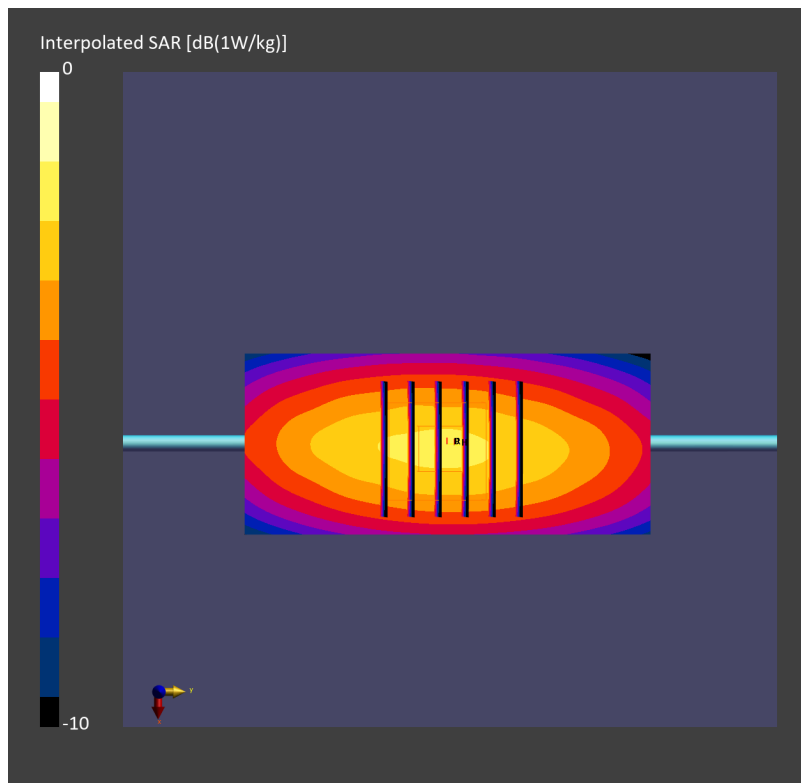

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240305 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.932$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.49, 9.77, 9.84); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.478 W/kg; SAR (10g) = 0.317 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 0.480 W/kg; SAR (8g) = 0.335 W/kg; SAR (10g) = 0.318 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

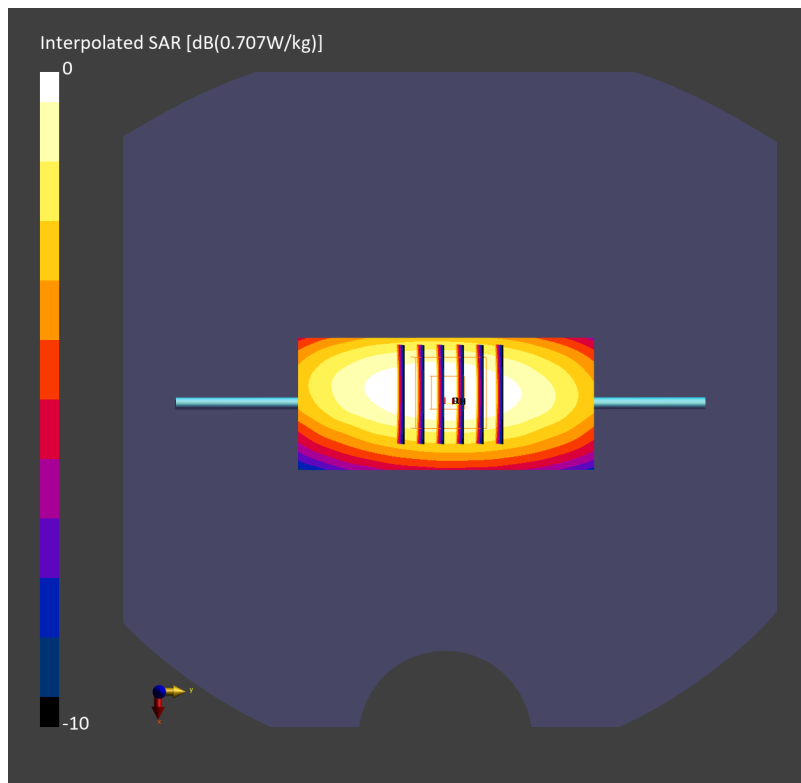

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240306 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.930$ S/m; $\epsilon_r = 42.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.48, 9.48, 9.48); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.512 W/kg; SAR (10g) = 0.337 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.512 W/kg; SAR (8g) = 0.351 W/kg; SAR (10g) = 0.332 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.0 %

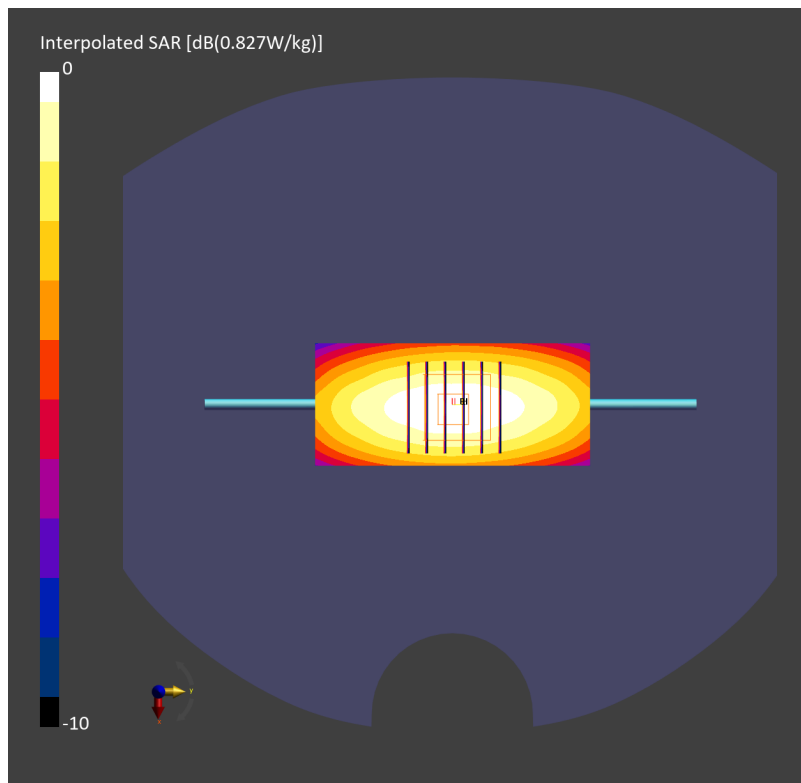

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240307 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.930$ S/m; $\epsilon_r = 41.9$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.48, 9.48, 9.48); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.517 W/kg; SAR (10g) = 0.339 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 0.515 W/kg; SAR (8g) = 0.354 W/kg; SAR (10g) = 0.335 W/kg

Smallest distance from peaks to all points 3 dB below = 18.0 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

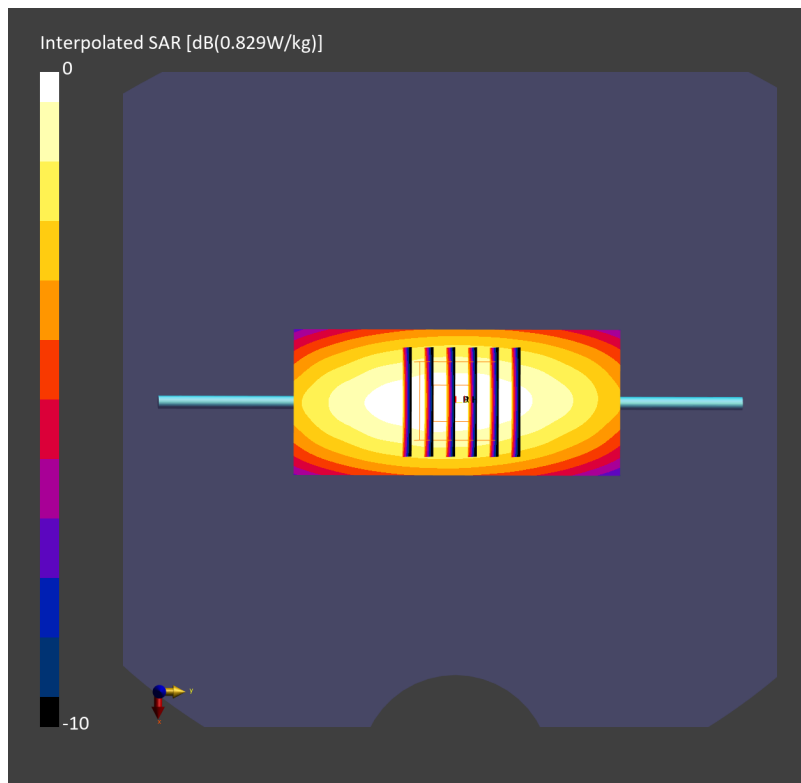

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240307 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.909$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.49, 9.77, 9.84); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.484 W/kg; SAR (10g) = 0.319 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.483 W/kg; SAR (8g) = 0.337 W/kg; SAR (10g) = 0.320 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

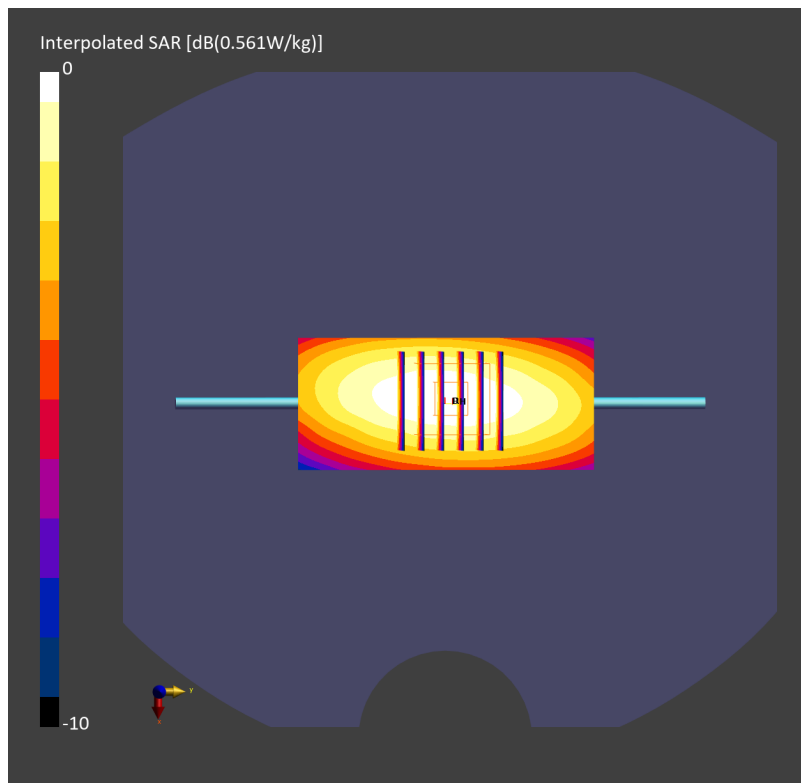

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240308 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.926$ S/m; $\epsilon_r = 41.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.49, 9.77, 9.84); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.488 W/kg; SAR (10g) = 0.321 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.492 W/kg; SAR (8g) = 0.344 W/kg; SAR (10g) = 0.326 W/kg

Smallest distance from peaks to all points 3 dB below = 17.4 mm

Ratio of SAR at M2 to SAR at M1 = 89.3 %

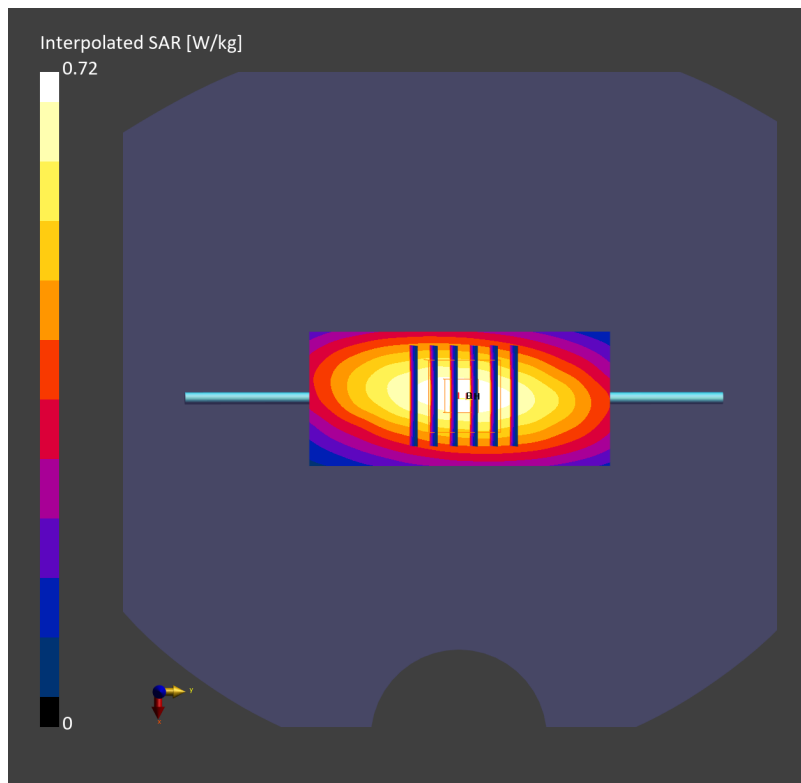

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240310 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.919$ S/m; $\epsilon_r = 43.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.48, 9.48, 9.48); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.520 W/kg; SAR (10g) = 0.340 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.04 dB

SAR (1g) = 0.519 W/kg; SAR (8g) = 0.357 W/kg; SAR (10g) = 0.339 W/kg

Smallest distance from peaks to all points 3 dB below = 16.1 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

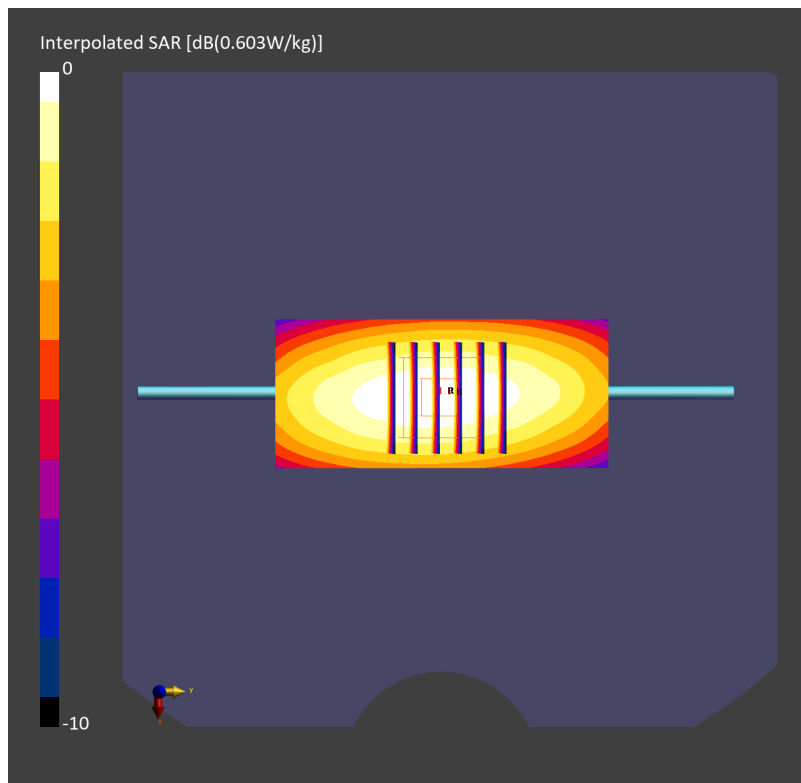

System Check_Head_835MHz

DUT: D835V2 - SN4d167

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240310 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.918$ S/m; $\epsilon_r = 42.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(9.49, 9.77, 9.84); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.496 W/kg; SAR (10g) = 0.326 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 0.483 W/kg; SAR (8g) = 0.337 W/kg; SAR (10g) = 0.320 W/kg

Smallest distance from peaks to all points 3 dB below = 17.2 mm

Ratio of SAR at M2 to SAR at M1 = 89.0 %

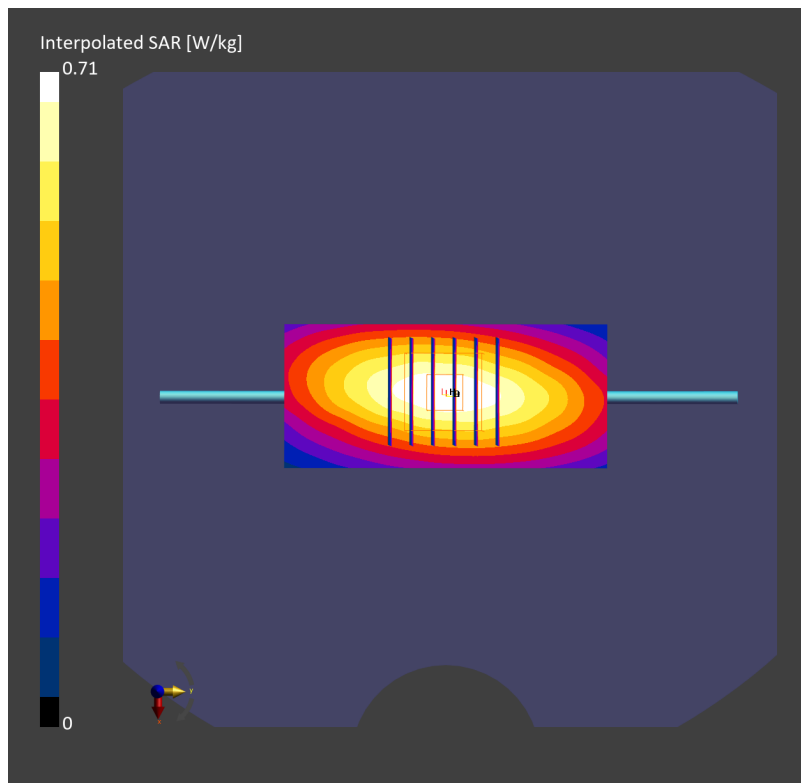

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240315 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.932$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(8.71, 9.44, 8.39); Calibrated: 2024-02-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.495 W/kg; SAR (10g) = 0.326 W/kg;


Pin=17dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.11 dB

SAR (1g) = 0.497 W/kg; SAR (8g) = 0.348 W/kg; SAR (10g) = 0.330 W/kg

Smallest distance from peaks to all points 3 dB below = 16.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.4 %

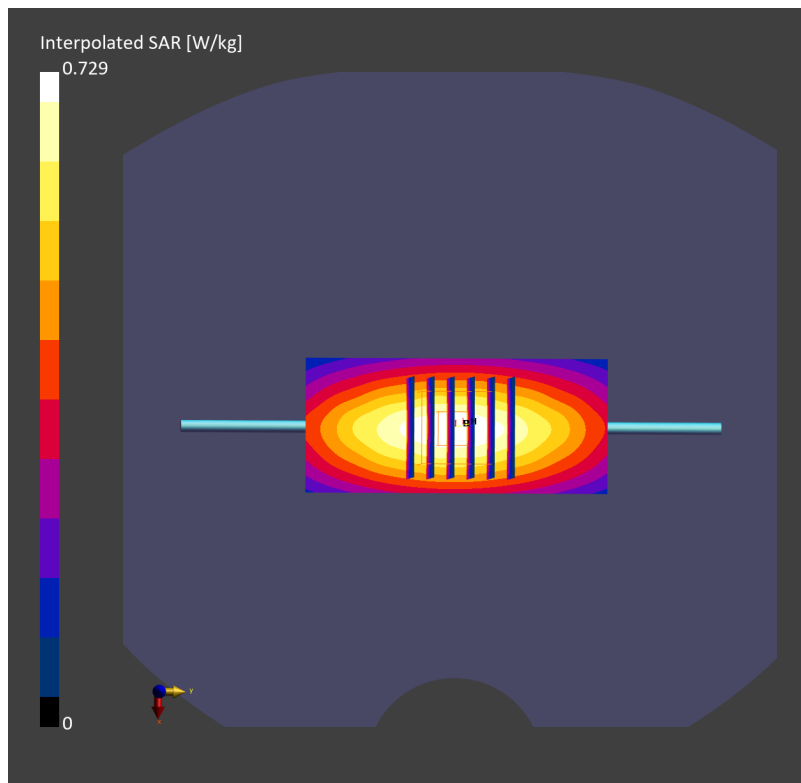

System Check_Head_835MHz

DUT: D835V2 - SN4d060

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL_850_240315 Medium parameters used: $f = 835.000$ MHz; $\sigma = 0.932$ S/m; $\epsilon_r = 42.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(9.25, 9.62, 9.49); Calibrated: 2023-05-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.486 W/kg; SAR (10g) = 0.320 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 0.492 W/kg; SAR (8g) = 0.344 W/kg; SAR (10g) = 0.327 W/kg

Smallest distance from peaks to all points 3 dB below = 18.4 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

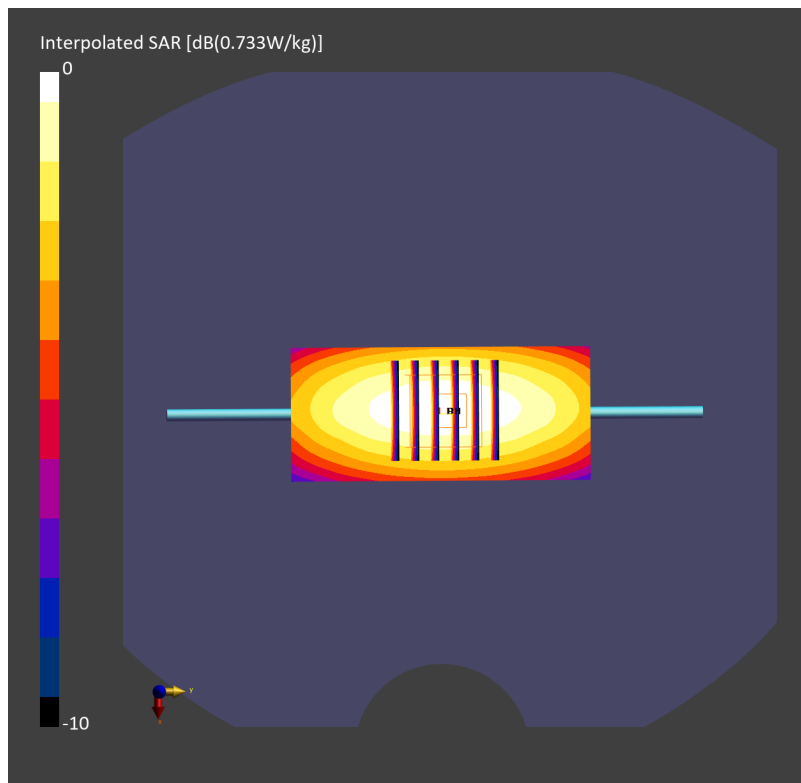

System Check_Head_1640MHz

DUT: D1640V2 - SN346

Communication System: CW; Frequency: 1640.000 MHz

Medium: HSL_1640_240309 Medium parameters used: $f = 1640.000$ MHz; $\sigma = 1.27$ S/m; $\epsilon_r = 39.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7785; ConvF(7.62, 7.1, 7.02); Calibrated: 2023-11-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1707; Calibrated: 2023-12-06
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2126; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.68 W/kg; SAR (10g) = 0.910 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 1.63 W/kg; SAR (8g) = 0.977 W/kg; SAR (10g) = 0.905 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 89.7 %

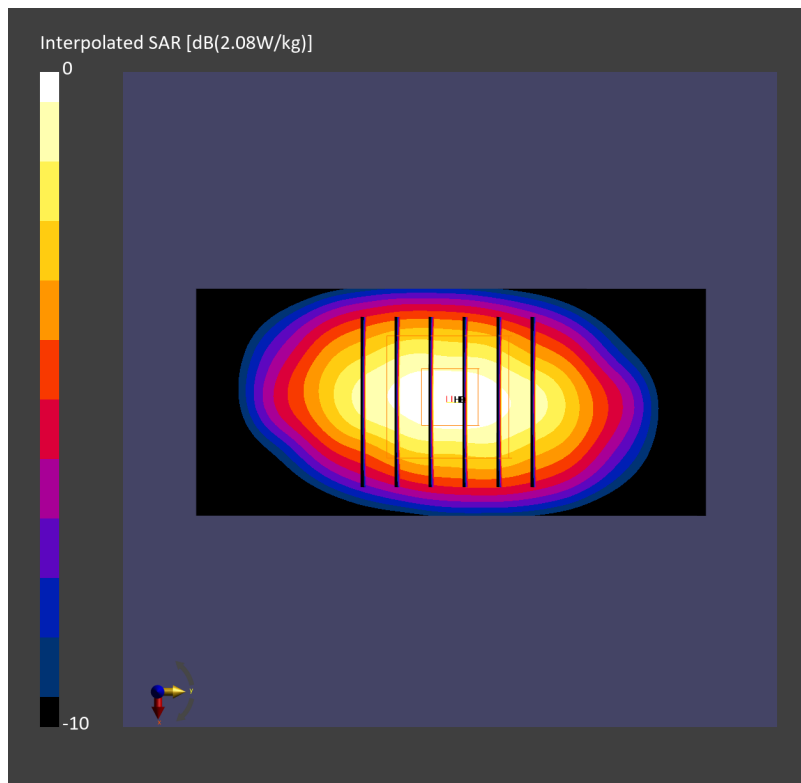

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240218 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.82, 8.82, 8.82); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.81 W/kg; SAR (10g) = 0.963 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.14 dB

SAR (1g) = 1.83 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.960 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 78.9 %

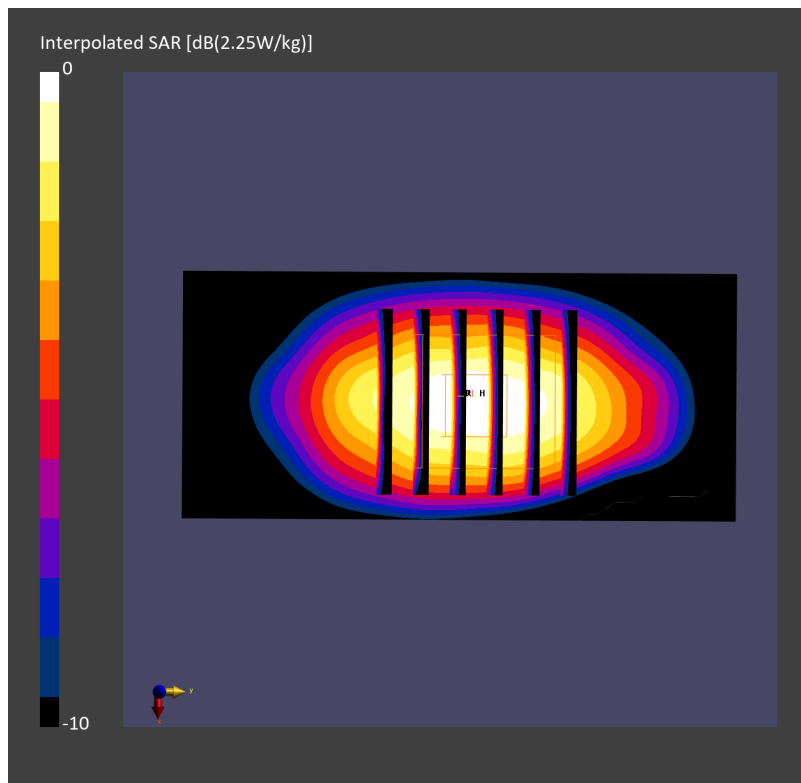

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240225 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.14, 8.24, 8.22); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.937 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.75 W/kg; SAR (8g) = 1.03 W/kg; SAR (10g) = 0.948 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

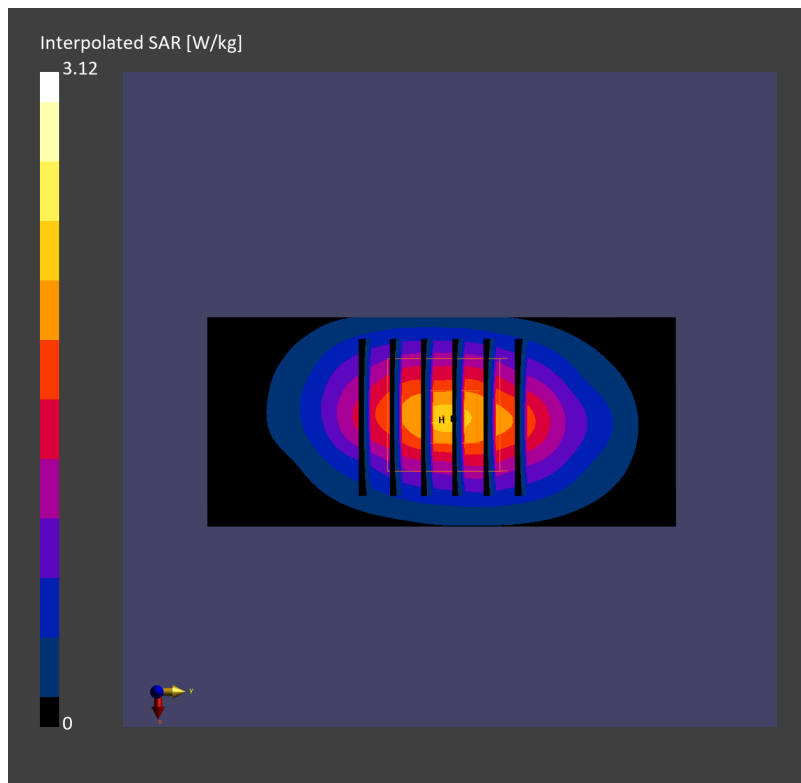

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240228 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.14, 8.24, 8.22); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.80 W/kg; SAR (10g) = 0.977 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.81 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.971 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 83.5 %

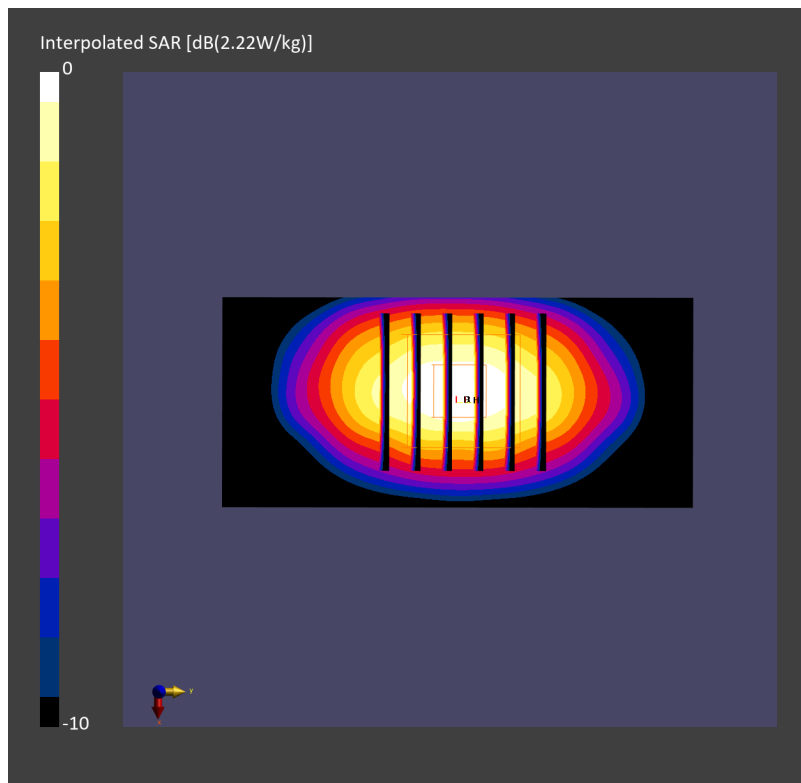

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240308 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.82, 8.82, 8.82); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.77 W/kg; SAR (10g) = 0.928 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 1.79 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.932 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.7 %

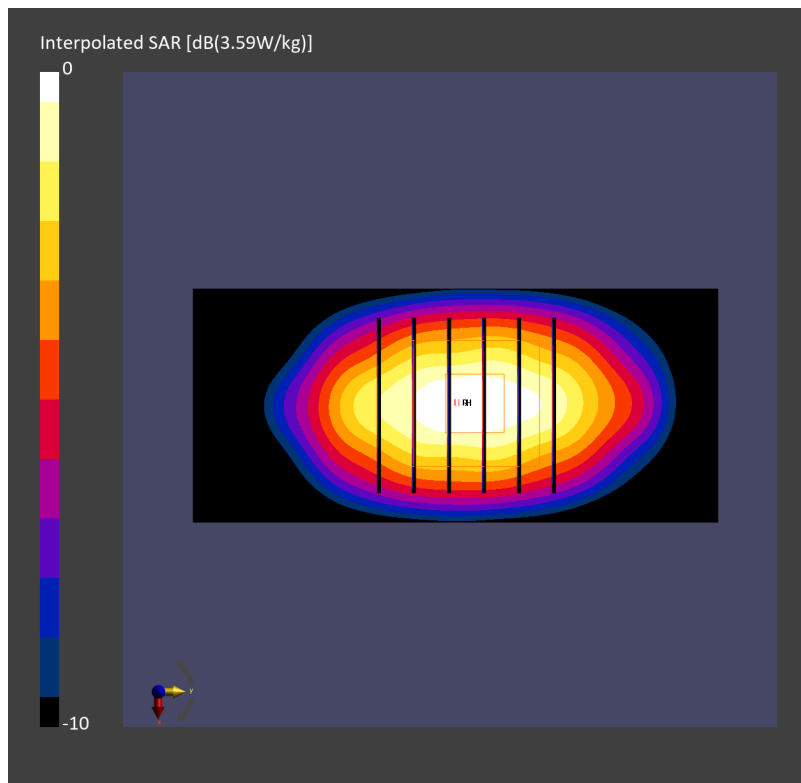

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240308 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.14, 8.24, 8.22); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.69 W/kg; SAR (10g) = 0.900 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.04 dB

SAR (1g) = 1.69 W/kg; SAR (8g) = 0.988 W/kg; SAR (10g) = 0.913 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 83.5 %

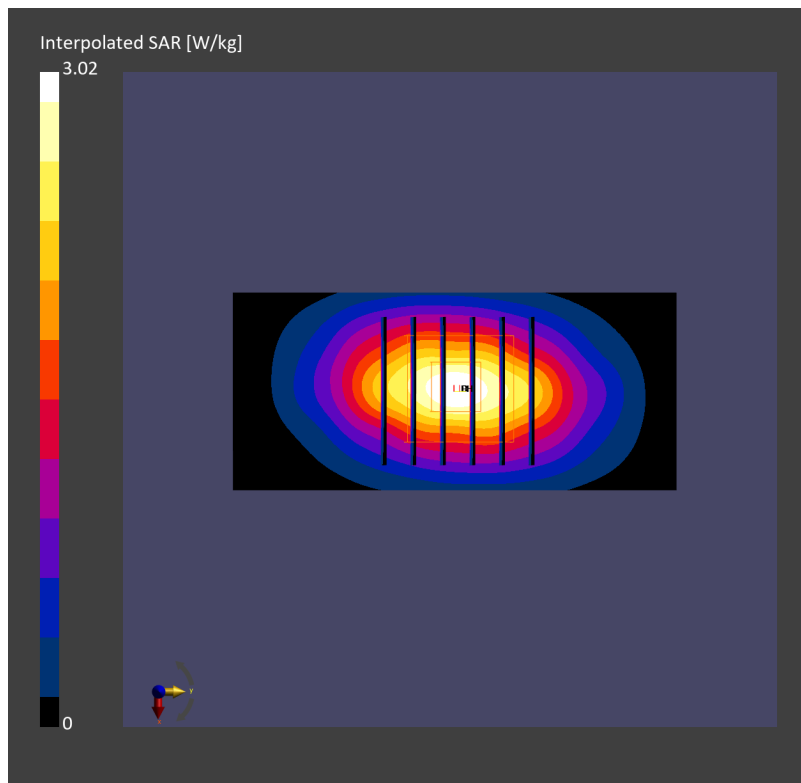

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240309 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.14, 8.24, 8.22); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.83 W/kg; SAR (10g) = 0.956 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.18 dB

SAR (1g) = 1.81 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.960 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 82.0 %

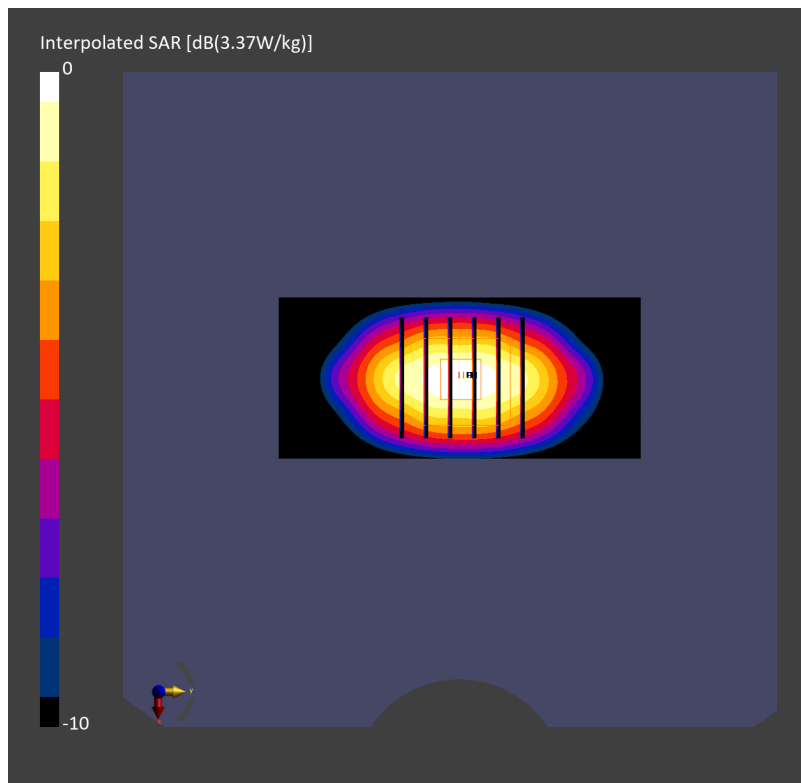

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240309 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.82, 8.82, 8.82); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.67 W/kg; SAR (10g) = 0.896 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 1.67 W/kg; SAR (8g) = 0.958 W/kg; SAR (10g) = 0.884 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 81.6 %

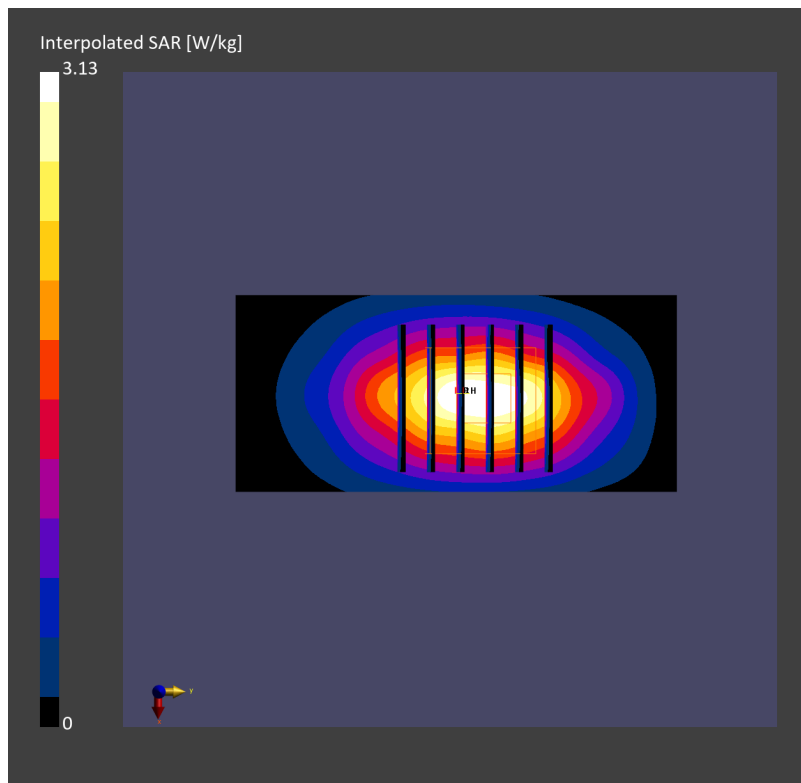

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240310 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.82, 8.82, 8.82); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.69 W/kg; SAR (10g) = 0.898 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.05 dB

SAR (1g) = 1.70 W/kg; SAR (8g) = 0.972 W/kg; SAR (10g) = 0.895 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 79.9 %

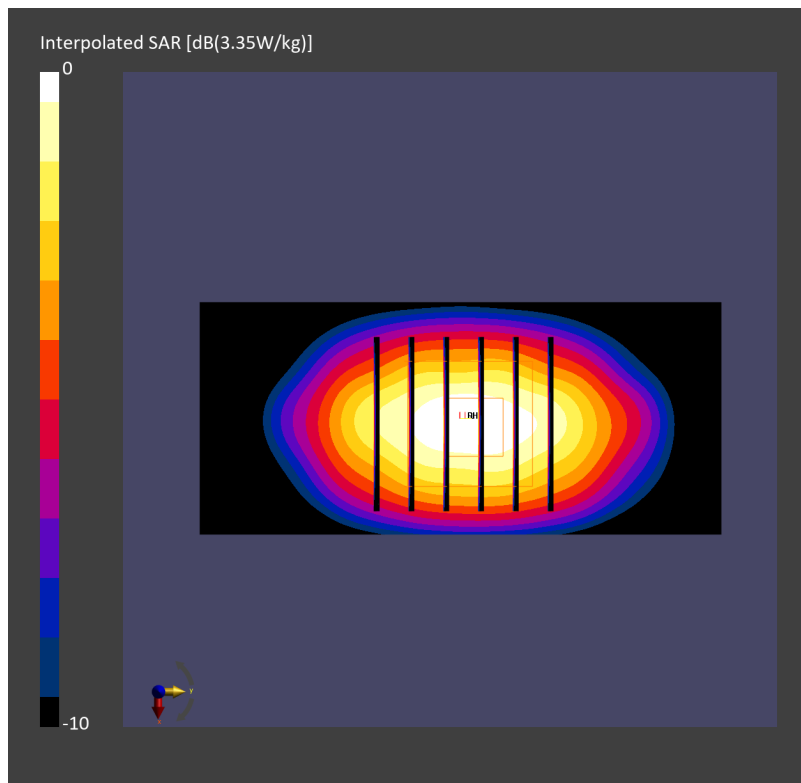

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240311 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 40.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.14, 8.24, 8.22); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.73 W/kg; SAR (10g) = 0.926 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.72 W/kg; SAR (8g) = 1.01 W/kg; SAR (10g) = 0.931 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 84.2 %

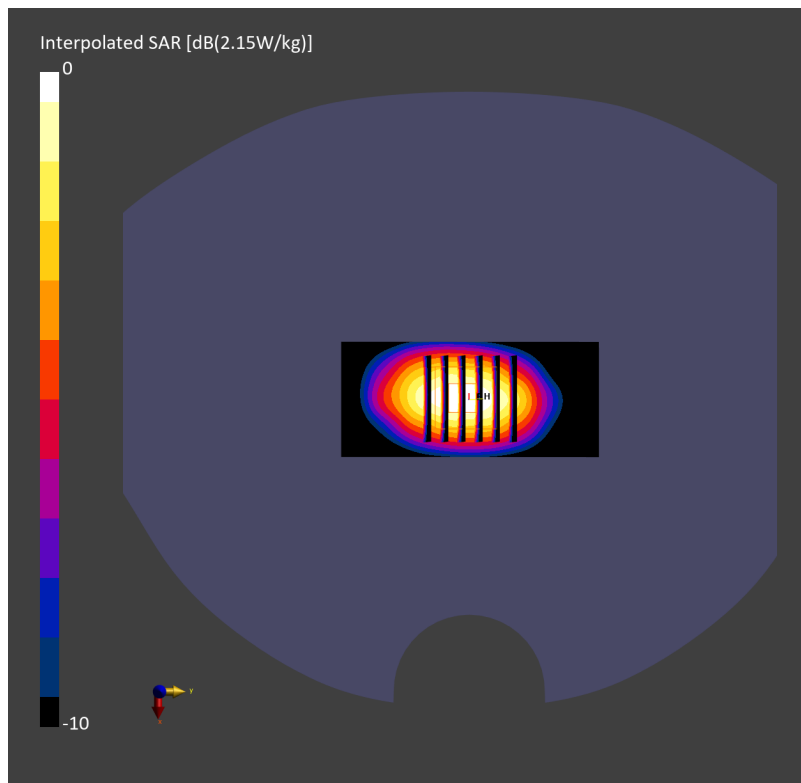

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240312 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(8.14, 8.24, 8.22); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.79 W/kg; SAR (10g) = 0.962 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.79 W/kg; SAR (8g) = 1.04 W/kg; SAR (10g) = 0.961 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

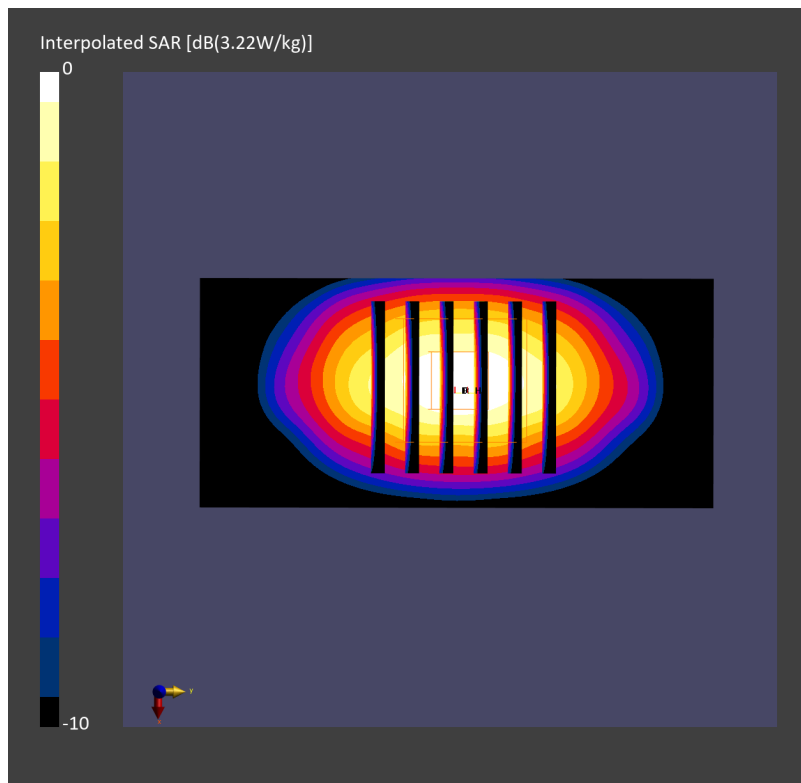

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240314 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(7.62, 8.22, 7.18); Calibrated: 2024-02-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.68 W/kg; SAR (10g) = 0.899 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 1.71 W/kg; SAR (8g) = 0.994 W/kg; SAR (10g) = 0.917 W/kg

Smallest distance from peaks to all points 3 dB below = 10.3 mm

Ratio of SAR at M2 to SAR at M1 = 82.9 %

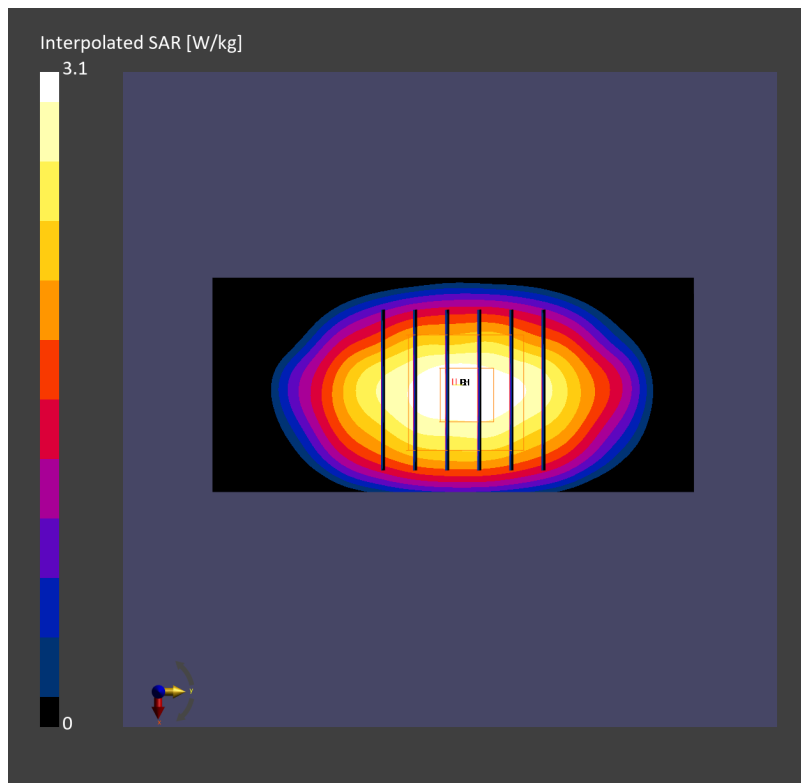

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240316 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(8.05, 8.4, 8.24); Calibrated: 2023-05-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.75 W/kg; SAR (10g) = 0.941 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.76 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.941 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 81.6 %

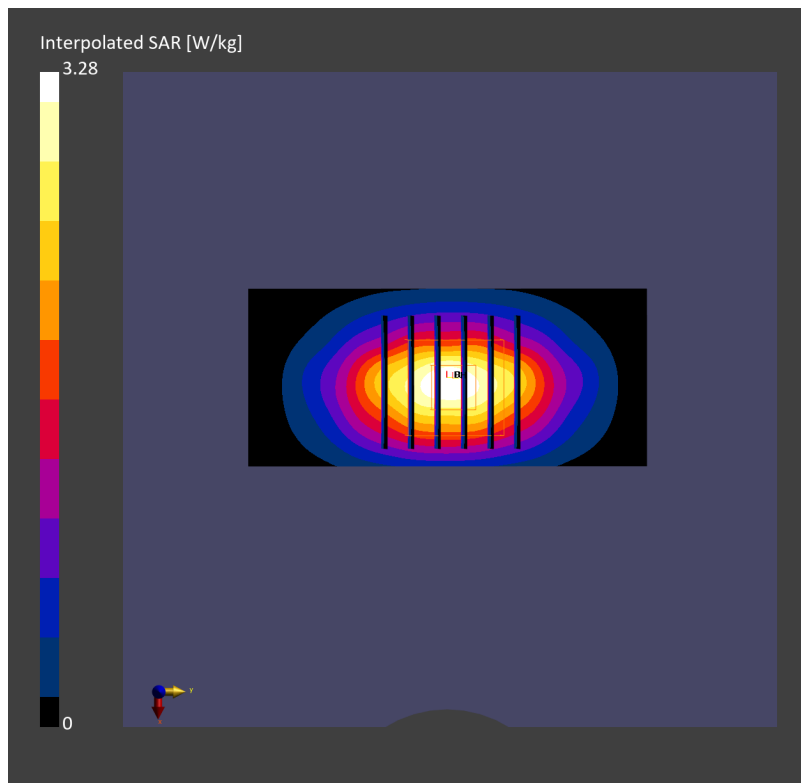

System Check_Head_1750MHz

DUT: D1750V2 - SN1112

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL_1750_240318 Medium parameters used: $f = 1750.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 41.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(8.05, 8.4, 8.24); Calibrated: 2023-05-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1647; Calibrated: 2023-12-27
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2079_For Gap; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.79 W/kg; SAR (10g) = 0.966 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.82 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.977 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 82.2 %

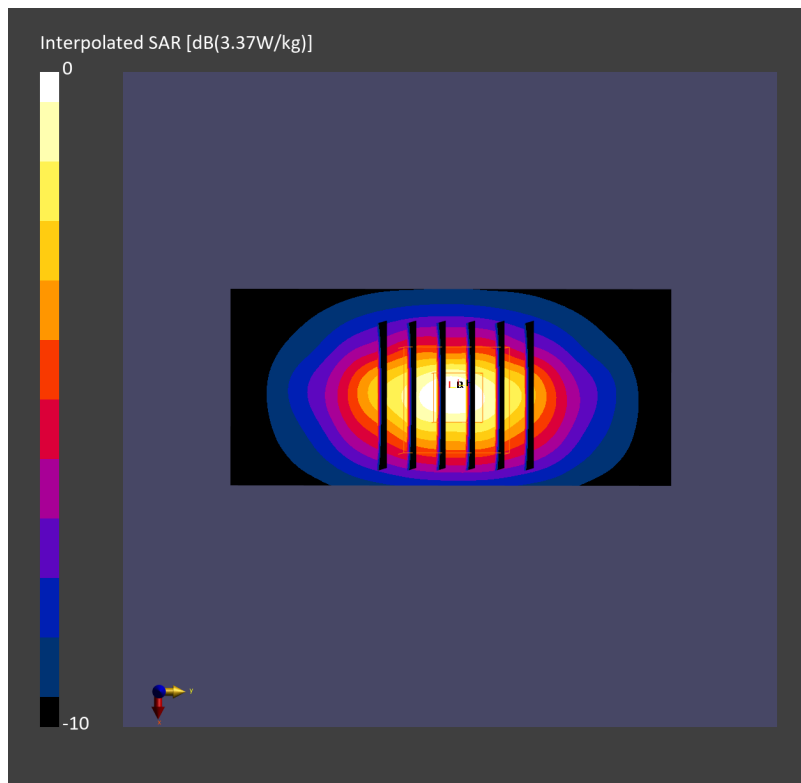

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_240225 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 40.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.7, 7.85, 7.85); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.95 W/kg; SAR (10g) = 1.00 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 1.91 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.00 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.9 %

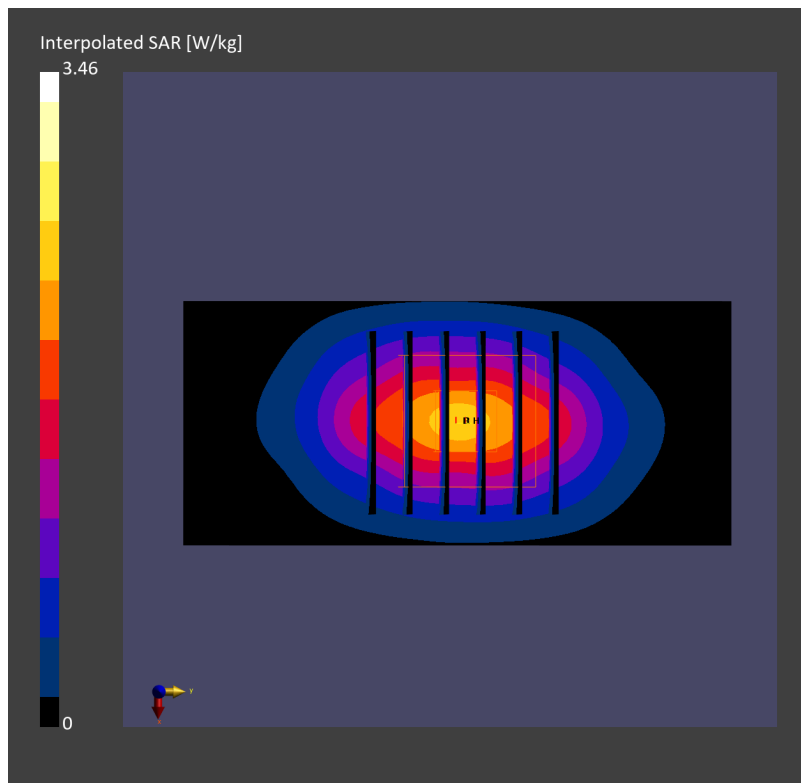

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_240228 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 40.2$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.7, 7.85, 7.85); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 0.989 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.90 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.993 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 83.6 %

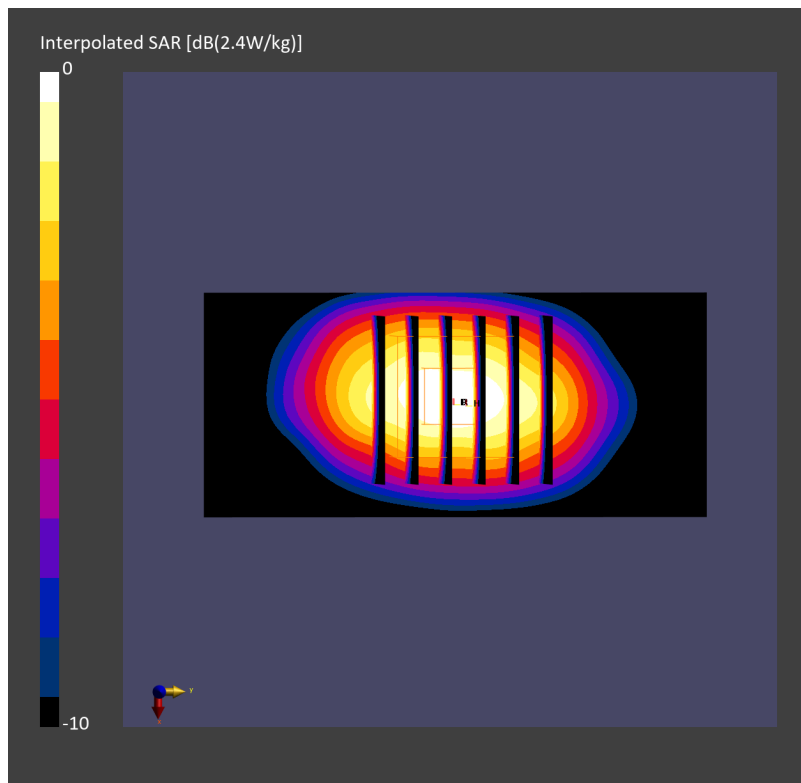

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_240301 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.3, 8.3, 8.3); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.08 W/kg; SAR (10g) = 1.08 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.17 dB

SAR (1g) = 2.00 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.07 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 81.5 %

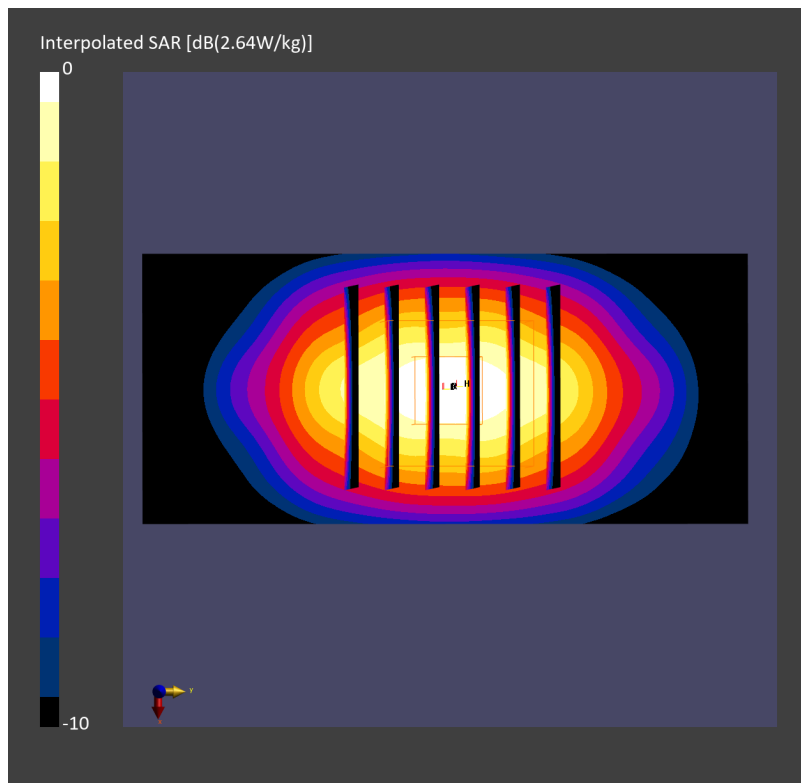

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_240305 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.3, 8.3, 8.3); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.15 W/kg; SAR (10g) = 1.11 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.18 dB

SAR (1g) = 2.05 W/kg; SAR (8g) = 1.15 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 80.8 %

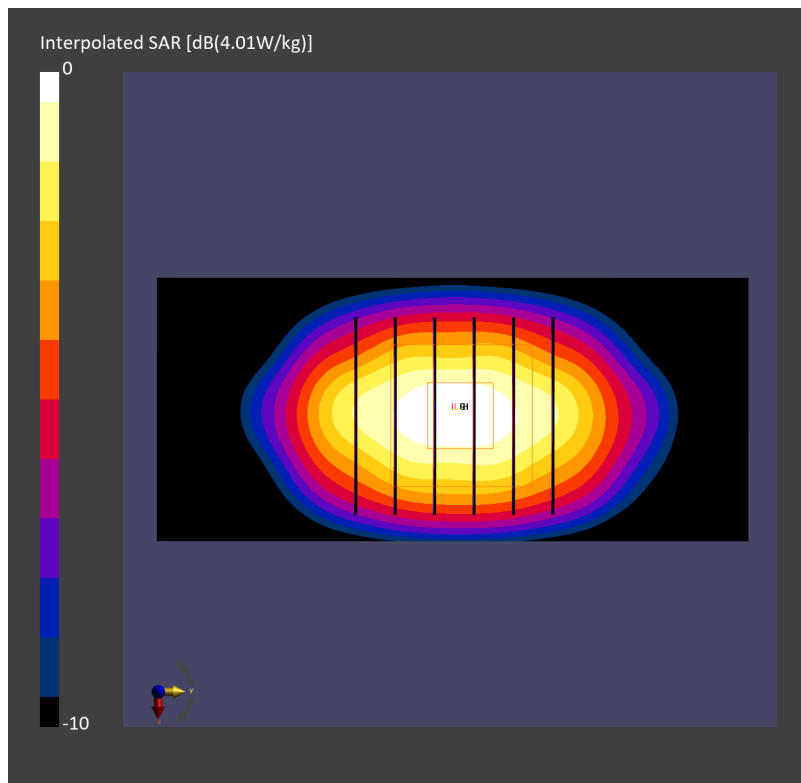

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_240307 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 40.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.7, 7.85, 7.85); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.02 W/kg; SAR (10g) = 1.04 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.99 W/kg; SAR (8g) = 1.14 W/kg; SAR (10g) = 1.05 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.8 %

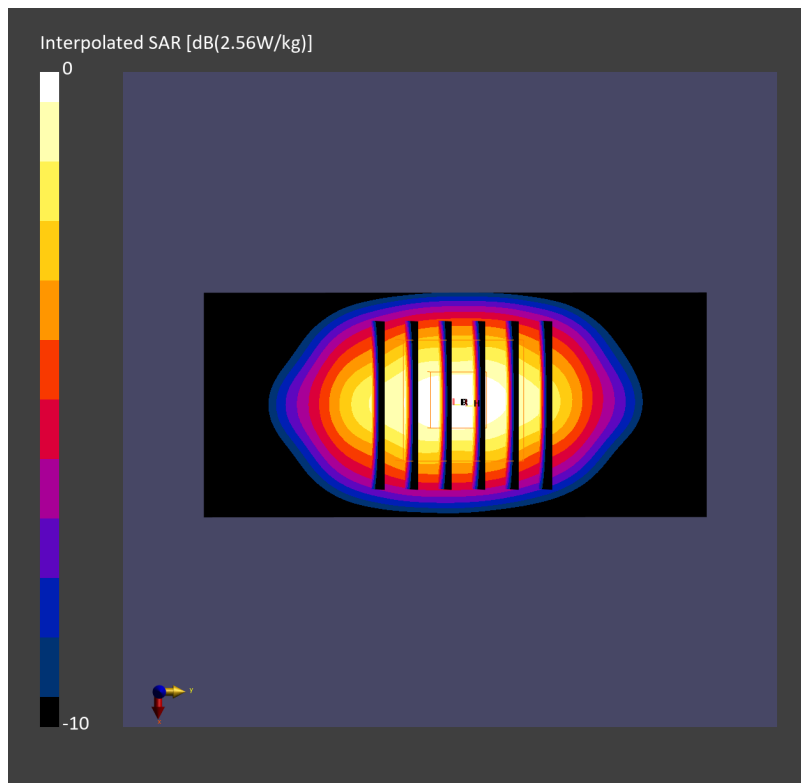

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_240308 Medium parameters used: $f=1900.000$ MHz; $\sigma=1.39$ S/m; $\epsilon_r=40.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7700; ConvF(7.7, 7.85, 7.85); Calibrated: 2024-02-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2145; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.95 W/kg; SAR (10g) = 1.00 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.17 dB

SAR (1g) = 1.78 W/kg; SAR (8g) = 1.02 W/kg; SAR (10g) = 0.939 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.0 %

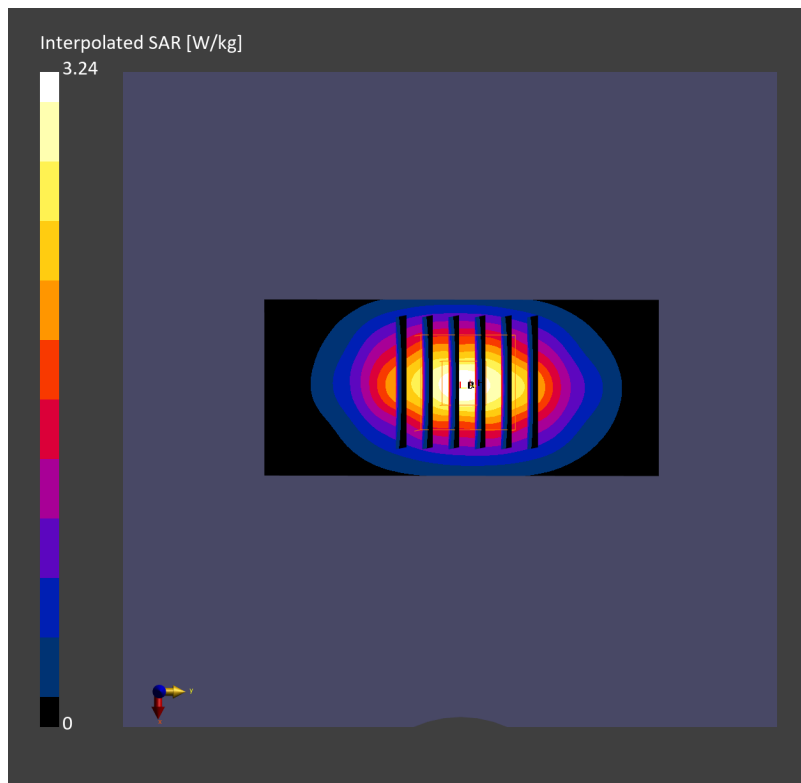

System Check_Head_1900MHz

DUT: D1900V2 - SN5d185

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL_1900_240308 Medium parameters used: $f = 1900.000$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 38.9$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.3, 8.3, 8.3); Calibrated: 2023-10-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1800; Calibrated: 2023-05-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2144; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.82 W/kg; SAR (10g) = 0.933 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 1.87 W/kg; SAR (8g) = 1.07 W/kg; SAR (10g) = 0.980 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 81.4 %

