
ATTACHMENT O: SAR VALIDATION PLOTS

DIGITAL EMC CO., LTD

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:464

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.891 \text{ mho/m}$; $\epsilon_r = 41.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

Probe: ET3DV6 - SN1703; ConvF(6.51, 6.51, 6.51); Calibrated: 2005-03-24; Electronics: DAE3 Sn520

Phantom: SAM with 835MHz; Type: SAM; Serial: TP-1223

Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 145

Test Date: 2005-08-05; Ambient Temp: 22.0; Tissue Temp: 21.7

Dipole Validation


Area Scan (51x101x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Power Drift = -0.047 dB

Peak SAR (extrapolated) = 3.43 W/kg

SAR(1 g) = 2.36 mW/g; SAR(10 g) = 1.53 mW/g

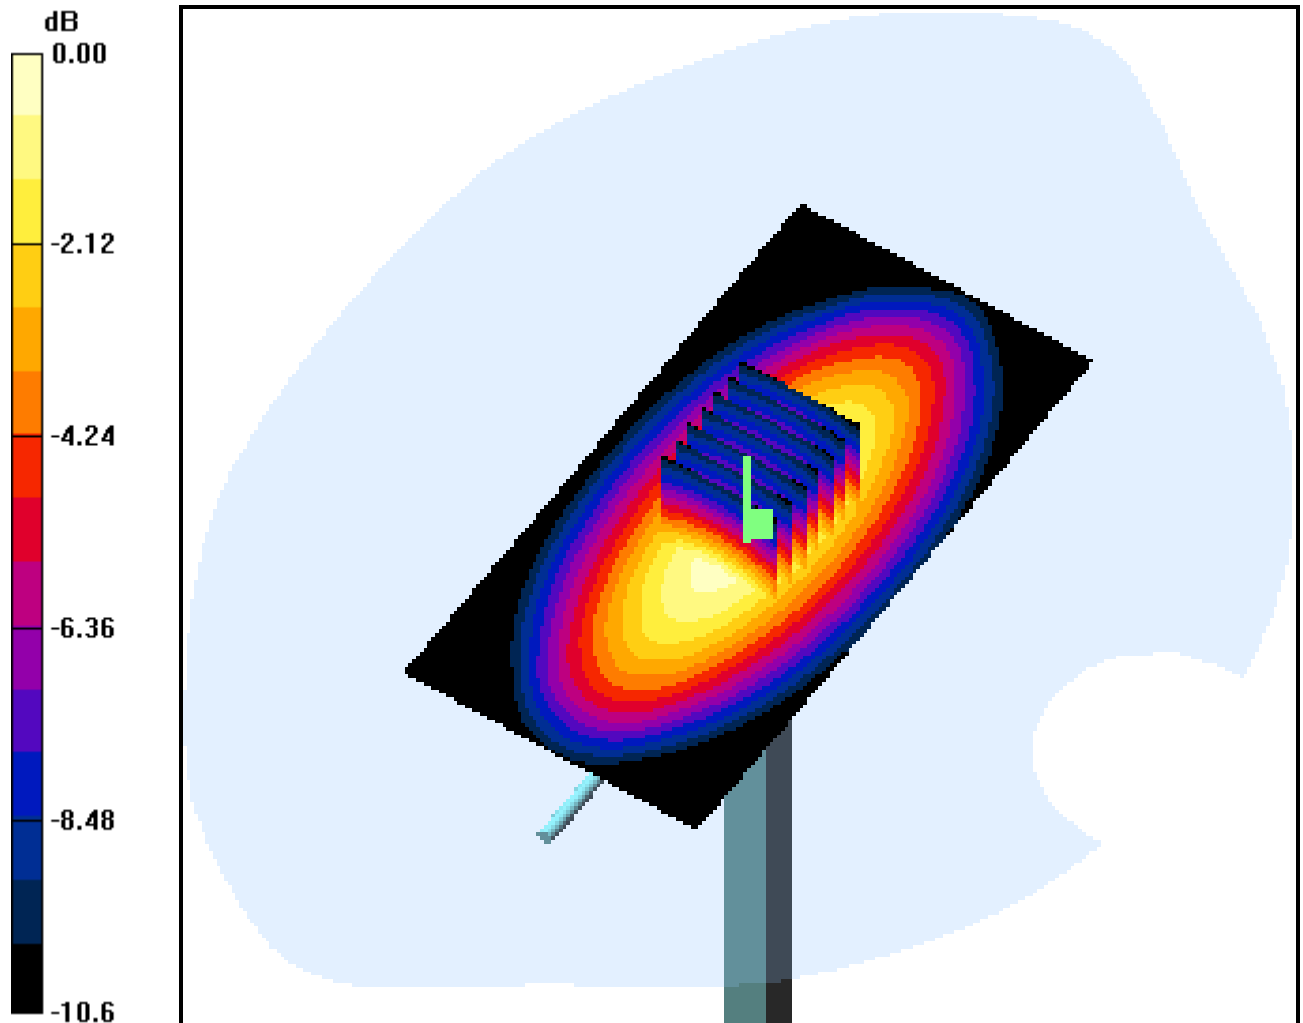

0 dB = 2.55mW/g

DIGITAL EMC CO., LTD

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d029

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 1900 \text{ MHz}$; $\sigma = 1.45 \text{ mho/m}$; $\epsilon_r = 39.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY4 Configuration:

Probe: ET3DV6 - SN1703; ConvF(5.27, 5.27, 5.27); Calibrated: 2005-03-24; Electronics: DAE3 Sn520

Phantom: SAM 1800/1900 MHz; Type: SAM; Serial: TP-1224

Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 145

Test Date: 2005-08-04; Ambient Temp: 22.0; Tissue Temp: 21.5

Dipole Validation


Area Scan (51x71x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Power Drift = -0.044 dB

Peak SAR (extrapolated) = 17.7 W/kg

SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.28 mW/g

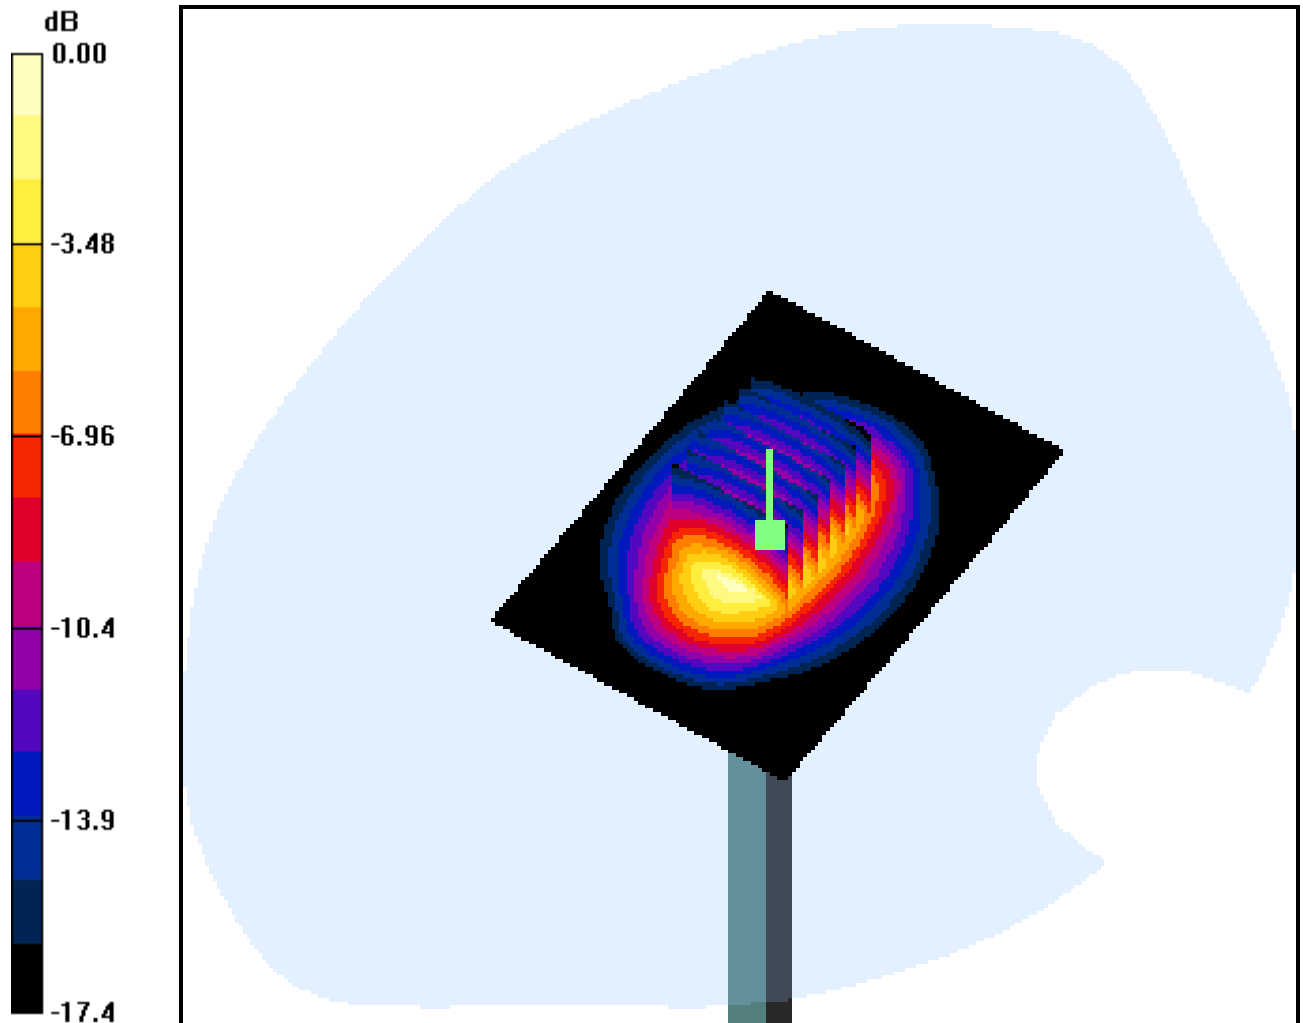

0 dB = 11.4mW/g