




|  |   |   |   |  |
|--|---|---|---|--|
|  | <u>Date(s) of Evaluation</u><br>Oct 5 2015  | <u>Test Report Serial No.</u><br>100115AMW-1334           | <u>Test Report Revision No.</u><br>Rev. 1.1             | <br>Test Lab Certificate No. 2470.01 |
|  | <u>Test Report Issue Date</u><br>Oct 8 2015 | <u>Description of Test(s)</u><br>Specific Absorption Rate | <u>RF Exposure Category</u><br>Gen. Pop. / Uncontrolled |  |

## APPENDIX E - DIPOLE CALIBRATION

|                         |                            |  |  |          |     |            |   |
|-------------------------|----------------------------|--|--|----------|-----|------------|---|
| Applicant:              | Uniden America Corporation |  | FCC ID:                                    | AMWUT653 | IC: | 513C-UT653 |  |
| Model(s):               | Atlantis 150               | DUT Type:  | Portable Marine Band PTT Radio Transceiver |          |     | VHF        |   |
| 2013 Celltech Labs Inc. |                            | This document is not to be reproduced in whole or in part without the prior written permission of Celltech Labs Inc. |  |          |     |            | Page 39 of 41   |



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client **Celltech**

Certificate No: **CLA150-4007\_Jan14/2**

## **CALIBRATION CERTIFICATE (Replacement of No: CLA150-4007\_Jan14)**

Object **CLA150 - SN: 4007**

Calibration procedure(s) **QA CAL-15.v8**  
**Calibration procedure for system validation sources below 700 MHz**

Calibration date: **January 24, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter E4419B          | GB41293874         | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Power sensor E4412A         | MY41498087         | 04-Apr-13 (No. 217-01733)         | Apr-14                 |
| Reference 3 dB Attenuator   | SN: S5054 (3c)     | 04-Apr-13 (No. 217-01737)         | Apr-14                 |
| Reference 20 dB Attenuator  | SN: S5058 (20k)    | 04-Apr-13 (No. 217-01736)         | Apr-14                 |
| Type-N mismatch combination | SN: 5047.3 / 06327 | 04-Apr-13 (No. 217-01739)         | Apr-14                 |
| Reference Probe EX3DV4      | SN: 3877           | 06-Jan-14 (No. EX3-3877_Jan14)    | Jan-15                 |
| DAE4                        | SN: 654            | 18-Jul-13 (No. DAE4-654_Jul13)    | Jul-14                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C       | US3642U01700       | 04-Aug-99 (in house check Apr-13) | In house check: Apr-16 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |

Calibrated by: **Israe El-Naouq**      Name: **Israe El-Naouq**      Function: **Laboratory Technician**

Approved by: **Katja Pokovic**      Name: **Katja Pokovic**      Function: **Technical Manager**

Signature

Issued: April 14, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2013
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- c) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                      |                        |                                 |
|----------------------|------------------------|---------------------------------|
| DASY Version         | DASY5                  | V52.8.7                         |
| Extrapolation        | Advanced Extrapolation |                                 |
| Phantom              | ELI4 Flat Phantom      | Shell thickness: $2 \pm 0.2$ mm |
| EUT Positioning      | Touch Position         |                                 |
| Zoom Scan Resolution | dx, dy, dz = 5.0 mm    |                                 |
| Frequency            | 150 MHz $\pm$ 1 MHz    |                                 |

## Head TSL parameters

The following parameters and calculations were applied.

|   | Temperature         | Permittivity   | Conductivity         |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 52.3           | 0.76 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 50.5 $\pm$ 6 % | 0.76 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|   |                  |                              |
|---|------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition        |                              |
| SAR measured  | 1 W input power  | 3.89 W/kg                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W | 3.86 W/kg $\pm$ 18.4 % (k=2) |

|   |                  |                              |
|---|------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition        |                              |
| SAR measured  | 1 W input power  | 2.57 W/kg                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W | 2.55 W/kg $\pm$ 18.0 % (k=2) |

## Body TSL parameters

The following parameters and calculations were applied.

|   | Temperature         | Permittivity   | Conductivity         |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 61.9           | 0.80 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 62.8 $\pm$ 6 % | 0.80 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|   |                  |                              |
|---|------------------|------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition        |                              |
| SAR measured  | 1 W input power  | 3.89 W/kg                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W | 3.90 W/kg $\pm$ 18.4 % (k=2) |

|   |                  |                              |
|---|------------------|------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition        |                              |
| SAR measured  | 1 W input power  | 2.59 W/kg                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W | 2.60 W/kg $\pm$ 18.0 % (k=2) |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 43.1 $\Omega$ - 7.3 j $\Omega$ |
| Return Loss                          | - 19.4 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 46.9 $\Omega$ - 9.2 j $\Omega$ |
| Return Loss                          | - 20.0 dB                      |

### Additional EUT Data

|                 |                   |
|-----------------|-------------------|
| Manufactured by | SPEAG             |
| Manufactured on | December 12, 2013 |



## DASY5 Validation Report for Head TSL

Date: 24.01.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4007**

Communication System: UID 0 - CW; Frequency: 150 MHz

Medium parameters used:  $f = 150 \text{ MHz}$ ;  $\sigma = 0.76 \text{ S/m}$ ;  $\epsilon_r = 50.5$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(11.76, 11.76, 11.76); Calibrated: 06.01.2014;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 18.07.2013
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

### CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan

**(81x81x1):** Interpolated grid:  $dx=1.500 \text{ mm}$ ,  $dy=1.500 \text{ mm}$

Maximum value of SAR (interpolated) =  $5.02 \text{ W/kg}$

### CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan


**(7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value =  $81.695 \text{ V/m}$ ; Power Drift =  $-0.04 \text{ dB}$

Peak SAR (extrapolated) =  $6.28 \text{ W/kg}$


**SAR(1 g) =  $3.89 \text{ W/kg}$ ; SAR(10 g) =  $2.57 \text{ W/kg}$**

Maximum value of SAR (measured) =  $5.03 \text{ W/kg}$

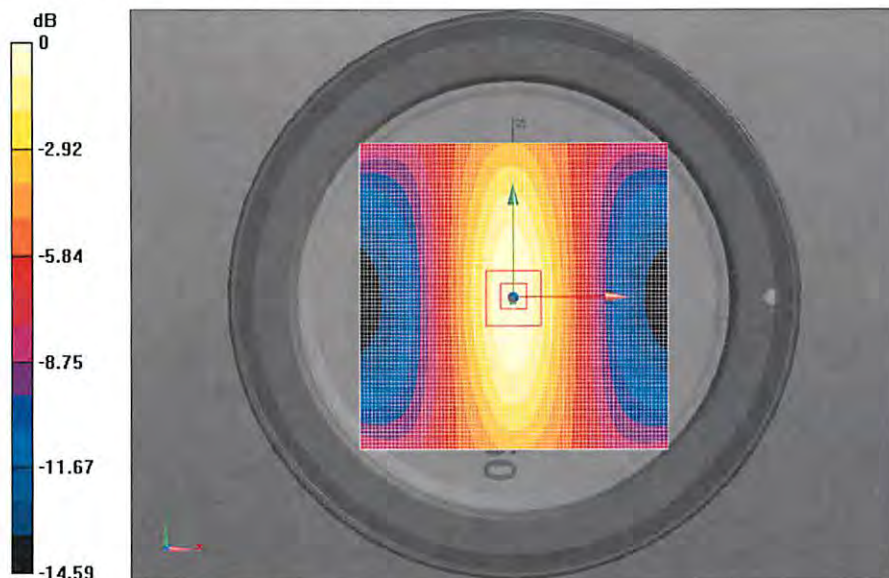

0 dB =  $5.02 \text{ W/kg}$  =  $7.01 \text{ dBW/kg}$

Impedance Measurement Plot for Head TSL

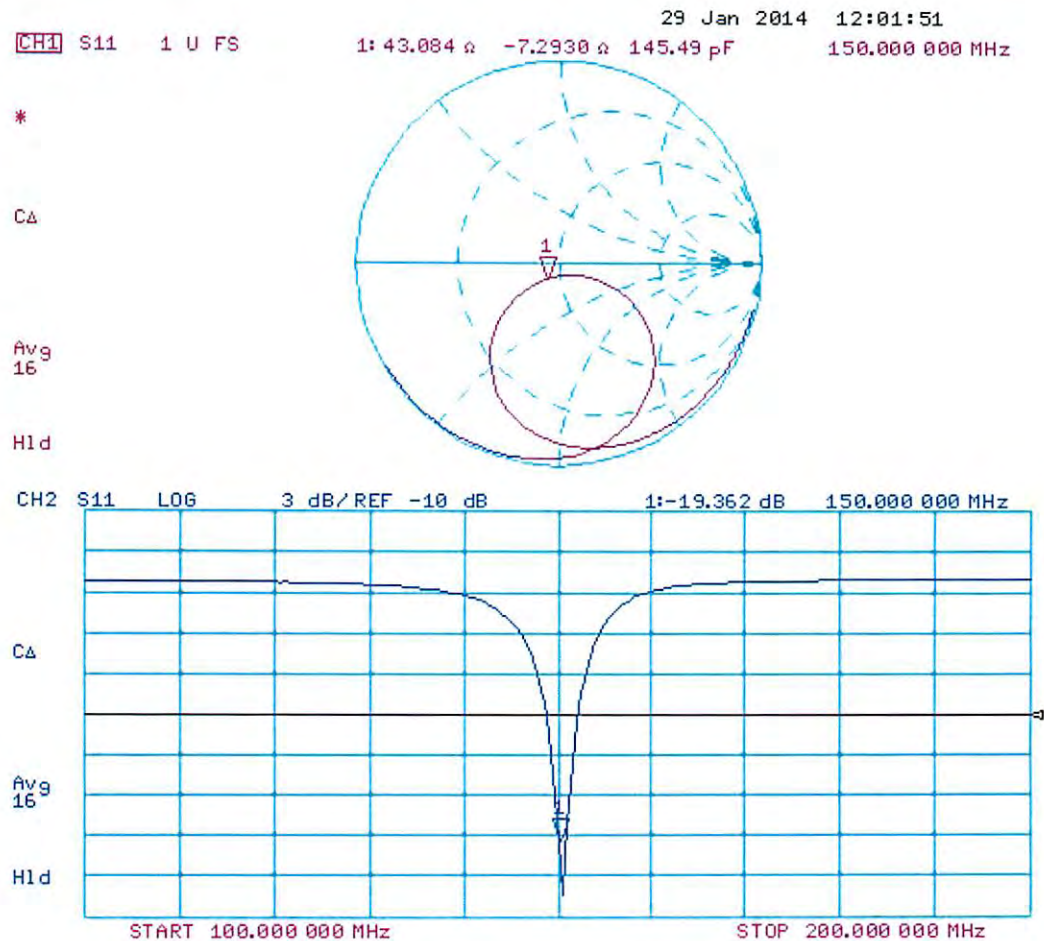



## DASY5 Validation Report for Body TSL

Date: 24.01.2014

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4007**

Communication System: UID 0 - CW; Frequency: 150 MHz

Medium parameters used:  $f = 150$  MHz;  $\sigma = 0.799$  S/m;  $\epsilon_r = 62.757$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(11.45, 11.45, 11.45); Calibrated: 06.01.2014;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 18.07.2013
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

### CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan

**(81x81x1):** Interpolated grid:  $dx=1.500$  mm,  $dy=1.500$  mm

Maximum value of SAR (interpolated) = 5.00 W/kg

### CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan


**(7x7x7)/Cube 0:** Measurement grid:  $dx=5$ mm,  $dy=5$ mm,  $dz=5$ mm

Reference Value = 79.120 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 6.25 W/kg

**SAR(1 g) = 3.89 W/kg; SAR(10 g) = 2.59 W/kg**


Maximum value of SAR (measured) = 5.02 W/kg

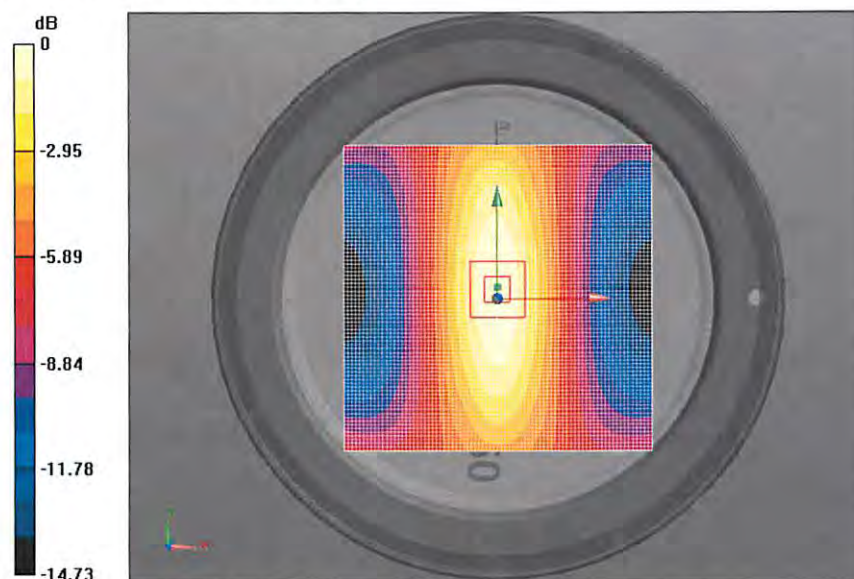



0 dB = 5.00 W/kg = 6.99 dBW/kg

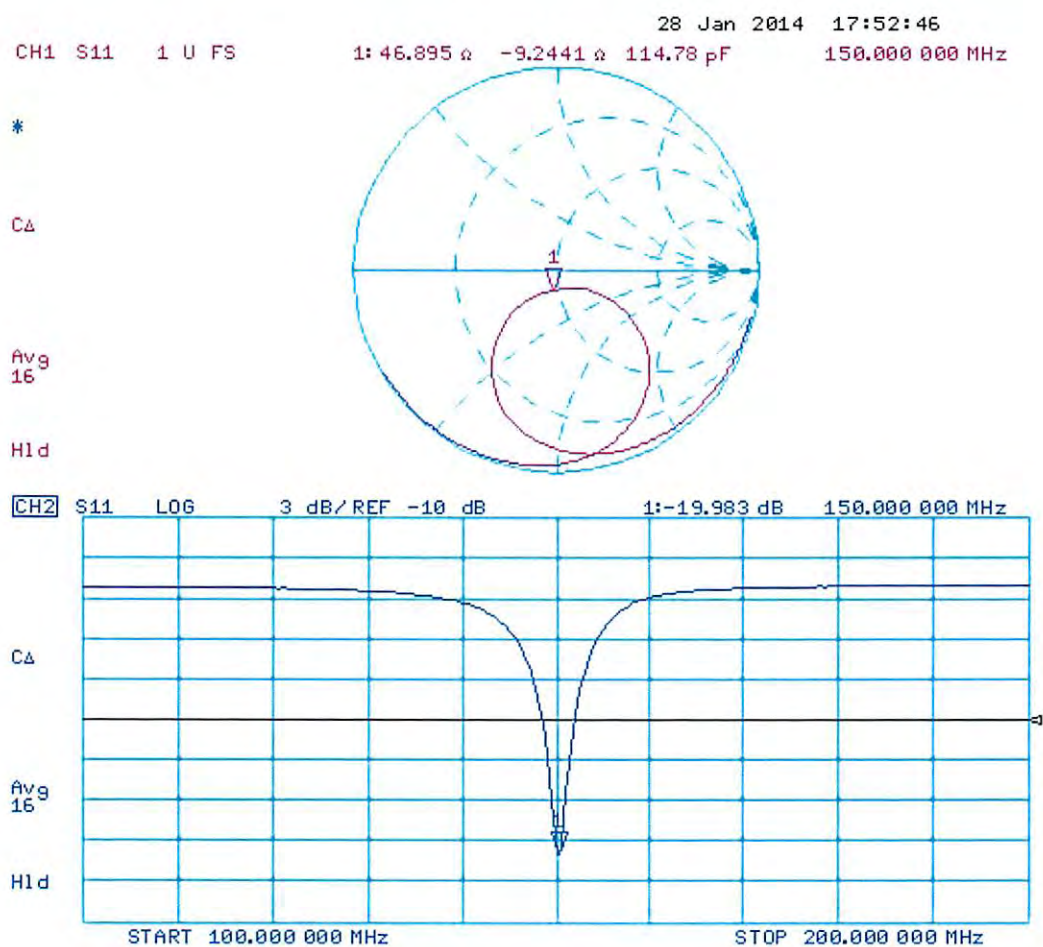


## Impedance Measurement Plot for Body TSL



|  |   |   |   |  |
|--|---|---|---|--|
|  | <u>Date(s) of Evaluation</u><br>Oct 5 2015  | <u>Test Report Serial No.</u><br>100115AMW-1334           | <u>Test Report Revision No.</u><br>Rev. 1.1             | <br>Test Lab Certificate No. 2470.01 |
|  | <u>Test Report Issue Date</u><br>Oct 8 2015 | <u>Description of Test(s)</u><br>Specific Absorption Rate | <u>RF Exposure Category</u><br>Gen. Pop. / Uncontrolled |  |

## APPENDIX F - PROBE CALIBRATION

|                         |                            |  |  |          |     |            |   |
|-------------------------|----------------------------|--|--|----------|-----|------------|---|
| Applicant:              | Uniden America Corporation |  | FCC ID:                                    | AMWUT653 | IC: | 513C-UT653 |  |
| Model(s):               | Atlantis 150               | DUT Type:  | Portable Marine Band PTT Radio Transceiver |          |     | VHF        |   |
| 2013 Celltech Labs Inc. |                            | This document is not to be reproduced in whole or in part without the prior written permission of Celltech Labs Inc. |  |          |     |            | Page 40 of 41   |



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 0108

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client **Celltech**

Certificate No: EX3-3600\_Apr15

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3600**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,  
QA CAL-25.v6  
Calibration procedure for dosimetric E-field probes**

Calibration date: **April 23, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 01-Apr-15 (No. 217-02128)         | Mar-16                 |
| Power sensor E4412A        | MY41498087      | 01-Apr-15 (No. 217-02128)         | Mar-16                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 01-Apr-15 (No. 217-02129)         | Mar-16                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 01-Apr-15 (No. 217-02132)         | Mar-16                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 01-Apr-15 (No. 217-02133)         | Mar-16                 |
| Reference Probe ES3DV2     | SN: 3013        | 30-Dec-14 (No. ES3-3013_Dec14)    | Dec-15                 |
| DAE4                       | SN: 660         | 14-Jan-15 (No. DAE4-660_Jan15)    | Jan-16                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-16 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-14) | In house check: Oct-15 |

|   | Name          | Function              | Signature              |
|---|---------------|-----------------------|------------------------|
| Calibrated by:  | Israe Elnaouq | Laboratory Technician |                        |
| Approved by:  | Katja Pokovic | Technical Manager     |                        |
|   |               |                       | Issued: April 25, 2015 |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |               |                       |                        |





Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                          |   |
|--------------------------|---|
| TSL                      | tissue simulating liquid  |
| NORM <sub>x,y,z</sub>    | sensitivity in free space   |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>  |
| DCP                      | diode compression point   |
| CF                       | crest factor (1/duty_cycle) of the RF signal  |
| A, B, C, D               | modulation dependent linearization parameters   |
| Polarization $\varphi$   | $\varphi$ rotation around probe axis  |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |
| Connector Angle          | information used in DASY system to align probe sensor X to the robot coordinate system  |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the  $E^2$ -field uncertainty inside TSL (see below *ConvF*).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).



# Probe EX3DV4

## SN:3600

Manufactured: January 10, 2007  
Calibrated: April 23, 2015

**Calibrated for DASY/EASY Systems**  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3600

### Basic Calibration Parameters

|   | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|---|----------|----------|----------|-----------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 0.49     | 0.49     | 0.41     | ± 10.1 %  |
| DCP (mV) <sup>B</sup>                                     | 98.1     | 100.9    | 98.6     |           |

### Modulation Calibration Parameters

| UID | Communication System Name |   | A<br>dB | B<br>dB/ $\mu\text{V}$ | C   | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-----|---------------------------|---|---------|------------------------|-----|---------|----------|---------------------------|
| 0   | CW                        | X | 0.0     | 0.0                    | 1.0 | 0.00    | 151.4    | ±2.7 %                    |
|     |                           | Y | 0.0     | 0.0                    | 1.0 |         | 158.5    |                           |
|     |                           | Z | 0.0     | 0.0                    | 1.0 |         | 152.6    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3600

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 150                  | 52.3                               | 0.76                            | 9.42    | 9.42    | 9.42    | 0.00               | 1.00                    | ± 13.3 %    |
| 300                  | 45.3                               | 0.87                            | 9.10    | 9.10    | 9.10    | 0.10               | 1.70                    | ± 13.3 %    |
| 450                  | 43.5                               | 0.87                            | 9.03    | 9.03    | 9.03    | 0.18               | 1.70                    | ± 13.3 %    |
| 835                  | 41.5                               | 0.90                            | 7.94    | 7.94    | 7.94    | 0.33               | 1.15                    | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 6.70    | 6.70    | 6.70    | 0.30               | 0.80                    | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 6.06    | 6.06    | 6.06    | 0.40               | 0.81                    | ± 12.0 %    |
| 5250                 | 35.9                               | 4.71                            | 4.55    | 4.55    | 4.55    | 0.35               | 1.80                    | ± 13.1 %    |
| 5600                 | 35.5                               | 5.07                            | 4.10    | 4.10    | 4.10    | 0.40               | 1.80                    | ± 13.1 %    |
| 5750                 | 35.4                               | 5.22                            | 4.21    | 4.21    | 4.21    | 0.40               | 1.80                    | ± 13.1 %    |

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3600

### Calibration Parameter Determined in Body Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 150                  | 61.9                               | 0.80                            | 8.94    | 8.94    | 8.94    | 0.00               | 1.00                    | ± 13.3 %    |
| 300                  | 58.2                               | 0.92                            | 8.89    | 8.89    | 8.89    | 0.08               | 1.20                    | ± 13.3 %    |
| 450                  | 56.7                               | 0.94                            | 8.80    | 8.80    | 8.80    | 0.09               | 1.10                    | ± 13.3 %    |
| 835                  | 55.2                               | 0.97                            | 7.73    | 7.73    | 7.73    | 0.21               | 1.50                    | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 6.49    | 6.49    | 6.49    | 0.31               | 0.94                    | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 6.19    | 6.19    | 6.19    | 0.33               | 0.80                    | ± 12.0 %    |
| 5250                 | 48.9                               | 5.36                            | 3.87    | 3.87    | 3.87    | 0.50               | 1.90                    | ± 13.1 %    |
| 5600                 | 48.5                               | 5.77                            | 3.25    | 3.25    | 3.25    | 0.55               | 1.90                    | ± 13.1 %    |
| 5750                 | 48.3                               | 5.94                            | 3.60    | 3.60    | 3.60    | 0.55               | 1.90                    | ± 13.1 %    |

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



## Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

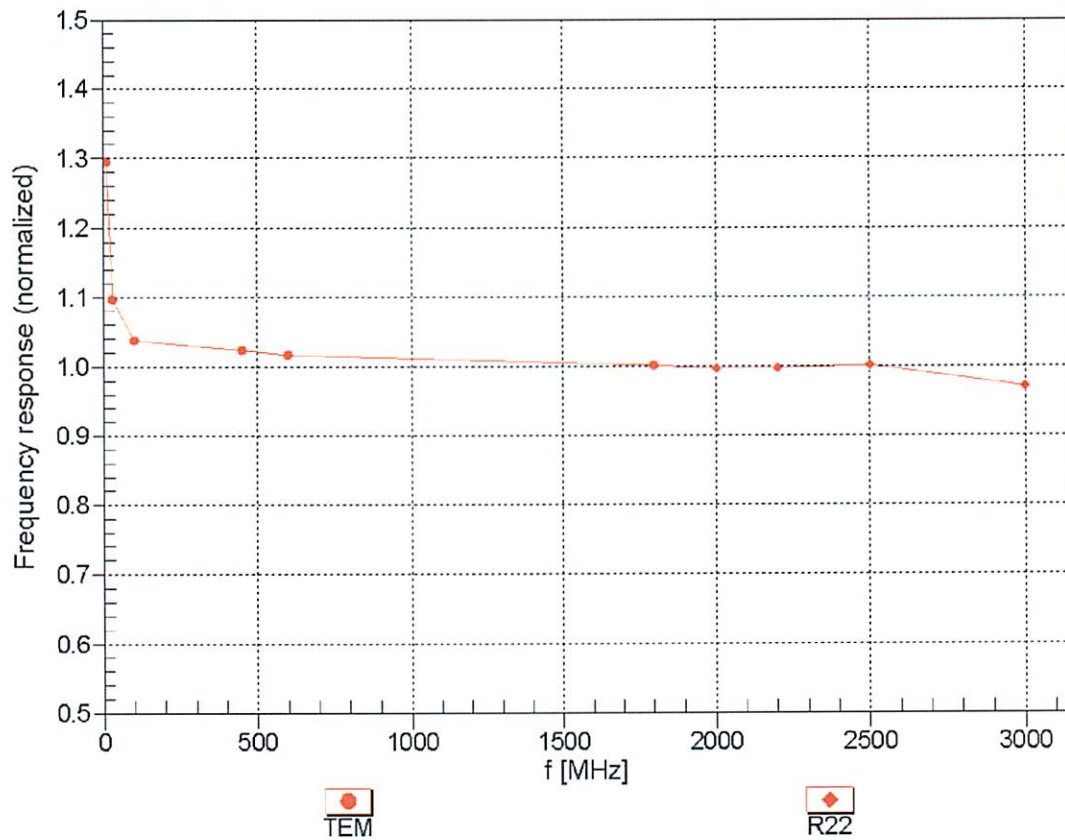



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$

f=600 MHz,TEM

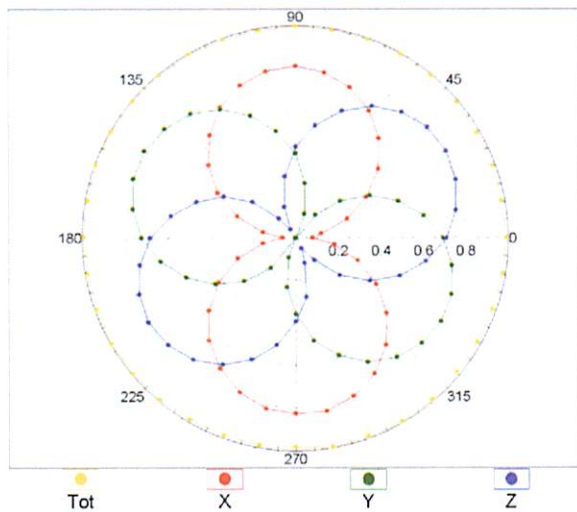


f=1800 MHz,R22

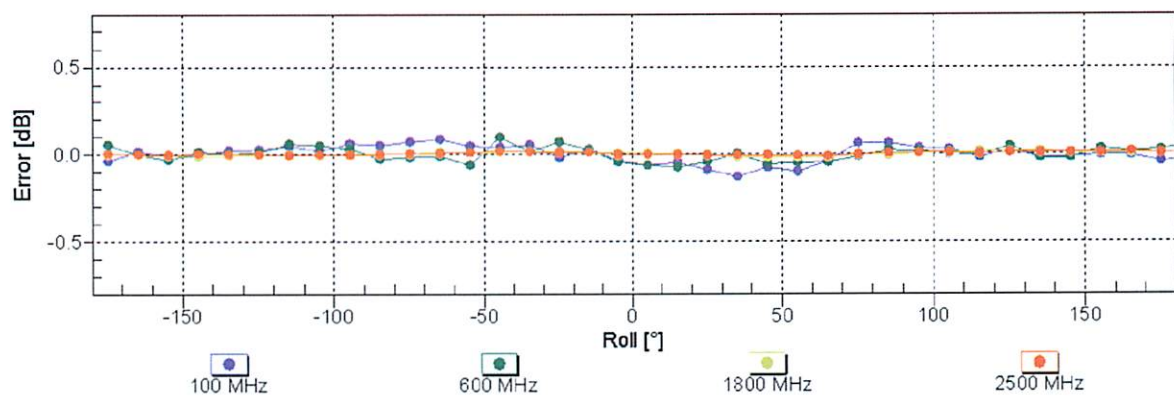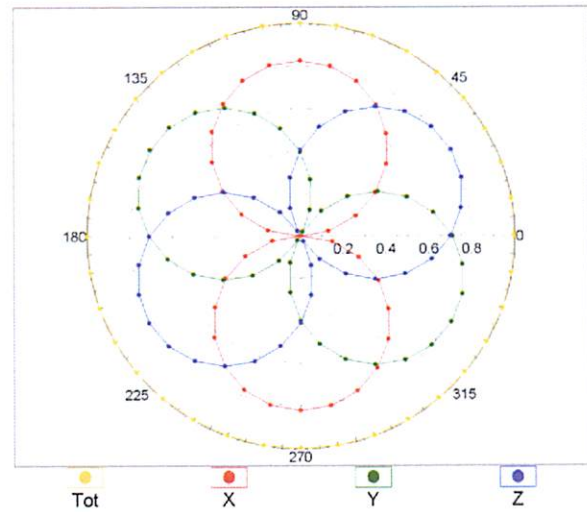

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )


## Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f_{\text{eval}} = 1900 \text{ MHz}$ )

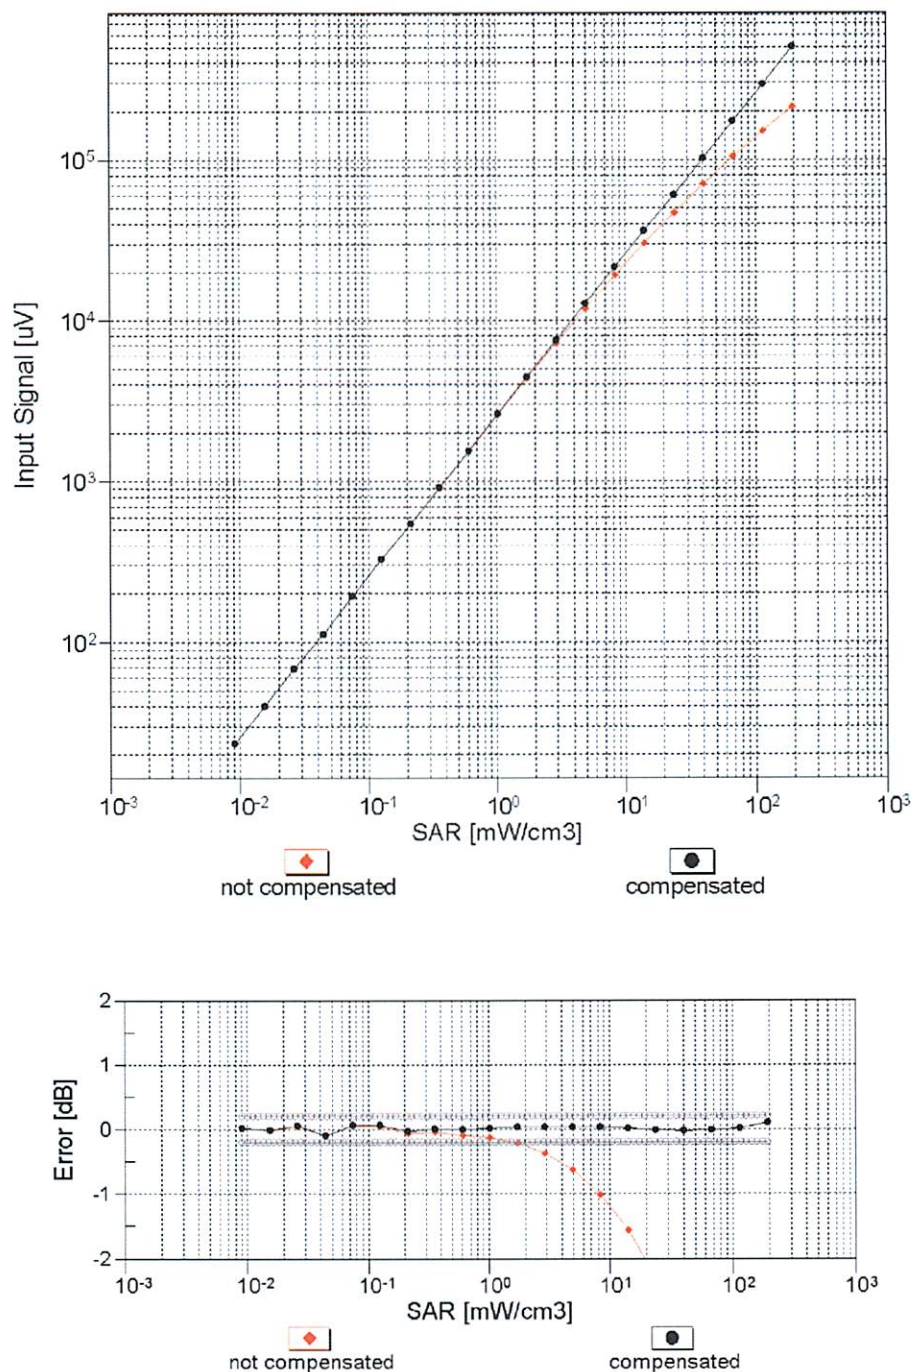

Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )





## Conversion Factor Assessment

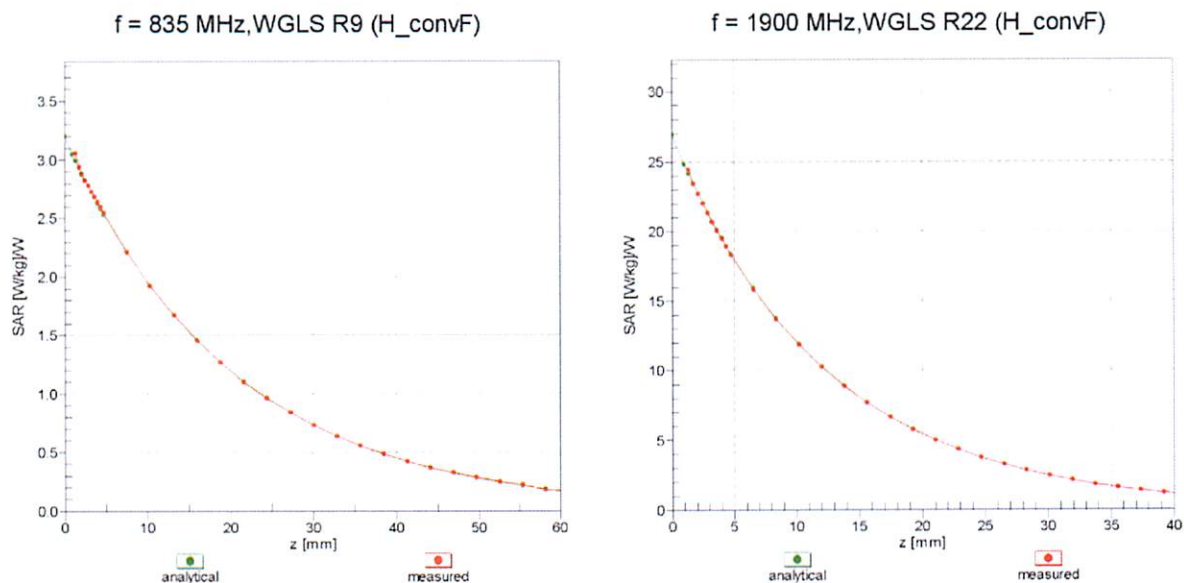

## Deviation from Isotropy in Liquid

Error ( $\phi, \vartheta$ ),  $f = 900 \text{ MHz}$

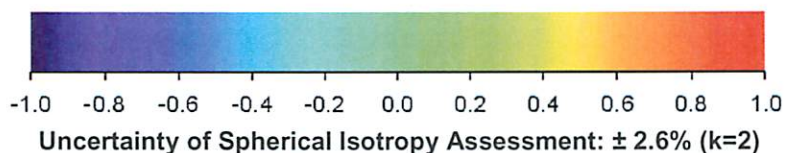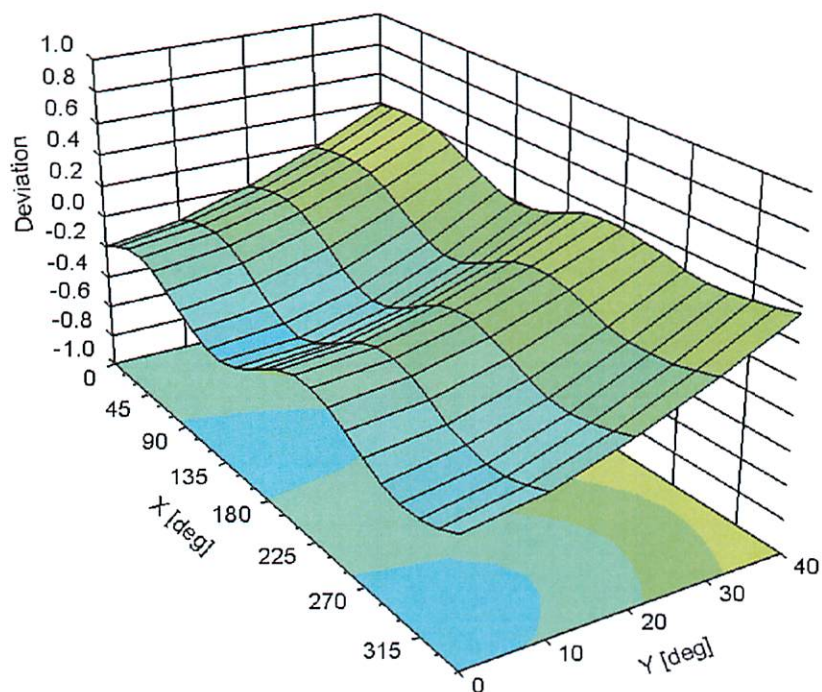



Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )



## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3600


### Other Probe Parameters

|   |            |
|---|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | 35.3       |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 9 mm       |
| Tip Diameter                                  | 2.5 mm     |
| Probe Tip to Sensor X Calibration Point       | 1 mm       |
| Probe Tip to Sensor Y Calibration Point       | 1 mm       |
| Probe Tip to Sensor Z Calibration Point       | 1 mm       |
| Recommended Measurement Distance from Surface | 1.4 mm     |

|  |   |   |   |  |
|--|---|---|---|--|
|  | <u>Date(s) of Evaluation</u><br>Oct 5 2015  | <u>Test Report Serial No.</u><br>100115AMW-1334           | <u>Test Report Revision No.</u><br>Rev. 1.1             |  |
|  | <u>Test Report Issue Date</u><br>Oct 8 2015 | <u>Description of Test(s)</u><br>Specific Absorption Rate | <u>RF Exposure Category</u><br>Gen. Pop. / Uncontrolled |  |

Test Lab Certificate No. 2470.01

## APPENDIX G - ELI PHANTOM CERTIFICATE OF CONFORMITY

|                         |                                   |  |   |                 |            |                   |   |
|-------------------------|-----------------------------------|--|---|-----------------|------------|-------------------|---|
| <b>Applicant:</b>       | <b>Uniden America Corporation</b> |  | <b>FCC ID:</b>                                    | <b>AMWUT653</b> | <b>IC:</b> | <b>513C-UT653</b> |  |
| <b>Model(s):</b>        | <b>Atlantis 150</b>               | <b>DUT Type:</b>   | <b>Portable Marine Band PTT Radio Transceiver</b> |                 |            | <b>VHF</b>        |   |
| 2013 Celltech Labs Inc. |                                   | This document is not to be reproduced in whole or in part without the prior written permission of Celltech Labs Inc. |   |                 |            |                   | Page 41 of 41   |

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Certificate of Conformity / First Article Inspection

|              |   |
|--------------|---|
| Item         | Oval Flat Phantom ELI 5.0   |
| Type No      | QD OVA 002 A  |
| Series No    | 1108 and higher   |
| Manufacturer | Untersee Composites<br>Knebelstrasse 8, CH-8268 Mannenbach, Switzerland |

### Tests

Complete tests were made on the prototype units QD OVA 001 A, pre-series units QD OVA 001 B as well as on some series units QD OVA 001 B. Some tests are made on all series units QD OVA 002 A.

| Test                 | Requirement   | Details  | Units tested              |
|----------------------|---|--|---------------------------|
| Shape                | Internal dimensions, depth and sagging are compatible with standards                | Bottom elliptical 600 x 400 mm, Depth 190 mm, dimension compliant with [1] for $f > 375$ MHz | Prototypes                |
| Material thickness   | Bottom: 2.0mm +/- 0.2mm   | dimension compliant with [3] for $f > 800$ MHz   | all                       |
| Material parameters  | rel. permittivity 2 – 5, loss tangent $\leq 0.05$ , at $f \leq 6$ GHz               | rel. permittivity 3.5 +/- 0.5 loss tangent $\leq 0.05$                                       | Material samples          |
| Material resistivity | Compatibility with tissue simulating liquids .                                      | Compatible with SPEAG liquids. **  | Phantoms, Material sample |
| Sagging              | Sagging of the flat section in tolerance when filled with tissue simulating liquid. | within tolerance for filling height up to 155 mm   | Prototypes, samples       |

\*\* Note: Compatibility restrictions apply certain liquid components mentioned in the standard, containing e.g. DGBE, DGMHE or Triton X-100. Observe technical note on material compatibility.

### Standards

- [1] OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Edition 01-01
- [2] IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003
- [3] IEC 62209–1 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", 2005-02-18
- [4] IEC 62209–2 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", 2010-03-30

### Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of **body-worn** SAR measurements and system performance checks as specified in [1 – 4] and further standards.

Date 25.7.2011

Signature / Stamp

**s p e a g**

Schmid & Partner Engineering AG  
 Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com