

NCL CALIBRATION LABORATORIES

Calibration File No: DC-515
Project Number: WISB-ALSAS10U-5121

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

WISB Validation Dipole

Manufacturer: APREL Laboratories

Part number: ALS-D-5800-S-2

Frequency: 5800 MHz

Serial No: 5800-240-00852

Customer: WISB

Calibrated: 4th March 2005
Released on: 4th March 2005

Released By: _____

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4162


Conditions

Dipole 5800-240-00852 was new and taken from stock prior to calibration.


Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

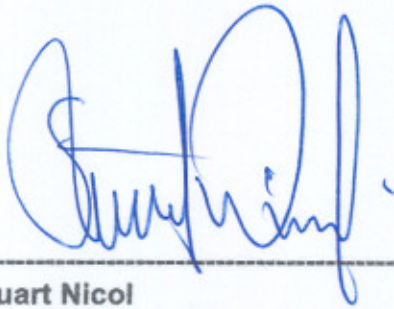

Stuart Nicol
Director Product Development

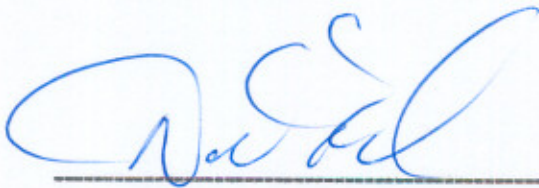

D. Brooks
Member of Engineering Staff
(Calibration Engineer)

Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions

Length: 21.6 mm

Height: 12.6 mm

Electrical Specification


SWR: 1.34 U

Return Loss: -17.0 dB

Impedance: 58.5 Ω

System Validation Results

| Frequency | 1 Gram | 10 Gram | Peak |
|-----------|--------|---------|-------|
| 5800 MHz | 58.3 | 18 | 207.1 |

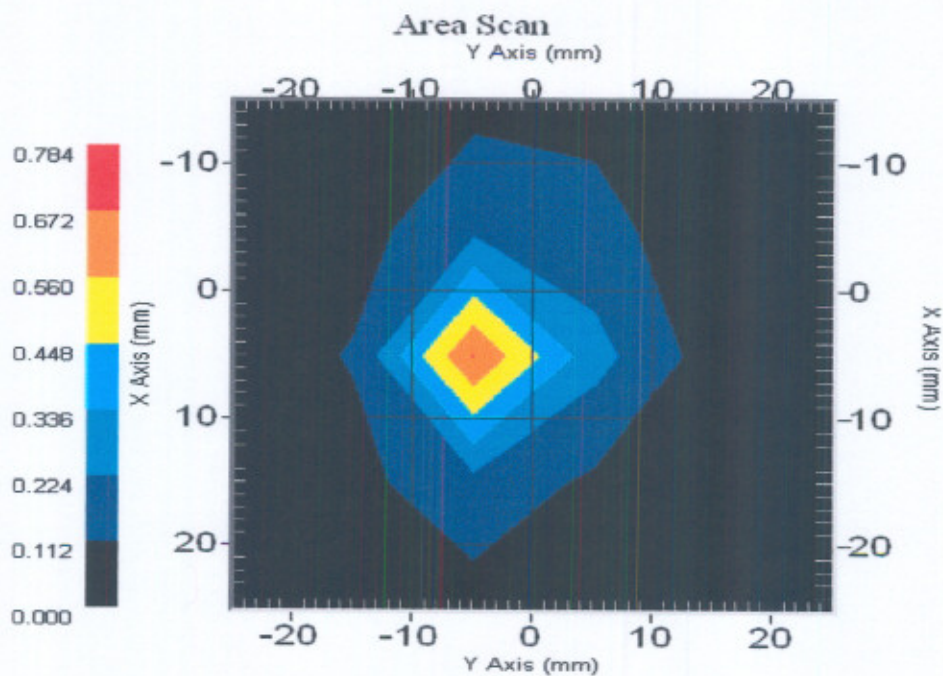

Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 5800-240-00852. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-020 130 MHz to 26 GHz E-Field Probe Serial Number 212.

References

SSI-TP-018-ALSAS Dipole Calibration Procedure

SSI-TP-016 Tissue Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

Conditions

Dipole 5800-240-00852 was new taken from stock.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 20 °C +/- 0.5°C

Dipole Calibration Results

Mechanical Verification

| APREL Length | APREL Height | Measured Length | Measured Height |
|--------------|--------------|-----------------|-----------------|
| 21.6 mm | 12.6 mm | 21.6 mm | 14.7 mm |

Tissue Validation

| Head Tissue 5800 MHz | Measured |
|-----------------------------------|----------|
| Dielectric constant, ϵ_r | 35.3 |
| Conductivity, σ [S/m] | 5.3 |

NCL Calibration Laboratories

Division of APREL Laboratories.

Electrical Calibration

| Test | Result |
|-----------|---------------|
| S11 R/L | -17.0 dB |
| SWR | 1.34 U |
| Impedance | 58.5 Ω |

The Following Graphs are the results as displayed on the Vector Network Analyzer.


S11 Parameter Return Loss

S22 REVERSE REFLECTION

LOG MAGNITUDE

REF = -15.000 dB

1.000 dB/DIV

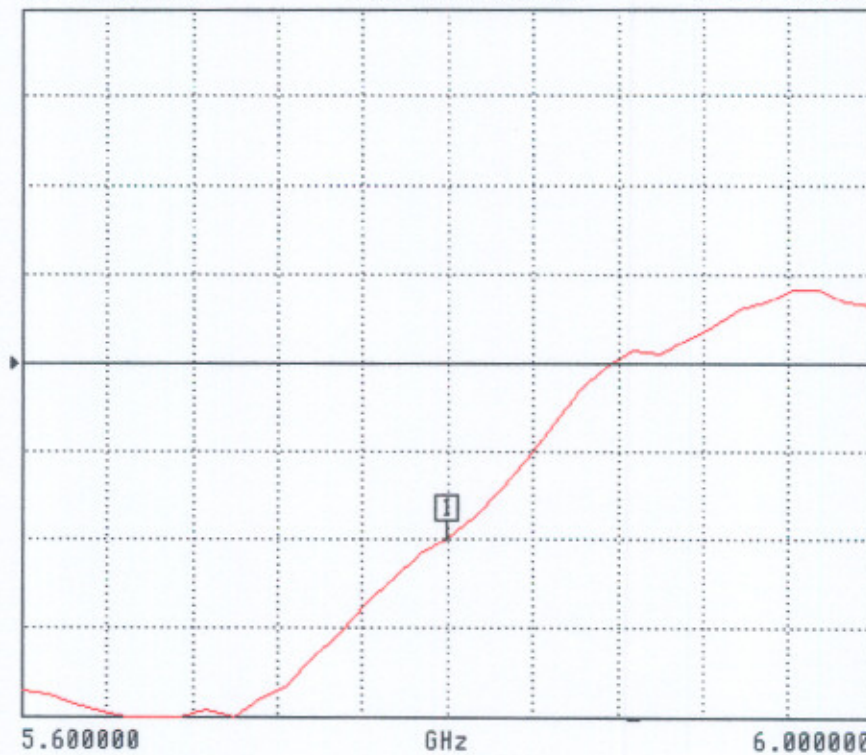

This page has been reviewed for content and attested to by signature within this document.


SWR

S22 REVERSE REFLECTION

SWR

REF=1.350 U

50.000 mU/DIV

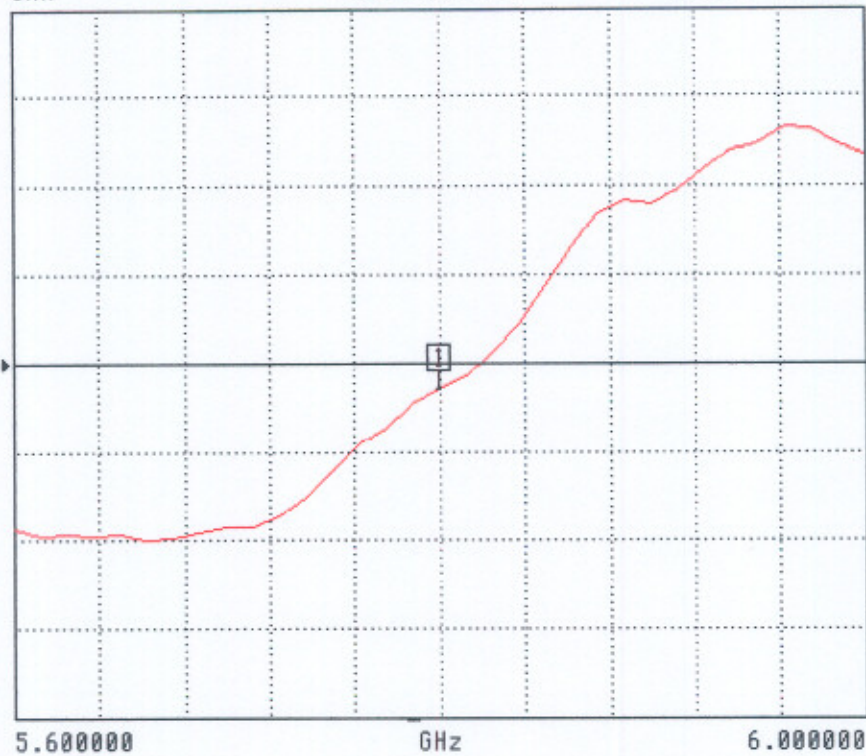

CH 4 - S22
REFERENCE PLANE
0.0000 mm


MARKER 1
5.800000 GHz
1.335 U

MARKER TO MAX
▶ MARKER TO MIN

MARKER READOUT
FUNCTIONS

Smith Chart Dipole Impedance

S22 REVERSE REFLECTION
IMPEDANCE

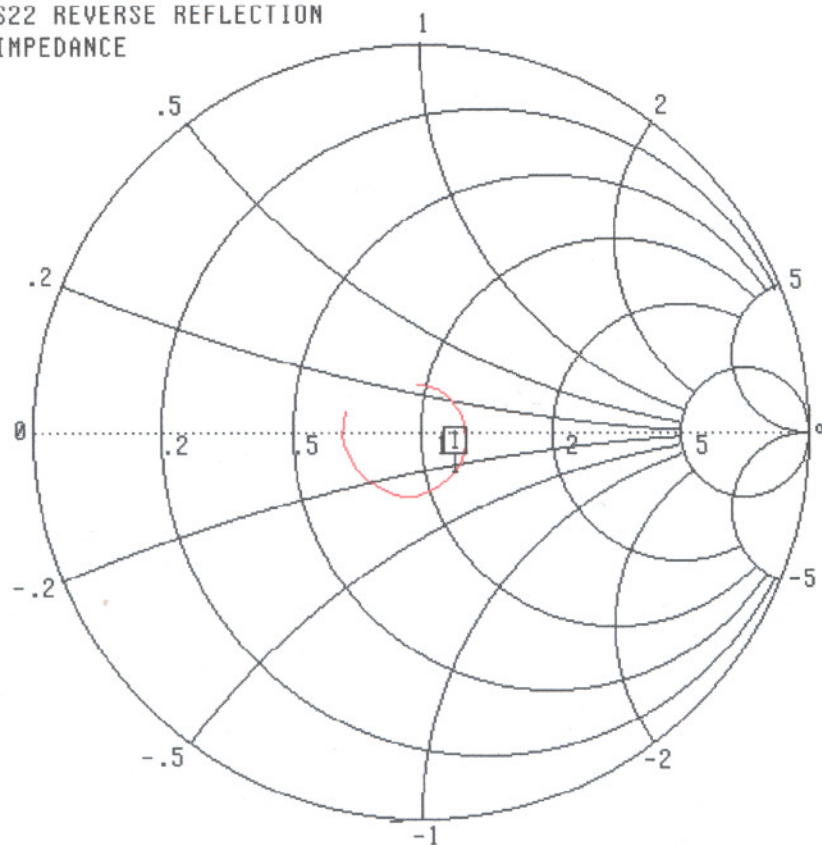

5.600000 - 6.000000 GHz

CH 4 - S22
REFERENCE PLANE
0.0000 mm


MARKER 1
5.800000 GHz
58.509 Ω
-12.692 $j\Omega$

MARKER TO MAX
▶ MARKER TO MIN

MARKER READOUT
FUNCTIONS

System Validation Results Using the Electrically Calibrated Dipole

| Head Tissue Frequency | 1 Gram | 10 Gram | Peak Above Feed Point |
|-----------------------|--------|---------|-----------------------|
| 5800 MHz | 58.3 | 18 | 207.1 |

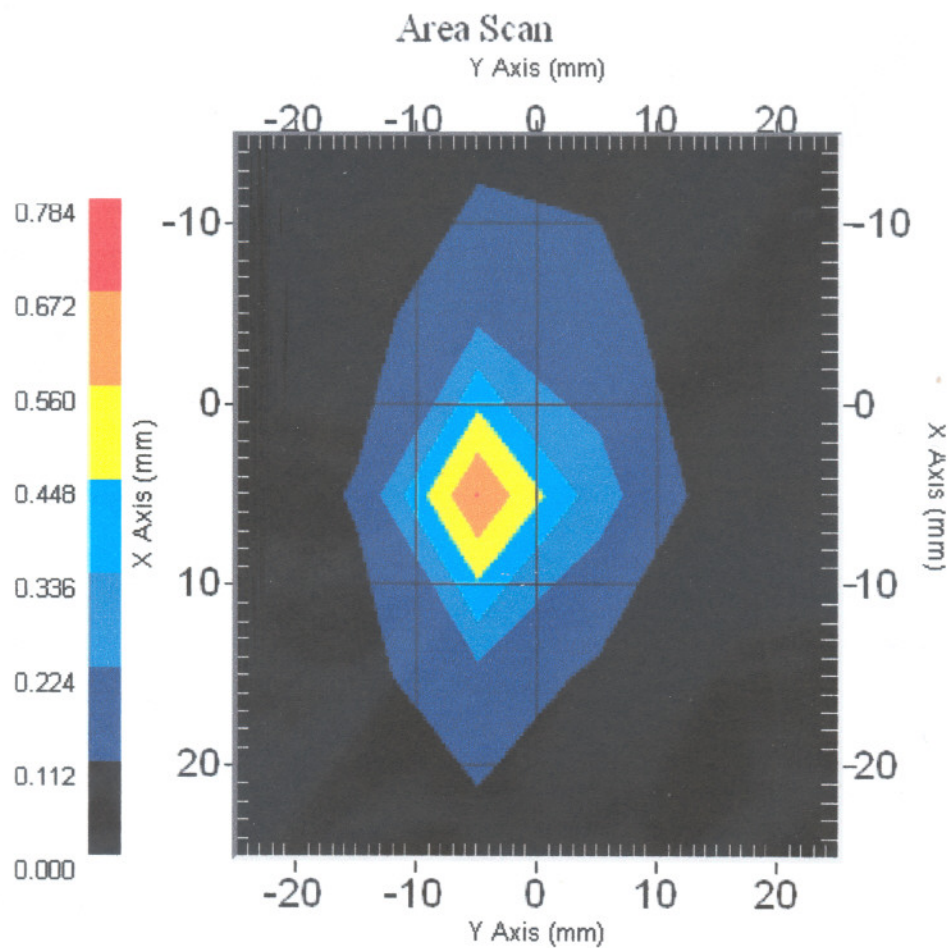

NCL Calibration Laboratories

Division of APREL Laboratories.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2004