

ROHDE & SCHWARZ

FSP · SPECTRUM ANALYZER · 9 kHz ... 40 GHz

Nemko

Liberty Labs, CAN
Serial 100032
CAL 08/05/2017
REV 08/05/2016
Tech SM 00444

1164.4391.40


PRESET

CAL

SETUP

HOLD

FSP

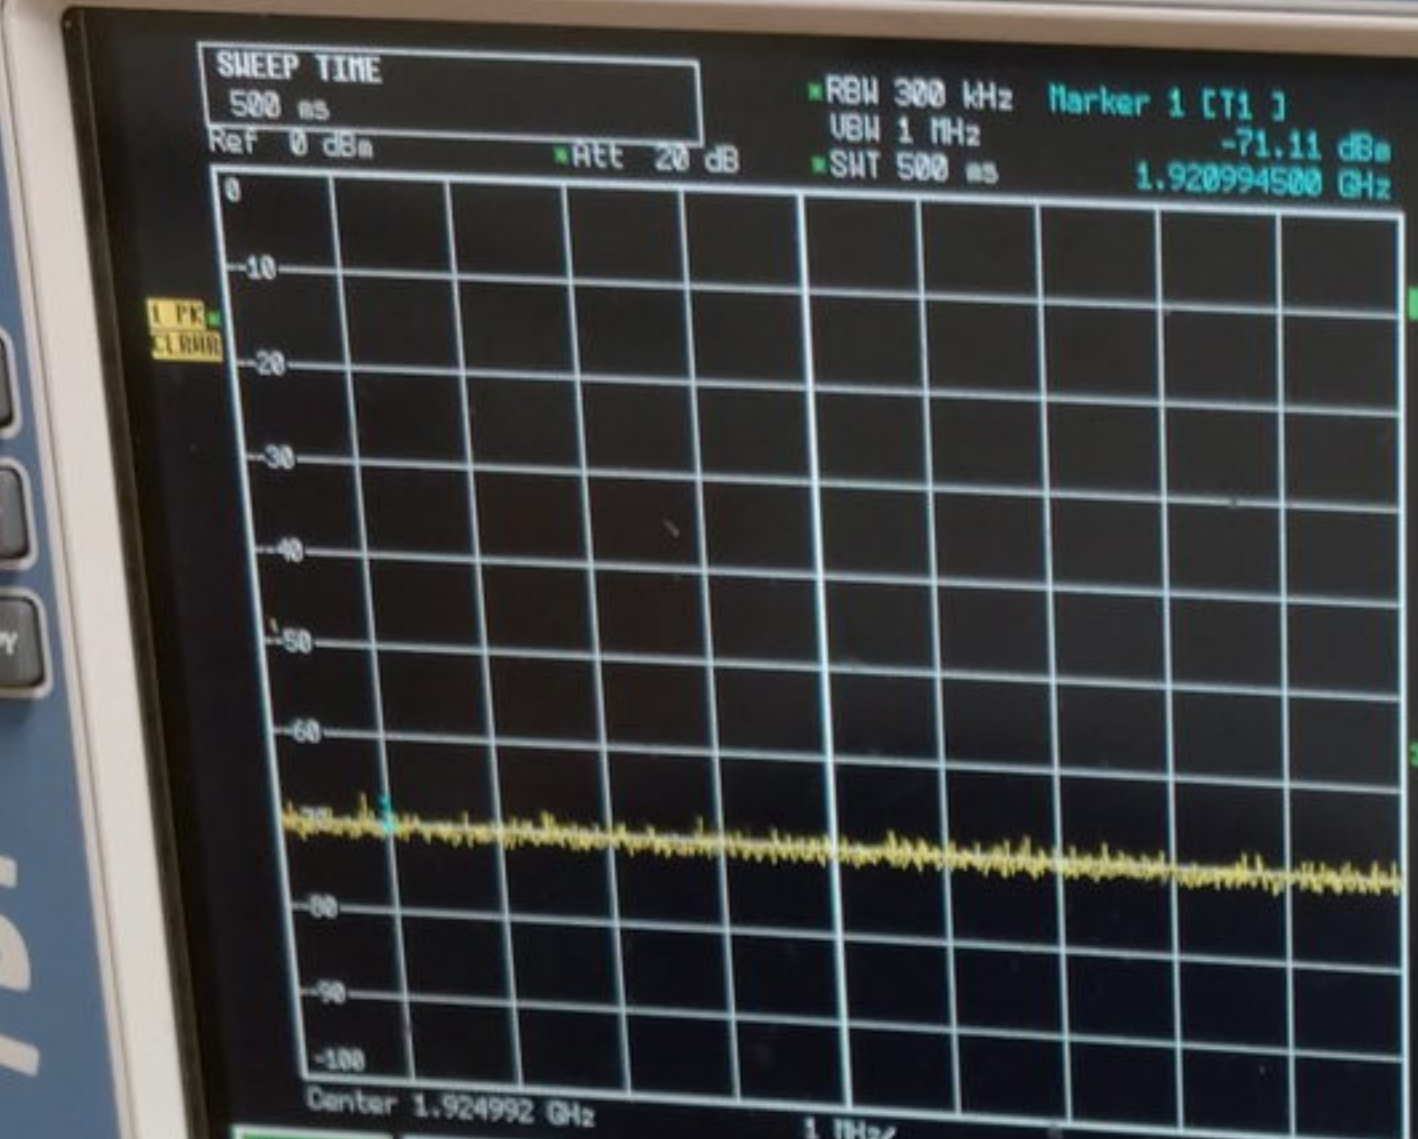

CONTINUOUS SWEEP

SINGLE SWEEP

CONTINUE SGL SWEEP

SWEEP TIME MANUAL

SWEEP TIME AUTO

SWEEP COUNT

SWEEP POINTS

SGL SWEEP DISP OFF

SCREEN B

PREV

NEXT

FREQ

SPAN

AMPT

MKR

MKR →

MKR FCTN

7

8

9

4

5

6

1

2

3

0

.

-

ESC CANCEL

ENTER

BACK

TRACE

LINES

DISP

FILE

AF OUTPUT

GEN OUTPUT 50 Ω

EXT MIXER

LO OUT / IF IN

MAX 8V DC

PROBE POWER

EXT MIXER

LO OUT / IF IN

IF IN

RF INPUT 50 Ω

MAX 8V DC

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

KEYBOARD

