

Date: 2024-11-11

System Check_Head_2450MHz**DUT: D2450V2 - SN736**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_241111 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(7.95, 7.95, 7.95); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2024-01-22
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.50 W/kg; SAR (10g) = 1.17 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.60 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 78.7 %

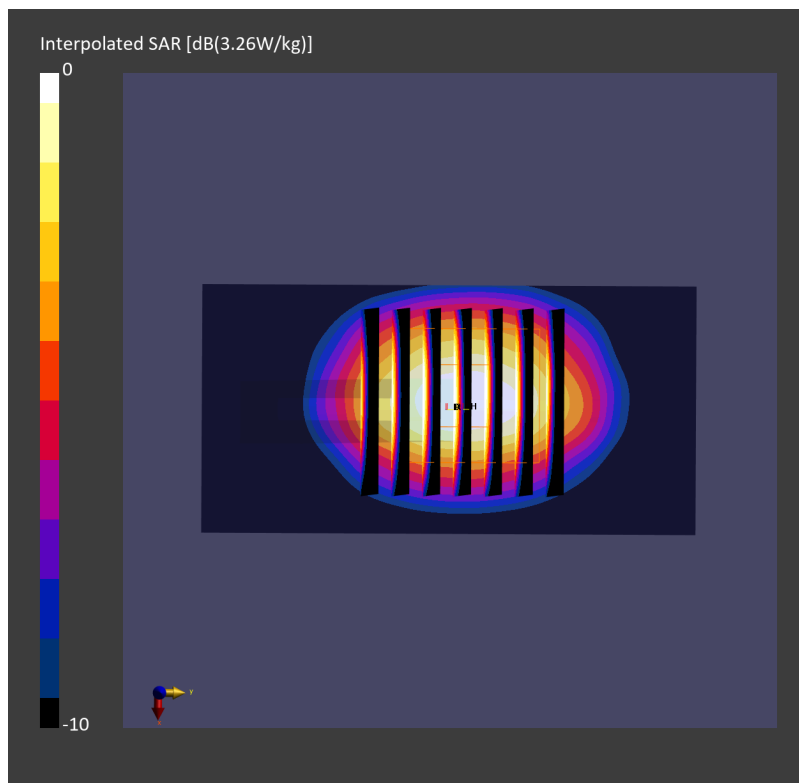

Date: 2024-12-06

System Check_Head_2450MHz**DUT: D2450V2 - SN736**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_241206 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 38.81$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.51, 6.73, 8.77); Calibrated: 2024-04-25
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1512; Calibrated: 2024-03-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156-; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.24 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5


mm

Power Drift = 0.08 dB

SAR (1g) = 2.58 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 8.6 mm

Ratio of SAR at M2 to SAR at M1 = 80.2 %

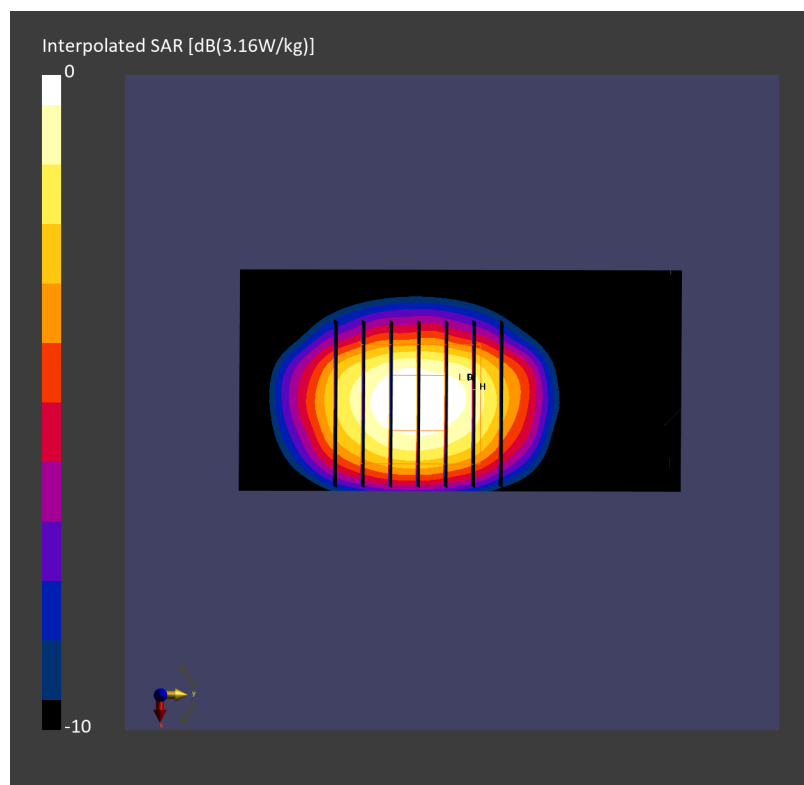

Date: 2024-11-09

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1171**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_241109 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.60$ S/m; $\epsilon_r = 36.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(5.67, 5.67, 5.67); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2024-01-22
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.50 W/kg; SAR (10g) = 1.03 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.88 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 67.6 %

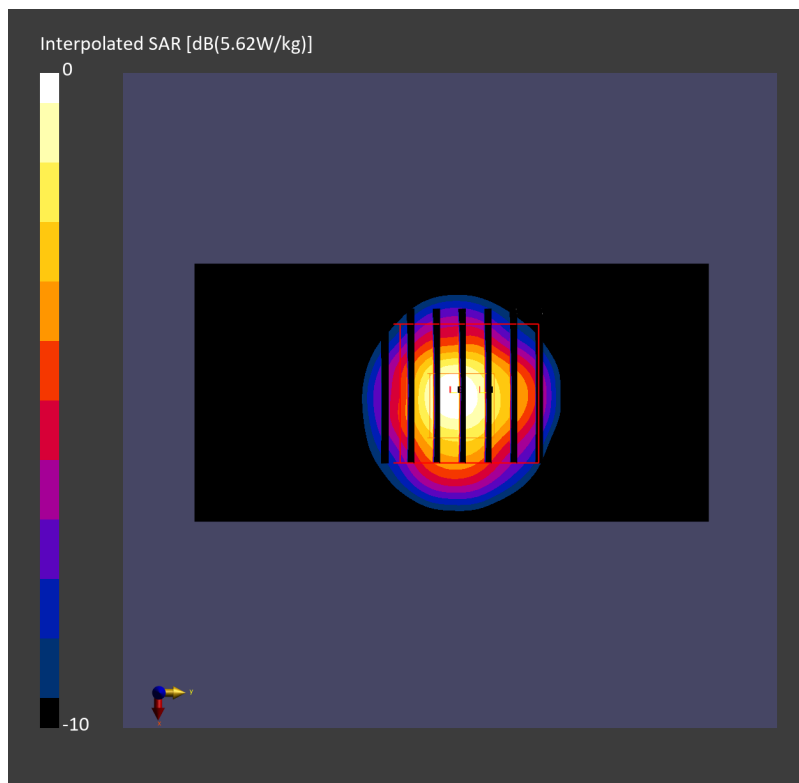

Date: 2024-11-09

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1171**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5G_241109 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.93$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(4.95, 4.95, 4.95); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2024-01-22
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.93 W/kg; SAR (10g) = 1.14 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 4.30 W/kg; SAR (8g) = 1.46 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.2 %

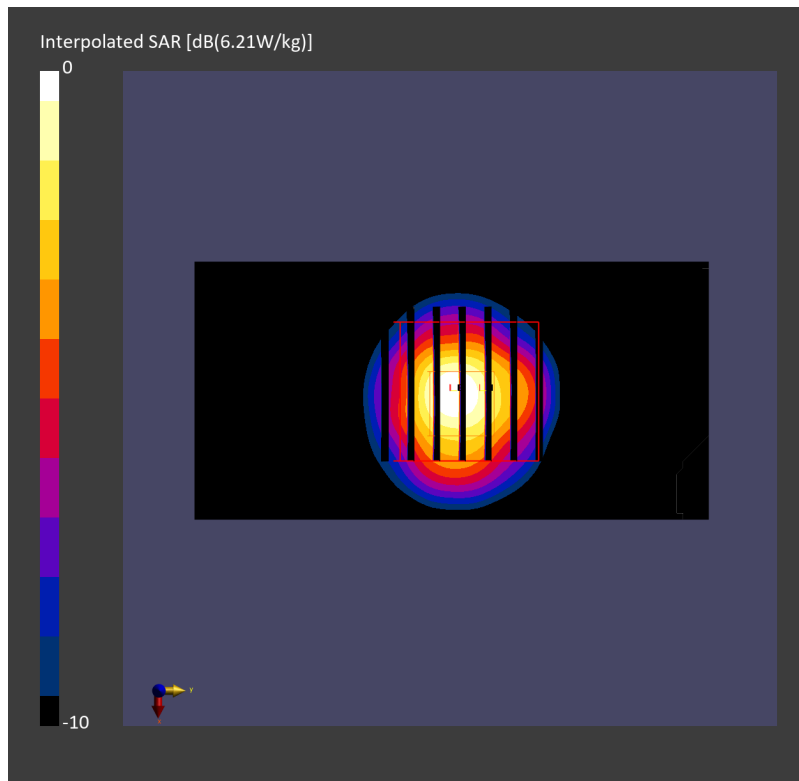

Date: 2024-11-09

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1171**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_5G_241109 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.15$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(5.08, 5.08, 5.08); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2024-01-22
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.69 W/kg; SAR (10g) = 1.07 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 4.05 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.8 %

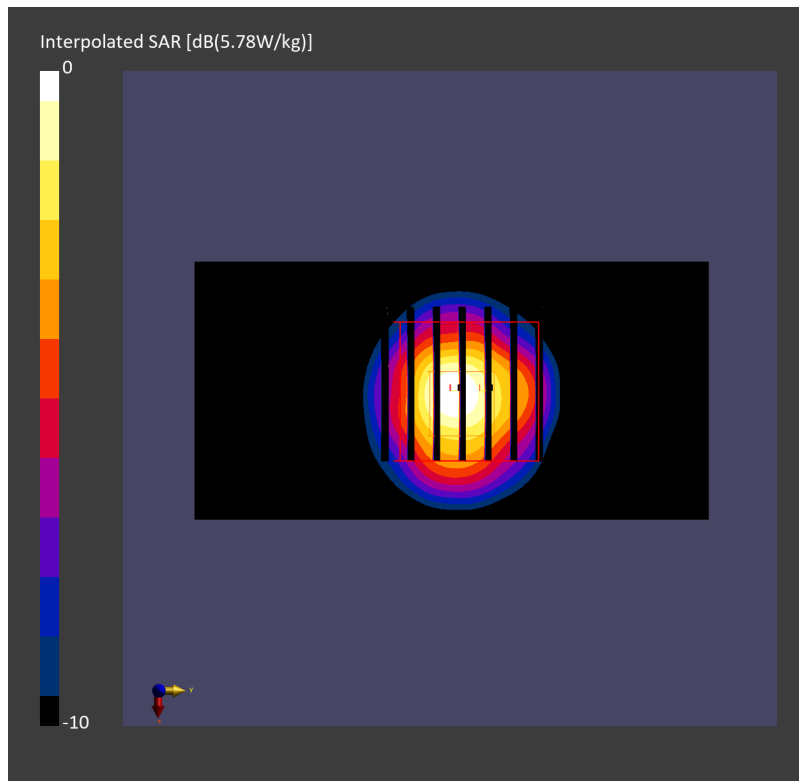

Date: 2024-11-10

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1003**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_6G_241110 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.18$ S/m; $\epsilon_r = 35.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(5.35, 5.35, 5.35); Calibrated: 2024-04-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn778; Calibrated: 2024-01-22
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1041; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 25.3 W/kg; SAR (10g) = 5.12 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 30.4 W/kg; SAR (8g) = 6.77 W/kg; SAR (10g) = 5.56 W/kg

Smallest distance from peaks to all points 3 dB below = 4.4 mm

Ratio of SAR at M2 to SAR at M1 = 55.7 %

psAPD (1.0cm², sq) = 304 [W/m²]; psAPD (4.0cm², sq) = 135 [W/m²]