


D450V3-SN:1113; 450Head

Calibrated impedance: 55.7Ω - $5.3j\Omega$; Measurement impedance: 59.3Ω - $6.9j\Omega$ (within 5Ω)



Calibrated return loss: -22.6dB; Measurement return loss: -22.8 dB(within 20%)

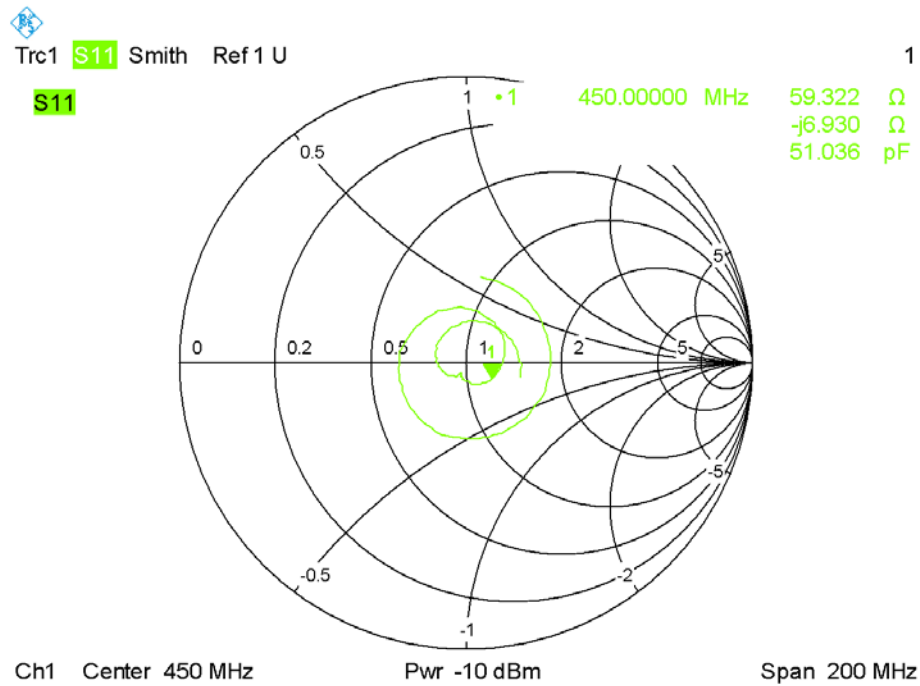