

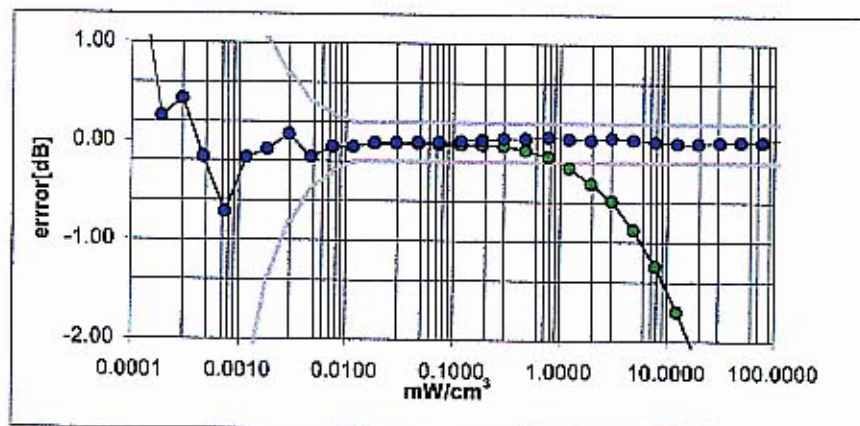


# Dynamic Range $f(\text{SAR}_{\text{brain}})$ ( TEM-Cell:ifi110 )

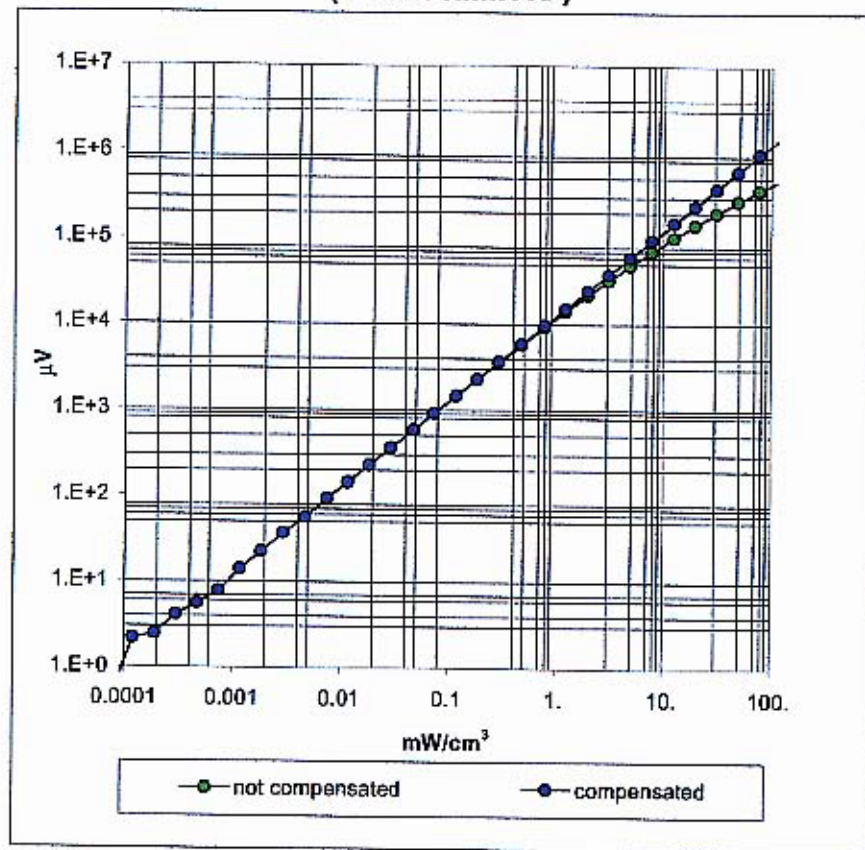


## Conversion Factor Assessment

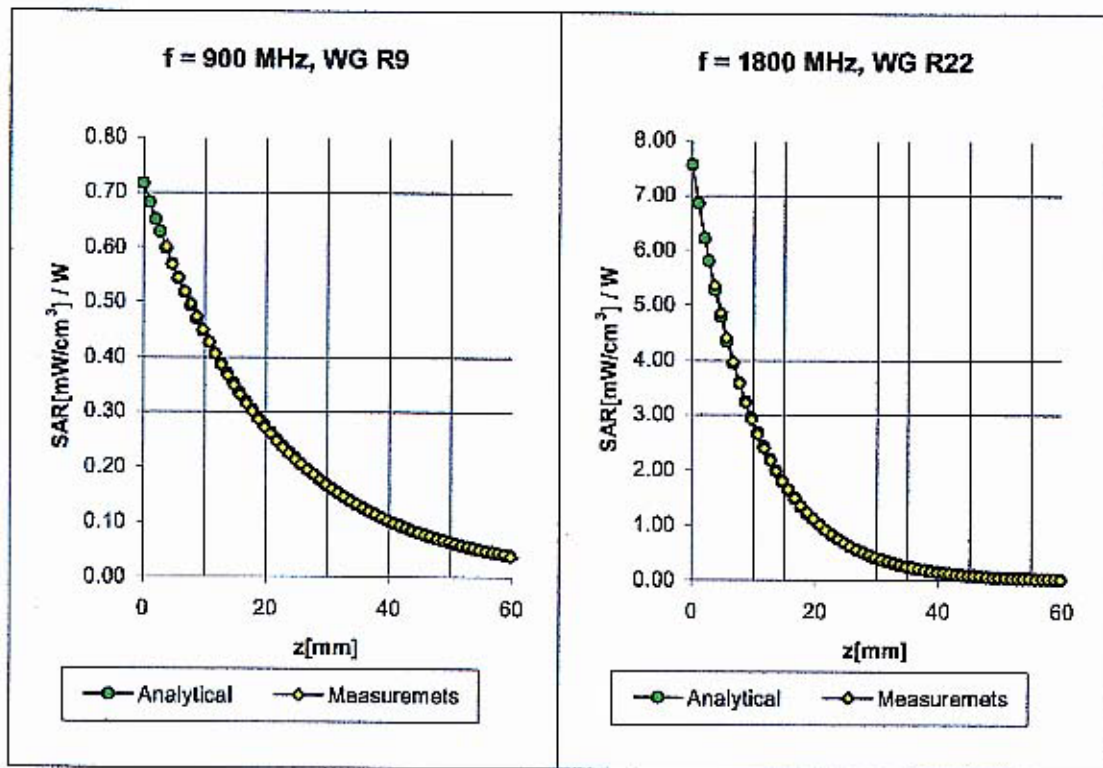



## Receiving Pattern ( $\phi$ )

( in brain tissue,  $z = 5 \text{ mm}$  )

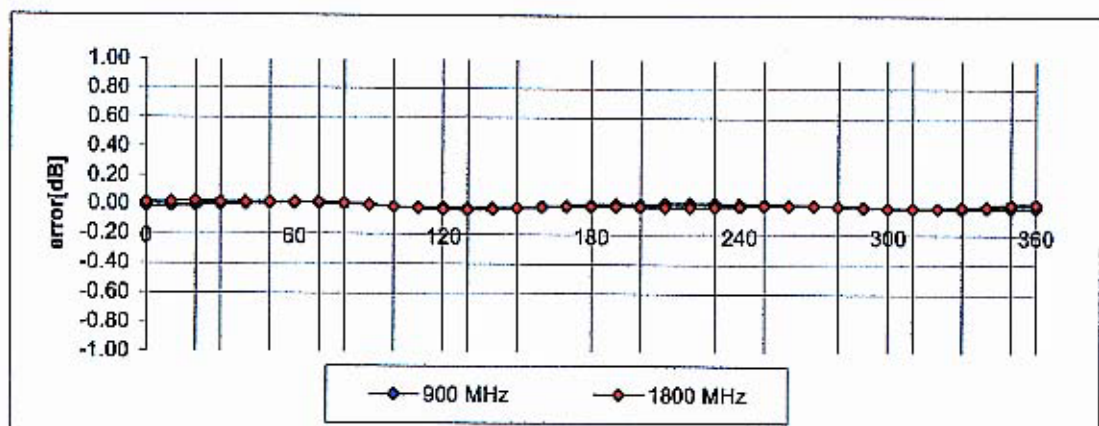

***APPENDIX "D" – TEST SETUP PHOTOGRAPHS***

**FACE-HELD SAR TEST SETUP PHOTOGRAPHS**  
**4.0cm Separation Distance**

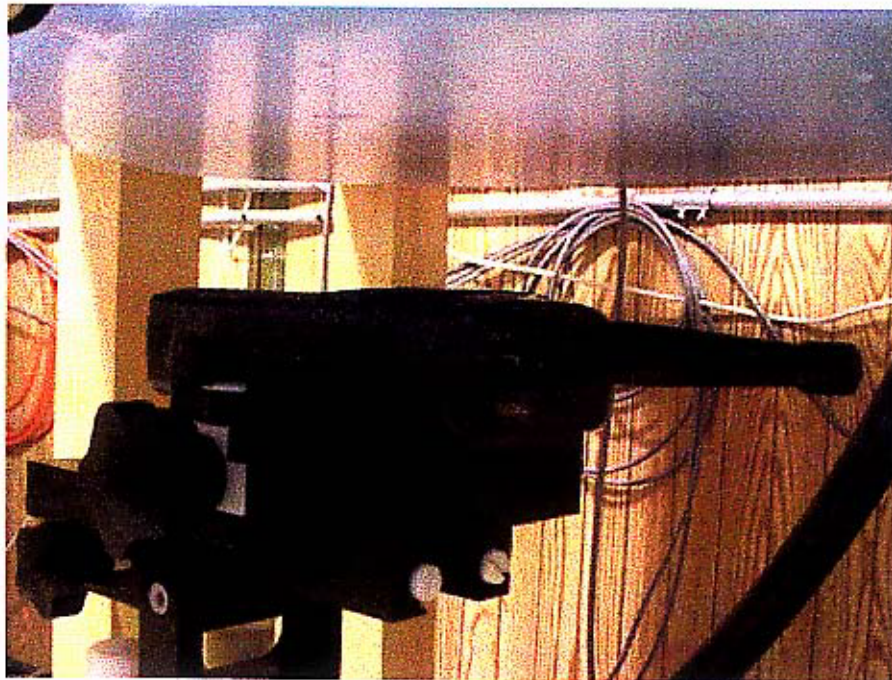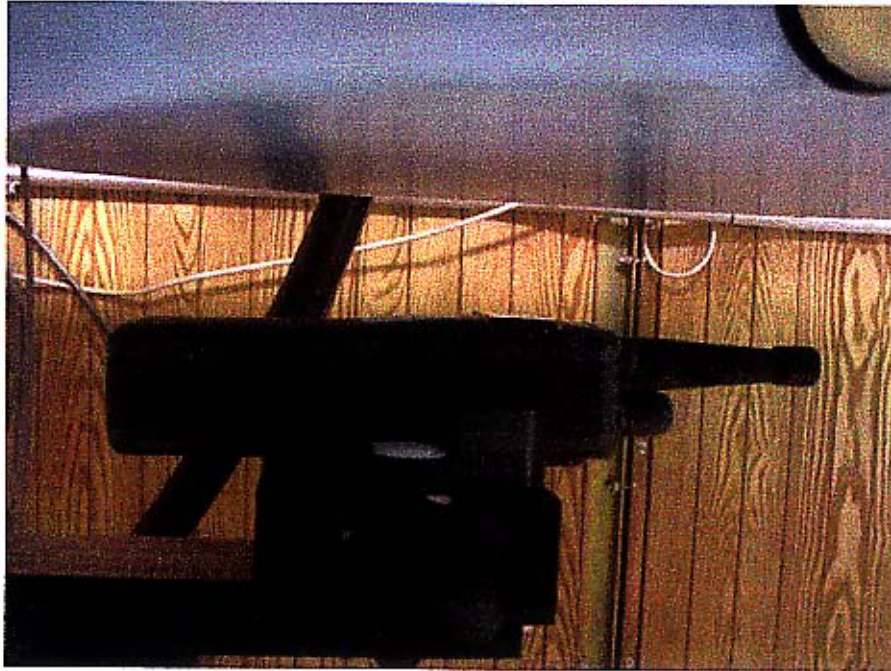

**BODY-WORN SAR TEST SETUP PHOTOGRAPHS**  
**0.8cm Separation Distance with Belt-Clip**

