



DASY5 Validation Report for Head TSL

Date: 20.07.2020

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1060

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5250 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz, Frequency: 5800 MHz Medium parameters used: f=5200 MHz; $\sigma=4.47$ S/m; $\epsilon_r=35.4$; $\rho=1000$ kg/m 3 , Medium parameters used: f=5250 MHz; $\sigma=4.52$ S/m; $\epsilon_r=35.4$; $\rho=1000$ kg/m 3 , Medium parameters used: f=5300 MHz; $\sigma=4.57$ S/m; $\epsilon_r=35.3$; $\rho=1000$ kg/m 3 , Medium parameters used: f=5500 MHz; $\sigma=4.77$ S/m; $\epsilon_r=35.3$; $\rho=1000$ kg/m 3 , Medium parameters used: f=5600 MHz; $\sigma=4.77$ S/m; $\epsilon_r=34.9$; $\rho=1000$ kg/m 3 , Medium parameters used: f=5600 MHz; $\sigma=4.88$ S/m; $\epsilon_r=34.9$; $\rho=1000$ kg/m 3 , Medium parameters used: f=5750 MHz; $\sigma=5.03$ S/m; $\epsilon_r=34.7$; $\rho=1000$ kg/m 3 , Medium parameters used: f=5800 MHz; $\sigma=5.09$ S/m; $\epsilon_r=34.6$; $\rho=1000$ kg/m 3

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.8, 5.8, 5.8) @ 5200 MHz, ConvF(5.5, 5.5, 5.5) @ 5250 MHz, ConvF(5.49, 5.49, 5.49) @ 5300 MHz, ConvF(5.25, 5.25, 5.25) @ 5500 MHz, ConvF(5.1, 5.1, 5.1) @ 5600 MHz, ConvF(5.08, 5.08, 5.08) @ 5750 MHz, ConvF(5.01, 5.01, 5.01) @ 5800 MHz; Calibrated: 31.12.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.12.2019
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 77.61 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 28.4 W/kg

SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.26 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 68.7%

Maximum value of SAR (measured) = 18.2 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 79.07 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 28.2 W/kg

SAR(1 g) = 8.08 W/kg; SAR(10 g) = 2.30 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 69.5%

Maximum value of SAR (measured) = 18.4 W/kg

Certificate No: D5GHzV2-1060_Jul20

Page 14 of 23





Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 78.56 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 29.6 W/kg

SAR(1 g) = 8.22 W/kg; SAR(10 g) = 2.33 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 68.3%

Maximum value of SAR (measured) = 19.0 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 78.44 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 33.9 W/kg

SAR(1 g) = 8.66 W/kg; SAR(10 g) = 2.42 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.9%

Maximum value of SAR (measured) = 20.7 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 78.89 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 31.6 W/kg

SAR(1 g) = 8.37 W/kg; SAR(10 g) = 2.37 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 66.8%

Maximum value of SAR (measured) = 20.2 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 75.69 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 32.1 W/kg

SAR(1 g) = 8.09 W/kg; SAR(10 g) = 2.29 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 65%

Maximum value of SAR (measured) = 19.9 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 75.77 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 32.8 W/kg

SAR(1 g) = 8.16 W/kg; SAR(10 g) = 2.28 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm


Ratio of SAR at M2 to SAR at M1 = 64.8%

Maximum value of SAR (measured) = 20.1 W/kg

Certificate No: D5GHzV2-1060_Jul20

Page 15 of 23



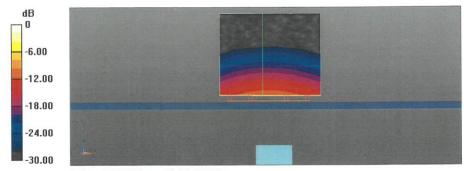

0 dB = 20.7 W/kg = 13.16 dBW/kg


Certificate No: D5GHzV2-1060_Jul20

Page 16 of 23





Impedance Measurement Plot for Head TSL (5200, 5250, 5300, 5500 MHz)

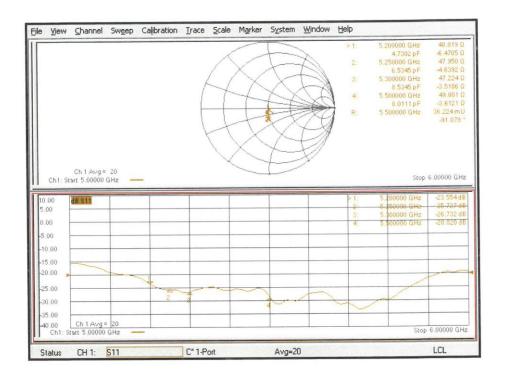


Certificate No: D5GHzV2-1060_Jul20

Page 17 of 23





Impedance Measurement Plot for Head TSL (5600, 5750, 5800 MHz)

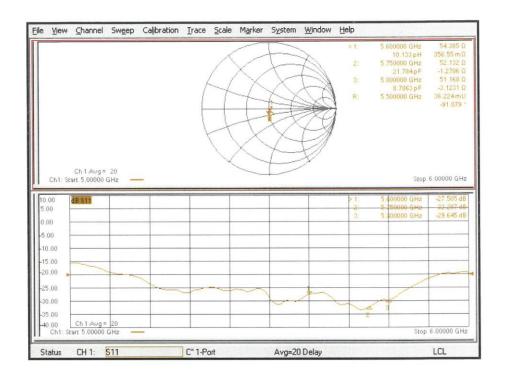

Certificate No: D5GHzV2-1060_Jul20 Page 18 of 23





DASY5 Validation Report for Body TSL

Date: 27.07.2020

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1060

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5250 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5500 MHz, Frequency: 5750 MHz, Frequency: 5800 MHz

Medium parameters used: f=5200 MHz; $\sigma=5.46$ S/m; $\epsilon_r=47.8$; $\rho=1000$ kg/m 3 , Medium parameters used: f=5250 MHz; $\sigma=5.53$ S/m; $\epsilon_r=47.7$; $\rho=1000$ kg/m 3 , Medium parameters used: f=5300 MHz; $\sigma=5.6$ S/m; $\epsilon_r=47.6$; $\rho=1000$ kg/m 3 ,

Medium parameters used: f = 5500 MHz; σ = 5.87 S/m; ϵ_r = 47.2; ρ = 1000 kg/m³ , Medium parameters used: f = 5600 MHz; σ = 6.01 S/m; ϵ_r = 47; ρ = 1000 kg/m³ ,

Medium parameters used: f = 5750 MHz; $\sigma = 6.22$ S/m; $\epsilon_r = 46.8$; $\rho = 1000$ kg/m³,

Medium parameters used: f = 5800 MHz; $\sigma = 6.29$ S/m; $\epsilon_r = 46.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.29, 5.29, 5.29) @ 5200 MHz, ConvF(5.26, 5.26, 5.26) @ 5250 MHz, ConvF(5.23, 5.23, 5.23) @ 5300 MHz, ConvF(4.84, 4.84, 4.84) @ 5500 MHz, ConvF(4.79, 4.79, 4.79) @ 5600 MHz, ConvF(4.66, 4.66, 4.66) @ 5750 MHz, ConvF(4.62, 4.62, 4.62) @ 5800 MHz; Calibrated: 31.12.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.12.2019
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.58 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 27.8 W/kg

SAR(1 g) = 7.3 W/kg; SAR(10 g) = 2.04 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 67.4%

Maximum value of SAR (measured) = 17.0 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.59 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 29.0 W/kg

SAR(1 g) = 7.45 W/kg; SAR(10 g) = 2.09 W/kg

Smallest distance from peaks to all points 3 dB below = 6.9 mm

Ratio of SAR at M2 to SAR at M1 = 66.5%

Maximum value of SAR (measured) = 17.4 W/kg

Certificate No: D5GHzV2-1060_Jul20

Page 19 of 23





Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.12 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 29.1 W/kg

SAR(1 g) = 7.36 W/kg; SAR(10 g) = 2.06 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 66.1%

Maximum value of SAR (measured) = 17.3 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 68.41 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 33.0 W/kg

SAR(1 g) = 7.86 W/kg; SAR(10 g) = 2.17 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.2%

Maximum value of SAR (measured) = 19.0 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.25 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 33.2 W/kg

SAR(1 g) = 7.72 W/kg; SAR(10 g) = 2.15 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.4%

Maximum value of SAR (measured) = 18.7 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.67 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 34.2 W/kg

SAR(1 g) = 7.61 W/kg; SAR(10 g) = 2.11 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62%

Maximum value of SAR (measured) = 18.7 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.55 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 32.7 W/kg

SAR(1 g) = 7.42 W/kg; SAR(10 g) = 2.04 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm


Ratio of SAR at M2 to SAR at M1 = 62.5%

Maximum value of SAR (measured) = 18.2 W/kg

Certificate No: D5GHzV2-1060_Jul20

Page 20 of 23



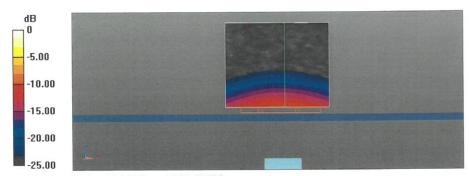

0 dB = 19.0 W/kg = 12.79 dBW/kg


Certificate No: D5GHzV2-1060_Jul20

Page 21 of 23





Impedance Measurement Plot for Body TSL (5200, 5250, 5300, 5500 MHz)

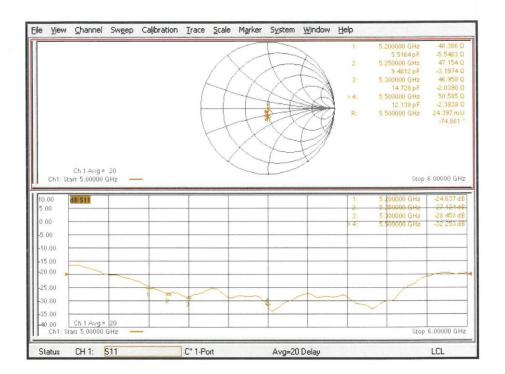


Certificate No: D5GHzV2-1060_Jul20

Page 22 of 23





Impedance Measurement Plot for Body TSL (5600, 5750, 5800 MHz)

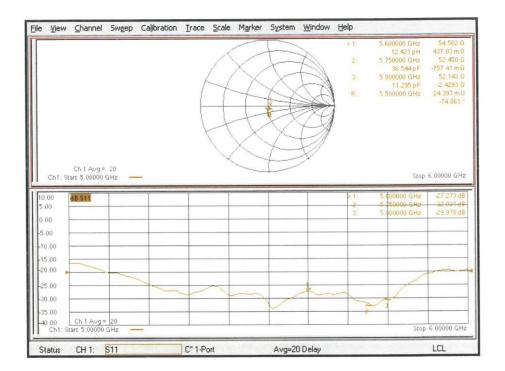

Certificate No: D5GHzV2-1060_Jul20

Page 23 of 23





2300 MHz Dipole Calibration Certificate

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client CTTL-BJ (Auden)

Calibration Procedure for SAR Validation Sources between 0.7-3 GHz Calibration date: July 21, 2020 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Apr-21 SN: 103245 01-Apr-20 (No. 217-03100) Apr-21 SN: 103245 01-Apr-20 (No. 217-03100) Apr-21 SN: 103245 01-Apr-20 (No. 217-03100) Apr-21 SN: 103245 01-Apr-20 (No. 217-03101) Apr-21 SN: 103245 01-Apr-20 (No. 217-03106) Apr-21 SN: 103245 01-Apr-20 (No. 217-03106) Apr-21 SN: 319982 / 06327 31-Mar-20 (No. 217-03104) A	CALIBRATION	CERTIFICAT	E	
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz Calibration date: July 21, 2020 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Dower meter NRP SN: 104778 01-Apr-20 (No. 217-03100/03101) Apr-21 SN: 103244 01-Apr-20 (No. 217-03100) Apr-21 SReference 20 dB Attenuator SN: BH9394 (20k) SN: 31-Mar-20 (No. 217-03106) Apr-21 Apr-21 SN: 310982 / 06327 SN: 31-Mar-20 (No. 217-03104) Apr-21 SN: 310982 / 06327 SN: 7349 29-Jun-20 (No. 217-03104) Apr-21 SN: 601 D# Check Date (in house) Scheduled Check Ower sensor HP 8481A SN: US37292783 O'-Oct-15 (in house check Feb-19) In house check: Oct-20	Object	D2300V2 - SN:	1018	
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz Calibration date: July 21, 2020 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Power meter NRP Power sensor NRP-291 SN: 104778 01-Apr-20 (No. 217-03100/03101) Apr-21 SN: 103244 01-Apr-20 (No. 217-03100) Apr-21 Reference 20 dB Attenuator SN: BH9394 (20k) SN: 31-Mar-20 (No. 217-03104) Apr-21 SN: 310982 / 06327 SN: 7349 29-Jun-20 (No. 217-03104) Apr-21 SN: 7349 29-Jun-20 (No. 217-03104) Apr-21 SN: 601 27-Dec-19 (No. DAE4-601_Dec19) Dec-20 Secondary Standards Fower meter E4419B SN: GB39512475 SN: GB39512475 SN: GB39512475 SN: GB39512475 SN: GB39512475 SN: GB39512475 SN: US37292783 Or-Oct-15 (in house check Feb-19) In house check: Oct-20 (in house check Oct-18) In house check: Oct-20 (in house check Oct-18) In house check: Oct-20 (in house check Oct-19) Amme Function Signature	Calibration procedure(s)	OA CAL-OF vit		
Calibration date: July 21, 2020 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Prower sensor NRP-291 SN: 104778 01-Apr-20 (No. 217-03100/003101) Apr-21 SN: 103244 01-Apr-20 (No. 217-03100) Apr-21 SN: 103245 01-Apr-20 (No. 217-03100) Apr-21 SN: 310982 / 06327 31-Mar-20 (No. 217-03104) Apr-21 SN: 310982 / 06327 SN: 310982 / 06327 31-Mar-20 (No. 217-03104) Apr-21 SN: 601 27-Dec-19 (No. DAE4-601_Dec19) Dec-20 Scheduled Check Sover sensor HP 8481A SN: US37292783 SN: GB39512475 SN: GB39512475 SN: US37292783 SN: U	,			
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards D# Cal Date (Certificate No.) Scheduled Calibration Primary Standards D# Cal Date (Certificate No.) Scheduled Calibration Primary Standards D# Cal Date (Certificate No.) Scheduled Calibration Apr-21 SN: 104778 01-Apr-20 (No. 217-03100) Apr-21 SN: 103244 01-Apr-20 (No. 217-03100) Apr-21 Paterience 20 dB Attenuator SN: B19394 (20k) 31-Mar-20 (No. 217-03101) Apr-21 Paterience 20 dB Attenuator SN: 310982 / 06327 31-Mar-20 (No. 217-03106) Apr-21 Paterience Probe EX3DV4 SN: 310982 / 06327 31-Mar-20 (No. 217-03104) Apr-21 Paterience Probe EX3DV4 SN: 7349 29-Jun-20 (No. EX3-7349_Jun20) Jun-21 Paterience Probe EX3DV4 SN: 601 27-Dec-19 (No. DAE4-601_Dec19) Dec-20 econdary Standards D# Check Date (in house) Scheduled Check Ower sensor HP 8481A SN: US37292783 OF-Oct-15 (in house check Feb-19) In house check: Oct-20 power sensor HP 8481A SN: US37292783 OF-Oct-15 (in house check Oct-18) In house check: Oct-20 Paterience Probe EX3DVA Name Function Signature Paterience Proposed by: Colt Paterience Proposed By Scheduled Check Colt Paterience Proposed by: Colt Paterience Proposed by: Colt Paterience Proposed By Scheduled Check Colt Paterience Proposed by: Colt Paterience Proposed By: Colt Paterience Proposed By Scheduled Check Colt Paterience Proposed By: Colt P		Cambration Frod	sedure for SAH validation Source	es between 0.7-3 GHz
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Trimary Standards Over meter NRP SN: 104778 O1-Apr-20 (No. 217-03100/03101) Apr-21 SN: 103244 O1-Apr-20 (No. 217-03100) Apr-21 SN: 103244 O1-Apr-20 (No. 217-03100) Apr-21 SN: 103245 O1-Apr-20 (No. 217-03101) Apr-21 SN: 310982 / 06327 31-Mar-20 (No. 217-03106) Apr-21 Ap				
All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Dever meter NRP SN: 104778 O1-Apr-20 (No. 217-03100/03101) SN: 103244 O1-Apr-20 (No. 217-03100) Apr-21 SN: 103244 O1-Apr-20 (No. 217-03100) Apr-21 SN: 103245 O1-Apr-20 (No. 217-03100) Apr-21 SN: 103245 O1-Apr-20 (No. 217-03101) Apr-21 SN: BH9394 (20k) SN: BH9394 (20k) SN: 310982 / 06327 SN: 310982 / 06327 SN: 601 Z7-Dec-19 (No. DAE4-601_Dec19) Dec-20 Becondary Standards Dip # Check Date (in house) Scheduled Check In house check: Oct-20 SN: US37292783 O7-Oct-15 (in house check Oct-18) In house check: Oct-20 SN: US41080477 SIDNAR Figenerator R&S SMT-06 SN: US41080477 SAMP SAMP Function Signature Function Spice and are part of the certificate. Scheduled Check Signature Function Signature	Calibration date:	July 21, 2020		
ID # Cal Date (Certificate No.) Scheduled Calibration		or macrice	probability are given on the following pages	and are part of the certificate.
Solution Calibrate (Certificate No.) Scheduled Calibration Apr-21				• • • • • • • • • • • • • • • • • • • •
SN: 104778	Primary Standards	ID#	Cal Data (Contificate No.)	
SN: 103244		SN: 104778		
SN: 103245 01-Apr-20 (No. 217-03101) Apr-21		SN: 103244	01-Apr-20 (No. 217-03100/03101)	100 100 100 100 100 100 100 100 100 100
SN: BH9394 (20k) SN: 310982 / 06327 SN: 601 SN				(1)************************************
SN: 310982 / 06327 SN: 31-Mar-20 (No. 217-03104) Apr-21		SN: BH9394 (20k)		
SN: 7349 SN: 601 SN: 6	ype-N mismatch combination	SN: 310982 / 06327		
SN: 601 27-Dec-19 (No. DAE4-601_Dec19) Dec-20		SN: 7349		
Scheduled Check Solver meter E4419B SN: GB39512475 SO-Oct-14 (in house check Feb-19) In house check: Oct-20 In house chec	AE4	SN: 601	27-Dec-19 (No. DAE4-601_Dec19)	
SN: GB39512475 SN: US37292783 O7-Oct-15 (in house check Oct-18) In house check: Oct-20 In hou	econdary Standards	ID#	Check Date (in house)	
SN: US37292783 SN: WY41092317 SN: MY41092317 SN: MY41092317 SN: MY41092317 SN: MY41092317 SN: MY41092317 SN: MY41092317 SN: US41080477 SN: US	2007 N. C.	SN: GB39512475		
SN: MY41092317 O7-Oct-15 (in house check Oct-18) In house check: Oct-20 In house check: Oct		SN: US37292783	07-Oct-15 (in house check Oct-19)	
Ski: 100972 15-Jun-15 (in house check Oct-18) In house check: Oct-20 stwork Analyzer Agilent E8358A Ski: US41080477 31-Mar-14 (in house check Oct-19) In house check: Oct-20 In house c		SN: MY41092317	07-Oct-15 (in house check Oct-18)	
Name Signature Vertice Retrieval: Name Function Signature Laboratory Technician Function Signature Additional Statement Signature Additional Signature Additional Signature Additional Signature Additional Signature	generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-18)	
Jeffrey Katzman Jeffrey Katzman Laboratory Technician Jeffrey Katzman Signature All Jeffrey Katzman	twork Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-19)	In house check: Oct-20
Jeffrey Katzman Laboratory Technician J. Kuffun Deroved by: Katio Releasing		Name	Function	
proved by: Katio Palania	librated by:	Jeffrey Katzman		Signature
proved by: Katja Pokovic Technical Manager				d. Kitu
Technical Manager				
the contract of the contract o	proved by:	Katja Pokovic	Toobnies! Man	

Certificate No: D2300V2-1018_Jul20

Page 1 of 8





Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

C Service suisse d'étalonnage Servizio svizzero di taratura

Accreditation No.: SCS 0108

S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2300V2-1018_Jul20	Page 2 of 8	



Measurement Conditions

DASY system configuration, as far as not given on page 1

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	V02.10.4
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	with opacer
Frequency	2300 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.0 ± 6 %	1.68 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	12.5 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	49.7 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.97 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.8 W/kg ± 16.5 % (k=2)

Body TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.9	1.81 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.8 ± 6 %	1.84 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.2 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	48.2 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.85 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.2 W/kg ± 16.5 % (k=2)

Certificate No: D2300V2-1018_Jul20

Page 3 of 8





Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	
Return Loss	50.1 Ω - 3.4 jΩ
	- 29.5 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	
Return Loss	46.7 Ω - 2.4 jΩ
	- 27.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	
(one direction)	1.169 ns
	1.100 113

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the according to the Standard. The SAR data are not affected by this change. The overall dipole length is still

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	
,	SPEAG
	J. 27G

Certificate No: D2300V2-1018_Jul20

Page 4 of 8





DASY5 Validation Report for Head TSL

Date: 21.07.2020

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN:1018

Communication System: UID 0 - CW; Frequency: 2300 MHz

Medium parameters used: f = 2300 MHz; $\sigma = 1.68$ S/m; $\epsilon_r = 39$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

• Probe: EX3DV4 - SN7349; ConvF(7.82, 7.82, 7.82) @ 2300 MHz; Calibrated: 29.06.2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 27.12.2019

Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001

DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 117.7 V/m; Power Drift = -0.07 dB


Peak SAR (extrapolated) = 23.8 W/kg

SAR(1 g) = 12.5 W/kg; SAR(10 g) = 5.97 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 52.9%

Maximum value of SAR (measured) = 20.0 W/kg

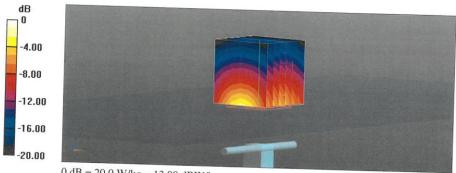

0 dB = 20.0 W/kg = 13.00 dBW/kg


Certificate No: D2300V2-1018_Jul20

Page 5 of 8





Impedance Measurement Plot for Head TSL

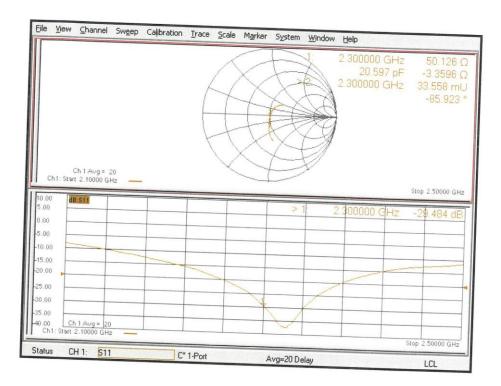

Certificate No: D2300V2-1018_Jul20

Page 6 of 8



DASY5 Validation Report for Body TSL

Date: 21.07.2020

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN:1018

Communication System: UID 0 - CW; Frequency: 2300 MHz

Medium parameters used: f = 2300 MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 51.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

• Probe: EX3DV4 - SN7349; ConvF(7.93, 7.93, 7.93) @ 2300 MHz; Calibrated: 29.06.2020

- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.12.2019
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 109.4 V/m; Power Drift = -0.08 dB


Peak SAR (extrapolated) = 23.4 W/kg

SAR(1 g) = 12.2 W/kg; SAR(10 g) = 5.85 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 53.6%

Maximum value of SAR (measured) = 19.4 W/kg

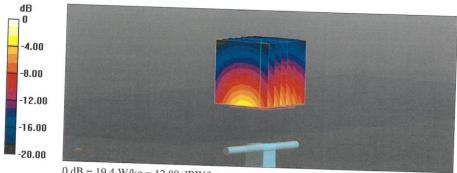

0 dB = 19.4 W/kg = 12.89 dBW/kg


Certificate No: D2300V2-1018_Jul20

Page 7 of 8





Impedance Measurement Plot for Body TSL

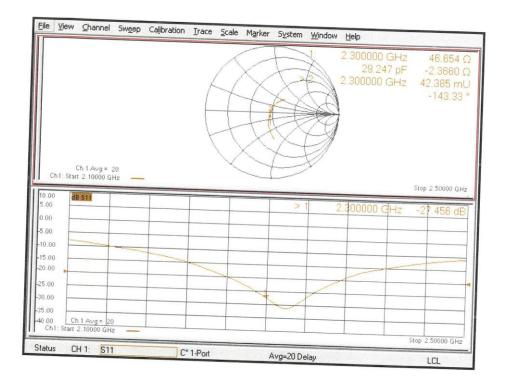

Certificate No: D2300V2-1018_Jul20

Page 8 of 8





ANNEX I Sensor Triggering Data Summary

Main Antenna:

Sensor	Back(mm)	27(mm)
Sensor	Front(mm)	22(mm)
Sensor	Top(mm)	27(mm)
Sensor	Left(mm)	13(mm)

WIFI Atenna(2.4G&5G):

Sensor	Back(mm)	15(mm)
Sensor	Front(mm)	25(mm)
Sensor	Top(mm)	28(mm)

According to the above description, this device was tested by the manufacturer to determine the SAR sensor triggering distances for the front, rear, left edge and top edge for main antenna and front,rear ,top edge for WIFI antenna of the device. The measured power state within ± 5 mm of the triggering points (or until touching the phantom) is included for rear and each applicable edge.

To ensure all production units are compliant it is necessary to test SAR at a distance 1mm less than the smallest distance from the device and SAR phantom with the device at maximum output power without power reduction.

We tested the level and got the different sensor triggering distances for front, rear, left edge and top edge. But the manufacturer has declared 22mm(front),27mm (rear), 27mm (top) / 13mm (left edge) are the most conservative triggering distance for main antenna and 15mm (rear) / 28mm (top edge), 25mm(for front) for WiFi antenna. Therefore base on the most conservative triggering distances as above, additional SAR measurements were required at 21mm(front),26mm (rear), 26mm (top),12mm (left edge) for main antenna and 14mm (rear) / 27mm (top edge), 24mm(for front)for wifi antenna.

Main antenna

Rear

Moving device toward the phantom:

The power state												
Distance [mm] 32 31 30 29 28 27 26 25 24 23 22										22		
Main antenna	Normal	Low										

Moving device away from the phantom:

		<u>'</u>									
The power state											
Distance [mm]	22	23	24	25	26	27	28	29	30	31	32
Main antenna	Low	Low	Low	Low	Low	Low	Low	Low	Low	Low	Normal



Front

Moving device toward the phantom:

The power state												
Distance [mm] 27 26 25 24 23 22 21 20 19 18 17											17	
Main antenna	Normal	Normal	Low									

Moving device away from the phantom:

The power state											
Distance [mm] 17 18 19 20 21 22 23 24 25 26 27										27	
Main antenna	Low	Normal	Normal								

Top Edge

Moving device toward the phantom:

The power state											
Distance [mm] 32 31 30 29 28 27 26 25 24 23 22											
Main antenna	Normal	Low									

Moving device away from the phantom:

The power state												
Distance [mm] 22 23 24 25 26 27 28 29 30 31 32										32		
Main antenna	Low	Normal										

Left Edge

Moving device toward the phantom:

The power state											
Distance [mm]											
Main antenna	Normal	Normal	Normal	Low							

Moving device away from the phantom:

The power state												
Distance [mm] 8 9 10 11 12 13 14 15 16 17 18										18		
Main antenna	Low	Normal	Normal	Normal								





WIFI antenna

Front

Moving device toward the phantom:

The power state											
Distance [mm]	30	29	28	27	26	25	24	23	22	21	20
Main antenna	Low										

Moving device away from the phantom:

The power state											
Distance [mm]	20	21	22	23	24	25	26	27	28	29	30
Main antenna	Low										

Top Edge

Moving device toward the phantom:

The power state											
Distance [mm] 33 32 31 30 29 28 27 26 25 24 2									23		
Main antenna	Normal	Normal	Low								

Moving device away from the phantom:

The power state											
Distance [mm] 23 24 25 26 27 28 29 30 31 32 3										33	
Main antenna	Low	Normal	Normal								

Rear

Moving device toward the phantom:


The power state											
Distance [mm]	20	19	18	17	16	15	14	13	12	11	10
Main antenna	Normal	Low									

Moving device away from the phantom:


The power state											
Distance [mm]	10	11	12	13	14	15	16	17	18	19	20
Main antenna	Low	Normal									

The influence of table tilt angles to proximity sensor triggering is determined by positioning each edge that contains a transmitting antenna, perpendicular to the flat phantom, at the smallest sensor triggering test distance by rotating the device around the edge next to the phantom in $\leq 10^{\circ}$ increments until the tablet is $\pm 45^{\circ}$ or more from the vertical position at 0° .



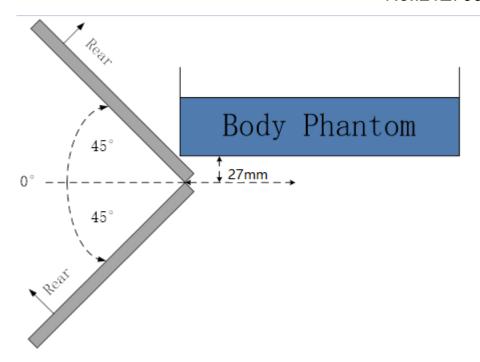


The rear evaluation for main antenna

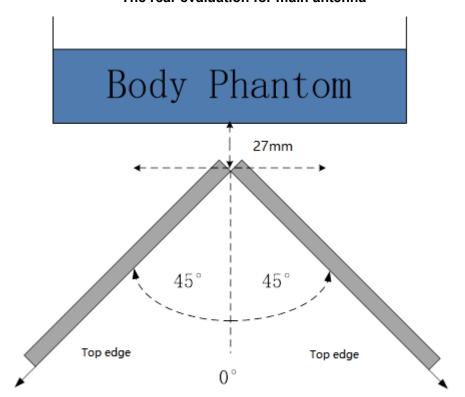


The top edge evaluation for main antenna



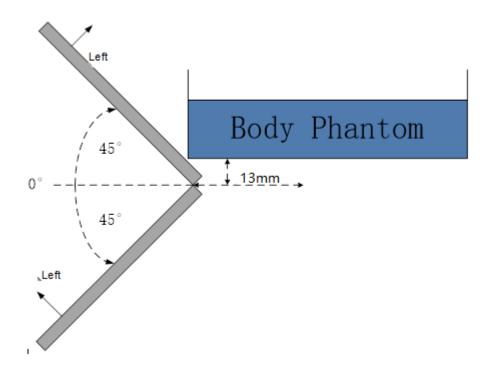


The Left edge evaluation for main antenna

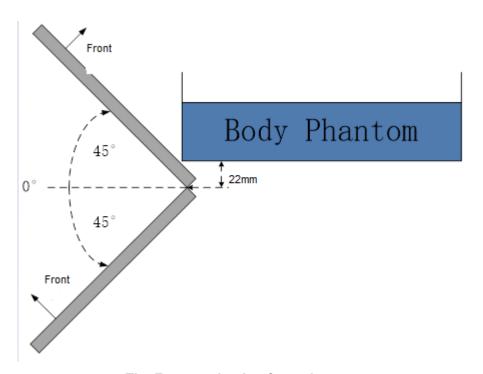


The Front evaluation for main antenna



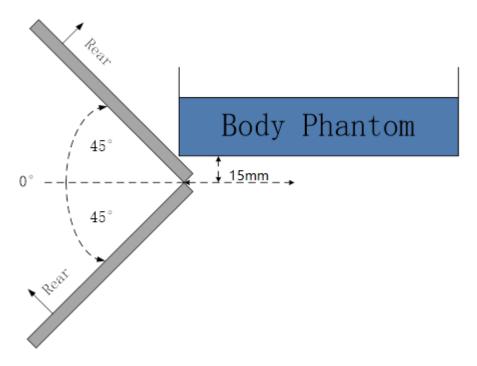


The rear evaluation for WIFI antenna

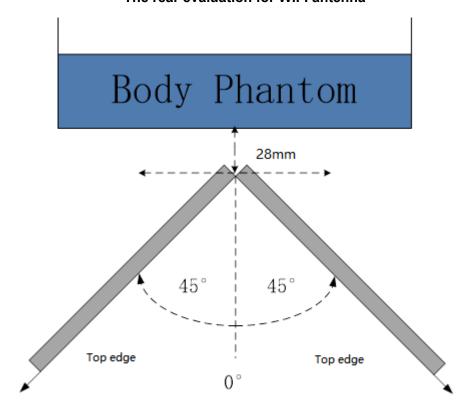

The top evaluation for WIFI antenna





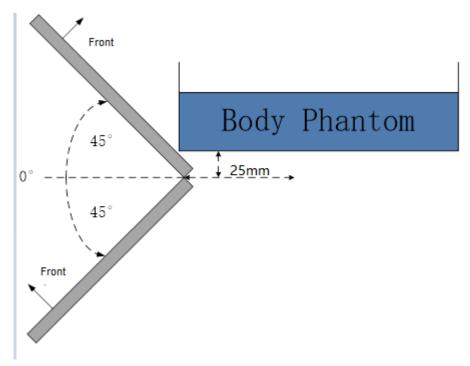

The front evaluation for WIFI antenna

Based on the above evaluation, we come to the conclusion that the sensor triggering is not released and normal maximum output power is not restored within the $\pm 45^{\circ}$ range at the smallest sensor triggering test distance declared by manufacturer.





ANNEX J Accreditation Certificate

United States Department of Commerce National Institute of Standards and Technology



Certificate of Accreditation to ISO/IEC 17025:2017

NVLAP LAB CODE: 600118-0

Telecommunication Technology Labs, CAICT

Beijing China

is accredited by the National Voluntary Laboratory Accreditation Program for specific services, listed on the Scope of Accreditation, for:

Electromagnetic Compatibility & Telecommunications

This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017.

This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality management system (refer to joint ISO-ILAC-IAF Communique dated January 2009).

2020-09-29 through 2021-09-30

Effective Dates



For the National Voluntary Laboratory Accreditation Program