



Impedance Plot for

SN 47/14 DIP 0G750-340; 750Head

Calibrated impedance: $54.2\Omega + 3.9j\Omega$; Measurement impedance: $57.7\Omega - 3.0j\Omega$ (within 5Ω)

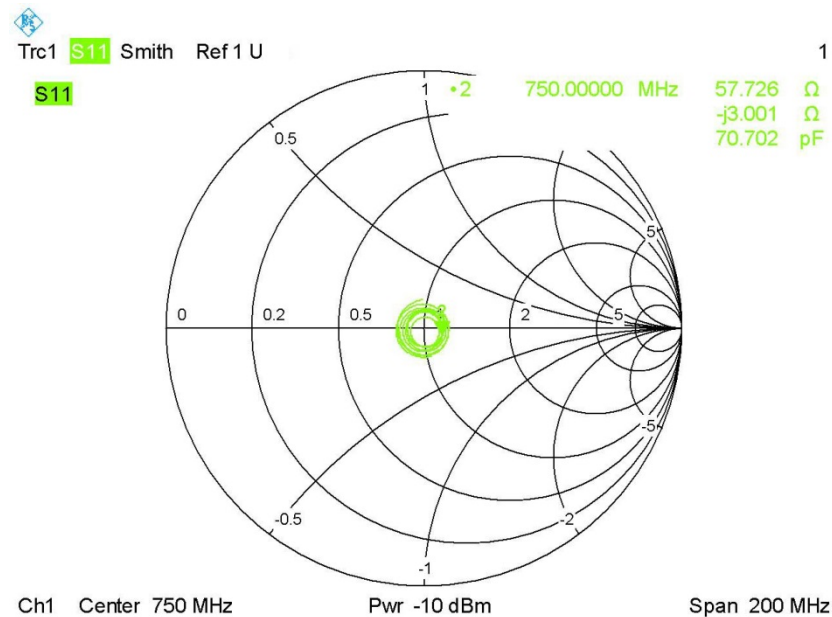


Calibrated return loss: -25.20dB; Measurement return loss: -24.41 dB (within 20%)

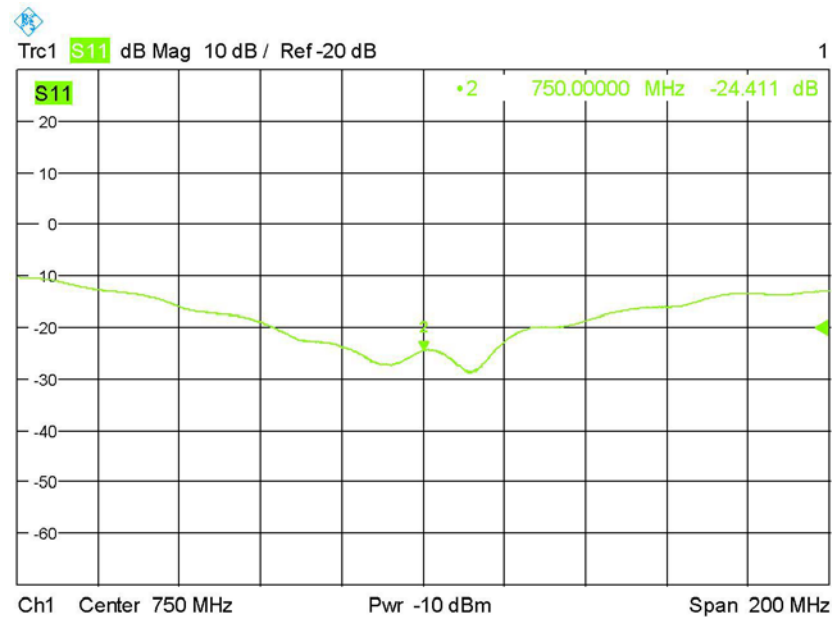


SN 29/15 DIP 0G835-383; 835Head



Calibrated impedance: $56.3\Omega + 0.8j\Omega$; Measurement impedance: $55.1\Omega - 4.7j\Omega$ (within 5Ω)

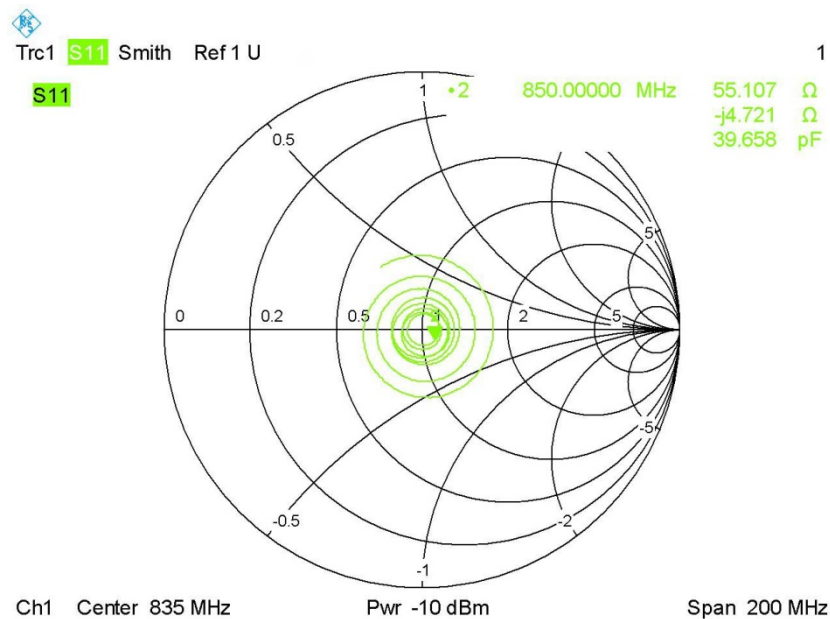

Calibrated return loss: -24.51dB; Measurement return loss: -24.34 dB (within 20%)

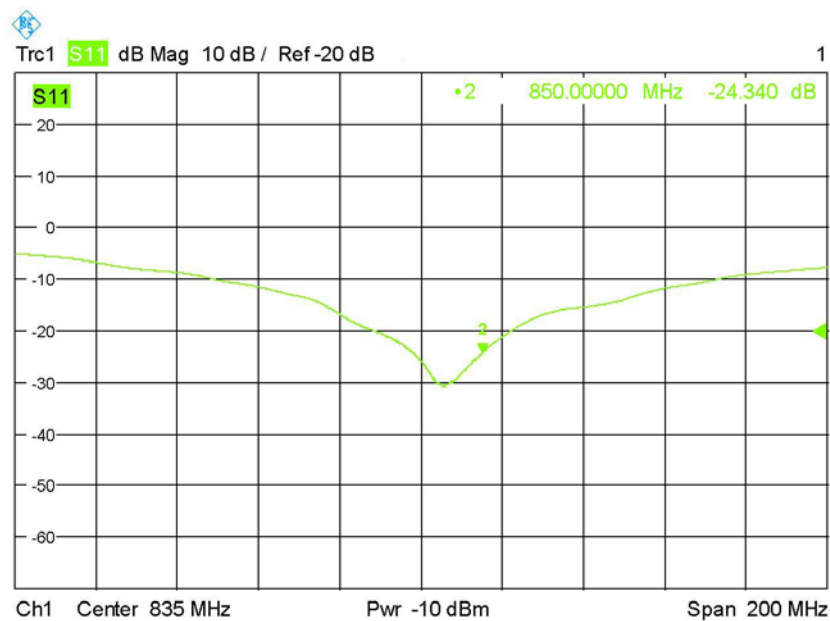


Calibrated impedance: $46.7\Omega + 3.0j\Omega$; Measurement impedance: $47.3\Omega + 1.6j\Omega$ (within 5Ω)

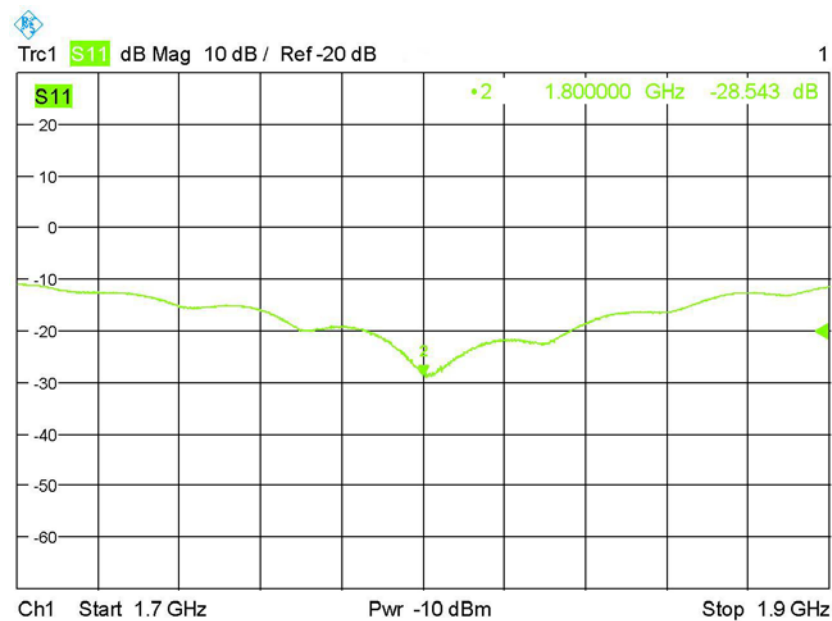


SN 46/11 DIP 1G900-187; 1900Head

Calibrated impedance: $50.7\Omega + 4.1j\Omega$; Measurement impedance: $48.2\Omega + 3.1j\Omega$ (within 5Ω)

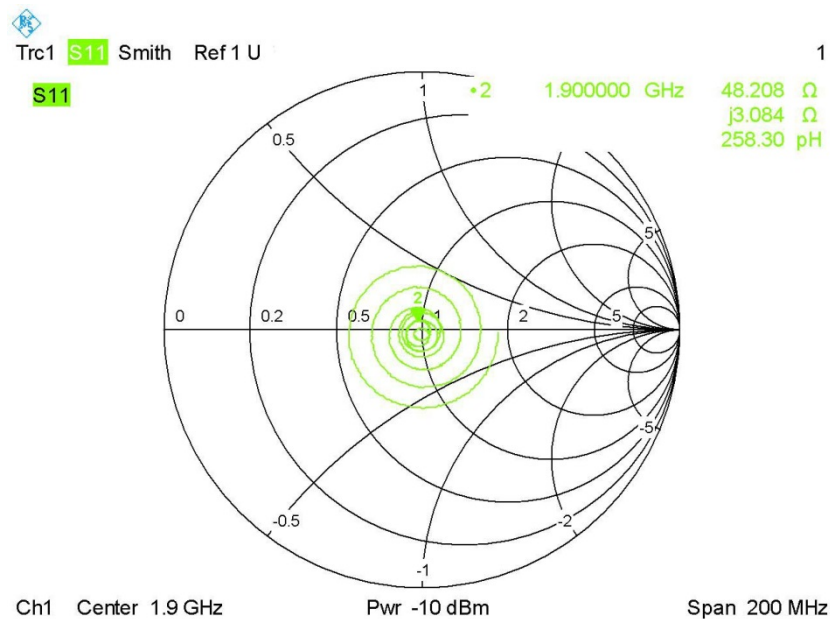


Calibrated return loss: -27.75dB; Measurement return loss: -28.32 dB(within 20%)

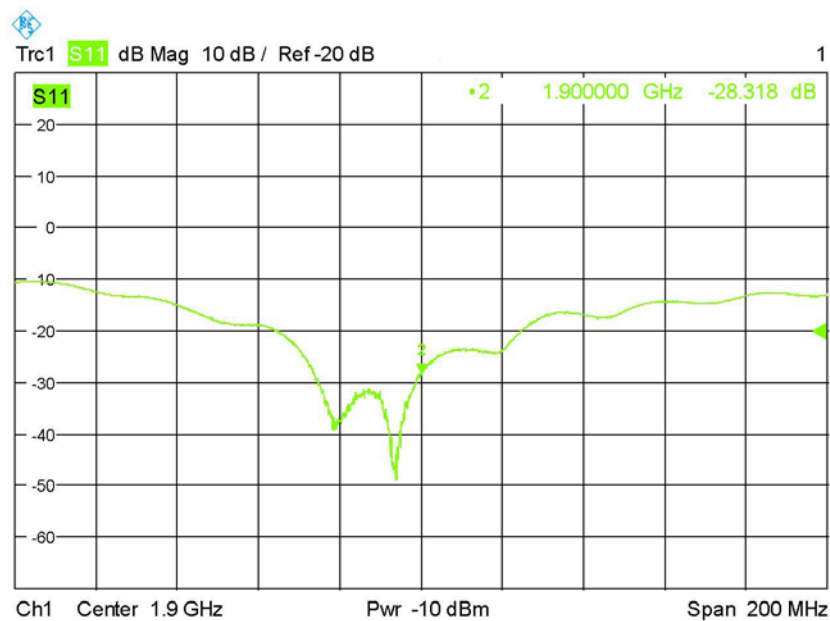


SN 46/11 DIP 2G450-189; 2450Head

Calibrated impedance: $49.8\Omega + 3.3j\Omega$; Measurement impedance: $51.9\Omega - 4.5j\Omega$ (within 5Ω)

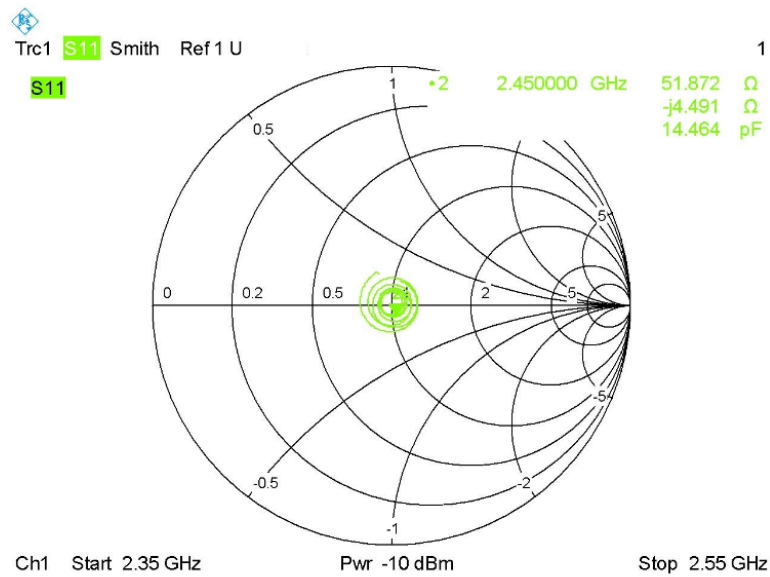


Calibrated return loss: -29.54dB; Measurement return loss: -29.55 dB(within 20%)

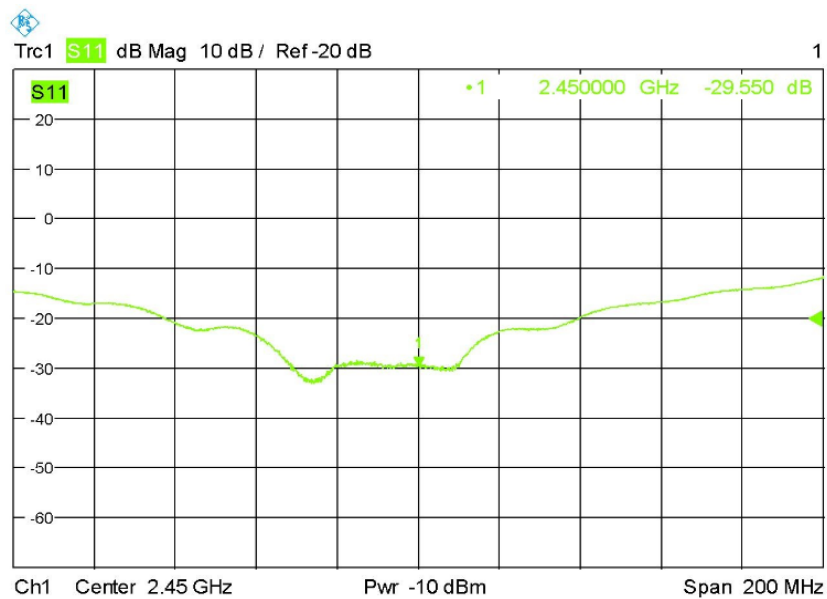

SN 47/14 DIP 2G600-342; 2600Head

Calibrated impedance: $55.5\Omega + 2.6j\Omega$; Measurement impedance: $57.7\Omega + 4.8j\Omega$ (within 5Ω)

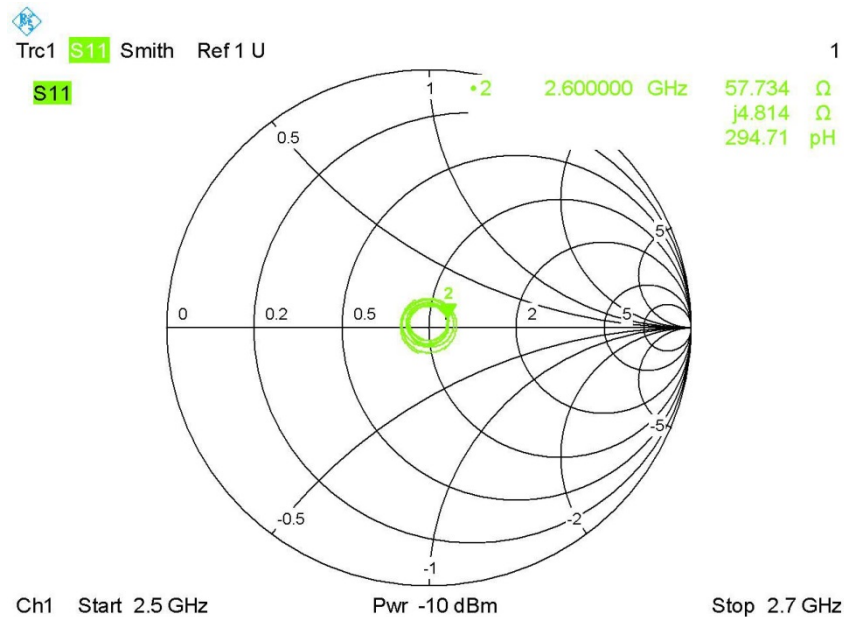

Calibrated return loss: -24.86dB; Measurement return loss: -23.18 dB(within 20%)

