

	MEDTRONIC CONFIDENTIAL THIS DOCUMENT IS THE PROPERTY OF MEDTRONIC, INC. AND MUST BE ACCOUNTED FOR. INFORMATION HEREIN IS CONFIDENTIAL. REVISION LEVELS ARE ELECTRONICALLY CONTROLLED. DO NOT REPRODUCE IT, REVEAL IT TO UNAUTHORIZED PERSONS OR SEND IT OUTSIDE MEDTRONIC WITHOUT PROPER AUTHORIZATION.	p. 1 of 5
		Doc. No.
		M961404A
TITLE	DEVICE REGULATORY LABEL MODEL 24970A	REV E

REVISION	DESCRIPTION
A	Initial release
B	Add tab -002 artwork. Revise note 7 add use-before-date requirement.
C	Add tab -003 artwork. Revise note 3 to change label background and graphic colors.
D	Add Pantone equivalent colors to Lab color callouts.
E	Release tabs -004 and -005 artwork. Tab -004 implements new the TUV NRTL marking and Tab -005 removes the CE mark.


1.0 SCOPE

This specification shall identify the procurement source for Device Regulatory Label for the Model 24970A Programmer.

2.0 COMPONENT IDENTIFICATION

1. Material: (.005") Thick velvet matte finish polycarbonate with PSA adhesive. Overall thickness excluding release liner (.007") nominal.
2. Adhesive: (.002") thick Acrylic PSA, 3M 467MP or Medtronic approved equivalent.
3. Colors: Background – Light Gray per *Lab* Color Space L:73, A:-1, B:-1 or equivalent Pantone Cool Gray 5 C. Graphics – Navy Blue L:15, A:2, B:-20 or equivalent Pantone 533C. Medtronic Logo is Medtronic Blue L:31, A:-2, B:- 40 or equivalent Pantone 2154 C.
4. See graphics file for artwork. Refer to associated artwork file (.eps file).
5. Packaging Kiss-cut on sheets with waste removed or die cut individual labels with release liner pull tab. Bulk package as to prevent damage and packaging waste.
6. All dimensions in View 1 are in inches unless otherwise noted. Tolerances are +/- .010".
7. Identify each label package with the Use-Before-Date and Part Number at a minimum. Shelf life expectation is one year.
8. All borders and window/s are represented by line-art. See the supplied artwork. Cut back the adhesive layer approx. (.040") REF. from window border. No adhesive allowed in window area.
9. This component to be RoHS compliant with restrictions on hazardous substances.

View 1 – Dimensions – (not to scale)

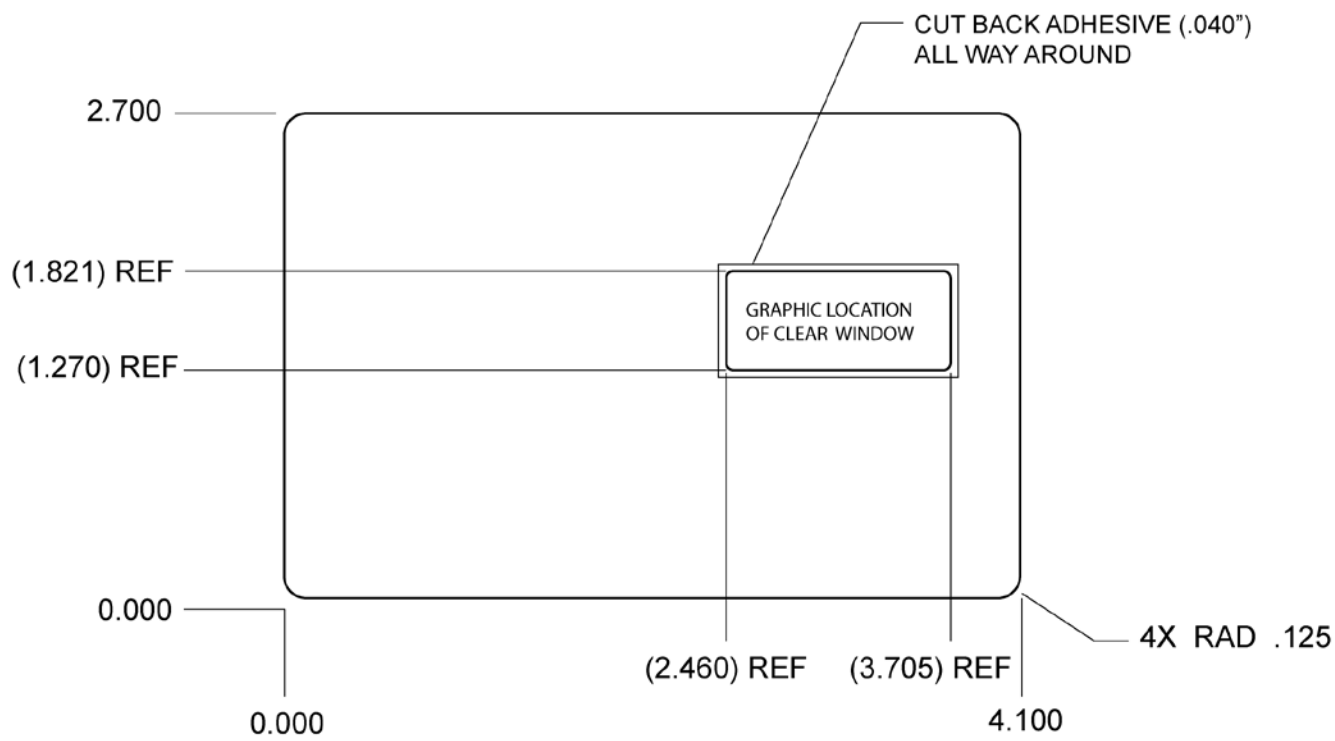

View 2 – Artwork Tabs (Reference use only not to scale)

TAB -001

 Model 24970A		 Medtronic, Inc. 710 Medtronic Parkway Minneapolis, MN 55432 USA	 Medtronic B.V. Earl Bakkenstraat 10 6422 PJ Heerlen The Netherlands
CE0123 Medical Electrical Equipment   IPX0    USA Rx Only  P/N: XXXXXXXXXXXX Input: Voltage 5V --- 3.0A		Made in Malaysia    XXX-XXXXXX  FCC ID: LF524970A CONTAINS FCC ID: T7V1316 IC: 3408D-24970A CONTAINS IC: 216Q-1316 This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.	

TAB -002

 Model 24970A		 Medtronic 710 Medtronic Parkway Minneapolis, MN 55432 USA	 Medtronic B.V. Earl Bakkenstraat 10 6422 PJ Heerlen The Netherlands
CE0123 Medical Electrical Equipment   IPX0    USA Rx Only  P/N: MENB1020A0540XXX Input: Voltage 5V --- 3.0A		Made in Malaysia    XXX-XXXXXX  FCC ID: LF524970A CONTAINS FCC ID: T7V1316 IC: 3408D-24970A CONTAINS IC: 216Q-1316 This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.	

TAB -003

 Model 24970A	Property of Medtronic, Inc.  Medtronic, Inc. 710 Medtronic Parkway Minneapolis, MN 55432 USA  Medtronic B.V. Earl Bakkenstraat 10 6422 PJ Heerlen The Netherlands
CE0123 Medical Electrical Equipment   IP2X   USA Rx Only  P/N: ME20A0540F03 Input: Voltage 5V --- 3.0A	   Made in Malaysia  FCC ID: LF524970A CONTAINS FCC ID: T7V1316 IC: 3408D-24970A CONTAINS IC: 216Q-1316 This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

TAB -004

 Model 24970A	Property of Medtronic, Inc.  Medtronic, Inc. 710 Medtronic Parkway Minneapolis, MN 55432 USA  Medtronic B.V. Earl Bakkenstraat 10 6422 PJ Heerlen The Netherlands
CE0123 Medical Electrical Equipment   IP2X   USA Rx Only  P/N: ME20A0540F03 Input: Voltage 5V --- 3.0A	   Made in Malaysia  FCC ID: LF524970A CONTAINS FCC ID: T7V1316 IC: 3408D-24970A CONTAINS IC: 216Q-1316 This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

TAB -005

 Model 24970A		Property of Medtronic, Inc.  Medtronic, Inc. 710 Medtronic Parkway Minneapolis, MN 55432 USA		 EC REP Medtronic B.V. Earl Bakkenstraat 10 6422 PJ Heerlen The Netherlands	
Medical Electrical Equipment  C US		   Made in Malaysia		 FCC ID: LF524970A CONTAINS FCC ID: T7V1316 IC: 3408D-24970A CONTAINS IC: 216Q-1316	
  IP2X  MR  10°C 50°F 35°C 95°F				This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.	
 ! USA Rx Only  P/N: ME20A0540F03 Input: Voltage 5V --- 3.0A					

3.0 HANDLING REQUIREMENT

The manufacturer shall package and ship the component parts in a manner designed for protection from physical damage and, if electrically susceptible, from electrostatic discharge.

4.0 NOTIFICATION OF CHANGE

Upon approval by Medtronic, Inc. of the initial design, any part, process changes or deviations considered by the manufacturer must be submitted to Medtronic, Inc. In writing for review, the information submitted should include a complete description of the change and effect the change will have on all characteristics of the device, material and /or process.

5.0 COMPLETION

This paragraph concludes this specification.

