



**Impedance Plot for D2450V2-SN: 968**  
**2450 Head**

Calibrated impedance:  $51.9\Omega + 3.63j\Omega$ ; Measurement impedance:  $50.4\Omega - 3.7j\Omega$  (within  $5\Omega$ )

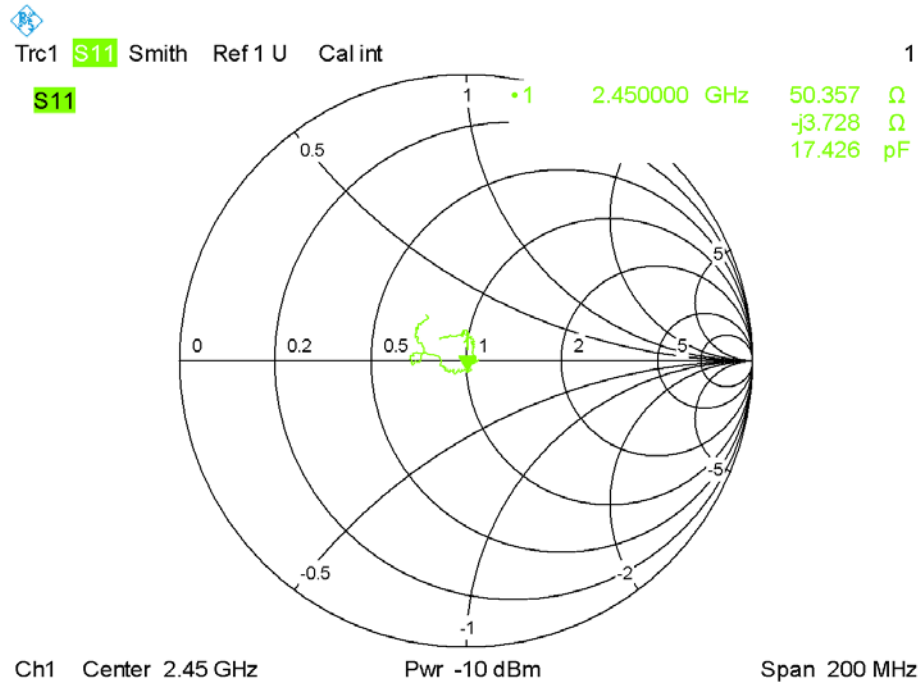

Date: 21.FEB.2024 19:04:46

Calibrated return loss: -27.9dB; Measurement return loss: -24.44dB (within 20%)

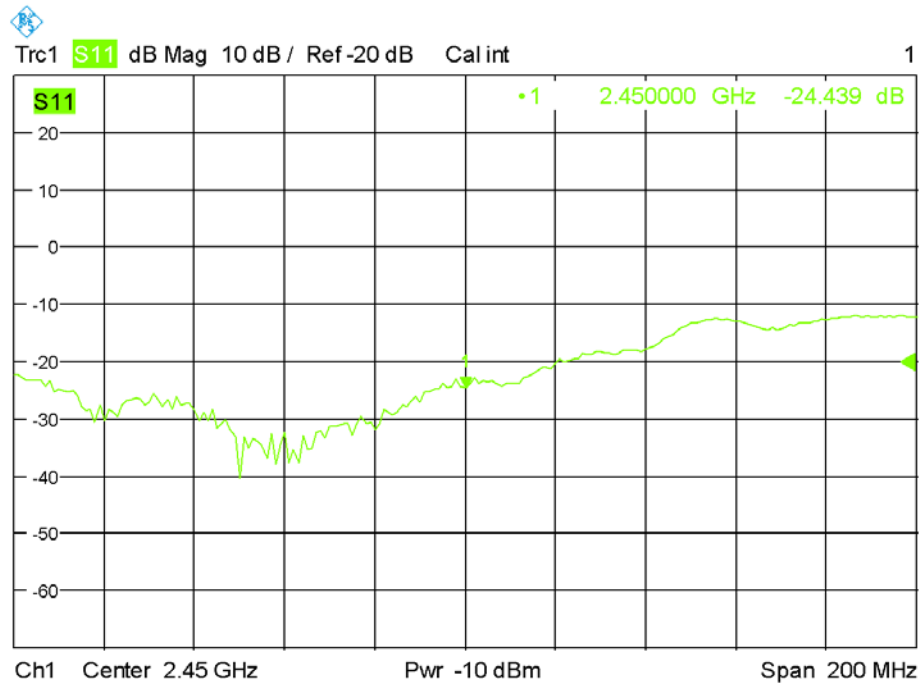

Date: 21.FEB.2024 19:04:29