

Appendix

Photographs of Test Setup

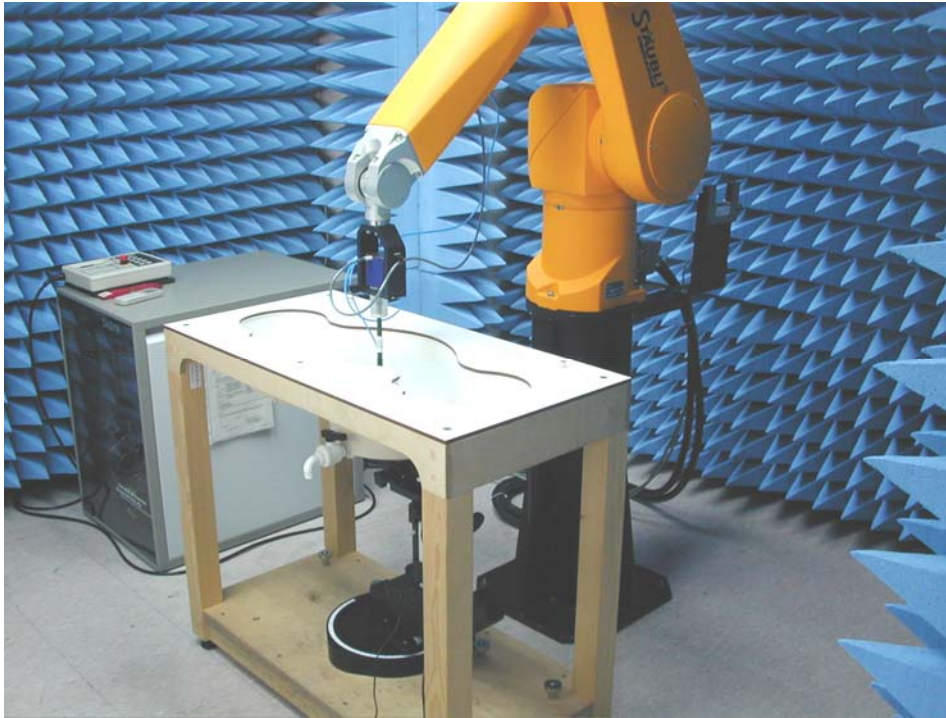


Fig.1 Photograph of the SAR measurement System

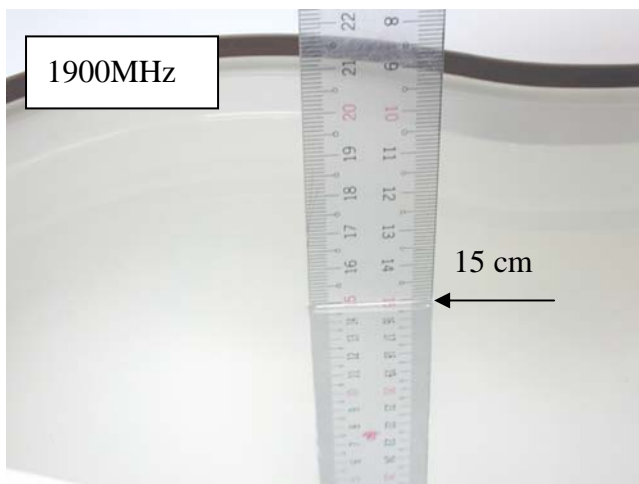


Fig.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side



Fig.3 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

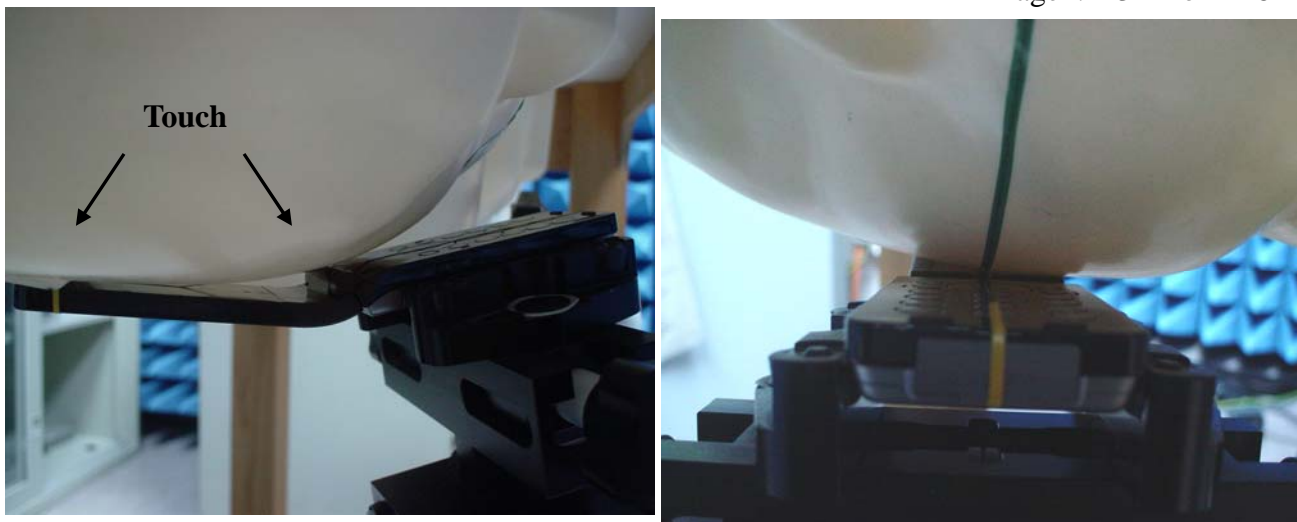


Fig.4 Right Head Section / Cheek-Touch Position

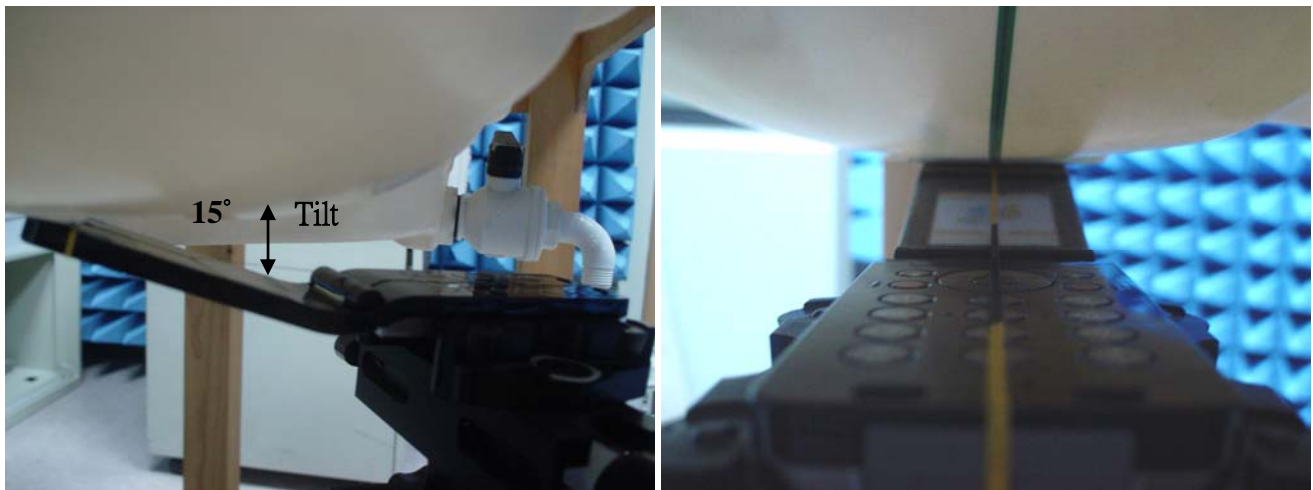


Fig.5 Right Head Section / Ear-Tilt Position(15°)

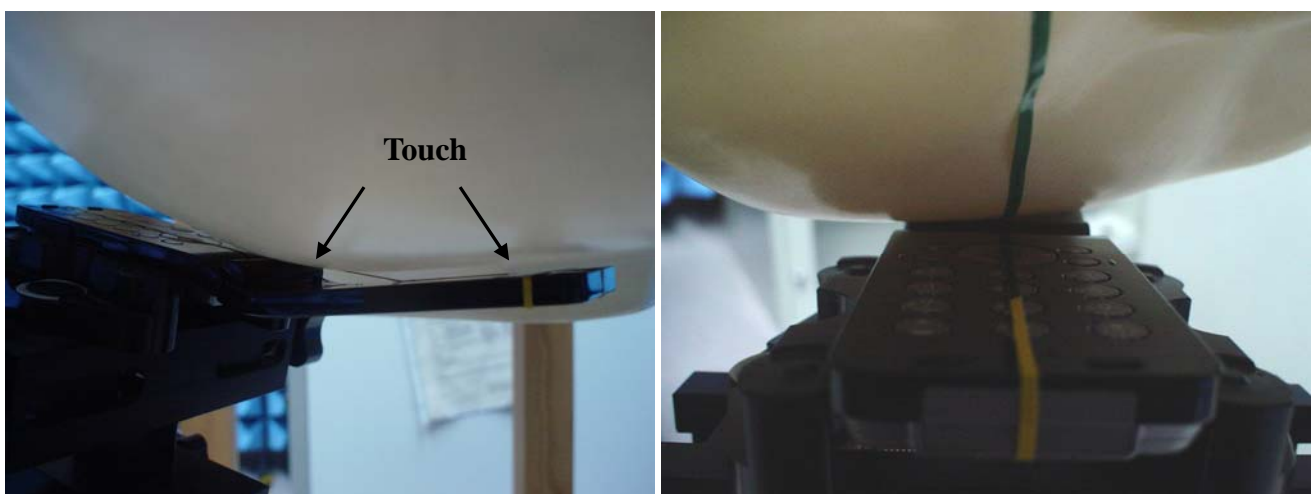


Fig.6 Left Head Section / Cheek-Touch Position



Fig.7 Left Head Section / Ear-Tilt Position(15°)

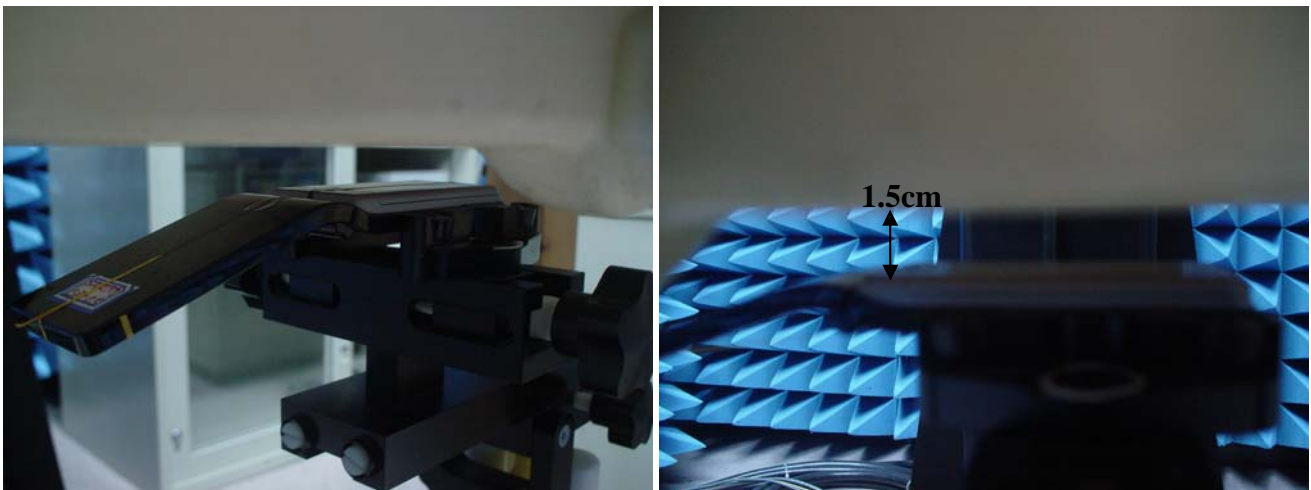


Fig.8 Body Section (Testing in GPRS Mode)