



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details






1. SAR measurement System





2. Photographs of Tissue Simulate Liquid

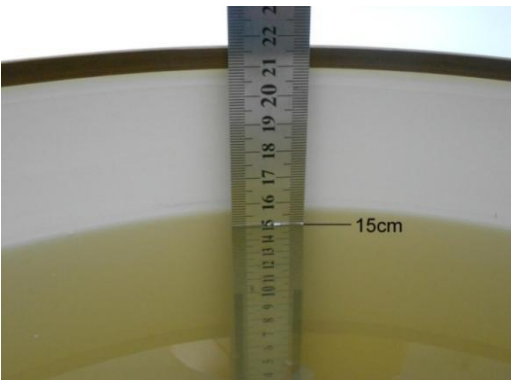Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2600	
	





3. Photographs of EUT test position

Photo 6: Left touch cheek

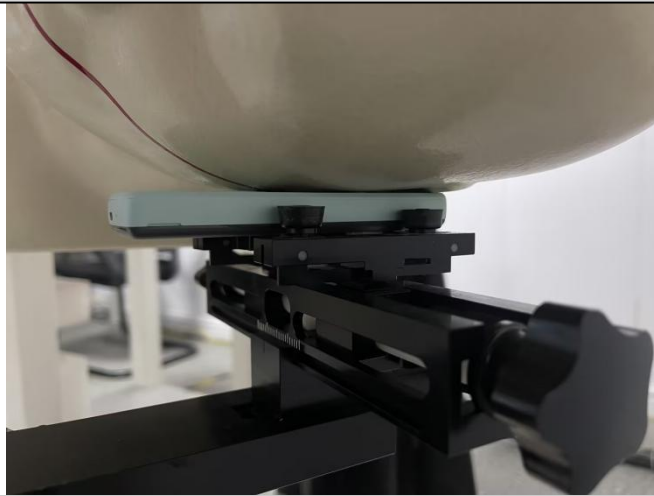


Photo 7: Left tilted 15 degree

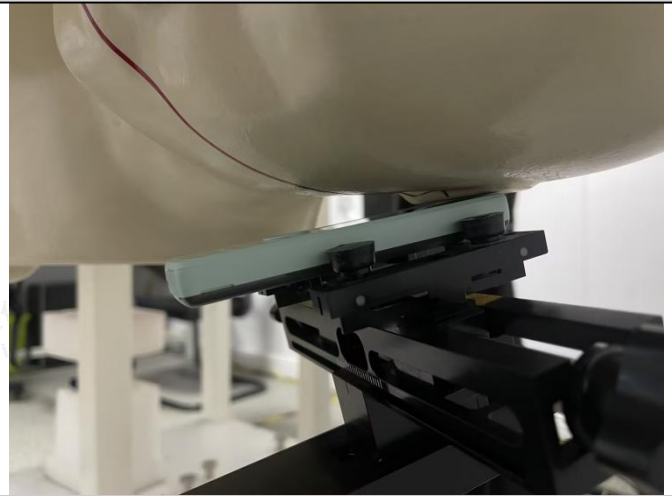


Photo 8: Right touch cheek

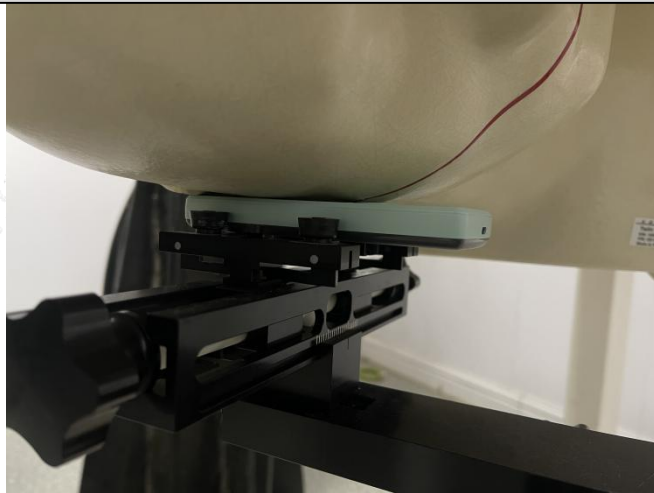


Photo 9: Right tilted 15 degree

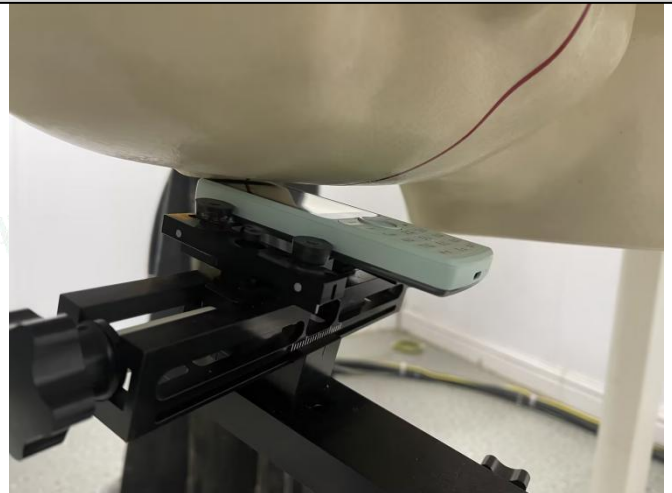


Photo 10: Front side 10mm



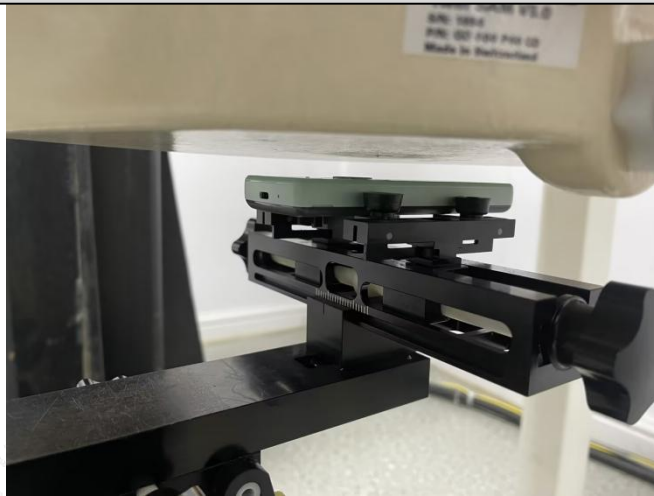


Photo 11: Back side 10mm



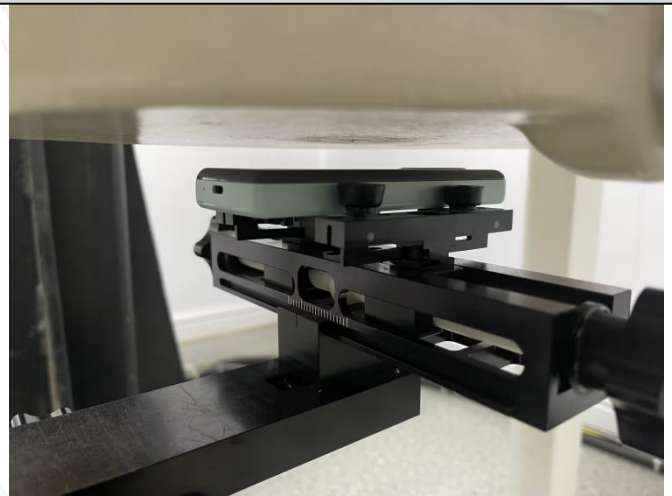

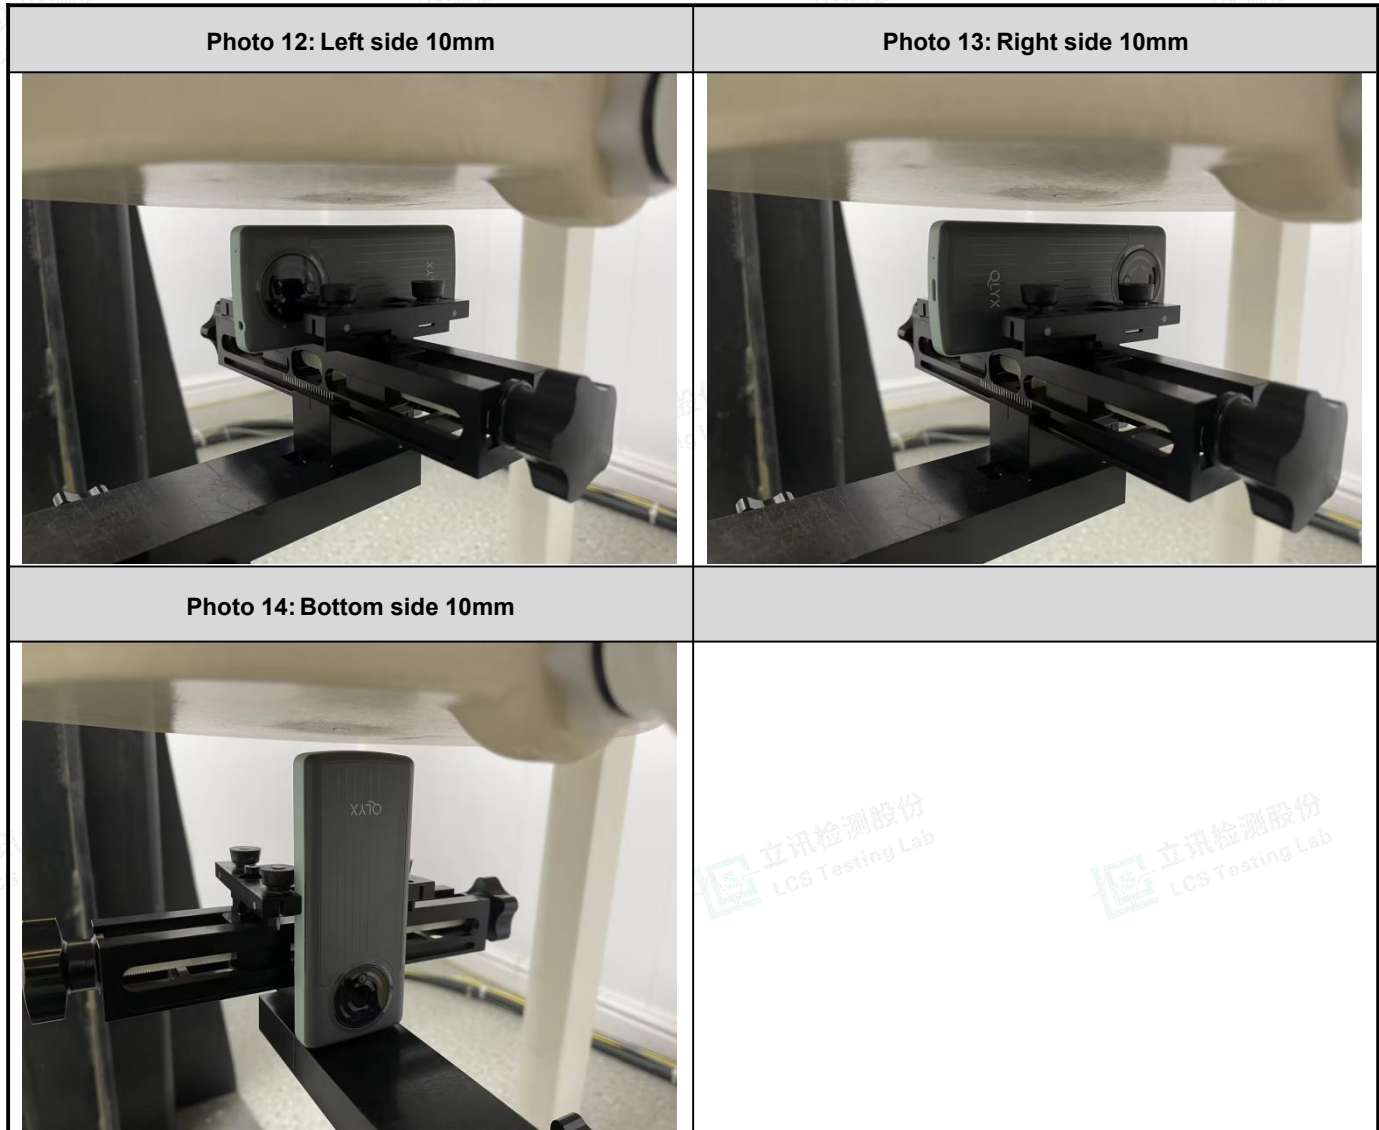

4. EUT Constructional Details

