

# Medtronic MiniMed

TEST REPORT FOR

**GST3C**

**Model: MMT-7811XNA**

**Tested To The Following Standard:**

**FCC Part 15 Subpart C Section(s)**

**15.247**

**(DTS 2400-2483.5 MHz)**

**Report No.: 98227-12**

**Date of issue: March 22, 2016**



This test report bears the accreditation symbol indicating that the testing performed herein meets the test and reporting requirements of ISO/IEC 17025 under the applicable scope of EMC testing for CKC Laboratories, Inc.

We strive to create long-term, trust based relationships by providing sound, adaptive, customer first testing services. We embrace each of our customers' unique EMC challenges, not as an interruption to set processes, but rather as the reason we are in business.

## TABLE OF CONTENTS

Administrative Information .....	3
Test Report Information .....	3
Report Authorization .....	3
Test Facility Information .....	4
Software Versions .....	4
Site Registration & Accreditation Information .....	4
Summary of Results .....	5
Modifications During Testing .....	5
Conditions During Testing .....	5
Equipment Under Test .....	6
General Product Information .....	6
FCC Part 15 Subpart C .....	7
15.247(a)(2) 6dB Bandwidth .....	7
15.247(b)(3) Output Power .....	12
15.247(e) Power Spectral Density .....	18
15.247(d) Radiated Emissions & Band Edge .....	24
Supplemental Information .....	39
Measurement Uncertainty .....	39
Emissions Test Details .....	39

## ADMINISTRATIVE INFORMATION

### Test Report Information

**REPORT PREPARED FOR:**

Medtronic MiniMed  
18000 Devonshire Street  
Northridge, CA 91325-1219

**REPORT PREPARED BY:**

Terri Rayle  
CKC Laboratories, Inc.  
5046 Sierra Pines Drive  
Mariposa, CA 95338

REPRESENTATIVE: Bob Vitti  
Customer Reference Number: 4500110418

Project Number: 98227

**DATE OF EQUIPMENT RECEIPT:**

February 19, 2016

**DATE(S) OF TESTING:**

February 19-21, 2016

### Report Authorization

The test data contained in this report documents the observed testing parameters pertaining to and are relevant for only the sample equipment tested in the agreed upon operational mode(s) and configuration(s) as identified herein. Compliance assessment remains the client's responsibility. This report may not be used to claim product endorsement by A2LA or any government agencies. This test report has been authorized for release under quality control from CKC Laboratories, Inc.

A handwritten signature in black ink, reading "Steve Behm", is positioned above a horizontal line.

**Steve Behm**  
**Director of Quality Assurance & Engineering Services**  
**CKC Laboratories, Inc.**

## Test Facility Information



Our laboratories are configured to effectively test a wide variety of product types. CKC utilizes first class test equipment, anechoic chambers, data acquisition and information services to create accurate, repeatable and affordable test results.

TEST LOCATION(S):  
CKC Laboratories, Inc.  
22116 23rd Drive S.E., Suite A  
Bothell, WA 98021-4413

## Software Versions

CKC Laboratories Proprietary Software	Version
EMITest Emissions	5.03.02

## Site Registration & Accreditation Information

Location	CB #	TAIWAN	CANADA	FCC	JAPAN
Bothell	US0081	SL2-IN-E-1145R	3082C-1	318736	A-0148

## SUMMARY OF RESULTS

### Standard / Specification: FCC Part 15 Subpart C - 15.247 (DTS)

Test Procedure	Description	Modifications	Results
15.247(a)(2)	6dB Bandwidth	NA	Pass
15.247(b)(3)	Output Power	NA	Pass
15.247(e)	Power Spectral Density	NA	Pass
15.247(d)	RF Conducted Emissions & Band Edge	NA	NA2
15.247(d)	Radiated Emissions & Band Edge	NA	Pass
15.207	AC Conducted Emissions	NA	NA1

NA = Not Applicable

NA1 = Not Applicable because the EUT is only battery operated.

NA2 = Not Applicable because the EUT does not have an antenna connector.

## Modifications During Testing

This list is a summary of the modifications made to the equipment during testing.

Summary of Conditions
No modifications were made during testing.

**Modifications listed above must be incorporated into all production units.**

## Conditions During Testing

This list is a summary of the conditions noted to the equipment during testing.

Summary of Conditions
None

## EQUIPMENT UNDER TEST (EUT)

During testing numerous configurations may have been utilized. The configurations listed below support compliance to the standard(s) listed in the Summary of Results section.

### Configuration 1

#### *Equipment Tested:*

Device	Manufacturer	Model #	S/N
GST3C	Medtronic MiniMed	MMT-7811XNA	GT6023231M

#### *Support Equipment:*

Device	Manufacturer	Model #	S/N
None			

## General Product Information:

Product Information	Manufacturer-Provided Details
Equipment Type:	Stand-Alone Equipment
Type of Wideband System:	802.15.4
Operating Frequency Range:	2420-2480MHz
Modulation Type(s):	QPSK, Chip Rate 2000 kchip/s, bit rate 250 kb/s
Maximum Duty Cycle:	52%
Number of TX Chains:	1
Antenna Type(s) and Gain:	Integral Folded Monopole 0dBi
Beamforming Type:	NA
Antenna Connection Type:	Integral
Nominal Input Voltage:	3.7V Battery
Firmware / Software used for Test:	Continuously Modulated Software

## FCC Part 15 Subpart C

### 15.247(a)(2) 6dB Bandwidth


Test Setup/Conditions			
Test Location:	Bothell Lab C3	Test Engineer:	S. Pittsford
Test Method:	ANSI C63.10 (2013), KDB 558074 D01 DTS Meas Guidance v03r04 Jan 7 <sup>th</sup> , 2016	Test Date(s):	2/19/2016
Configuration:	1		
Test Setup:	<p>Firmware power setting: Max Power EUT Firmware: Continuous Modulation Software Modulation: QPSK</p> <p>Antenna type: Integral Monopole Dipole Antenna Gain : 0.0 dBi. Frequency tested: 2420MHz, 2450MHz &amp; 2480MHz</p> <p>Duty Cycle: 100%</p> <p>Test Mode: Continuously modulated Setup: The EUT is set on a Styrofoam test bench centered on the turntable. The EUT is oriented in X, Y &amp; Z axis with only the worst case reported. The EUT has a fully charged battery.</p>		

Environmental Conditions			
Temperature (°C)	22	Relative Humidity (%):	42

Test Equipment					
Asset#	Description	Manufacturer	Model	Cal Date	Cal Due
02872	Spectrum Analyzer	Agilent	E4440A	11/18/2015	11/18/2017
P06540	Cable	Andrews	Helix	10/29/2015	10/29/2017
03540	Preamplifier	HP	83017A	4/30/2015	4/30/2017
01467	Horn Antenna	EMCO	3115	8/12/2015	8/12/2017
P05305	Cable	Andrews	ETSI-50T	2/15/2016	2/15/2018


Test Data Summary					
Frequency (MHz)	Antenna Port	Modulation	Measured (kHz)	Limit (kHz)	Results
2420	1	QPSK	1596	≥500	Pass
2450	1	QPSK	1591	≥500	Pass
2480	1	QPSK	1583	≥500	Pass

## Plots

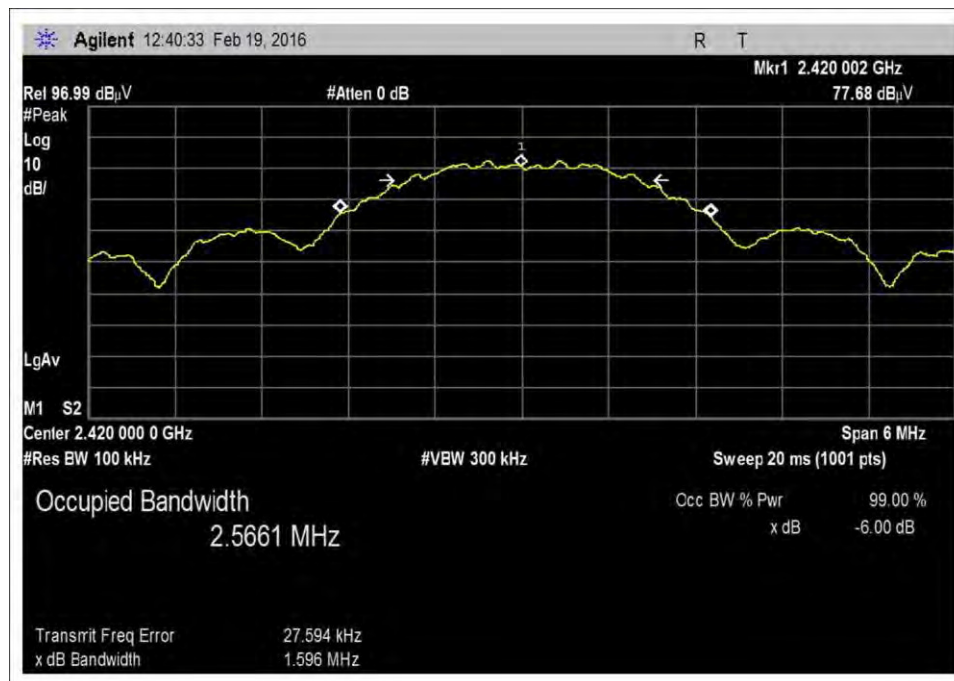


Low



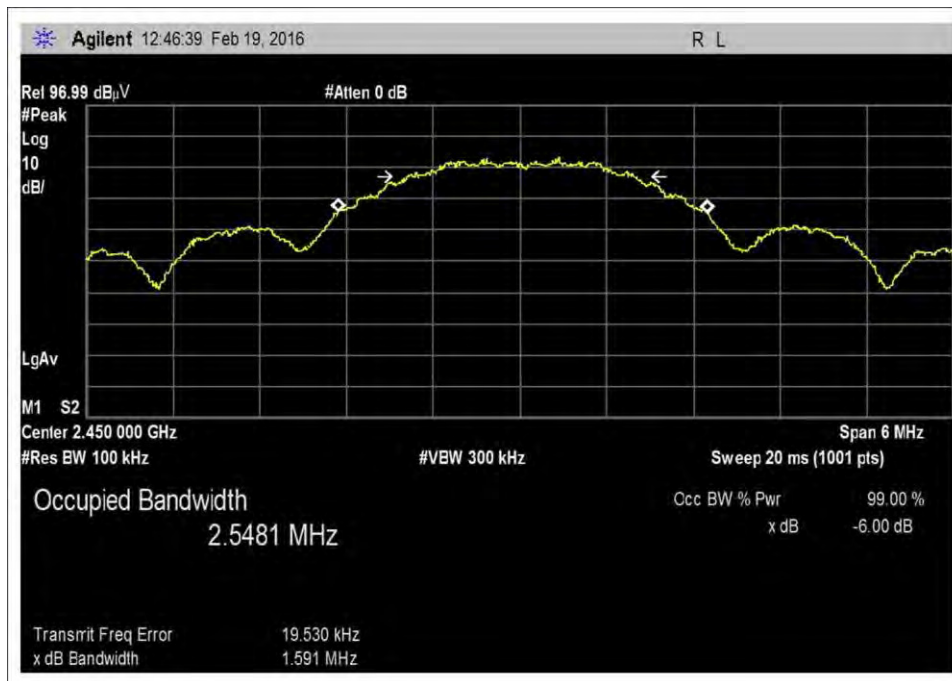

Middle

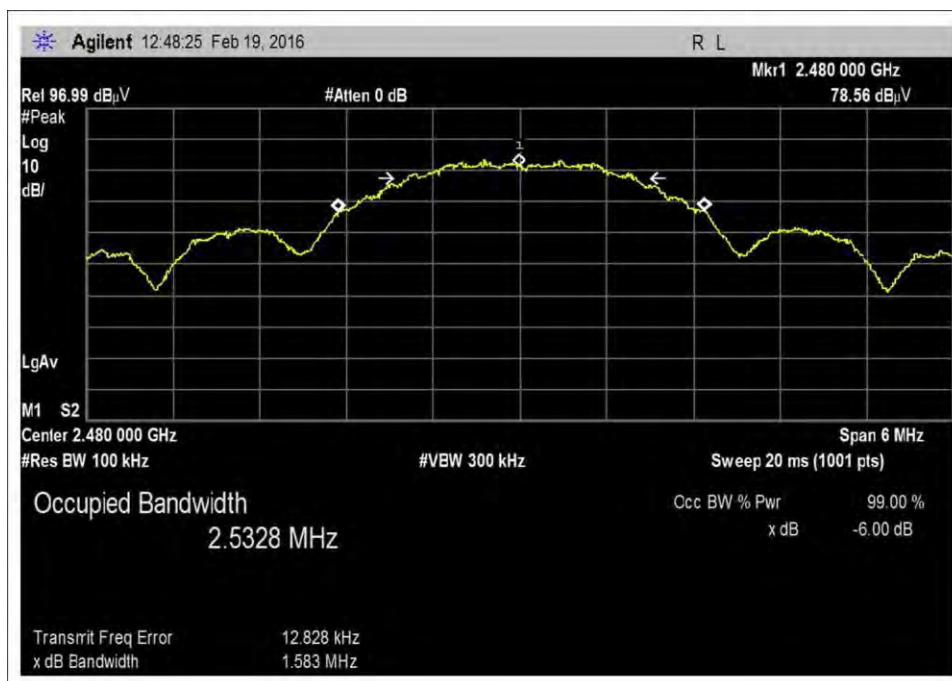

High

**Test Setup Photos**



Above 1GHz



X Axis



Y Axis



Z Axis

## 15.247(b)(3) Output Power

### Test Setup / Conditions / Data

Test Location: CKC Laboratories, Inc. • 22116 23rd Dr. SE, Suite A • Bothell, WA 98021 • (425) 402-1717  
 Customer: **Medtronic MiniMed**  
 Specification: **15.247(b) Power Output (2400-2483.5 MHz DTS)**  
 Work Order #: **97869** Date: 2/21/2016  
 Test Type: **Maximized Emissions** Time: 09:20:47  
 Tested By: Steven Pittsford Sequence#: 4  
 Software: EMITest 5.03.02

#### Equipment Tested:

Device	Manufacturer	Model #	S/N
Configuration 1			

#### Support Equipment:

Device	Manufacturer	Model #	S/N
Configuration 1			

#### Test Conditions / Notes:

Test Method: ANSI C63.10 (2013) & KDB 558074 D01 DTS Meas Guidance v03r04 Jan 7th, 2016

Frequency tested: 2420MHz, 2450MHz & 2480MHz  
 Firmware power setting: Max Power  
 EUT Firmware: Continuous Modulation Software  
 Modulation: QPSK


Antenna type: Integral Monopole Dipole  
 Antenna Gain : 0.0 dBi.

Duty Cycle: 100%

Test Mode: Continuously modulated  
 Setup: The EUT is set on a Styrofoam test bench centered on the turntable.  
 The EUT is oriented in X, Y & Z axis with only the worst case reported.  
 The EUT has a fully charged battery.  
 Corrections due to antennas cables and amplifiers are added as an offset in the Spectrum Analyzer screen captures.

Environmental Conditions  
 Temperature: 22°C  
 Relative Humidity: 40%

Medtronic MiniMed W/O#: 97869 Sequence#: 4 Date: 2/21/2016  
15.247(b) Power Output (2400-2483.5 MHz DTS) Test Distance: 3 Meters Vert & Horz

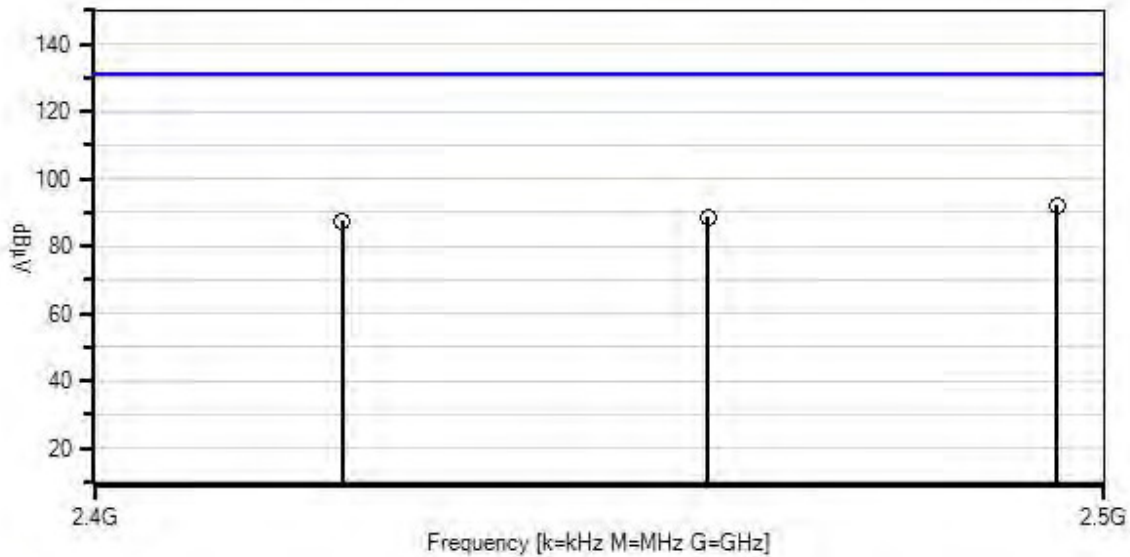

— Readings  
× QP Readings  
▼ Ambient  
○ Peak Readings  
\* Average Readings  
Software Version: 5.03.02  
1 - 15.247(b) Power Output (2400-2483.5 MHz DTS)

#### Test Equipment:

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	ANP06540	Cable	Heliax	10/29/2015	10/29/2017
T2	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T3	AN03540	Preamp	83017A	4/30/2015	4/30/2017
T4	AN01467	Horn Antenna- ANSI C63.5 Calibration	3115	8/12/2015	8/12/2017
T5	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018

#### Measurement Data:

Reading listed by margin.

Test Distance: 3 Meters

#	Freq	Rdng	T1 T5	T2	T3	T4	Dist	Corr	Spec	Margin	Polar
	MHz	dBμV	dB	dB	dB	dB	Table	dBμV	dBμV	dB	Ant
1	2479.490M	95.5	+0.6 +2.9	+0.0	-34.5	+27.7	+0.0 42	92.2	131.2	-39.0	Vert 145
2	2450.390M	92.0	+0.6 +2.9	+0.0	-34.5	+27.7	+0.0 22	88.7	131.2	-42.5	Vert 153
3	2420.280M	90.9	+0.6 +2.8	+0.0	-34.6	+27.7	+0.0 31	87.4	131.2	-43.8	Vert 164



### Test Data Summary - Radiated Measurement

Measurement Option: RBW > DTS Bandwidth

Frequency (MHz)	Modulation	Ant. Type / Gain (dBi)	Field Strength (dBuV/m @3m)	Calculated (dBm)	Limit (dBm)	Results
2420	QPSK	0	87.4	-7.829	≤30	Pass
2450	QPSK	0	88.7	-6.529	≤30	Pass
2480	QPSK	0	92.2	-3.029	≤30	Pass


Conducted RF output power calculated in accordance with ANSI C63.10.

$$P(W) = \frac{(E \cdot d)^2}{30 G}$$


Or equivalently, in logarithmic form:

$$P(\text{dBm}) = E(\text{dBuV/m}) + 20\text{LOG}(d) - G - 104.77$$


### Plots

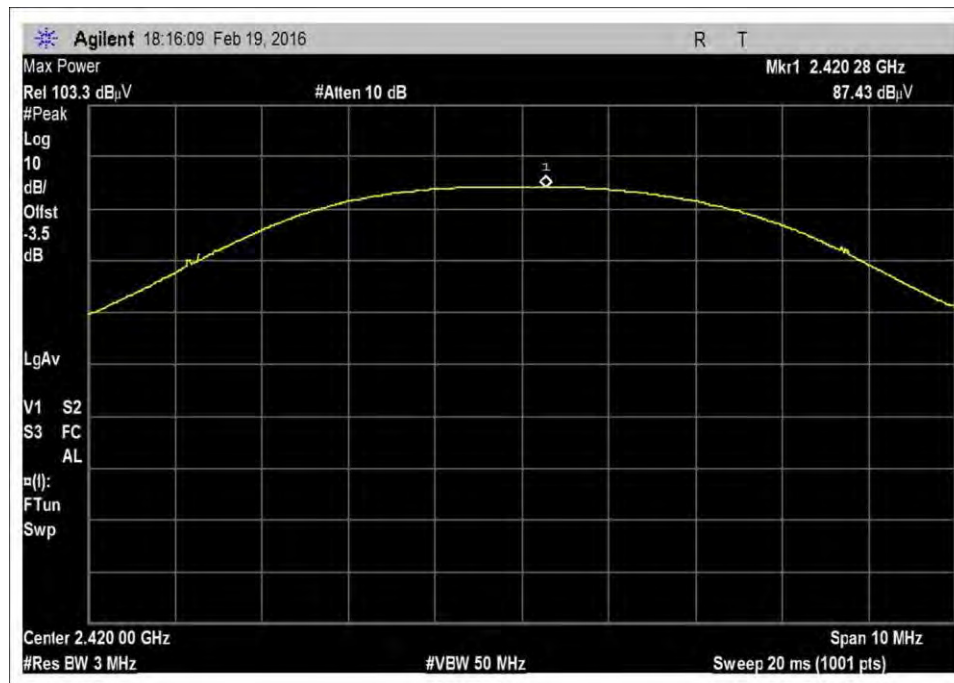

Low

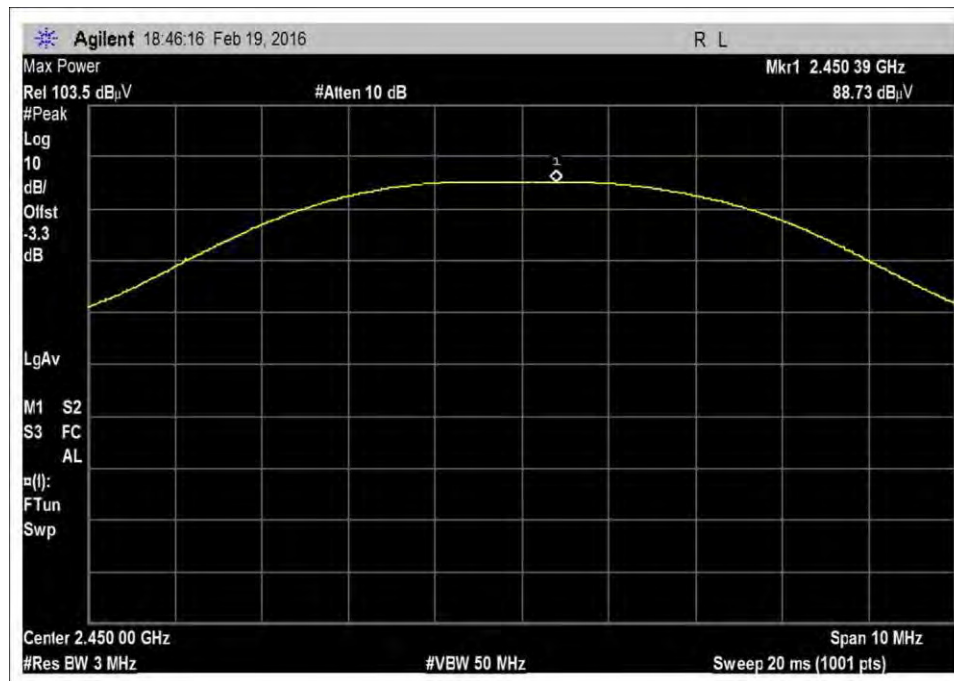

Middle

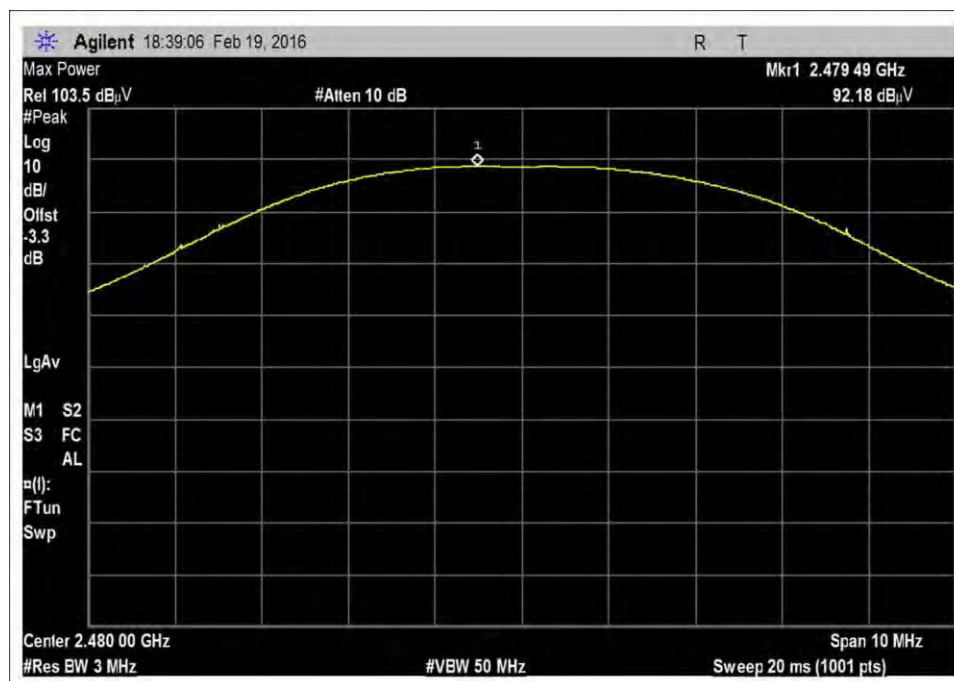

High

**Test Setup Photos**



Above 1GHz



X Axis





Y Axis



Z Axis

## 15.247(e) Power Spectral Density

### Test Setup / Conditions / Data

Test Location: CKC Laboratories, Inc. • 22116 23rd Dr. SE, Suite A • Bothell, WA 98021 • (425) 402-1717  
 Customer: **Medtronic MiniMed**  
 Specification: **15.247(e) Peak Power Spectral Density (2400-2483.5 MHz DTS)**  
 Work Order #: **97869** Date: 2/21/2016  
 Test Type: **Maximized Emissions** Time: 09:23:51  
 Tested By: Steven Pittsford Sequence#: 4  
 Software: EMITest 5.03.02

#### Equipment Tested:

Device	Manufacturer	Model #	S/N
Configuration 1			


#### Support Equipment:

Device	Manufacturer	Model #	S/N
Configuration 1			

#### Test Conditions / Notes:

Test Method: ANSI C63.10 (2013) & KDB 558074 D01 DTS Meas Guidance v03r04 Jan 7th, 2016  
  
 Frequency tested: 2420MHz, 2450MHz & 2480MHz  
 Firmware power setting: Max Power  
 EUT Firmware: Continuous Modulation Software  
 Modulation: QPSK  
  
 Antenna type: Integral Monopole Dipole  
 Antenna Gain : 0.0 dBi.  
  
 Duty Cycle: 100%  
  
 Test Mode: Continuously modulated  
 Setup: The EUT is set on a Styrofoam test bench centered on the turntable.  
 The EUT is oriented in X, Y & Z axis with only the worst case reported.  
 The EUT has a fully charged battery.  
 Corrections due to antennas cables and amplifiers are added as an offset in the Spectrum Analyzer screen captures.  
  
 Environmental Conditions  
 Temperature: 22°C  
 Relative Humidity: 40%

Medtronic MiniMed WQ#: 97869 Sequence#: 4 Date: 2/21/2016  
15.247(e) Peak Power Spectral Density (2400-2483.5 MHz DTS) Test Distance: None Vert & Horz

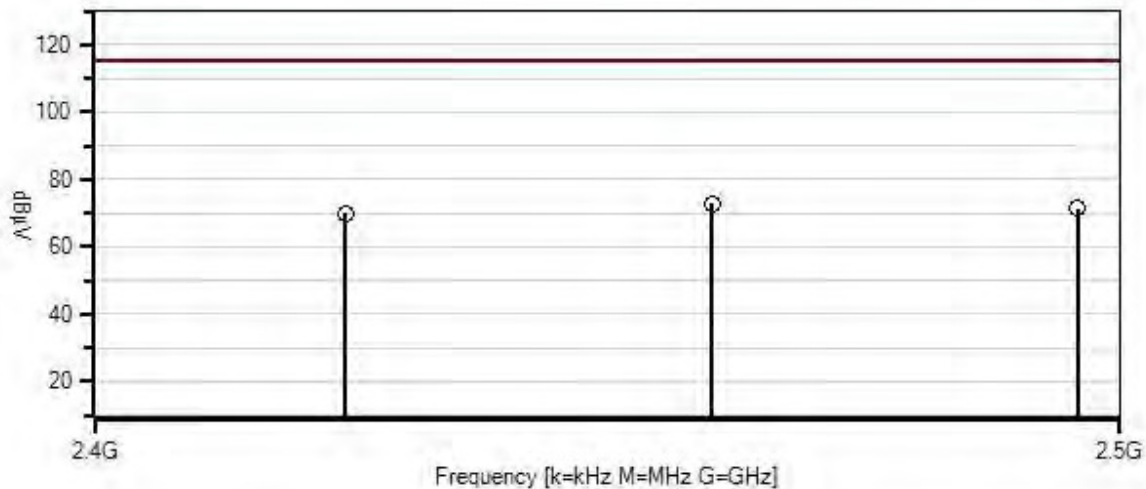

— Readings  
○ Peak Readings  
× QP Readings  
\* Average Readings  
▼ Ambient  
Software Version: 5.03.02  
— 1 - 15.247(e) Peak Power Spectral Density (2400-2483.5 MHz DTS)

**Test Equipment:**

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	ANP06540	Cable	Helix	10/29/2015	10/29/2017
T2	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T3	AN03540	Preamp	83017A	4/30/2015	4/30/2017
T4	AN01467	Horn Antenna- ANSI C63.5 Calibration	3115	8/12/2015	8/12/2017
T5	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018

**Measurement Data:**

Reading listed by margin.

Test Distance: None

#	Freq	Rdng	T1 T5	T2	T3	T4	Dist	Corr	Spec	Margin	Polar
	MHz	dBμV	dB	dB	dB	dB	Table	dBμV	dBμV	dB	Ant
1	2449.928M	76.2	+0.6 +2.9	+0.0	-34.5	+27.7	+0.0 22	72.9	115.0	-42.1	Vert 153
2	2480.000M	74.8	+0.6 +2.9	+0.0	-34.5	+27.7	+0.0 22	71.5	115.0	-43.5	Vert 153
3	2420.141M	73.4	+0.6 +2.8	+0.0	-34.6	+27.7	+0.0 33	69.9	115.0	-45.1	Vert 162

### Test Data Summary - Radiated Measurement

Measurement Method: PKPSD

Frequency (MHz)	Modulation	Ant. Type / Gain (dBi)	Field Strength (dBuV/m @3m)	Calculated (dBm/3kHz)	Limit (dBm/3kHz)	Results
2420	QPSK	0	69.9	-25.329	≤8	Pass
2450	QPSK	0	72.9	-22.329	≤8	Pass
2480	QPSK	0	71.5	-23.729	≤8	Pass


Conducted RF output power calculated in accordance with ANSI C63.10.

$$P(W) = \frac{(E \cdot d)^2}{30 G}$$


Or equivalently, in logarithmic form:

$$P(dBm) = E(dBuV/m) + 20LOG(d) - G - 104.77$$


### Plots

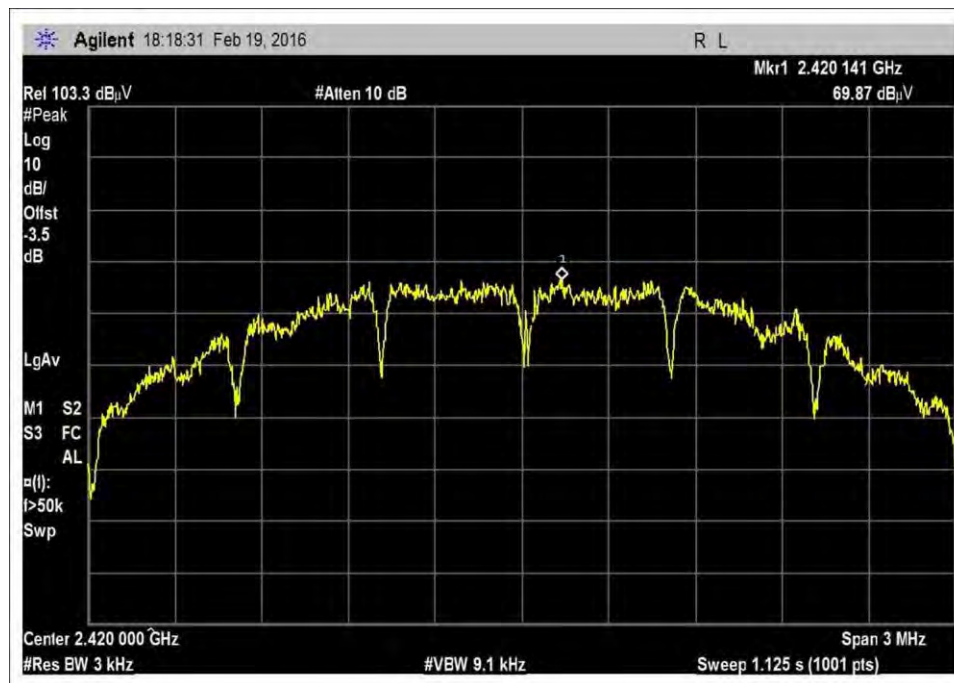

Low

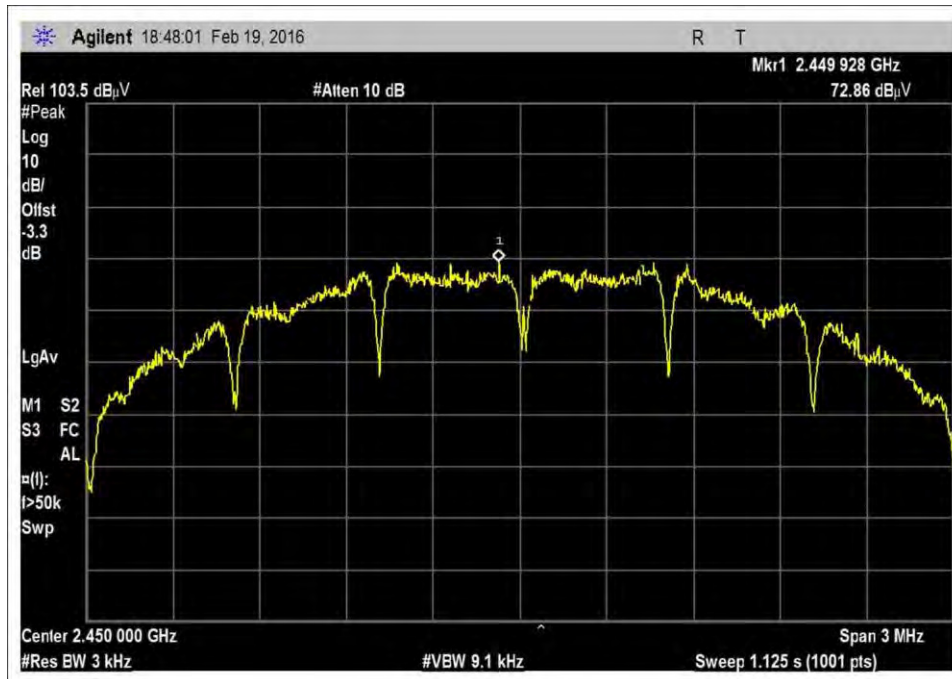

Middle

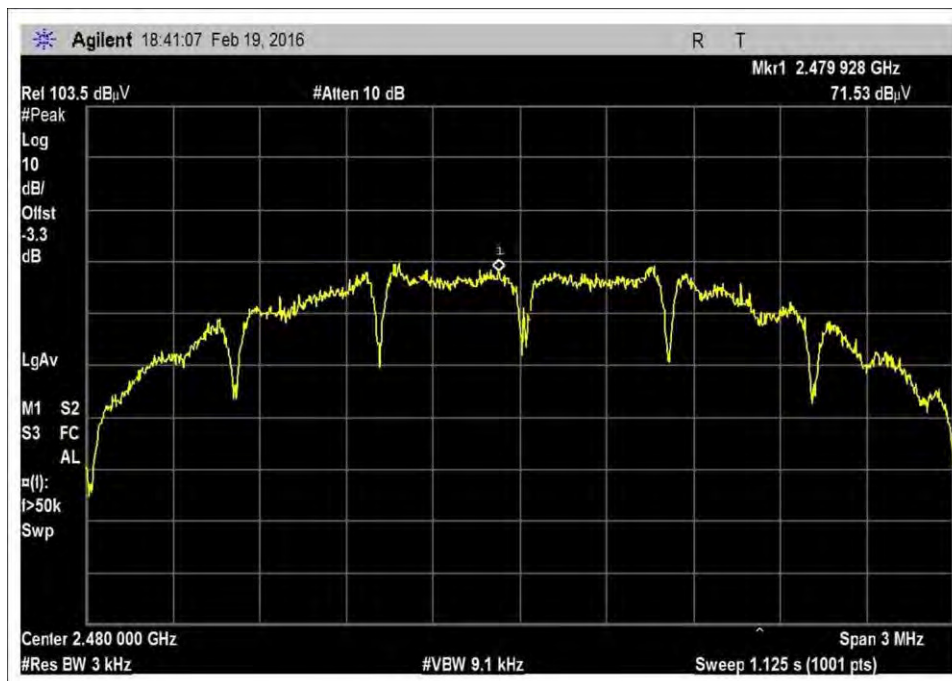

High



Test Setup Photos



Above 1GHz



X Axis



Y Axis



Z Axis

## 15.247(d) Radiated Emissions & Band Edge

### Test Setup / Conditions / Data

Test Location: CKC Laboratories, Inc. • 22116 23rd Dr. SE, Suite A • Bothell, WA 98021 • (425) 402-1717  
 Customer: **Medtronic MiniMed**  
 Specification: **15.247(d) / 15.209 Radiated Spurious Emissions**  
 Work Order #: **97869** Date: 2/21/2016  
 Test Type: **Maximized Emissions** Time: 13:43:51  
 Tested By: Steven Pittsford Sequence#: 4  
 Software: EMITest 5.03.02

#### Equipment Tested:

Device	Manufacturer	Model #	S/N
Configuration 1			

#### Support Equipment:

Device	Manufacturer	Model #	S/N
Configuration 1			

#### Test Conditions / Notes:

Test Method: ANSI C63.10 (2013) & KDB 558074 D01 DTS Meas Guidance v03r04 Jan 7th, 2016

Frequency Range: 9k-25GHz  
 Frequency tested: 2420MHz, 2450MHz & 2480MHz  
 Firmware power setting: Max Power  
 EUT Firmware: Continuous Modulation Software  
 Modulation: QPSK

Antenna type: Integral Monopole Dipole  
 Antenna Gain : 0.0 dBi.


Duty Cycle: 100%

Test Mode: Continuously modulated  
 Setup: The EUT is set on a Styrofoam test bench centered on the turntable.  
 The EUT is oriented in X, Y & Z axis with only the worst case reported.  
 The EUT has a fully charged battery.

Environmental Conditions  
 Temperature: 22°C  
 Relative Humidity: 37% to 40%



Medtronic MiniMed W/D#: 97869 Sequence#: 4 Date: 2/21/2016  
 15.247(d) / 15.209 Radiated Spurious Emissions Test Distance: 3 Meters Vert & Horz

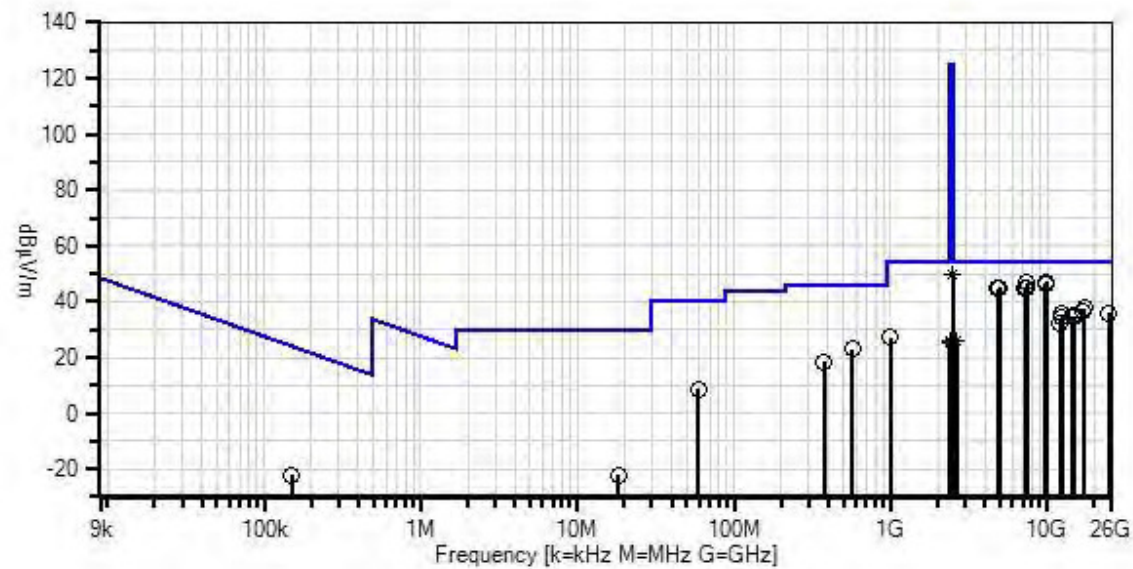

— Readings  
 × QP Readings  
 ▼ Ambient  
 — 1 - 15.247(d) / 15.209 Radiated Spurious Emissions

○ Peak Readings  
 \* Average Readings  
 Software Version: 5.03.02

**Test Equipment:**

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	ANP06540	Cable	Helix	10/29/2015	10/29/2017
	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T2	AN02741	Active Horn Antenna	AMFW-5F-12001800-20-10P	1/14/2015	1/14/2017
T3	AN02742	Active Horn Antenna	AMFW-5F-18002650-20-10P	1/14/2015	1/14/2017
T4	AN02763-69	Waveguide	Multiple	5/21/2014	5/21/2016
T5	AN03122	Cable	32026-2-29801-36	5/13/2014	5/13/2016
	ANP06678	Cable	32026-29801-29801-144	9/18/2014	9/18/2016
T6	AN03540	Preamp	83017A	4/30/2015	4/30/2017
T7	AN01467	Horn Antenna-ANSI C63.5 Calibration	3115	8/12/2015	8/12/2017
T8	AN02307	Preamp	8447D	2/15/2016	2/15/2018
T9	AN01996	Biconilog Antenna	CBL6111C	7/16/2014	7/16/2016
T10	ANP05360	Cable	RG214	12/1/2014	12/1/2016
T11	ANP05963	Cable	RG-214	2/21/2014	2/21/2016
T12	AN00052	Loop Antenna	6502	5/20/2014	5/20/2016
T13	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018

**Measurement Data:**

Reading listed by margin.

Test Distance: 3 Meters

#	Freq	Rdng	T1 T5 T9 T13	T2 T6 T10	T3 T7 T11	T4 T8 T12	Dist	Corr	Spec	Margin	Polar
	MHz	dB $\mu$ V	dB	dB	dB	dB	Table	dB $\mu$ V/m	dB $\mu$ V/m	dB	Ant
1	2483.500M	52.9	+0.6	+0.0	+0.0	+0.0	+0.0	49.6	54.0	-4.4	Vert
	Ave		+0.0	-34.5	+27.7	+0.0	42				145
			+0.0	+0.0	+0.0	+0.0					
			+2.9								
^	2483.500M	63.3	+0.6	+0.0	+0.0	+0.0	+0.0	60.0	54.0	+6.0	Vert
			+0.0	-34.5	+27.7	+0.0	42				145
			+0.0	+0.0	+0.0	+0.0					
			+2.9								
3	9920.485M	37.6	+1.3	+0.0	+0.0	+0.0	+0.0	47.0	54.0	-7.0	Vert
			+0.0	-35.2	+37.2	+0.0	360		High		153
			+0.0	+0.0	+0.0	+0.0					
			+6.1								
4	7438.380M	38.8	+1.3	+0.0	+0.0	+0.0	+0.0	46.8	54.0	-7.2	Vert
			+0.0	-34.7	+36.6	+0.0	360		High		159
			+0.0	+0.0	+0.0	+0.0					
			+4.8								

5	9680.505M	36.4	+1.5 +0.0 +0.0 +6.1	+0.0 -35.0 +0.0	+0.0 +37.3 +0.0	+0.0 +0.0 +0.0	46.3 198	54.0 Low	-7.7	Vert 156
6	9799.755M	36.2	+1.4 +0.0 +0.0 +6.1	+0.0 -35.1 +0.0	+0.0 +37.3 +0.0	+0.0 +0.0 +0.0	45.9 360	54.0 Mid	-8.1	Vert 150
7	7349.635M	37.6	+1.2 +0.0 +0.0 +4.7	+0.0 -34.6 +0.0	+0.0 +36.2 +0.0	+0.0 +0.0 +0.0	45.1 360	54.0 Mid	-8.9	Vert 161
8	4960.215M	41.1	+0.9 +0.0 +0.0 +4.4	+0.0 -34.2 +0.0	+0.0 +32.8 +0.0	+0.0 +0.0 +0.0	45.0	54.0 High	-9.0	Vert 155
9	4899.940M	41.0	+0.9 +0.0 +0.0 +4.4	+0.0 -34.2 +0.0	+0.0 +32.7 +0.0	+0.0 +0.0 +0.0	44.8 360	54.0 Mid	-9.2	Vert 161
10	7259.475M	37.6	+1.2 +0.0 +0.0 +4.6	+0.0 -34.5 +0.0	+0.0 +35.9 +0.0	+0.0 +0.0 +0.0	44.8 261	54.0 Low	-9.2	Vert 156
11	4839.895M	40.9	+0.9 +0.0 +0.0 +4.3	+0.0 -34.2 +0.0	+0.0 +32.7 +0.0	+0.0 +0.0 +0.0	44.6 360	54.0 Low	-9.4	Vert 161
12	17362.740 M	38.5	+2.0 +0.0 +0.0 +8.8	-11.5 +0.0 +0.0	+0.0 +0.0 +0.0	+0.0 +0.0 +0.0	37.8 200	54.0 High	-16.2	Vert 230
13	17145.730 M	37.8	+2.0 +0.0 +0.0 +8.7	-11.8 +0.0 +0.0	+0.0 +0.0 +0.0	+0.0 +0.0 +0.0	36.7 356	54.0 Mid	-17.3	Vert 140
14	16938.270 M	37.6	+2.1 +0.0 +0.0 +8.6	-11.9 +0.0 +0.0	+0.0 +0.0 +0.0	+0.0 +0.0 +0.0	36.4 213	54.0 Low	-17.6	Vert 134
15	24765.600 M	42.8	+0.0 +2.7 +0.0 +0.0	+0.0 +0.0 +0.0	-12.3 +0.0 +0.0	+2.8 +0.0 +0.0	36.0	54.0	-18.0	Vert 147
16	12403.140 M	40.9	+1.6 +0.0 +0.0 +6.4	-13.4 +0.0 +0.0	+0.0 +0.0 +0.0	+0.0 +0.0 +0.0	35.5 360	54.0 High	-18.5	Vert 140
17	14881.230 M	39.6	+1.8 +0.0 +0.0 +7.7	-14.1 +0.0 +0.0	+0.0 +0.0 +0.0	+0.0 +0.0 +0.0	35.0 281	54.0 High	-19.0	Vert 175

18	14521.510 M	39.7	+1.8 +0.0 +0.0 +7.7	-14.3 +0.0 +0.0	+0.0 +0.0 +0.0	+0.0 +0.0 +0.0	294	34.9	54.0	-19.1	Vert 134
19	12248.560 M	39.5	+1.5 +0.0 +0.0 +6.6	-13.3 +0.0 +0.0	+0.0 +0.0 +0.0	+0.0 +0.0 +0.0	170	34.3	54.0	-19.7	Vert 134
20	14704.510 M	38.7	+1.8 +0.0 +0.0 +7.8	-14.2 +0.0 +0.0	+0.0 +0.0 +0.0	+0.0 +0.0 +0.0	291	34.1	54.0	-19.9	Vert 140
21	12104.570 M	37.6	+1.5 +0.0 +0.0 +6.5	-13.4 +0.0 +0.0	+0.0 +0.0 +0.0	+0.0 +0.0 +0.0	360	32.2	54.0	-21.8	Vert 141
22	574.200M	28.4	+0.3 +0.0 +19.8 +0.0	+0.0 +0.0 +1.6	+0.0 +0.0 +1.2	+0.0 -28.2 +0.0	+0.0	23.1	46.0	-22.9	Vert 147
23	995.200M	26.1	+0.4 +0.0 +24.0 +0.0	+0.0 +0.0 +2.2	+0.0 +0.0 +1.6	+0.0 -27.0 +0.0	+0.0	27.3	54.0	-26.7	Vert 147
24	374.400M	27.4	+0.3 +0.0 +15.9 +0.0	+0.0 +0.0 +1.2	+0.0 +0.0 +1.0	+0.0 -27.4 +0.0	+0.0	18.4	46.0	-27.6	Vert 147
25	2655.000M Ave	28.4	+0.7 +0.0 +0.0 +3.0	+0.0 -34.5 +0.0	+0.0 +28.4 +0.0	+0.0 +0.0 +0.0	42	26.0	54.0	-28.0	Vert 145
^	2655.000M	40.1	+0.7 +0.0 +0.0 +3.0	+0.0 -34.5 +0.0	+0.0 +28.4 +0.0	+0.0 +0.0 +0.0	42	37.7	54.0	-16.3	Vert 145
27	2399.980M Ave	29.5	+0.6 +0.0 +0.0 +2.8	+0.0 -34.6 +0.0	+0.0 +27.7 +0.0	+0.0 +0.0 +0.0	33	26.0	54.0	-28.0	Vert 162
^	2399.980M	41.2	+0.6 +0.0 +0.0 +2.8	+0.0 -34.6 +0.0	+0.0 +27.7 +0.0	+0.0 +0.0 +0.0	33	37.7	54.0	-16.3	Vert 162
29	2389.970M Ave	28.6	+0.6 +0.0 +0.0 +2.8	+0.0 -34.6 +0.0	+0.0 +27.7 +0.0	+0.0 +0.0 +0.0	33	25.1	54.0	-28.9	Vert 162
^	2389.970M	41.0	+0.6 +0.0 +0.0 +2.8	+0.0 -34.6 +0.0	+0.0 +27.7 +0.0	+0.0 +0.0 +0.0	33	37.5	54.0	-16.5	Vert 162

31	59.100M	28.8	+0.1	+0.0	+0.0	+0.0	+0.0	8.6	40.0	-31.4	Vert 147
			+0.0	+0.0	+0.0	-27.8					
			+6.8	+0.4	+0.3	+0.0					
			+0.0								
32	150.000k	48.3	+0.0	+0.0	+0.0	+0.0	-80.0	-22.1	24.1	-46.2	Perp 147
			+0.0	+0.0	+0.0	+0.0					
			+0.0	+0.0	+0.0	+9.6					
			+0.0								
33	18.329M	9.8	+0.0	+0.0	+0.0	+0.0	-40.0	-22.0	29.5	-51.5	Perp 147
			+0.0	+0.0	+0.0	+0.0					
			+0.0	+0.0	+0.0	+7.9					
			+0.3								
34	77.808k	39.2	+0.0	+0.0	+0.0	+0.0	-80.0	-31.0	29.8	-60.8	Perp 147
			+0.0	+0.0	+0.0	+0.0	360				
			+0.0	+0.0	+0.0	+9.8					
			+0.0								

Band Edge Summary					
Frequency (MHz)	Modulation	Ant. Type	Field Strength (dBuV/m @3m)	Limit (dBuV/m @3m)	Results
2390.0	QPSK	Integral Folded Monopole	25.1	<54	Pass
2400.0	QPSK	Integral Folded Monopole	26.0	<54	Pass
2483.5	QPSK	Integral Folded Monopole	49.6	<54	Pass

### Band Edge Setup / Conditions / Data

Test Location: CKC Laboratories, Inc. • 22116 23rd Dr. SE, Suite A • Bothell, WA 98021 • (425) 402-1717  
 Customer: **Medtronic MiniMed**  
 Specification: **15.247(d) / 15.209 Radiated Spurious Emissions (Peak Limit)**  
 Work Order #: **97869** Date: 2/21/2016  
 Test Type: **Maximized Emissions** Time: 09:11:18  
 Tested By: Steven Pittsford Sequence#: 4  
 Software: EMITest 5.03.02

#### Equipment Tested:

Device	Manufacturer	Model #	S/N
Configuration 1			


#### Support Equipment:

Device	Manufacturer	Model #	S/N
Configuration 1			

#### Test Conditions / Notes:

Test Method: ANSI C63.10 (2013) & KDB 558074 D01 DTS Meas Guidance v03r04 Jan 7th, 2016  Frequency tested: 2420MHz, & 2480MHz Firmware power setting: Max Power EUT Firmware: Continuous Modulation Software Modulation: QPSK  Antenna type: Integral Monopole Dipole Antenna Gain : 0.0 dBi  Duty Cycle: 100%  Test Mode: Continuously modulated Setup: The EUT is set on a Styrofoam test bench centered on the turntable. The EUT is oriented in X, Y & Z axis with only the worst case reported. The EUT has a fully charged battery.  Environmental Conditions Temperature: 22°C Relative Humidity: 40%
---

Medtronic MiniMed W/D#: 97869 Sequence#: 4 Date: 2/21/2016  
15.247(d) / 15.209 Radiated Spurious Emissions (Peak Limit) Test Distance: 3 Meters Vert & Horz

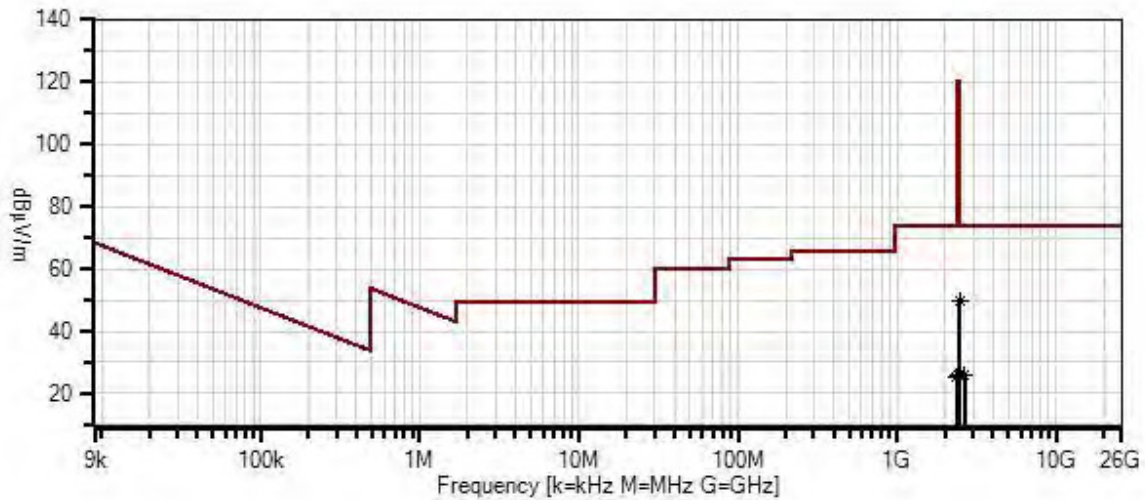

- Readings
- Peak Readings
- × QP Readings
- \* Average Readings
- ▼ Ambient
- Software Version: 5.03.02
- 1 - 15.247(d) / 15.209 Radiated Spurious Emissions (Peak Limit)

**Test Equipment:**

ID	Asset #	Description	Model	Calibration Date	Cal Due Date
T1	ANP06540	Cable	Heliac	10/29/2015	10/29/2017
T2	AN02872	Spectrum Analyzer	E4440A	11/18/2015	11/18/2017
T3	AN03540	Preamplifier	83017A	4/30/2015	4/30/2017
T4	AN01467	Horn Antenna- ANSI C63.5 Calibration	3115	8/12/2015	8/12/2017
T5	ANP05305	Cable	ETSI-50T	2/15/2016	2/15/2018

**Measurement Data:**



Reading listed by margin.



Test Distance: 3 Meters



#	Freq	Rdng	T1 T5	T2	T3	T4	Dist	Corr	Spec	Margin	Polar
	MHz	dBμV	dB	dB	dB	dB	Table	dBμV/m	dBμV/m	dB	Ant
1	2483.500M	52.9	+0.6	+0.0	-34.5	+27.7	+0.0	49.6	54.0	-4.4	Vert
	Ave		+2.9				42				145
^	2483.500M	63.3	+0.6	+0.0	-34.5	+27.7	+0.0	60.0	74.0	-14.0	Vert
			+2.9				42				145
3	2399.980M	29.5	+0.6	+0.0	-34.6	+27.7	+0.0	26.0	54.0	-28.0	Vert
	Ave		+2.8				33				162
^	2399.980M	41.2	+0.6	+0.0	-34.6	+27.7	+0.0	37.7	74.0	-36.3	Vert
			+2.8				33				162
5	2655.000M	28.4	+0.7	+0.0	-34.5	+28.4	+0.0	26.0	54.0	-28.0	Vert
	Ave		+3.0				42				145
^	2655.000M	40.1	+0.7	+0.0	-34.5	+28.4	+0.0	37.7	74.0	-36.3	Vert
			+3.0				42				145
7	2389.970M	28.6	+0.6	+0.0	-34.6	+27.7	+0.0	25.1	54.0	-28.9	Vert
	Ave		+2.8				33				162
^	2389.970M	41.0	+0.6	+0.0	-34.6	+27.7	+0.0	37.5	74.0	-36.5	Vert
			+2.8				33				162



## Band Edge Plots

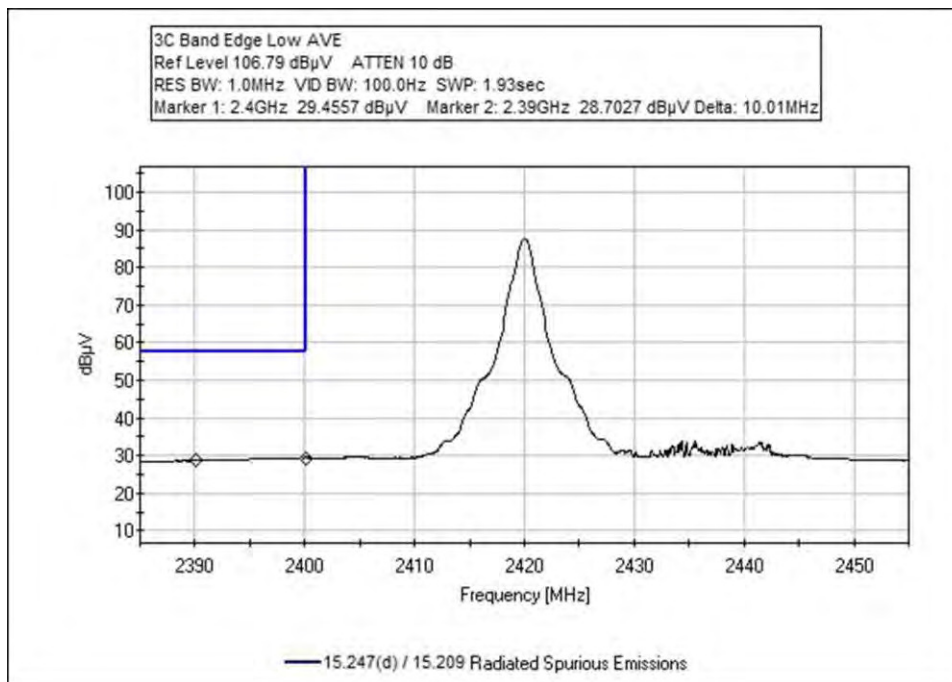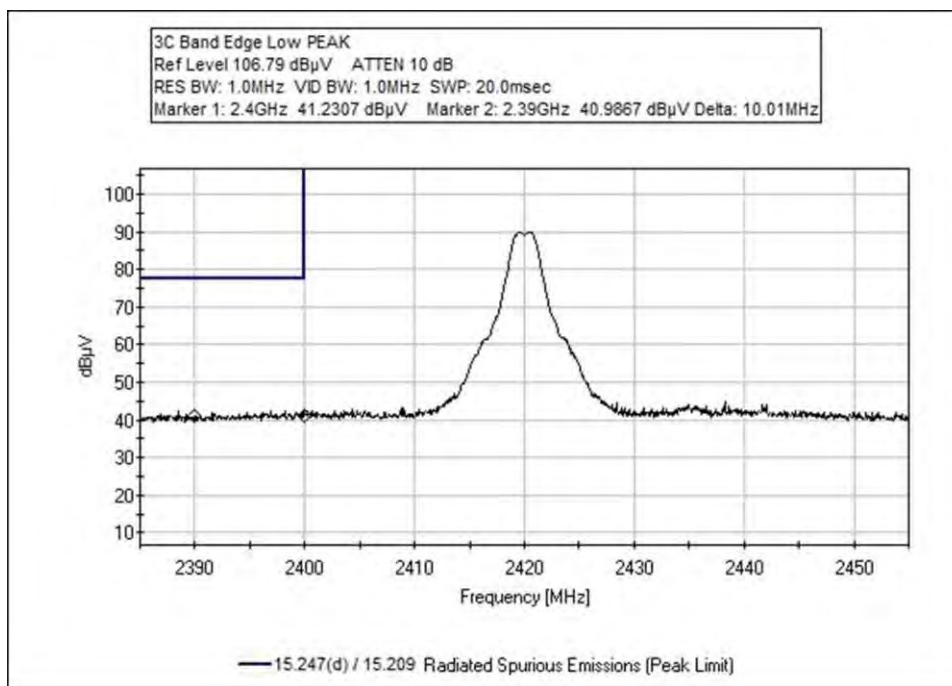

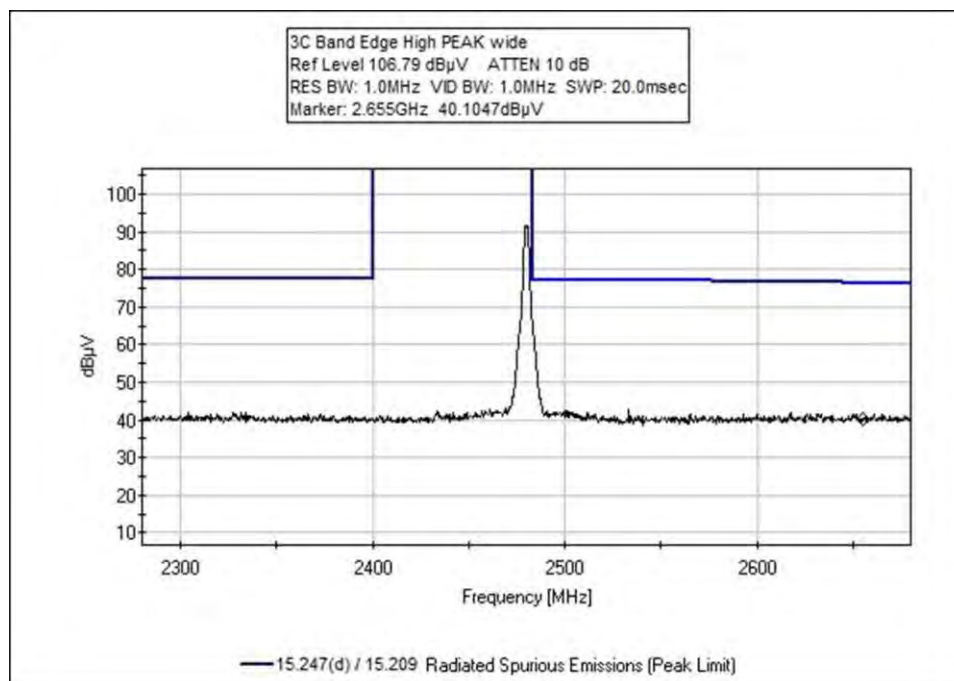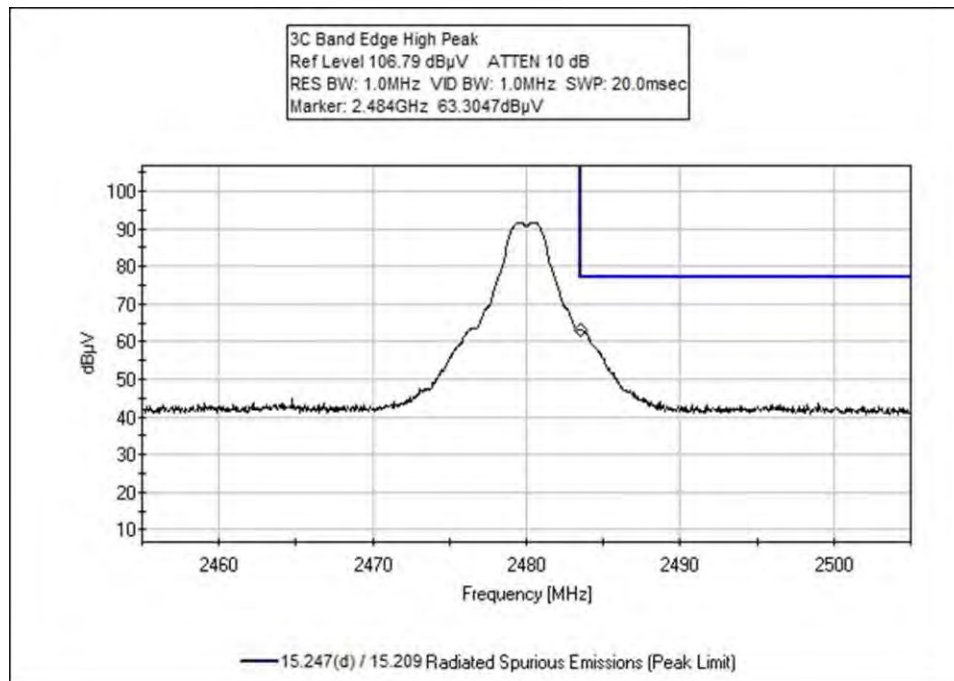

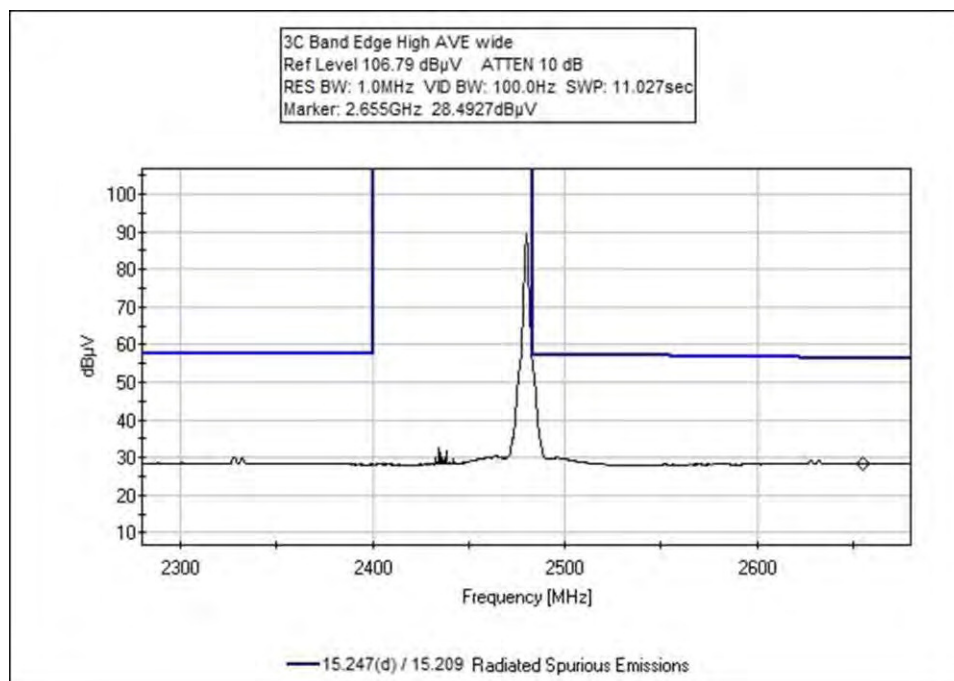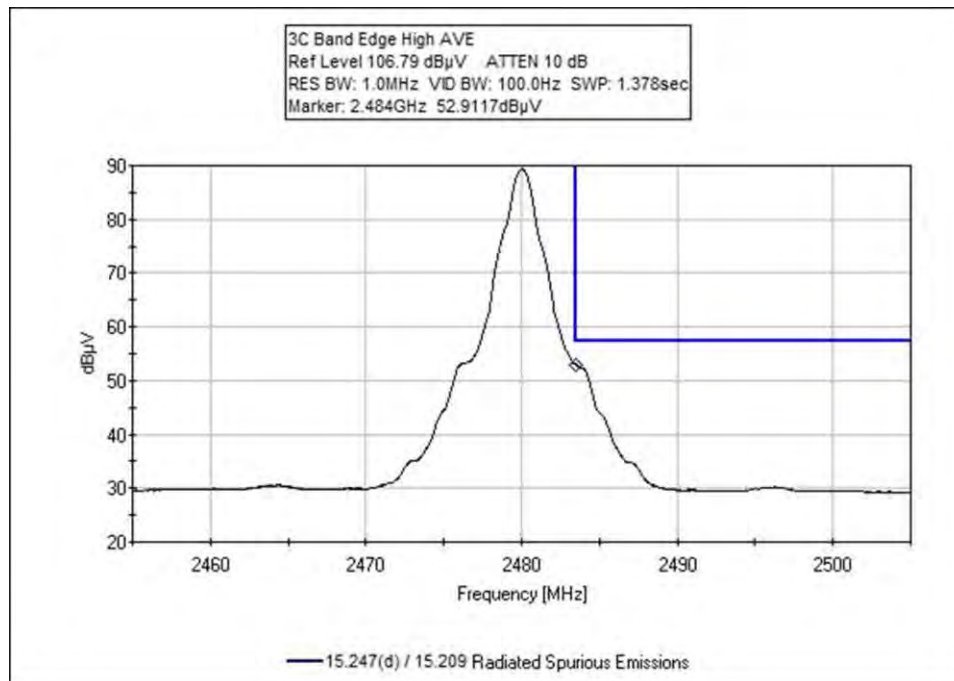

**Test Setup Photos**



Below 1GHz



Above 1GHz



X Axis



Y Axis





Z Axis

## SUPPLEMENTAL INFORMATION

### Measurement Uncertainty

Uncertainty Value	Parameter
4.73 dB	Radiated Emissions
3.34 dB	Mains Conducted Emissions
3.30 dB	Disturbance Power

Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of  $k=2$ . Compliance is deemed to occur provided measurements are below the specified limits.

### Emissions Test Details

#### TESTING PARAMETERS

Unless otherwise indicated, the following configuration parameters are used for equipment setup: The cables were routed consistent with the typical application by varying the configuration of the test sample. Interface cables were connected to the available ports of the test unit. The effect of varying the position of the cables was investigated to find the configuration that produced maximum emissions. Cables were of the type and length specified in the individual requirements. The length of cable that produced maximum emissions was selected.

The equipment under test (EUT) was set up in a manner that represented its normal use, as shown in the setup photographs. Any special conditions required for the EUT to operate normally are identified in the comments that accompany the emissions tables.

The emissions data was taken with a spectrum analyzer or receiver. Incorporating the applicable correction factors for distance, antenna, cable loss and amplifier gain, the data was reduced as shown in the table below. The corrected data was then compared to the applicable emission limits. Preliminary and final measurements were taken in order to ensure that all emissions from the EUT were found and maximized.

#### CORRECTION FACTORS

The basic spectrum analyzer reading was converted using correction factors as shown in the highest emissions readings in the tables. For radiated emissions in  $\text{dB}\mu\text{V}/\text{m}$ , the spectrum analyzer reading in  $\text{dB}\mu\text{V}$  was corrected by using the following formula. This reading was then compared to the applicable specification limit. Individual measurements were compared with the displayed limit value in the margin column. The margin was calculated based on the limit value subtracting the corrected measured value; a negative margin represents a measurement less than the limit while a positive margin represents a measurement exceeding the limit.

SAMPLE CALCULATIONS		
	Meter reading	( $\text{dB}\mu\text{V}$ )
+	Antenna Factor	( $\text{dB}/\text{m}$ )
+	Cable Loss	( $\text{dB}$ )
-	Distance Correction	( $\text{dB}$ )
-	Preamplifier Gain	( $\text{dB}$ )
=	Corrected Reading	( $\text{dB}\mu\text{V}/\text{m}$ )

## TEST INSTRUMENTATION AND ANALYZER SETTINGS

The test instrumentation and equipment listed were used to collect the emissions data. A spectrum analyzer or receiver was used for all measurements. Unless otherwise specified, the following table shows the measuring equipment bandwidth settings that were used in designated frequency bands. For testing emissions, an appropriate reference level and a vertical scale size of 10 dB per division were used.

MEASURING EQUIPMENT BANDWIDTH SETTINGS PER FREQUENCY RANGE			
TEST	BEGINNING FREQUENCY	ENDING FREQUENCY	BANDWIDTH SETTING
CONDUCTED EMISSIONS	150 kHz	30 MHz	9 kHz
RADIATED EMISSIONS	9 kHz	150 kHz	200 Hz
RADIATED EMISSIONS	150 kHz	30 MHz	9 kHz
RADIATED EMISSIONS	30 MHz	1000 MHz	120 kHz
RADIATED EMISSIONS	1000 MHz	>1 GHz	1 MHz

## SPECTRUM ANALYZER/RECEIVER DETECTOR FUNCTIONS

The notes that accompany the measurements contained in the emissions tables indicate the type of detector function used to obtain the given readings. Unless otherwise noted, all readings were made in the "positive peak" detector mode. Whenever a "quasi-peak" or "average" reading was recorded, the measurement was annotated with a "QP" or an "Ave" on the appropriate rows of the data sheets. In cases where quasi-peak or average limits were employed and data exists for multiple measurement types for the same frequency then the peak measurement was retained in the report for reference, however the numbering for the affected row was removed and an arrow or caret ("^") was placed in the far left-hand column indicating that the row above takes precedence for comparison to the limit. The following paragraphs describe in more detail the detector functions and when they were used to obtain the emissions data.

### Peak

In this mode, the spectrum analyzer or receiver recorded all emissions at their peak value as the frequency band selected was scanned. By combining this function with another feature called "peak hold," the measurement device had the ability to measure intermittent or low duty cycle transient emission peak levels. In this mode the measuring device made a slow scan across the frequency band selected and measured the peak emission value found at each frequency across the band.

### Quasi-Peak

Quasi-peak measurements were taken using the quasi-peak detector when the true peak values exceeded or were within 2 dB of a quasi-peak specification limit. Additional QP measurements may have been taken at the discretion of the operator.

### Average

Average measurements were taken using the average detector when the true peak values exceeded or were within 2 dB of an average specification limit. Additional average measurements may have been taken at the discretion of the operator. If the specification or test procedure requires trace averaging, then the averaging was performed using 100 samples or as required by the specification. All other average measurements are performed using video bandwidth averaging. To make these measurements, the test engineer reduces the video bandwidth on the measuring device until the modulation of the signal is filtered out. At this point the measuring device is set into the linear mode and the scan time is reduced.