

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

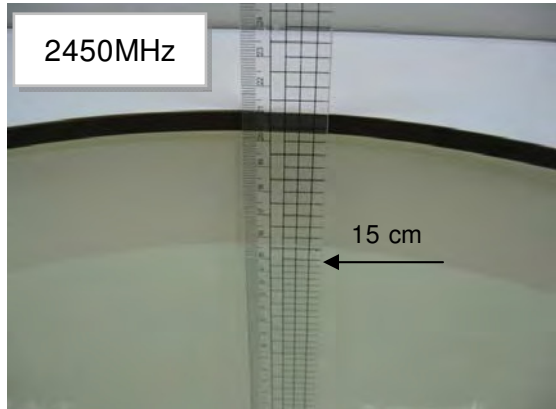


Fig.2.1

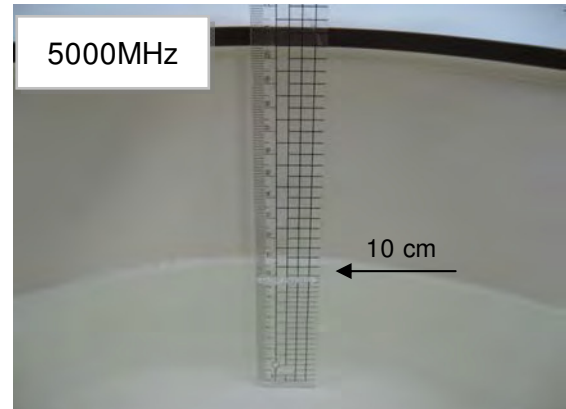


Fig.2.2

Body - distance between flat phantom and EUT is 0 mm

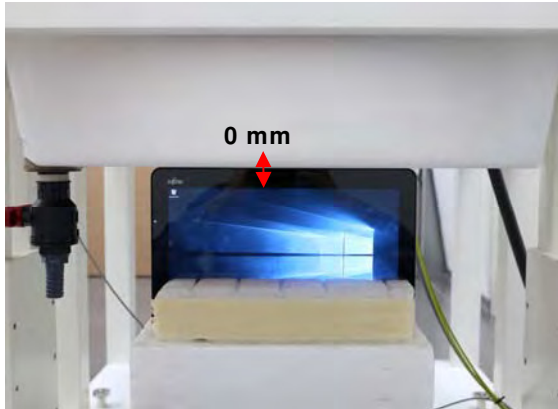


Fig.3 EUT Top side to flat phantom



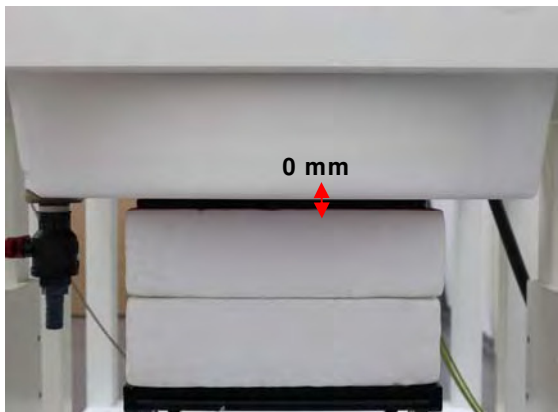


Fig.4 EUT Back side to flat phantom



Fig.5 EUT Right side to flat phantom

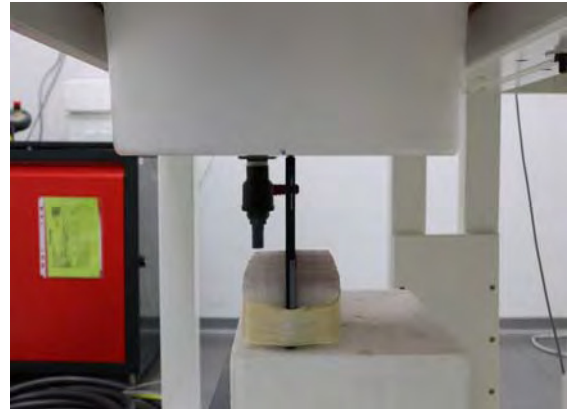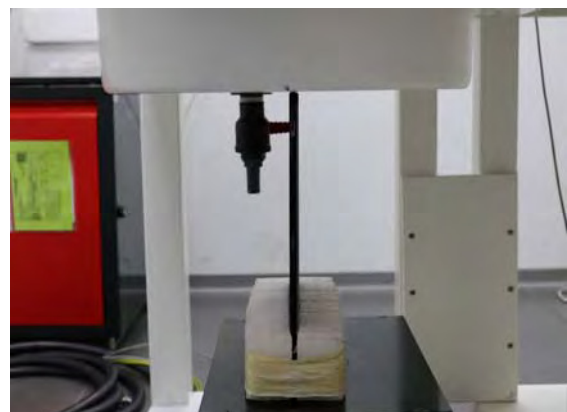

Body - distance between flat phantom and EUT is 0 mm

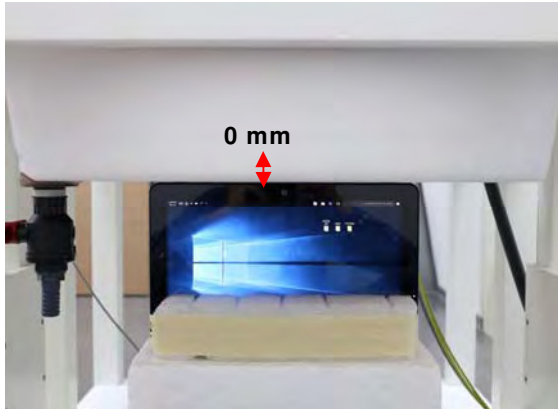


Fig.6 EUT Bottom side to flat phantom

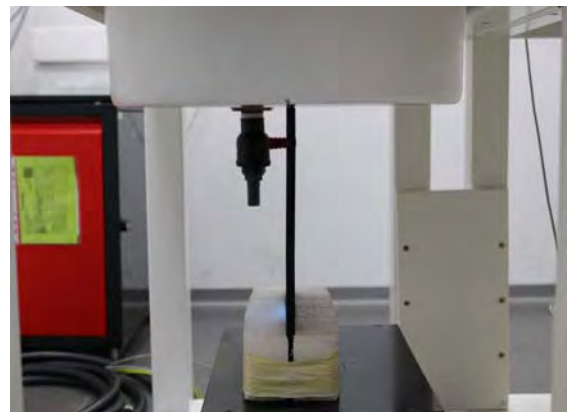
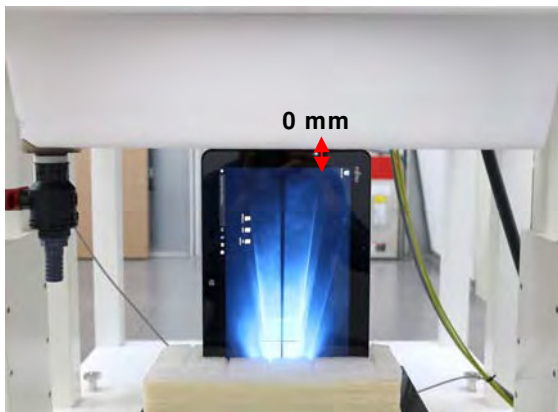


Fig.7 EUT Left side to flat phantom

12. Photographs of the EUT



Fig.8 Front view of EUT



Fig.9 Back view of EUT

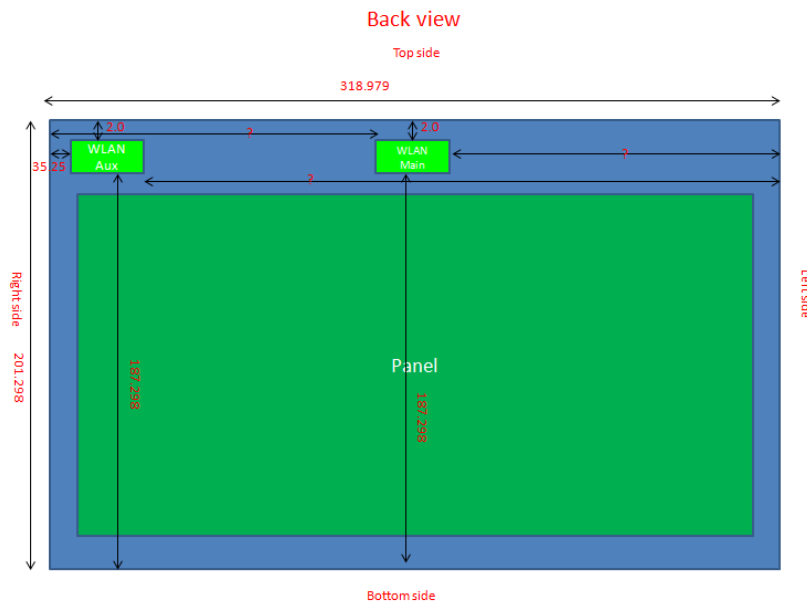


Fig.10 Antenna position of EUT (Back view)

- End of Report -