

Test report No:
NIE: 71695RAN.001

Test report

Antenna Gain and Radiation Pattern Tests

| | |
|---|--|
| (*) Identification of 1tem tested | Bluetooth enabled blood glucose meter. |
| (*) Trademark | OneTouch |
| (*) Model and /or type reference tested | Verio Reflect |
| (*) Other identification of the product | HW version: rev E SW version: 4.1.2 |
| (*) Features | Bluetooth LE |
| (*) Manufacturer | Lifescan Europe GmbH Gubelstrasse 34, 6300 Zug, Switzerland |
| Test methodology according to | [1] 3GPP TS 34.114: "User Equipment (UE) / Mobile Station (MS) Over The Air (OTA) antenna performance; Conformance testing", V 12.2.0, (2016-10-05). |
| Approved by (name / position & signature) | Miguel Lacave Antennas Lab Manager |
| Date of issue | 2022-08-22 |
| Report template No | FAN41_01 (*) "Data provided by the client" |

Index

Competences and guarantees3

General conditions3

Uncertainty3

Data provided by the client.....3

Usage of samples4

Test sample description4

Identification of the client.....4

Testing period and place.....4

Document history4

Remarks and comments5

Appendix A: Test results6

Appendix B: Photographs14

Competences and guarantees

DEKRA Testing and Certification, S.A.U. is a testing laboratory competent to carry out the tests described in this report.

In order to assure the traceability to other national and international laboratories, DEKRA Testing and Certification, S.A.U. has a calibration and maintenance program for its measurement equipment.

DEKRA Testing and Certification, S.A.U. guarantees the reliability of the data presented in this report, which is the result of the measurements and the tests performed to the item under test on the date and under the conditions stated on the report and, it is based on the knowledge and technical facilities available at DEKRA Testing and Certification, S.A.U. at the time of performance of the test.

DEKRA Testing and Certification, S.A.U. is liable to the client for the maintenance of the confidentiality of all information related to the item under test and the results of the test.

The results presented in this Test Report apply only to the particular item under test established in this document.

IMPORTANT: No parts of this report may be reproduced or quoted out of context, in any form or by any means, except in full, without the previous written permission of DEKRA Testing and Certification, S.A.U.

General conditions

1. This report is only referred to the item that has undergone the test.
2. This report does not constitute or imply on its own an approval of the product by the Certification Bodies or competent Authorities.
3. This document is only valid if complete; no partial reproduction can be made without previous written permission of DEKRA Testing and Certification, S.A.U.
4. This test report cannot be used partially or in full for publicity and/or promotional purposes without previous written permission of DEKRA Testing and Certification, S.A.U. and the Accreditation Bodies.

Uncertainty

Uncertainty (factor $k=2$) was calculated according to the following documents:

1. FAN02 - OTA SISO CTIA - AMS-8500 Uncertainty report

Data provided by the client

The following data has been provided by the client:

1. Information relating to the description of the sample ("Identification of the item tested", "Trademark", "Model and/or type reference tested", "Other identification of the product", "Features", "Manufacturer" and "Test sample description").

DEKRA Testing and Certification, S.A.U. declines any responsibility with respect to the information provided by the client and that may affect the validity of results.

Usage of samples

Samples undergoing test have been selected by the client.

Sample M/01 is composed of the following elements:

| Control Nº | Description | Model | S/N | Date of reception |
|------------|---|---------------|-----|-------------------|
| 71695B/006 | Bluetooth enabled blood glucose meter Radiated | Verio Reflect | - | 2022-05-17 |
| 71695B/002 | Bluetooth enabled blood glucose meter Conducted | Verio Reflect | - | 2022-05-09 |

1. Sample M/01 has undergone the test(s) specified in subclause "Test method requested".

Test sample description

The device under test consist of a blood glucose meter for measuring the levels of Glucose in a patient's blood. Bluetooth is used to transfer the patients result(s) to their smart device.

Identification of the client

Company name: Lifescan Scotland Ltd

Postal address: Beechwood Park North, Inverness, IV2 3ED, UK

Contact person: Andrew Finlayson

E-mail: afinlays@lifescan.com

Testing period and place

| | |
|---------------|--|
| Test Location | DEKRA Testing and Certification S.A.U. |
| Date (start) | 2022-05-25 |
| Date (finish) | 2022-05-26 |

Document history

| Report number | Date | Description |
|---------------|------------|---------------|
| 71695RAN.001 | 2022-08-22 | First release |

Remarks and comments

The instrumentation utilized to perform the tests covered in this test report is listed in the following table.

| | Equipment | Calibration Date | S/N | DEKRA Control Number |
|----|---|------------------|------------|----------------------|
| 1. | Anechoic chamber ETS LINDGREN AMS-8500 | N/A | 3954 | 2729 |
| 2. | RF unit switch Agilent Technologies 3499A | N/A | MY42003363 | 2831 |
| 3. | Positioning system controller ETS LINDGREN 2115-72 | N/A | - | 2731 |
| 4. | OTA measurement software ETS LINDGREN EMQuest v1.14 | N/A | 1095 | 4428 |
| 5. | Spectrum analyzer Agilent Technologies PSA | 2020/11 | MY44300521 | 2327 |
| 6. | Temperature and Pico Technology, model Humidiprobe | 2022/04 | ZNR30/064 | 3547 |

Testing has been performed by Francisco José Alcaide.

Appendix A: Test results

Index

- 1. TEST CONDITIONS8
 - 1.1 Test frequencies and output power8
 - 1.2 Antenna orientation and setup requirements8
- 2. TEST RESULTS9
 - 2.1 Peak antenna gain9
- 3. 3D RADIATION PATTERNS11
 - 3.1 Free Space - Radiation Pattern – 2402 MHz.....11
 - 3.2 Free Space - Radiation Pattern – 2440 MHz.....12
 - 3.3 Free Space - Radiation Pattern – 2480 MHz.....13

1. TEST CONDITIONS

1.1 Test frequencies and output power

3D radiation pattern and conducted power measurements were performed at 2402 MHz, 2440 MHz and 2480 MHz test frequencies.

The output power of the device under test was set to maximum for all tests.

1.2 Antenna orientation and setup requirements

For the 3D radiation pattern measurements the EUT is rotated along two different spherical axes: theta (θ) and phi (Φ). The relationship between the 3D Cartesian coordinate system (X, Y, Z) and the theta and phi axes is illustrated in the following figure. This coordinate system should be used as reference in all 3D radiation pattern graphs in section 3 as well as test setup photographs in Appendix B.

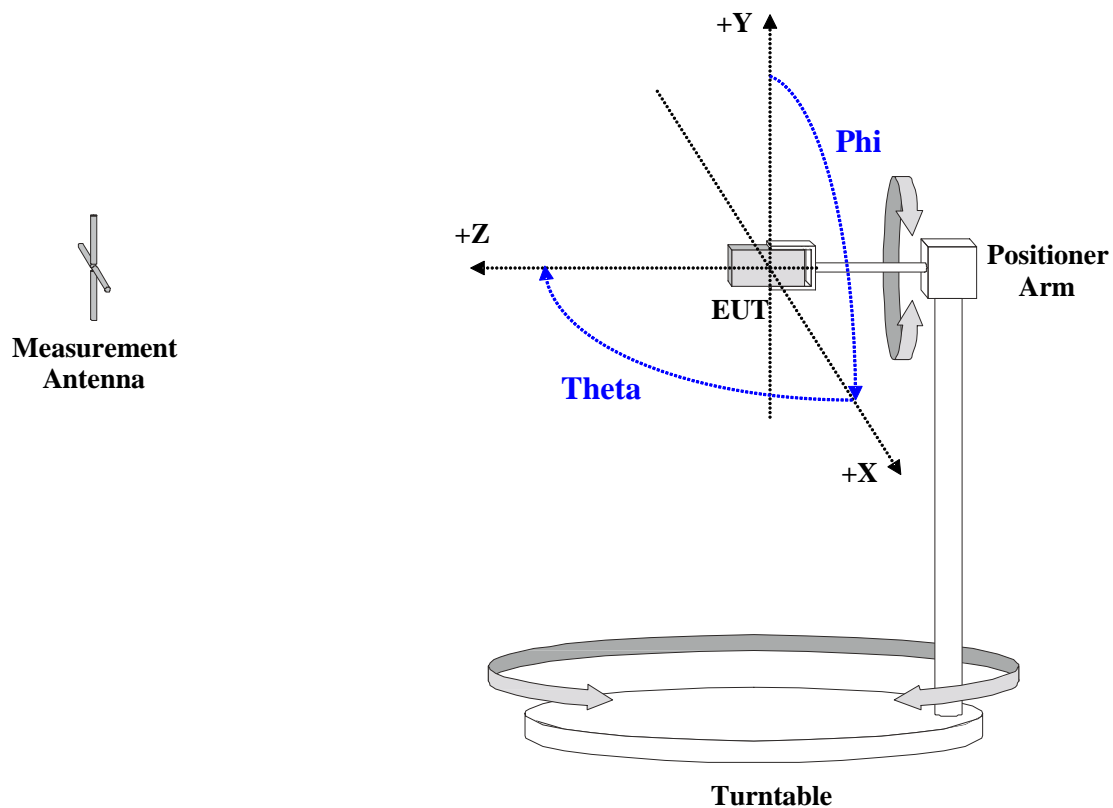


Fig. 1. Coordinate system.

Theta is the spherical axis that rotates along the Cartesian Y axis while Phi is the spherical axis that rotates along the Cartesian Z axis. The initial measurement position (Theta = 0° and Phi = 0°) is illustrated in each of the test setup photographs in Appendix B. The EUT has only one mechanical configuration and it was tested in the "Free-space" placed 5 meters away from the measurement antenna.

2. TEST RESULTS

2.1 Peak antenna gain

The test setup used to derive test results in this clause is illustrated below.

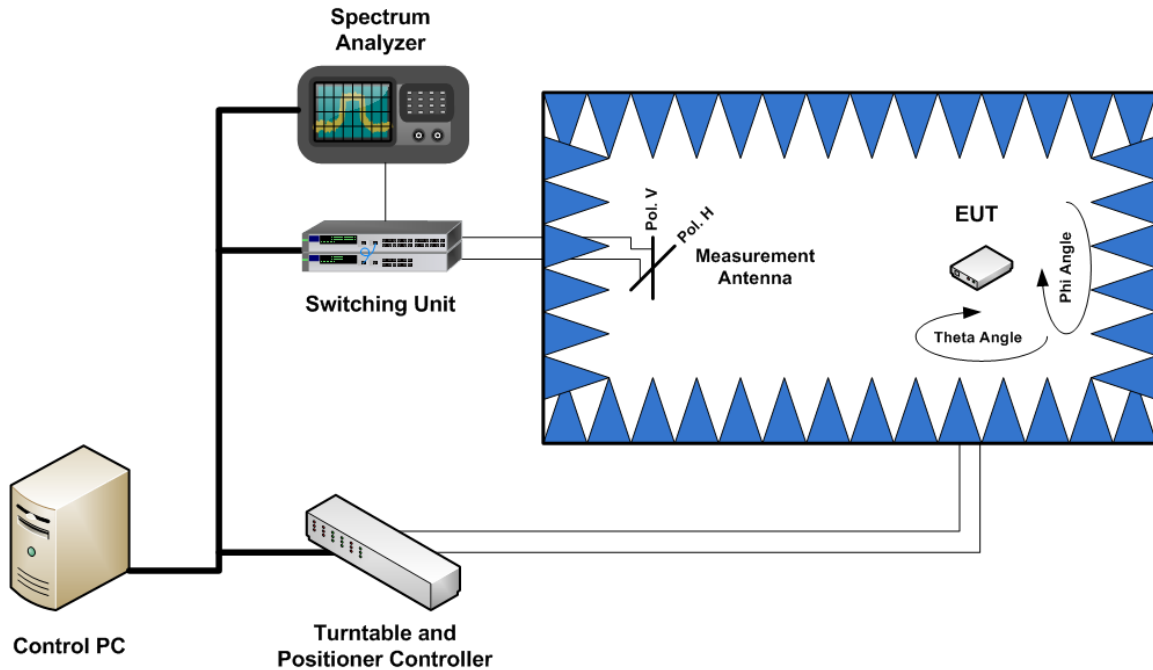


Fig. 2. Equipment and connections for peak antenna gain measurements.

For radiated tests, the EUT was placed inside a fully anechoic test system and hold on a multi-axis positioning system for Free Space (FS) configuration (see Figure 7). The EUT was set to operate on a test mode radiating a CW signal at maximum output power for the frequencies under test. Equivalent Isotropically Radiated Power (EIRP) measurements were performed using a power spectrum analyzer. EIRP measurements were performed at intervals of 15 degrees along the theta and phi axes and at both horizontal and vertical polarizations.

For conducted tests, the EUT was set to operate on a CW test mode signal at maximum output power for the frequencies under test. Conducted output power measurements were performed over the output module connector using a power spectrum analyzer.

Peak EIRP measurements for Free Space configuration are presented below.

| Frequency (MHz) | TRP (dBm) | Peak EIRP (dBm) | Theta Angle (°) | Phi Angle (°) |
|-----------------|-----------|-----------------|-----------------|---------------|
| 2402 | -5.63 | -2.18 | 135 | 330 |
| 2440 | -7.89 | -4.46 | 75 | 345 |
| 2480 | -6.83 | -3.28 | 0 | 75 |

Conducted output power measurements are presented below.

| Frequency (MHz) | Conducted Power (dBm) |
|-----------------|-----------------------|
| 2402 | -4.32 |
| 2440 | -3.99 |
| 2480 | -3.66 |

Peak antenna gain results are presented below.

| Frequency (MHz) | Antenna Peak Gain (dBi) |
|-----------------|-------------------------|
| 2402 | 2.14 |
| 2440 | -0.47 |
| 2480 | 0.38 |

3. 3D RADIATION PATTERNS

3.1 Free Space - Radiation Pattern – 2402 MHz

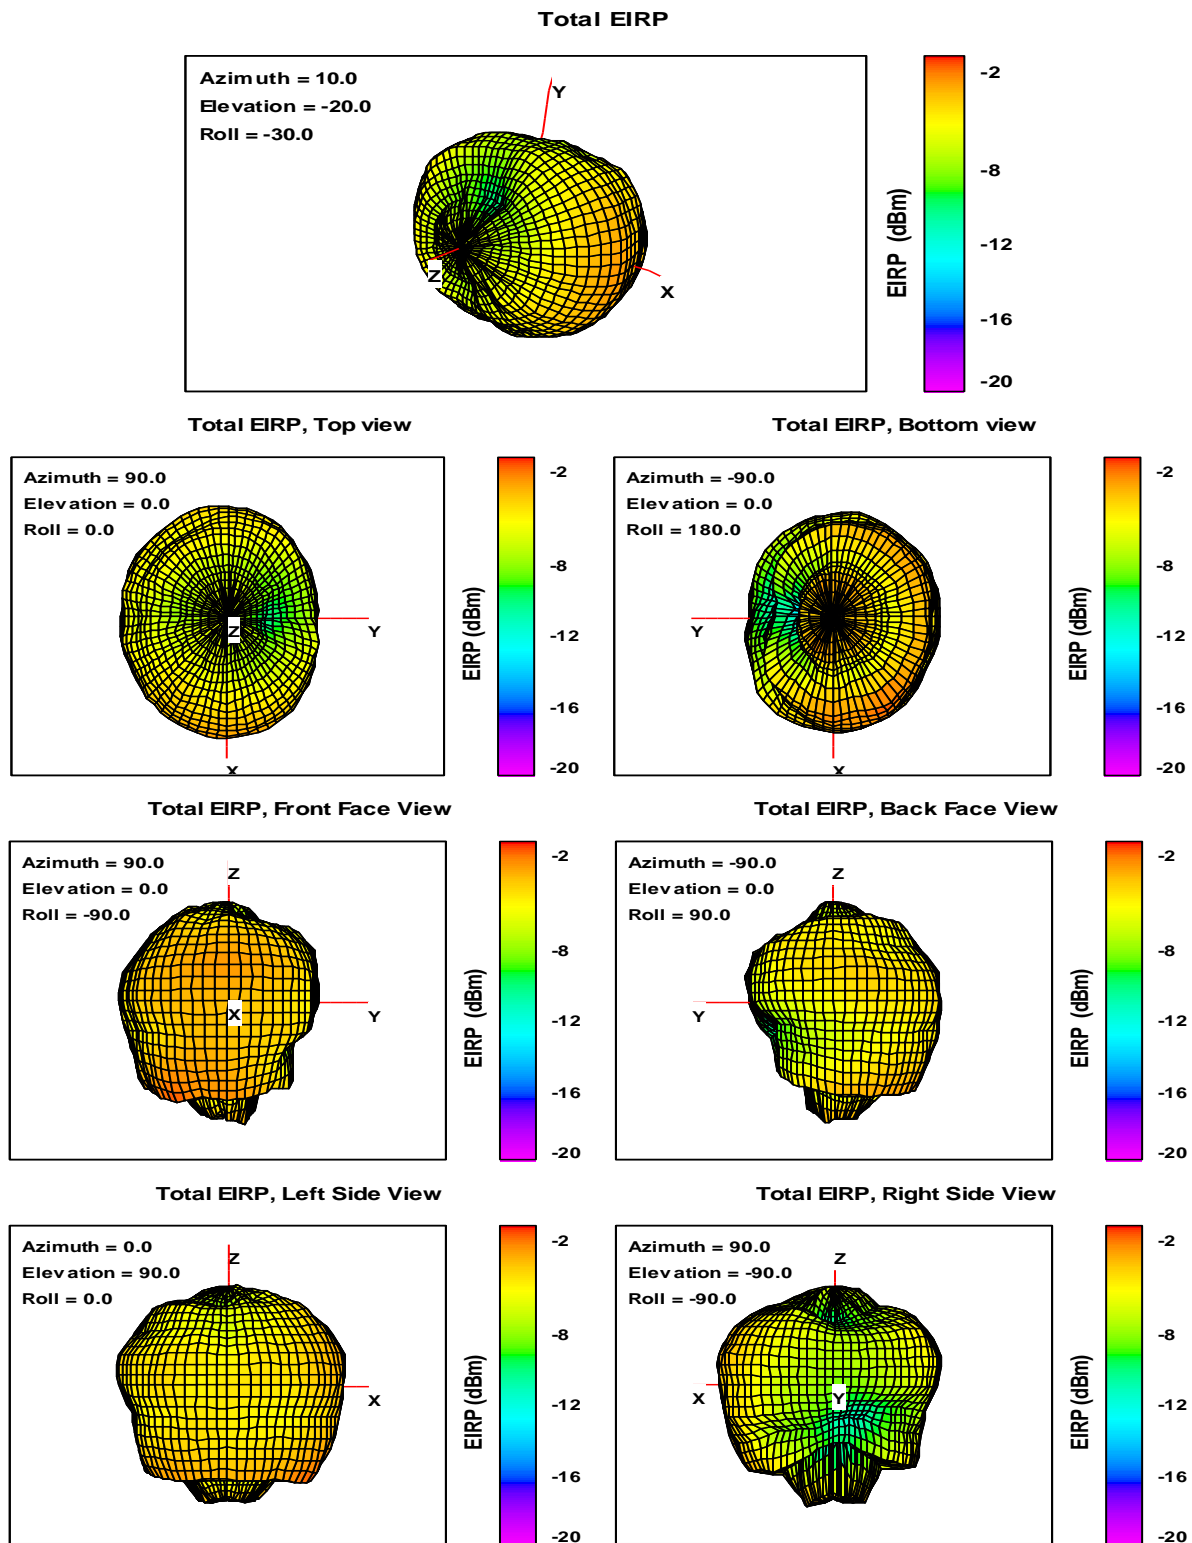


Fig. 3. Total EIRP, Free Space, 2402 MHz.

3.2 Free Space - Radiation Pattern – 2440 MHz

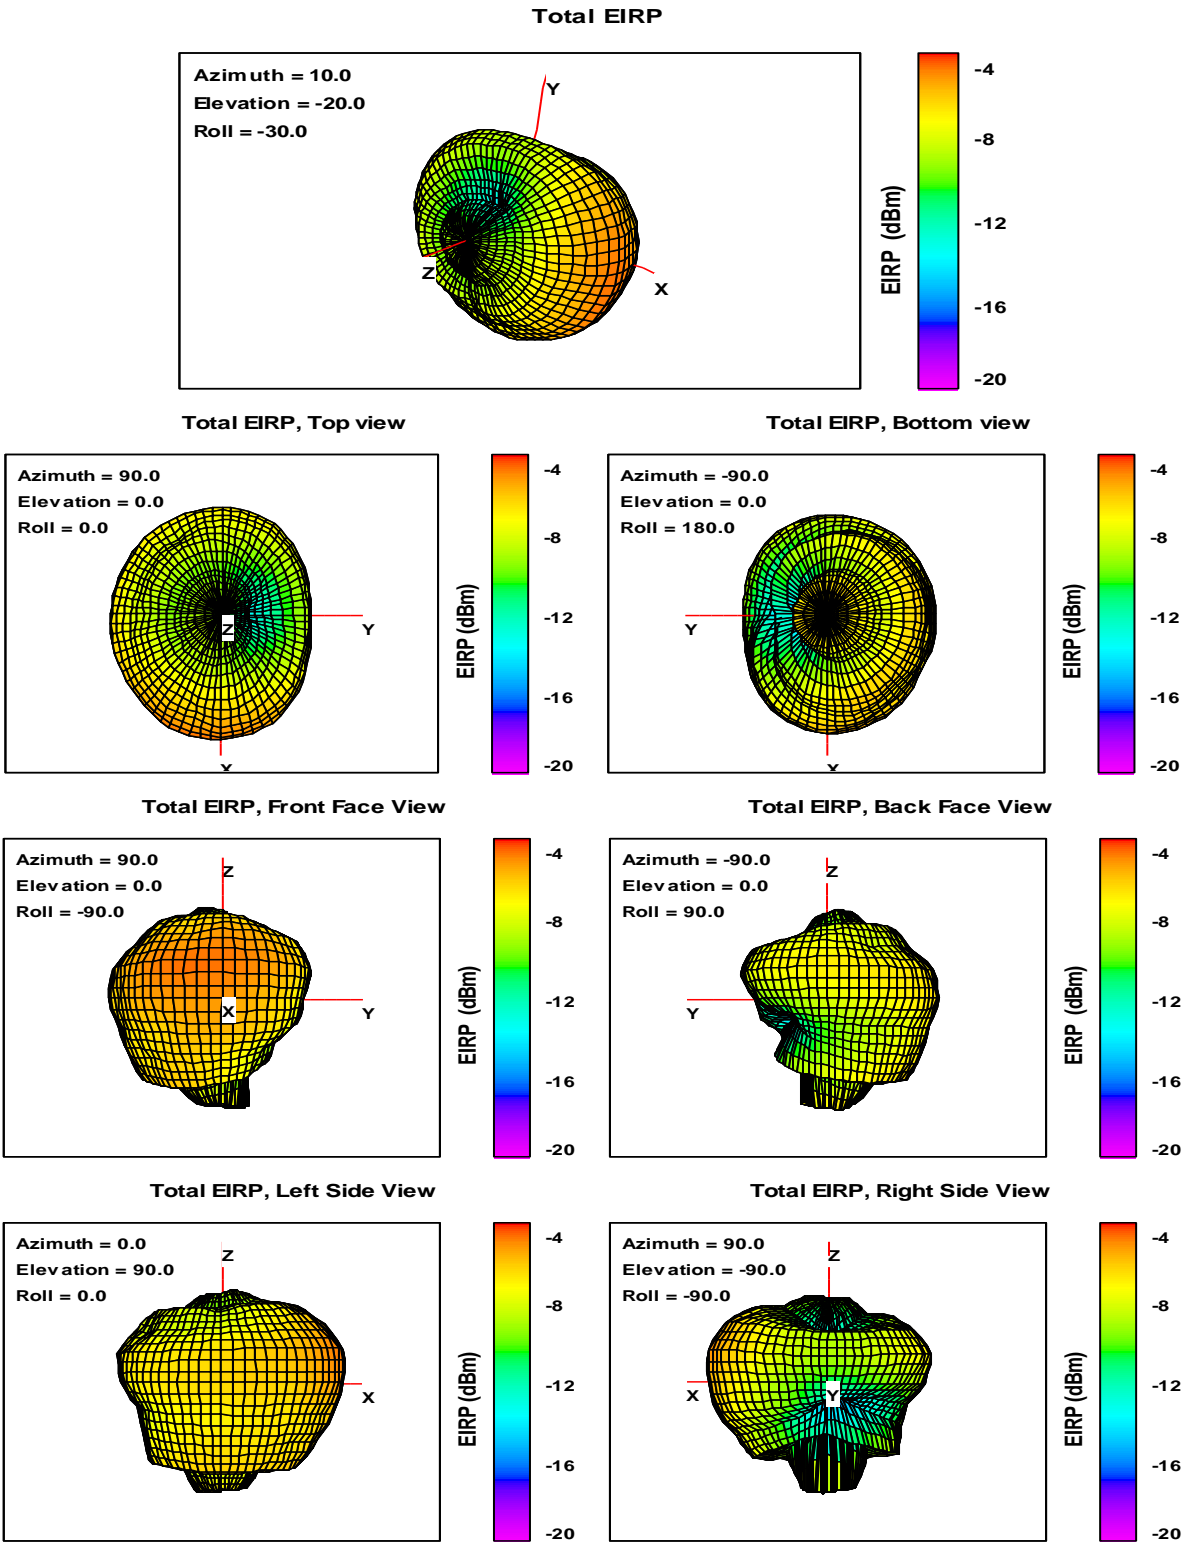


Fig. 4. Total EIRP, Free Space, 2440 MHz.

3.3 Free Space - Radiation Pattern – 2480 MHz

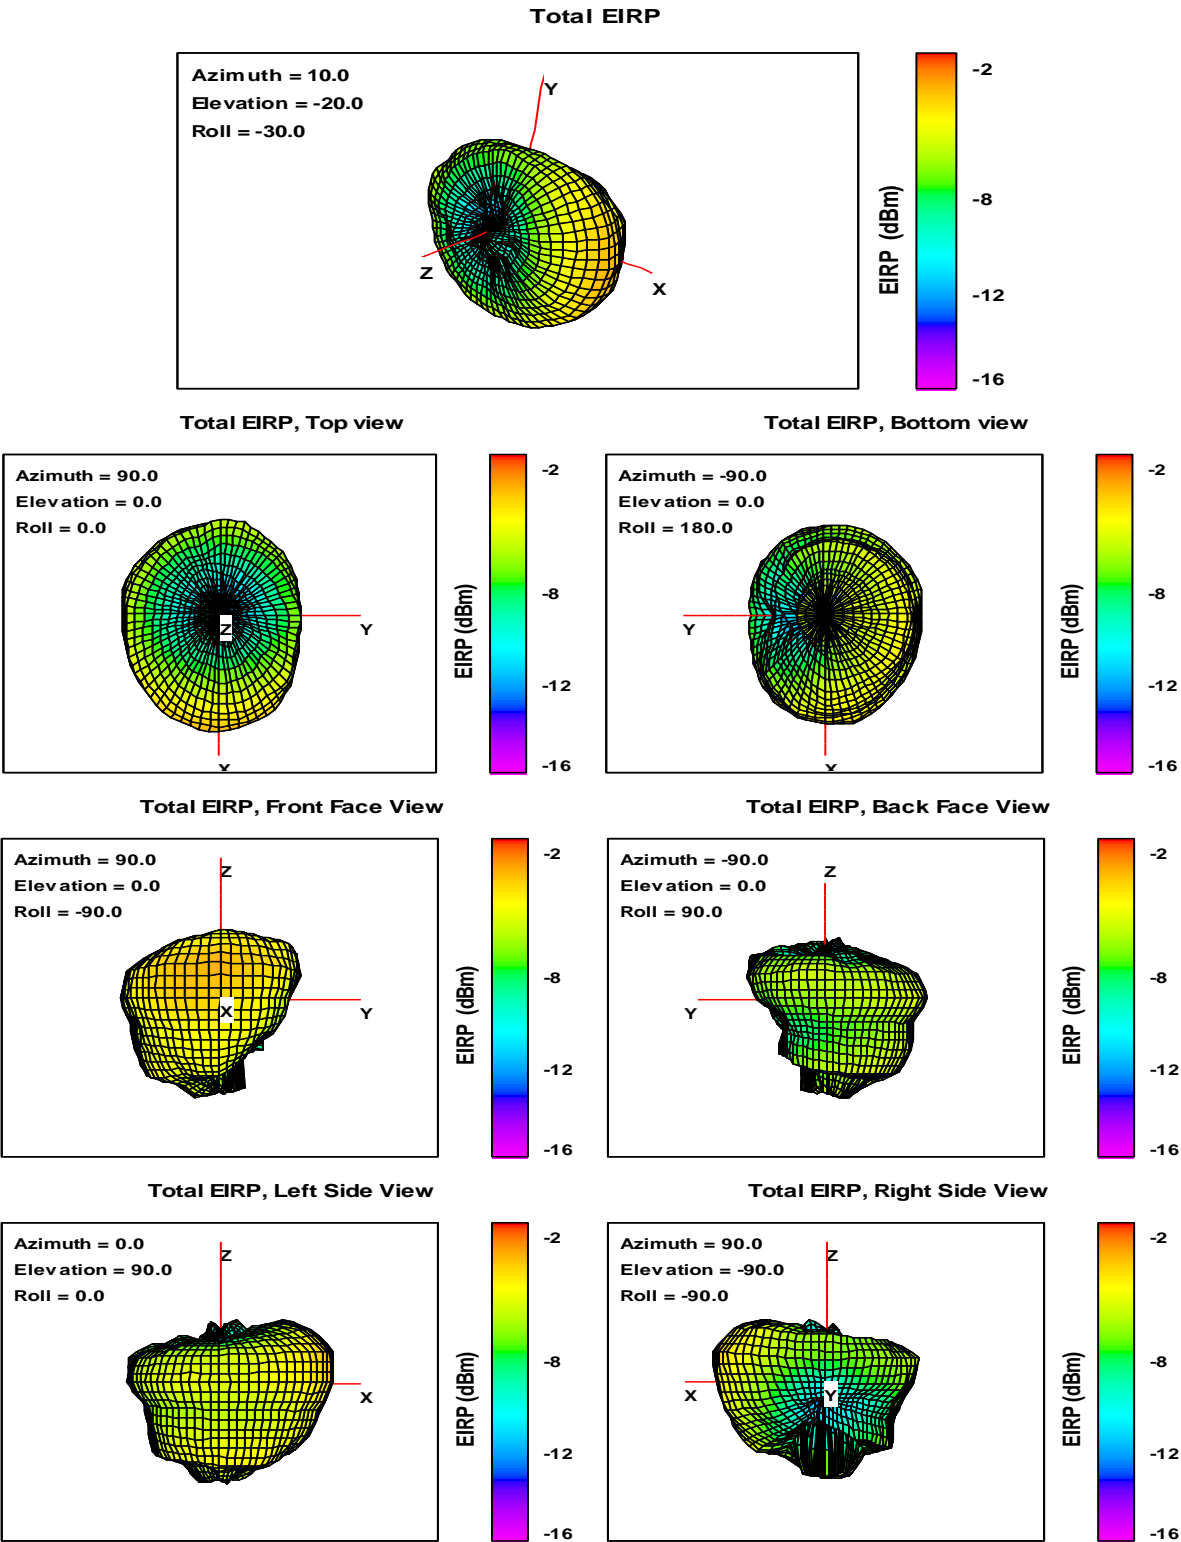


Fig. 5. Total EIRP, Free Space, 2480 MHz.

Appendix B: Photographs

Equipment under test:

- EUT front view:



Fig 6. EUT radiated and conducted back view.

- EUT back view:



Fig 7. EUT back view.

Test set:

- **Free Space set-up: Initial position: $\Theta = 0^\circ$, $\Phi = 0^\circ$**

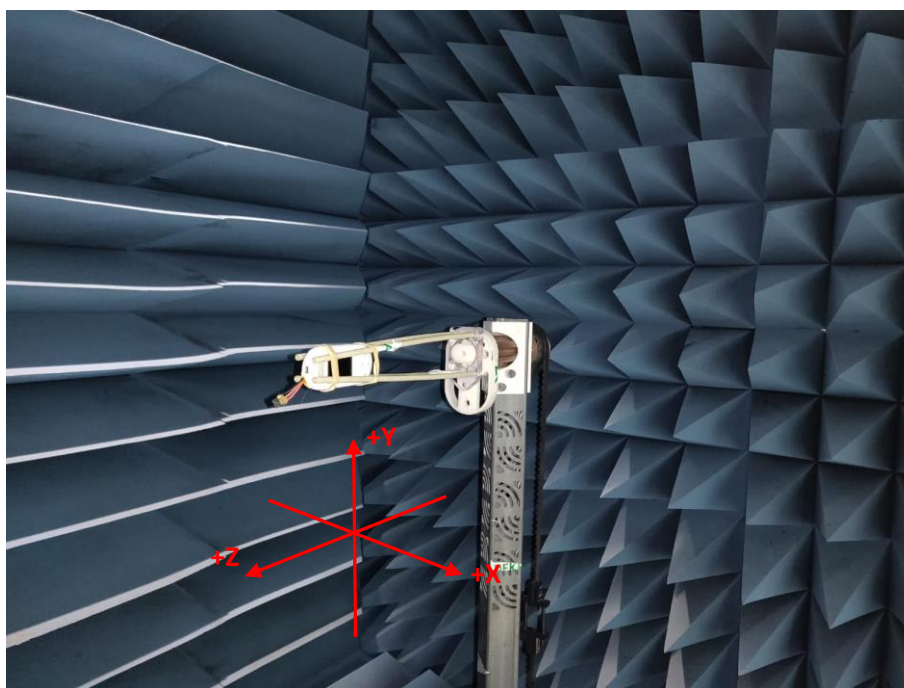
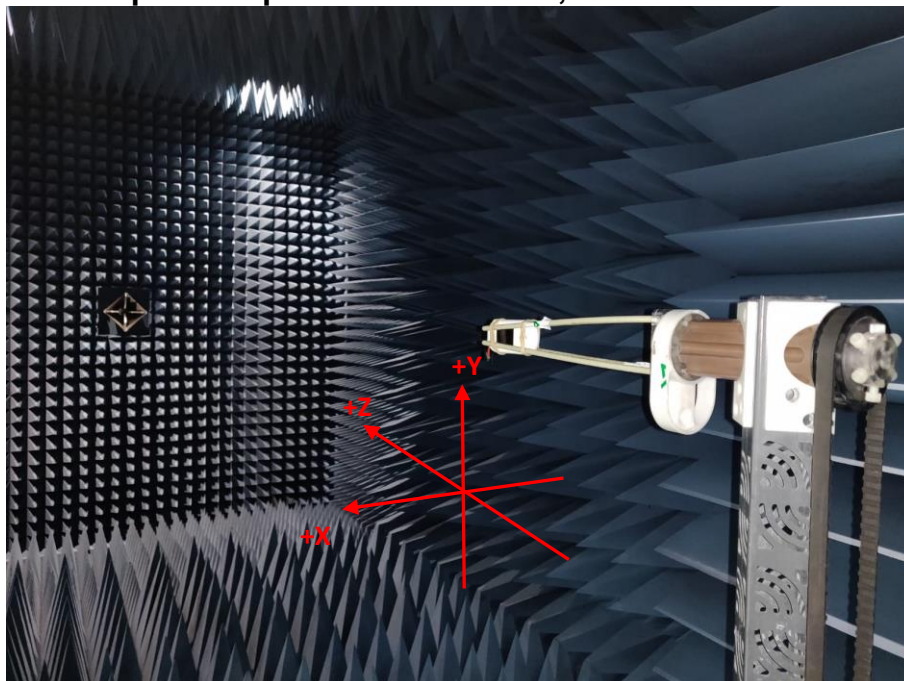


Fig 8. Free Space configuration set-up view.