



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

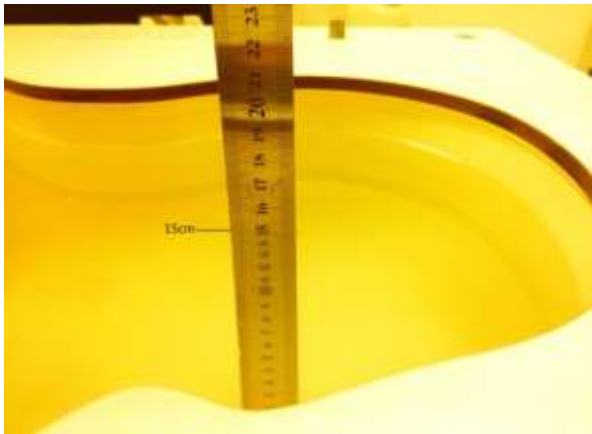
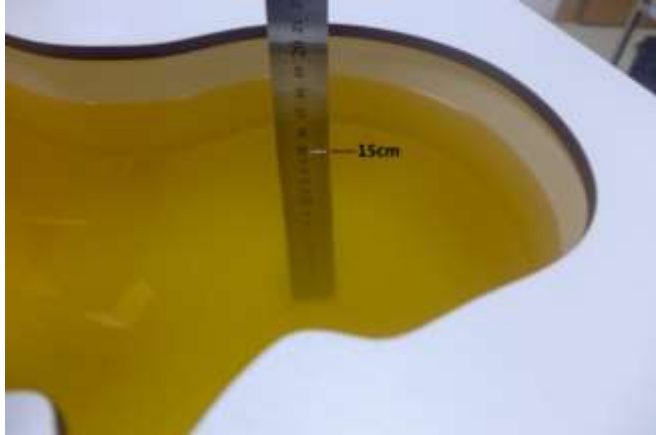
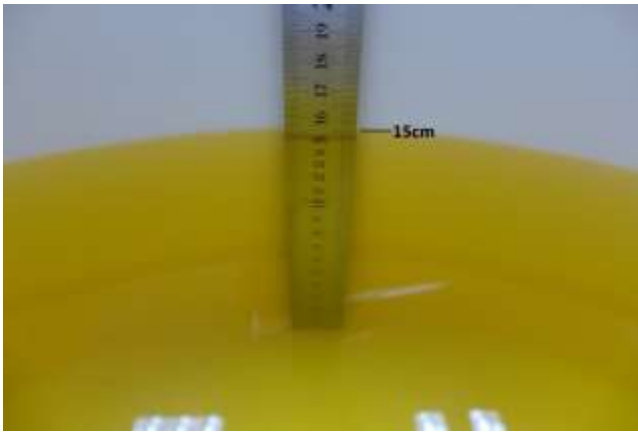
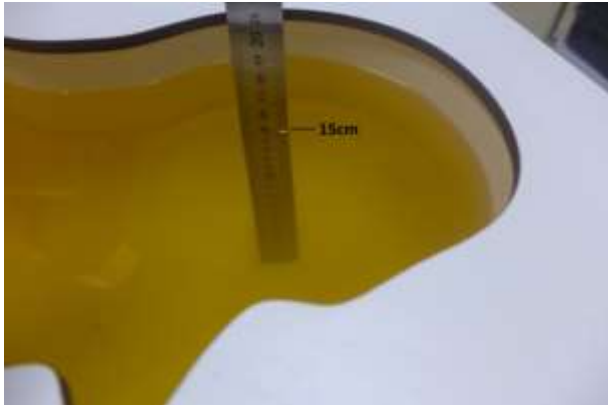
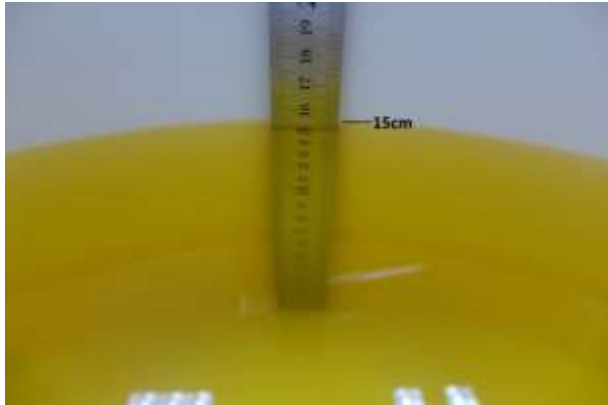
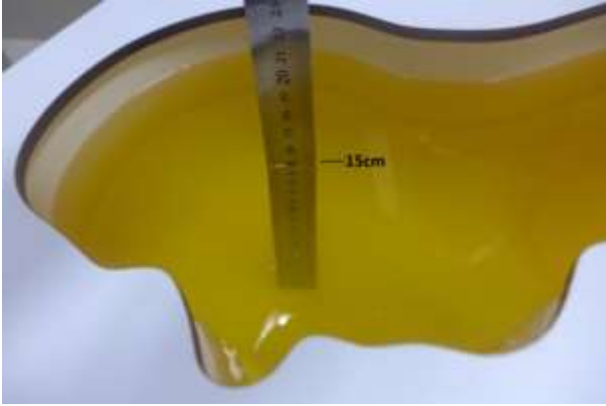
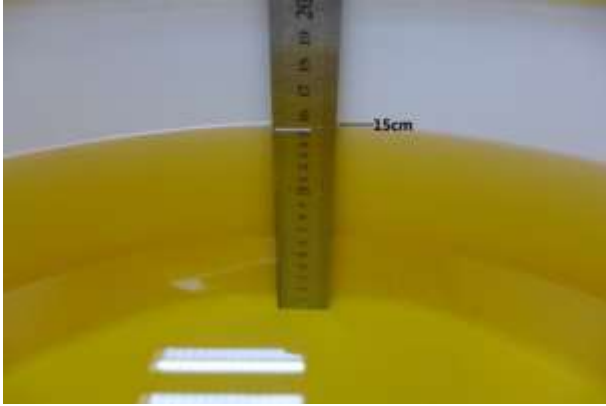
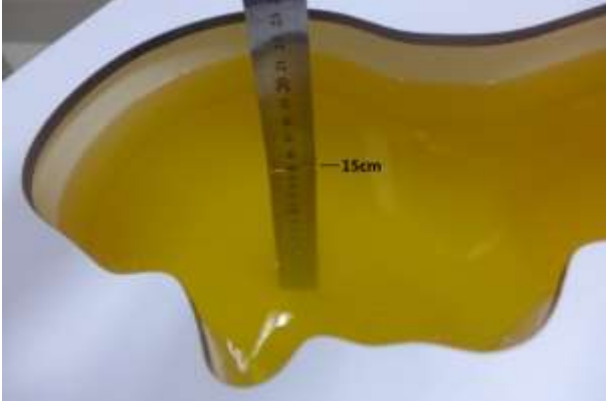
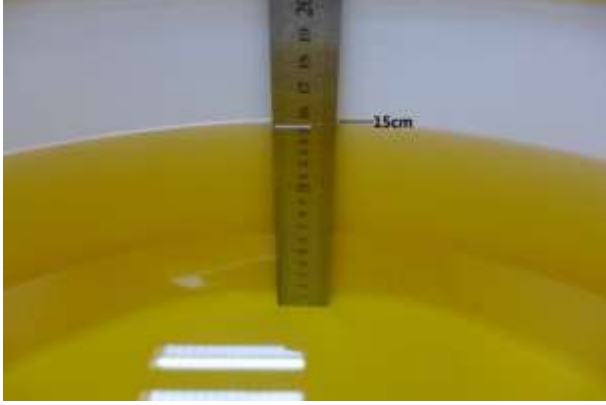
Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Body 1750
	
Photo 5: Tissue Simulant Liquid for Head 1900	Photo 6: Tissue Simulant Liquid for Body 1900
	

Photo 7: Tissue Simulant Liquid for Head 2450	Photo 8: Tissue Simulant Liquid for Body 2450
	
Photo 9: Tissue Simulant Liquid for Head 2600	Photo 10: Tissue Simulant Liquid for Body 2600
	

3. Photographs of EUT test position

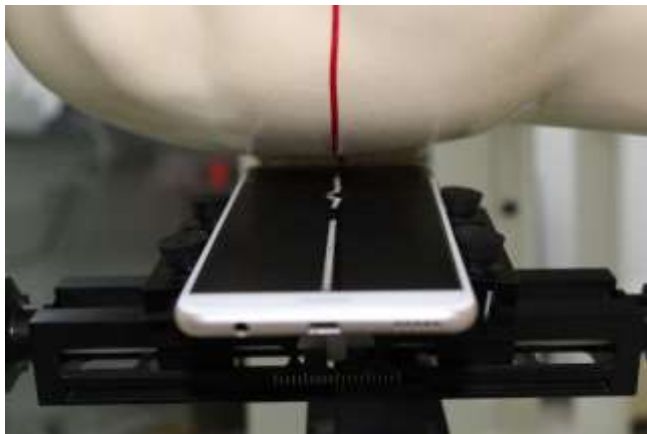
Photo 11: Left touch cheek	Photo 12: Left tilted 15 degree
	
Photo 13: Right touch cheek	Photo 14: Right tilted 15 degree
	
Photo 15: Front side 10mm	Photo 16: Back side 10mm
	

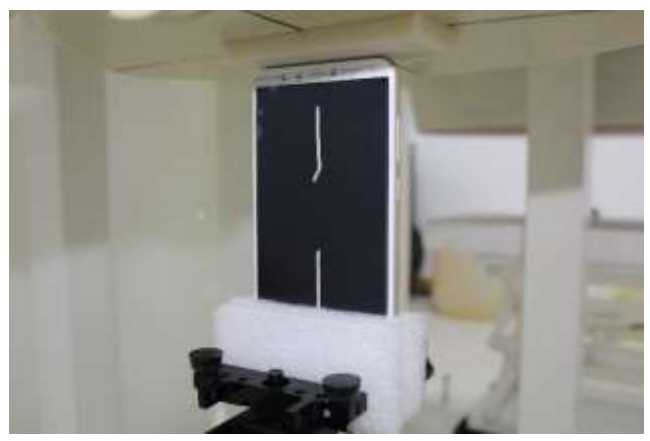
Photo 17: Left side 10mm	Photo 18: Right side 10mm
	
Photo 19: Top side 10mm	Photo 20: Bottom side 10mm
	
Photo 21: Front Side 0mm	Photo 22: Back Side 0mm
	

Photo 23: Bottom Side 0mm	Photo 24: Back Side 15mm
	
Photo 25: Front Side 15mm	Photo 26: Back Side 16mm
	
Photo 27: Front Side 12mm	NA
	NA

4. EUT Constructional Details

