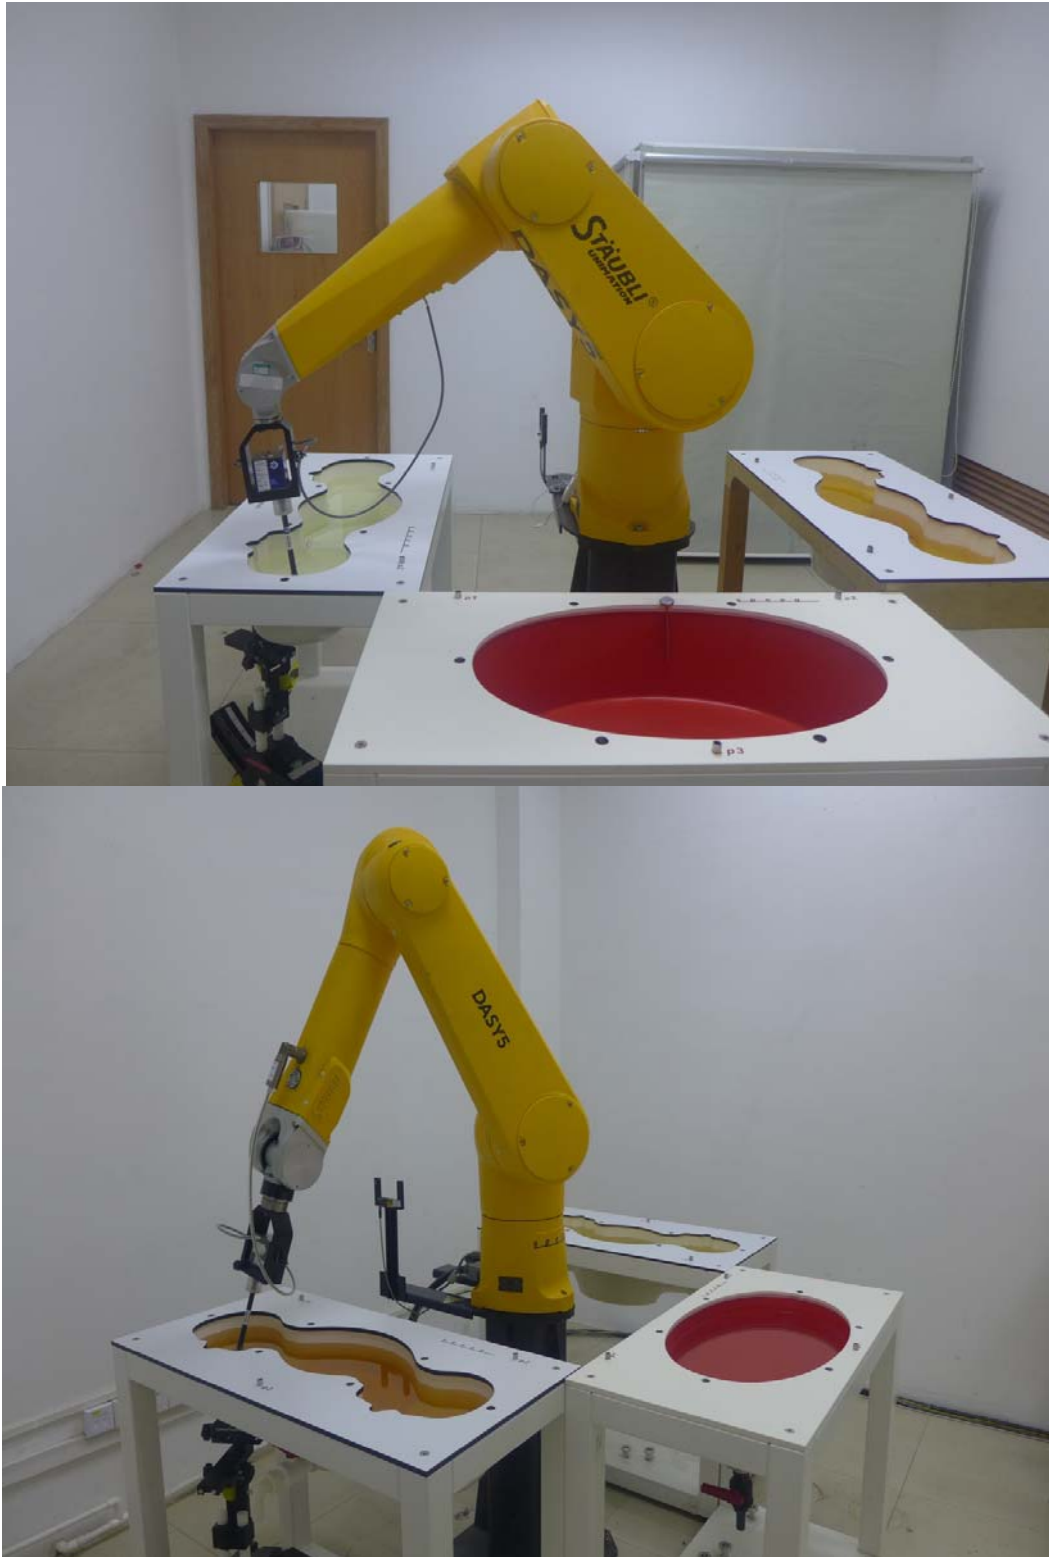


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

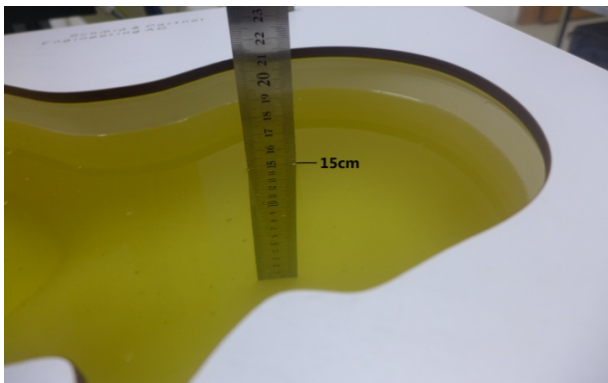
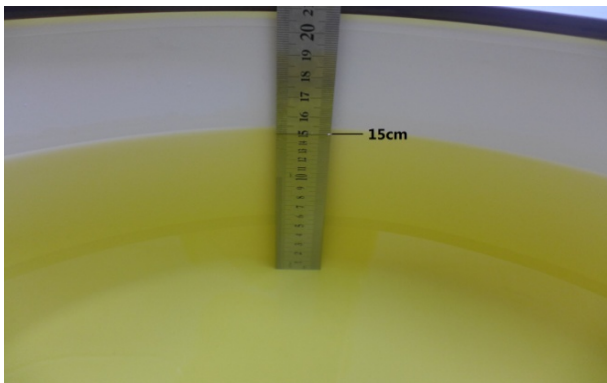
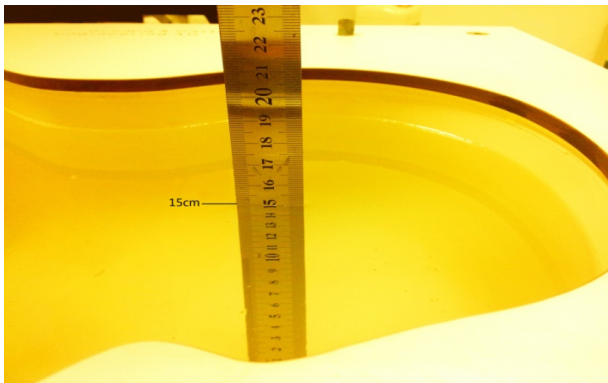
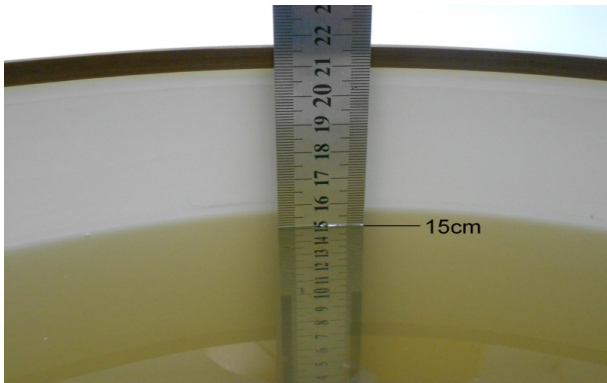
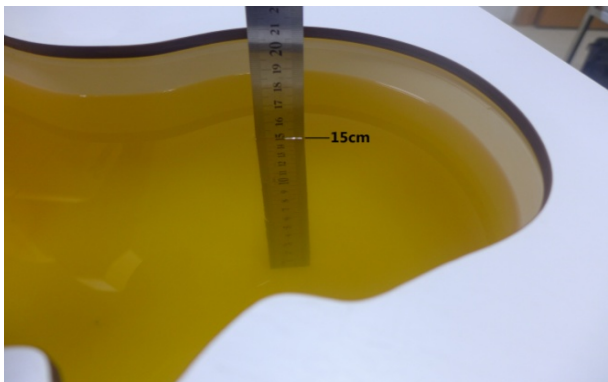
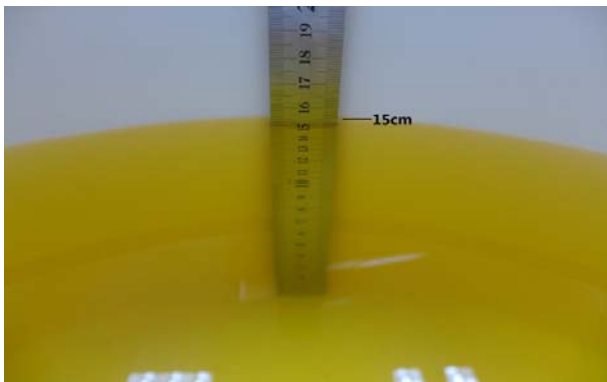
Photo 1: Tissue Simulant Liquid for Head 750 	Photo 2: Tissue Simulant Liquid for Body 750 
Photo 3: Tissue Simulant Liquid for Head 835 	Photo 4: Tissue Simulant Liquid for Body 835 
Photo 5: Tissue Simulant Liquid for Head 1750 	Photo 6: Tissue Simulant Liquid for Body 1750 

Photo 7: Tissue Simulant Liquid for Head 1900

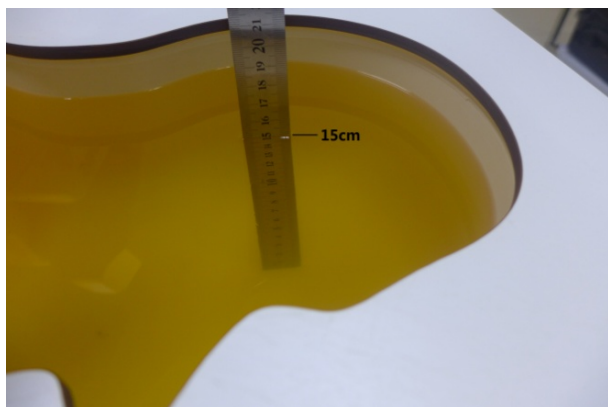


Photo 8: Tissue Simulant Liquid for Body 1900

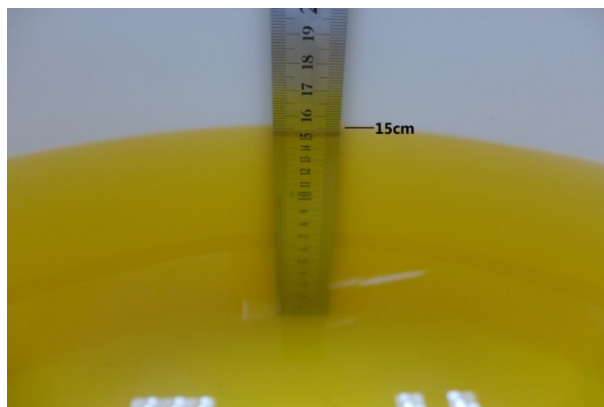


Photo 9: Tissue Simulant Liquid for Head 2450

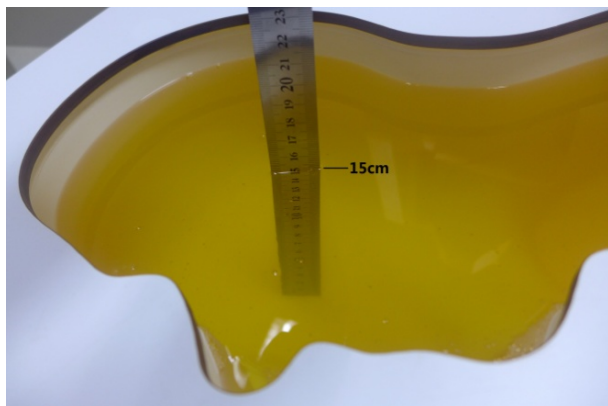


Photo 10: Tissue Simulant Liquid for Body 2450

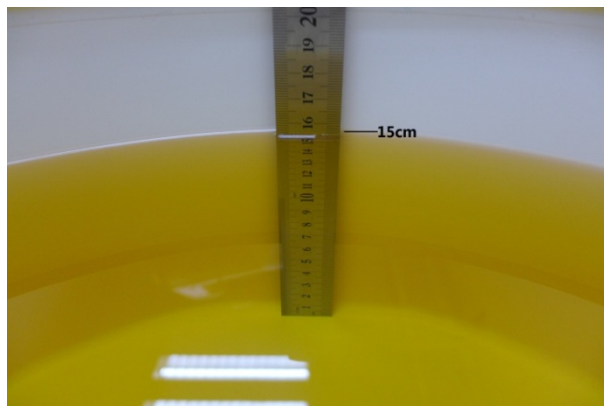


Photo 11: Tissue Simulant Liquid for Head 2600

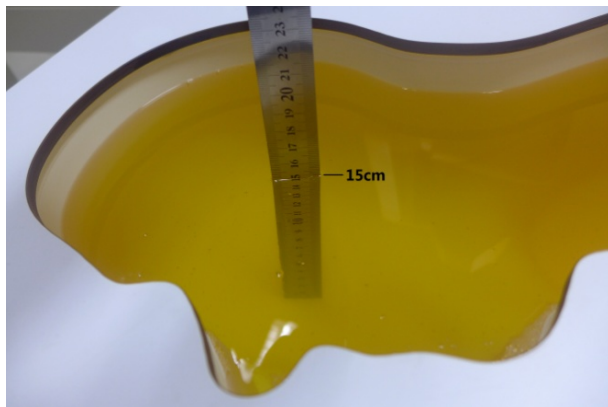


Photo 12: Tissue Simulant Liquid for Body 2600

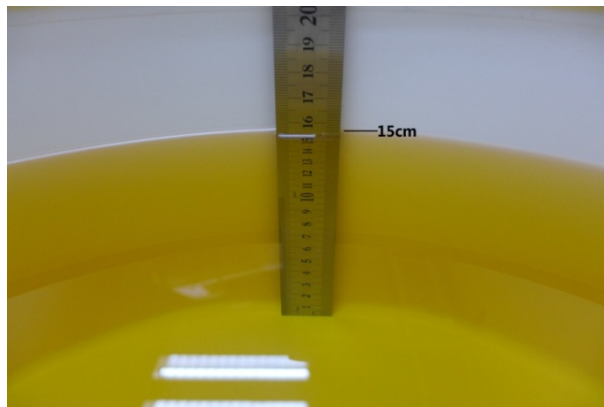


Photo 13: Tissue Simulant Liquid for Head 5G

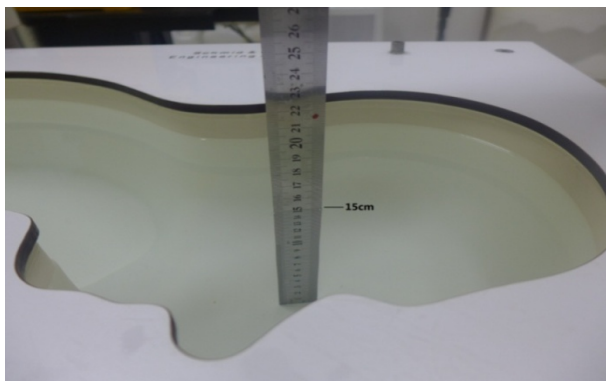
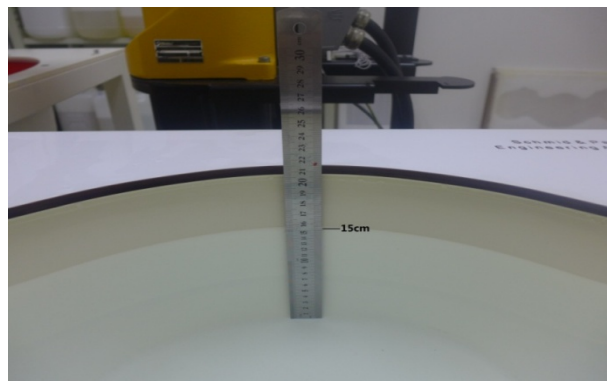


Photo 14: Tissue Simulant Liquid for Body 5G



3. Photographs of EUT test position

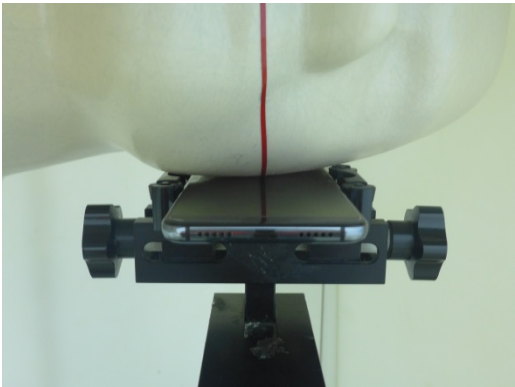
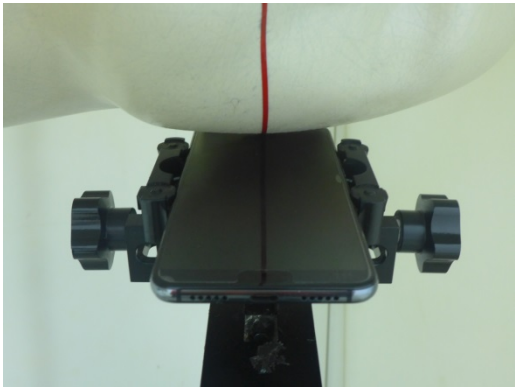
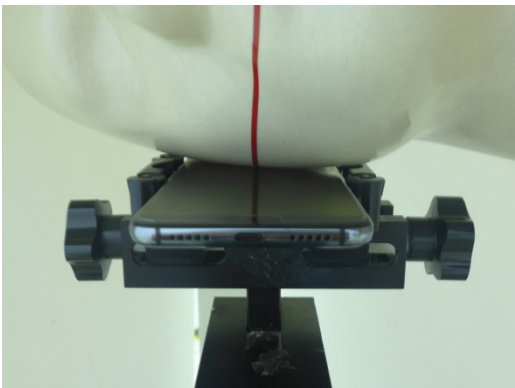
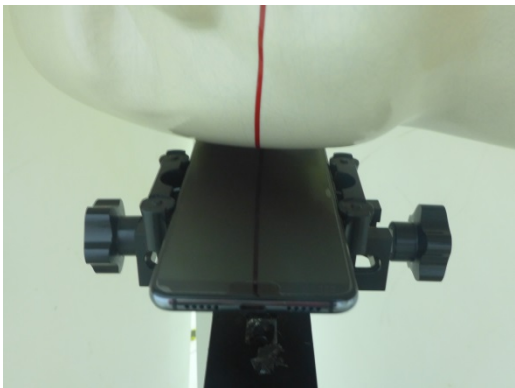
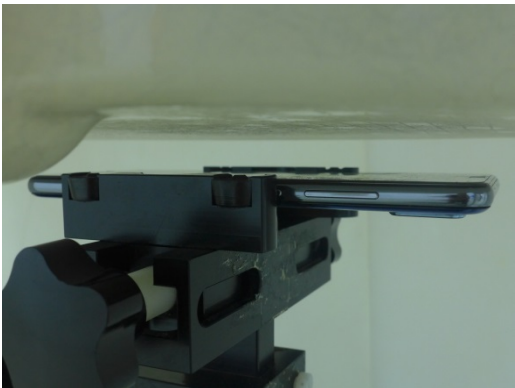
Photo 15: Left touch cheek	Photo 16: Left tilted 15 degree
	
Photo 17: Right touch cheek	Photo 18: Right tilted 15 degree
	
Photo 19: Front side 15mm	Photo 20: Back side 15mm
	

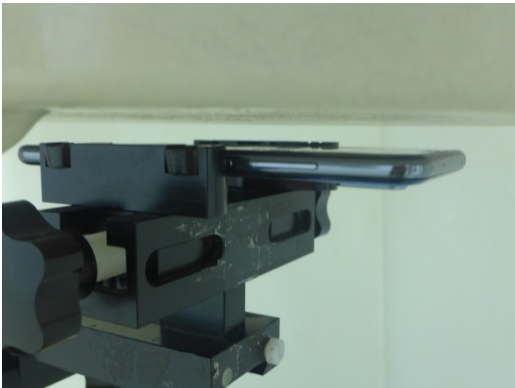
Photo 21: Front side 10mm	Photo 22: Back side 10mm
	
Photo 23: Left side 10mm	Photo 24: Right side 10mm
	
Photo 25: Top side 10mm	Photo 26: Bottom side 10mm
	

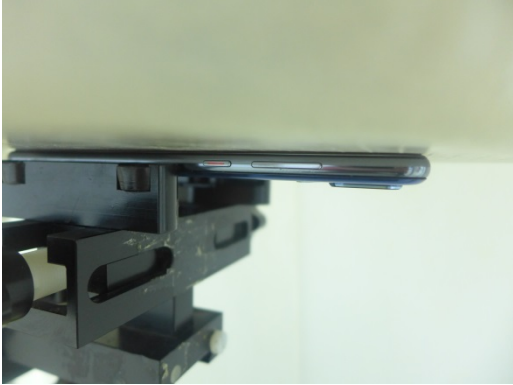
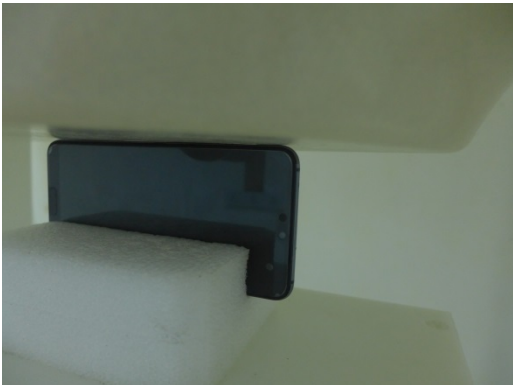
Photo 27: Front side 0mm	Photo 28: Back side 0mm
	
Photo 29: Left side 0mm	Photo 30: Right side 0mm
	
Photo 31: Top side 0mm	Photo 32: Bottom side 0mm
	

Photo 33: Bottom side 9mm	Photo 34: Bottom side 4mm
	

4. EUT Constructional Details

Photo 35: Front View	Photo 36: Back View
	