

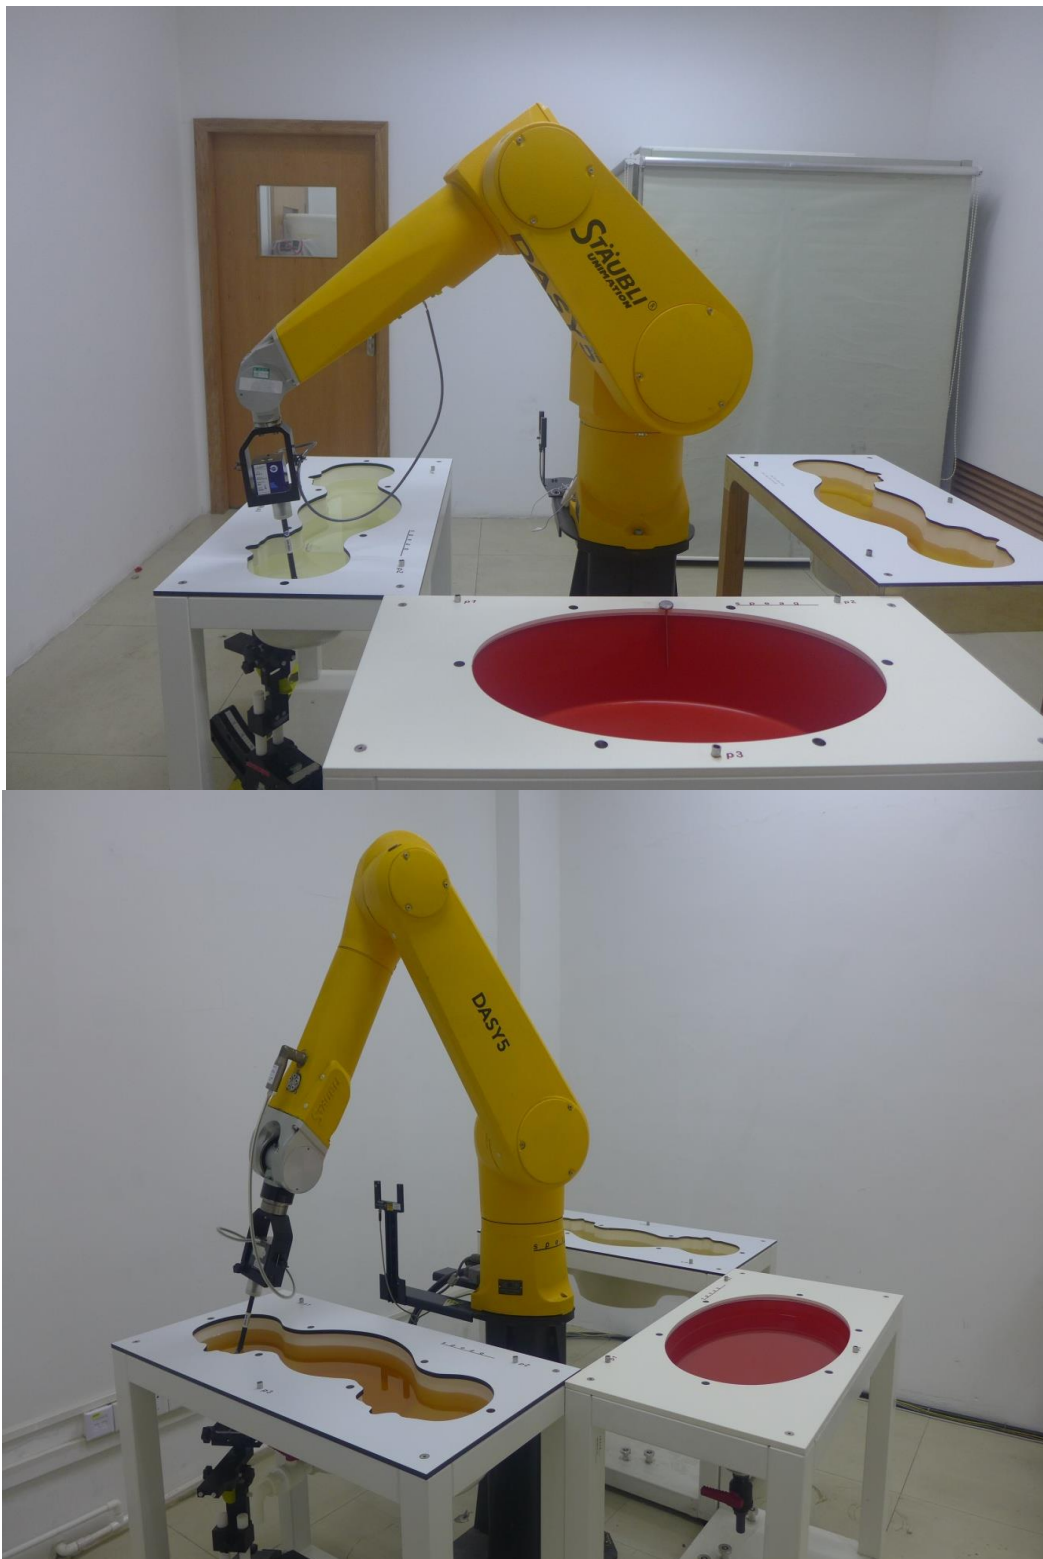


Appendix D

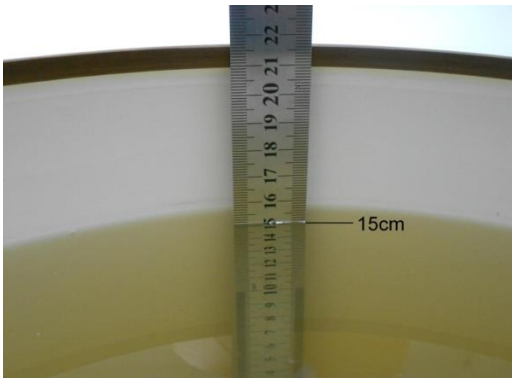


Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1900
	
Photo 3: Tissue Simulant Liquid for Head 2450	NA
	<p>NA</p>

3. Photographs of EUT test position

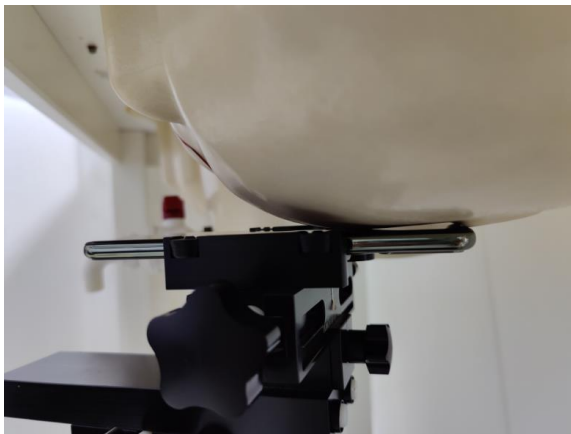
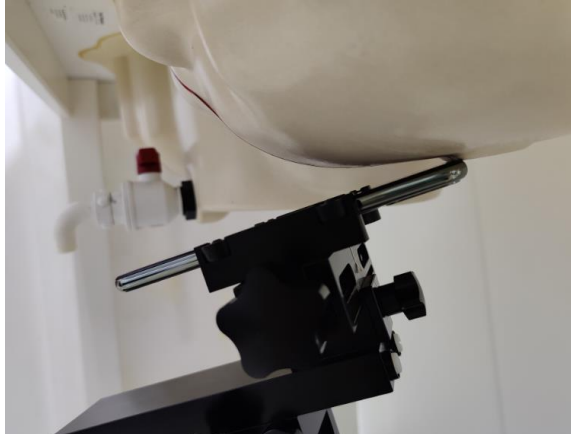
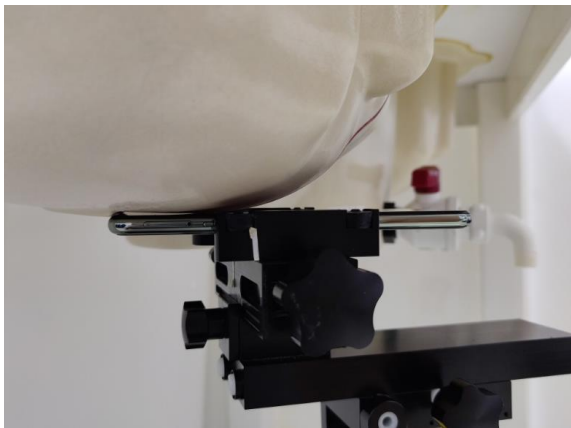







<p>Photo 4: Left touch cheek</p>	<p>Photo 5: Left tilted 15 degree</p>
	
<p>Photo 6: Right touch cheek</p>	<p>Photo 7: Right tilted 15 degree</p>
	
<p>Photo 8: Front side 10mm</p>	<p>Photo 9: Back side 10mm</p>
	



Photo 10: Left side 10mm	Photo 11: Right side 10mm
	
Photo 12: Top side 10mm	Photo 13: Bottom side 10mm
	

4. EUT Constructional Details

Photo 14: Front View	Photo 15: Back View
