

# Appendix D

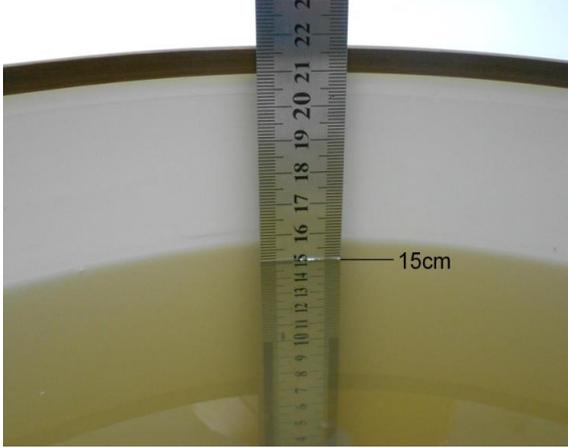
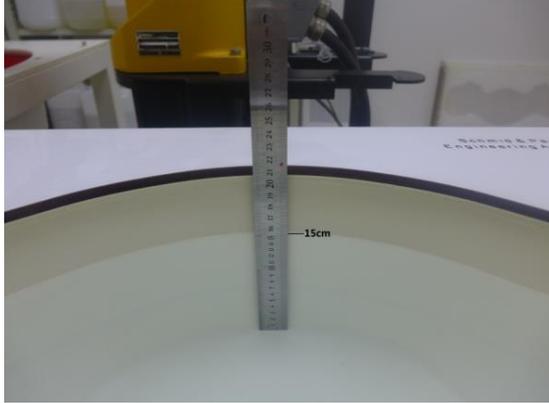
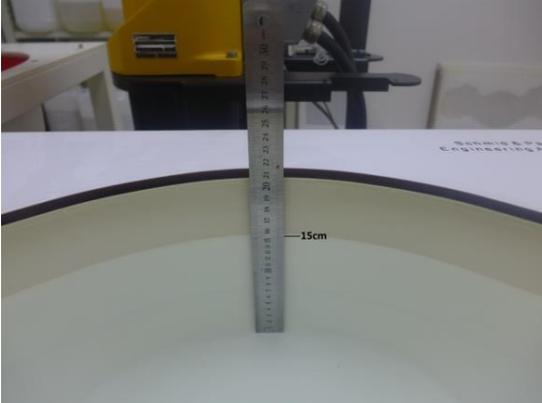
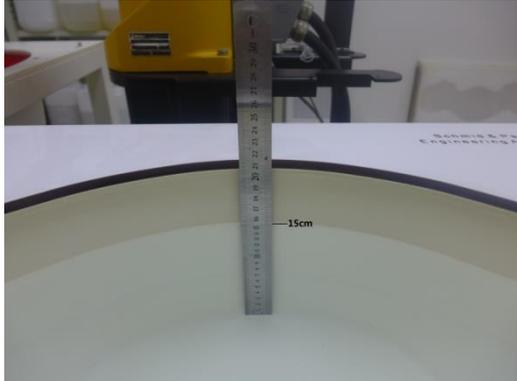
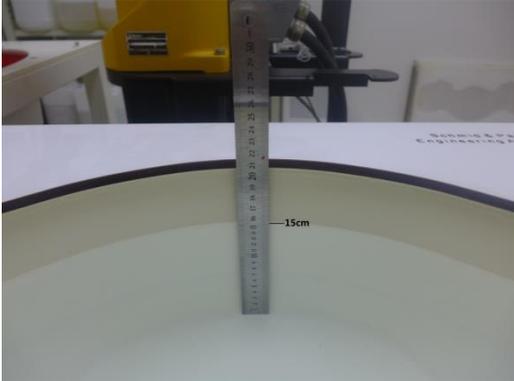
## Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System



## 2. Photographs of Tissue Simulate Liquid

<p><b>Photo 1: Tissue Simulant Liquid for Head 835</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Head 1800</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 1900</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Head 2450</b></p>
	
<p><b>Tissue Simulant Liquid for Head 2600</b></p>	
	

### 3. Photographs of EUT test position

<p>Photo 5: Front side 0mm</p>	<p>Photo 6: Back side 0mm</p>
	
<p>Photo 7: Left side 0mm</p>	<p>Photo 8: Right side 0mm</p>
	
<p>Photo 9: Top side 0mm</p>	<p>Photo 10: Bottom side 0mm</p>
	

## 4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.