

**Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

**DASY**

**Dipole Validation Kit**

**Type: D835V2**

**Serial: 437**

Manufactured: December 15, 2000  
Calibrated: August 23, 2001

## 1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with muscle simulating solution of the following electrical parameters at 835 MHz:

Relative Dielectricity	55,3	± 5%
Conductivity	0.92 mho/m	± 5%

The DASY3 System (Software version 3.1c) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.10 at 835 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW ± 3 %. The results are normalized to 1W input power.

## 2. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 1. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

averaged over 1 cm <sup>3</sup> (1 g) of tissue:	<b>10.3 mW/g</b>
averaged over 10 cm <sup>3</sup> (10 g) of tissue:	<b>6.68 mW/g</b>

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well. The estimated sensitivities of SAR-values and penetration depths to the liquid parameters are listed in the DASY Application

Note 4: 'SAR Sensitivities'.

### 3. Dipole impedance and return loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	<b>1.458 ns</b>	(one direction)
Transmission factor:	<b>0.989</b>	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 835 MHz:	$\text{Re}\{Z\} = 44,9 \, \Omega$
	$\text{Im}\{Z\} = -10,4 \, \Omega$
Return Loss at 835 MHz	<b>-18,3 dB</b>

### 4. Handling

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Do not apply excessive force to the dipole arms, because they might bend. If the dipole arms have to be bent back, take care to release stress to the soldered connections near the feedpoint; they might come off.


After prolonged use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

calibration\_data\_fcc\_supplement\_c\_2.0.doc/28.09.2001/AB


06/23/01

Validation Dipole D835V2 SN-437, d = 15 mm

Frequency: 835 MHz; Antenna Input Power: 250 [mW]  
SAR Phantom: Flat Section; Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0  
Probe: ET3DV6 - SN1507; Conn-F(6, 10, 6, 10) at 835 MHz; Muscle 835 MHz;  $\sigma = 0.92 \text{ mho/m}$ ,  $\epsilon_r = 55.3$ ,  $\rho = 1.00 \text{ g/cm}^3$   
Cubes (2): Peak: 4.04 mW/g  $\pm 0.02 \text{ dB}$ , SAR (1g): 2.57 mW/g  $\pm 0.02 \text{ dB}$ , SAR (10g): 1.67 mW/g  $\pm 0.02 \text{ dB}$  (Worst-case extrapolation)  
Penetration depth: 12.9 (11.2, 14.9) [mm]  
Power drift: -0.01 dB

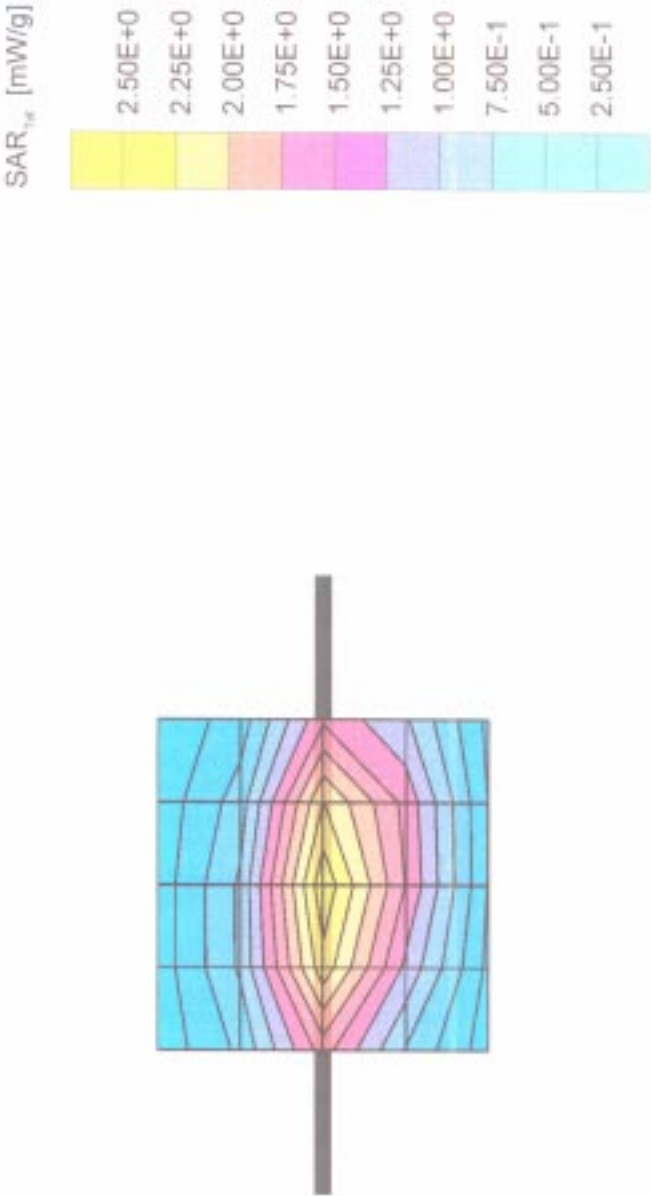

Schmid & Partner Engineering AG, Zurich, Switzerland

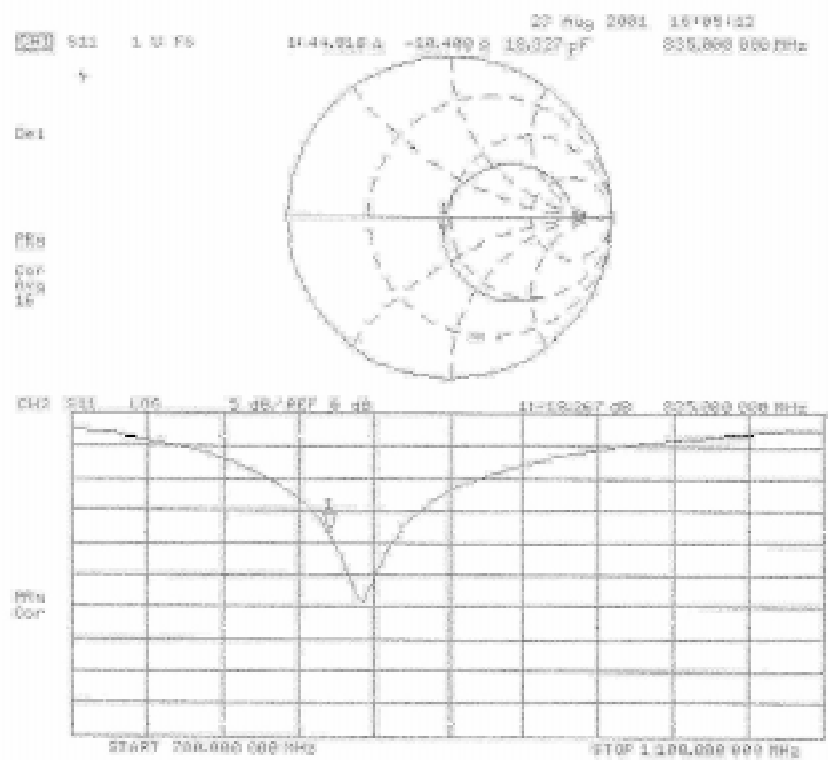

## Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

### Calibration Certificate

#### 1900 MHz System Validation Dipole

Type:

**D1900V2**

Serial Number:

**535**

Place of Calibration:

**Zurich**

Date of Calibration:

**Apr. 24, 2001**

Calibration Interval:

**24 months**

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

*M. Klotz, M. J. J. J.*

Approved by:

*Polina C. Klotz*

**Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

**DASY3**

**Dipole Validation Kit**

**Type: D1900V2**

**Serial: 535**

Manufactured: March 22, 2001  
Calibrated: April 24, 2001

## 1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with brain simulating sugar solution of the following electrical parameters at 1900 MHz:

Relative permittivity	<b>39.2</b>	± 5%
Conductivity	<b>1.47 mho/m</b>	± 10%

The DASY3 System (Software version 3.1c) with a dosimetric E-field probe ET3DV6 (SN:1507, conversion factor 5.57 at 1800 MHz) was used for the measurements.

The dipole feedpoint was positioned below the center marking and oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW ± 3 %. The results are normalized to 1W input power.

## 2. SAR Measurement

Standard SAR-measurements were performed with the head phantom according to the measurement conditions described in section 1. The results (see figure) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

averaged over 1 cm <sup>3</sup> (1 g) of tissue:	<b>43.2 mW/g</b>
averaged over 10 cm <sup>3</sup> (10 g) of tissue:	<b>21.9 mW/g</b>

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well. The estimated sensitivities of SAR-values and penetration depths to the liquid parameters are listed in the DASY Application Note 4: 'SAR Sensitivities'.



### 3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	<b>1.204 ns</b>	(one direction)
Transmission factor:	<b>0.988</b>	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 1900 MHz:	$\text{Re}\{Z\} = $ <b>51.0 <math>\Omega</math></b>
----------------------------------	---

	$\text{Im}\{Z\} = $ <b>-0.1 <math>\Omega</math></b>
--	---

Return Loss at 1900 MHz	<b>-40.3 dB</b>
-------------------------	-----------------

### 4. Handling

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.


Do not apply excessive force to the dipole arms, because they might bend. If the dipole arms have to be bent back, take care to release stress to the soldered connections near the feedpoint, they might come off.


After prolonged use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


04/23/01

Validation Dipole D1900V2 SN:535, d = 10 mm

Frequency: 1900 MHz; Antenna Input Power: 250 [mW]  
Generic Twin Phantom; Flat Section; Grid Spacing: Dx = 15.0, Dy = 15.0, Dz = 10.0  
Probe: ET3DV6 - SN1507; ConvF(5.57,5.57) at 1800 MHz; IEEE1528 1900 MHz;  $\alpha = 1.47$  mho/m;  $\rho = 39.2$  g = 1.00 g/cm<sup>3</sup>  
Cubes (2): Peak: 20.8 mW/g  $\pm$  0.04 dB; SAR (1g): 10.8 mW/g  $\pm$  0.03 dB; SAR (10g): 5.48 mW/g  $\pm$  0.02 dB (Worst-case extrapolation)  
Penetration depth: 7.8 (7.4, 8.9) [mm]  
Powerdrift: 0.01 dB

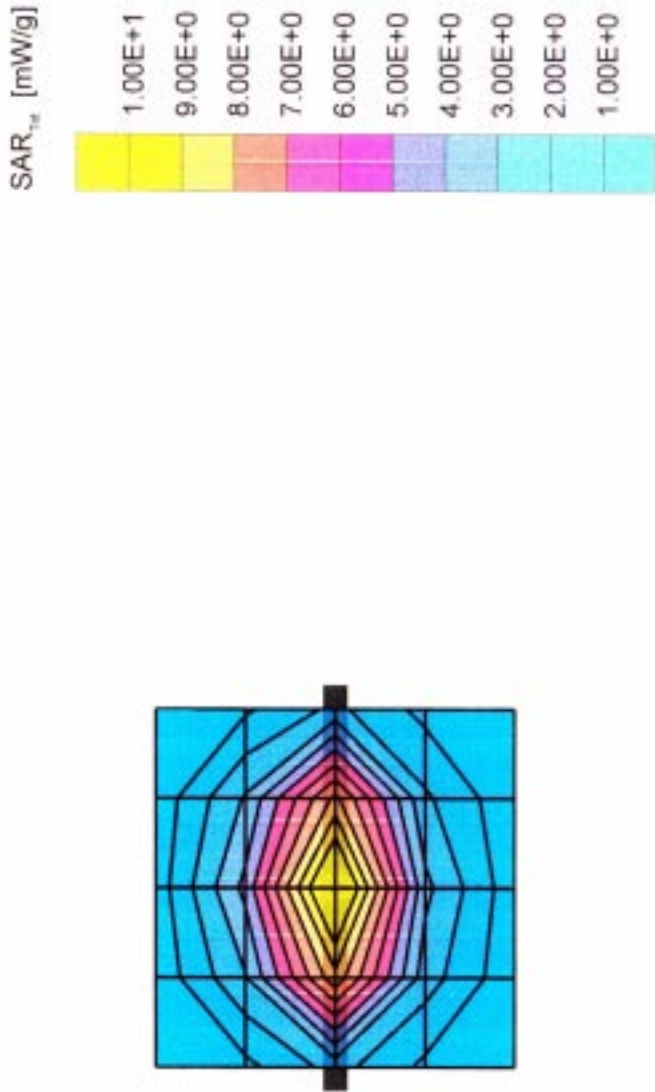

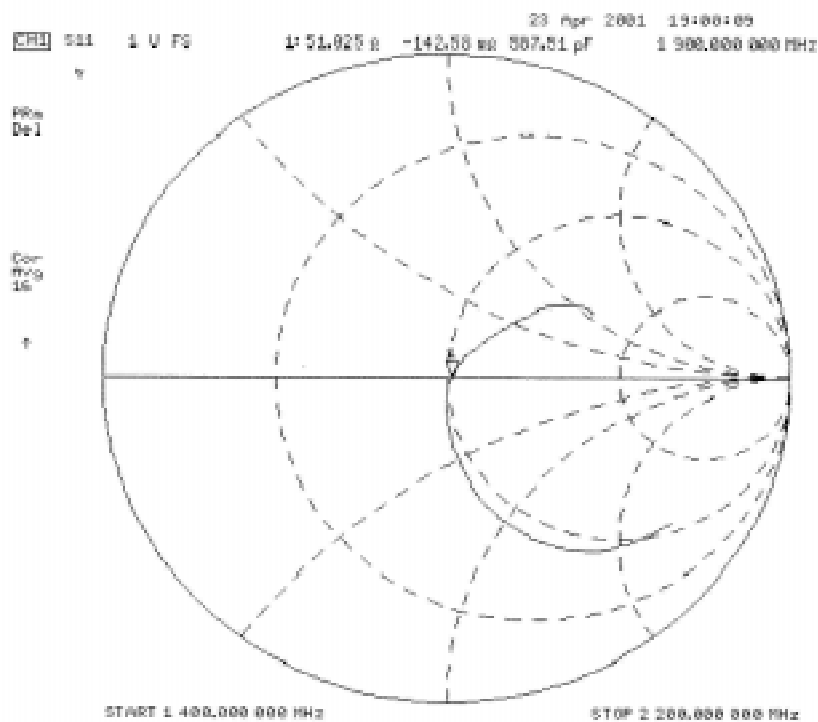

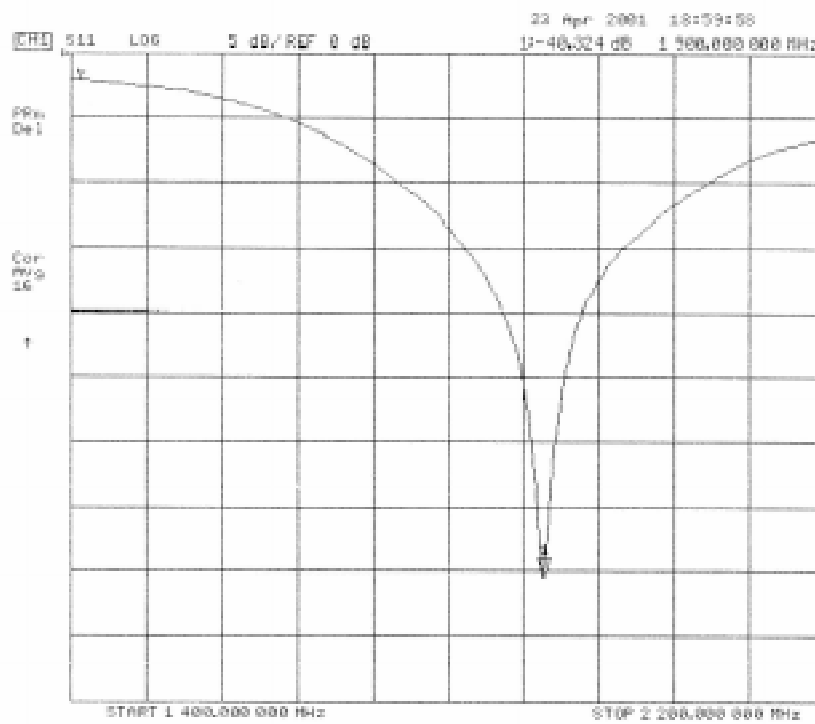

## Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

### Calibration Certificate

#### 1900 MHz System Validation Dipole (Muscle Tissue)

Type:

D1900V2

Serial Number:

535

Place of Calibration:

Zurich

Date of Calibration:

August 23, 2001


Calibration Interval:

24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:



Approved by:



**Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

**DASY**

**Dipole Validation Kit**

**Type: D1900V2**

**Serial: 535**

Manufactured: March 22, 2001  
Calibrated: August 23, 2001

## 1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with muscle simulating solution of the following electrical parameters at 1900 MHz:

Relative Dielectricity	53.5	± 5%
Conductivity	1.46 mho/m	± 5%

The DASY3 System (Software version 3.1c) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 5.0 at 1900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 20mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW ± 3 %. The results are normalized to 1W input power.

## 2. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 1. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

averaged over 1 cm <sup>3</sup> (1 g) of tissue:	40.8 mW/g
averaged over 10 cm <sup>3</sup> (10 g) of tissue:	21.2 mW/g

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well. The estimated sensitivities of SAR-values and penetration depths to the liquid parameters are listed in the DASY Application Note 4: "SAR Sensitivities".

### 3. Dipole impedance and return loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	<b>1.203 ns</b>	(one direction)
Transmission factor:	<b>0.993</b>	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 1900 MHz:  $\text{Re}\{Z\} = 42.0 \, \Omega$

$\text{Im}\{Z\} = -9.5 \, \Omega$

Return Loss at 1900 MHz: **-17.5 dB**

### 4. Handling

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Do not apply excessive force to the dipole arms, because they might bend. If the dipole arms have to be bent back, take care to release stress to the soldered connections near the feedpoint; they might come off.

After prolonged use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.



08/23/01

Validation Dipole D1900V2 SN:535, d = 10 mm

Frequency: 1900 MHz; Antenna Input Power: 250 [mW]  
SAR Phantom: Flat Section; Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0  
Probe: ET3DV6 - SN1507; ConvF(5.00,5.00) at 1900 MHz; Muscle 1900 MHz;  $\sigma = 1.46 \text{ mho/m}$ ,  $\epsilon_r = 53.5$ ,  $\rho = 1.00 \text{ g/cm}^3$   
Cubes (2): Peak: 19.1 mW/g  $\pm 0.04 \text{ dB}$ , SAR (1g): 10.2 mW/g  $\pm 0.03 \text{ dB}$ , SAR (10g): 5.29 mW/g  $\pm 0.03 \text{ dB}$  (Worst-case extrapolation)  
Penetration depth: 8.8 (7.9, 10.5) [mm]  
Powerdrift: 0.01 dB

