

System Performance Check Report for D1750V2 - SN1180

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1750.000	TSL Permittivity	40.1
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.38
Conversion Factor	7.82	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2025-01-22	Phantom	ELI V8.0 (20deg probe tilt)
DAE Calibration Date	DAE4 Sn1591 2025-02-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.61	3.61
psSAR10g [W/Kg]	1.99	2.00
Power Drift [dB]		-0.04
Dist 3dB Peak [mm]		10.8
M2/M1 [%]		83.0

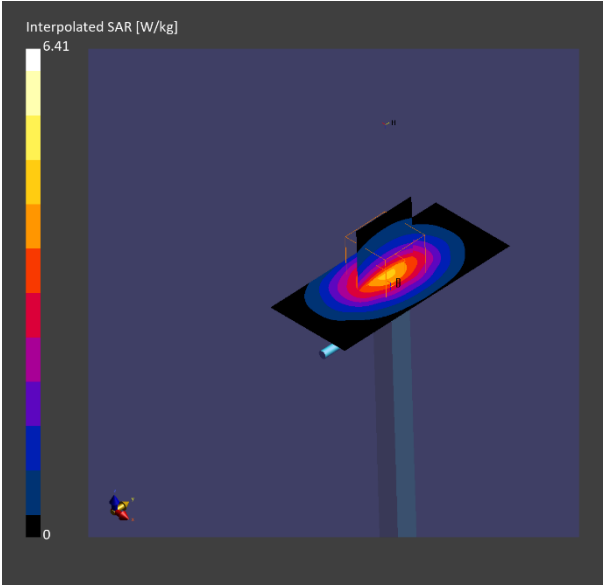

System Performance Check Report for D2600V2 - SN1097

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2600.000	TSL Permittivity	38.7
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.94
Conversion Factor	7.03	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2025-01-22	Phantom	ELI V8.0 (20deg probe tilt)
DAE Calibration Date	DAE4 Sn1591 2025-02-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	5.75	5.84
psSAR10g [W/Kg]	2.57	2.71
Power Drift [dB]		0.01
Dist 3dB Peak [mm]		9.0
M2/M1 [%]		80.7

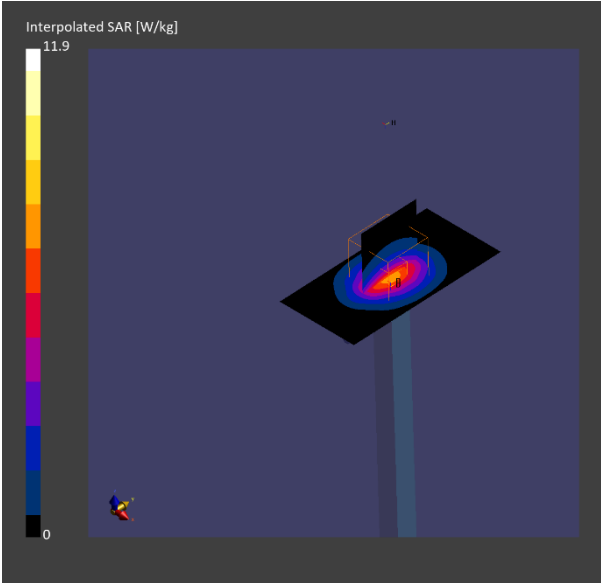

System Performance Check Report for D1900V2 - SN5d199

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1900.000	TSL Permittivity	40.1
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.40
Conversion Factor	7.51	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2025-01-22	Phantom	ELI V8.0 (20deg probe tilt)
DAE Calibration Date	DAE4 Sn1591 2025-02-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.84	3.85
psSAR10g [W/Kg]	2.03	2.08
Power Drift [dB]		0.03
Dist 3dB Peak [mm]		10.8
M2/M1 [%]		84.3

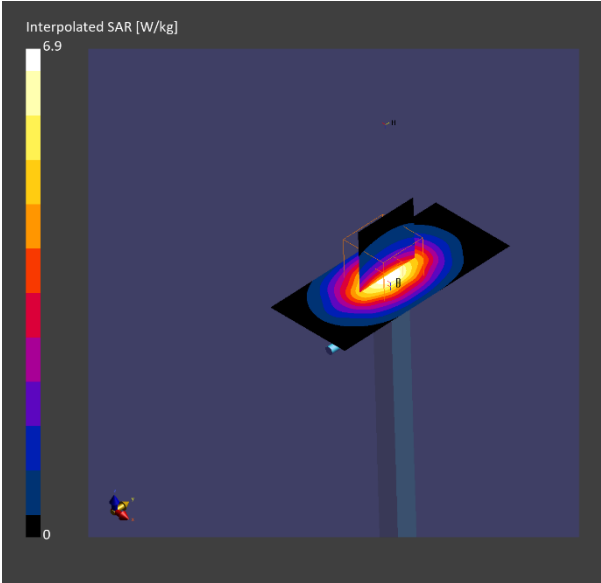

System Performance Check Report for D750V3 - SN1122

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	750.000	TSL Permittivity	42.7
Group / UID	CW / 0--	TSL Conductivity [S/m]	0.896
Conversion Factor	9.46	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2025-01-22	Phantom	ELI V8.0 (20deg probe tilt)
DAE Calibration Date	DAE4 Sn1591 2025-02-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.793	0.808
psSAR10g [W/Kg]	0.536	0.554
Power Drift [dB]		-0.01
Dist 3dB Peak [mm]		> 15.0
M2/M1 [%]		87.6

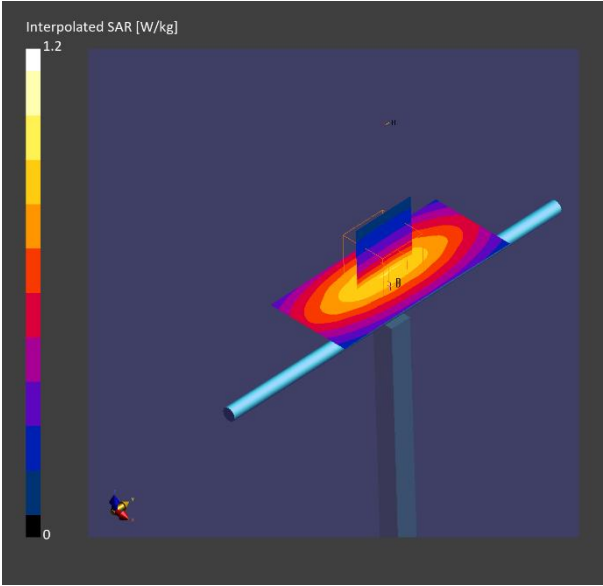

System Performance Check Report for D2450V2 - SN960

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2450.000	TSL Permittivity	39.9
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.74
Conversion Factor	7.39	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2025-01-22	Phantom	ELI V8.0 (20deg probe tilt)
DAE Calibration Date	DAE4 Sn1591 2025-02-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	5.29	5.36
psSAR10g [W/Kg]	2.49	2.64
Power Drift [dB]		0.04
Dist 3dB Peak [mm]		9.5
M2/M1 [%]		84.6

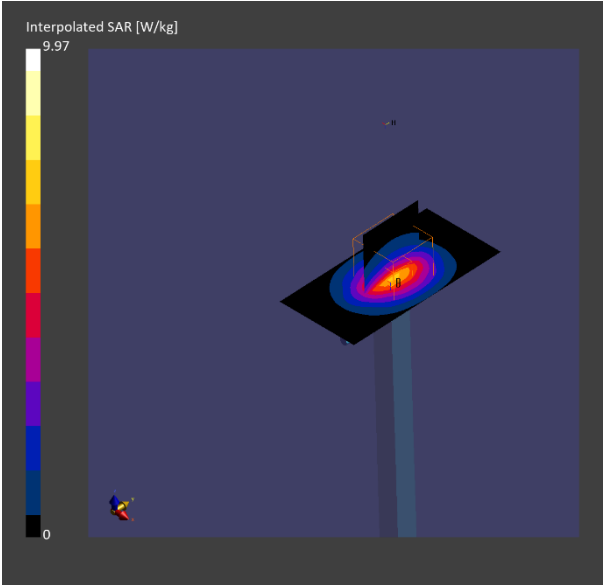

System Performance Check Report for D5GHzV2 - SN1209

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	5600.000	TSL Permittivity	35.4
Group / UID	CW / 0--	TSL Conductivity [S/m]	5.04
Conversion Factor	5.21	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2025-01-22	Phantom	ELI V8.0 (20deg probe tilt)
DAE Calibration Date	DAE4 Sn1591 2025-02-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	6.97	7.53
psSAR10g [W/Kg]	2.00	2.25
Power Drift [dB]		0.03
Dist 3dB Peak [mm]		7.6
M2/M1 [%]		65.0

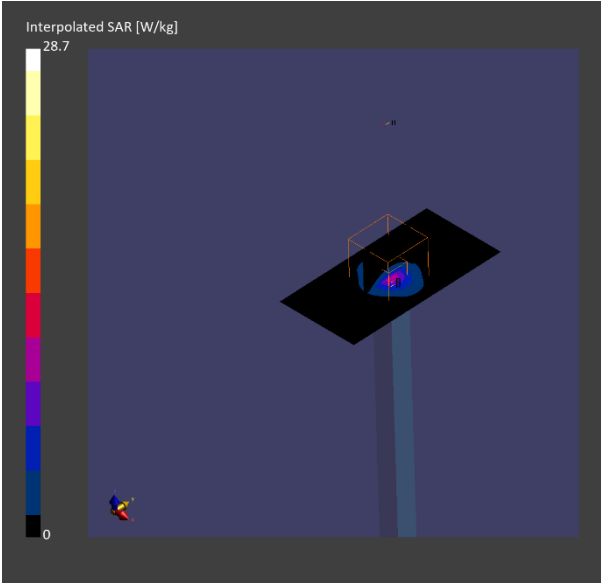

System Performance Check Report for D835V2 - SN4d194

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	835.000	TSL Permittivity	42.1
Group / UID	CW / 0--	TSL Conductivity [S/m]	0.883
Conversion Factor	9.11	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration

Probe Calibration Date	EX3DV4 - SN7646 2025-01-22	Phantom	ELI V8.0 (20deg probe tilt)
DAE Calibration Date	DAE4 Sn1591 2025-02-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.929	0.924
psSAR10g [W/Kg]	0.614	0.624
Power Drift [dB]		-0.03
Dist 3dB Peak [mm]		> 15.0
M2/M1 [%]		88.4

