

# Appendix D

## Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System



## 2. Photographs of Tissue Simulate Liquid





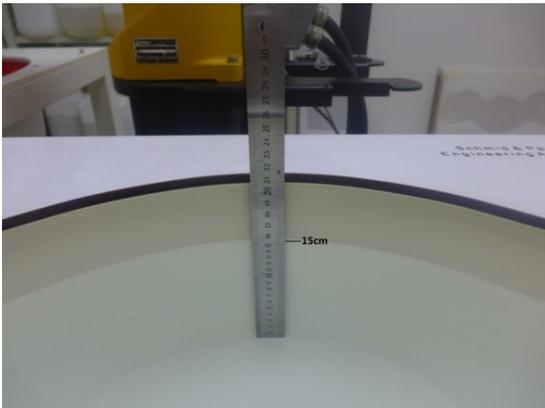
<p><b>Photo 1: Tissue Simulant Liquid for Body 835</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Body 1900</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Body 2450</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Head 835</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Head 1900</b></p>	<p><b>Photo 6: Tissue Simulant Liquid for Head 2300</b></p>
	

Photo 7: Tissue Simulant Liquid for Head 2600

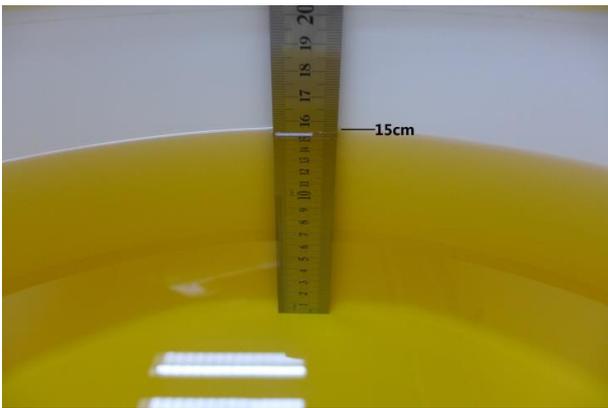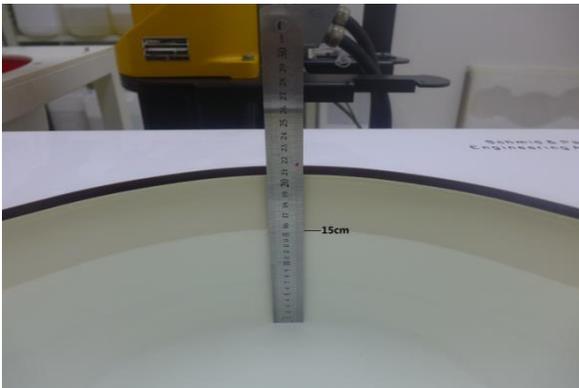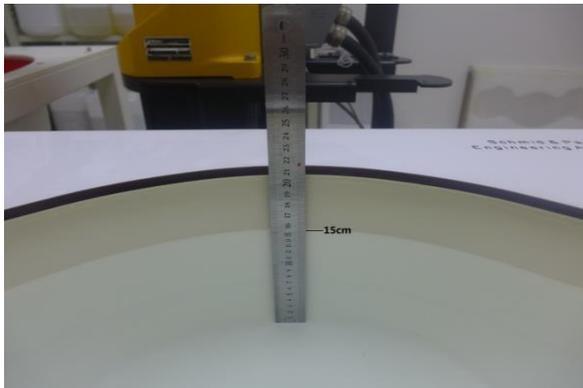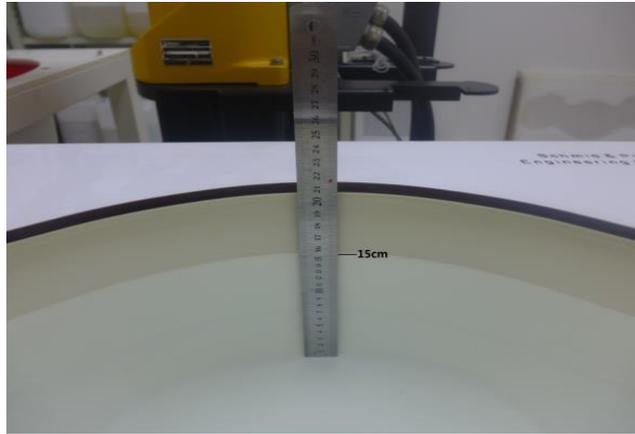

### 3. Photographs of EUT test position

<p>Photo 8: Front side 5mm</p>	<p>Photo 9: Back side 5mm</p>
	
<p>Photo 10: Left side 5mm</p>	<p>Photo 11: Right side 5mm</p>
	
<p>Photo 12: Top side 5mm</p>	<p>Photo 13: Bottom side 5mm</p>
	

<p><b>Photo 14: Front side 0mm</b></p>	<p><b>Photo 15: Back side 0mm</b></p>
	
<p><b>Photo 16: Left side 0mm</b></p>	<p><b>Photo 17: Right side 0mm</b></p>
	
<p><b>Photo 18: Top side 0mm</b></p>	<p><b>Photo 19: Bottom side 0mm</b></p>
	

### 4. EUT Constructional Details

<p align="center"><b>Photo 20: Front View</b></p>	<p align="center"><b>Photo 21: Back View</b></p>
	
<p align="center"><b>Photo 22: Left View</b></p>	<p align="center"><b>Photo 23: Right View</b></p>
	
<p align="center"><b>Photo 24: Top View</b></p>	<p align="center"><b>Photo 25: Bottom View</b></p>
	