

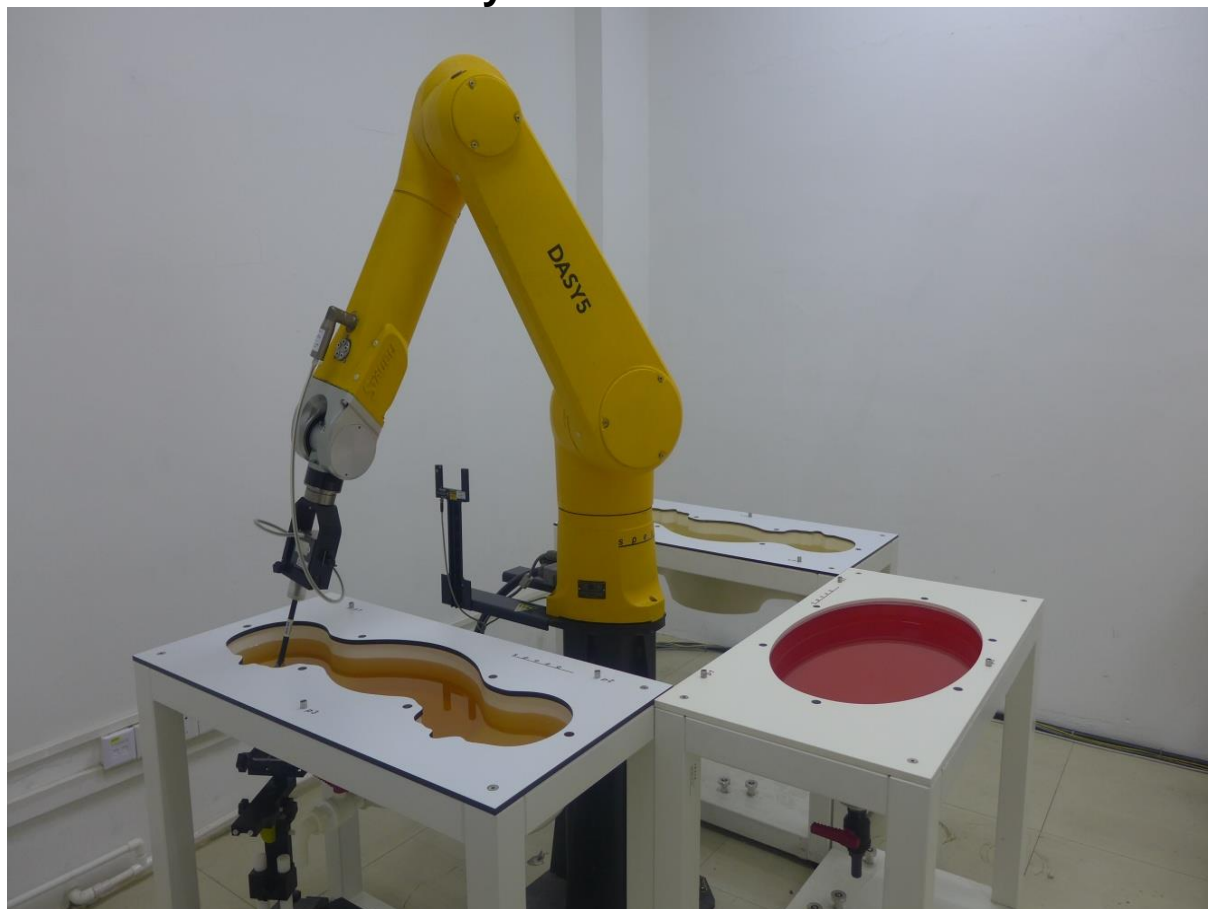


Appendix D

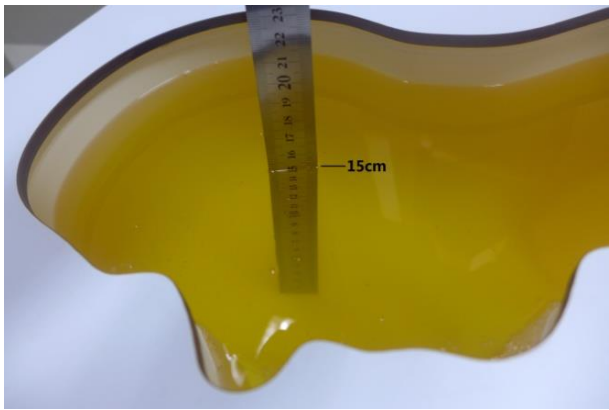
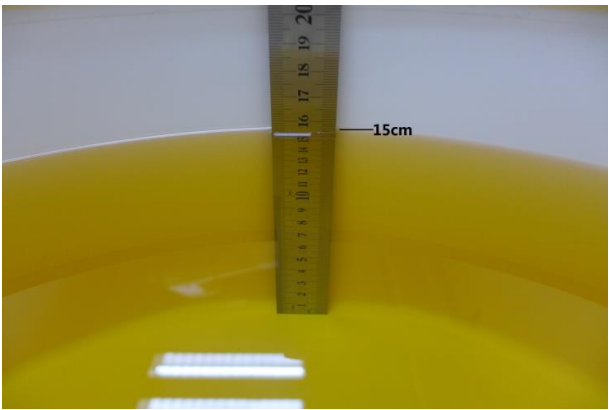
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

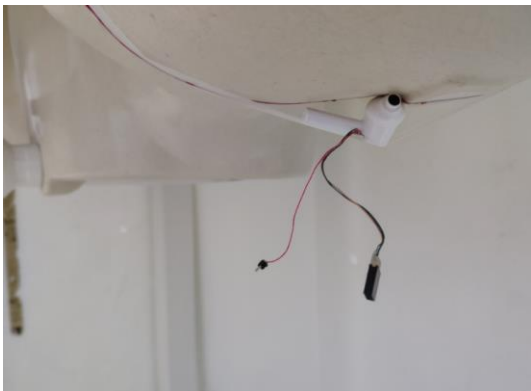
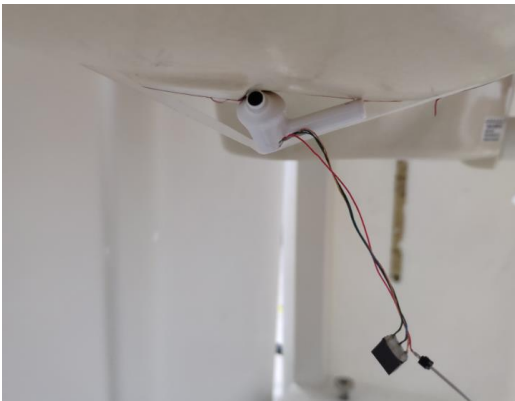
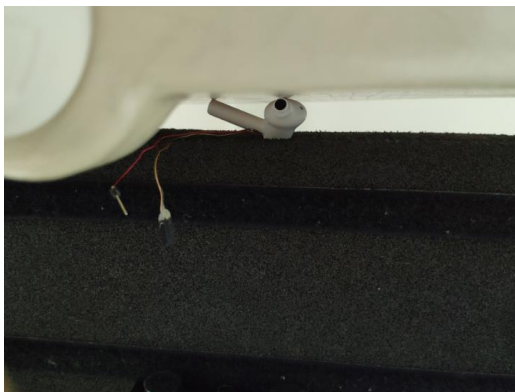

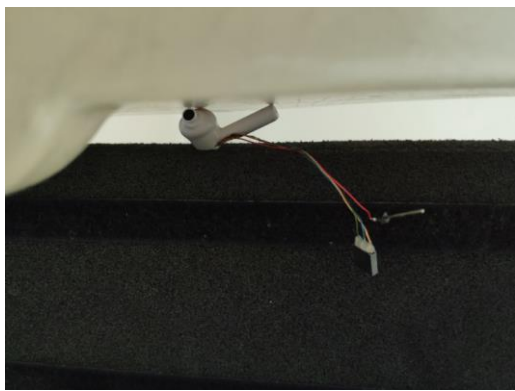
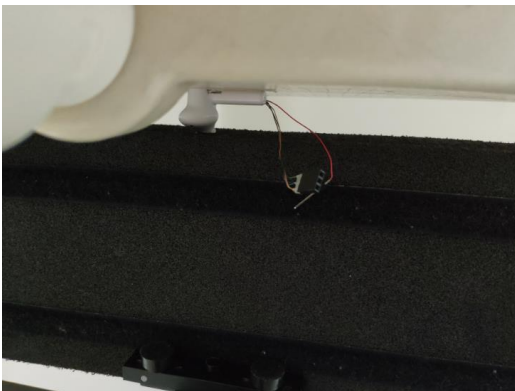
1. SAR measurement System





2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2450	Photo 2: Tissue Simulant Liquid for Head 2450
	

3. Photographs of EUT test position

<p>Photo 3: Left touch cheek</p>	<p>Photo 4: Right touch cheek</p>
	
<p>Photo 5: Side 1 0mm</p>	<p>Photo 6: Side 2 0mm</p>
	
<p>Photo 7: Side 3 0mm</p>	<p>Photo 8: Side 4 0mm</p>
	

4. EUT Constructional Details

Photo 9: Front View	Photo 10: Back View
 <p>Two white, cylindrical electronic components are shown from the front. They are positioned vertically on a blue background. A ruler is placed horizontally below them, showing a scale from 0 to 10 cm. The components have a small, circular feature on their front face. Wires are visible extending from the bottom of each component.</p>	 <p>The same two white electronic components are shown from the back. The back view reveals the internal circuitry and the connection points for the wires. A ruler is placed horizontally below them, showing a scale from 0 to 10 cm. The components are positioned vertically on a blue background.</p>