Shenzhen Huatongwei International Inspection Co., Ltd.

1/F,Bldg 3,Hongfa Hi-tech Industrial Park,Genyu Road,Tianliao,Gongming,Shenzhen,China Phone:86-755-26748019 Fax:86-755-26748089 http://www.szhtw.com.cn



TEST REPORT

Report Reference No.:: TRE18030129 R/C..... 90210

FCC ID.....: 2AE6CEP5800VHF

Applicant's name: Shenzhen Excera Technology Co., Ltd.

3rd Floor, Jiada R&D Building, No.5 Songpingshan Road, Address....:

Hi-Tech Park North, Nanshan District, Shenzhen, China

Manufacturer..... Shenzhen Excera Technology Co., Ltd.

3rd Floor, Jiada R&D Building, No.5 Songpingshan Road, Address....:

Hi-Tech Park North, Nanshan District, Shenzhen, China

Test item description....:: **Digital Portable Radio**

Trade Mark....: **EXCERA**

Model/Type reference.....: EP5800 VHF

Listed Model(s): EP5500 VHF, EP5000 VHF

FCC 47 CFR Part2.1093 Standard::

ANSI/IEEE C95.1: 1999

IEEE 1528: 2013

Date of receipt of test sample.....: Mar. 16, 2018

Date of testing..... Mar. 17, 2018 - Apr. 03, 2018

Date of issue....: Apr. 04, 2018

Result.....: **PASS**

Testing Laboratory Name:

Compiled by

(position+printed name+signature).: File administrators: Charley Wu

Supervised by

(position+printed name+signature).: Test Engineer: Charley Wu Charley.Wu Charley.Wu Homs Hy

Approved by

(position+printed name+signature).: Manager: Hans Hu

Shenzhen Huatongwei International Inspection Co., Ltd

Address....:: 1/F, Bldg 3, Hongfa Hi-tech Industrial Park, Genyu Road, Tianliao,

Gongming, Shenzhen, China

Shenzhen Huatongwei International Inspection Co., Ltd. All rights reserved.

This publication may be reproduced in whole or in part for non-commercial purposes as long as the Shenzhen Huatongwei International Inspection Co., Ltd is acknowledged as copyright owner and source of the material. Shenzhen Huatongwei International Inspection Co., Ltd takes no responsibility for and will not assume liability for damages resulting from the reader's interpretation of the reproduced material due to its placement and context.

The test report merely correspond to the test sample.

Report No: TRE18030129 Page: 2 of 33 Issued: 2018-04-04

Contents

<u>1.</u>	Test Standards and Report version	3
1.1.	Test Standards	3
1.2.	Report version	3
<u>2.</u>	Summary	4
2.1.	Client Information	4
2.2.	Product Description	4
2.3.	Test frequency list	6
<u>3.</u>	Test Environment	7
3.1. 3.2.	Test laboratory Test Facility	7 7
	•	
<u>4.</u> 5	Equipments Used during the Test	
<u>5.</u>	Measurement Uncertainty	
<u>6.</u>	SAR Measurements System Configuration	
6.1. 6.2.	SAR Measurement Set-up DASY5 E-field Probe System	11 12
6.3.	Phantoms	13
6.4.	Device Holder	13
<u>7.</u>	SAR Test Procedure	14
7.1.	Scanning Procedure	14
7.2.	Data Storage and Evaluation	16
<u>8.</u>	Position of the wireless device in relation to the phantom	18
8.1.	Front-of-face	18
8.2.	Body Position	18
<u>9.</u>	SAR System Validation	19
<u>10.</u>	System Verification	20
	Tissue Dielectric Parameters	20
10.2.	SAR System Verification	21
<u>11.</u>	SAR Exposure Limits	25
<u>12.</u>	Conducted Power Measurement Results	26
<u>13.</u>	Maximum Tune-up Limit	27
<u>14.</u>	SAR Measurement Results	28
<u>15.</u>	Simultaneous Transmission analysis	32
<u>16.</u>	Test Setup Photos	33
17.	Photos of the EUT	33

Report No: TRE18030129 Page: 3 of 33 Issued: 2018-04-04

1. Test Standards and Report version

1.1. Test Standards

The tests were performed according to following standards:

FCC 47 Part 2.1093: Radiofrequency Radiation Exposure Evaluation: Portable Devices

<u>IEEE Std C95.1, 1999:</u> IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 KHz to 300 GHz.

<u>IEEE Std 1528™-2013:</u> IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques.

KDB 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r04: SAR Measurement Requirements for 100 MHz to 6 GHz

<u>KDB 865664 D02 RF Exposure Reporting v01r02:</u> RF Exposure Compliance Reporting and Documentation Considerations

KDB 447498 D01 General RF Exposure Guidance v06: Mobile and Portable Device RF Exposure Procedures and Equipment Authorization Policies

<u>KDB 643646 D01:SAR Test for PTT Radios v01r03:</u> SAR Test Reduction Considerations for Occupational PTT Radios

1.2. Report version

Revision No.	Date of issue	Description
N/A	Apr. 04, 2018	Original

Report No: TRE18030129 Page: 4 of 33 Issued: 2018-04-04

2. Summary

2.1. Client Information

Applicant:	Shenzhen Excera Technology Co., Ltd.
Address:	3rd Floor, Jiada R&D Building, No.5 Songpingshan Road, Hi-Tech Park North, Nanshan District, Shenzhen, China
Manufacturer:	Shenzhen Excera Technology Co., Ltd.
Address:	3rd Floor, Jiada R&D Building, No.5 Songpingshan Road, Hi-Tech Park North, Nanshan District, Shenzhen, China

2.2. Product Description

Name of EUT:	Digital Portable R	Radio							
Trade mark:	EXCERA	XCERA							
Model/Type reference:	EP5800 VHF	EP5800 VHF							
Listed model(s):	EP5500 VHF, EP	25000 VHF							
Accessories	Belt Clip								
Device Category:	Portable								
RF Exposure Environment:	Occupational / Co	ontrolled							
Power supply:	7.4V from Interna	l battery							
Maximum SAR Value									
Separation Distance:	Body:	0mm							
	Face:	25mm							
Maximun SAR Value (1g):	Body:	1.93 W/Kg							
	Face:	1.69 W/Kg							
PMR									
Operation Frequency Range:	From 136MHz to	174MHz							
Rated Output Power:	⊠ High Power:	5W (37.00dBm)	□ Low Power	1W (30.00dBm)					
Modulation Type:	Analog:	FM							
	Digital:	4FSK							
Channel Separation:	Analog:		20kHz	25kHz					
	Digital:	☐ 6.25kHz							
Digital Type:	DMR								
Bluetooth-EDR									
Version:	Supported BT4.0	+EDRcompatibility							
Modulation:	GFSK, π/4DQPS	K, 8DPSK							
Operation frequency:	2402MHz~2480N	ИHz							
Channel number:	79								
Channel separation:	1MHz								
Antenna type:	Integral Antenna								

Report No: TRE18030129 Page: 5 of 33 Issued: 2018-04-04

Bluetooth-BLE	
Version:	Supported BT4.0+BLE
Modulation:	GFSK
Operation frequency:	2402MHz~2480MHz
Channel number:	40
Channel separation:	2MHz
Antenna type:	Integral Antenna

Report No: TRE18030129 Page: 6 of 33 Issued: 2018-04-04

2.3. Test frequency list

When the frequency channels required for SAR testing are not specified in the published RF exposure KDB procedures, the following should be applied to determine the number of required test channels. The test channels should be evenly spread across the transmission frequency band of each wireless mode:

$$N_{\rm c}$$
 = 2 * roundup [10* $(f_{\rm high} - f_{\rm low})/f_{\rm c}$] + 1

fc: is the centre frequency of the band in hertz; fhigh: is the highest frequency in the band in hertz; flow: is the lowest frequency in the band in hertz;

Nc: is the number of channels;

f: is the width of the transmit frequency band in hertz.

Operation	Test Frequency	
Start Frequency	number	
136	174	7

ModulationType	Channel	T (0)	Test Frequency (MHz)			
Modulation I ype	Separation	l est Channel	Channel TX CH1 136.05 CH2 142.30 CH3 148.60 CH4 154.90 CH5 161.20 CH6 167.50 CH7 173.95 CH1 136.05 CH2 142.30 CH3 148.60	RX		
		CH1	136.05	136.05		
		CH2	142.30	142.30		
		CH3	148.60	148.60		
Analog	12.5kHz	CH4	154.90	154.90		
		CH5	161.20	161.20		
		CH6	167.50	167.50		
		CH7	173.95	173.95		
		CH1	136.05	136.05		
		CH2	142.30	142.30		
		CH3	148.60	148.60		
Digital	12.5kHz	CH4	154.90	154.90		
		CH5	161.20	161.20		
		CH6	167.50	167.50		
		CH7	173.95	173.95		

Report No: TRE18030129 Page: 7 of 33 Issued: 2018-04-04

3. Test Environment

3.1. Test laboratory

Laboratory:Shenzhen Huatongwei International Inspection Co., Ltd.

Address: 1/F, Bldg 3, Hongfa Hi-tech Industrial Park, Genyu Road, Tianliao, Gongming, Shenzhen, China

3.2. Test Facility

CNAS-Lab Code: L1225

Shenzhen Huatongwei International Inspection Co., Ltd. has been assessed and proved to be in compliance with CNAS-CL01 Accreditation Criteria for Testing and Calibration Laboratories (identical to ISO/IEC17025:2005 General Requirements) for the Competence of Testing and Calibration Laboratories

A2LA-Lab Cert. No. 3902.01

Shenzhen Huatongwei International Inspection Co., Ltd. EMC Laboratory has been accredited by A2LA for technical competence in the field of electrical testing, and proved to be in compliance with ISO/IEC 17025: 2005 General Requirements for the Competence of Testing and Calibration Laboratories and any additional program requirements in the identified field of testing.

FCC-Registration No.: 762235

Shenzhen Huatongwei International Inspection Co., Ltd. EMC Laboratory has been registered and fully described in a report filed with the FCC (Federal Communications Commission). The acceptance letter from the FCC is maintained in our files.

IC-Registration No.:5377B

Two 3m Alternate Test Site of Shenzhen Huatongwei International Inspection Co., Ltd. has been registered by Certification and Engineering Bureau of Industry Canada for the performance of radiated measurements with Registration No.: 5377B

ACA

Shenzhen Huatongwei International Inspection Co., Ltd. EMC Laboratory can also perform testing for the Australian C-Tick mark as a result of our A2LA accreditation.

Report No: TRE18030129 Page: 8 of 33 Issued: 2018-04-04

4. Equipments Used during the Test

				Calibration		
Test Equipment	Manufacturer	Type/Model	Serial Number	Last Calibration	Calibration Interval	
Data Acquisition Electronics DAEx	SPEAG	DAE4	1315	2017/08/15	1	
E-field Probe	SPEAG	ES3DV3	3292	2018/01/25	1	
System Validation Antennas	SPEAG	CLA-150	4019	2016/02/11	3	
Dielectric Assessment Kit	SPEAG	DAK-3.5	1038	2016/08/25	3	
Network analyzer	Agilent	N9923A	MY51491493	2017/09/05	1	
Power meter	Agilent	N1914A	MY52090010	2018/03/22	1	
Power sensor	Agilent	E9304A	MY52140008	2018/03/22	1	
Power sensor	Agilent	E9301H	MY54470001	2017/06/02	1	
Signal Generator	ROHDE & SCHWARZ	SMB100A	175248	2017/09/02	1	
Power Amplifier	Mini-Circuits	ZHL-42W	QA1202003	2017/11/27	1	
Dual Directional Coupler	Agilent	778D	MY48220612	2018/03/22	1	

Note:

^{1.} The Probe, Dipole and DAE calibration reference to the Appendix A.

Report No: TRE18030129 Page: 9 of 33 Issued: 2018-04-04

5. Measurement Uncertainty

	Measurement Uncertainty									
No.	Error Description	Туре	Uncertainty Value	Probably Distribution	Div.	(Ci) 1g	(Ci) 10g	Std. Unc. (1g)	Std. Unc. (10g)	Degree of freedom
	ent System		0.00/					0.00/	0.00/	
11	Probe calibration Axial	В	6.0%	N	1	1	1	6.0%	6.0%	8
2	isotropy	В	4.70%	R	$\sqrt{3}$	0.7	0.7	1.90%	1.90%	80
3	Hemispherical isotropy	В	9.60%	R	$\sqrt{3}$	0.7	0.7	3.90%	3.90%	8
4	Boundary Effects	В	1.00%	R	$\sqrt{3}$	1	1	0.60%	0.60%	8
5	Probe Linearity	В	4.70%	R	$\sqrt{3}$	1	1	2.70%	2.70%	8
6	Detection limit	В	1.00%	R	$\sqrt{3}$	1	1	0.60%	0.60%	8
7	RF ambient conditions-noise	В	0.00%	R	√3	1	1	0.00%	0.00%	8
8	RF ambient conditions-reflection	В	0.00%	R	√3	1	1	0.00%	0.00%	8
9	Response time	В	0.80%	R	$\sqrt{3}$	1	1	0.50%	0.50%	8
10	Integration time	В	5.00%	R	$\sqrt{3}$	1	1	2.90%	2.90%	8
11	RF ambient	В	3.00%	R	$\sqrt{3}$	1	1	1.70%	1.70%	8
12	Probe positioned mech. restrictions	В	0.40%	R	$\sqrt{3}$	1	1	0.20%	0.20%	8
13	Probe positioning with respect to phantom shell	В	2.90%	R	√3	1	1	1.70%	1.70%	8
14	Max.SAR evalation	В	3.90%	R	$\sqrt{3}$	1	1	2.30%	2.30%	8
Test Samp	le Related					•	•		•	
15	Test sample positioning	Α	1.86%	N	1	1	1	1.86%	1.86%	8
16	Device holder uncertainty	Α	1.70%	N	1	1	1	1.70%	1.70%	8
17	Drift of output power	В	5.00%	R	$\sqrt{3}$	1	1	2.90%	2.90%	8
Phantom a									1	
18	Phantom uncertainty	В	4.00%	R	$\sqrt{3}$	1	1	2.30%	2.30%	8
19	Liquid conductivity (target)	В	5.00%	R	√3	0.64	0.43	1.80%	1.20%	8
20	Liquid conductivity (meas.)	Α	0.50%	N	1	0.64	0.43	0.32%	0.26%	8
21	Liquid permittivity (target)	В	5.00%	R	$\sqrt{3}$	0.64	0.43	1.80%	1.20%	80
22	Liquid cpermittivity (meas.)	Α	0.16%	N	1	0.64	0.43	0.10%	0.07%	8
Combined	standard uncertainty	$u_c = 1$	$\sum_{i=1}^{22} c_i^2 u_i^2$	/	/	/	/	9.79%	9.67%	∞
	ided uncertainty ce interval of 95 %)	u _e	$u_c = 2u_c$	R	K=2	/	/	19.57%	19.34%	8

Report No: TRE18030129 Page: 10 of 33 Issued: 2018-04-04

	System Check Uncertainty									
No.	Error Description	Туре	Uncertainty	Probably	Div.	(Ci)	(Ci)	Std. Unc.	Std. Unc.	Degree of
	nent System	Турс	Value	Distribution	DIV.	1g	10g	(1g)	(10g)	freedom
1	Probe calibration	В	6.0%	N	1	1	1	6.0%	6.0%	∞
2	Axial	В	4.70%	R	√3	0.7	0.7	1.90%	1.90%	∞
	isotropy	Ь	4.7070	IX.		0.7	0.7	1.50 /6	1.50 /6	
3	Hemispherical isotropy	В	9.60%	R	$\sqrt{3}$	0.7	0.7	3.90%	3.90%	∞
4	Boundary Effects	В	1.00%	R	$\sqrt{3}$	1	1	0.60%	0.60%	∞
5	Probe Linearity	В	4.70%	R	$\sqrt{3}$	1	1	2.70%	2.70%	∞
6	Detection limit	В	1.00%	R	$\sqrt{3}$	1	1	0.60%	0.60%	∞
7	RF ambient conditions-noise	В	0.00%	R	$\sqrt{3}$	1	1	0.00%	0.00%	8
8	RF ambient conditions-reflection	В	0.00%	R	√3	1	1	0.00%	0.00%	∞
9	Response time	В	0.80%	R	$\sqrt{3}$	1	1	0.50%	0.50%	∞
10	Integration time	В	5.00%	R	$\sqrt{3}$	1	1	2.90%	2.90%	∞
11	RF ambient	В	3.00%	R	√3	1	1	1.70%	1.70%	∞
12	Probe positioned mech. restrictions	В	0.40%	R	√3	1	1	0.20%	0.20%	∞
13	Probe positioning with respect to phantom shell	В	2.90%	R	√3	1	1	1.70%	1.70%	∞
14	Max.SAR evalation	В	3.90%	R	√3	1	1	2.30%	2.30%	∞
System va	lidation source-dipole		T	1				1	1	ı
15	Deviation of experimental dipole from numerical dipole	А	1.58%	N	1	1	1	1.58%	1.58%	∞
16	Dipole axis to liquid distance	Α	1.35%	N	1	1	1	1.35%	1.35%	∞
17	Input power and SAR drift	В	4.00%	R	$\sqrt{3}$	1	1	2.30%	2.30%	∞
Phantom a				T	_	1	1	T	1	T
18	Phantom uncertainty	В	4.00%	R	$\sqrt{3}$	1	1	2.30%	2.30%	∞
20	Liquid conductivity (meas.)	Α	0.50%	N	1	0.64	0.43	0.32%	0.26%	8
22	Liquid cpermittivity (meas.)	Α	0.16%	N	1	0.64	0.43	0.10%	0.07%	∞
	standard uncertainty	$u_c = 1$	$\sum_{i=1}^{22} c_i^2 u_i^2$	/	/	/	/	8.80%	8.79%	8
	nded uncertainty nce interval of 95 %)	u_{ϵ}	$u_c = 2u_c$	R	K=2	/	/	17.59%	17.58%	8

Report No: TRE18030129 Page: 11 of 33 Issued: 2018-04-04

6. SAR Measurements System Configuration

6.1. SAR Measurement Set-up

The DASY5 system for performing compliance tests consists of the following items:

A standard high precision 6-axis robot (Stäubli RX family) with controller and software. An arm extension for accommodating the data acquisition electronics (DAE).

A dosimetric probe, i.e. an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.

A data acquisition electronic (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.

A unit to operate the optical surface detector which is connected to the EOC.

The Electro-Optical Coupler (EOC) performs the conversion from the optical into a digital electric signal of the DAE. The EOC is connected to the DASY5 measurement server.

The DASY5 measurement server, which performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation. A computer operating Windows 2003.

DASY5 software and SEMCAD data evaluation software.


Remote control with teach panel and additional circuitry for robot safety such as warning lamps, etc.

The generic twin phantom enabling the testing of left-hand and right-hand usage.

The device holder for handheld Mobile Phones.

Tissue simulating liquid mixed according to the given recipes.

System validation dipoles allowing to validate the proper functioning of the system.

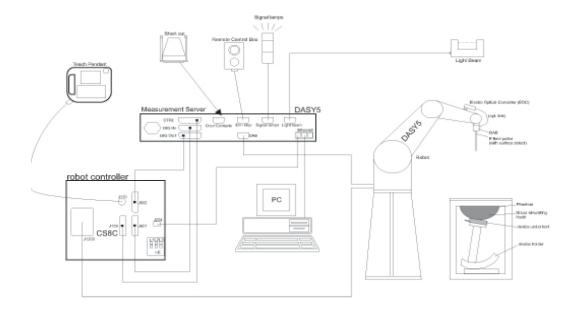

Report No: TRE18030129 Page: 12 of 33 Issued: 2018-04-04

6.2. DASY5 E-field Probe System

The SAR measurements were conducted with the dosimetric probe ES3DV3 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation.

Probe Specification

ConstructionSymmetrical design with triangular core

Interleaved sensors

Built-in shielding against static charges

PEEK enclosure material (resistant to organic solvents, e.g., DGBE)

CalibrationISO/IEC 17025 calibration service available.

Frequency 10 MHz to 4 GHz;

Linearity: ± 0.2 dB (30 MHz to 4 GHz)

Directivity $\pm 0.2 \text{ dB}$ in HSL (rotation around probe axis)

± 0.3 dB in tissue material (rotation normal to probe axis)

Dynamic Range 5 μ W/g to > 100 mW/g;

Linearity: ± 0.2 dB

Dimensions Overall length: 337 mm (Tip: 20 mm)

Tip diameter: 3.9 mm (Body: 12 mm)

Distance from probe tip to dipole centers: 2.0 mm

Application General dosimetry up to 4 GHz


Dosimetry in strong gradient fields Compliance tests of Mobile Phones

Compatibility DASY3, DASY4, DASY52 SAR and higher, EASY4/MRI

Isotropic E-Field Probe

The isotropic E-Field probe has been fully calibrated and assessed for isotropicity, and boundary effect within a controlled environment. Depending on the frequency for which the probe is calibrated the method utilized for calibration will change.

The E-Field probe utilizes a triangular sensor arrangement as detailed in the diagram below:



Report No: TRE18030129 Page: 13 of 33 Issued: 2018-04-04

6.3. Phantoms

Phantom for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30 MHz to 6 GHz. ELI isfully compatible with the IEC 62209-2 standard and all known tissuesimulating liquids. ELI has been optimized regarding its performance and can beintegrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurementgrids, by teaching three points. The phantom is compatible with all SPEAGdosimetric probes and dipoles.



ELI4 Phantom

6.4. Device Holder

The device was placed in the device holder (illustrated below) that is supplied by SPEAG as an integral part of the DASY system.

The DASY device holder is designed to cope with the different positions given in the standard. It has two scales for device rotation (with respect to the body axis) and device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (ERP). Thus the device needs no repositioning when changing the angles.



Device holder supplied by SPEAG

Report No: TRE18030129 Page: 14 of 33 Issued: 2018-04-04

7. SAR Test Procedure

7.1. Scanning Procedure

The DASY5 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.

The "reference" and "drift" measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. ± 5 %.

The "surface check" measurement tests the optical surface detection system of the DASY5 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above \pm 0.1mm). To prevent wrong results tests are only executed when the liquid is free of air bubbles. The difference between the optical surface detection and the actual surface depends on the probe and is specified with each probe (It does not depend on the surface reflectivity or the probe angle to the surface within \pm 30°.)

Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values before running a detailed measurement around the hot spot.Before starting the area scan a grid spacing of 15 mm x 15 mm is set. During the scan the distance of the probe to the phantom remains unchanged. After finishing area scan, the field maxima within a range of 2 dB will be ascertained.

Zoom Scan

After the maximum interpolated values were calculated between the points in the cube, the SAR was averaged over the spatial volume (1g or 10g) using a 3D-Spline interpolation algorithm. The 3D-spline is composed of three one-dimensional splines with the "Not a knot" condition (in x, y, and z directions). The volume was then integrated with the trapezoidal algorithm.

Spatial Peak Detection

The procedure for spatial peak SAR evaluation has been implemented and can determine values of masses of 1g and 10g, as well as for user-specific masses. The DASY5 system allows evaluations that combine measured data and robot positions, such as:

- maximum search
- extrapolation
- · boundary correction
- peak search for averaged SAR

During a maximum search, global and local maxima searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation. Extrapolation routines require at least 10 measurement points in 3-D space.

They are used in the Zoom Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation.

A Z-axis scan measures the total SAR value at the x-and y-position of the maximum SAR value found during the cube scan. The probe is moved away in z-direction from the bottom of the SAM phantom in 5mm steps.

Report No: TRE18030129 Page: 15 of 33 Issued: 2018-04-04

Table 1: Area and Zoom Scan Resolutions per FCC KDB Publication 865664 D01v04

i abie 1. Area and Zo	oom sca	n Resolutions per F	CC KDB Publication 8656	004 DU I VU4	
			≤3 GHz	> 3 GHz	
Maximum distance fro (geometric center of pr		measurement point rs) to phantom surface	$5 \text{ mm} \pm 1 \text{ mm}$	$\frac{1}{2} \cdot \hat{\delta} \cdot \ln(2) \text{ mm} \pm 0.5 \text{ mm}$	
Maximum probe angle surface normal at the r			30° ± 1°	20° ± 1°	
			\leq 2 GHz: \leq 15 mm 2 – 3 GHz: \leq 12 mm	3 – 4 GHz: ≤ 12 mm 4 – 6 GHz: ≤ 10 mm	
Maximum area scan spatial resolution: Δx_{Area} , Δy_{Area}			When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be \leq the corresponding x or y dimension of the test device with at least one measurement point on the test device.		
Maximum zoom scan	Maximum zoom scan spatial resolution: Δx _{Zoom} , Δy _{Zoom}			$3 - 4 \text{ GHz: } \le 5 \text{ mm}^*$ $4 - 6 \text{ GHz: } \le 4 \text{ mm}^*$	
	uniform	grid: Δz _{Zoom} (n)	≤ 5 mm	$3 - 4 \text{ GHz}: \le 4 \text{ mm}$ $4 - 5 \text{ GHz}: \le 3 \text{ mm}$ $5 - 6 \text{ GHz}: \le 2 \text{ mm}$	
Maximum zoom scan spatial resolution, normal to phantom surface	graded	Δz _{Zoom} (1): between 1 st two points closest to phantom surface	≤ 4 mm	$3 - 4 \text{ GHz:} \le 3 \text{ mm}$ $4 - 5 \text{ GHz:} \le 2.5 \text{ mm}$ $5 - 6 \text{ GHz:} \le 2 \text{ mm}$	
F	grid \[\Delta z_{Zoom}(n>1):\] between subsequent points		$\leq 1.5 \cdot \Delta z_{Zoom}(n-1) \text{ mm}$		
Minimum zoom scan volume	x, y, z		≥ 30 mm	$3 - 4 \text{ GHz:} \ge 28 \text{ mm}$ $4 - 5 \text{ GHz:} \ge 25 \text{ mm}$ $5 - 6 \text{ GHz:} \ge 22 \text{ mm}$	

Note: δ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see IEEE Std 1528-2013 for details.

^{*} When zoom scan is required and the <u>reported</u> SAR from the <u>area scan based 1-g SAR estimation</u> procedures of KDB Publication 447498 is ≤ 1.4 W/kg, ≤ 8 mm, ≤ 7 mm and ≤ 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.

Report No: TRE18030129 Page: 16 of 33 Issued: 2018-04-04

7.2. Data Storage and Evaluation

Data Storage

The DASY5 software stores the acquired data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension ".DA4". The software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of incorrect parameter settings. For example, if a measurement has been performed with a wrong crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be re-evaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type ([V/m], [A/m], [°C], [mW/g], [mW/cm²], [dBrel], etc.). Some of these units are not available in certain situations or show meaningless results, e.g., a SAR output in a lossless media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

Data Evaluation

The SEMCAD software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters: Sensitivity: Normi, ai0, ai1, ai2

Conversion factor: ConvFi
Diode compression point: Dcpi

Device parameters: Frequency: f

Crest factor: cf
Conductivity: σ

Media parameters: Conductivity: σ

Density: ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY5 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

Vi: compensated signal of channel (i = x, y, z)

Ui: input signal of channel (i = x, y, z)

cf: crest factor of exciting field (DASY parameter) dcpi: diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E – fieldprobes :
$$E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

H – field
probes :
$$H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}$$

Vi: compensated signal of channel (i = x, y, z) Normi: sensor sensitivity of channel (i = x, y, z),

[mV/(V/m)2] for E-field Probes

ConvF: sensitivity enhancement in solution

aij: sensor sensitivity factors for H-field probes

f: carrier frequency [GHz]

Ei: electric field strength of channel i in V/m
Hi: magnetic field strength of channel i in A/m

Report No: TRE18030129 Page: 17 of 33 Issued: 2018-04-04

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.
$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1'000}$$

local specific absorption rate in mW/g SAR:

Etot: total field strength in V/m

conductivity in [mho/m] or [Siemens/m] σ: equivalent tissue density in g/cm3 ρ:


Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid.

Report No: TRE18030129 Page: 18 of 33 Issued: 2018-04-04

8. Position of the wireless device in relation to the phantom


8.1. Front-of-face

A typical example of a front-of-face device is a two-way radio that is held at a distance from the face of the user when transmitting. In these cases the device under test shall be positioned at the distance to the phantom surface that corresponds to the intended use as specified by the manufacturer in the user instructions. If the intended use is not specified, a separation distance of 25 mm between the phantom surface and the device shall be used.

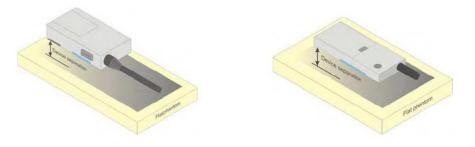

8.2. Body Position

A typical example of a body-worn device is a mobile phone, wireless enabled PDA or other battery operated wireless device with the ability to transmit while mounted on a person's body using a carry accessory approved by the wireless device manufacturer.

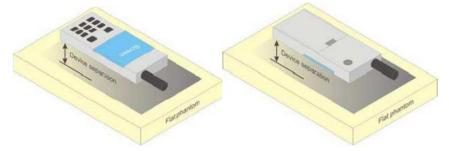

Report No: TRE18030129 Page: 19 of 33 Issued: 2018-04-04

9. SAR System Validation

Per FCC KDB 865664 D02,SAR system validadion status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the required tissue-equivalent media for system validation, according to the procedures outlined in FCC KDB 865664 D01 and IEEE 1528-2013. Since SAR probe calibrations are frequency dependent, each probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probes and tissue dielectric parameters has been included.

SAR System Validation Summary

Probe Probe type	Probe	Calibration				Dielectric P	Dielectric Parameters CW Validation			n	Modulation Validation			
	type			Conductivity	Permittivity	Sensitivity	Probe linearity	Probe Isotropy	Moduation type	Duty factor	PAR			
3842	EX3DV4	150	Head	0.76	52.3	PASS	PASS	PASS	4FSK/FM	PASS	N/A			
3842	EX3DV4	150	Body	0.80	61.9	PASS	PASS	PASS	4FSK/FM	PASS	N/A			

NOTE:

While the probes have been calibrated for both CW and modulated signals, all measurements were performed using communication systems calibrated for CW signals only. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01 for scenarios when CW probe calibrations are used with other signal types.

Report No: TRE18030129 Page: 20 of 33 Issued: 2018-04-04

10. System Verification

10.1. Tissue Dielectric Parameters

The liquid used for the frequency consisted of water, sugar, salt and Cellulose. The liquid has been previously proven to be suited for worst-case. The Table 1 show the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the KDB865664 D01.

Table 1. Composition of the Tissue Equivalent Matter

Misture 0/	Frequenc	y 450MHz	
Mixture %	Head	Body	
Water	38.36	46.22	
Sugar	55.42	49.78	
Salt	5.11	3.07	
Preventol	0.10	0.10	
Cellulose	1.07	0.47	
Dielectric Parameters Target Value	f=150MHz εr=52.3 σ=0.76	f=150MHz εr=61.9 σ=0.80	

CheckResult:

	Dielectric performance of Head tissue simulating liquid							
Frequency (MHz)	Description	DielectricPa	Temp					
	Description	εr	σ(s/m)	${\mathbb C}$				
150	Recommended result ±5% window	52.3 49.69–54.92	0.76 0.72–0.80	/				
150	Measurement value 2018-03-30	53.5	0.77	21				

	Dielectric performance of Body tissue simulating liquid							
Frequency	Description	DielectricPa	DielectricParameters					
(MHz)	` '	εr	σ(s/m)	${\mathbb C}$				
450	Recommended result ±5% window	61.9 58.81–65.00	0.80 0.76–0.84	/				
150	Measurement value 2018-03-30	60.7	0.79	21				


Report No: TRE18030129 Page: 21 of 33 Issued: 2018-04-04

10.2. SAR System Verification

The purpose of the system check is to verify that the system operates within its specifications at the decice test frequency. The system check is simple check of repeatability to make sure that the system works correctly at the time of the compliance test;

System check results have to be equal or near the values determined during dipole calibration with the relevant liquids and test system (±10 %).

System check is performed regularly on all frequency bands where tests are performed with the DASY5 system.

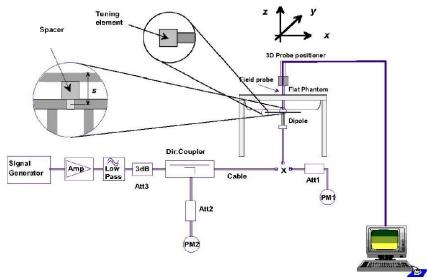

The output power on dipole port must be calibrated to 30 dBm (1000mW) before dipole is connected.



Photo of Dipole Setup

Report No: TRE18030129 Page: 22 of 33 Issued: 2018-04-04

Check Result:

	System Validation Result for Head							
Frequency (MHz)	Description	SAR(Temp					
	Description	1g	10g	$^{\circ}\!\mathbb{C}$				
	Recommended result ±5% window	3.79 3.60 – 3.98	2.52 2.39–2.65	/				
150	Measurement value 2018-03-30	3.85	2.56	21				

	System Validation Result for Body							
Frequency Description	Description	SAR(Temp					
	Description	1g	10g	$^{\circ}\!\mathbb{C}$				
	Recommended result ±5% window	3.89 3.70 – 4.08	2.59 2.46–2.72	/				
150	Measurement value 2018-03-30	3.96	2.68	21				

Note:

- 1. the graph results see follow.
- 2. Recommended Values used derive from the calibration certificate and 398mW is used asfeeding power to the calibrated dipole.

Report No: TRE18030129 Page: 23 of 33 Issued: 2018-04-04

System Performance Check at 150 MHz Head

DUT: Dipole150 MHz; Type: CLA150; Serial: 4019

Date: 2018-03-30

Communication System: DuiJiangJi; Frequency: 150 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 150 MHz; $\sigma = 0.77 \text{ S/m}$; $\varepsilon_r = 53.5$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY5 Configuration:

•Probe: ES3DV3 - SN3292;ConvF(7.85, 7.85, 7.85); Calibrated: 25/01/2018;

•Sensor-Surface: 4mm (Mechanical Surface Detection)

•Electronics: DAE4 Sn1315; Calibrated: 15/08/2017

•Phantom: ELI v4.0; Type: QDOVA001BB

•Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

System Performance Check at 150MHz/Area Scan (61x201x1):Interpolated grid: dx=1.500 mm, dy=1.50 mm

Maximum value of SAR (interpolated) = 4.19 W/Kg


System Performance Check at 150MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm,

dv=5mm, dz=5mm

Reference Value = 25.0 V/m; Power Drift = -0.11 dB

Peak SAR (extrapolated) = 6.22 W/kg

SAR(1 g) = 3.85 mW/g; SAR(10 g) = 2.56 mW/g Maximum value of SAR (measured) = 4.17 mW/g

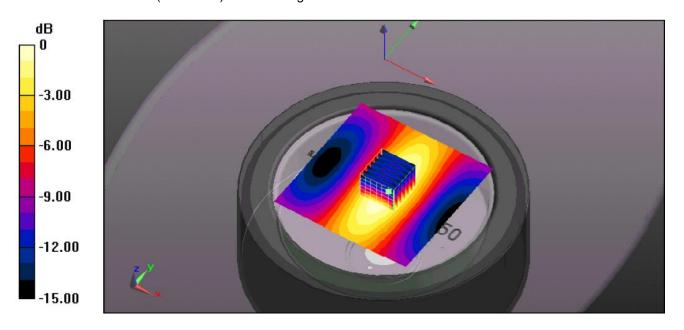

System Performance Check 150MHz Head 1 W

Report No: TRE18030129 Page: 24 of 33 Issued: 2018-04-04

System Performance Check at 150 MHz Body

DUT: Dipole150 MHz; Type: CLA150; Serial: 4019

Date: 2018-03-30

Communication System: DuiJiangJi; Frequency: 150 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 150 MHz; $\sigma = 0.79 \text{S/m}$; $\epsilon_r = 60.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

DASY5 Configuration:

•Probe: ES3DV3 - SN3292;ConvF(7.59, 7.59, 7.59); Calibrated: 25/01/2018;

•Sensor-Surface: 4mm (Mechanical Surface Detection)

•Electronics: DAE4 Sn1315; Calibrated: 15/08/2017

•Phantom: ELI v4.0; Type: QDOVA001BB

•Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

System Performance Check at 150MHz/Area Scan (61x201x1):Interpolated grid: dx=1.500 mm, dy=1.50 mm

Maximum value of SAR (interpolated) = 4.28 W/Kg


System Performance Check at 150MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm,

dv=5mm, dz=5mm

Reference Value = 25.33 V/m; Power Drift = -0.11 dB

Peak SAR (extrapolated) = 6.36 W/kg

SAR(1 g) = 3.96 mW/g; SAR(10 g) = 2.68 mW/g Maximum value of SAR (measured) = 4.42 mW/g

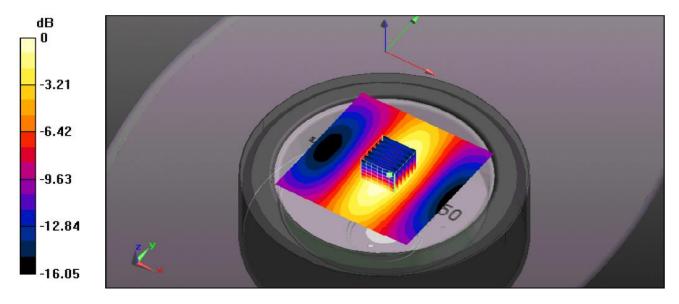

System Performance Check 150MHz Body 1 W

Report No: TRE18030129 Page: 25 of 33 Issued: 2018-04-04

11. SAR Exposure Limits

	Limit (W/kg)				
Type Exposure	General Population / Uncontrolled Exposure Environment	Occupational / Controlled Exposure Environment			
Spatial Average SAR (whole body)	0.08	0.4			
Spatial Peak SAR (1g cube tissue for head and trunk)	1.60	8.0			
Spatial Peak SAR (10g for limb)	4.0	20.0			

Population/Uncontrolled Environments: are defined as locations where there is the exposure of individual who have no knowledge or control of their exposure.

Occupational/Controlled Environments: are defined as locations where there is exposure that may be incurred by people who are aware of the potential for exposure (i.e. as a result of employment or occupation).

Report No: TRE18030129 Page: 26 of 33 Issued: 2018-04-04

12. Conducted Power Measurement Results

	PMR							
Mode	Channel	Fred	quency	Conducted Power				
Mode	Separation	Channel	MHz	(dBm)				
		CH1	136.05	36.90				
		CH2	142.30	36.92				
		CH3	148.60	36.79				
Analog	12.5KHz	CH4	154.90	36.80				
		CH5	161.20	36.83				
		CH6	167.50	36.73				
		CH7	173.95	36.80				
		CH1	136.05	37.00				
		CH2	142.30	37.00				
		CH3	148.60	36.89				
Digtal	12.5KHz	CH4	154.90	36.90				
		CH5	161.20	36.93				
		CH6	167.50	36.83				
		CH7	173.95	36.90				

Bluetooth						
Mode	Channel	Frequency (MHz)	Conducted power (dBm)			
	00	2402	7.58			
GFSK	39	2441	8.12			
	78	2480	7.78			
	00	2402	7.63			
π/4QPSK	39	2441	6.92			
	78	2480	6.52			
	00	2402	6.05			
8DPSK	39	2441	6.34			
	78	2480	6.52			
	0	2402	7.27			
BLE	19	2440	7.98			
	39	2480	7.65			

Report No: TRE18030129 Page: 27 of 33 Issued: 2018-04-04

13. Maximum Tune-up Limit

This device operates using the following maximum output power specifications. SAR values were scaled to the maximum allowed power to determine compliance per KDB publication 447498 D01

PMR							
Mode	Channel Separation (KHz)	Operation Frequency Range (MHz)	Maximum tune up power (dBm)				
Analog	12.5	136~174	37.00				
Digtial	12.5	136~174	37.00				

		Bluetooth	
Mode	Mode Channel Frequency (Maximum Conducted power (dBm)
	0	2402	
GFSK	39	2441	8.50
	78	2480	
	0	2402	
π/4QPSK	39	2441	8.00
	78	2480	
	0	2402	
8DPSK	39	2441	7.00
	78	2480	
	0	2402	
BLE(GFSK)	E(GFSK) 19		8.00
	39	2480	

Per KDB 447498 D01, the 1-g and 10-g SAR test exclusion thresholds for 100MHz to 6GHz at test separation distances ≤50mm are determined by:

[(max. Power of channel, including tune-up tolerance, mW) / (min. test separation distance, mm)] * [$\sqrt{f(GHz)}$] ≤ 15.0 for 1-g SAR

Per KDB 447498 D01, when the minimum test separation distance is <5mm, a distance of 5mm is applied to determine SAR test exclusion.

Bluetooth Tune up power		SAR Exclusion Thre	shold Power (mW)	SAR Exclusion		
dBm	mW	Front of Face	Body Worn	Front of Face	e Body Worn	
8.50	7.08	239.58	47.92	Yes	Yes	

Report No: TRE18030129 Page: 28 of 33 Issued: 2018-04-04

14. SAR Measurement Results

					Front of	Face					
Mode Channel Separation	, ,	Conducted Power	Tune up limit	Tune up scaling	Power	Measured SAR(1g)	Report SAR(1g)	50% Duty SAR	Test Plot		
	СН	MHz	(dBm)	(dBm) IImit (dBm)	factor	Drift(dB)	(W/kg)	(W/kg)	(W/kg)	FIOL	
		CH1	136.05	36.90	37.00	1.02	-	-	-	1	-
		CH2	142.30	36.92	37.00	1.02	0.12	3.32	3.38	1.69	AF
		СНЗ	148.60	36.79	37.00	1.05	-	1	ı	ı	•
Analog	12.5KHz	CH4	154.90	36.80	37.00	1.05	-0.05	3.14	3.29	1.65	-
		CH5	161.20	36.83	37.00	1.04	-	1	ı	ı	-
		CH6	167.50	36.73	37.00	1.07	0.17	3.12	3.32	1.66	-
		CH7	173.95	36.80	37.00	1.05	-	-	1	ı	-
		CH1	136.05	37.00	37.00	1.00	-	-	-	-	-
		CH2	142.30	37.00	37.00	1.00	0.05	2.78	2.78	1.39	-
		СНЗ	148.60	36.89	37.00	1.03	-	-	-		-
Digtal	12.5KHz	CH4	154.90	36.90	37.00	1.02	0.11	2.65	2.71	1.36	•
		CH5	161.20	36.93	37.00	1.02	-	1		ı	•
		CH6	167.50	36.83	37.00	1.04	0.13	2.64	2.75	1.37	
		CH7	173.95	36.90	37.00	1.02	-	-	-	-	-

Note:

- 1. The value with blue color is the maximum SAR Value of each test band.
- 2. Batteries are fully charged at the beginning of the SAR measurements
- 3. The EUT was tested for face-held SAR with a 2.5cm separation distance between the front of the EUT and the outer surface of the planer phantom
- 4. When the SAR for all antennas tested using the default battery is ≤ 3.5 W/kg (50% PTT duty factor), testing of all other required channels is not necessary.
- 5. When the SAR of an antenna tested on the highest output power using the default battery is > 3.5 W/Kg and ≤ 4.0 W/Kg (50% PTT duty factor), testing of the immediately adjacent channel(s) is not necessary, but testing of other required channels may still be required.
- 6. When the SAR for all antennas tested using the default battery ≤ 4.0 W/kg(50% PTT duty factor), test additional batteries using the antenna and channel configuration that resulted in the highest SAR.

Report No: TRE18030129 Page: 29 of 33 Issued: 2018-04-04

	Body Worn (Rear Side)										
Mode	Channel Separation	Frequency		Conducted Power	Tune up limit	Tune up scaling	Power Drift(dB)	Measured SAR(1g)	Report SAR(1g)	50% Duty SAR	Test Plot
		СН	MHz	(dBm)	(dBm)	factor	Dilit(GB)	(W/kg)	(W/kg)	(W/kg)	1 100
		CH1	136.05	36.90	37.00	1.02	-	-	-	-	-
		CH2	142.30	36.92	37.00	1.02	0.08	3.78	3.85	1.93	AF
		СНЗ	148.60	36.79	37.00	1.05	-	-	-	-	-
Analog	12.5KHz	CH4	154.90	36.80	37.00	1.05	0.12	3.46	3.62	1.81	
		CH5	161.20	36.83	37.00	1.04	-	-	-	-	-
		CH6	167.50	36.73	37.00	1.07	-0.07	3.46	3.68	1.84	-
		CH7	173.95	36.80	37.00	1.05	-	-	-	-	-
		CH1	136.05	37.00	37.00	1.00	-	-	-	-	-
		CH2	142.30	37.00	37.00	1.00	0.05	3.02	3.02	1.51	-
	12.5KHz	СНЗ	148.60	36.89	37.00	1.03	-	-	1	ı	-
Digtal		CH4	154.90	36.90	37.00	1.02	-0.14	3.12	3.19	1.59	-
		CH5	161.20	36.93	37.00	1.02	-	-	ı	ı	-
		CH6	167.50	36.83	37.00	1.04	-0.11	2.98	3.10	1.55	-
		CH7	173.95	36.90	37.00	1.02	-	-	-	-	-

Note:

- 1. The value with blue color is the maximum SAR Value of each test band.
- 2. Batteries are fully charged at the beginning of the SAR measurements
- 3. The Body-worn SAR evaluation was performed with the Leather Case body-worn accessory attached to the DUT and touching the outer surface of the planar phantom
- 4. When the SAR for all antennas tested using the default battery is ≤ 3.5 W/kg (50% PTT duty factor), testing of all other required channels is not necessary.
- 5. When the SAR of an antenna tested on the highest output power using the default battery is > 3.5 W/Kg and ≤ 4.0 W/Kg (50% PTT duty factor), testing of the immediately adjacent channel(s) is not necessary, but testing of other required channels may still be required.
- 6. When the SAR for all antennas tested using the default battery ≤ 4.0 W/kg(50% PTT duty factor), test additional batteries using the antenna and channel configuration that resulted in the highest SAR.

SAR Test Data Plots

Report No: TRE18030129 Page: 30 of 33 Issued: 2018-04-04

Test Plot: AF Front of Face **Test Position:**

Date:2018-03-30

Communication System: Customer System; Frequency: 142.30MHz;

Medium parameters used (interpolated): f = 142.30 MHz; $\sigma = 0.77 \text{ S/m}$; $\epsilon r = 53.43$; $\rho = 1000 \text{ kg/m}$ 3

Phantom section: Flat Section

DASY5 Configuration:

•Probe: ES3DV3 - SN3292;ConvF(7.85, 7.85, 7.85); Calibrated: 25/01/2018;

•Sensor-Surface: 4mm (Mechanical Surface Detection)

•Electronics: DAE4 Sn1315; Calibrated: 15/08/2017

•Phantom: ELI v4.0; Type: QDOVA001BB

•Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

Area Scan(51x201x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm


Maximum value of SAR (interpolated) = 4.06 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7mm, dy=7mm, dz=5mm

Reference Value = 32.936 V/m; Power Drift = 0.12 dB

Peak SAR (extrapolated) = 4.480 mW/g

SAR(1 g) = 3.32 mW/g; SAR(10 g) = 1.84 mW/gMaximum value of SAR (measured) = 4.17 W/kg

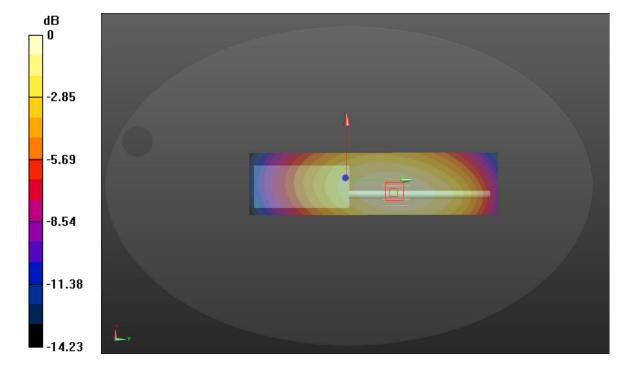

Report No: TRE18030129 Page: 31 of 33 Issued: 2018-04-04

Test Plot: AB Test Position: Body-worn

Date:2018-03-30

Communication System: Customer System; Frequency: 142.30 MHz;

Medium parameters used (interpolated): f = 142.30 MHz; $\sigma = 0.79 \text{ S/m}$; $\epsilon r = 60.08$; $\rho = 1000 \text{ kg/m}$ 3

Phantom section: Flat Section

DASY5 Configuration:

•Probe: ES3DV3 - SN3292;ConvF(7.59, 7.59, 7.59); Calibrated: 25/01/2018;

•Sensor-Surface: 4mm (Mechanical Surface Detection)

•Electronics: DAE4 Sn1315; Calibrated: 15/08/2017


•Phantom: ELI v4.0; Type: QDOVA001BB

•Measurement SW: DASY52, Version 52.8 (2); SEMCAD X Version 14.6.6 (6824)

Area Scan(51x201x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm Maximum value of SAR (interpolated) = 4.23 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7mm, dy=7mm, dz=5mm Reference Value = 43.391 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 4.457 mW/g SAR(1 g) = 3.78 mW/g; SAR(10 g) = 2.44 mW/g Maximum value of SAR (measured) = 4.02 W/kg

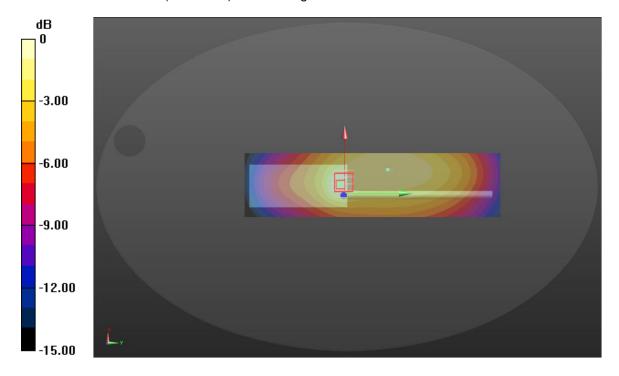

Report No: TRE18030129 Page: 32 of 33 Issued: 2018-04-04

15. Simultaneous Transmission analysis

No	Simultaneous Transmission Configurations	Front to face	Body-worn	Note
1	PMR + Bluetooth	Yes	Yes	

General note:

- For simultaneous transmission analysis, Bluetooth SAR is estimated per KDB 447498 D01 based on the formula below
 - a) [(max. Power of channel, including tune-up tolerance, mW) / (min. test separation distance, mm)] * $[\sqrt{f(GHz)/x}]W/kg$ for test separation distances ≤ 50 mm; whetn x=7.5 for 1-g SAR, and x=18.75 for 10-g SAR.
 - b) When the minimum separation distance is <5mm, the distance is used 5mm to determine SAR test exclusion
 - c) 0.4 W/kg for 1-g SAR and 1.0W/kg for 10-g SAR, when the test separation distances is >50mm.

Bluetooth Maximum Power	Estimated SAR (W/kg)		
(dBm)	Front of Face (25mm)	Body Worn (0mm)	
8.50	0.059	0.295	

Maximum reported SAR value

Evacura Position	PMR mode	Max SAI	Summed SAR	
Exposure Position	PIVIK IIIOGE	PMR	Bleutooth	(W/kg)
Front of Face	Analog	1.690	0.059	1.749
FIGHT OF FACE	Digtal	1.390	0.059	1.449
Pady Warn	Analog	1.930	0.295	2.225
Body Worn	Digtal	1.590	0.295	1.885

Report No: TRE18030129 Page: 33 of 33 Issued: 2018-04-04


16. Test Setup Photos



Liquid depth in the flat Phantom (150 MHz) (15.3cm deep)



Body Worn (0mm)

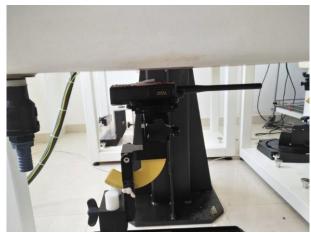

Front of face (25mm)

17. Photos of the EUT

Please referce to the test report No.: TRE1803012801.

-----End of Report-----

1.1. Probe Calibration Certificate

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

CIQ-SZ (Auden)

Certificate No: ES3-3292_Jan18

CALIBRATION CERTIFICATE

Object

ES3DV3 - SN:3292

Calibration procedure(s)

QA CAL-01.v9, QA CAL-12.v9, QA CAL-23.v5, QA CAL-25.v6

Calibration procedure for dosimetric E-field probes

Calibration date:

January 25, 2018

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02525)	Apr-18
Reference 20 dB Attenuator	SN: S5277 (20x)	07-Apr-17 (No. 217-02528)	Apr-18
Reference Probe ES3DV2	SN: 3013	30-Dec-17 (No. ES3-3013_Dec17)	Dec-18
DAE4	SN: 660	21-Dec-17 (No. DAE4-660_Dec17)	Dec-18
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-16)	In house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	of 2 1/2
Approved by:	Katja Pokovic	Technical Manager	All y
			Issued: January 25, 2018
This calibration certificate	e shall not be reproduced except in ful	Il without written approval of the laborator	y.

Certificate No: ES3-3292_Jan18

Page 1 of 11

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal A, B, C, D modulation dependent linearization parameters

Polarization φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, ", "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from handheld and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no
 uncertainty required).

Certificate No: ES3-3292_Jan18 Page 2 of 11

ES3DV3 - SN:3292

January 25, 2018

Probe ES3DV3

SN:3292

Manufactured: Calibrated:

July 6, 2010 January 25, 2018

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: ES3-3292_Jan18

Page 3 of 11

January 25, 2018

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3292

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) ²) ^A	0.95	0.96	0.93	± 10.1 %
DCP (mV) ⁸	104.2	107.6	112.3	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	191.5	±3.3 %
		Y	0.0	0.0	1.0		187.6	
		Z	0.0	0.0	1.0		190.2	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

 ^h The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).
 ^B Numerical linearization parameter: uncertainty not required.
 ^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3-SN:3292 January 25, 2018

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3292

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k=2)
150	52.3	0.76	7.85	7.85	7.85	0.04	1,20	± 13.3 %
450	43.5	0.87	7.12	7.12	7.12	0.18	1.20	± 13.3 %

^C Frequency validity above 300 MHz of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to \pm 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is \pm 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to \pm 110 MHz.

Fat frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to \pm 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than \pm 1% for frequencies below 3 GHz and below \pm 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: ES3-3292_Jan18 Page 5 of 11

diameter from the boundary.

January 25, 2018

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3292

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k=2)
150	61.9	0.80	7.59	7.59	7.59	0.04	1.20	± 13.3 %
450	56.7	0.94	7.28	7.28	7.28	0.12	1.20	± 13.3 %

 $^{^{\}text{C}}$ Frequency validity above 300 MHz of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to \pm 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is \pm 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to \pm 110 MHz.


Fat frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to \pm 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than \pm 1% for frequencies below 3 GHz and below \pm 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

diameter from the boundary.

January 25, 2018

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

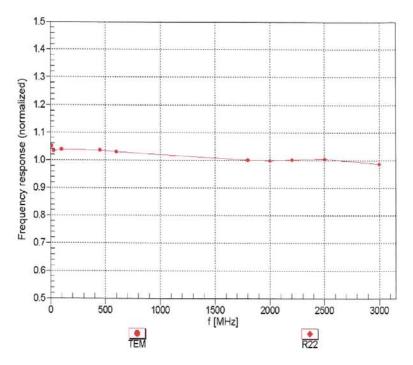



Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Receiving Pattern (φ), 9 = 0°

January 25, 2018

ποσοινική τ αποτιτ (ψ), σ

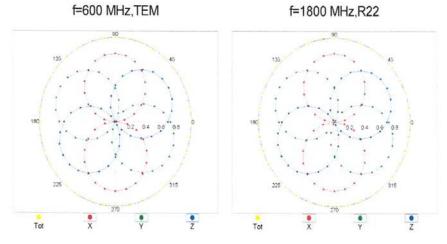


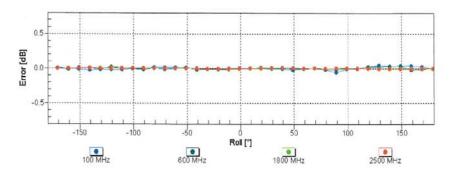


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

January 25, 2018

Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

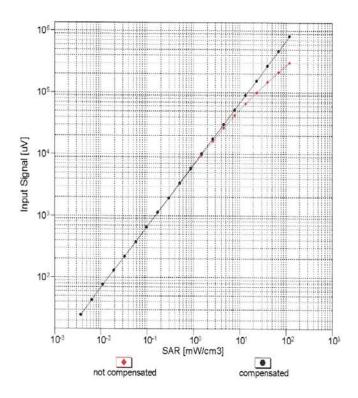

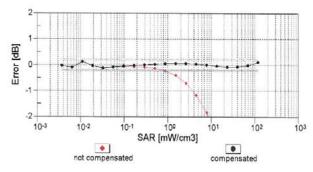


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: ES3-3292_Jan18


Page 9 of 11

ES3DV3- SN:3292 January 25, 2018

Conversion Factor Assessment

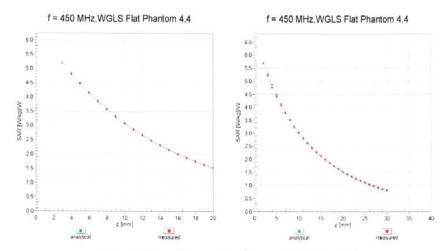

Deviation from Isotropy in Liquid

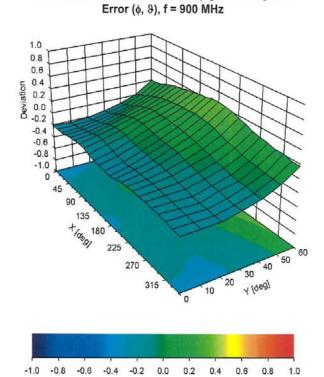

Certificate No: ES3-3292_Jan18 Page 10 of 11

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

10 of 23

January 25, 2018

ES3DV3- SN:3292

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3292

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	39.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

1.2. 150 Dipole Calibration Certificate

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Issued: February 15, 2016

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signitories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

CALIBRATION	CERTIFICATE		
Object	CLA150 - SN: 40	119	
Calibration procedure(s)	QA CAL-15.v8 Calibration proce	dure for system validation source	es below 700 MHz
Calibration date:	February 11,201	6	
This calibration certificate docum The measurements and the unce	ents the traceability to nat ertainties with confidence p	ional standards, which realize the physical un robability are given on the following pages an	its of measurements (SI), d are part of the certificate.
Il galibrationa bassa t			
Calibration Equipment used (M&	TE critical for calibration)	ry facility: environment temperature (22±3)°0	and humidity < 70%.
alibration Equipment used (M& rimary Standards	TE critical for calibraton)	Cal Date (Cerificate No.)	C and humidity < 70%. Schedulad Calibration
alibration Equipment used (M& imary Standards ower meter E4419B	TE critical for calibraton) ID # GB41293874	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128)	
hibration Equipment used (M& mary Standards wer meter E4419B wer sensor E4412A	ID # GB41293874 MY41498087	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128)	Schedulad Calibration
hibration Equipment used (M& many Standards wer meter E4419B wer sensor E4412A ference 3 dB Attenuator	ID # GB41293874 MY41498087 SN: S5054 (3c)	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128)	Schedulad Calibration Mar-16
dibration Equipment used (M& imary Standards wer meter E4419B wer sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator	ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20k)	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128)	Schedulad Calibration Mar-16 Mar-16
tlibration Equipment used (M& imary Standards ower meter E4419B ower sensor E4412A oference 3 dB Attenuator oference 20 dB Attenuator pe-N mismatch combination	ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20k) SN: 5047.2 / 06327	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129)	Schedulad Calibration Mar-16 Mar-16 Mar-16
alibration Equipment used (M& imary Standards ower meter E4419B ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator ope-N mismatch combination eference Probe EX3DV4	ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20k) SN: 5047.2 / 06327 SN: 3877	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131)	Schedulad Calibration Mar-16 Mar-16 Mar-16
alibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator ype-N mismatch combination eference Probe EX3DV4	ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20k) SN: 5047.2 / 06327	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02134)	Schedulad Calibration Mar-16 Mar-16 Mar-16 Mar-16 Mar-16
alibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator ype-N mismatch combination eference Probe EX3DV4 AE4	ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20k) SN: 5047.2 / 06327 SN: 3877	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02134) 31-Dec-15 (Nc. EX3-3877_Dec15) 08-Jul-15 (No. DAE4-654_Jul15)	Schedulad Calibration Mar-16 Mar-16 Mar-16 Mar-16 Mar-16 Dec-16 Jul-16
rimary Standards ower meter E4419B ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator eference Probe EX3DV4 AE4 econdary Standards	ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20k) SN: 5047.2 / 06327 SN: 3877 SN: 654 ID #	Cal Date (Cerifficate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02134) 31-Dec-15 (No. EX3-3877_Dec15) 08-Jul-15 (No. DAE4-654_Jul15) Check Date (in house)	Schedulad Calibration Mar-16 Mar-16 Mar-16 Mar-16 Mar-16 Jul-16 Schedulad Check
alibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator ype-N mismatch combination eference Probe EX3DV4 AE4	TE critical for calibraton) ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20k) SN: S5058 (20k) SN: 6047.2 / 06327 SN: 3877 SN: 654 ID # US3642U01700	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02131) 31-Dec-15 (No. EX3-3877_Dec15) 08-Jul-15 (No. DAE4-654_Jul15) Check Date (in house) 04-Aug-99 (in house check Apr-13)	Schedulad Calibration Mar-16 Mar-16 Mar-16 Mar-16 Mar-16 Jul-16 Schedulad Check In house check: Apr-16
alibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator ype-N mismatch combination elerence Probe EX3DV4 AE4 econdary Standards F generator HP 8648C	ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20k) SN: 5047.2 / 06327 SN: 3877 SN: 654 ID #	Cal Date (Cerifficate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02134) 31-Dec-15 (No. EX3-3877_Dec15) 08-Jul-15 (No. DAE4-654_Jul15) Check Date (in house)	Schedulad Calibration Mar-16 Mar-16 Mar-16 Mar-16 Mar-16 Jul-16 Schedulad Check
rimary Standards fower meter E4419B fower sensor E4412A feference 3 dB Attenuator feference 20 dB Attenuator feference Probe EX3DV4 fAE4 fecondary Standards fegererator HP 8648C	TE critical for calibraton) ID # GB41293874 MY41498087 SN: S5054 (3c) SN: S5058 (20k) SN: S5058 (20k) SN: 6047.2 / 06327 SN: 3877 SN: 654 ID # US3642U01700	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02131) 31-Dec-15 (No. EX3-3877_Dec15) 08-Jul-15 (No. DAE4-654_Jul15) Check Date (in house) 04-Aug-99 (in house check Apr-13)	Schedulad Calibration Mar-16 Mar-16 Mar-16 Mar-16 Dec-16 Jul-16 Schedulad Check In house check: Apr-16 In house check: Oct-16
calibration Equipment used (M& trimary Standards Power meter E4419B Power sensor E4412A teference 3 dB Attenuator teference 20 dB Attenuator type-N mismatch combination teference Probe EX3DV4 PAE4 secondary Standards IF generator HP 8648C letwork Analyzer HP 8753E	TE critical for calibraton) ID # GB41293874 MY41498087 SN: S\$054 (3c) SN: S\$054 (3c) SN: \$5058 (20k) SN: \$6047.2 / 06327 SN: 3877 SN: 654 ID # US3642U01700 US37390585	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02131) 31-Dec-15 (No. EX3-3877_Dec15) 08-Jul-15 (No. DAE4-654_Jul15) Check Date (in house) 04-Aug-99 (in house check Apr-13) 18-Oct-01 (in nouse check Oct-15)	Schedulad Calibration Mar-16 Mar-16 Mar-16 Mar-16 Mar-16 Jul-16 Schedulad Check In house check: Apr-16
	ID # GB41293874 MY41498087 SN: \$5054 (3c) SN: \$5054 (20k) SN: \$647.2 / 06327 SN: 654 ID # US3642U01700 US37390585 Name	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. EX3-3877_Dec15) 08-Jul-15 (No. DAE4-654_Jul15) Check Date (in house) 04-Aug-99 (in house check Apr-13) 18-Oct-01 (in house check Oct-15)	Schedulad Calibration Mar-16 Mar-16 Mar-16 Mar-16 Dec-16 Jul-16 Schedulad Check In house check: Apr-16 In house check: Oct-16
calibration Equipment used (M& trimary Standards Power meter E4419B Power sensor E4412A teference 3 dB Attenuator teference 20 dB Attenuator type-N mismatch combination teference Probe EX3DV4 PAE4 secondary Standards IF generator HP 8648C letwork Analyzer HP 8753E	ID # GB41293874 MY41498087 SN: \$5054 (3c) SN: \$5054 (20k) SN: \$647.2 / 06327 SN: 654 ID # US3642U01700 US37390585 Name	Cal Date (Cerificate No.) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02128) 01-Apr-15 (Nc. 217-02129) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. 217-02131) 01-Apr-15 (Nc. EX3-3877_Dec15) 08-Jul-15 (No. DAE4-654_Jul15) Check Date (in house) 04-Aug-99 (in house check Apr-13) 18-Oct-01 (in house check Oct-15)	Schedulad Calibration Mar-16 Mar-16 Mar-16 Mar-16 Dec-16 Jul-16 Schedulad Check In house check: Apr-16 In house check: Oct-16

Certificate No: CLA150-4019_Feb16

Page 1 of 8

Calibration Laboratory of

Schmid & Partner Engineering AG





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 0108

Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossarv:

TSL

tissue simulating liquid

ConvF N/A

sensitivity in TSL / NORM x.v.z not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The source is mcunted in a touch configuration below the center marking of the flat phantom.
- Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: CLA150-4019_Feb16

Page 2 of 8

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY5	V52.8.8
Advanced Extrapolation	
ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Touch Position	
dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
150 MHz ± 1 MHz	
	Advanced Extrapolation ELI4 Flat Phantom Touch Position dx, dy = 4.0 mm, dz = 1.4 mm

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	52.3	0.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	50.4 ± 6 %	0.78 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.90 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.79 W/kg ± 18.4 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	s guida
SAR measured	1 W input power	2.59 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	2.52 W/kg ± 18.0 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	61.9	0.80 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	60.4 ± 6 %	0.84 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	1 W input power	4.06 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	3.89 W/kg ± 18.4 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	1 W input power	2.70 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (k=2)

Certificate No: CLA150-4019_Feb16

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	47.4 Ω - 5.3 jΩ	
Return Loss	· 24.4 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.9 Ω - 8.0 jΩ		
Return Loss	- 22.0 dB		

Additional EUT Data

Manufactured by	SPEAG		
Manufactured on	November 25, 2015		

Certificate No: CLA150-4019_Feb16

DASY5 Validation Report for Head TSL

Date: 11.02.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4019

Communication System: UID 0 - CW; Frequency: 150 MHz

Medium parameters used: f = 150 MHz; $\sigma = 0.78 \text{ S/m}$; $\varepsilon_r = 50.4$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

Probe: EX3DV4 - SN3877; ConvF(12.02, 12.02, 12.02); Calibrated: 31.12.2015;

• Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn654; Calibrated: 08.07.2015

Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003

DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan

(81x81x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm Maximum value of SAR (interpolated) = 5.13 W/kg

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan,


dist=1.4mm (8x9x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 83.28 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 7.21 W/kg

SAR(1 g) = 3.9 W/kg; SAR(10 g) = 2.59 W/kg

Maximum value of SAR (measured) = 5.45 W/kg

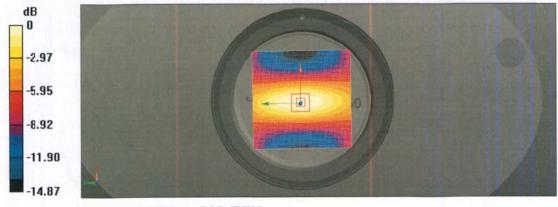


0 dB = 5.46 W/kg = 7.37 dBW/kg

Certificate No: CLA150-4019_Feb16

Page 5 of 8

Impedance Measurement Plot for Head TSL

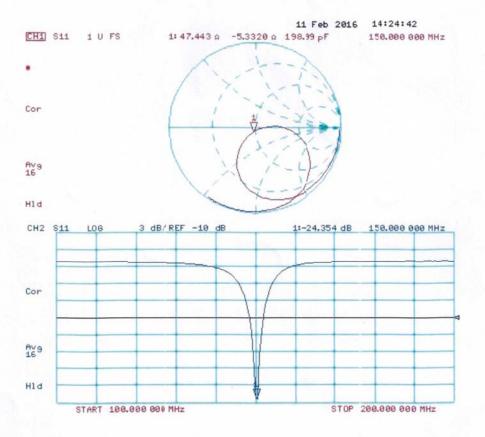

DASY5 Validation Report for Body TSL

Date: 11.02.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4019

Communication System: UID 0 - CW; Frequency: 150 MHz

Medium parameters used: f = 150 MHz; $\sigma = 0.84 \text{ S/m}$; $\varepsilon_r = 60.4$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

Probe: EX3DV4 - SN3877; ConvF(11.44, 11.44, 11.44); Calibrated: 31.12.2015;

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn654; Calibrated: 08.07.2015

Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003

DASY52 52.8.8(1258); SEMCAD X 14.6.10(7372)

CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan

(81x81x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm Maximum value of SAR (interpolated) = 5.71 W/kg

CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan,


dist=1.4mm (8x9x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 82.17 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 7.49 W/kg

SAR(1 g) = 4.06 W/kg; SAR(10 g) = 2.7 W/kg

Maximum value of SAR (measured) = 5.65 W/kg

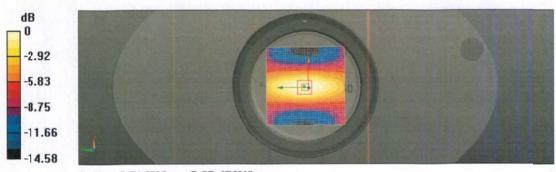


0 dB = 5.71 W/kg = 7.57 dBW/kg

Certificate No: CLA150-4019_Feb16

Page 7 of 8

Impedance Measurement Plot for Body TSL

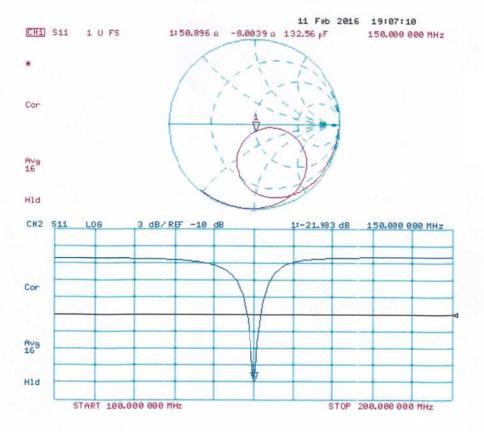

Extended Dipole Calibrations

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dB, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Head						
Date of measurement	Return-loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary impedance (ohm)	Delta (ohm)
2016-02-11	-24.4		47.4		-5.3	
2017-02-06	-23.8	2.46	47.6	0.2	-5.4	0.10

Body						
Date of measurement	Return-loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary impedance (ohm)	Delta (ohm)
2016-02-11	-22.0		50.9		-8.0	
2017-02-06	-21.5	2.71	51.2	0.3	-8.3	-0.30

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 50hm of prior calibration. Therefore the verification result should support extended calibration.

1.2. DAE4 Calibration Certificate



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2218 Fax: +86-10-62304633-2209 E-mail: cttl@chinattl.com Http://www.chinattl.cn

Client:

CIQ(Shenzhen)

Certificate No: Z17-97109

CALIBRATION CERTIFICATE

Object

DAE4 - SN: 1315

Calibration Procedure(s)

FF-Z11-002-01

Calibration Procedure for the Data Acquisition Electronics

(DAEx)

Calibration date:

August 15, 2017

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22 \pm 3) °C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards ID # Cal Date(Calibrated by, Certificate No.)

Scheduled Calibration

Process Calibrator 753

1971018

Name

27-Jun-17 (CTTL, No.J17X05859)

June-18

Calibrated by:

Function

Yu Zongying

Qi Dianyuan

SAR Test Engineer

Reviewed by:

Lin Hao SAR Test Engineer

Approved by:

SAR Project Leader

Issued: August 16, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z17-97109

Page 1 of 3



Add: No.51 Xueyuan Road, Haidian District, Bejjing, 100191, China Tel: +86-10-62304633-2218 Fax: +86-10-62304633-2209 E-mail: cttl@chinattl.com Http://www.chinattl.cn

Glossary:

DAE data acquisition electronics

Connector angle information used in DASY system to align probe sensor X

to the robot coordinate system.

Methods Applied and Interpretation of Parameters:

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

Certificate No: Z17-97109



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2218 Fax: +86-10-62304633-2209 E-mail: cttl@chinattl.com Http://www.chinattl.cn

DC Voltage Measurement

A/D - Converter Resolution nominal High Range: 1LSB = 6 Low Range: 1LSB = 6.1μV , 61nV , full range = -100...+300 mV Low Range: 1LSB = 61nV , full range = -1......+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Υ	Z
High Range	405.175 ± 0.15% (k=2)	405.013 ± 0.15% (k=2)	404.971 ± 0.15% (k=2)
Low Range	3.99087 ± 0.7% (k=2)	3.98644 ± 0.7% (k=2)	3.98913 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system 20.5° ± 1 °	Connector Angle to be used in DASY system	20.5° ± 1 °
---	---	-------------

Certificate No: Z17-97109 Page 3 of 3

-----End-----