



Impedance Plot for SN 15/16 DIP 0G835-399

835 Head

Calibrated impedance: $59.4\Omega - 0.8j\Omega$; Measurement impedance: $62.7\Omega - 1.3j\Omega$ (within 5Ω)

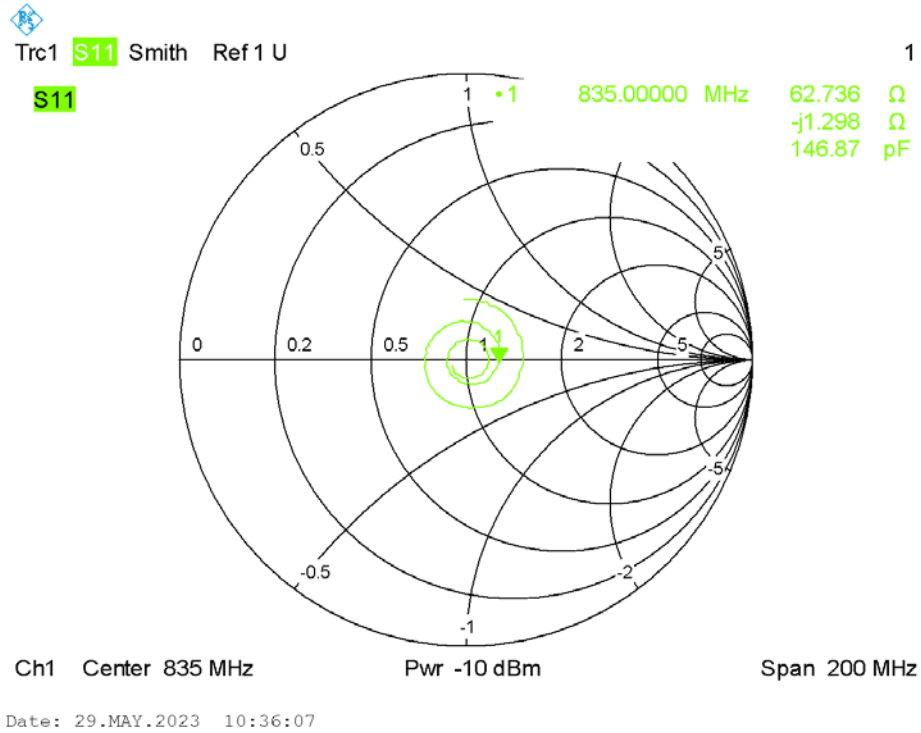


Calibrated return loss: -20.99dB; Measurement return loss: -21.73dB (within 20%)

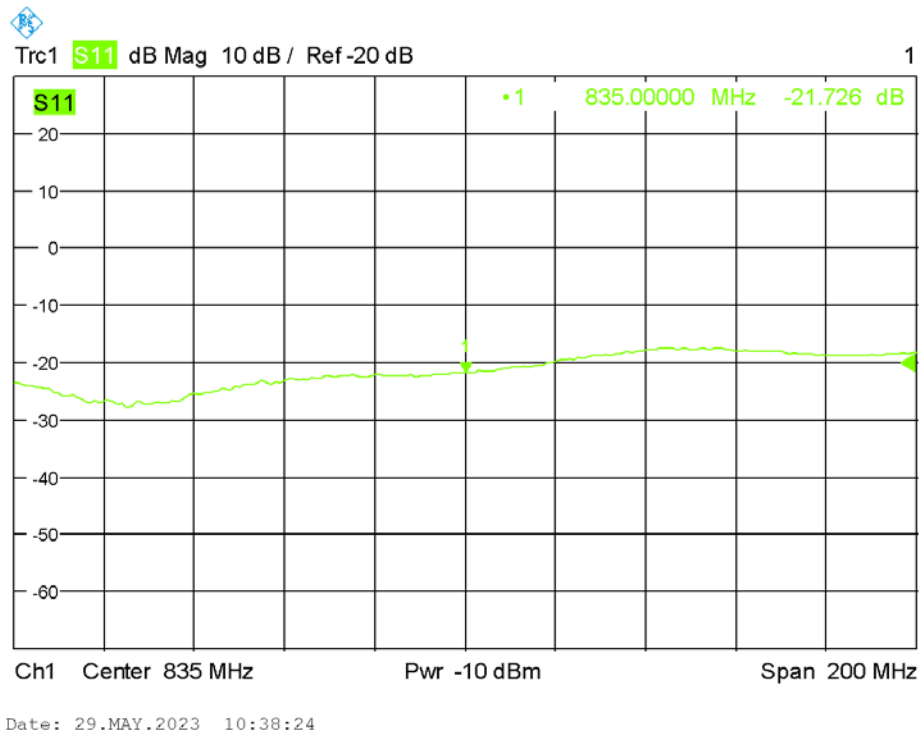


Impedance Plot for SN 46/11 DIP 1G800-186

1800 Head

Calibrated impedance: $47.2\Omega + 4.6j\Omega$; Measurement impedance: $47.7\Omega + 1.5j\Omega$ (within 5Ω)

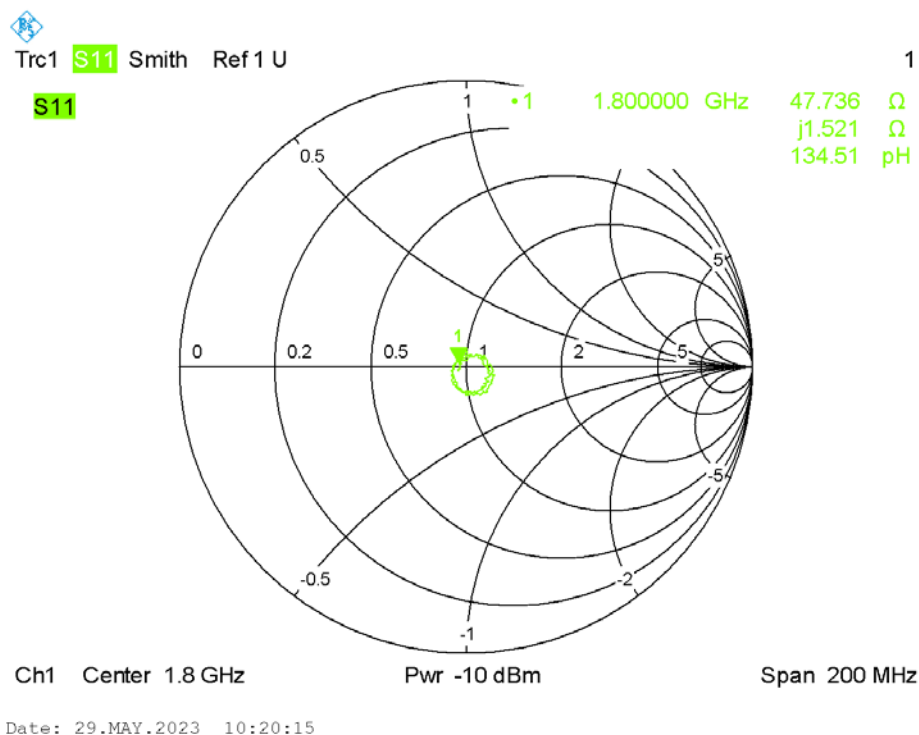


Calibrated return loss: -25.33dB; Measurement return loss: -27.28dB (within 20%)

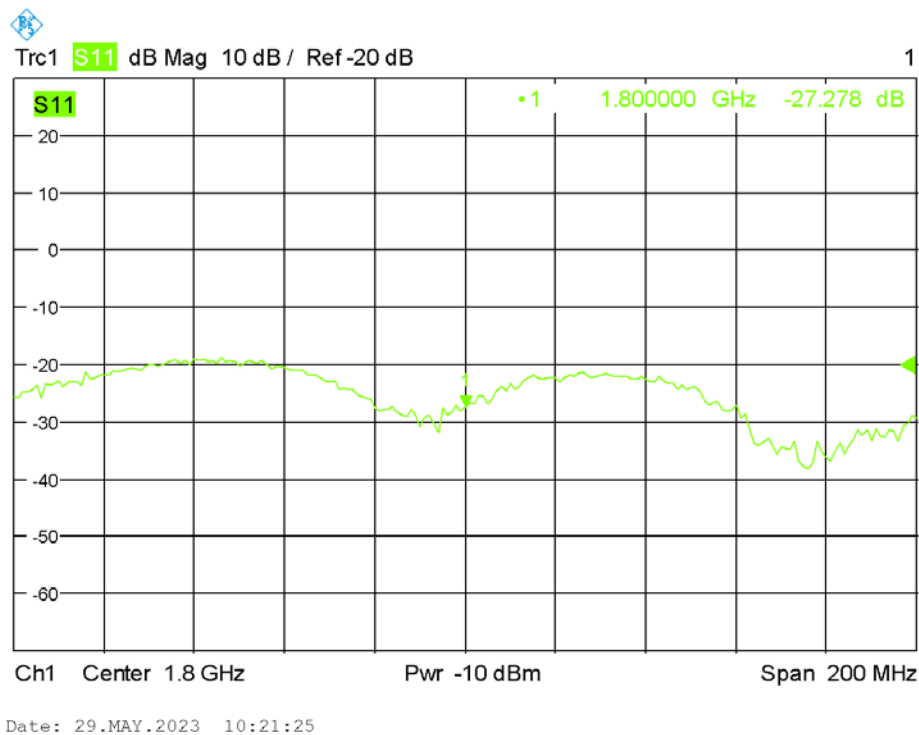


Impedance Plot for SN 29/15 DIP 1G900-389

1900 Head

Calibrated impedance: $52.2\Omega + 6.1j\Omega$; Measurement impedance: $51.0\Omega + 3.2j\Omega$ (within 5Ω)

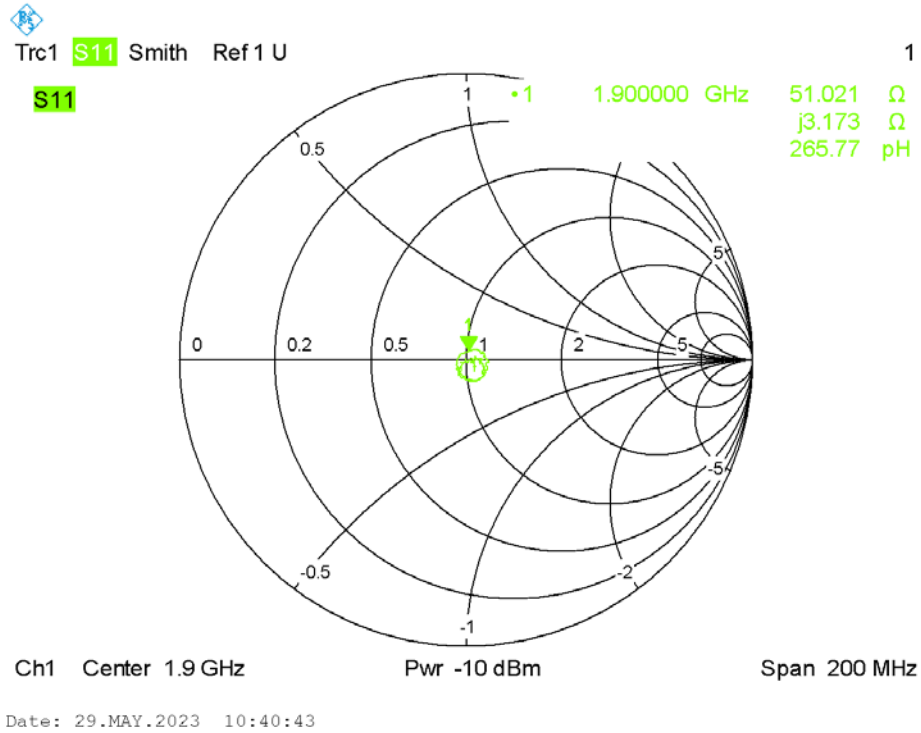


Calibrated return loss: -23.76dB; Measurement return loss: -21.07dB (within 20%)

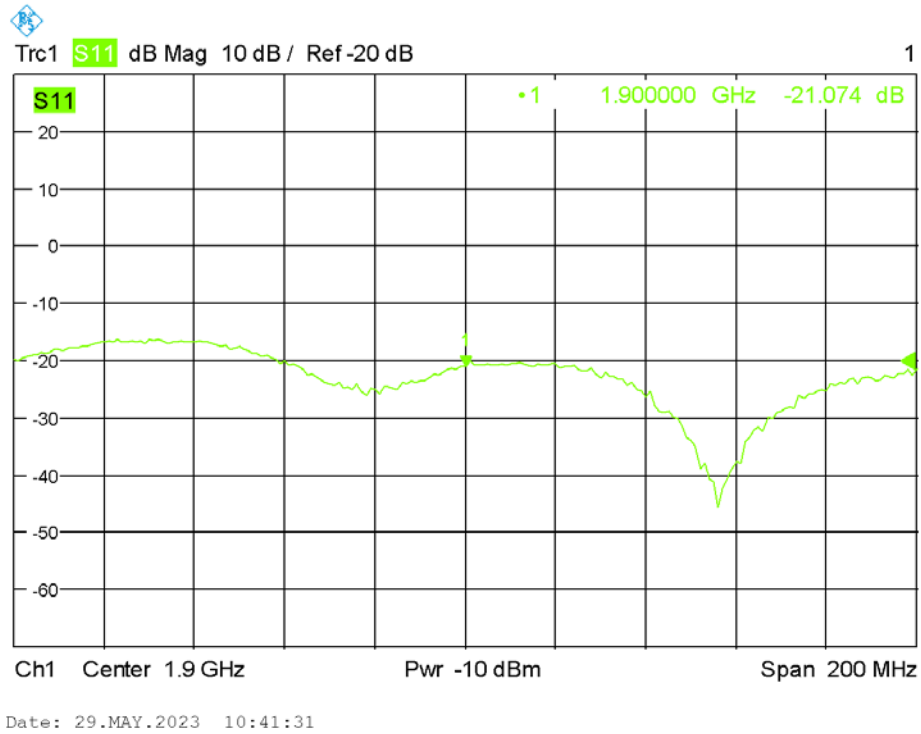

Impedance Plot for SN 29/15 DIP 2G450-393


2450 Head

Calibrated impedance: $52.3\Omega + 3.4j\Omega$; Measurement impedance: $55.8\Omega + 1.6j\Omega$ (within 5Ω)

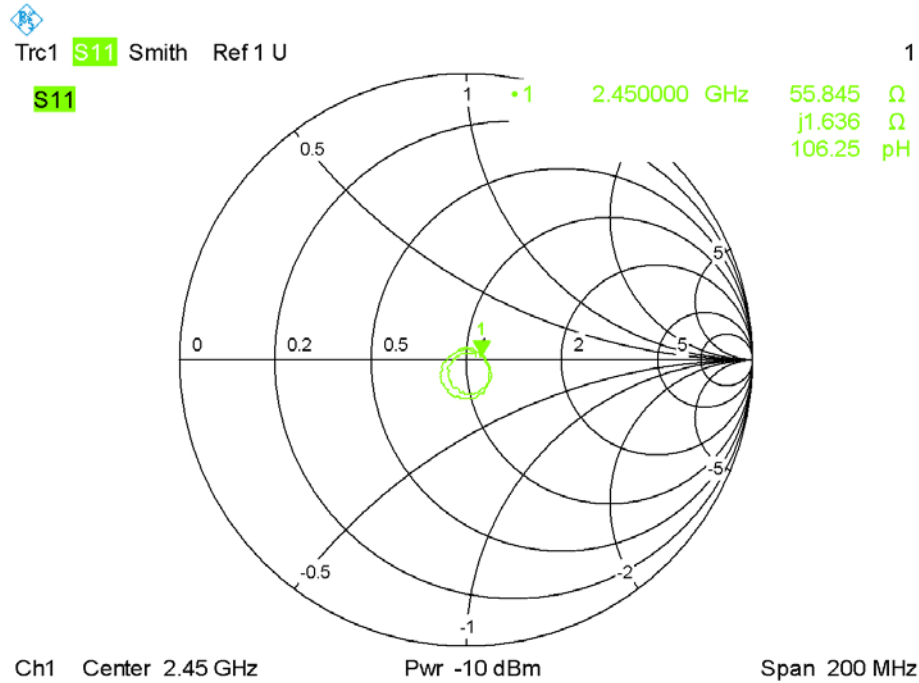

Date: 29.MAY.2023 10:49:23

Calibrated return loss: -27.80dB; Measurement return loss: -24.53dB (within 20%)

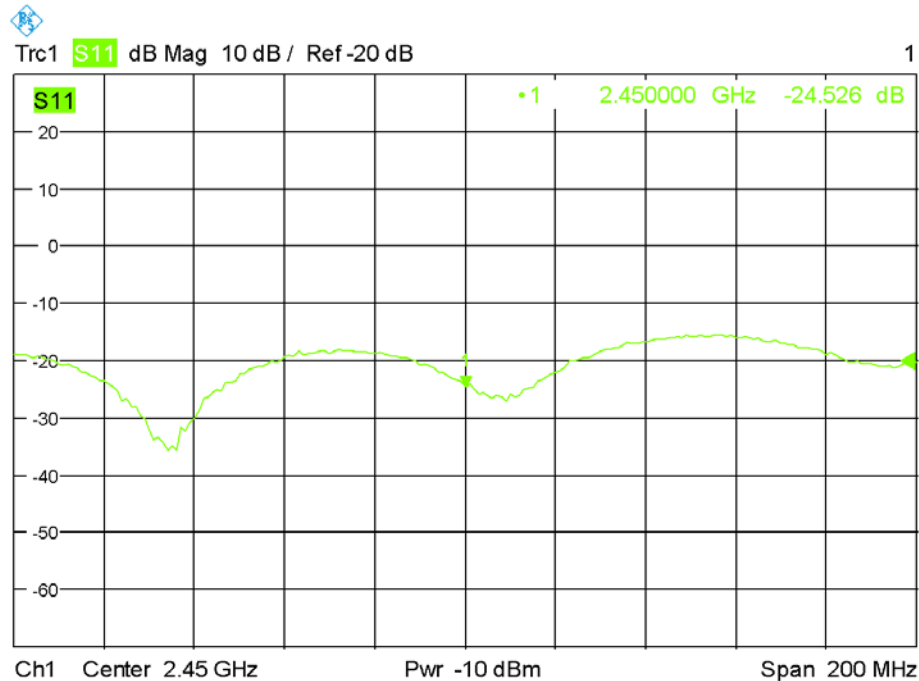


Date: 29.MAY.2023 10:50:11

Impedance Plot for SN 22/16 DIP 2G600-407

2600 Head

Calibrated impedance: $51.0\Omega + 5.3j\Omega$; Measurement impedance: $60.0\Omega + 3.6j\Omega$ (within 5Ω)

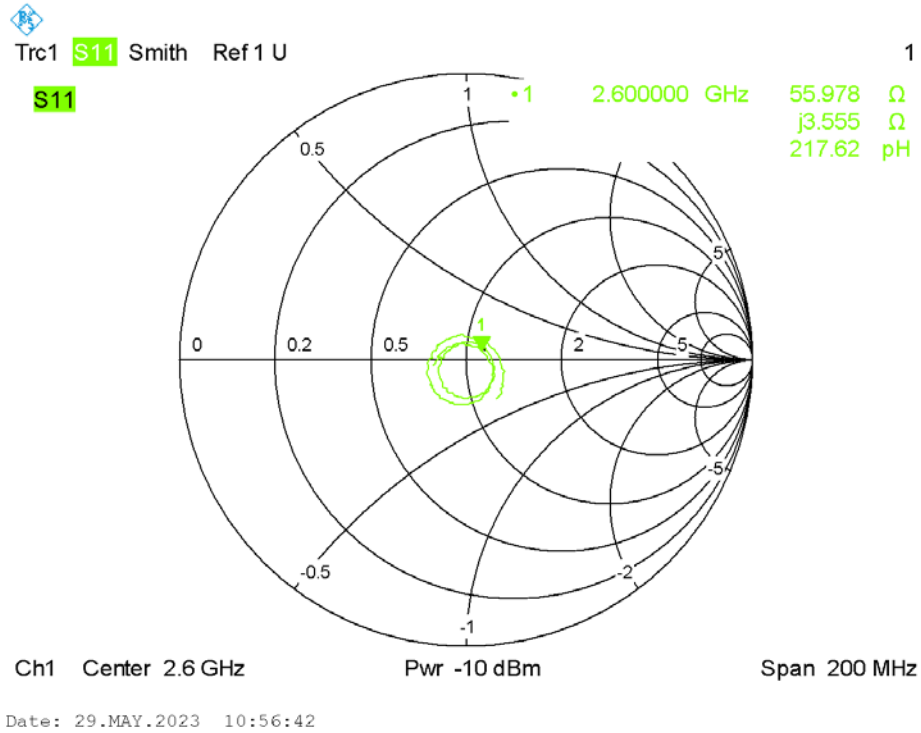

Calibrated return loss: -25.28dB; Measurement return loss: -23.29dB (within 20%)

