


# Appendix D


## Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System

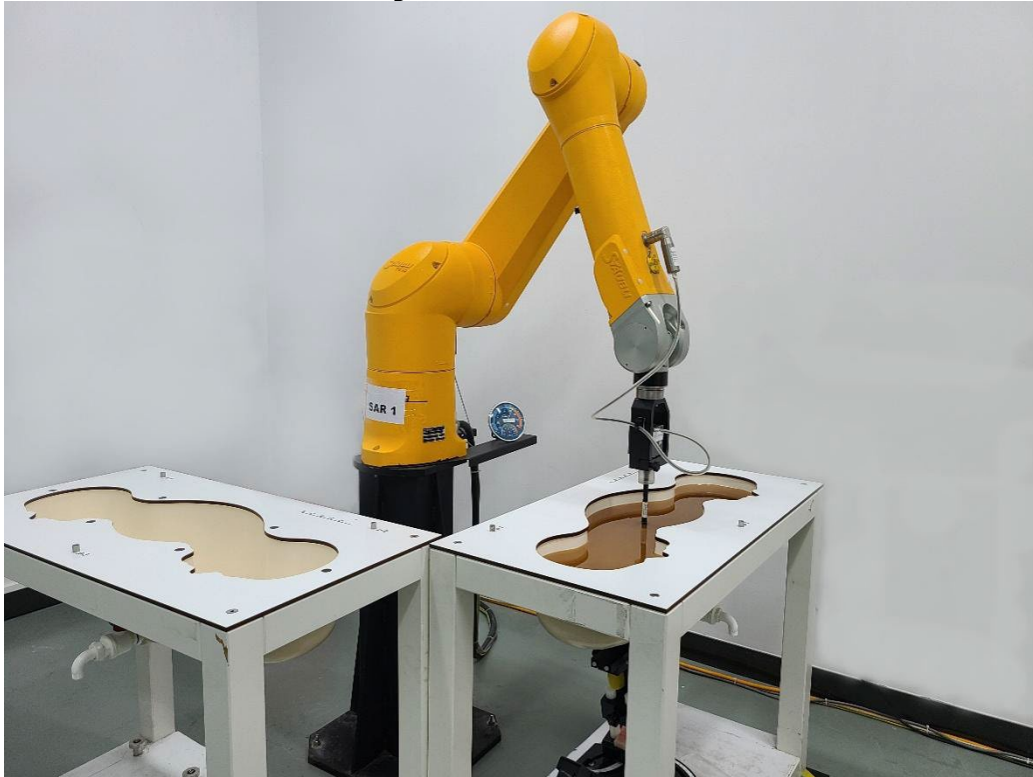

## 2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 A photograph showing a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically next to the container, with the 10 cm mark visible. The container has a blue outer rim and a white inner lining. The liquid level is approximately 8 cm high.	NA

### 3. Photographs of EUT test position

Photo 2: Left Cheek	Photo 3: Left Tilted
	
Photo 4: Right Cheek	Photo 5: Right Tilted
	
Photo 6: Front Side 15mm	Photo 7: Back Side 15mm
	

Photo 8: Front Side 10mm



Photo 9: Back Side 10mm



Photo 10: Left Side 10mm



Photo 11: Right Side 10mm



Photo 12: Top Side 10mm

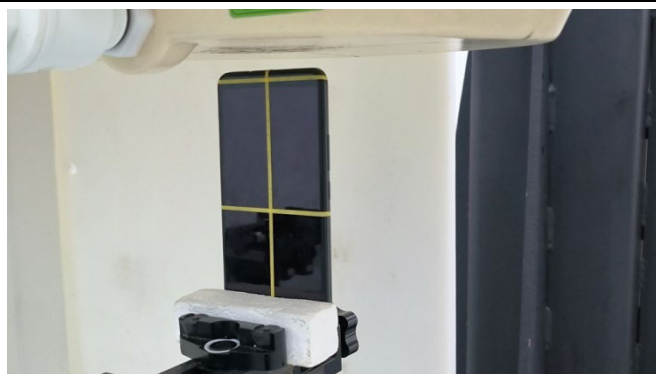


Photo 13: Bottom Side 10mm



#### 4. EUT Constructional Details

