

Annex B: Probe and dipole description and calibration certificates

B.1 Probe, measurement chain description, specification and calibration certificate



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Page

2(14)

Author Data

Daoud Attayi

Dates of Test


March 18-24, Nov. 05-14, 2014

Report No RTS-6057-1411-18


FCC ID L6ARGV160LW

DASY Dosimetric Assessment System by Schmid & Partner Engineering AG



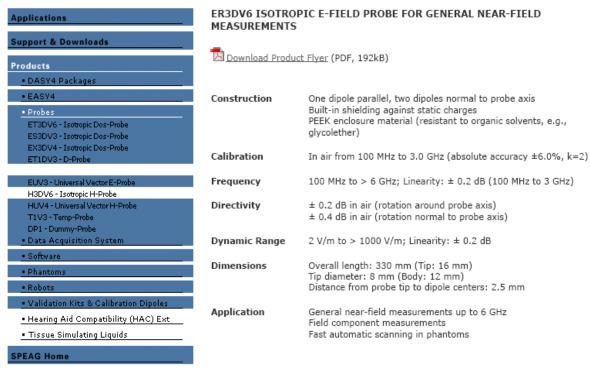


http://www.dasy4.com/er3.htm



All measurements were performed to the nearest element point as per the C63.19 standard. Offset distances were entered in the DASY5 software so that the measurement was to the nearest element.

Figures 1, provided by the manufacturer, illustrate detail of the probe tip and its dimensions.

ER3DV6 E-Field probe: The distances from the probe tip to the closest points on the dipole sensors are 1.45mm for X and Y and 1.25mm for Z. From the probe tip to the center of the sensors is 2.5mm.

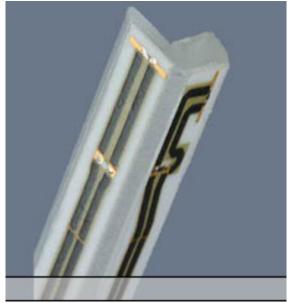

E-Field Probe (ER3DV6)



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Report No

4(14)

Page

Author Data

Daoud Attavi

Dates of Test

March 18-24, Nov. 05-14, 2014

RTS-6057-1411-18

FCC ID L6ARGV160LW

The following information is from the system manufacturer user manual describing the process chain:

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcv_i}$$
(20.1)

 $\begin{array}{lll} \text{with} & V_i & = \text{compensated signal of channel i} & (i = x, y, z) \\ U_i & = \text{input signal of channel i} & (i = x, y, z) \\ cf & = \text{crest factor of exciting field} & (DASY parameter) \\ dcp_i & = \text{diode compression point} & (DASY parameter) \end{array}$

From the compensated input signals the primary field data for each channel can be evaluated:

E – field
probes :
$$E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

H – field
probes :
$$H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}$$

with
$$V_i$$
 = compensated signal of channel i (i = x, y, z)
 $Norm_i$ = sensor sensitivity of channel i (i = x, y, z)

 $\mu V/(V/m)^2$ for E-field Probes

ConvF = sensitivity enhancement in solution

 a_{ij} = sensor sensitivity factors for H-field probes

f = carrier frequency [GHz]

 E_i = electric field strength of channel i in V/m H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$
(20.2)

The measurement / integration time per point is > 500 ms, as per the system manufacturer:

The time response of the field probes has been assessed by exposing the probe to a well-controlled field producing signals larger than HAC E- and H-fields of class M4. The signal response time is evaluated as the time required by the system to reach 90% of the expected final value after an on/off switch of the power source with an integration time of 500 ms and a probe response time of <5 ms. In the current implementation, DASY4 waits longer than 100 ms after having reached the grid point before starting a measurement, i.e., the response time uncertainty is negligible.

If the device under test does not emit a CW signal, the integration time applied to measure the electric field at a specific point may introduce additional uncertainties due to the discretization. The tolerances for the different systems had the worst-case of 2.6%.



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Page

5(14)

Author Data

Daoud Attayi

Dates of Test

March 18-24, Nov. 05-14, 2014

Report No

RTS-6057-1411-18

FCC ID L6ARGV160LW

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerlscher Kalibrierdienst
C Service sulsse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Muttilateral Agreement for the recognition of calibration certificates

Citent Black

Blackberry Waterloo

Certificate No: ER3-2286_Jan14

Accreditation No.: SCS 108

CALIBRATION CERTIFICATE

Object

ER3DV6 - SN:2286

Calibration procedure(s)

QA CAL-02.v8, QA CAL-25.v6

Calibration procedure for E-field probes optimized for close near field

evaluations in air

Calibration date:

January 17, 2014

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration	
Power meter E4419B	GB41293874	04-Apr-13 (No. 217-01733)	Apr-14	
Power sensor E4412A	MY41498087	04-Apr-13 (No. 217-01733)	Apr-14	
Reference 3 dB Attenuator	SN: S5054 (3c)	04-Apr-13 (No. 217-01737)	Apr-14	
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-13 (No. 217-01735)	Apr-14	
Reference 30 dB Attenuator	SN: S5129 (30b)	04-Apr-13 (No. 217-01738)	Apr-14	
Reference Probe ER3DV6	SN: 2328	10-Oct-13 (No. ER3-2328_Oct13)	Oct-14	
DAE4	SN: 789	15-May-13 (No. DAE4-789_May13)	May-14	
Secondary Standards	ID	Check Date (in house)	Scheduled Check	
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16	
Network Analyzer HP 8753E	etwork Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-13) in hos		In house check: Oct-14	

	Name	Function	Sighature }
Calibrated by:	Claudio Leubler	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	ING.
	e shall not be reproduced except in fu		Issued: January 17, 2014

Certificate No: ER3-2286_Jan14

Page 1 of 10



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Page

6(14)

Author Data

Daoud Attayi

Dates of Test

March 18-24, Nov. 05-14, 2014

Report No RTS-6057-1411-18 FCC ID L6ARGV160LW

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kallbrierdienst
C Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

NORMx,y,z DCP

sensitivity in free space

CF

diode compression point crest factor (1/duty_cycle) of the RF signal

A, B, C, D

modulation dependent linearization parameters

Polarization φ

φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Connector Angle

information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1309-2005, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005
- b) CTIA Test Plan for Hearing Aid Compatibility, April 2010.

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ = 0 for XY sensors and θ = 90 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart).
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ER3-2286 Jan14

Page 2 of 10



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

7(14)

Page

Author Data

Daoud Attavi

March 18-24, Nov. 05-14, 2014

Report No

RTS-6057-1411-18

L6ARGV160LW

ER3DV6 - SN:2286

January 17, 2014

Probe ER3DV6

SN:2286

Manufactured:

September 18, 2002

Calibrated:

January 17, 2014

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ER3-2286_Jan14

Page 3 of 10



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Report No

. . . .

Page

8(14)

Author Data

Daoud Attayi

Dates of Test

March 18-24, Nov. 05-14, 2014

RTS-6057-1411-18

FCC ID L6ARGV160LW

ER3DV6-SN:2286

January 17, 2014

DASY/EASY - Parameters of Probe: ER3DV6 - SN:2286

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) ²)	2.24	1.46	1.50	± 10.1 %
DCP (mV) ^B	98.6	100.7	100.5	

Modulation Calibration Parameters

UID	Communication System Name		Α	В	С	D	VR	Unc
			dB	dB√μV		dB	mV	(k=2)
0	CW	Х	0.0	0.0	1.0	0.00	181.8	±3.5 %
		Y	0.0	0.0	1.0		196.2	
		Z	0.0	0.0	1.0		175.8	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

⁸ Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

9(14)

Page

Author Data

Daoud Attayi

Dates of Test

March 18-24, Nov. 05-14, 2014

Report No

RTS-6057-1411-18


FCC ID L6ARGV160LW

ER3DV6- SN:2286

January 17, 2014

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

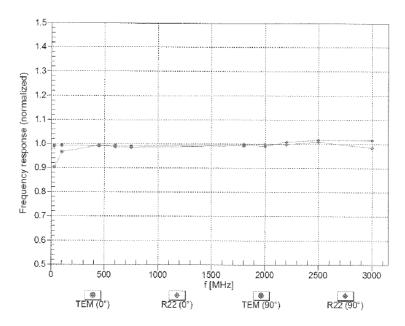

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Page

10(14)

Author Data

Daoud Attayi

Dates of Test

March 18-24, Nov. 05-14, 2014


Report No RTS-6057-1411-18

FCC ID L6ARGV160LW


ER3DV6-- SN:2286

January 17, 2014

Receiving Pattern (ϕ), $9 = 0^{\circ}$

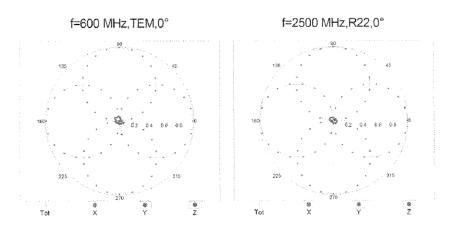

Receiving Pattern (ϕ), $\vartheta = 90^{\circ}$

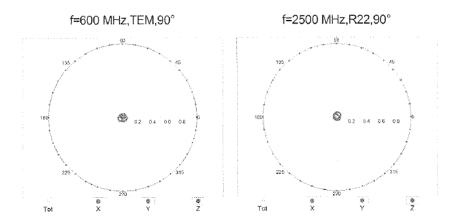

Certificate No: ER3-2286_Jan14

Page 6 of 10



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Page

11(14)

Author Data

Daoud Attayi

Dates of Test

March 18-24, Nov. 05-14, 2014


Report No **RTS-6057-1411-18**

FCC ID L6ARGV160LW

ER3DV6- SN:2286


January 17, 2014

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

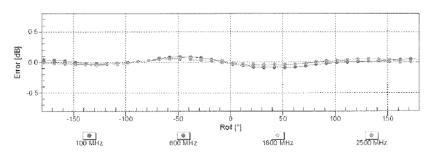

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Receiving Pattern (ϕ), $9 = 90^{\circ}$

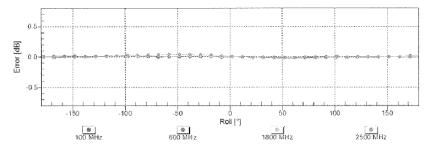

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ER3-2286_Jan14

Page 7 of 10



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Page

12(14)

Author Data

Daoud Attayi

Dates of Test

March 18-24, Nov. 05-14, 2014


Report No RTS-6057-1411-18


FCC ID L6ARGV160LW

ER3DV6-- SN:2286

January 17, 2014

Dynamic Range f(E-field) (TEM cell , f = 900 MHz)

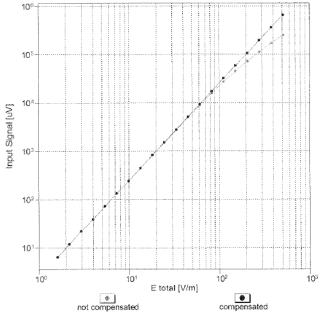

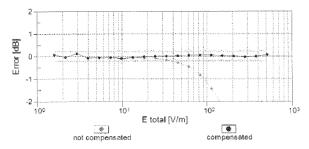

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: ER3-2286_Jan14

Page 8 of 10



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Page

13(14)

Author Data

Daoud Attayi

Dates of Test

March 18-24, Nov. 05-14, 2014

Report No RTS-6057-1411-18


FCC ID L6ARGV160LW

ER3DV6-- SN:2286

January 17, 2014

Deviation from Isotropy in Air

Error (φ, θ), f = 900 MHz

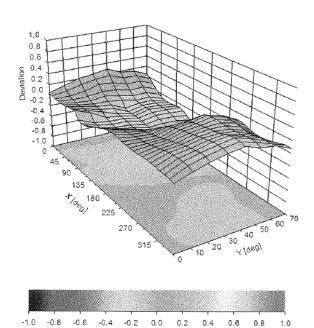

Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ (k=2)

Certificate No: ER3-2286_Jan14

Page 9 of 10



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGV161LW (SQW100-3)

Page

14(14)

Author Data

Daoud Attayi

Dates of Test

March 18-24, Nov. 05-14, 2014

Report No RTS-6057-1411-18

FCC ID L6ARGV160LW

ER3DV6-- SN:2286

January 17, 2014

DASY/EASY - Parameters of Probe: ER3DV6 - SN:2286

Other Probe Parameters

Sensor Arrangement	Rectangular
Connector Angle (°)	-8.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	8 mm
Probe Tip to Sensor X Calibration Point	2.5 mm
Probe Tip to Sensor Y Calibration Point	2.5 mm
Probe Tip to Sensor Z Calibration Point	2.5 mm

Certificate No: ER3-2286_Jan14

Page 10 of 10