

# **Appendix B - DAE & Probe Calibration Certificate**

eughausstrasse 43, 8004 Zurio		Holdedalah	S Swiss Calibration Service
Accredited by the Swiss Accredit The Swiss Accreditation Servin Multilateral Agreement for the	ce is one of the signatories	s to the EA	ion No.: SCS 0108
Client SGS			
Taoyuan City		Certificate	No: DAE4-1751_Mar24
CALIBRATION	CERTIFICATE		
Object	DAE4 SD 000 D	04 BP - SN: 1751	
00,001	DAL4 - 30 000 L	04 DP - SN: 1751	
Calibration procedure(s)	QA CAL-06.v30		
	Calibration procee	dure for the data acquisition ele	ectronics (DAE)
Calibration date:	March 10,0001		
Canoradon udle:	March 13, 2024		
The measurements and the unce	ortainties with confidence pro	anal standards, which realize the physical $i$ obability are given on the following pages $i$ facility: environment temperature (22 $\pm$ 3)	and are part of the certificate.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M&	rtainties with confidence pro- cted in the closed laboratory TE critical for calibration)	obability are given on the following pages i / facility: environment temperature ( $22 \pm 3$ )	and are part of the certificate. )℃ and humidity < 70%.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards	ortainties with confidence pro	obability are given on the following pages , ( facility: environment temperature (22 ± 3) Cal Date (Certificate No.)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001	trainties with confidence pro- cted in the closed laboratory TE critical for calibration) ID # SN: 0810278	Obability are given on the following pages if facility: environment temperature (22 ± 3)         Cal Date (Certificate No.)         29-Aug-23 (No:37421)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Aug-24
The measurements and the unce	trainties with confidence pro- cted in the closed laboratory TE critical for calibration)   D #   SN: 0810278   ID #	obability are given on the following pages .         / facility: environment temperature (22 ± 3)         Cal Date (Certificate No.)         29-Aug-23 (No:37421)         Check Date (in house)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Aug-24 Scheduled Check
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards	trainties with confidence pro- cted in the closed laboratory TE critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001	obability are given on the following pages .         / facility: environment temperature (22 ± 3)         Cal Date (Certificate No.)         29-Aug-23 (No:37421)         Check Date (in house)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Aug-24
All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit	trainties with confidence pro- cted in the closed laboratory TE critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001	obability are given on the following pages i         facility: environment temperature (22 ± 3)         Cal Date (Certificate No.)         29-Aug-23 (No:37421)         Check Date (in house)         23-Jan-24 (in house check)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Aug-24 Scheduled Check In house check: Jan-25
All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit	trainties with confidence pro- cted in the closed laboratory TE critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001	obability are given on the following pages i         facility: environment temperature (22 ± 3)         Cal Date (Certificate No.)         29-Aug-23 (No:37421)         Check Date (in house)         23-Jan-24 (in house check)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Aug-24 Scheduled Check In house check: Jan-25 In house check: Jan-25
All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit	ttainties with confidence pro- ted in the closed laboratory TE critical for calibration)  D # SN: 0810278  ID # SE UWS 053 AA 1001 SE UMS 006 AA 1002	obability are given on the following pages ; ( facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 29-Aug-23 (No:37421) Check Date (in house) 23-Jan-24 (in house check) 23-Jan-24 (in house check)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Aug-24 Scheduled Check In house check: Jan-25
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit Calibrator Box V2.1	ID #         SN: 0810278         ID #         SN: 0810278         ID #         SE UWS 053 AA 1001         SE UMS 006 AA 1002	Deablifty are given on the following pages .         / facility: environment temperature (22 ± 3)         Cal Date (Certificate No.)         29-Aug-23 (No:37421)         Check Date (in house)         23-Jan-24 (in house check)         23-Jan-24 (in house check)         23-Jan-24 (in house check)         Function	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Aug-24 Scheduled Check In house check: Jan-25 In house check: Jan-25

Certificate No: DAE4-1751\_Mar24

Page 1 of 5

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document dear and the contract and company's mining all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 2 of 45

### Calibration Laboratory of Schmid & Partner Engineering AG eughausstrasse 43, 8004 Zurich, Switzerland

ilac-MR

Schweizerischer Kalibrierdier Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

S

С

S

credited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary

Zeuah

DAE Connector angle

# data acquisition electronics

information used in DASY system to align probe sensor X to the robot coordinate system

#### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement. Output voltage and statistical results over a large number of . zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated
  - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-1751 Mar24

Page 2 of 5

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction form exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 3 of 45

#### DC Voltage Measurement

Calibration Factors	х		Y		z
DASY measurement par	rameters: Auto a	Zero Time: 3	sec; Measuring	time: 3 sec	
Low Range:	1LSB =	61nV,		-1+3mV	
High Range:					
	1LSB =	6.1uV.	full range -	-100+300 mV	
A/D - Converter Resolut	ion norminal				

High Range         404.302 ± 0.02% (k=2)         404.262 ± 0.02% (k=2)         404.527 ± 0.02% (k				
	High Range	404.302 ± 0.02% (k=2)	404.262 ± 0.02% (k=2)	$404.527 \pm 0.02\% \text{ (k=2)}$
Low Range 3.98545 ± 1.50% (k=2) 4.00007 ± 1.50% (k=2) 4.00889 ± 1.50% (k	Low Range	3.98545 ± 1.50% (k=2)	4.00007 ± 1.50% (k=2)	4.00889 ± 1.50% (k=2)

#### **Connector Angle**

Connector Angle to be used in DASY system	340.0 $^{\circ}$ $\pm$ 1 $^{\circ}$
---	-------------------------------------

Certificate No: DAE4-1751\_Mar24

Page 3 of 5

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留的天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

www.sgs.com.tw



# Report No: TESA2410000648ES Page: 4 of 45

### Appendix (Additional assessments outside the scope of SCS0108)

#### 1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	200004.24	2.04	0.00
Channel X + Input	20012.21	2.36	0.01
Channel X - Input	-19991.98	2.30	-0.01
Channel Y + Input	200003.93	1.59	0.00
Channel Y + Input	20008.65	-1.27	-0.01
Channel Y - Input	-19993.86	0.47	-0.00
Channel Z + Input	200002.71	0.78	0.00
Channel Z + Input	20006.16	-3.77	-0.02
Channel Z - Input	-19994.26	0.07	-0.00

Low Range		Reading (µV)	Difference (µV)	Error (%)
Channel X	+ Input	2009.98	1.17	0.06
Channel X	+ Input	208.49	-0.63	-0.30
Channel X	- Input	-190.51	0.27	-0.14
Channel Y	+ Input	2009.15	0.31	0.02
Channel Y	+ Input	208.94	-0.18	-0.08
Channel Y	- Input	-191.11	-0.35	0.18
Channel Z	+ Input	2008.91	0.14	0.01
Channel Z	+ Input	208.43	-0.60	-0.29
Channel Z	- Input	-192.33	-1.42	0.74

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	9.27	7.52
	- 200	-7.71	-8.70
Channel Y	200	12.87	12.77
	- 200	-14.29	-14.57
Channel Z	200	3.15	3.40
	- 200	-5.72	-5.94

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	*	1.78	-3.96
Channel Y	200	6.24	-	2.54
Channel Z	200	7.70	4.26	1

Certificate No: DAE4-1751\_Mar24

Page 4 of 5

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document dear and the contract and company's mining all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.



# Report No: TESA2410000648ES Page: 5 of 45

### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15782	13277
Channel Y	16207	15182
Channel Z	16262	14305

### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input  $10M\Omega$ 

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.39	-1.17	2.70	0.53
Channel Y	-0.25	-1.19	0.54	0.33
Channel Z	-0.57	-1.68	0.44	0.38

### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

### 8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

#### 9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)	
Supply (+ Vcc)	+0.01	+6	+14	
Supply (- Vcc)	-0.01	-8	-9	

Certificate No: DAE4-1751\_Mar24

Page 5 of 5

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 6 of 45

ngineering AG	y of		Schweizerischer Kalibrierdiens Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
eughausstrasse 43, 8004 Zu	rich, Switzerland	The failed and the set	
ccredited by the Swiss Accre ne Swiss Accreditation Ser ultilateral Agreement for th	rvice is one of the signato	ries to the EA	reditation No.: SCS 0108
lient SGS Taoyuan City		Certificate No.	X-7823_Jul24
CALIBRATION C	ERTIFICATE		
Object	EX3DV4 - SN:78	323	
Calibration procedure(s)	QA CAL-25.v8	QA CAL-12.v10, QA CAL-14.v7,	
Calibration date	July 31, 2024		
The measurements and the All calibrations have been co	uncertainties with confidence onducted in the closed laboration	national standards, which realize the physical e probability are given on the following pages atory facility: environment temperature ( $22 \pm 3$	and are part of the certificate.
The measurements and the All calibrations have been co	uncertainties with confidenc	e probability are given on the following pages atory facility: environment temperature ( $22 \pm 3$	and are part of the certificate.
The measurements and the All calibrations have been or Calibration Equipment used	uncertainties with confidence onducted in the closed laboration	e probability are given on the following pages atory facility: environment temperature ( $22 \pm 3$	and are part of the certificate.
The measurements and the All calibrations have been co Calibration Equipment used Primary Standards Power meter NRP2	uncertainties with confidence onducted in the closed labora (M&TE critical for calibration ID SN: 104778	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 26-Mar-24 (No. 217-04036/04037)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Mar-25
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-Z91	uncertainties with confidence anducted in the closed labora (M&TE critical for calibration ID SN: 104778 SN: 103244	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 26-Mar-24 (No. 217-04036/04037) 26-Mar-24 (No. 217-04036)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25
The measurements and the All calibrations have been co Calibration Equipment used Primary Standards Power meter: NRP2 Power sensor NRP-291 OCP DAK-3.5 (weighted)	uncertainties with confidenc anducted in the closed labora (M&TE critical for calibration ID SN: 104778 SN: 104244 SN: 103244 SN: 1249	e probability are given on the following pages tory facility: environment temperature (22±3) ) Cal Date (Certificate No.) 26-Mar-24 (No. 217-04036/04037) 26-Mar-24 (No. 217-04036) 05-Oct 23 (OCP-DAK3.5-1249_Oct23)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Cct-24
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-Z91 OCP DAK-3.5 (weighted) OCP DAK-3.5 (weighted)	uncertainties with confidence anducted in the closed labors (M&TE critical for calibration ID SN: 104778 SN: 103244 SN: 103244 SN: 1249 SN: 1016	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 26-Mar-24 (No. 217-04036)(04037) 26-Mar-24 (No. 217-04036) 05-Oct-23 (OCP-DAK13.5-1249_Oct23) 05-Oct-23 (OCP-DAK13.5-1249_Oct23)	and are part of the certificate. %C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Oct-24 Oct-24
The measurements and the All calibrations have been cc Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-3.5 (weighted) OCP DAK-12 Reference 20 dB Attenuator	uncertainties with confidence anducted in the closed labora (M&TE critical for calibration ID SN: 104778 SN: 104778 SN: 103244 SN: 1249 SN: 1016 SN: C2552 (20x)	e probability are given on the following pages tory facility: environment temperature (22±3 ) Cal Date (Certificate No.) 26-Mar-24 (No. 217-04036/04037) 28-Mar-24 (No. 217-04036) 05-Oct-23 (OCP-DAK3.5-1249_Oct23) 05-Oct-23 (OCP-DAK12-1016_Oct23) 26-Mar-24 (No. 217-04046)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Mar-25 Oct-24 Mar-25 Mar-25
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-35 (weighted) OCP DAK-35 (weighted) OCP DAK-42 (weighted) DAE4	uncertainties with confidence anducted in the closed labors (M&TE critical for calibration ID SN: 104778 SN: 103244 SN: 103244 SN: 1249 SN: 1016	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 26-Mar-24 (No. 217-04036)(04037) 26-Mar-24 (No. 217-04036) 05-Oct-23 (OCP-DAK13.5-1249_Oct23) 05-Oct-23 (OCP-DAK13.5-1249_Oct23)	and are part of the certificate. %C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Oct-24 Oct-24
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-35 (weighted) OCP DAK-12 Reference 20 dB Attenuator DAE4 Reference Probe EX3DV4	uncertainties with confidence onducted in the closed labors (M&TE critical for calibration SN: 104778 SN: 103244 SN: 1016 SN: 1016 SN: 20452 (20x) SN: 660 SN: 7349	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 26-Mar-24 (No. 217-04036/04037) 26-Mar-24 (No. 217-04036/04037) 05-Oct 23 (OCP-DAK3.5-1249_Oct23) 05-Oct 23 (OCP-DAK3.5-1249_Oct23) 26-Mar-24 (No. 217-04046) 23-Feb-24 (No. DAE4-660_Feb24) 03-Jun-24 (No. EX3-7349_Jun24)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Mar-25 Oct-24 Mar-25 Cot-24 Mar-25 Feb-25 Jun-25
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-Z91 OCP DAK-35 (weighted) OCP DAK-45 (weighted) OCP DAK-45 (weighted) DCP DAK-47 (weighted) DCP DAK-47 (weighted) DCP DAK-47 (weighted) DCP DAK-47 (weighted) Secondary Standards	uncertainties with confidence anducted in the closed labors (M&TE critical for calibration SN: 104776 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 1016 SN: CC2552 (20x) SN: 660 SN: 7349	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 28-Mar-24 (No. 217-04036/04037) 28-Mar-24 (No. 217-04036/04037) 09-Oct 23 (OCP-DAK 5-1249_Oct23) 05-Oct 23 (OCP-DAK 5-1249_Oct23) 28-Mar-24 (No. 217-04046) 23-Feb-24 (No. 2R24-606_Feb24) 03-Jun-24 (No. EX3-7349_Jun24) Check Date (in house)	and are part of the certificate. %C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Oct-24 Oct-24 Oct-24 Mar-25 Jun-25 Scheduled Check
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-3.5 (weighted) OCP DAK-12 Reference 20 dB Attenuator DAE4 Reference Probe EX3DV4 Secondary Standards Power meter E4419B	uncertainties with confidence onducted in the closed labors (M&TE critical for calibration SN: 104778 SN: 103244 SN: 1016 SN: 1016 SN: 20452 (20x) SN: 660 SN: 7349	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 26-Mar-24 (No. 217-04036/04037) 26-Mar-24 (No. 217-04036/04037) 26-Mar-24 (No. 217-04046) 23-Feb-24 (No. DAE4-660_Feb24) 03-Jun-24 (No. EX3-7349_Jun24) Check Date (in house check Jun-24)	and are part of the certificate. )*C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Oct-24 Oct-24 Mar-25 Feb-25 Jun-25 Scheduled Check In house check: Jun-26
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-32 (weighted) OCP DAK-12 (weighted) OCP DAK-12 (weighted) OCP DAK-12 (weighted) OCP DAK-12 Reference 20 dB Attenuator DAE4 Reference Probe EX3DV4 Secondary Standards Power sensor E4412A Power sensor E4412B	uncertainties with confidence onducted in the closed labors (M&TE critical for calibration SN: 104778 SN: 103244 SN: 1249 SN: 1016 SN: CC2552 (20x) SN: 660 SN: 7349 ID SN: GB41293874	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 28-Mar-24 (No. 217-04036/04037) 28-Mar-24 (No. 217-04036/04037) 09-Oct 23 (OCP-DAK 5-1249_Oct23) 05-Oct 23 (OCP-DAK 5-1249_Oct23) 28-Mar-24 (No. 217-04046) 23-Feb-24 (No. 2R24-606_Feb24) 03-Jun-24 (No. EX3-7349_Jun24) Check Date (in house)	and are part of the certificate. %C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Oct-24 Oct-24 Cot-24 Mar-25 Feb-25 Jun-25 Scheduled Check
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-12 (weighted) OCP DAK-12 (weighted) OCP DAK-12 (weighted) OCP DAK-12 Reference Probe EX3DV4 Secondary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Power sensor E4412A Pre generator HP 8648C	uncertainties with confidence onducted in the closed labors (M&TE critical for calibration SN: 104778 SN: 108244 SN: 108244 SN: 108244 SN: 1016 SN: 20552 (20x) SN: 660 SN: 7349 ID SN: 0B41293874 SN: MY41498087 SN: 000110210 SN: 000110210	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 26-Mar-24 (No. 217-04036/04037) 28-Mar-24 (No. 217-04036) 05-Oct 23 (OCP-DAK3 F.1249_Oct23) 05-Oct 23 (OCP-DAK3 F.1249_Oct23) 28-Mar-24 (No. 217-04046) 23-Feb-24 (No. 217-04046) 03-Jun-24 (No. EX3-7349_Jun24) Check Date (in house check Jun-24) 06-Apr-16 (in house check Jun-24)	and are part of the certificate. %C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Oct-24 Oct-24 Oct-24 Oct-24 Oct-24 Jun-25 Feb-25 Jun-25 Scheduled Check In house check: Jun-26 In house check: Jun-26
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-12 (weighted) OCP DAK-12 (weighted) OCP DAK-12 (weighted) OCP DAK-12 Reference Probe EX3DV4 Secondary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Power sensor E4412A Pre generator HP 8648C	uncertainties with confidence anducted in the closed labors (M&TE critical for calibration SN: 104776 SN: 103244 SN: 103244 SN: 103244 SN: 1036 SN: CC2552 (20x) SN: 6C2552 (20x) SN: 6C2552 (20x) SN: 7349 ID SN: GB41293874 SN: MY41498087 SN: MY41498087 SN: 00110210	e probability are given on the following pages tory facility: environment temperature (22 ± 3 ) Cal Date (Certificate No.) 28-Mar-24 (No. 217-04036)04037) 28-Mar-24 (No. 217-04036) 05-Oct 23 (OCP-DAK12-1016_Oct23) 05-Oct 23 (OCP-DAK12-1016_Oct23) 28-Mar-24 (No. 217-04046) 23-Feb-24 (No. 2AE4-60,Feb24) 03-Jun-24 (No. EX3-7349_Jun24) Check Date (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 06-Apr-16 (in house check Jun-24)	and are part of the certificate. %C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Oct-24 Oct-24 Oct-24 Cot-24 Jun-25 Scheduled Check In house check: Jun-26 In house check: Jun-26 In house check: Jun-26
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-12 (weighted) OCP DAK-12 (weighted) OCP DAK-12 (weighted) OCP DAK-12 Reference Probe EX3DV4 Secondary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Power sensor E4412A Pre generator HP 8648C	uncertainties with confidence onducted in the closed labors (M&TE critical for calibration SN: 104778 SN: 108244 SN: 108244 SN: 108244 SN: 1016 SN: 20552 (20x) SN: 660 SN: 7349 ID SN: 0B41293874 SN: MY41498087 SN: 000110210 SN: 000110210	e probability are given on the following pages totry facility: environment temperature (22 ± 3 ) Cal Date (Cartificate No.) 26-Mar-24 (No. 217-04036/04037) 26-Mar-24 (No. 217-04036) 05-Oct 23 (OCP-DAK3:15424_Oct23) 05-Oct 23 (OCP-DAK3:15424_Oct23) 26-Mar-24 (No. 217-04046) 23-Feb-24 (No. 217-04046) 23-Feb-24 (No. 217-04046) 23-Feb-24 (No. 217-04046) Check Date (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 06-Apr-16 (in house check Jun-24)	and are part of the certificate. )*C and humidity < 70%. Scheduled Calibration Mar-25 Oct-24 Oct-24 Mar-25 Feb-25 Feb-25 Jun-25 Scheduled Check In house check: Jun-26 In house check: Jun-26
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-12 (seejahted) OCP DAK-12 (seejahted) OCP DAK-12 (seejahted) Reference 20 dB Attenuator DAE4 Reference Probe EX3DV4 Secondary Standards Power meter E44198 Power sensor E4412A Prover sensor E4412A Pre generator HP 8648C Network Analyzer E8358A	uncertainties with confidence onducted in the closed labors (M&TE critical for calibration SN: 104778 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 202552 (20x) SN: 660 SN: 7349 ID SN: GB41293874 SN: GB41293874 SN: 000110210 SN: US342001700 SN: US342001700 SN: US342001770	e probability are given on the following pages totry facility: environment temperature (22 ± 3 ) Cal Date (Cartificate No.) 26-Mar-24 (No. 217-04036/04037) 26-Mar-24 (No. 217-04036) 05-Oct 23 (OCP-DAK3:15424_Oct23) 05-Oct 23 (OCP-DAK3:15424_Oct23) 26-Mar-24 (No. 217-04046) 23-Feb-24 (No. 217-04046) 23-Feb-24 (No. 217-04046) 23-Feb-24 (No. 217-04046) Check Date (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 06-Apr-16 (in house check Jun-24)	and are part of the certificate. )*C and humidity < 70%. Scheduled Calibration Mar-25 Oct-24 Oct-24 Mar-25 Feb-25 Feb-25 Jun-25 Scheduled Check In house check: Jun-26 In house check: Jun-26 In house check: Jun-26 In house check: Jun-26 In house check: Jun-26
The measurements and the All calibrations have been co	uncertainties with confidence onducted in the closed labors (M&TE critical for calibration SN: 104778 SN: 102244 SN: 102244 SN: 1016 SN: 62552 (20x) SN: 66241293874 SN: 00614293874 SN: 006142193874 SN: 00614210700 SN: US34201700 SN: US34201700 SN: US341080477	e probability are given on the following pages totry facility: environment temperature (22 ± 3 ) Cal Date (Cartificate No.) 26-Mar-24 (No. 217-04036/04037) 28-Mar-24 (No. 217-04036) 05-Oct 23 (OCP-DAKS: 1249_Oct23) 05-Oct 23 (OCP-DAKS: 1249_Oct23) 28-Mar-24 (No. 217-04046) 23-Feb-24 (No. DAE4-660_Feb24) 03-Jun-24 (No. DAE4-660_Feb24) 05-Apr-16 (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 04-Aug-90 (in blues check Jun-24) 31-Mar-14 (in house check Jun-24)	and are part of the certificate. )*C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Oct-24 Oct-24 Oct-24 Oct-24 Jun-25 Scheduled Check In house check: Jun-26 In house check: Oct-24 Signifuture Market Market Mar
The measurements and the All calibrations have been or Calibration Equipment used Primary Standards Power meter NRP2 Power sensor NRP-291 OCP DAK-12 (seejahted) OCP DAK-12 (seejahted) OCP DAK-12 (seejahted) Reference 20 dB Attenuator DAE4 Reference Probe EX3DV4 Secondary Standards Power meter E44198 Power sensor E4412A Prover sensor E4412A Pre generator HP 8648C Network Analyzer E8358A	uncertainties with confidence onducted in the closed labors (M&TE critical for calibration SN: 104778 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 202552 (20x) SN: 660 SN: 7349 ID SN: GB41293874 SN: GB41293874 SN: 000110210 SN: US342001700 SN: US342001700 SN: US342001770	e probability are given on the following pages totry facility: environment temperature (22 ± 3 ) Cal Date (Cartificate No.) 26-Mar-24 (No. 217-04036/04037) 28-Mar-24 (No. 217-04036) 05-Oct 23 (OCP-DAK3: 5.1249_Oct23) 05-Oct 23 (OCP-DAK3: 5.1249_Oct23) 28-Mar-24 (No. 217-04046) 23-Feb-24 (No. 217-04046) 23-Feb-24 (No. 217-04046) Check Date (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 06-Apr-16 (in house check Jun-24) 04-Aug-90 (in house check Jun-24) 31-Mar-14 (in house check Jun-24) Function	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Mar-25 Mar-25 Oct-24 Oct-24 Oct-24 Oct-24 Mar-25 Feb-25 Jun-25 Scheduled Check In house check: Jun-26 In house check: Jun-26

Certificate No: EX-7823\_Jul24

Page 1 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責。同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

```
www.sgs.com.tw
```



# Report No: TESA2410000648ES Page: 7 of 45

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

S

С

S

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\vartheta$	$\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta$ = 0 is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

 a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices – Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020. b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization ∂ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E<sup>2</sup>-field uncertainty inside TSL (see
- below ConvF). NORM(I)x,yz = NORMx,yz \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of
- · DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.
- · PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics Axi, yz; Bx, yz; Cx, yz; Cx, yz; VR, yz; A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- Calibration range expressed in hinks voltage across the diode. ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f < 800MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to *NORMx,y,z* \* *ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from +50 MHz to +100 MHz
- · Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance requi
- · Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: EX-7823\_Jul24

Page 2 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction form exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 8 of 45

#### EX3DV4 - SN:7823

July 31, 2024

### Parameters of Probe: EX3DV4 - SN:7823

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k = 2)
Norm $(\mu V/(V/m)^2)^A$	0.60	0.61	0.58	±10.1%
DCP (mV) B	107.6	106.0	107.1	±4.7%

### Calibration Results for Modulation Response

UID	Communication System Name		A dB	$dB\sqrt{\mu V}$	с	D dB	VR mV	Max dev.	Max Unc <sup>E</sup> k = 2				
0	CW	X	0.00	0.00	1.00	0.00	130.0	±1.6%	±4.7%				
		Y	0.00	0.00	1.00		133.8						
		Z	0.00	0.00	1.00		125.8						
10352	Pulse Waveform (200Hz, 10%)	X	1.38	60.00	6.14	10.00	60.0	±2.5%	±9.6%				
	1	Y	1.49	60.59	6.41		60.0						
		Z	1.72	61.48	6.81		60.0						
10353	Pulse Waveform (200Hz, 20%)	X	10.00	72.00	9.00	6.99	80.0	±2.3%	±9.6%				
		Y	0.81	60.00	4.96		80.0	1					
		Z	0.81	60.00	4.95		80.0	1					
10354	Pulse Waveform (200Hz, 40%)	X	0.16	138.07	0.23	3.98	95.0	±2.8%	±9.6%				
	, , , , , , , , , , , , , , , , , , ,	Y	22.00	72.00	7.00			1			95.0		
		Z	22.00	72.00	7.00		95.0						
10355	Pulse Waveform (200Hz, 60%)	Х	11.33	93.62	0.05	2.22	120.0 ±1.7%	±9.6%					
		Y	11.42	154.30	11.24		120.0						
		Z	9.72	86.24	0.07	1	120.0	1					
10387	QPSK Waveform, 1 MHz	X	0.65	66.31	14.06	1.00	150.0	±3.1%	±9.6%				
		Y	0.49	62.40	11.65	1	150.0						
		Z	0.59	66.20	14.31	1	150.0						
10388	QPSK Waveform, 10 MHz	X	1.47	67.44	14.78	0.00	150.0	±1.0%	±9.6%				
		Y	1.23	65.05	13.10		150.0						
		Z	1.45	67.94	14.87	1	150.0						
10396	64-QAM Waveform, 100 kHz	X	1.75	65.20	16.26	3.01	150.0	±0.8%	±9.6%				
		Y	1.66	64.00	15.53	1	150.0	1					
		Z	1.73	65.11	16.18		150.0						
10399	64-QAM Waveform, 40 MHz	Х	2.93	66.97	15.49	0.00	150.0	±1.5%	±9.6%				
		Y	2.76	66.09	14.89		150.0						
		Z	2.88	67.11	15.56		150.0						
10414	WLAN CCDF, 64-QAM, 40 MHz	X	3.90	66.50	15.55	0.00	150.0	±2.6%	±9.6%				
		Y	3.68	65.87	15.06		150.0						
		Z	3.79	66.60	15.54		150.0						

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6). <sup>1</sup> Uncertainty parameter uncertainty for maximum specified field strength. <sup>2</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX-7823\_Jul24

Page 3 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document dear and the contract and company's mining all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 9 of 45

#### EX3DV4 - SN:7823

July 31, 2024

### Parameters of Probe: EX3DV4 - SN:7823

#### Sensor Model Parameters

	C1 fF	C2 fF	α V <sup>-1</sup>	T1 ms V <sup>-2</sup>	T2 ms V <sup>-1</sup>	T3 ms	T4 V <sup>-2</sup>	T5 V <sup>-1</sup>	Т6
X	9.4	67.56	33.00	3.15	0.00	4.90	0.47	0.00	1.00
y	8.3	60.37	33.74	2.92	0.00	4.90	0.37	0.00	1.00
z	8.3	59.27	32.77	2.85	0.00	4.90	0.47	0.00	1.00

#### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle	29.5°
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Note: Measurement distance from surface can be increased to 3-4 mm for an Area Scan job.

Certificate No: EX-7823\_Jul24

Page 4 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document dear and the contracts are company's mining all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司

f (886-2) 2298-0488

www.sgs.com.tw



### Report No: TESA2410000648ES Page: 10 of 45

EX3DV4 - SN:7823

July 31, 2024

### Parameters of Probe: EX3DV4 - SN:7823

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity <sup>F</sup> (S/m)	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc <sup>H</sup> (k = 2)
750	41.9	0.89	9.75	8.90	9.05	0.35	1.27	±11.0%
835	41.5	0.90	9.60	8.76	8.90	0.35	1.27	±11.0%
900	41.5	0.97	9.36	8.55	8.68	0.35	1.27	±11.0%
1450	40.5	1.20	8.60	7.85	7.98	0.35	1.27	±11.0%
1750	40.1	1.37	8.34	7.61	7.73	0.36	1.27	±11.0%
1900	40.0	1.40	7.85	7.16	7.28	0.36	1.27	±11.0%
2000	40.0	1.40	7.81	7.13	7.24	0.36	1.27	±11.0%
2300	39.5	1.67	7.64	6.97	7.09	0.36	1.27	±11.0%
2450	39.2	1.80	7.29	6.66	6.76	0.36	1.27	±11.0%
2600	39.0	1.96	7.22	6.59	6.69	0.36	1.27	±11.0%
3300	38.2	2.71	6.83	6.23	6.33	0.37	1.27	±13.1%
3500	37.9	2.91	6.63	6.05	6.15	0.37	1.27	±13.1%
3700	37.7	3,12	6.55	5.98	6.08	0.37	1.27	±13.1%
3900	37.5	3.32	6.49	5.92	6.02	0.37	1.27	±13.1%
4100	37.2	3.53	6.44	5.88	5.98	0.37	1.27	±13.1%
4200	37.1	3.63	6.38	5.83	5.92	0.37	1.27	±13.1%
4400	36.9	3.84	6.24	5.70	5.79	0.37	1.27	±13.1%
4600	36.7	4.04	6.07	5.54	5.63	0.37	1.27	±13.1%
4800	36.4	4.25	5.99	5.46	5.55	0.38	1.27	±13.1%
4950	36.3	4.40	5.87	5.35	5.44	0.36	1.27	±13.1%
5250	35.9	4.71	5.57	5.08	5.16	0.33	1.27	±13.1%
5600	35.5	5.07	5.05	4.61	4.69	0.29	1.27	±13.1%
5750	35.4	5.22	5.19	4.74	4.81	0.28	1.27	±13.1%
5850	35.2	5.32	4.99	4.55	4.62	0.27	1.27	±13.1%

<sup>C</sup> Frequency validity above 300 MHz of ±100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ±50 MHz. The uncertainty is the RSS of the ComF suscentrality at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ±10, 25, 40, 50 and 70 MHz for ComF assessments at 30, 46, 128, 150 and 220 MHz respectively. Validity of ComF assessed at 13 MHz is 9–19 MHz. Above 5GHz frequency validity can be extended to ±110 MHz.
<sup>Th</sup> The probes are calibrated using lisuse simulating liquids (TSL) that deviate for a rand or by loss than ±5% from the target values (typically beter than +3%) and are valid for TSL with deviations of up to ±10% if SAR correction is applied.
<sup>A</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below ±2% for frequencies between 3–6 GHz at any distance larger than half the probe tip diameter from the boundary.
<sup>H</sup> The stated uncertainty is the total calibration uncertainty (*k* = 2) of Norm ConvF. This is equivalent to the uncertainty component with the symbol CF in Table 9 of IEC/IEEE 62209-1528-2020.

Certificate No: EX-7823\_Jul24

Page 5 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document dear and the contracts are company's mining all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 11 of 45

EX3DV4 - SN:7823

July 31, 2024

### Parameters of Probe: EX3DV4 - SN:7823

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity <sup>F</sup> (S/m)	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc <sup>H</sup> ( <i>k</i> = 2)
6500	34.5	6.07	5.34	4.87	4.95	0.20	1.27	±18.6%
7000	33.9	6.65	5.47	4.99	5.07	0.20	1.27	±18.6%

<sup>C</sup> Frequency validity at 6.5 GHz is -600(+700 MHz, and  $\pm$ 700 MHz at or above 7 GHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. <sup>E</sup> The probes are calibrated using tissue simulating liquids (TSL) that deviate for e and  $\sigma$  by less than  $\pm$ 10% from the target values (typically better than  $\pm$ 6%) and rare valid for TSL with deviations of up to  $\pm$ 1%. <sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than  $\pm$ 1% for frequencies between 6–10 GHz at any distance larger than half the probe tip diameter from the boundary.

and a function of proceeding the postment of contrast y (k = 2) of Norm-ConvF. This is equivalent to the uncertainty component with the symbol CF in Table 9 of IEC/IEEE 62209-1528:2020.

Certificate No: EX-7823\_Jul24

Page 6 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document dear and the contracts are company's mining all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.


SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號



Report No: TESA2410000648ES Page: 12 of 45

EX3DV4 - SN:7823

July 31, 2024

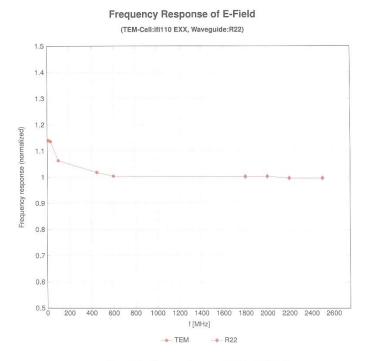



Certificate No: EX-7823 Jul24

Page 7 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.


```
www.sgs.com.tw
```



Report No: TESA2410000648ES Page: 13 of 45

EX3DV4 - SN:7823

July 31, 2024

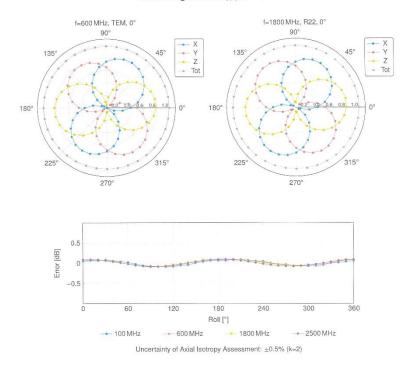

### Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

Certificate No: EX-7823 Jul24

Page 8 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sqs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.


f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 14 of 45

EX3DV4 - SN:7823

July 31, 2024

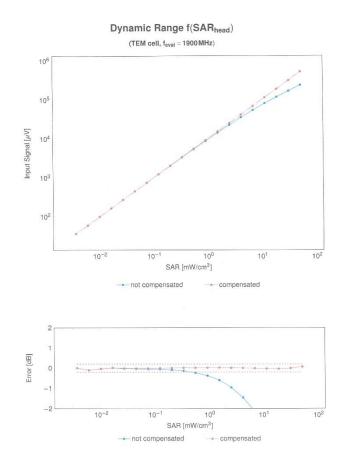

Uncertainty of Linearity Assessment: ±0.6% (k=2)

Certificate No: EX-7823\_Jul24

Page 9 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.


No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.

f (886-2) 2298-0488

www.sgs.com.tw



# Report No: TESA2410000648ES Page: 15 of 45

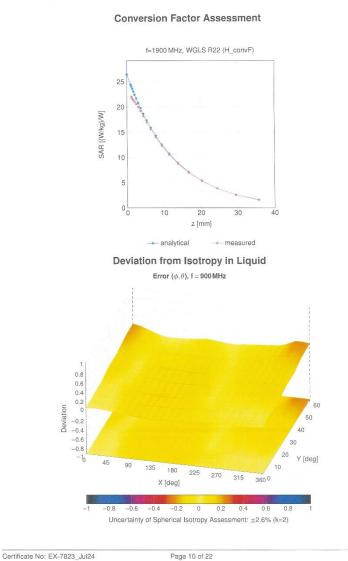

EX3DV4 - SN:7823

July 31, 2024

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號 SGS Taiwan Ltd.

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 16 of 45

EX3DV4 - SN:7823

July 31, 2024

### Appendix: Modulation Calibration Parameters

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
0		CW	CW	0.00	±4,7
0010	CAB	SAR Validation (Square, 100 ms, 10 ms)	Test	10.00	±9.6
0011	CAC	UMTS-FDD (WCDMA)	WCDMA	2.91	±9.6
0012	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	WLAN	1.87	<u>⊥</u> 9.6
0013	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps)	WLAN	9.46	±9.6
0021	DAC	GSM-FDD (TDMA, GMSK)	GSM	9.39	±9.6
10023	DAC	GPRS-FDD (TDMA, GMSK, TN 0)	GSM	9.57	±9.6
10.023	DAC	GPRS-FDD (TDMA, GMSK, TN 0-1)	GSM	6.56	±9.6
10024	DAC	EDGE-FDD (TDMA, 8PSK, TN 0)	GSM	12.62	±9.6
10025	DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1)	GSM	9.55	±9.6
10028	DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	GSM	4.80	+9.6
10027	DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	GSM	3.55	±9.6
	DAC	EDGE-FDD (TDMA, GMSK, TN 0-1-2-3)	GSM	7.78	±9.6
10029			Bluetooth	5.30	±9.6
10030	CAA	IEEE 802.15.1 Bluetooth (GFSK, DH1)	Bluetooth	1.87	+9.6
10031	CAA	IEEE 802.15.1 Bluetooth (GFSK, DH3)	Bluetooth	1.16	+9.6
10032	CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	Bluetooth	7.74	±9.6
10033	CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH1)		4.53	±9.6
10034	CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH3)	Bluetooth		
10035	CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH5)	Bluetooth	3.83	±9.6
10036	CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH1)	Bluetooth	8.01	±9.6
10037	CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH3)	Bluetooth	4.77	±9.6
10038	CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH5)	Bluetooth	4.10	±9.6
10039	CAB	CDMA2000 (1xRTT, RC1)	CDMA2000	4.57	±9.6
10042	CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Halfrate)	AMPS	7.78	±9.6
10044	CAA	IS-91/EIA/TIA-553 FDD (FDMA, FM)	AMPS	0.00	±9.6
10048	CAA	DECT (TDD, TDMA/FDM, GFSK, Full Slot, 24)	DECT	13.80	+9.6
10049	CAA	DECT (TDD, TDMA/FDM, GFSK, Double Slot, 12)	DECT	10.79	±9.6
10056	CAA	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	TD-SCDMA	11.01	±9.6
10058	DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	GSM	6.52	±9.6
10059	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps)	WLAN	2.12	±9.6
10060	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps)	WLAN	2.83	±9.6
10061	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	WLAN	3.60	+9.6
10062	CAE	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps)	WLAN	8.68	±9.6
10063	CAE	IEEE 802.11a/h WIFI 5 GHz (OFDM, 9 Mbps)	WLAN	8.63	±9.6
10064	CAE	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps)	WLAN	9.09	±9.6
10065	CAE	IEEE 802,11a/h WiFi 5 GHz (OFDM, 18 Mbps)	WLAN	9.00	±9.6
10066	CAE	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps)	WLAN	9.38	19.6
10067	CAE	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps)	WLAN	10.12	±9.6
10068	CAE	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps)	WLAN	10.24	±9.6
10069	CAE	IEEE 802.11a/h WiFI 5 GHz (OFDM, 54 Mbps)	WLAN	10.56	±9.6
10071	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)	WLAN	9.83	±9.6
10072	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	WLAN	9.62	±9.6
10073		IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 18 Mbps)	WLAN	9.94	±9.6
10073		IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 24 Mbps)	WLAN	10.30	19.6
10074		IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 36 Mbps)	WLAN	10.77	±9.6
10075		IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 38 Mbps)	WLAN	10.94	±9.6
10076		IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 46 Mbps)	WLAN	11.00	±9.6
10077	CAB	CDMA2000 (1xRTT, RC3)	CDMA2000	3.97	±9.6
10081		IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Fullrate)	AMPS	4,77	±9.6
10082		GPRS-FDD (TDMA, GMSK, TN 0-4)	GSM	6.56	±9.6
			WCDMA	3.98	±9.6
10097		UMTS-FDD (HSDPA)	WCDMA	3.98	±9.6 ±9.6
10098		UMTS-FDD (HSUPA, Subtest 2)		9.55	±9.6 ±9.6
10099		EDGE-FDD (TDMA, 8PSK, TN 0-4)	GSM	9.55	
10100		LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	LTE-FDD		±9.6
10101		LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	LTE-FDD	6.42	±9.6
10102		LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	LTE-FDD	6.60	±9.6
10103			LTE-TDD	9.29	±9.6
10104			LTE-TDD	9,97	±9.6
10105			LTE-TDD	10.01	±9.6
10108			LTE-FDD	5.80	±9.6
10109			LTE-FDD	6.43	±9.6
10110	CAH	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	LTE-FDD	5.75	±9.6
10111			LTE-FDD	6.44	±9.6

Certificate No: EX-7823 Jul24

Page 11 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document dear and the contracts are company's mining all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

```
www.sgs.com.tw
```



# Report No: TESA2410000648ES Page: 17 of 45

EX3DV4 - SN:7823

July 31, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
0112	CAH	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	LTE-FDD	6.59	±9.6
0113	CAH	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	LTE-FDD	6.62	±9.6
0114	CAE	IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	WLAN	8.10	±9.6
0115	CAE	IEEE 802,11n (HT Greenfield, 81 Mbps, 16-QAM)	WLAN	8.46	±9.6
0116	CAE	IEEE 802,11n (HT Greenfield, 135 Mbps, 64-QAM)	WLAN	8.15	±9.6
0117	CAE	IEEE 802,11n (HT Mixed, 13.5 Mbps, BPSK)	WLAN	8.07	±9.6
0118	CAE	IEEE 802.11n (HT Mixed, 81 Mbps, 16-QAM)	WLAN	8.59	±9.6
0119	CAE	IEEE 802.11n (HT Mixed, 135 Mbps, 64-QAM)	WLAN	8.13	±9.6
0140	CAF	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	6.49	±9.6
0140	CAF	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.53	±9.6
0142	CAF	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	LTE-FDD	5.73	±9.6
0142	CAF	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	LTE-FDD	6.35	±9.6
0143	CAF	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	LTE-FDD	6.65	±9.6
	CAG	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	LTE-FDD	5.76	±9.6
0145			LTE-FDD	6.41	±9.6
0146	CAG	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	LTE-FDD	6,72	+9.6
0147	CAG	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.42	±9.6
0149	CAF	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)			±9.6
0150	CAF	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	LTE-FDD	6.60	
0151	CAH	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	LTE-TDD	9.28	±9.6
0152	CAH	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	LTE-TDD	9.92	±9.6
0153	CAH	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	LTE-TDD	10.05	±9.6
0154	CAH	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	LTE-FDD	5.75	±9.6
0155	CAH	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	LTE-FDD	6.43	±9.6
0156	CAH	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	LTE-FDD	5.79	±9.6
0157	CAH	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	LTE-FDD	6.49	±9.6
0158	CAH	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	LTE-FDD	6.62	±9.6
0159	CAH	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	LTE-FDD	6.56	±9.6
0160	CAF	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	LTE-FDD	5.82	±9.6
0161	CAF	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	LTE-FDD	6,43	±9.6
0162	CAF	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	LTE-FDD	6.58	±9.6
10166	CAG	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	LTE-FDD	5.46	19.6
10167	CAG	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	LTE-FDD	6.21	+9.6
10168	CAG	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.79	±9.6
10169	CAF	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	LTE-FDD	5.73	±9.6
10170	CAF	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	LTE-FDD	6.52	±9.6
10170	AAF	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	LTE-FDD	6,49	+9.6
10171	CAH	LTE-TDD (SC-FDIMA, 1 RB, 20 MHz, QPSK)	LTE-TDD	9.21	+9.6
			LTE-TDD	9.21	±9.6
10173	CAH	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)		10.25	
10174	CAH	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	LTE-TDD		±9.6
10175	CAH	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	LTE-FDD	5.72	±9,6
10176	CAH	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	LTE-FDD	6.52	±9.6
10177	CAJ	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	LTE-FDD	5.73	±9.6
10178	CAH	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	LTE-FDD	6.52	±9.6
10179	CAH	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	LTE-FDD	6.50	±9.6
10180	CAH	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	LTE-FDD	6.50	±9.6
10181	CAF	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	LTE-FDD	5.72	±9.6
10182	CAF	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	LTE-FDD	6.52	±9.6
10183	AAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	LTE-FDD	6.50	+9.6
10184	CAF	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	LTE-FDD	5.73	±9.6
10185	CAF	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	LTE-FDD	6.51	±9.6
10186	AAF	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	LTE-FDD	6.50	±9.0
10187	CAG	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	LTE-FDD	5.73	±9.
10188		LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	LTE-FDD	6.52	±9.
10189		LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.50	±9.
10 193		IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	WLAN	8.09	±9,
10194		IEEE 802.11n (HT Greenfield, 39 Mbps, 16-QAM)	WLAN	8.12	±9.
10195		IEEE 802.11n (HT Greenfield, 65 Mbps, 64-QAM)	WLAN	8.21	±9.
10195		IEEE 802.11n (HT Mixed, 6.5 Mbps, 8PSK)	WLAN	8.10	±9.
10196		IEEE 802.11n (HT Mixed, 9.5 Mbps, br3K) IEEE 802.11n (HT Mixed, 39 Mbps, 16-QAM)	WLAN	8.13	±9.0 ±9.0
10197			WLAN	8.13	±9.0 ±9.0
		IEEE 802.11n (HT Mixed, 65 Mbps, 64-QAM)			
10219		IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)	WLAN	8.03	±9.0
10220		IEEE 802.11n (HT Mixed, 43.3 Mbps, 16-QAM)	WLAN	8.13	±9.
10221		IEEE 802.11n (HT Mixed, 72.2 Mbps, 64-QAM)	WLAN	8.27	±9.
10222		IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	WLAN	8.06	±9.
10223		IEEE 802.11n (HT Mixed, 90 Mbps, 16-QAM)	WLAN	8.48	±9.
10224	CAE	IEEE 802.11n (HT Mixed, 150 Mbps, 64-QAM)	WLAN	8.08	±9.

Certificate No: EX-7823 Jul24

Page 12 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責。同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 18 of 45

EX3DV4 - SN:7823

July 31, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
0225	CAC	UMTS-FDD (HSPA+)	WCDMA	5.97	±9.6
0226	CAC	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	LTE-TDD	9.49	±9.6
0227	CAC	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	LTE-TDD	10.26	±9.6
0228	CAC	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	LTE-TDD	9.22	±9.6
1229	CAE	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	LTE-TDD	9.48	±9.6
0230	CAE	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	LTE-TDD	10.25	±9.6
0231	CAE	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	LTE-TDD	9.19	±9.6
0232	CAH	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	LTE-TDD	9.48	±9.6
0233	CAH	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	LTE-TDD	10.25	±9.6
0234	CAH	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	LTE-TDD	9.21	±9.6
0234	CAH	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	LTE-TDD	9.48	±9.6
0235	CAH	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	LTE-TDD	10.25	+9.6
	CAH	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	LTE-TDD	9.21	±9.6
0237		LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	LTE-TDD	9.48	±9.6
0238	CAG	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 10-QAM) LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	LTE-TDD	10.25	±9.6
0239	CAG		LTE-TDD	9.21	±9.6
0240	CAG	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	LTE-TDD	9.82	±9.6
0241	CAC	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	LTE-TDD	9.86	±9.6
0242	CAC	LTE-TDD (SC-FDMA, 50% RB, 1,4 MHz, 64-QAM)		9.46	±9.6
0243	CAC	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	LTE-TDD		
0244	CAE	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	LTE-TDD	10.06	±9.6
0245	CAE	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	LTE-TDD	10.06	±9.6
0246	CAE	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	LTE-TDD	9.30	±9.6
0247	CAH	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	LTE-TDD	9.91	±9.6
0248	CAH	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	LTE-TDD	10.09	±9.6
0249	CAH	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	LTE-TDD	9.29	±9.6
0250	CAH	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	LTE-TDD	9.81	±9.6
0251	CAH	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	LTE-TDD	10.17	±9.6
0252	CAH	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	LTE-TDD	9.24	±9.6
0253	CAG	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	LTE-TDD	9.90	±9.6
0254	CAG	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	LTE-TDD	10.14	±9.6
0255	CAG	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	LTE-TDD	9.20	±9.6
0256	CAC	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	LTE-TDD	9.96	±9.6
0257	CAC	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-TDD	10.08	+9.6
10258	CAC	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	LTE-TDD	9.34	±9.6
0259	CAE	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	LTE-TDD	9.98	±9.6
10260	CAE	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	LTE-TDD	9.97	±9.6
10261	CAE	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	LTE-TDD	9.24	±9.6
10262	CAH	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	LTE-TDD	9.83	±9.6
10263	CAH	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	LTE-TDD	10.16	19.6
10264	CAH	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	LTE-TDD	9.23	+9.6
10265	CAH	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	LTE-TDD	9.92	±9.6
10266	CAH	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	LTE-TDD	10.07	±9.6
0267	CAH	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	LTE-TDD	9.30	±9.6
10268	CAG	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-TDD	10.06	±9.6
10269	CAG	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-TDD	10.13	±9.6
10209	CAG	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	LTE-TDD	9.58	±9.6
10270	CAG	UMTS-FDD (HSUPA, Subjest 5, 3GPP Rel8,10)	WCDMA	4.87	±9.6
10274	CAC	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10) UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	WCDMA	3.96	±9.6
			PHS	11.81	+9.6
10277	CAA	PHS (QPSK)	PHS	11.81	±9.6
10278	CAA	PHS (QPSK, BW 884 MHz, Rolloff 0.5)	PHS	12.18	±9.6 ±9.6
10279	CAA	PHS (QPSK, BW 884 MHz, Rolloff 0.38)		3.91	
10290	AAB	CDMA2000, RC1, SO55, Full Rate	CDMA2000		±9.4
10291	AAB	CDMA2000, RC3, SO55, Full Rate	CDMA2000	3.46	±9.
10292	AAB	CDMA2000, RC3, SO32, Full Rate	CDMA2000	3.39	±9.
10293	AAB	CDMA2000, RC3, SO3, Full Rate	CDMA2000	3.50	19.6
10295	AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	CDMA2000	12.49	±9.6
10297	AAE	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	LTE-FDD	5.81	±9.
10298	AAE	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	LTE-FDD	5.72	±9.1
10299		LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	LTE-FDD	6.39	±9.
10300		LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	LTE-FDD	6.60	±9.1
10301	AAA	IEEE 802,16e WIMAX (29:18, 5 ms, 10 MHz, QPSK, PUSC)	WiMAX	12.03	±9.
10302	AAA	IEEE 802.16e WIMAX (29:18, 5 ms, 10 MHz, QPSK, PUSC, 3 CTRL symbols)	WiMAX	12.57	±9.
10303	AAA	IEEE 802.16e WIMAX (31:15, 5 ms, 10 MHz, 64QAM, PUSC)	WIMAX	12.52	±9.
10304		IEEE 802.16e WIMAX (29:18, 5 ms, 10 MHz, 64QAM, PUSC)	WiMAX	11.86	±9.
10305		IEEE 802.16e WIMAX (31:15, 10 ms, 10 MHz, 64QAM, PUSC, 15 symbols)	WiMAX	15.24	±9.
10306		IEEE 802.16e WIMAX (29:18. 10 ms, 10 MHz, 64QAM, PUSC, 18 symbols)	WiMAX	14.67	±9.

Certificate No: EX-7823 Jul24

Page 13 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責。同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 19 of 45

EX3DV4 - SN:7823

July 31, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
0307	AAA	IEEE 802.16e WIMAX (29:18, 10 ms, 10 MHz, QPSK, PUSC, 18 symbols)	WiMAX	14.49	±9.6
0308	AAA	IEEE 802,16e WIMAX (29:18, 10 ms, 10 MHz, 16QAM, PUSC)	WIMAX	14.46	±9.6
0309	AAA	IEEE 802.16e WIMAX (29:18, 10 ms, 10 MHz, 16QAM, AMC 2x3, 18 symbols)	WIMAX	14.58	±9.6
0310	AAA	IEEE 802.16e WiMAX (29:18, 10 ms, 10 MHz, QPSK, AMC 2x3, 18 symbols)	WIMAX	14,57	±9.6
0310	AAA	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	LTE-FDD	6.06	±9.6
		IDEN 1:3	IDEN	10.51	±9.6
0313	AAA		IDEN	13.48	±9.6
0314	AAA	IDEN 1:6	WLAN	1,71	±9.6
0315	AAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle)		8.36	±9.6
0316	AAB	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 96pc duty cycle)	WLAN	0100	
0317	AAE	IEEE 802.11a WIFI 5 GHz (OFDM, 6 Mbps, 96pc duty cycle)	WLAN	8.36	±9.6
0352	AAA	Pulse Waveform (200Hz, 10%)	Generic	10.00	±9.6
0353	AAA	Pulse Waveform (200Hz, 20%)	Generic	6.99	±9.6
0354	AAA	Pulse Waveform (200Hz, 40%)	Generic	3.98	±9.6
0355	AAA	Pulse Waveform (200Hz, 60%)	Generic	2.22	±9.6
0356	AAA	Pulse Waveform (200Hz, 80%)	Generic	0.97	±9.6
0387	AAA	QPSK Waveform, 1 MHz	Generic	5.10	±9.6
0388	AAA	QPSK Waveform, 10 MHz	Generic	5,22	±9.6
0396	AAA	64-QAM Waveform, 100 kHz	Generic	6,27	+9.6
0399	AAA	64-QAM Waveform, 40 MHz	Generic	6,27	±9.6
0 4 0 0	AAF	IEEE 802.11ac WiFi (20 MHz, 64-QAM, 99pc duty cycle)	WLAN	8.37	19.6
0400	AAF	IEEE 802.11ac WiFi (20 MHz, 64-QAM, 99pc duty cycle)	WLAN	8.60	+9.6
		IEEE 802.11ac WIFI (40 MHz, 64-QAM, 99pc duty cycle) IEEE 802.11ac WIFI (80 MHz, 64-QAM, 99pc duty cycle)	WLAN	8,53	±9.6
0402	AAF		CDMA2000	3.76	±9.6
0403	AAB	CDMA2000 (1xEV-DO, Rev. 0)	CDMA2000	3.76	=9.6
0404	AAB	CDMA2000 (1xEV-DO, Rev. A)			
0406	AAB	CDMA2000, RC3, SO32, SCH0, Full Rate	CDMA2000	5.22	±9.6
0410	AAH	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9, Subframe Conf=4)	LTE-TDD	7.82	±9.6
0414	AAA	WLAN CCDF, 64-QAM, 40 MHz	Generic	8.54	±9.6
0415	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	WLAN	1.54	±9.6
0416	AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	WLAN	8.23	+9.6
0417	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	WLAN	8.23	±9.6
0418	AAA	IEEE 802,11g WiFi 2,4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preambule)	WLAN	8.14	±9.6
0419	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Short preambule)	WLAN	8.19	±9.6
0422	AAD	IEEE 802.11n (HT Greenfield, 7.2 Mbps, BPSK)	WLAN	8.32	±9.6
0423	AAD	IEEE 802.11n (HT Greenfield, 43.3 Mbps, 16-QAM)	WLAN	8.47	±9.6
10424	AAD	IEEE 802.11n (HT Greenfield, 72.2 Mbps, 64-QAM)	WLAN	8.40	19.6
10425	AAD	IEEE 802.11n (HT Greenfield, 15 Mbps, BPSK)	WLAN	8.41	+9.6
10425	AAD	IEEE 802.11n (HT Greenfield, 90 Mbps, 16-QAM)	WLAN	8,45	±9.6
			WLAN	8.41	±9.6
10427	AAD	IEEE 802,11n (HT Greenfield, 150 Mbps, 64-QAM)		8.28	±9.6
10430	AAE	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1)	LTE-FDD		
10431	AAE	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1)	LTE-FDD	8.38	±9.6
10432	AAD	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1)	LTE-FDD	8.34	±9.6
10433	AAD	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1)	LTE-FDD	8.34	±9.0
10434	AAB	W-CDMA (BS Test Model 1, 64 DPCH)	WCDMA	8.60	±9.0
10435	AAG	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.82	±9.
10447	AAE	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	LTE-FDD	7.56	±9.0
10448	AAE	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1, Clippin 44%)	LTE-FDD	7.53	±9.
10449	AAD	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1, Cliping 44%)	LTE-FDD	7.51	±9.
10450	AAD	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	LTE-FDD	7.48	±9.
10451	AAB	W-CDMA (BS Test Model 1, 64 DPCH, Clipping 44%)	WCDMA	7.59	±9.
10453	AAE	Validation (Square, 10ms, 1 ms)	Test	10.00	±9.
10455	AAD	IEEE 802,11ac WiFi (160 MHz, 64-QAM, 99pc duty cycle)	WLAN	8.63	±9.
10456	AAB	UMTS-FDD (DC-HSDPA)	WCDMA	6.62	±9.
	12.000		CDMA2000	6.55	±9.
10458	AAA	CDMA2000 (1xEV-DO, Rev. B, 2 carriers)	CDMA2000	8.25	±9.
10459		CDMA2000 (1xEV-DO, Rev. B, 3 carriers)			
10460	AAB	UMTS-FDD (WCDMA, AMR)	WCDMA	2.39	±9.
10461	AAC	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.82	±9.
10462		LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2.3,4,7,8,9)	LTE-TDD	8.30	±9.
10463		LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.56	±9.
10464	AAD	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.82	±9.
10465	AAD	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.32	±9.
10466	AAD	LTE-TDD (SC-FDMA, 1 RB. 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.57	±9.
10467		LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.82	±9.
10468		LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.32	±9.
10469			LTE-TDD	8.56	±9.
10409		LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM, 0L Subframe=2,3,4,7,6,9) LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7,82	±9.
10470					

Certificate No: EX-7823 Jul24

Page 14 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責。同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 20 of 45

EX3DV4 - SN:7823

July 31, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
0472	AAG	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.57	±9.6
0473	AAF	LTE-TDD (SC-FDMA, 1 RB, 15MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.82	±9.6
0473	AAF	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.32	±9.6
		LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.57	±9.6
0475	AAF		LTE-TDD	8.32	±9.6
0477	AAG	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.57	±9.6
0478	AAG	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)		7.74	±9.6
0479	AAC	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD		
0480	AAC	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.18	±9.6
0481	AAC	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7.8,9)	LTE-TDD	8.45	±9.6
0482	AAD	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL Subframe=2.3,4,7.8,9)	LTE-TDD	7.71	±9.6
0483	AAD	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8.9)	LTE-TDD	8.39	±9.6
0484	AAD	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.47	±9.6
0485	AAG	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.59	±9.6
0486	AAG	LTE-TDD (SC-FDMA, 50% RB, 5MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.38	±9.6
0487	AAG	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.60	±9.6
		LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.70	±9.6
0488	AAG	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8.9)	LTE-TDD	8,31	±9.6
0489	AAG		LTE-TDD	8.54	±9.6
0490	AAG	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)			
0491	AAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7,74	±9.6
0492	AAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.41	±9.6
0493	AAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM, UL Subframe=2,3.4,7.8,9)	LTE-TDD	8.55	±9.6
0494	AAG	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.74	±9.6
0495	AAG	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM, UL Subframe=2.3,4,7,8.9)	LTE-TDD	8.37	±9.6
0496	AAG	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.54	±9.6
0497	AAC	LTE-TDD (SC-FDMA, 100% RB, 1,4 MHz, QPSK, UL Subframe=2.3,4,7,8,9)	LTE-TDD	7.67	±9.6
0498	AAC	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.40	±9.6
0499	AAC	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.68	±9.6
		LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.67	+9.6
0500	AAD	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 0F3K, 0L Subiranie=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.44	+9.6
0501	AAD			8.52	±9.6
0502	AAD	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD		
0503	AAG	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.72	±9.6
0504	AAG	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.31	±9.6
10505	AAG	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.54	±9.6
0506	AAG	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8.9)	LTE-TDD	7.74	±9.6
0507	AAG	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL Subframe=2.3,4.7,8,9)	LTE-TDD	8.36	±9.6
0508	AAG	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.55	±9.6
0509	AAF	LTE-TDD (SC-FDMA, 100% RB, 15MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.99	±9.6
10510	AAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.49	±9.6
10511	AAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL Subframe=2.3,4.7,8.9)	LTE-TDD	8.51	±9.6
10512	AAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2.3,4,7,8.9)	LTE-TDD	7,74	±9.6
10512	AAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.42	±9.6
		LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.45	±9.6
10514	AAG		WLAN	1.58	+9.6
10515	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)			
10516	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 99pc duty cycle)	WLAN	1.57	±9.6
10517	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 99pc duty cycle)	WLAN	1.58	±9.6
10518		IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 99pc duty cycle)	WLAN	8.23	±9.6
10519		IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 99pc duty cycle)	WLAN	8.39	±9.6
10520	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 99pc duty cycle)	WLAN	8.12	±9.6
10521	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 99pc duty cycle)	WLAN	7.97	±9.6
10522	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 99pc duty cycle)	WLAN	8.45	±9.6
10523		IEEE 802,11a/h WiFi 5 GHz (OFDM, 48 Mbps, 99pc duty cycle)	WLAN	8.08	±9.6
10524		IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 99pc duty cycle)	WLAN	8.27	1.9.6
10525		IEEE 802.11ac WiFi (20 MHz, MCS0, 99pc duty cycle)	WLAN	8.36	19.6
10525		IEEE 802.11ac WiFi (20 MHz, MC30, 99pc duty cycle)	WLAN	8.42	±9.
10526		IEEE 802.11ac WiFI (20 MHz, MCS1, 99pc duty cycle)	WLAN	8.21	±9.0
			WLAN	8.36	±9.4
10528		IEEE 802.11ac WiFi (20 MHz, MCS3, 99pc duty cycle)			
10529		IEEE 802.11ac WiFi (20 MHz, MCS4, 99pc duty cycle)	WLAN	8.36	±9.1
10531	-	IEEE 802.11ac WiFi (20 MHz, MCS6, 99pc duty cycle)	WLAN	8.43	±9.6
10532	AAD	IEEE 802.11ac WiFi (20 MHz, MCS7, 99pc duty cycle)	WLAN	8.29	±9.6
10533	AAD	IEEE 802.11ac WiFi (20 MHz, MCS8, 99pc duty cycle)	WLAN	8.38	±9.
10534	AAD	IEEE 802.11ac WiFi (40 MHz, MCS0, 99pc duty cycle)	WLAN	8.45	±9.6
10535		IEEE 802.11ac WiFi (40 MHz, MCS1, 99pc duty cycle)	WLAN	8.45	±9.1
10536		IEEE 802.11ac WIFI (40 MHz, MCS2, 99pc duty cycle)	WLAN	8.32	±9.1
		IEEE 802.11ac WiFi (40 MHz, MCS3, 99pc duty cycle)	WLAN	8.44	+9.
10527		here over the third to be in the model, only only of the			
10537		IEEE 802,11ac WiFi (40 MHz, MCS4, 99pc duty cycle)	WLAN	8.54	±9.

Certificate No: EX-7823 Jul24

Page 15 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 21 of 45

EX3DV4 - SN:7823

July 31, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
10541	AAD	IEEE 802.11ac WiFi (40 MHz, MCS7, 99pc duty cycle)	WLAN	8.46	±9.6
0542	AAD	IEEE 802,11ac WiFi (40 MHz, MCS8, 99pc duty cycle)	WLAN	8.65	±9.6
0543	AAD	IEEE 802.11ac WiFi (40 MHz, MCS9, 99pc duty cycle)	WLAN	8.65	±9.6
0544	AAD	IEEE 802,11ac WiFi (80 MHz, MCS0, 99pc duty cycle)	WLAN	8.47	±9.6
0545	AAD	IEEE 802,11ac WiFi (80 MHz, MCS1, 99pc duty cycle)	WLAN	8.55	±9.6
	AAD	IEEE 802,11ac WiFi (80 MHz, MCS2, 99pc duty cycle)	WLAN	8.35	±9.6
0546	AAD	IEEE 802,11ac WiFI (80 MHz, MCS3, 99pc duty cycle)	WLAN	8.49	±9.6
0547		IEEE 802.11ac WIFI (80 MHz, MCS3, 99pc duty cycle)	WLAN	8.37	±9.6
0548	AAD		WLAN	8.38	±9.6
0550	AAD	IEEE 802.11ac WiFi (80 MHz, MCS6, 99pc duty cycle)	WLAN	8.50	±9.6
0551	AAD	IEEE 802.11ac WiFi (80 MHz, MCS7, 99pc duty cycle)		8.42	±9.6
0552	AAD	IEEE 802.11ac WiFi (80 MHz, MCS8, 99pc duty cycle)	WLAN		
0553	AAD	IEEE 802.11 ac WiFi (80 MHz, MCS9, 99pc duty cycle)	WLAN	8.45	±9.6
0554	AAE	IEEE 802.11ac WiFi (160 MHz, MCS0, 99pc duty cycle)	WLAN	8.48	±9.6
0555	AAE	IEEE 802.11ac WiFi (160 MHz, MCS1, 99pc duty cycle)	WLAN	8.47	±9,6
0556	AAE	IEEE 802.11ac WiFi (160 MHz, MCS2, 99pc duty cycle)	WLAN	8.50	±9.6
0557	AAE	IEEE 802.11ac WiFi (160 MHz, MCS3, 99pc duty cycle)	WLAN	8.52	±9.6
0558	AAE	IEEE 802.11ac WiFi (160 MHz, MCS4, 99pc duty cycle)	WLAN	8.61	±9,6
0560	AAE	IEEE 802.11ac WIFi (160 MHz, MCS6, 99pc duty cycle)	WLAN	8.73	±9.6
0561	AAE	IEEE 802,11ac WiFi (160 MHz, MCS7, 99pc duty cycle)	WLAN	8.56	±9.6
0562	AAE	IEEE 802.11ac WiFi (160 MHz, MCS8, 99pc duty cycle)	WLAN	8.69	±9.6
0563	AAE	IEEE 802,11ac WiFi (160 MHz, MCS9, 99pc duty cycle)	WLAN	8.77	±9.6
0564	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty cycle)	WLAN	8.25	±9.6
0565	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 99pc duty cycle)	WLAN	8.45	±9.6
0566	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 99pc duty cycle)	WLAN	8.13	±9.6
0567	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 10 Mips, 35pc duty cycle)	WLAN	8.00	+9.6
		IEEE 802.11g WiFi 2.4 GHz (DSSS-OF DM, 24 Mbps, 99pc duty cycle)	WLAN	8.37	±9.6
10568	AAA		WLAN	8.10	±9,6
10569	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 99pc duty cycle)		Colore Colorest and	±9.6
10570	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 99pc duty cycle)	WLAN	8.30	
10571	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	WLAN	1.99	±9.6
10572	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	WLAN	1,99	+9.6
10573	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 90pc duty cycle)	WLAN	1.98	±9.6
10574	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 90pc duty cycle)	WLAN	1.98	±9.6
10575	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	WLAN	8.59	±9.6
10576	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	WLAN	8.60	±9.6
10577	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 90pc duty cycle)	WLAN	8.70	±9.6
10578	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 90pc duty cycle)	WLAN	8.49	±9.6
10579	AAA	IEEE 802.11g WIFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 90pc duty cycle)	WLAN	8.36	+9.6
10580	AAA	IEEE 802,11g WiFi 2,4 GHz (DSSS-OFDM, 36 Mbps, 90pc duty cycle)	WLAN	8.76	±9.6
10581	AAA	IEEE 802,11g WiFi 2,4 GHz (DSSS-OFDM, 48 Mbps, 90pc duty cycle)	WLAN	8.35	±9.6
10582	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 90pc duty cycle)	WLAN	8.67	±9.6
10583	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	WLAN	8.59	±9.6
10584	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)	WLAN	8.60	±9.6
10585	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 3 Mbps, 90pc duty cycle)	WLAN	8,70	+9.6
		IEEE 802.11a/h WIFI 5 GHz (OFDM, 12 Mbps, 90pc duty cycle)	WLAN	8.49	±9.6
10586	AAD			8.36	±9.6
10587	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 90pc duty cycle)	WLAN		
10588	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 90pc duty cycle)	WLAN	8.76	±9.0
10589	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 90pc duty cycle)	WLAN	8.35	±9.1
10590	AAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 90pc duty cycle)	WLAN	8.67	±9.0
10591	AAD	IEEE 802.11n (HT Mixed, 20 MHz, MCS0, 90pc duty cycle)	WLAN	8.63	±9.1
10592	AAD	IEEE 802,11n (HT Mixed, 20 MHz, MCS1, 90pc duty cycle)	WLAN	8.79	±9.
10593	AAD	IEEE 802.11n (HT Mixed, 20 MHz, MCS2, 90pc duty cycle)	WLAN	8.64	±9.
10594	AAD	IEEE 802.11n (HT Mixed, 20 MHz, MCS3, 90pc duty cycle)	WLAN	8.74	±9.
10595	AAD	IEEE 802.11n (HT Mixed, 20 MHz, MCS4, 90pc duty cycle)	WLAN	8.74	±9.
10596	AAD	IEEE 802.11n (HT Mixed, 20 MHz, MCS5, 90pc duty cycle)	WLAN	8.71	±9.
10597	AAD	IEEE 802.11n (HT Mixed, 20 MHz, MCS6, 90pc duty cycle)	WLAN	8.72	±9.
10598	-	IEEE 802.11n (HT Mixed, 20 MHz, MCS7, 90pc duty cycle)	WLAN	8.50	±9.
10599	AAD	IEEE 802.11n (HT Mixed, 40 MHz, MCS0, 90pc duty cycle)	WLAN	8.79	±9.
10600		IEEE 802.11n (HT Mixed, 40 MHz, MCS1, 90pc duty cycle)	WLAN	8.88	±9.
10600	AAD	IEEE 802.11n (HT Mixed, 40 MHz, MCS1, 90pc duty cycle)	WLAN	8.82	±9.
10601		IEEE 802.11n (H1 Mixed, 40 MHz, MCS2, 90pc duty cycle) IEEE 802.11n (HT Mixed, 40 MHz, MCS3, 90pc duty cycle)	WLAN	8,94	±9. ±9.
				9.03	
10603	AAD	IEEE 802.11n (HT Mixed, 40 MHz, MCS4, 90pc duty cycle)	WLAN		±9.
10604		IEEE 802.11n (HT Mixed, 40 MHz, MCS5, 90pc duty cycle)	WLAN	8.76	±9.
10605	AAD	IEEE 802.11n (HT Mixed, 40 MHz, MCS6, 90pc duty cycle)	WLAN	8.97	±9.
10606		IEEE 802.11n (HT Mixed, 40 MHz, MCS7, 90pc duty cycle)	WLAN	8.82	±9.
10607	AAD	IEEE 802.11ac WiFi (20 MHz, MCS0, 90pc duty cycle)	WLAN	8.64	+9.
10608	AAD	IEEE 802.11ac WiFi (20 MHz, MCS1, 90pc duty cycle)	WLAN	8,77	±9.

Certificate No: EX-7823 Jul24

Page 16 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

www.sgs.com.tw



# Report No: TESA2410000648ES Page: 22 of 45

EX3DV4 - SN:7823

July 31, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
10609	AAD	IEEE 802.11ac WiFi (20 MHz, MCS2, 90pc duty cycle)	WLAN	8.57	±9.6
	AAD	IEEE 802.11ac WiFi (20 MHz, MCS3, 90pc duty cycle)	WLAN	8.78	±9.6
0610			WLAN	8.70	±9.6
0611	AAD	IEEE 802.11ac WiFi (20 MHz, MCS4, 90pc duty cycle)	WLAN	8.77	±9.6
0612	AAD	IEEE 802.11ac WiFi (20 MHz, MCS5, 90pc duty cycle)		8.94	
0613	AAD	IEEE 802.11ac WiFi (20 MHz, MCS6, 90pc duty cycle)	WLAN		±9.6
0614	AAD	IEEE 802.11ac WiFi (20 MHz, MCS7, 90pc duty cycle)	WLAN	8.59	±9.6
0615	AAD	IEEE 802.11ac WiFi (20 MHz, MCS8, 90pc duty cycle)	WLAN	8.82	±9.6
0616	AAD	IEEE 802.11ac WiFi (40 MHz, MCS0, 90pc duty cycle)	WLAN	8.82	±9.6
0617	AAD	IEEE 802.11ac WiFi (40 MHz, MCS1, 90pc duty cycle)	WLAN	8.81	±9.6
0618	AAD	IEEE 802.11ac WiFi (40 MHz, MCS2, 90pc duty cycle)	WLAN	8.58	±9.6
0619	AAD	IEEE 802.11ac WiFi (40 MHz, MCS3, 90pc duty cycle)	WLAN	8.86	±9.6
			WLAN	8.87	±9.6
0620	AAD	IEEE 802.11ac WiFi (40 MHz, MCS4, 90pc duty cycle)	WLAN	8.77	+9.6
0621	AAD	IEEE 802.11ac WiFi (40 MHz, MCS5, 90pc duty cycle)			
0622	AAD	IEEE 802.11ac WiFi (40 MHz, MCS6, 90pc duty cycle)	WLAN	8.68	±9.6
0623	AAD	IEEE 802.11ac WiFi (40 MHz, MCS7, 90pc duty cycle)	WLAN	8.82	±9.6
0624	AAD	IEEE 802.11ac WiFi (40 MHz, MCS8, 90pc duty cycle)	WLAN	8.96	±9.6
0 6 2 5	AAD	IEEE 802,11ac WiFi (40 MHz, MCS9, 90pc duty cycle)	WLAN	8,96	±9.6
0626	AAD	IEEE 802,11 ac WiFi (80 MHz, MCS0, 90pc duty cycle)	WLAN	8.83	±9.6
0627	AAD	IEEE 802.11ac WiFi (80 MHz, MCS1, 90pc duty cycle)	WLAN	8.88	±9.6
			WLAN	8.71	±9.6
0628	AAD	IEEE 802.11ac WiFi (80 MHz, MCS2, 90pc duty cycle)		8.85	±9.6
0629	AAD	IEEE 802.11ac WiFi (80 MHz, MCS3, 90pc duty cycle)	WLAN	0100	
0630	AAD	IEEE 802.11ac WIFI (80 MHz, MCS4, 90pc duty cycle)	WLAN	8.72	±9.6
0631	AAD	IEEE 802.11ac WiFi (80 MHz, MCS5, 90pc duty cycle)	WLAN	8.81	±9.6
0632	AAD	IEEE 802.11ac WiFi (80 MHz, MCS6, 90pc duty cycle)	WLAN	8.74	±9.6
0633	AAD	IEEE 802.11ac WiFi (80 MHz, MCS7, 90pc duty cycle)	WLAN	8.83	±9.6
0634	AAD	IEEE 802.11ac WiFi (80 MHz, MCS8, 90pc duty cycle)	WLAN	8.80	±9.6
10635	AAD	IEEE 802.11ac WiFi (80 MHz, MCS9, 90pc duty cycle)	WLAN	8.81	±9.6
	AAE		WLAN	8,83	±9.6
10636		IEEE 802.11ac WiFi (160 MHz, MCS0, 90pc duty cycle)		8.79	
10637	AAE	IEEE 802.11ac WiFi (160 MHz, MCS1, 90pc duty cycle)	WLAN		±9.6
0638	AAE	IEEE 802.11ac WiFi (160 MHz, MCS2, 90pc duty cycle)	WLAN	8.86	±9.6
0639	AAE	IEEE 802.11ac WiFi (160 MHz, MCS3, 90pc duty cycle)	WLAN	8.85	+9.6
10640	AAE	IEEE 802.11ac WiFi (160 MHz, MCS4, 90pc duty cycle)	WLAN	8.98	±9.6
10641	AAE	IEEE 802.11ac WiFi (160 MHz, MCS5, 90pc duty cycle)	WLAN	9.06	±9.6
10642	AAE	IEEE 802.11ac WiFi (160 MHz, MCS6, 90pc duty cycle)	WLAN	9.06	±9.6
10643	AAE	IEEE 802.11ac WiFi (160 MHz, MCS7, 90pc duty cycle)	WLAN	8.89	±9.6
			WLAN	9.05	19.6
10644	AAE	IEEE 802.11ac WiFi (160 MHz, MCS8, 90pc duty cycle)		0.55.5	
10645	AAE	IEEE 802,11ac WiFi (160 MHz, MCS9, 90pc duty cycle)	WLAN	9.11	±9.6
10646	AAH	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,7)	LTE-TDD	11.96	±9.6
10647	AAG	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,7)	LTE-TDD	11.96	±9.6
10648	AAA	CDMA2000 (1x Advanced)	CDMA2000	3.45	±9.6
10652	AAF	LTE-TDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	LTE-TDD	6.91	±9.6
10653	AAF	LTE-TDD (OFDMA, 10 MHz, E-TM 3.1, Clipping 44%)	LTE-TDD	7.42	±9.6
10654	AAE	LTE-TDD (OFDMA, 15 MHz, E-TM 3.1, Clipping 44%)	LTE-TDD	6.96	±9.6
	AAF		LTE-TDD	7.21	+9.6
10655		LTE-TDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)		10.00	
10658	AAB	Pulse Waveform (200Hz, 10%)	Test		±9.6
10659	AAB	Pulse Waveform (200Hz, 20%)	Test	6.99	±9.6
10660	AAB	Pulse Waveform (200Hz, 40%)	Test	3.98	±9.6
10661	AAB	Pulse Waveform (200Hz, 60%)	Test	2.22	±9.6
10662	AAB	Pulse Waveform (200Hz, 80%)	Test	0.97	±9.6
10670	AAA	Bluetooth Low Energy	Bluetooth	2.19	+9.6
10671	AAC	IEEE 802.11ax (20 MHz, MCS0, 90pc duty cycle)	WLAN	9.09	±9.6
10672	AAC	IEEE 802,11ax (20 MHz, MCS0, solid duty cycle)	WLAN	8.57	±9.6
			WLAN	8.78	
10673	AAC	IEEE 802.11ax (20 MHz, MCS2, 90pc duty cycle)			±9.6
10674	AAC	IEEE 802.11ax (20 MHz, MCS3, 90pc duty cycle)	WLAN	8.74	±9.6
10675	AAC	IEEE 802.11ax (20 MHz, MCS4, 90pc duty cycle)	WLAN	8.90	±9.6
10676	AAC	IEEE 802.11ax (20 MHz, MCS5, 90pc duty cycle)	WLAN	8.77	±9.6
10677	AAC	IEEE 802.11ax (20 MHz, MCS6, 90pc duty cycle)	WLAN	8.73	±9.6
10678	AAC	IEEE 802.11ax (20 MHz, MCS7, 90pc duty cycle)	WLAN	8.78	±9.6
10679		IEEE 802.11ax (20 MHz, MCS8, 90pc duty cycle)	WLAN	8.89	±9.6
10680		IEEE 802.11ax (20 MHz, MCS8, 90pc duty cycle)	WLAN	8.80	+9.6
			WLAN	8.62	±9.0
10681	AAC	IEEE 802.11ax (20 MHz, MCS10, 90pc duty cycle)			
10682	AAC	IEEE 802.11ax (20 MHz, MCS11, 90pc duty cycle)	WLAN	8.83	±9.6
10683	AAC	IEEE 802.11ax (20 MHz, MCS0, 99pc duty cycle)	WLAN	8.42	±9.6
10684	AAC	IEEE 802.11ax (20 MHz, MCS1, 99pc duty cycle)	WLAN	8.26	±9.
10685	AAC	IEEE 802.11ax (20 MHz, MCS2, 99pc duty cycle)	WLAN	8.33	±9.0
		IEEE 802.11ax (20 MHz, MCS3, 99pc duty cycle)	WLAN	8.28	±9.

Certificate No: EX-7823 Jul24

Page 17 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 23 of 45

EX3DV4 - SN:7823

July 31, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
0687	AAC	IEEE 802.11ax (20 MHz, MCS4, 99pc duty cycle)	WLAN	8.45	±9.6
0688	AAC	IEEE 802,11ax (20 MHz, MCS5, 99pc duty cycle)	WLAN	8.29	±9.6
		IEEE 802.11ax (20 MHz, MCS6, 99pc duty cycle)	WLAN	8.55	±9.6
0689	AAC		WLAN	8.29	±9.6
0690	AAC	IEEE 802.11ax (20 MHz, MCS7, 99pc duty cycle)	WLAN	8.25	±9.6
0691	AAC	IEEE 802.11ax (20 MHz, MCS8, 99pc duty cycle)	WLAN	8.29	±9.6
0692	AAC	IEEE 802.11ax (20 MHz, MCS9, 99pc duty cycle)		0100	
0693	AAC	IEEE 802.11ax (20 MHz, MCS10, 99pc duty cycle)	WLAN	8.25	±9.6
0694	AAC	IEEE 802.11ax (20 MHz, MCS11, 99pc duty cycle)	WLAN	8.57	±9.6
0695	AAC	IEEE 802.11ax (40 MHz, MCS0, 90pc duty cycle)	WLAN	8.78	±9.6
0696	AAC	IEEE 802.11ax (40 MHz, MCS1, 90pc duty cycle)	WLAN	8.91	±9.6
)697	AAC	IEEE 802.11ax (40 MHz, MCS2, 90pc duty cycle)	WLAN	8.61	±9.6
0698	AAC	IEEE 802.11ax (40 MHz, MCS3, 90pc duty cycle)	WLAN	8.89	±9.6
		IEEE 802.11ax (40 MHz, MCS4, 90pc duty cycle)	WLAN	8.82	±9.6
0699	AAC		WLAN	8.73	±9.6
0700	AAC	IEEE 802.11ax (40 MHz, MCS5, 90pc duty cycle)		8.86	±9.6
0701	AAC	IEEE 802.11ax (40 MHz, MCS6, 90pc duty cycle)	WLAN		
0702	AAC	IEEE 802.11ax (40 MHz, MCS7, 90pc duty cycle)	WLAN	8.70	±9.6
0703	AAC	IEEE 802,11ax (40 MHz, MCS8, 90pc duty cycle)	WLAN	8.82	±9.6
0704	AAC	IEEE 802.11ax (40 MHz, MCS9, 90pc duty cycle)	WLAN	8.56	±9.6
0705	AAC	IEEE 802.11ax (40 MHz, MCS10, 90pc duty cycle)	WLAN	8.69	±9.6
0706	AAC	IEEE 802.11ax (40 MHz, MCS11, 90pc duty cycle)	WLAN	8.66	±9.6
0707	AAC	IEEE 802.11ax (40 MHz, MCS0. 99pc duty cycle)	WLAN	8.32	±9.6
			WLAN	8.55	+9.6
0708	AAC	IEEE 802.11ax (40 MHz, MCS1, 99pc duty cycle)		8.33	±9.6
0709	AAC	IEEE 802.11ax (40 MHz, MCS2, 99pc duty cycle)	WLAN		
0710	AAC	IEEE 802.11ax (40 MHz, MCS3, 99pc duty cycle)	WLAN	8.29	±9.6
0711	AAC	IEEE 802.11ax (40 MHz, MCS4, 99pc duty cycle)	WLAN	8.39	±9.6
0712	AAC	IEEE 802.11ax (40 MHz, MCS5, 99pc duty cycle)	WLAN	8.67	±9.6
0713	AAC	IEEE 802.11ax (40 MHz, MCS6, 99pc duty cycle)	WLAN	8.33	±9.6
0714	AAC	IEEE 802.11ax (40 MHz, MCS7, 99pc duty cycle)	WLAN	8.26	±9.6
0715	AAC	IEEE 802.11ax (40 MHz, MCS8, 99pc duty cycle)	WLAN	8.45	±9.6
0716	AAC	IEEE 802,11ax (40 MHz, MCS9, 99pc duty cycle)	WLAN	8,30	±9.6
			WLAN	8.48	±9.6
0717	AAC	IEEE 802.11ax (40 MHz, MCS10, 99pc duty cycle)		8.24	+9.6
0718	AAC	IEEE 802.11ax (40 MHz, MCS11, 99pc duty cycle)	WLAN		
0719	AAC	IEEE 802.11ax (80 MHz, MCS0, 90pc duty cycle)	WLAN	8.81	1.9.6
0720	AAC	IEEE 802.11ax (80 MHz, MCS1, 90pc duty cycle)	WLAN	8.87	±9.6
0721	AAC	IEEE 802.11ax (80 MHz, MCS2, 90pc duty cycle)	WLAN	8.76	±9.6
0722	AAC	IEEE 802,11ax (80 MHz, MCS3, 90pc duty cycle)	WLAN	8.55	±9.6
0723	AAC	IEEE 802.11ax (80 MHz, MCS4, 90pc duty cycle)	WLAN	8.70	+9.6
0724	AAC	IEEE 802.11ax (80 MHz, MCS5, 90pc duty cycle)	WLAN	8,90	±9.6
0725	AAC	IEEE 802.11ax (80 MHz, MCS6, 90pc duty cycle)	WLAN	8.74	±9.6
0726	AAC	IEEE 802,11ax (80 MHz, MCS7, 90pc duty cycle)	WLAN	8.72	±9.6
			WLAN	8.66	±9.0
0727	AAC	IEEE 802.11ax (80 MHz, MCS8, 90pc duty cycle)			
0728	AAC	IEEE 802.11ax (80 MHz, MCS9, 90pc duty cycle)	WLAN	8.65	±9.6
0729	AAC	IEEE 802.11ax (80 MHz, MCS10, 90pc duty cycle)	WLAN	8.64	±9.6
0730	AAC	IEEE 802.11ax (80 MHz, MCS11, 90pc duty cycle)	WLAN	8.67	±9.1
0731	AAC	IEEE 802.11ax (80 MHz, MCS0, 99pc duty cycle)	WLAN	8.42	±9.6
0732	AAC	IEEE 802.11ax (80 MHz, MCS1, 99pc duty cycle)	WLAN	8.46	±9.
0733	AAC	IEEE 802.11ax (80 MHz, MCS2, 99pc duty cycle)	WLAN	8,40	±9.6
0734	AAC	IEEE 802.11ax (80 MHz, MCS3, 99pc duty cycle)	WLAN	8.25	±9.6
0735	AAC	IEEE 802.11ax (80 MHz, MCS3, 99pc duty cycle)	WLAN	8.33	±9.6
			WLAN	8.27	+9.6
0736	AAC	IEEE 802.11ax (80 MHz, MCS5, 99pc duty cycle)			
0737	AAC	IEEE 802,11ax (80 MHz, MCS6, 99pc duty cycle)	WLAN	8.36	±9.6
10738	AAC	IEEE 802.11ax (80 MHz, MCS7, 99pc duty cycle)	WLAN	8.42	±9.
10739	AAC	IEEE 802.11ax (80 MHz, MCS8, 99pc duty cycle)	WLAN	8.29	±9.
0740	AAC	IEEE 802.11ax (80 MHz, MCS9, 99pc duty cycle)	WLAN	8.48	±9.6
0741	AAC	IEEE 802.11ax (80 MHz, MCS10, 99pc duty cycle)	WLAN	8.40	±9.
10742	AAC	IEEE 802.11ax (80 MHz, MCS11, 99pc duty cycle)	WLAN	8.43	±9.
0743		IEEE 802.11ax (160 MHz, MCS0, 90pc duty cycle)	WLAN	8.94	±9.
10744		IEEE 802.11ax (160 MHz, MCS1, 90pc duty cycle)	WLAN	9.16	±9.
10744		IEEE 802.11ax (160 MHz, MCS1, supe duty cycle)	WLAN	8.93	±9.
10746	1.1.1.0	IEEE 802.11ax (160 MHz, MCS3, 90pc duty cycle)	WLAN	9.11	±9.
10747		IEEE 802.11ax (160 MHz, MCS4, 90pc duty cycle)	WLAN	9.04	±9.
10748		IEEE 802.11ax (160 MHz, MCS5, 90pc duty cycle)	WLAN	8.93	±9.
10749	AAC	IEEE 802.11ax (160 MHz, MCS6, 90pc duty cycle)	WLAN	8.90	±9.
10750		IEEE 802.11ax (160 MHz, MCS7, 90pc duty cycle)	WLAN	8.79	±9.
10751	AAC	IEEE 802.11ax (160 MHz, MCS8, 90pc duty cycle)	WLAN	8.82	±9.
	1 mmo	IEEE 802.11ax (160 MHz, MCS9, 90pc duty cycle)	WLAN	8.81	±9.

Certificate No: EX-7823 Jul24

Page 18 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 24 of 45

EX3DV4 - SN:7823

July 31, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
0753	AAC	IEEE 802.11ax (160 MHz, MCS10, 90pc duty cycle)	WLAN	9.00	±9.6
0754	AAC	IEEE 802.11ax (160 MHz, MCS11, 90pc duty cycle)	WLAN	8.94	±9.6
0755	AAC	IEEE 802,11ax (160 MHz, MCS0, 99pc duty cycle)	WLAN	8.64	+9.6
0756	AAC	IEEE 802,11ax (160 MHz, MCS1, 99pc duty cycle)	WLAN	8,77	±9.6
		IEEE 802,11ax (160 MHz, MCS2, 99pc duty cycle)	WLAN	8,77	±9.6
0757	AAC		WLAN	8.69	±9.6
0758	AAC	IEEE 802.11ax (160 MHz, MCS3, 99pc duty cycle)		8.58	
0759	AAC	IEEE 802.11ax (160 MHz, MCS4, 99pc duty cycle)	WLAN		±9.6
0760	AAC	IEEE 802.11ax (160 MHz, MCS5, 99pc duty cycle)	WLAN	8.49	±9.6
0761	AAC	IEEE 802.11ax (160 MHz, MCS6, 99pc duty cycle)	WLAN	8.58	±9.6
0762	AAC	IEEE 802.11ax (160 MHz, MCS7, 99pc duty cycle)	WLAN	8.49	±9.6
0763	AAC	IEEE 802.11ax (160 MHz, MCS8, 99pc duty cycle)	WLAN	8.53	±9.6
0764	AAC	IEEE 802.11ax (160 MHz, MCS9, 99pc duty cycle)	WLAN	8.54	±9.6
0765	AAC	IEEE 802.11ax (160 MHz, MCS10, 99pc duty cycle)	WLAN	8.54	±9.6
	AAC	IEEE 802.11ax (160 MHz, MCS11, 99pc duty cycle)	WLAN	8.51	±9.6
0766			5G NR FR1 TDD	7.99	+9.6
0767	AAG	5G NR (CP-OFDM, 1 RB, 5 MHz, QPSK, 15 kHz)		1100	
0768	AAE	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.01	±9.6
0769	AAD	5G NR (CP-OFDM, 1 RB, 15MHz, QPSK, 15kHz)	5G NR FR1 TDD	8.01	±9.6
0770	AAE	5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.02	±9.6
0771	AAD	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.02	±9.6
0772	AAE	5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.23	±9.6
0773	AAF	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.03	±9.6
0774	AAF	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.02	±9.6
			5G NR FR1 TDD	8.31	±9.6
0775	AAF	5G NR (CP-OFDM, 50% RB, 5 MHz, QPSK, 15 kHz)		8.30	+9.6
0776	AAE	5G NR (CP-OFDM, 50% RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.30	+9.6
0777	AAC	5G NR (CP-OFDM, 50% RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	0100	
0778	AAE	5G NR (CP-OFDM, 50% RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.34	±9.6
10779	AAC	5G NR (CP-OFDM, 50% RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.42	±9.6
10780	AAE	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.38	+9.6
0781	AAF	5G NR (CP-OFDM, 50% RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.38	±9.6
0782	AAE	5G NR (CP-OFDM, 50% RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.43	±9.6
10783	AAG	5G NR (CP-OFDM, 100% RB, 5 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.31	±9.6
			5G NR FR1 TDD	8.29	±9.6
10784	AAE	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 15 kHz)		8.40	
10785	AAD	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	0110	±9.6
10786	AAE	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.35	±9.6
10787	AAD	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.44	±9.6
10788	AAE	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.39	±9.6
10789	AAF	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.37	±9.6
10790	AAE	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.39	±9.6
10791	AAG	5G NR (CP-OFDM, 1 RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7,83	±9.6
10792	AAE	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.92	19.6
		5G NR (CP-OFDM, 1 RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.95	±9.6
10793	AAD			7.82	±9.6
10794	AAE	5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		
10795	AAD	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.84	±9.6
10796	AAE	5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.82	±9.0
10797	AAF	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.01	±9.6
10798	AAE	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.89	±9.6
10799	AAF	5G NR (CP-OFDM, 1 RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.93	±9.
10801	AAF	5G NR (CP-OFDM, 1 RB, 80 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.89	±9.4
10802	AAE	5G NR (CP-OFDM, 1 RB, 90 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.87	±9.0
10803	AAF	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.93	±9.
	AAF		5G NR FR1 TDD		±9.
10805		5G NR (CP-OFDM, 50% RB, 10 MHz, QPSK, 30 kHz)			
10806	AAD	5G NR (CP-OFDM, 50% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.37	1.9.
10809	AAE	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	±9.
10810		5G NR (CP-OFDM, 50% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		±9.
10812	AAF	5G NR (CP-OFDM, 50% RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.35	±9.
10817	AAG	5G NR (CP-OFDM, 100% RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.35	±9.
10818		5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		±9.
10819	AAD	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		±9.
10820		5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		±9.
10821	AAD	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		±9.
10822		5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		±9.
10823	AAF	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.36	±9.
10824	AAE	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.39	+9.
10825	AAF	5G NR (CP-OFDM, 100% RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.41	±9.
	AAF	5G NR (CP-OFDM, 100% RB, 80 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		±9.
10827			0011111100		10.

Certificate No: EX-7823 Jul24

Page 19 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# Report No: TESA2410000648ES Page: 25 of 45

EX3DV4 - SN:7823

July 31, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	$Unc^{E} k = 2$
10829	AAF	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.40	±9.6
0.830	AAE	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.63	±9.6
0831	AAD	5G NR (CP-OFDM, 1 RB, 15 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.73	±9.6
0832	AAE	5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.74	+9.6
0833	AAD	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.70	±9.6
		5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7 75	±9.6
0834	AAE		5G NR FR1 TDD	7.70	±9.6
0835	AAF	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.66	±9.6
0836	AAE	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 60 kHz)			
0837	AAF	5G NR (CP-OFDM, 1 RB, 60 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.68	±9.6
0839	AAF	5G NR (CP-OFDM, 1 RB, 80 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.70	±9.6
0840	AAE	5G NR (CP-OFDM, 1 RB, 90 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.67	±9.6
0841	AAF	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.71	±9.6
0843	AAD	5G NR (CP-OFDM, 50% RB, 15 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.49	±9.6
0844	AAE	5G NR (CP-OFDM, 50% RB, 20 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.34	±9.6
0846	AAE	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	±9.6
0854	AAE	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.34	±9.6
0855	AAD	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.36	±9,6
0856	AAE	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.37	+9.6
0855	AAE	5G NR (CP-OFDM, 100% HB, 20 MHz, QFSK, 60 kHz)	5G NR FR1 TDD	8.35	±9.6
				8.36	±9.6
0858	AAE	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.36	±9.6
0859	AAF	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 60 kHz)	Contract the		
0860	AAE	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	±9.6
0861	AAF	5G NR (CP-OFDM, 100% RB, 60 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.40	±9.6
0863	AAF	5G NR (CP-OFDM, 100% RB, 80 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	±9.6
10864	AAE	5G NR (CP-OFDM, 100% RB, 90 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.37	±9.6
10865	AAF	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	±9.6
10866	AAF	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9,6
10868	AAF	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.89	±9.6
10869	AAE	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.75	±9.6
10870	AAE	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.86	±9.6
10871	AAE	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, 16QAM, 120 KHz)	5G NR FR2 TDD	5.75	±9.6
10872	AAE	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.52	±9.6
10873	AAE	5G NR (DFT-s-OFDM, 100 % ND, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.61	±9.6
			5G NR FR2 TDD	6.65	±9.6
10874	AAE	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, 64QAM, 120 kHz)			
10875	AAE	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	7.78	±9.6
10876	AAE	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	8.39	±9.6
10877	AAE	5G NR (CP-OFDM, 1 RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	7.95	±9.6
10878	AAE	5G NR (CP-OFDM, 100% RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	8.41	±9.6
10879	AAE	5G NR (CP-OFDM, 1 RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.12	±9.6
10880	AAE	5G NR (CP-OFDM, 100% RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.38	±9.6
10881	AAE	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.75	±9.6
10882	AAE	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.96	±9.6
10883	AAE	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.57	±9.6
10884	AAE	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.53	±9.6
10885	AAE	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.61	±9.6
10886	AAE	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.65	±9.6
10887	AAE	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	7.78	±9.6
10888	AAE	5G NR (CP-OFDM, 140% RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	8.35	±9.6
10888	AAE	5G NR (CP-OFDM, 100% RB, 50 MHz, 16QAM, 120 KHz)	5G NR FR2 TDD	8.02	+9.6
10889	AAE		5G NR FR2 TDD	8.40	±9.6
		5G NR (CP-OFDM, 100% RB, 50 MHz, 16QAM, 120 kHz)		8.40	±9.6
10891	AAE	5G NR (CP-OFDM, 1 RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD		
10892		5G NR (CP-OFDM, 100% RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.41	±9.6
10897	AAE	5G NR (DFT-s-OFDM, 1 RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.66	±9.6
10898		5G NR (DFT-s-OFDM, 1 RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.67	±9.6
10899		5G NR (DFT-s-OFDM, 1 RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.67	±9.6
10900	AAC	5G NR (DFT-s-OFDM, 1 RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10901	AAB	5G NR (DFT-s-OFDM, 1 RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10902	AAC	5G NR (DFT-s-OFDM, 1 RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10903		5G NR (DFT-s-OFDM, 1 RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10904		5G NR (DFT-s-OFDM, 1 RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10905		5G NR (DFT-s-OFDM, 1 RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	+9.6
10905		5G NR (DFT-s-OFDM, 1 RB, 80 MHz, QPSK, 30 KHz)	5G NR FR1 TDD	5.68	±9.6
10907		5G NR (DFT-s-OFDM, 50% RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		±9.6
10908		5G NR (DFT-s-OFDM, 50% RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.93	±9.6
10909		5G NR (DFT-s-OFDM, 50% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD		±9.6
10910	AAC	5G NR (DFT-s-OFDM, 50% RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.83	±9.6

Certificate No: EX-7823 Jul24

Page 20 of 22

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責。同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's not reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Taiwan Ltd. No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488