

Appendix C

System Verification Scans

Motorola Solutions, Inc. EME Laboratory

Date/Time: 8/30/2022 8:00:52 AM

Robot#: DASY5-PG-03 | Run#: BAD-SYSP-835H-220830-01

Dipole Model#: D835V2
 Phantom#: ELI4 1050
 Tissue Temp: 22.0 (C)
 Serial#: 4D029
 Test Freq: 835.0000 (MHz)
 Start Power: 250 (mW)
 Rotation (1D): 0.068 dB
 Adjusted SAR (1W): 10.16 mW/g (1g)

Comments:

Communication System Band: Dipole 835, Communication System UID: 0, Duty Cycle: 1:1,

Medium parameters used: $f = 835$ MHz; $\sigma = 0.92$ S/m; $\epsilon_r = 40.5$; $\rho = 1000$ kg/m³

Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 835 MHz, ConvF(9.8, 9.8, 9.8) @ 835 MHz

Electronics: DAE4 Sn684, Calibrated: 2/22/2022

Below 2 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (41x131x1):

Interpolated grid: dx=1.500 mm, dy=1.500 mm

Reference Value = 62.61 V/m; Power Drift = 0.14 dB

Fast SAR: SAR(1 g) = 2.64 W/kg; SAR(10 g) = 1.72 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 3.47 W/kg

Below 2 GHz-Rev.3/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 62.61 V/m; Power Drift = 0.14 dB

Peak SAR (extrapolated) = 3.98 W/kg

SAR(1 g) = 2.54 W/kg; SAR(10 g) = 1.65 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 18.3 mm


Ratio of SAR at M2 to SAR at M1 = 64.4%

Maximum value of SAR (measured) = 3.49 W/kg

Below 2 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17): Measurement

grid: dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 3.44 W/kg

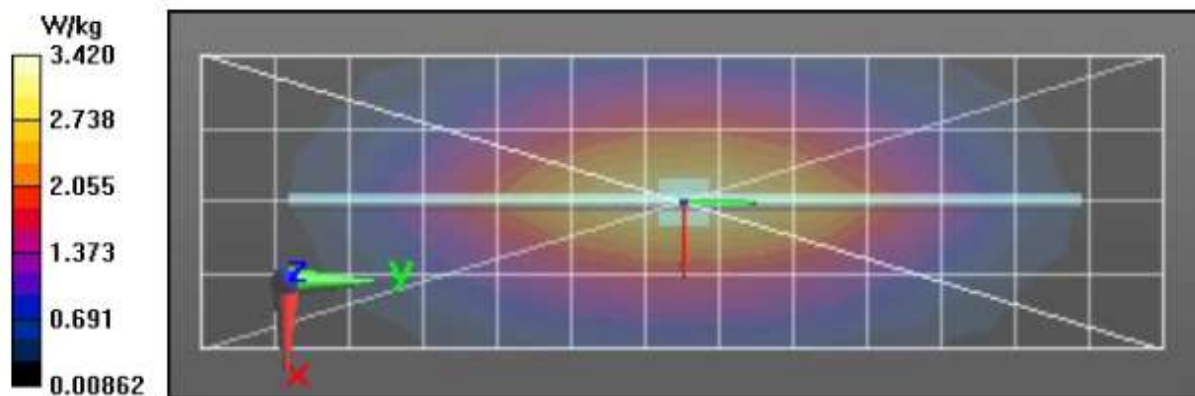

Motorola Solutions, Inc. EME Laboratory

Date/Time: 11/25/2022 11:18:57 AM

Robot#: DASY5-PG-3 | Run#: DAN-SYSP-2450H-221125-06
 Dipole Model# D2450V3
 Phantom#: ELI4 1037
 Tissue Temp: 21.1(C)
 Serial#: 782
 Test Freq: 2450.0000(MHz)
 Start Power: 31.6(mW)
 Rotation (1D): 0.140dB
 Adjusted SAR (1W): 50.63mW/g (1g)

Comments:

Communication System Band: Dipole 2450, Communication System UID: 0, Duty Cycle: 1:1,

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.71$ S/m; $\epsilon_r = 39$; $\rho = 1000$ kg/m³

Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 2450 MHz, ConvF(7.71, 7.71, 7.71) @ 2450 MHz

Electronics: DAE4 Sn684, Calibrated: 2/22/2022

2-3 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (51x71x1): Interpolated grid:

$dx=1.200$ mm, $dy=1.200$ mm

Reference Value = 40.00 V/m; Power Drift = -0.04 dB

Fast SAR: SAR(1 g) = 1.7 W/kg; SAR(10 g) = 0.781 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 2.80 W/kg

2-3 GHz-Rev.3/System Performance Check/0-Degree Cube (7x7x7)/Cube 0: Measurement

grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 40.00 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 3.24 W/kg

SAR(1 g) = 1.6 W/kg; SAR(10 g) = 0.746 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 9 mm


Ratio of SAR at M2 to SAR at M1 = 48.6%

Maximum value of SAR (measured) = 2.61 W/kg

2-3 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17): Measurement grid:

$dx=20$ mm, $dy=20$ mm, $dz=10$ mm

Maximum value of SAR (measured) = 2.61 W/kg

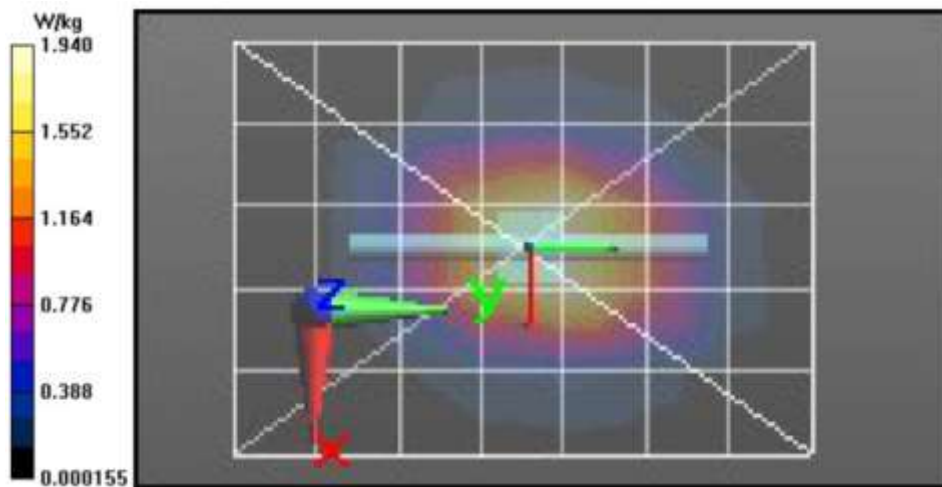

Motorola Solutions, Inc. EME Laboratory

Date/Time: 9/5/2022 8:22:06 AM

Robot#: DASY5-PG-2 | Run#: SAN-SYSP-5250H-220905-04
 Dipole Model# D5GHzV2
 Phantom#: ELI4 1108
 Tissue Temp: 22.0 (C)
 Serial#: 1022
 Test Freq: 5250.0000(MHz)
 Start Power: 100 (mW)
 Rotation (1D): 0.200 dB
 Adjusted SAR (1W): 83.60 mW/g (1g)

Comments:

Communication System Band: Dipole 5000, Communication System UID: 0, Duty Cycle: 1:1,
 Medium parameters used: $f = 5250$ MHz; $\sigma = 4.61$ S/m; $\epsilon_r = 38.7$; $\rho = 1000$ kg/m³
 Probe: EX3DV4 - SN7364, Calibrated: 2/28/2022, Frequency: 5250 MHz, ConvF(5.21, 5.21, 5.21) @ 5250 MHz
 Electronics: DAE4 Sn1294, Calibrated: 2/22/2022

4-6 GHz-Rev.5/System Performance Check/Dipole Area Scan 2 (61x61x1): Interpolated grid:

dx=0.9000 mm, dy=0.9000 mm

Reference Value = 75.50 V/m; Power Drift = 0.06 dB

Fast SAR: SAR(1 g) = 8.37 W/kg; SAR(10 g) = 2.36 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 21.3 W/kg

4-6 GHz-Rev.5/System Performance Check/0-Degree Cube (8x8x12)/Cube 0: Measurement

grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 75.50 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 31.8 W/kg

SAR(1 g) = 8.36 W/kg; SAR(10 g) = 2.42 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 6.9 mm


Ratio of SAR at M2 to SAR at M1 = 56%

Maximum value of SAR (measured) = 18.8 W/kg

4-6 GHz-Rev.5/System Performance Check/Z-Axis Retraction (1x1x17): Measurement grid:

dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 20.9 W/kg

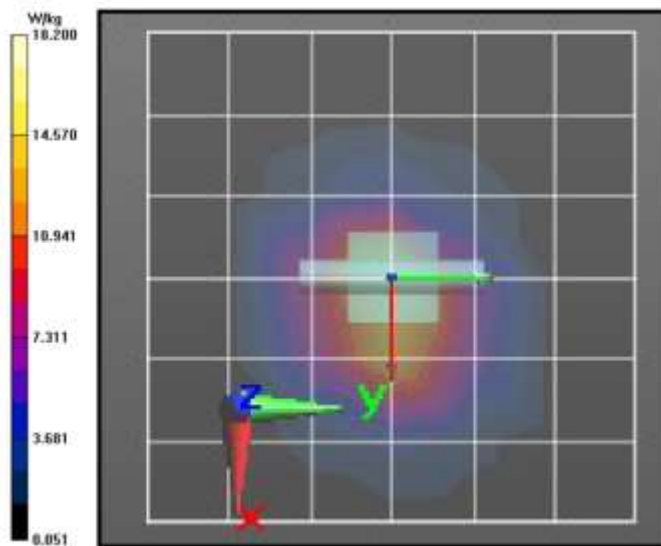

Motorola Solutions, Inc. EME Laboratory

Date/Time: 11/17/2022 3:54:56 PM

Robot#: DASY5-PG-3 | Run#: SAN(ZIQ)-SYSP-5250H-221117-07

Dipole Model# D5GHzV2

Phantom#: ELI4 1037

Tissue Temp: 21.3 (C)

Serial#: 1026

Test Freq: 5250.0000 (MHz)

Start Power: 100 (mW)

Rotation (1D): 0.071 dB

Adjusted SAR (1W): 77.00 mW/g (1g)

Comments:

Communication System Band: Dipole 5000, Communication System UID: 0, Duty Cycle: 1:1,

Medium parameters used: $f = 5250$ MHz; $\sigma = 4.26$ S/m; $\epsilon_r = 33.7$; $\rho = 1000$ kg/m³

Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 5250 MHz, ConvF(5.6, 5.6, 5.6) @ 5250 MHz

Electronics: DAE4 Sn684, Calibrated: 2/22/2022

4-6 GHz-Rev.5/System Performance Check/Dipole Area Scan 2 (61x61x1): Interpolated grid:

dx=0.9000 mm, dy=0.9000 mm

Reference Value = 72.00 V/m; Power Drift = 0.17 dB

Fast SAR: SAR(1 g) = 6.97 W/kg; SAR(10 g) = 1.93 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 18.3 W/kg

4-6 GHz-Rev.5/System Performance Check/0-Degree Cube (8x8x12)/Cube 0: Measurement

grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 72.00 V/m; Power Drift = 0.17 dB

Peak SAR (extrapolated) = 31.0 W/kg

SAR(1 g) = 7.7 W/kg; SAR(10 g) = 2.18 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 7.2 mm


Ratio of SAR at M2 to SAR at M1 = 55.9%

Maximum value of SAR (measured) = 17.9 W/kg

4-6 GHz-Rev.5/System Performance Check/Z-Axis Retraction (1x1x17): Measurement grid:

dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 19.5 W/kg

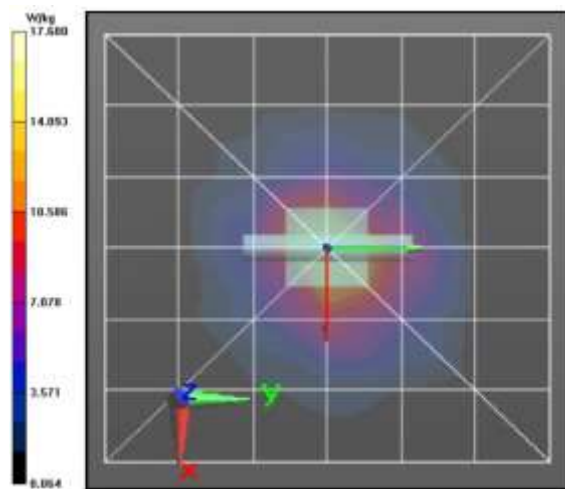

Motorola Solutions, Inc. EME Laboratory

Date/Time: 9/4/2022 2:22:30 PM

Robot#: DASY5-PG-2 | Run#: SAN-SYSP-5600H-220904-09
 Dipole Model#: D5GHzV2
 Phantom#: ELI4 1108
 Tissue Temp: 21.9 (C)
 Serial#: 1022
 Test Freq: 5600.0000(MHz)
 Start Power: 100 (mW)
 Rotation (1D): 0.120 dB
 Adjusted SAR (1W): 84.50 mW/g (1g)

Comments:

Communication System Band: Dipole 5000, Communication System UID: 0, Duty Cycle: 1:1,
 Medium parameters used: $f = 5600$ MHz; $\sigma = 4.68$ S/m; $\epsilon_r = 35.9$; $\rho = 1000$ kg/m³
 Probe: EX3DV4 - SN7364, Calibrated: 2/28/2022, Frequency: 5600 MHz, ConvF(4.64, 4.64, 4.64) @ 5600 MHz
 Electronics: DAE4 Sn1294, Calibrated: 2/22/2022

4-6 GHz-Rev.5/System Performance Check/Dipole Area Scan 2 (61x61x1): Interpolated grid:

dx=0.9000 mm, dy=0.9000 mm

Reference Value = 74.83 V/m; Power Drift = -0.02 dB

Fast SAR: SAR(1 g) = 7.91 W/kg; SAR(10 g) = 2.19 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 21.3 W/kg

4-6 GHz-Rev.5/System Performance Check/0-Degree Cube (8x8x12)/Cube 0: Measurement

grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 74.83 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 35.5 W/kg

SAR(1 g) = 8.45 W/kg; SAR(10 g) = 2.41 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 7.2 mm


Ratio of SAR at M2 to SAR at M1 = 53.1%

Maximum value of SAR (measured) = 19.8 W/kg

4-6 GHz-Rev.5/System Performance Check/Z-Axis Retraction (1x1x17): Measurement grid:

dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 21.9 W/kg

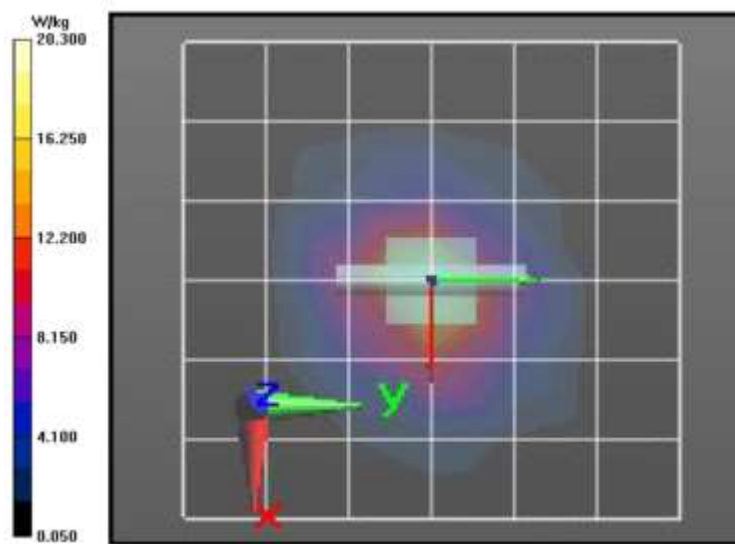

Motorola Solutions, Inc. EME Laboratory

Date/Time: 11/17/2022 5:53:22 PM

Robot#: DASY5-PG-3 | Run#: SAN(ZIQ)-SYSP-5600H-221117-08
 Dipole Model# D5GHzV2
 Phantom#: ELI4 1037
 Tissue Temp: 21.5 (C)
 Serial#: 1026
 Test Freq: 5600.0000 (MHz)
 Start Power: 100 (mW)
 Rotation (1D): 0.100 dB
 Adjusted SAR (1W): 86.20 mW/g (1g)

Comments:

Communication System Band: Dipole 5000, Communication System UID: 0, Duty Cycle: 1:1,
 Medium parameters used: $f = 5600$ MHz; $\sigma = 4.62$ S/m; $\epsilon_r = 33.2$; $\rho = 1000$ kg/m³
 Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 5600 MHz, ConvF(4.83, 4.83, 4.83) @ 5600 MHz
 Electronics: DAE4 Sn684, Calibrated: 2/22/2022

4-6 GHz-Rev.5/System Performance Check/Dipole Area Scan 2 (61x61x1): Interpolated grid:

dx=0.9000 mm, dy=0.9000 mm

Reference Value = 76.80 V/m; Power Drift = -0.02 dB

Fast SAR: SAR(1 g) = 8.07 W/kg; SAR(10 g) = 2.23 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 22.2 W/kg

4-6 GHz-Rev.5/System Performance Check/0-Degree Cube (8x8x12)/Cube 0: Measurement

grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 76.80 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 37.8 W/kg

SAR(1 g) = 8.62 W/kg; SAR(10 g) = 2.45 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 7.2 mm


Ratio of SAR at M2 to SAR at M1 = 52.1%

Maximum value of SAR (measured) = 20.6 W/kg

4-6 GHz-Rev.5/System Performance Check/Z-Axis Retraction (1x1x17): Measurement grid:

dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 22.8 W/kg

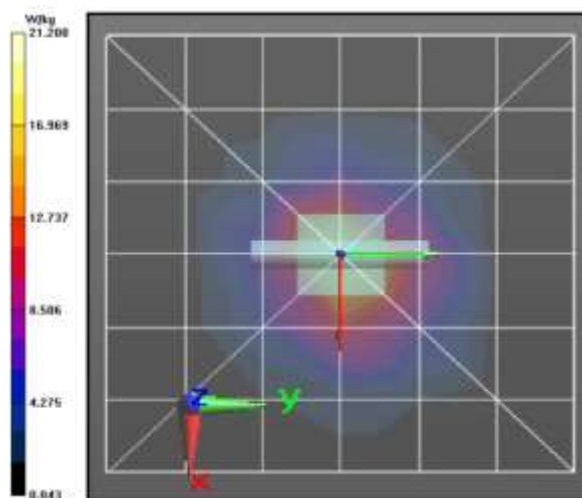

Motorola Solutions, Inc. EME Laboratory

Date/Time: 9/12/2022 8:53:55 PM

Robot#: DASY5-PG-1 | Run#: BL-SYSP-5750H-220912-01
 Dipole Model# D5GHzV2
 Phantom#: ELI4 1037
 Tissue Temp: 20.3 (C)
 Serial#: 1022
 Test Freq: 5750.0000 (MHz)
 Start Power: 100 (mW)
 Rotation (1D): 0.12 dB
 Adjusted SAR (1W): 76.60 mW/g (1g)

Comments:

Communication System Band: D5GHz, Communication System UID: 0, Duty Cycle: 1:1,
 Medium parameters used: $f = 5750$ MHz; $\sigma = 4.79$ S/m; $\epsilon_r = 32.2$; $\rho = 1000$ kg/m³
 Probe: EX3DV4 - SN7485, Calibrated: 4/25/2022, Frequency: 5750 MHz, ConvF(5.11, 5.11, 5.11) @ 5750 MHz
 Electronics: DAE4 Sn850, Calibrated: 4/14/2022

4-6 GHz-Rev.5/System Performance Check/Dipole Area Scan 2 (61x61x1): Interpolated grid:

dx=0.9000 mm, dy=0.9000 mm

Reference Value = 72.03 V/m; Power Drift = -0.20 dB

Fast SAR: SAR(1 g) = 7.36 W/kg; SAR(10 g) = 2.02 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 20.6 W/kg

4-6 GHz-Rev.5/System Performance Check/0-Degree Cube (8x8x12)/Cube 0: Measurement

grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 72.03 V/m; Power Drift = -0.20 dB

Peak SAR (extrapolated) = 34.7 W/kg

SAR(1 g) = 7.66 W/kg; SAR(10 g) = 2.19 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 7.9 mm


Ratio of SAR at M2 to SAR at M1 = 51%

Maximum value of SAR (measured) = 19.1 W/kg

4-6 GHz-Rev.5/System Performance Check/Z-Axis Retraction (1x1x17): Measurement grid:

dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 19.4 W/kg

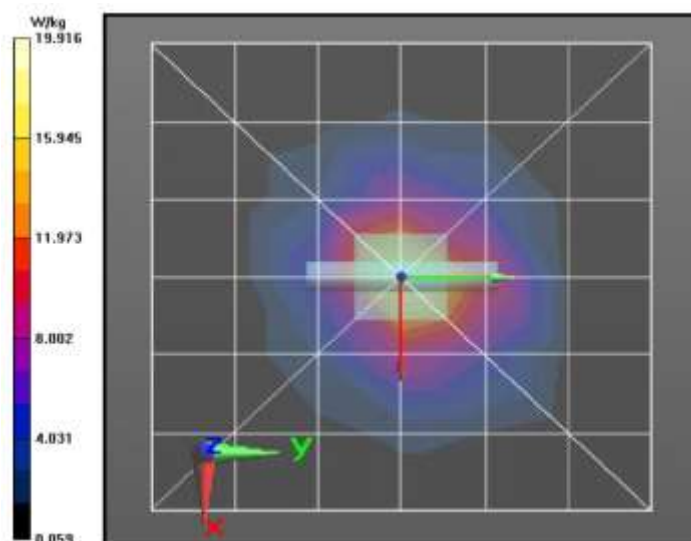

Motorola Solutions, Inc. EME Laboratory

Date/Time: 11/18/2022 9:20:39 AM

Robot#: DASY5-PG-3 | Run#: BL(ZIQ)-SYSP-5750H-221118-03

Dipole Model# D5GHzV2

Phantom#: ELI4 1037

Tissue Temp: 21.1 (C)

Serial#: 1026

Test Freq: 5750.0000 (MHz)

Start Power: 100 (mW)

Rotation (1D): 0.087 dB

Adjusted SAR (1W): 82.50 mW/g (1g)

Comments:

Communication System Band: Dipole 5000, Communication System UID: 0, Duty Cycle: 1:1,

Medium parameters used: $f = 5750$ MHz; $\sigma = 4.78$ S/m; $\epsilon_r = 32.3$; $\rho = 1000$ kg/m³

Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 5750 MHz, ConvF(5.05, 5.05, 5.05) @ 5750 MHz

Electronics: DAE4 Sn684, Calibrated: 2/22/2022

4-6 GHz-Rev.5/System Performance Check/Dipole Area Scan 2 (61x61x1): Interpolated grid:

dx=0.9000 mm, dy=0.9000 mm

Reference Value = 74.91 V/m; Power Drift = -0.07 dB

Fast SAR: SAR(1 g) = 7.96 W/kg; SAR(10 g) = 2.15 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 22.5 W/kg

4-6 GHz-Rev.5/System Performance Check/0-Degree Cube (8x8x12)/Cube 0: Measurement

grid: dx=4mm, dy=4mm, dz=2mm

Reference Value = 74.91 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 36.6 W/kg

SAR(1 g) = 8.25 W/kg; SAR(10 g) = 2.35 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 7.4 mm


Ratio of SAR at M2 to SAR at M1 = 52%

Maximum value of SAR (measured) = 19.8 W/kg

4-6 GHz-Rev.5/System Performance Check/Z-Axis Retraction (1x1x17): Measurement grid:

dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 22.1 W/kg

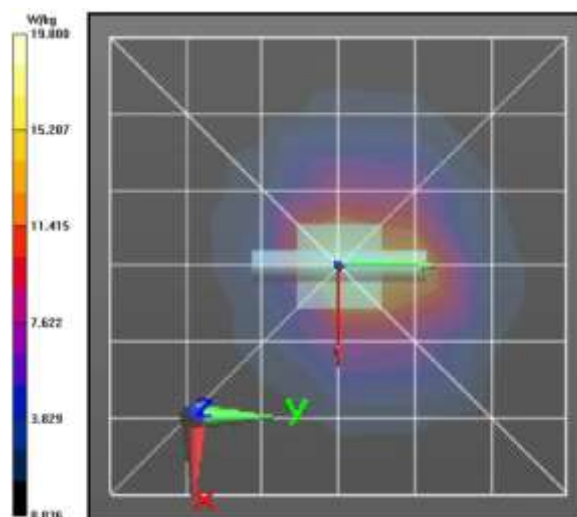

Motorola Solutions, Inc. EME Laboratory

Date/Time: 11/15/2022 7:43:16 PM

Robot#: DASY5-PG-3 | Run#: IRA-SYSP-750H-221115-01
 Dipole Model#: D750V3
 Phantom#: ELI4 1037
 Tissue Temp: 21.2 (C)
 Serial#: 1098
 Test Freq: 750.0000(MHz)
 Start Power: 250 (mW)
 Rotation (1D): 0.069 dB
 Adjusted SAR (1W): 9.08 mW/g (1g)

Comments:

Communication System Band: Dipole 750, Communication System UID: 0, Duty Cycle: 1:1,
 Medium parameters used: $f = 750$ MHz; $\sigma = 0.86$ S/m; $\epsilon_r = 43.3$; $\rho = 1000$ kg/m³
 Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 750 MHz, ConvF(10.22, 10.22, 10.22) @ 750 MHz
 Electronics: DAE4 Sn684, Calibrated: 2/22/2022

Below 2 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (41x151x1):


Interpolated grid: $dx=1.500$ mm, $dy=1.500$ mm
 Reference Value = 60.95 V/m; Power Drift = -0.01 dB
Fast SAR: SAR(1 g) = 2.32 W/kg; SAR(10 g) = 1.53 W/kg (SAR corrected for target medium)
 Maximum value of SAR (interpolated) = 2.89 W/kg

Below 2 GHz-Rev.3/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:

Measurement grid: $dx=7.5$ mm, $dy=7.5$ mm, $dz=5$ mm
 Reference Value = 60.95 V/m; Power Drift = -0.01 dB
 Peak SAR (extrapolated) = 3.27 W/kg
SAR(1 g) = 2.27 W/kg; SAR(10 g) = 1.49 W/kg (SAR corrected for target medium)
 Smallest distance from peaks to all points 3 dB below: Larger than measurement grid
 Ratio of SAR at M2 to SAR at M1 = 67%
 Maximum value of SAR (measured) = 2.91 W/kg

Below 2 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17): Measurement

grid: $dx=20$ mm, $dy=20$ mm, $dz=10$ mm
 Maximum value of SAR (measured) = 2.91 W/kg

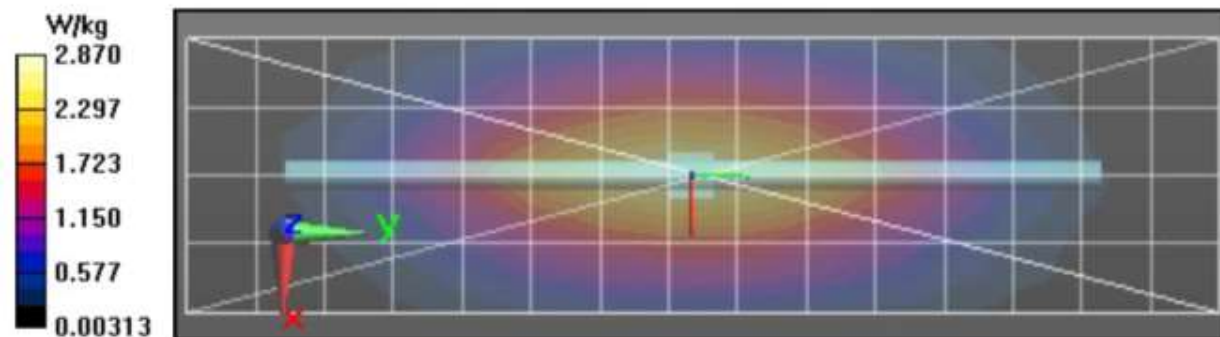

Motorola Solutions, Inc. EME Laboratory

Date/Time: 8/25/2022 3:39:11 PM

Robot#: DASY5-PG-03 | Run#: IRA-SYSP-1800H-220825-19
 Dipole Model#: D1800V2
 Phantom#: ELI4 1050
 Tissue Temp: 22.3 (C)
 Serial#: 2D120
 Test Freq: 1800.0000(MHz)
 Start Power: 250(mW)
 Rotation (1D): 0.150 dB
 Adjusted SAR (1W): 35.04 mW/g (1g)

Comments:

Communication System Band: Dipole 1800, Communication System UID: 0, Duty Cycle: 1:1,
 Medium parameters used: $f = 1800$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 41.7$; $\rho = 1000$ kg/m³
 Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 1800 MHz, ConvF(8.43, 8.43, 8.43) @ 1800 MHz
 Electronics: DAE4 Sn684, Calibrated: 2/22/2022

Below 2 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (41x101x1):


Interpolated grid: dx=1.500 mm, dy=1.500 mm
 Reference Value = 103.3 V/m; Power Drift = -0.06 dB
 Fast SAR: SAR(1 g) = 9.15 W/kg; SAR(10 g) = 4.7 W/kg (SAR corrected for target medium)
 Maximum value of SAR (interpolated) = 13.0 W/kg

Below 2 GHz-Rev.3/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm
 Reference Value = 103.3 V/m; Power Drift = -0.06 dB
 Peak SAR (extrapolated) = 15.4 W/kg
 SAR(1 g) = 8.76 W/kg; SAR(10 g) = 4.6 W/kg (SAR corrected for target medium)
 Smallest distance from peaks to all points 3 dB below = 10.5 mm
 Ratio of SAR at M2 to SAR at M1 = 54.7%
 Maximum value of SAR (measured) = 13.0 W/kg

Below 2 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17): Measurement

grid: dx=20mm, dy=20mm, dz=10mm
 Maximum value of SAR (measured) = 13.0 W/kg

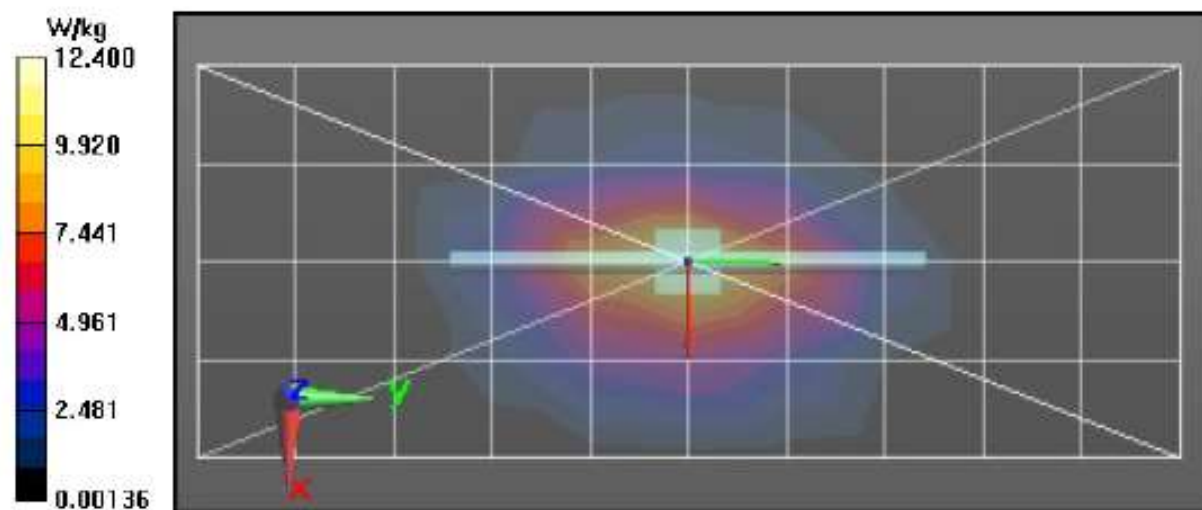

Motorola Solutions, Inc. EME Laboratory

Date/Time: 11/16/2022 9:03:33 AM

Robot#: DASY5-PG-3 | Run#: SAN(ZIQ)-SYSP-1800H-221116-05
 Dipole Model#: D1800V2
 Phantom#: ELI4 1037
 Tissue Temp: 20.40 (C)
 Serial#: 2d119
 Test Freq: 1800.0000(MHz)
 Start Power: 250 (mW)
 Rotation (1D): 0.069 dB
 Adjusted SAR (1W): 40.00 mW/g (1g)

Comments:

Communication System Band: Dipole 1800, Communication System UID: 0, Duty Cycle: 1:1,

Medium parameters used: $f = 1800$ MHz; $\sigma = 1.33$ S/m; $\epsilon_r = 41.8$; $\rho = 1000$ kg/m³

Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 1800 MHz, ConvF(8.43, 8.43, 8.43) @ 1800 MHz

Electronics: DAE4 Sn684, Calibrated: 2/22/2022

Below 2 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (41x81x1):

Interpolated grid: dx=1.500 mm, dy=1.500 mm

Reference Value = 111.2 V/m; Power Drift = -0.16 dB

Fast SAR: SAR(1 g) = 10.3 W/kg; SAR(10 g) = 5.29 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 14.6 W/kg

Below 2 GHz-Rev.3/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:

Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 111.2 V/m; Power Drift = -0.16 dB

Peak SAR (extrapolated) = 17.4 W/kg

SAR(1 g) = 10 W/kg; SAR(10 g) = 5.26 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 10.5 mm


Ratio of SAR at M2 to SAR at M1 = 55.6%

Maximum value of SAR (measured) = 14.6 W/kg

Below 2 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17): Measurement

grid: dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 14.8 W/kg

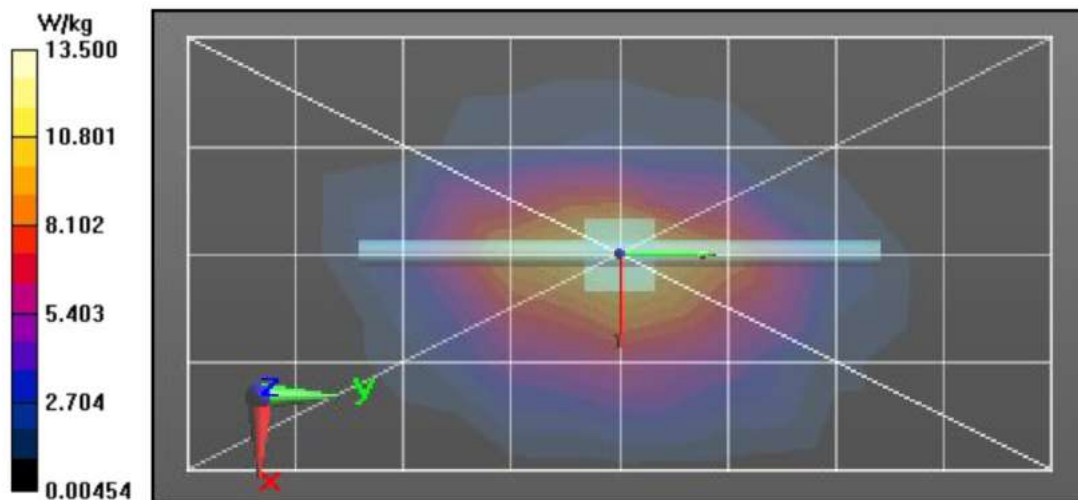

Motorola Solutions, Inc. EME Laboratory

Date/Time: 8/29/2022 3:55:01 AM

Robot#: DASY5-PG-03 | Run#: IRA-SYSP-1900H-220829-04

Dipole Model#: D1900V2
 Phantom#: ELI4 1050
 Tissue Temp: 21.6 (C)
 Serial#: 5D065
 Test Freq: 1900.0000 (MHz)
 Start Power: 250 (mW)
 Rotation (1D): 0.052 dB
 Adjusted SAR (1W): 38.76 mW/g (1g)

Comments:

Communication System Band: Dipole 1900, Communication System UID: 0, Duty Cycle: 1:1,
 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 39.5$; $\rho = 1000$ kg/m³
 Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 1900 MHz, ConvF(8.36, 8.36, 8.36) @ 1900 MHz
 Electronics: DAE4 Sn684, Calibrated: 2/22/2022

Below 2 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (41x101x1):


Interpolated grid: $dx=1.500$ mm, $dy=1.500$ mm
 Reference Value = 108.7 V/m; Power Drift = -0.10 dB
 Fast SAR: SAR(1 g) = 10.2 W/kg; SAR(10 g) = 5.18 W/kg (SAR corrected for target medium)
 Maximum value of SAR (interpolated) = 15.5 W/kg

Below 2 GHz-Rev.3/System Performance Check/0-Degree Cube (5x5x7)/Cube 0:

Measurement grid: $dx=7.5$ mm, $dy=7.5$ mm, $dz=5$ mm
 Reference Value = 108.7 V/m; Power Drift = -0.10 dB
 Peak SAR (extrapolated) = 18.4 W/kg
 SAR(1 g) = 9.69 W/kg; SAR(10 g) = 5.06 W/kg (SAR corrected for target medium)
 Smallest distance from peaks to all points 3 dB below = 10.5 mm
 Ratio of SAR at M2 to SAR at M1 = 53.7%
 Maximum value of SAR (measured) = 15.3 W/kg

Below 2 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17): Measurement

grid: $dx=20$ mm, $dy=20$ mm, $dz=10$ mm
 Maximum value of SAR (measured) = 15.4 W/kg

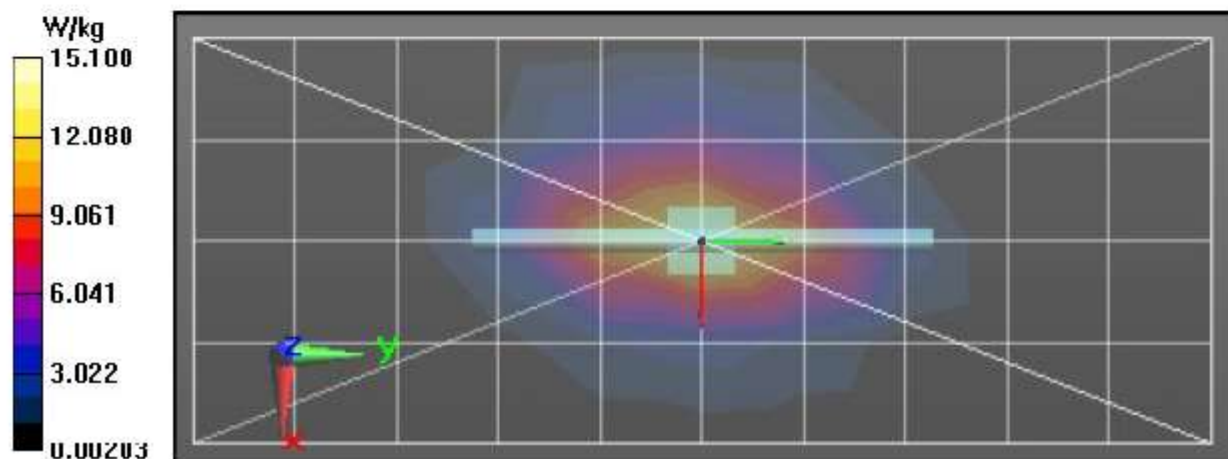

Motorola Solutions, Inc. EME Laboratory

Date/Time: 8/29/2022 1:12:35 AM

Robot#: DASY5-PG-3 | Run#: IRA-SYSP-2600H-220829-01

Dipole Model#: D2600V2

Phantom#: ELI4 1050

Tissue Temp: 21.6 (C)

Serial#: 1011

Test Freq: 2600.0000(MHz)

Start Power: 250(mW)

Rotation (1D): 0.130 dB

Adjusted SAR (1W): 60.00 mW/g (1g)

Comments:

Communication System Band: Dipole 2600, Communication System UID: 0, Duty Cycle: 1:1,

Medium parameters used: $f = 2600$ MHz; $\sigma = 1.9$ S/m; $\epsilon_r = 37.5$; $\rho = 1000$ kg/m³

Probe: EX3DV4 - SN7519, Calibrated: 2/28/2022, Frequency: 2600 MHz, ConvF(7.36, 7.36, 7.36) @ 2600 MHz

Electronics: DAE4 Sn684, Calibrated: 2/22/2022

2-3 GHz-Rev.3/System Performance Check/Dipole Area Scan 2 (51x81x1): Interpolated grid:

dx=1.200 mm, dy=1.200 mm

Reference Value = 123.0 V/m; Power Drift = -0.02 dB

Fast SAR: SAR(1 g) = 16.2 W/kg; SAR(10 g) = 7.2 W/kg (SAR corrected for target medium)

Maximum value of SAR (interpolated) = 27.3 W/kg

2-3 GHz-Rev.3/System Performance Check/0-Degree Cube (7x7x7)/Cube 0: Measurement

grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 123.0 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 32.3 W/kg

SAR(1 g) = 15 W/kg; SAR(10 g) = 6.7 W/kg (SAR corrected for target medium)

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 46.4%

Maximum value of SAR (measured) = 25.7 W/kg

2-3 GHz-Rev.3/System Performance Check/Z-Axis Retraction (1x1x17): Measurement grid:

dx=20mm, dy=20mm, dz=10mm

Maximum value of SAR (measured) = 27.4 W/kg

