

System Performance Check Report for D1900V2 - SN5d190

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1900.0	TSL Permittivity	39.2
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.44
Conversion Factor	8.12	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7651 2024-03-18	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1468 2024-08-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.75	3.89
psSAR10g [W/Kg]	2.01	2.01
Power Drift [dB]		-0.18
Dist 3dB Peak [mm]		10.8
M2/M1 [%]		82.0

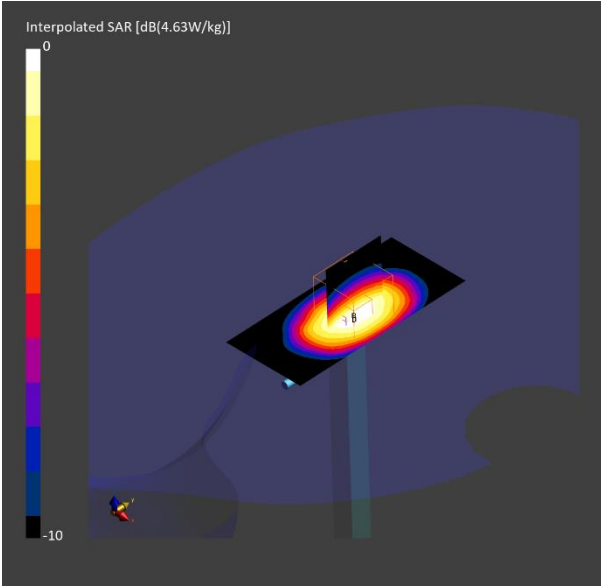

System Performance Check Report for D835V2 - SN4d174

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	835.0	TSL Permittivity	40.7
Group / UID	CW / 0--	TSL Conductivity [S/m]	0.893
Conversion Factor	8.91	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2024-03-15	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1670 2024-05-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.988	0.992
psSAR10g [W/Kg]	0.653	0.668
Power Drift [dB]		0.01
Dist 3dB Peak [mm]		17.5
M2/M1 [%]		89.0

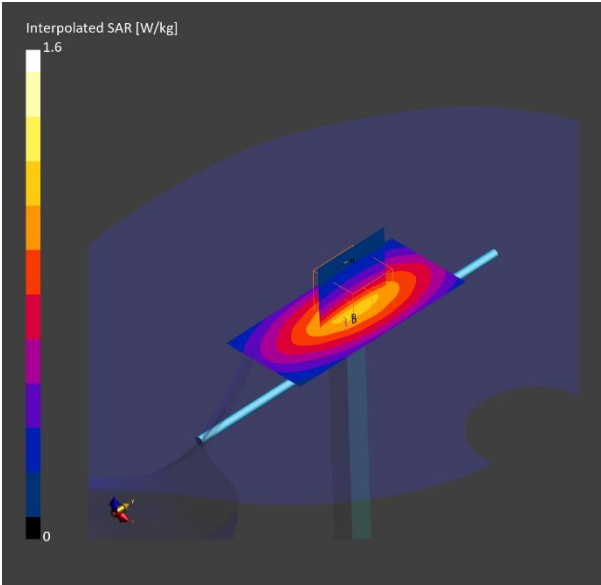

System Performance Check Report for D1750V2 - SN1125

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1750.0	TSL Permittivity	40.1
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.33
Conversion Factor	7.94	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2024-03-15	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1670 2024-05-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.39	3.74
psSAR10g [W/Kg]	1.87	2.04
Power Drift [dB]		0.06
Dist 3dB Peak [mm]		9.9
M2/M1 [%]		84.4

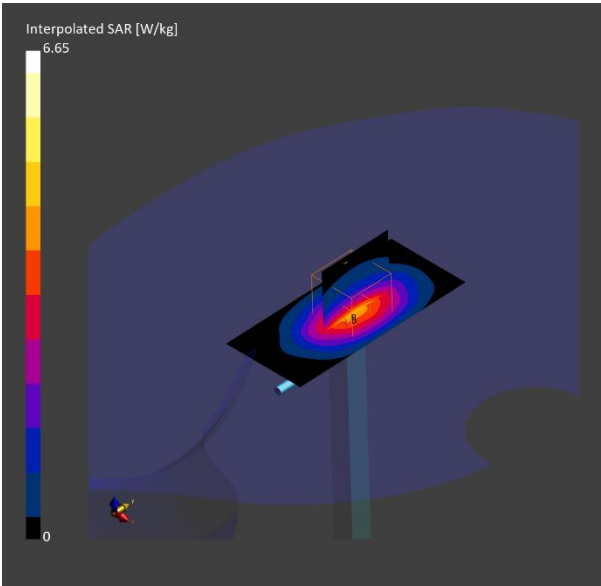

System Performance Check Report for D1900V2 - SN5d190

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1900.0	TSL Permittivity	40.0
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.42
Conversion Factor	7.61	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2024-03-15	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1670 2024-05-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.82	4.19
psSAR10g [W/Kg]	2.03	2.23
Power Drift [dB]		0.02
Dist 3dB Peak [mm]		9.6
M2/M1 [%]		84.5

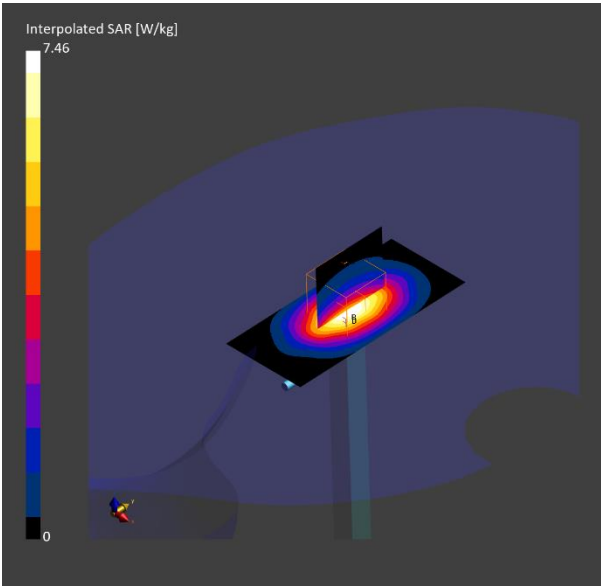

System Performance Check Report for D3500V2 - SN1075

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	3500.0	TSL Permittivity	37.7
Group / UID	CW / 0--	TSL Conductivity [S/m]	3.01
Conversion Factor	6.64	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7651 2024-03-18	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2024-07-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	28.0 x 28.0 x 28.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	6.19	6.46
psSAR10g [W/Kg]	2.43	2.60
Power Drift [dB]		0.01
Dist 3dB Peak [mm]		9.0
M2/M1 [%]		79.7

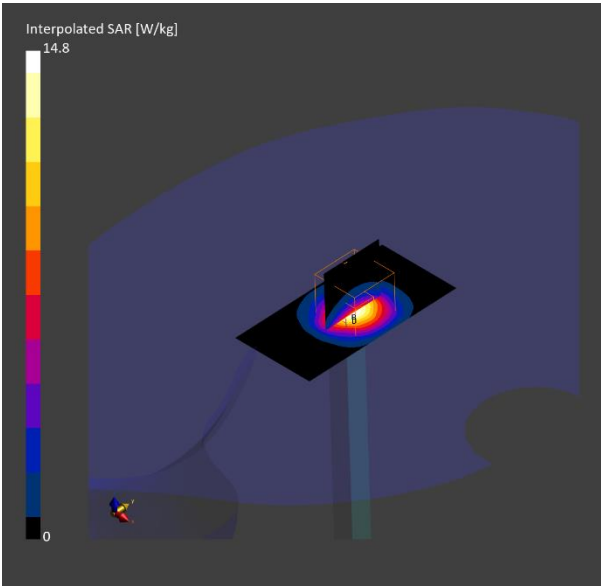

System Performance Check Report for D3700V2 - SN1036

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	3700.0	TSL Permittivity	37.4
Group / UID	CW / 0--	TSL Conductivity [S/m]	3.21
Conversion Factor	6.25	Phantom Section / TSL	Flat / HSL

DASY Configuration

Probe Calibration Date	EX3DV4 - SN7651 2024-03-18	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2024-07-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	28.0 x 28.0 x 28.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	6.47	6.70
psSAR10g [W/Kg]	2.46	2.63
Power Drift [dB]		0.01
Dist 3dB Peak [mm]		8.6
M2/M1 [%]		78.1

