
# **Appendix D**

# **Photographs**

- 1. SAR measurement System
- 2. Photographs of Tissue Simulate Liquid
- 3. Photographs of EUT test position
- 4. EUT Constructional Details

# 1. SAR measurement System

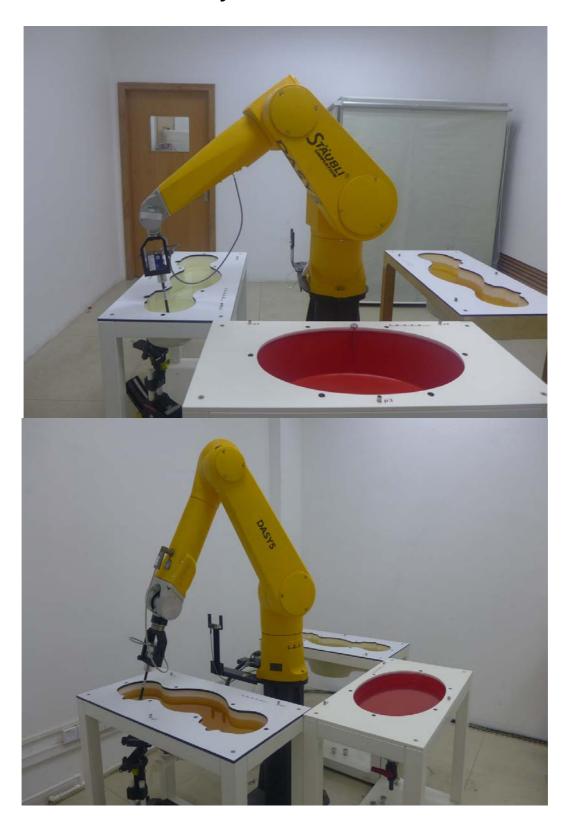

### 2. Photographs of Tissue Simulate Liquid


Photo 2: Tissue Simulant Liquid for Body 750 Photo 1: Tissue Simulant Liquid for Head 750 Photo 3: Tissue Simulant Liquid for Head 835 Photo 4: Tissue Simulant Liquid for Body 835 15cm Photo 5: Tissue Simulant Liquid for Head 1750 Photo 6: Tissue Simulant Liquid for Body 1750

Photo 7: Tissue Simulant Liquid for Head 1900

Photo 8: Tissue Simulant Liquid for Body 1900

Photo 9: Tissue Simulant Liquid for Head 2600

Photo 10: Tissue Simulant Liquid for Body 2600

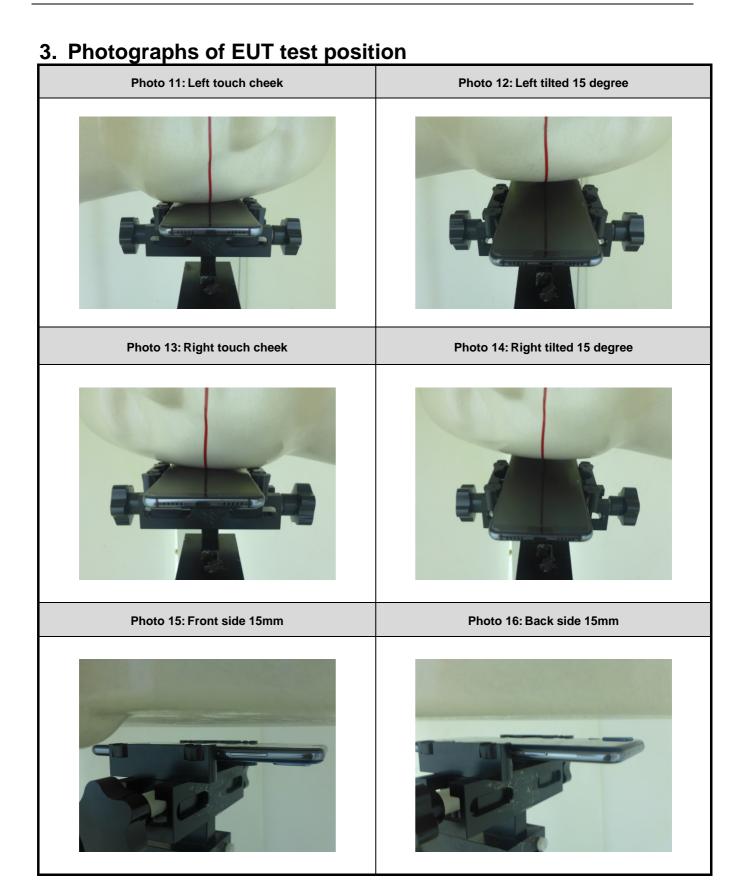


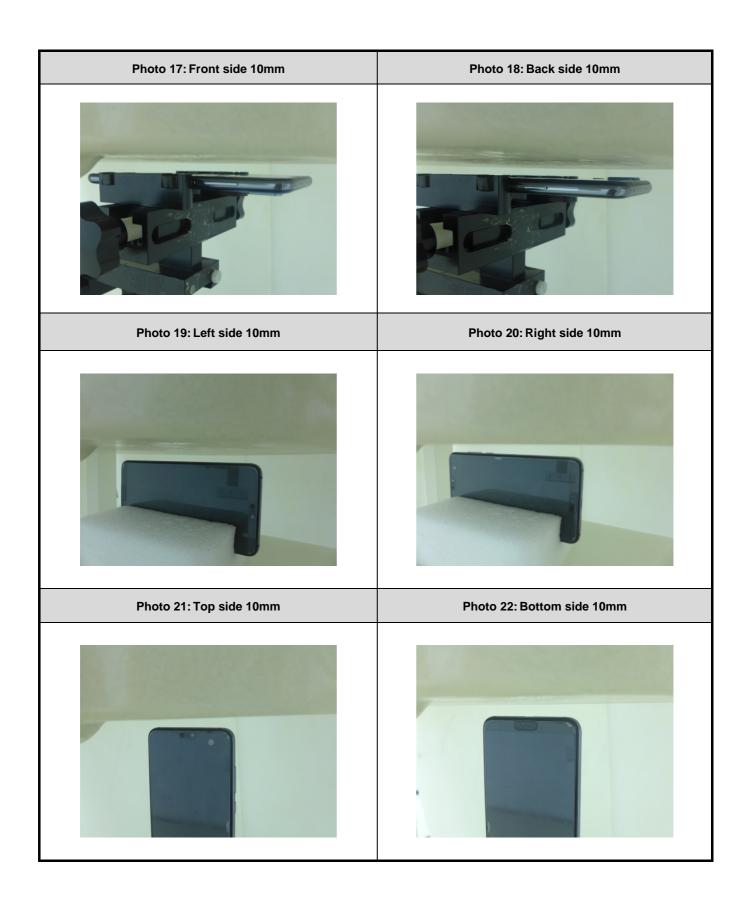


Photo 23: Front side 0mm Photo 24: Back side 0mm Photo 26: Right side 0mm Photo 25: Left side 0mm Photo 27: Top side 0mm Photo 28: Bottom side 0mm



### 4. EUT Constructional Details

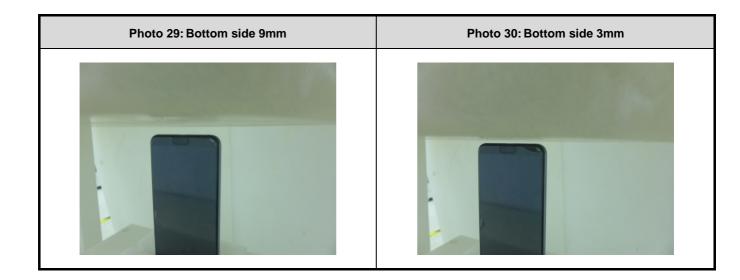