

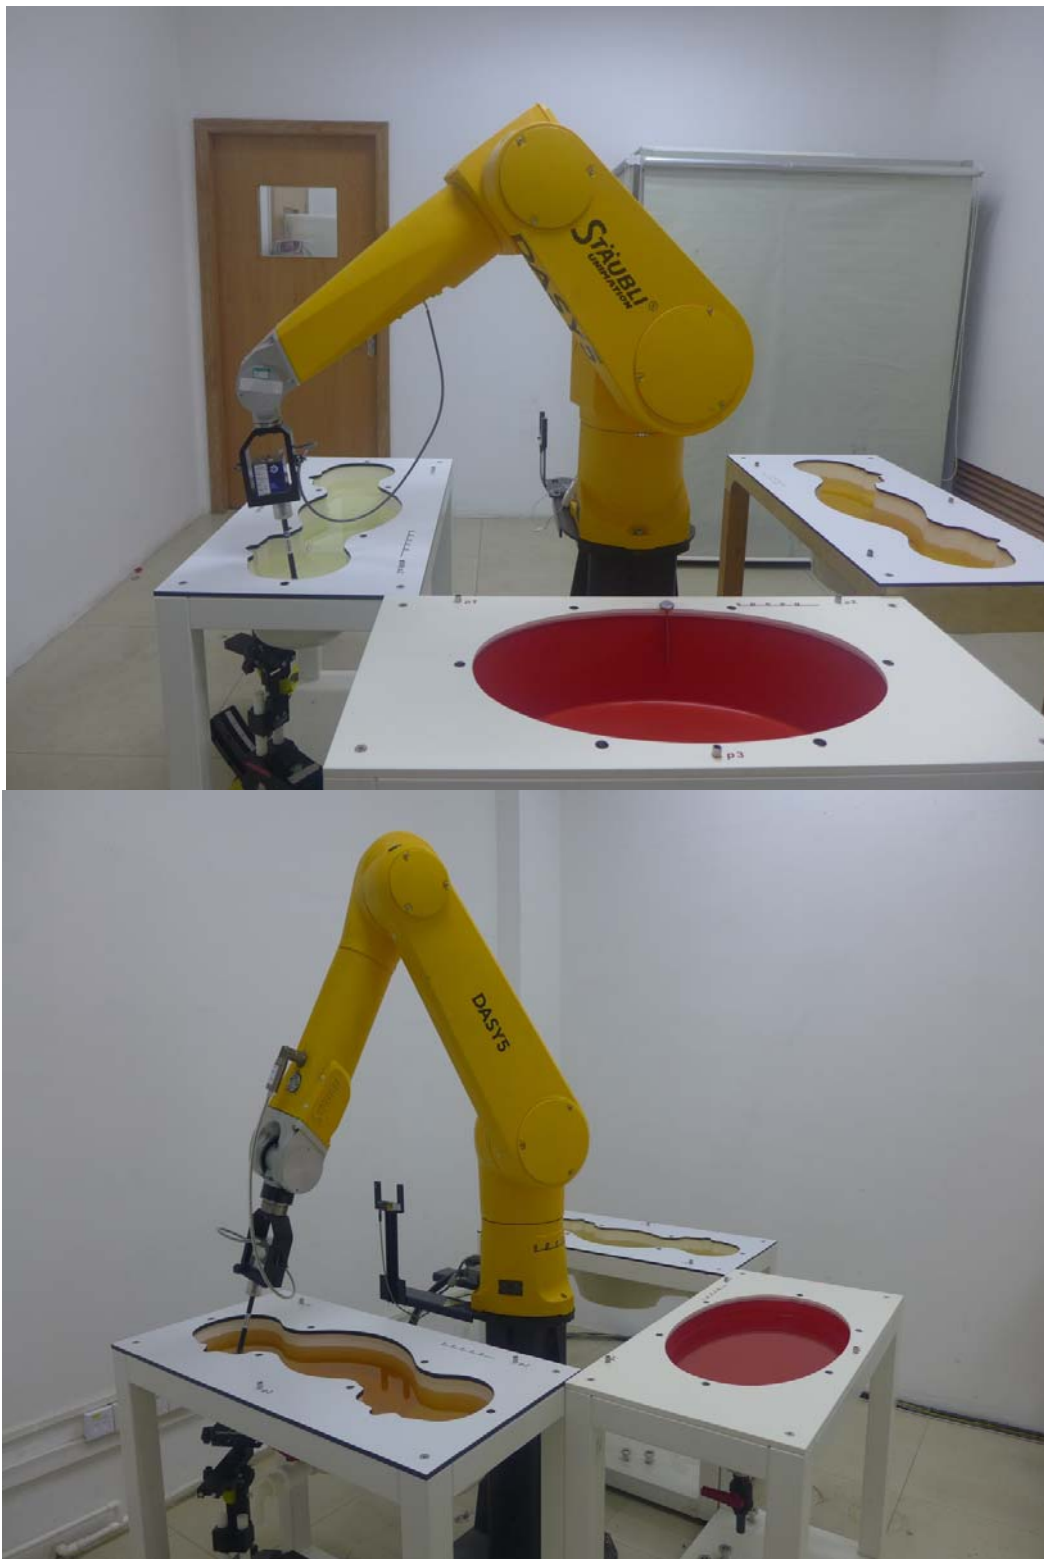


# **Appendix D**

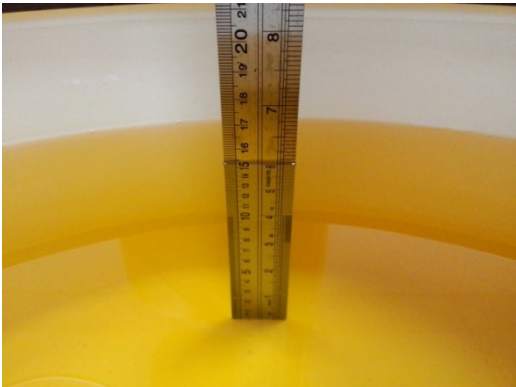
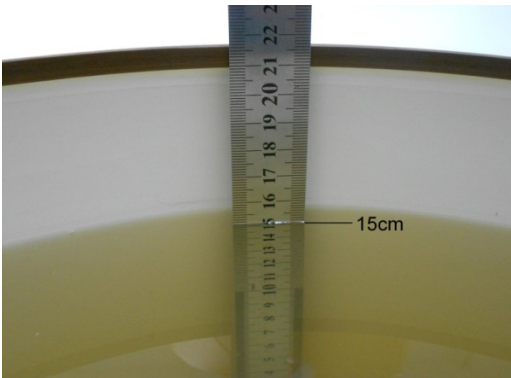
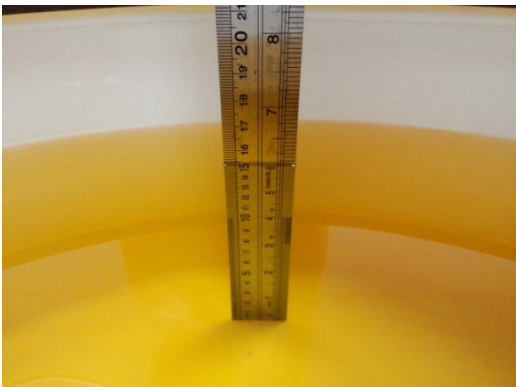


## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System



## 2. Photographs of Tissue Simulate Liquid

<p><b>Photo 1: Tissue Simulant Liquid for Head 750</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Head 835</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 1750</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Head 1900</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Head 2450</b></p>	<p><b>NA</b></p>
	<p><b>NA</b></p>

### 3. Photographs of EUT test position

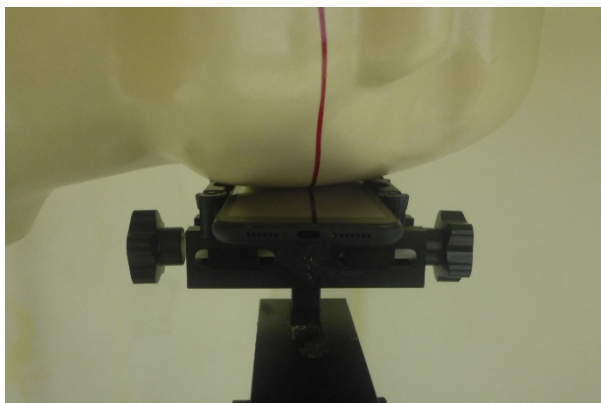
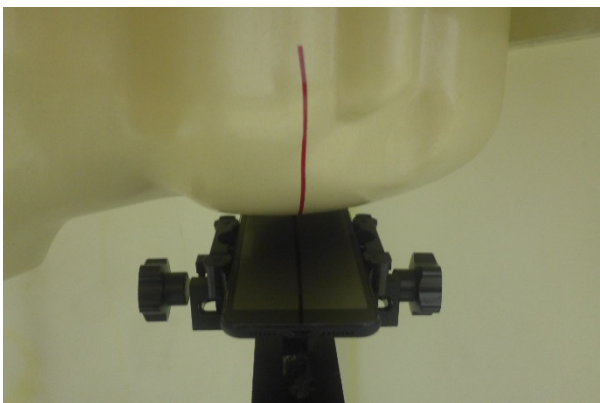
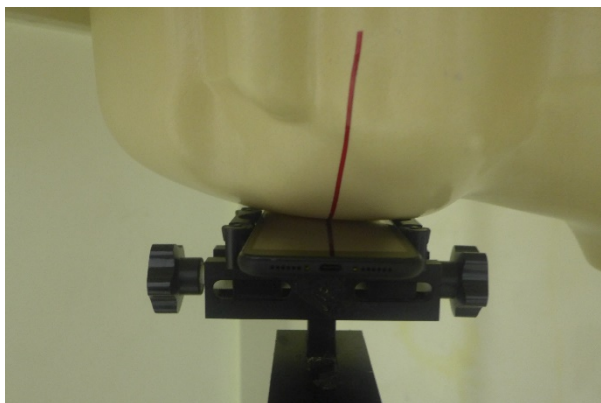
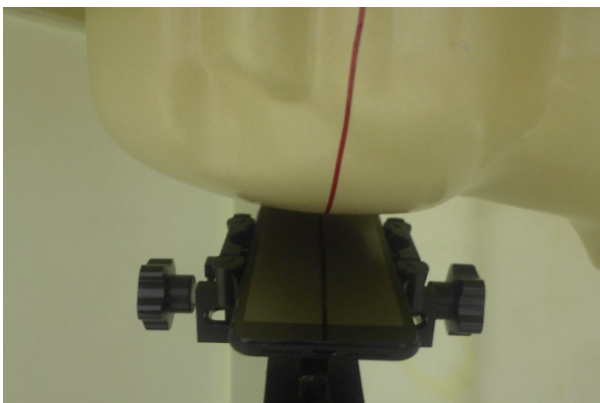








<p><b>Photo 6: Left touch cheek</b></p>	<p><b>Photo 7: Left tilted 15 degree</b></p>
	
<p><b>Photo 8: Right touch cheek</b></p>	<p><b>Photo 9: Right tilted 15 degree</b></p>
	
<p><b>Photo 10: Front side 15mm</b></p>	<p><b>Photo 11: Back side 15mm</b></p>
	



Photo 12: Front side 10mm	Photo 13: Back side 10mm
	
Photo 14: Left side 10mm	Photo 15: Right side 10mm
	
Photo 16: Top side 10mm	Photo 17: Bottom side 10mm
	

## 4. EUT Constructional Details

