




Appendix I

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

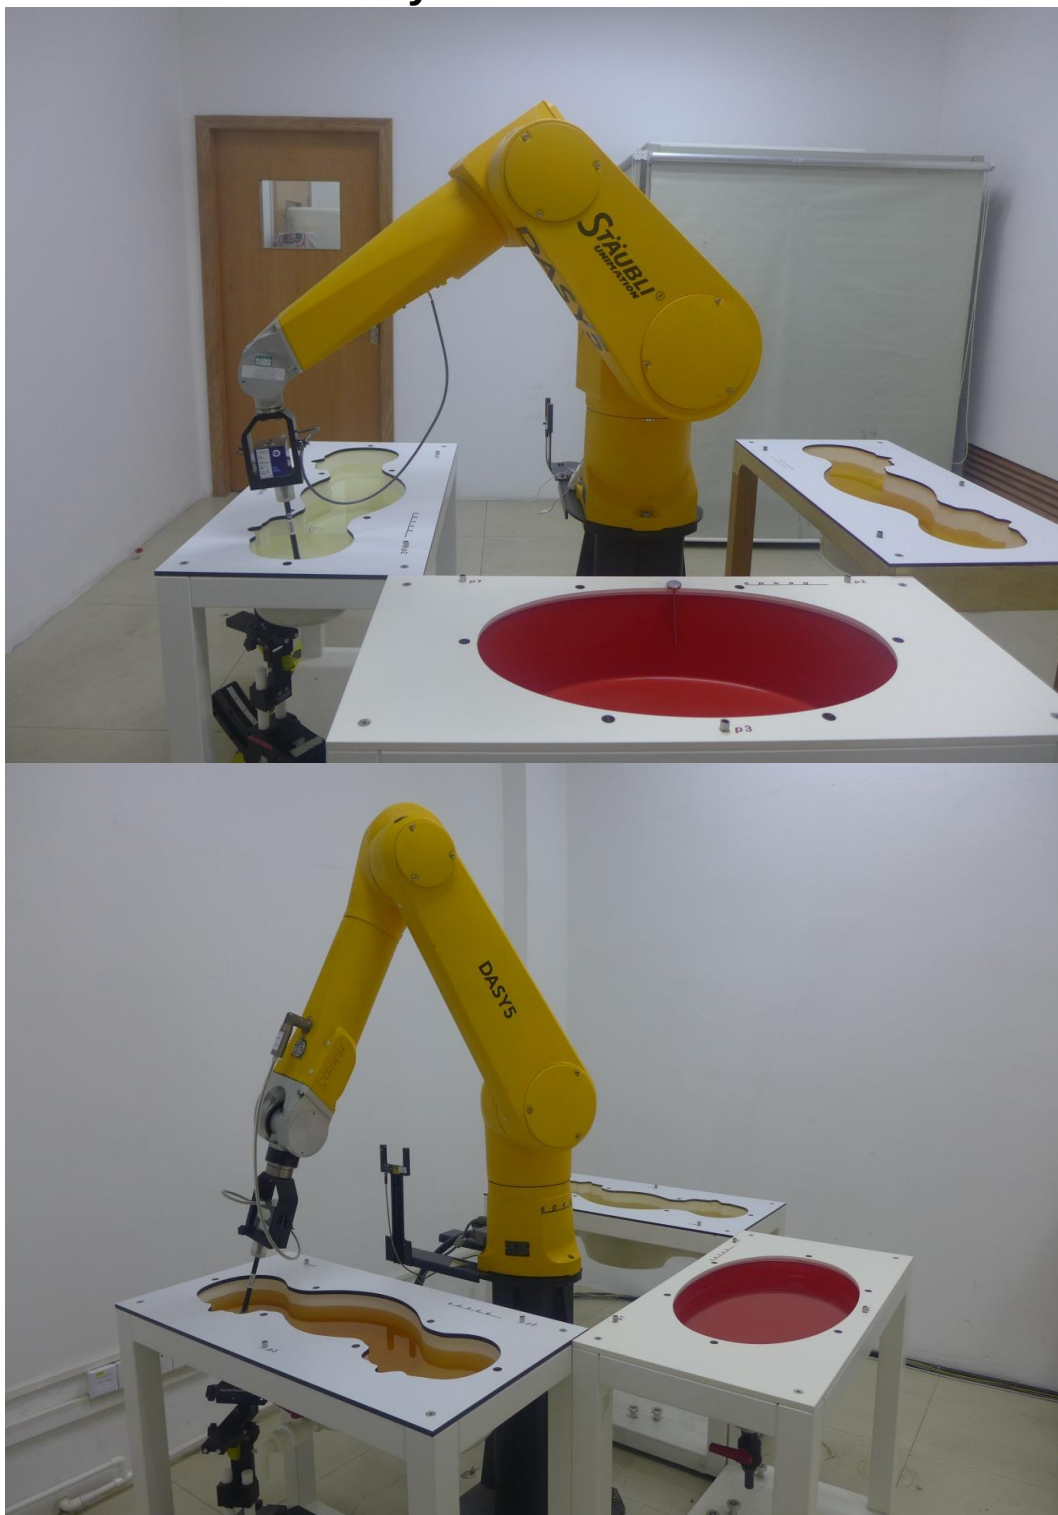

2. Photographs of Tissue Simulate Liquid

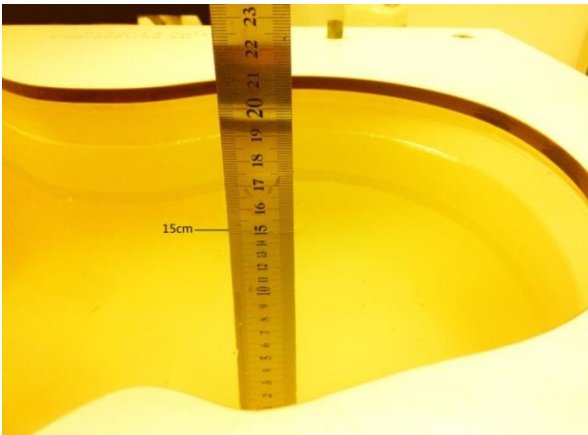
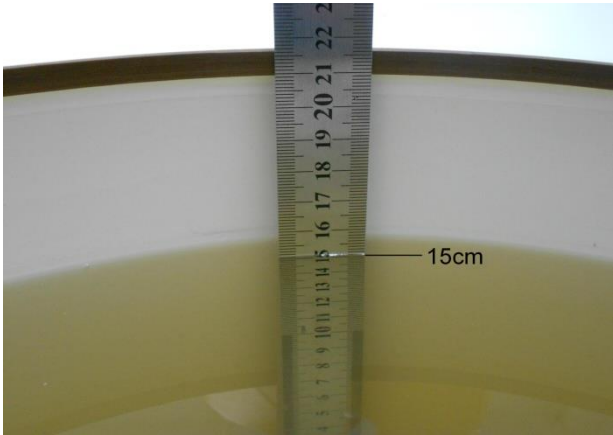
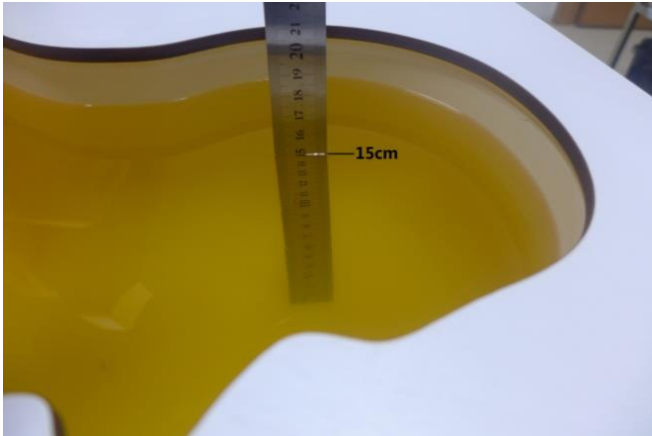
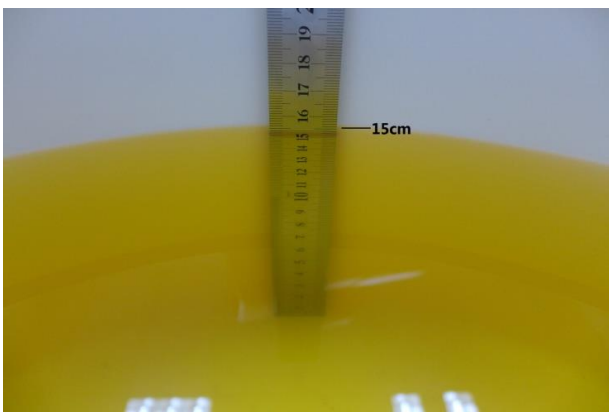
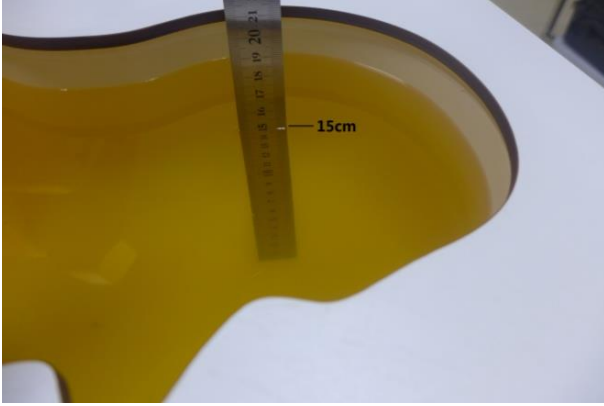
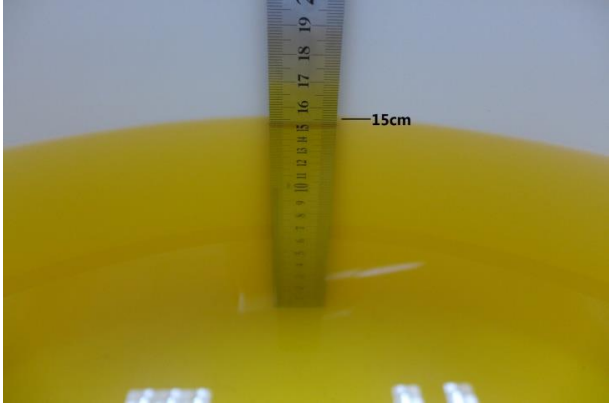
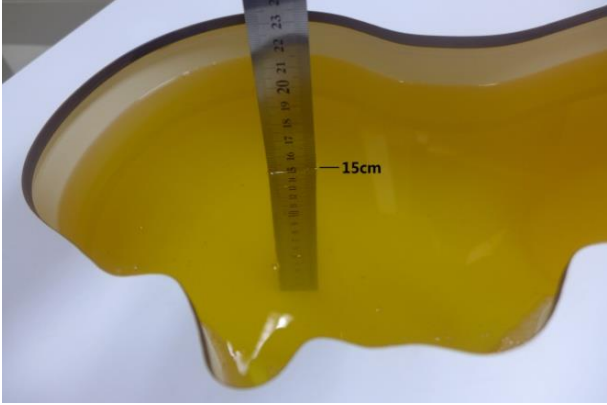
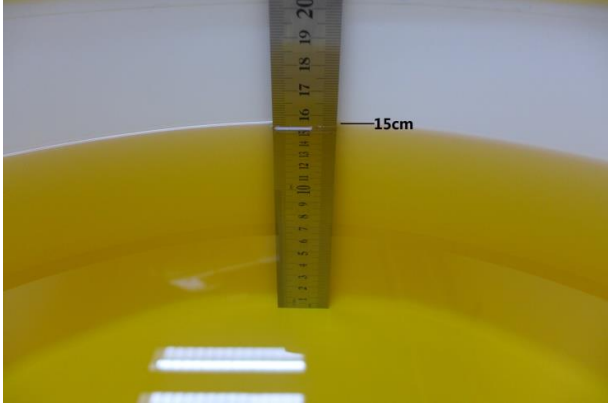
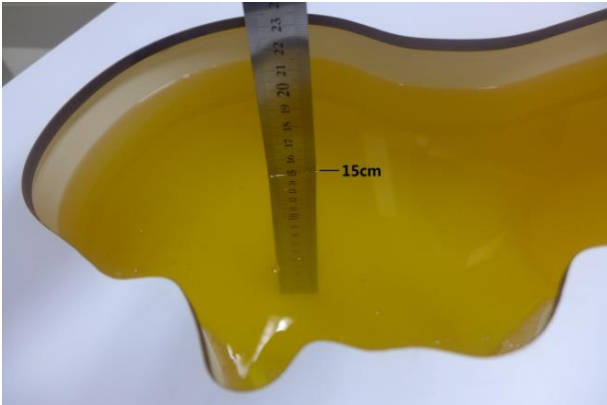
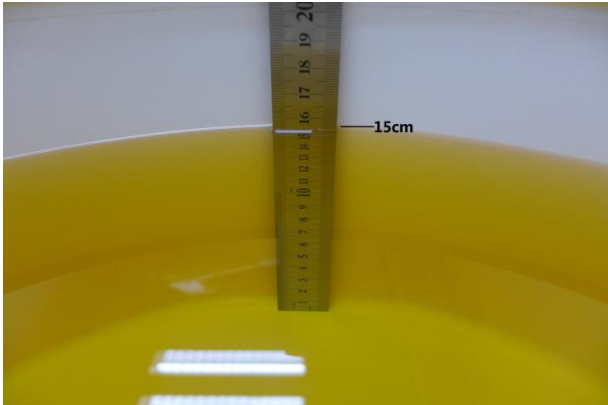
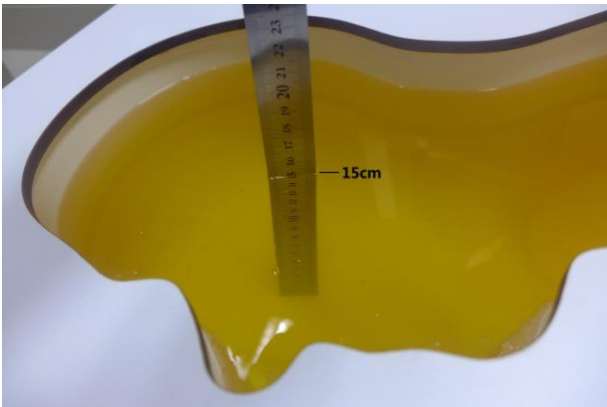
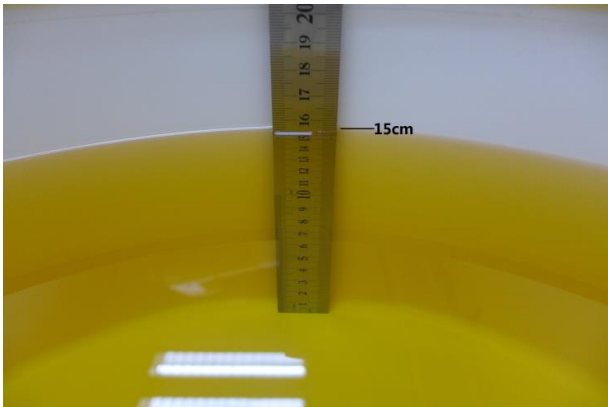
Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Body 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Body 1750
	
Photo 5: Tissue Simulant Liquid for Head 1900	Photo 6: Tissue Simulant Liquid for Body 1900
	

Photo 7: Tissue Simulant Liquid for Head 2300	Photo 8: Tissue Simulant Liquid for Body 2300
	
Photo 9: Tissue Simulant Liquid for Head 2450	Photo 10: Tissue Simulant Liquid for Body 2450
	
Photo 11: Tissue Simulant Liquid for Head 2600	Photo 12: Tissue Simulant Liquid for Body 2600
	

3. Photographs of EUT test position

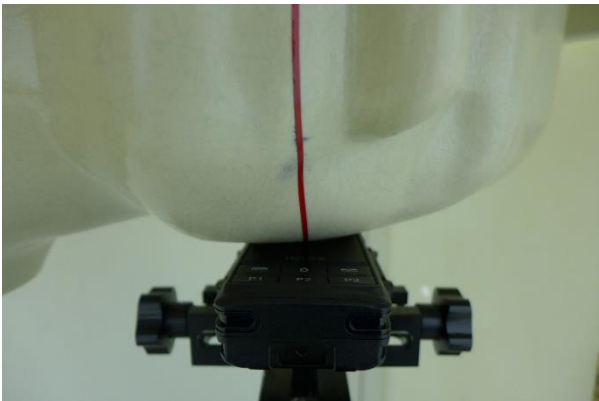
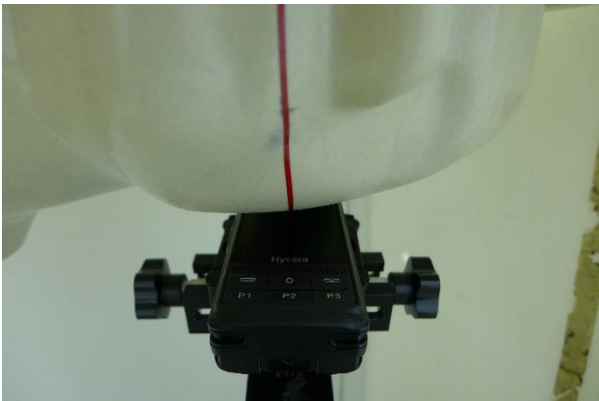
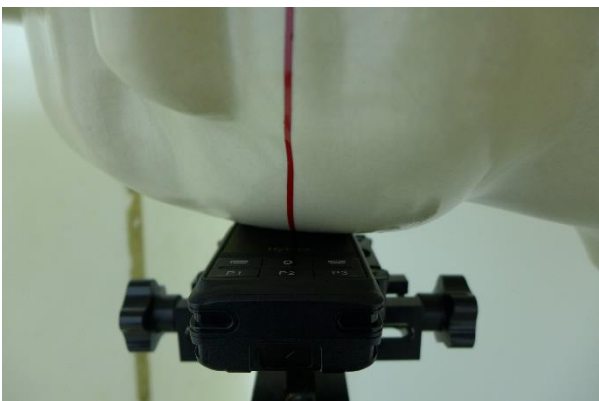
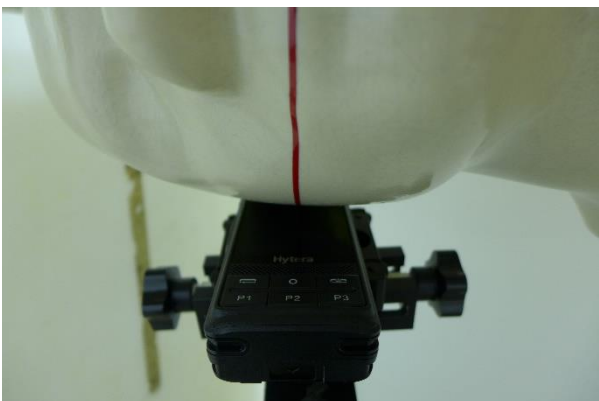
Photo 13: Left touch cheek	Photo 14: Left tilted 15 degree
	
Photo 15: Right touch cheek	Photo 16: Right tilted 15 degree
	
Photo 17: Front side 15mm	Photo 18: Back side 15mm
	



Photo 19: Front side 10mm	Photo 20: Back side 10mm
	
Photo 21: Left side 10mm	Photo 22: Right side 10mm
	
Photo 23: Top side 10mm	Photo 24: Bottom side 10mm
	



Photo 25: Back splint 0mm	NA
	NA

4. EUT Constructional Details

Photo 26: Front View	Photo 27: Back View
	
Photo 28: Accessory	NA
	NA