


Impedance Measurement Plot for Body TSL

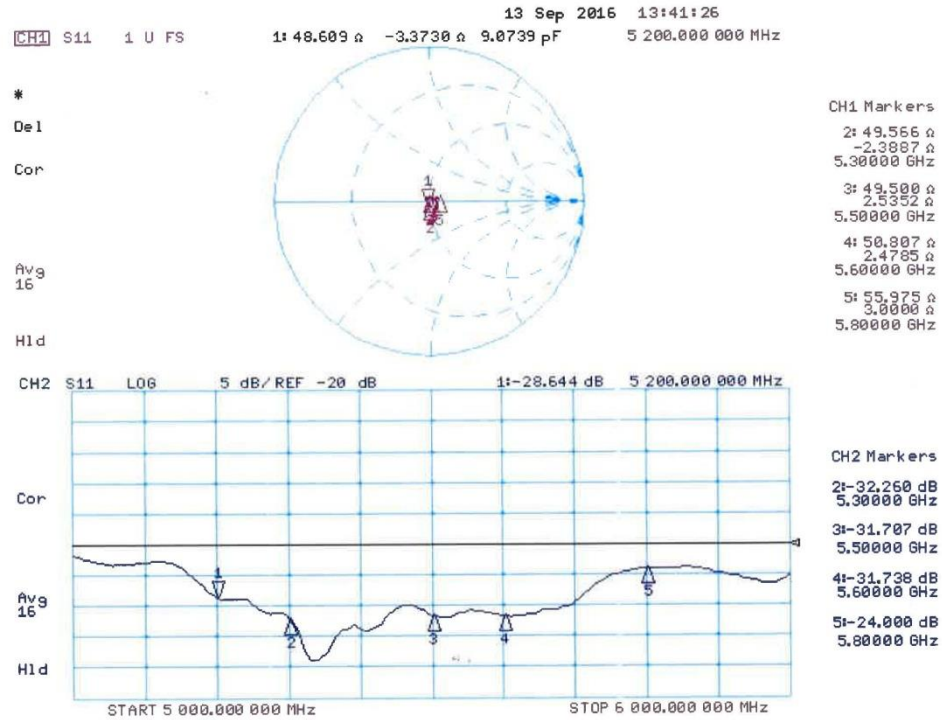

ANNEX K Extended Calibration SAR Dipole

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dBm, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole D750V3– serial no.1163

Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2016-09-19	-26.8	/	54.5	/	-1.8	/
2017-09-17	-25.4	5.2	53.2	1.3	-2.5	-0.7
2018-09-15	-24.9	7.6	52.7	1.8	-2.8	-1.0

Body						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2016-09-19	-29.0	/	49.8	/	-3.5	/
2017-09-17	-25.2	13.1	46.9	2.9	-2.8	0.7
2018-09-15	-24.4	15.9	45.5	4.3	-3.0	0.5

Justification of Extended Calibration SAR Dipole D1750V2– serial no.1152

Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2016-09-09	-42.9	/	50.5	/	-0.5	/
2017-09-08	-40.6	5.4	48.8	1.7	-0.4	0.1
2018-09-06	-38.7	9.8	46.5	4.0	-0.3	0.2

Body						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2016-09-09	-27.6	/	46.3	/	-1.6	/
2017-09-08	-25.8	6.5	45.4	0.9	-1.4	0.2
2018-09-06	-24.6	10.9	44.7	1.6	-1.2	0.4

Justification of Extended Calibration SAR Dipole D5GHzV2– serial no.1238

Head							
Date of Measurement	Frequency	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2016-09-21	5200MHz	-23.6	/	47.1	/	5.80	/
2017-09-20		-21.7	8.1	48.3	1.2	3.38	2.42
2018-09-18		-21.2	10.2	48.7	1.6	3.25	2.55
2016-09-21	5300MHz	-29.8	/	50.5	/	3.20	/
2017-09-20		-27.8	6.7	51.9	1.4	4.51	1.31
2018-09-18		-26.2	12.1	53.3	2.8	4.82	1.62
2016-09-21	5500MHz	-31.2	/	49.0	/	2.50	/
2017-09-20		-29.5	5.4	50.3	1.3	1.24	1.26
2018-09-18		-28.1	9.9	51.4	2.4	1.55	0.95
2016-09-21	5600MHz	-44.1	/	50.0	/	0.60	/
2017-09-20		-42.6	3.4	51.5	1.5	2.55	1.95
2018-09-18		-40.5	8.2	53.3	3.3	3.01	2.41
2016-09-21	5800MHz	-25.1	/	55.6	/	1.90	/
2017-09-20		-23.8	5.2	56.9	1.3	3.04	1.14
2018-09-18		-22.7	9.6	57.3	1.7	2.88	0.98

Body							
Date of Measurement	Frequency	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2016-09-21	5200MHz	-28.6	/	48.6	/	3.40	/
2017-09-20		-26.4	7.7	50.0	1.4	3.72	0.32
2018-09-18		-24.6	14.0	51.2	2.6	3.85	0.45
2016-09-21	5300MHz	-32.3	/	49.6	/	2.40	/
2017-09-20		-30.5	5.6	51.3	1.7	3.64	1.24
2018-09-18		-28.9	10.5	52.6	3.0	3.77	1.37
2016-09-21	5500MHz	-31.7	/	49.5	/	2.50	/
2017-09-20		-29.8	6.0	51.4	1.9	4.25	1.75
2018-09-18		-27.5	13.2	52.8	3.3	4.44	1.94
2016-09-21	5600MHz	-31.7	/	50.8	/	2.50	/
2017-09-20		-29.5	6.9	52.3	1.5	2.91	0.41
2018-09-18		-28.6	9.8	52.9	2.1	3.03	0.53
2016-09-21	5800MHz	-24.0	/	56.0	/	3.00	/
2017-09-20		-22.8	5.0	57.3	1.3	4.23	1.23
2018-09-18		-21.5	10.4	57.8	1.6	4.46	1.46

The Return-Loss is <-20dB, and within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the value result should support extended c.