

## System Check\_Head\_750MHz

**DUT: D750V3 - SN:1087**

Communication System: ; Frequency: 750.0

Medium: HSL. Medium parameters used:  $f = 750.0$  MHz;  $\sigma = 0.890$  S/m;  $\epsilon_r = 42.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(8.92, 7.91, 9.02); Calibrated: 2023-07-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.396 W/kg; SAR (10g) = 0.265 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.01 dB

SAR (1g) = 0.395 W/kg; SAR (10g) = 0.260 W/kg;

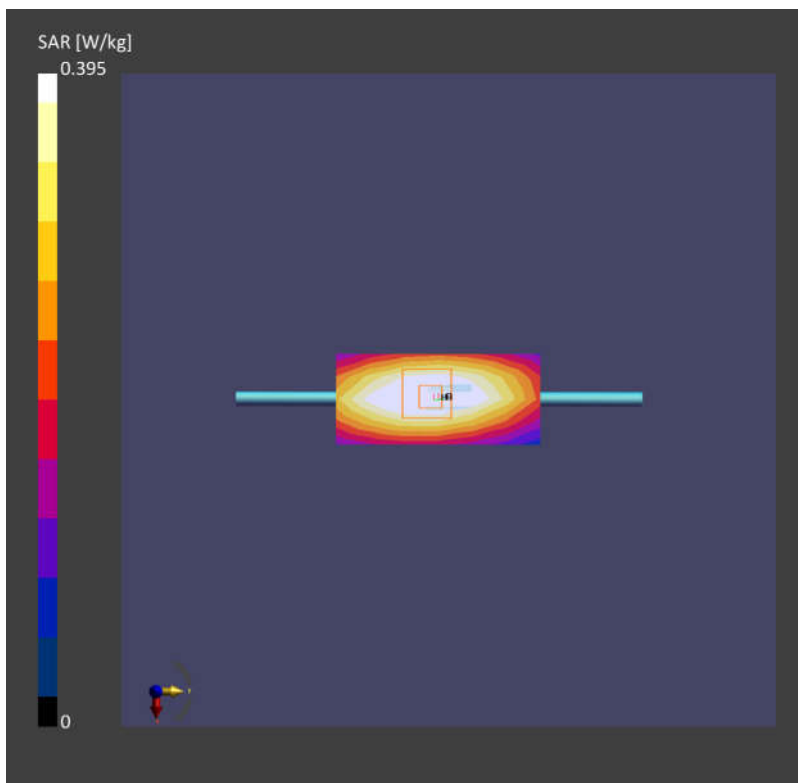

## System Check\_Head\_1750MHz

**DUT: D1750V2 - SN:1090**

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used:  $f = 1750.0$  MHz;  $\sigma = 1.32$  S/m;  $\epsilon_r = 40.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(7.86, 7.19, 7.8); Calibrated: 2023-07-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.66 W/kg; SAR (10g) = 0.933 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.08 dB

SAR (1g) = 1.79 W/kg; SAR (10g) = 0.942 W/kg;

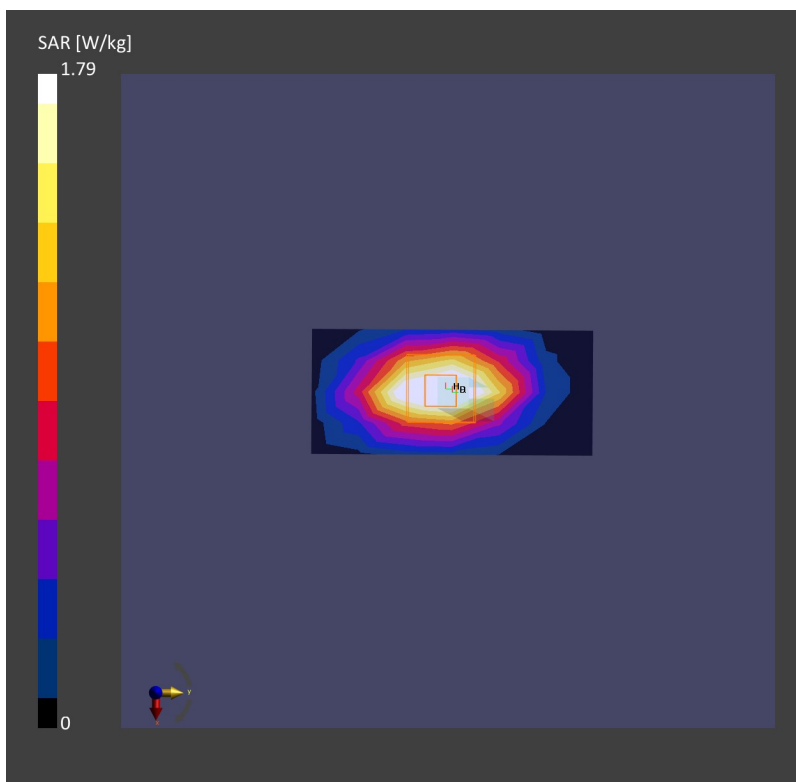

## System Check\_Head\_1900MHz

**DUT: D1900V2 - SN:5d118**

Communication System: ; Frequency: 1900.0

Medium: HSL. Medium parameters used:  $f = 1900.0$  MHz;  $\sigma = 1.40$  S/m;  $\epsilon_r = 40.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7774; ConvF(7.41, 6.68, 7.32); Calibrated: 2023-07-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2022-12-12
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2151
- Measurement Software: cDASY6 V6.6.0.13926

**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.88 W/kg; SAR (10g) = 0.977 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.02 dB

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.984 W/kg;

