

APPENDIX C - PROBE CALIBRATION

Probe ET3DV6

SN:1590

Manufactured:	March 19, 2001
Calibrated:	March 26, 2001

Calibrated for System DASY3

DASY3 - Parameters of Probe: ET3DV6 SN:1590

Sensitivity in Free Space

NormX	1.77 $\mu\text{V}/(\text{V}/\text{m})^2$
NormY	1.91 $\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	1.67 $\mu\text{V}/(\text{V}/\text{m})^2$

Diode Compression

DCP X	100 mV
DCP Y	100 mV
DCP Z	100 mV

Sensitivity in Tissue Simulating Liquid

Head **450 MHz** $\epsilon_r = 43.5 \pm 5\%$ $s = 0.87 \pm 10\% \text{ mho/m}$

ConvF X	7.36 extrapolated	Boundary effect:	
ConvF Y	7.36 extrapolated	Alpha	0.29
ConvF Z	7.36 extrapolated	Depth	2.72

Head **900 MHz** $\epsilon_r = 42 \pm 5\%$ $s = 0.97 \pm 10\% \text{ mho/m}$

ConvF X	6.83 $\pm 7\%$ (k=2)	Boundary effect:	
ConvF Y	6.83 $\pm 7\%$ (k=2)	Alpha	0.37
ConvF Z	6.83 $\pm 7\%$ (k=2)	Depth	2.48

Head **1500 MHz** $\epsilon_r = 40.4 \pm 5\%$ $s = 1.23 \pm 10\% \text{ mho/m}$

ConvF X	6.13 interpolated	Boundary effect:	
ConvF Y	6.13 interpolated	Alpha	0.47
ConvF Z	6.13 interpolated	Depth	2.17


Head **1800 MHz** $\epsilon_r = 40 \pm 5\%$ $s = 1.40 \pm 10\% \text{ mho/m}$


ConvF X	5.78 $\pm 7\%$ (k=2)	Boundary effect:	
ConvF Y	5.78 $\pm 7\%$ (k=2)	Alpha	0.53
ConvF Z	5.78 $\pm 7\%$ (k=2)	Depth	2.01

Sensor Offset


Probe Tip to Sensor Center	2.7	mm
Optical Surface Detection	1.2 $\pm$ 0.2	mm

Receiving Pattern (f) , q = 0°

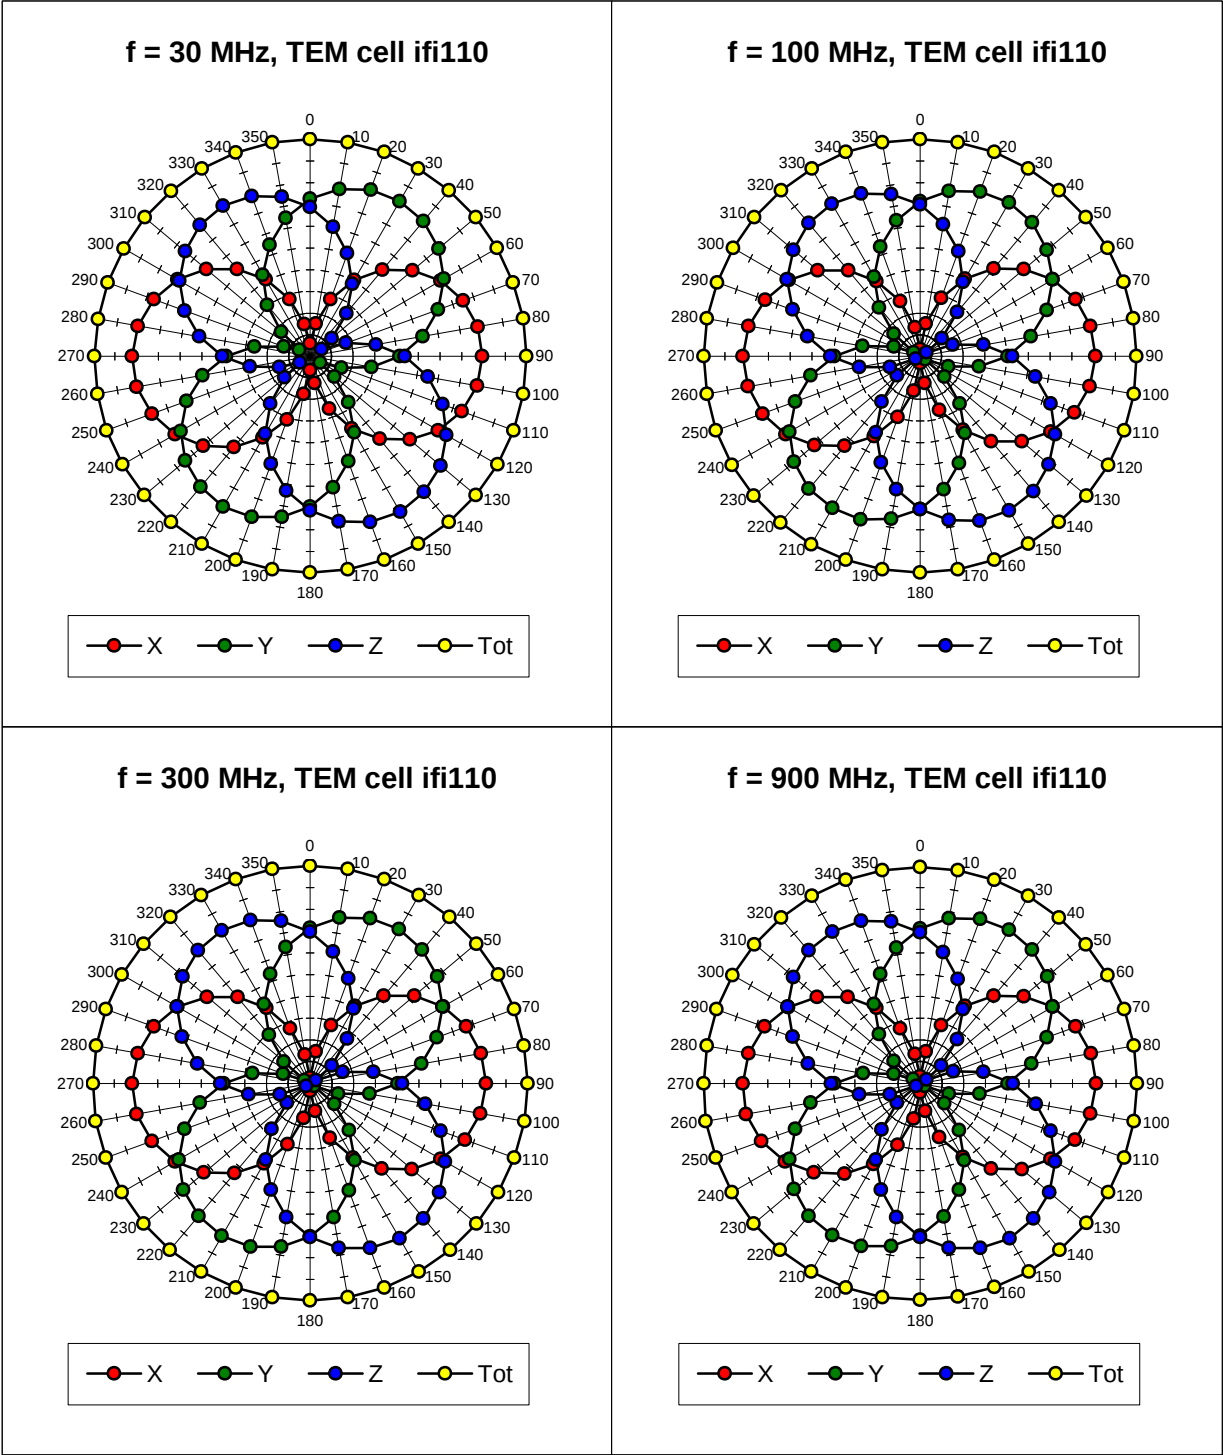

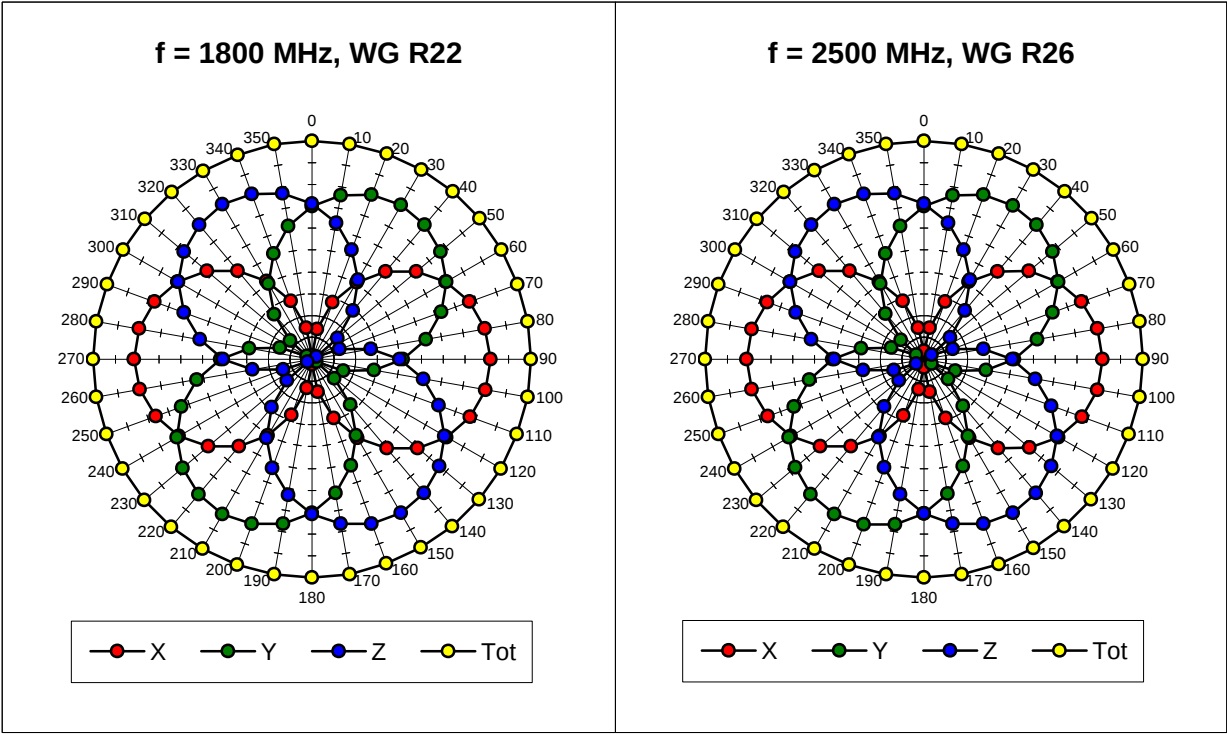


Isotropy Error (f), q = 0°


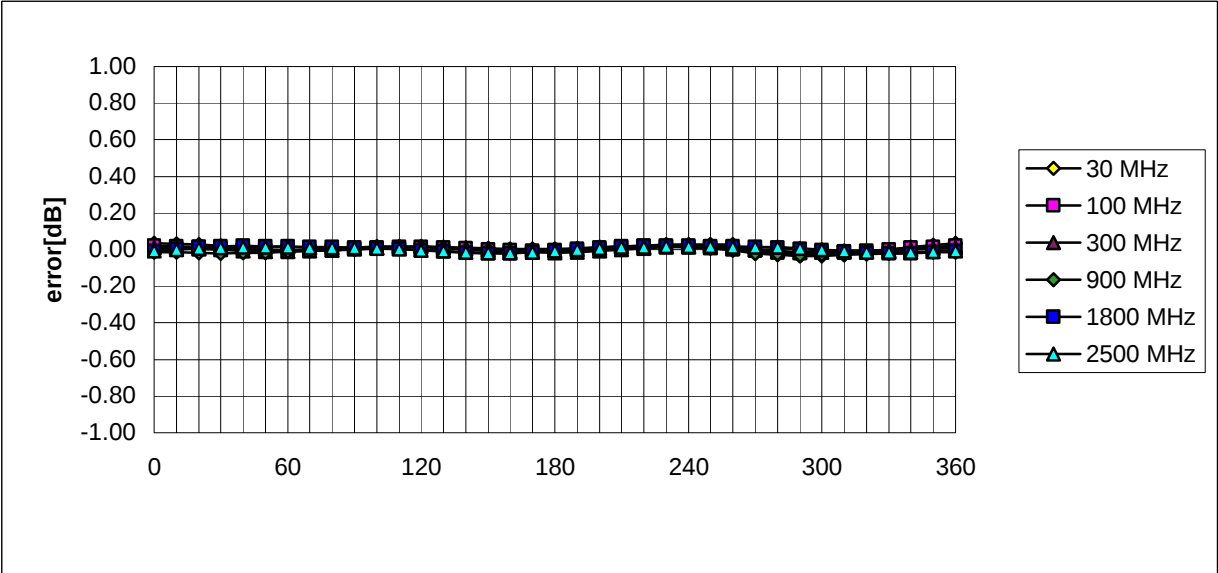


Frequency Response of E-Field


(TEM-Cell:ifi110, Waveguide R22)

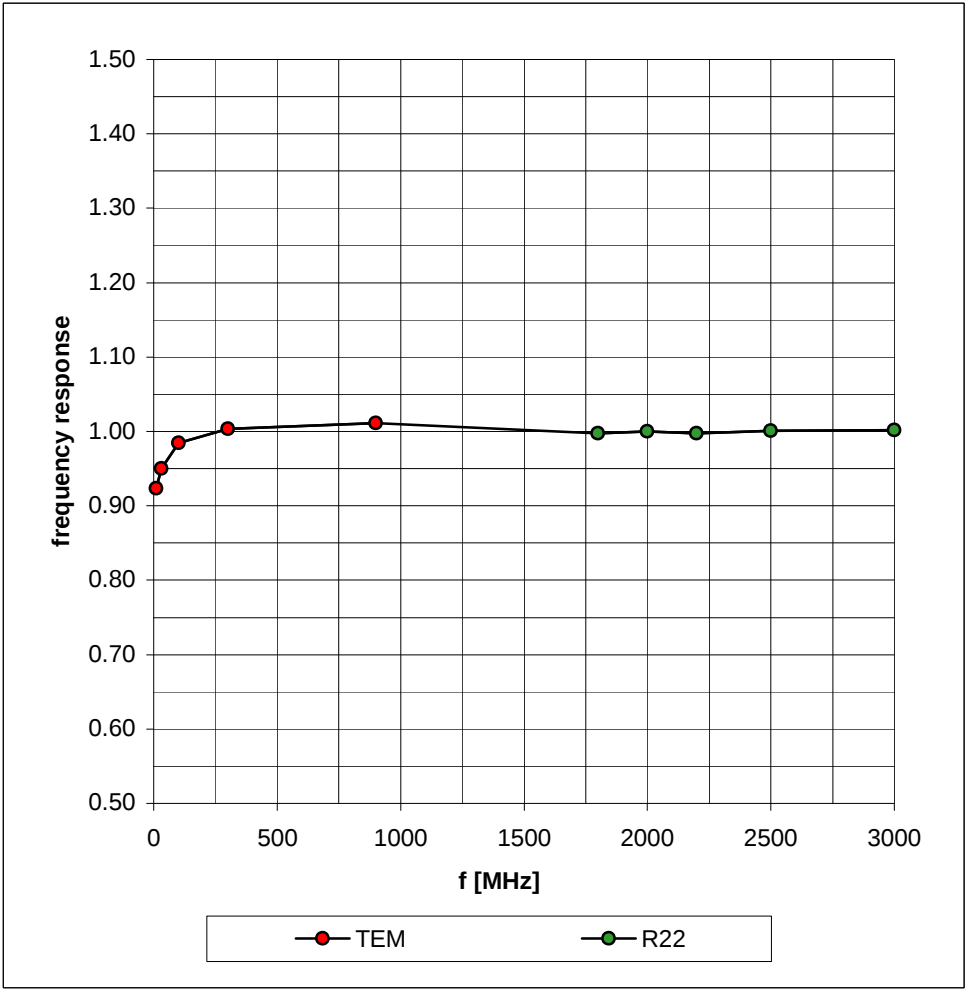

Dynamic Range f(SAR_{brain})
(TEM-Cell:ifi110)

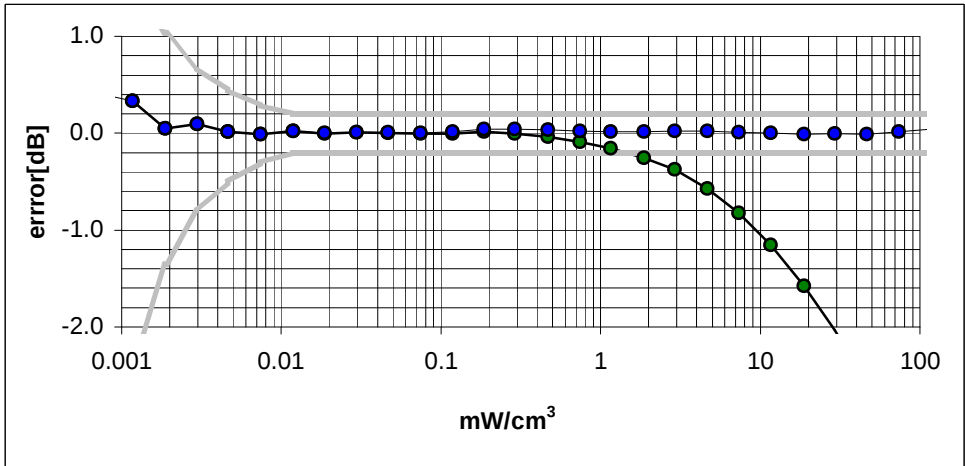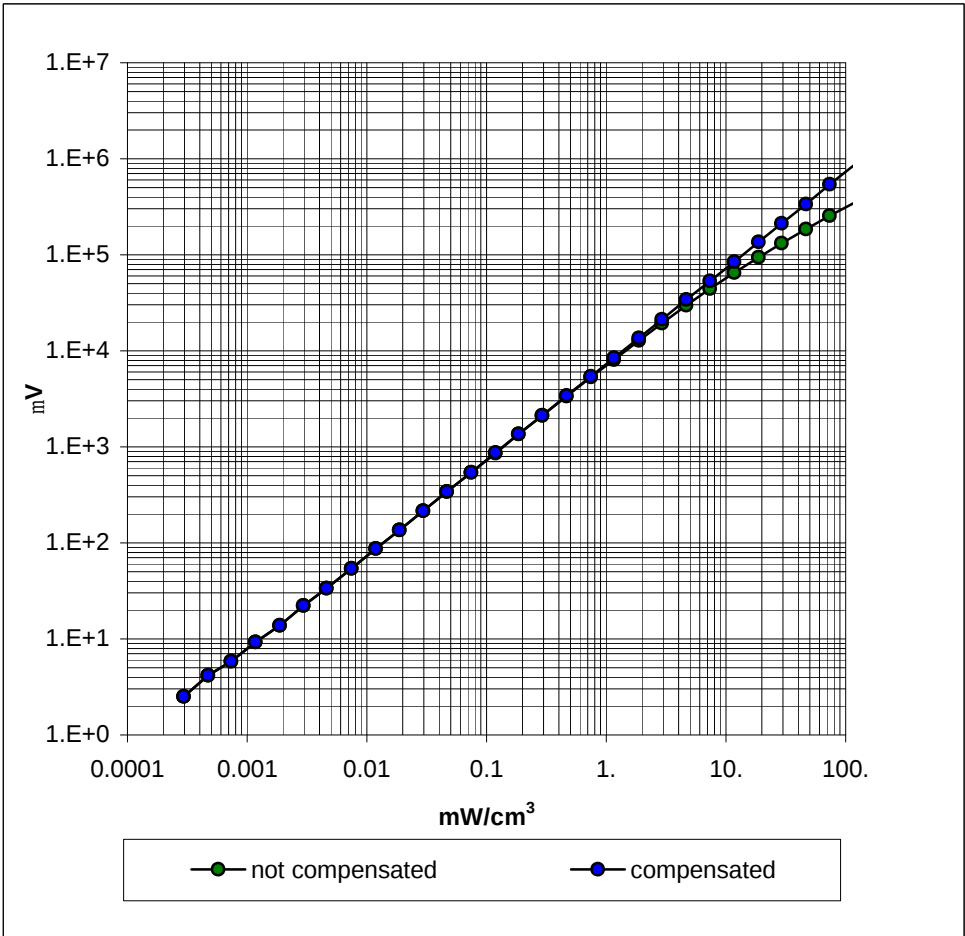

Conversion Factor Assessment

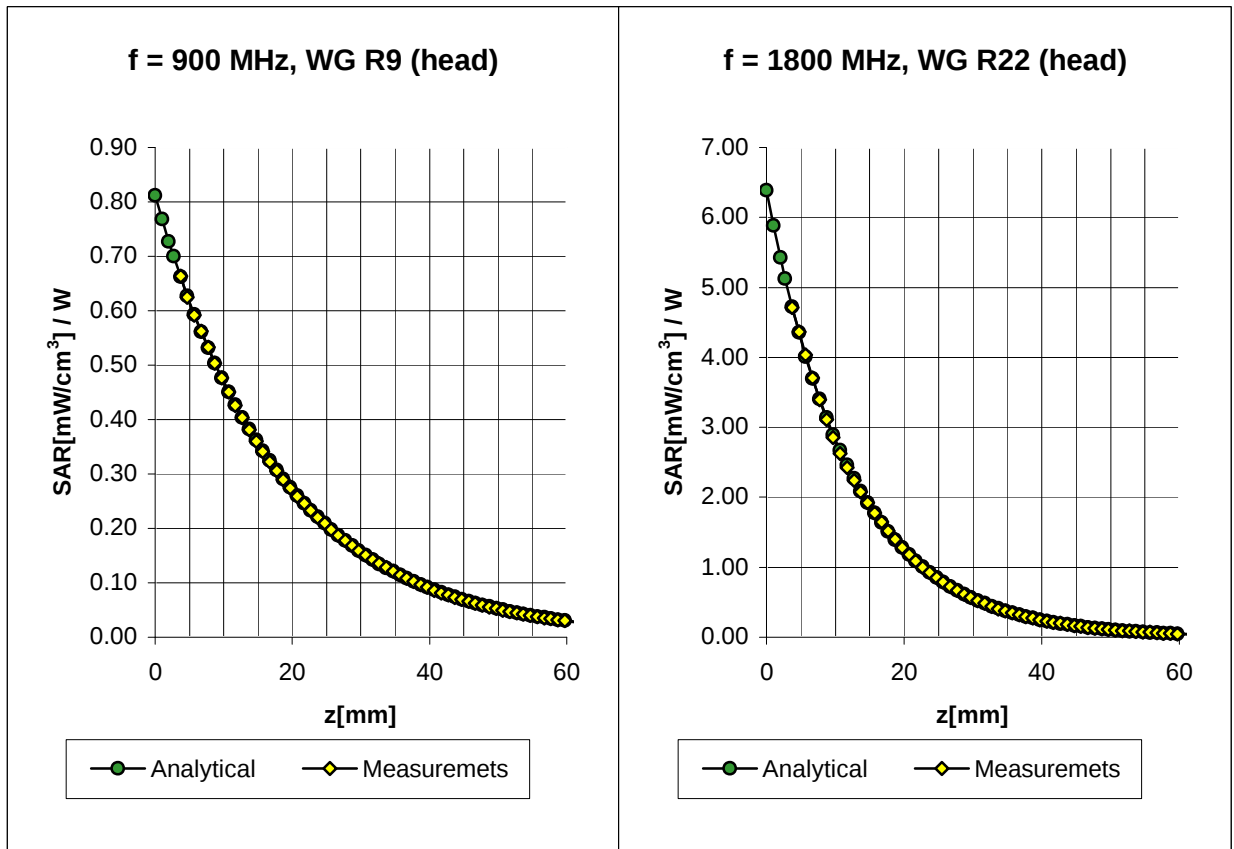


Head	900 MHz	$\epsilon_r = 42 \pm 5\%$	$s = 0.97 \pm 10\% \text{ mho/m}$
	ConvF X	6.83 $\pm 7\%$ (k=2)	Boundary effect:
	ConvF Y	6.83 $\pm 7\%$ (k=2)	Alpha 0.37
	ConvF Z	6.83 $\pm 7\%$ (k=2)	Depth 2.48
Head	1800 MHz	$\epsilon_r = 40 \pm 5\%$	$s = 1.40 \pm 10\% \text{ mho/m}$
	ConvF X	5.78 $\pm 7\%$ (k=2)	Boundary effect:
	ConvF Y	5.78 $\pm 7\%$ (k=2)	Alpha 0.53
	ConvF Z	5.78 $\pm 7\%$ (k=2)	Depth 2.01

ET3DV6 SN:1590

Deviation from Isotropy in HSL

Error (qf), f = 900 MHz

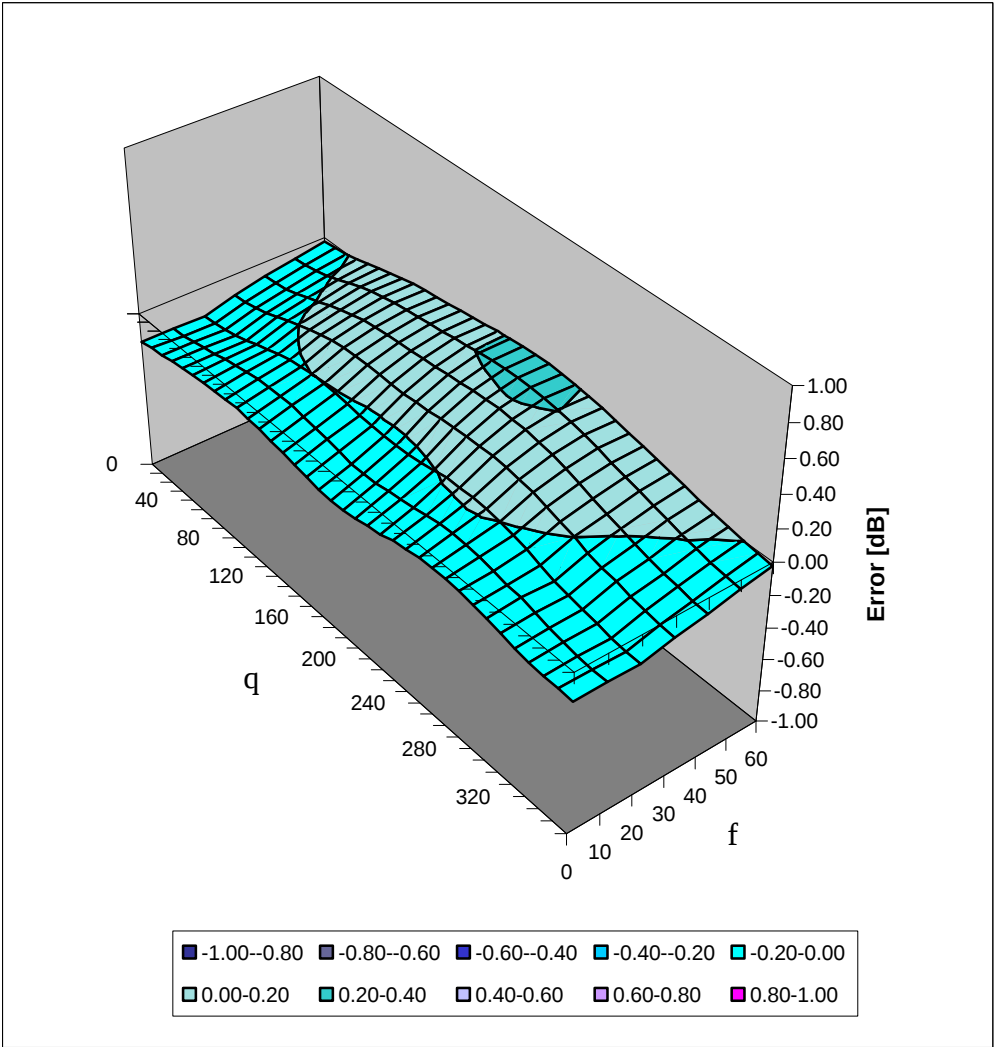

APPENDIX D - SAR TEST SETUP PHOTOGRAPHS


HAND & BODY SAR TEST SETUP PHOTOGRAPHS
Front of Handheld PC with 0.0cm Separation Distance



HAND SAR TEST SETUP PHOTOGRAPHS
Back of Handheld PC with 0.0cm Separation Distance



BODY SAR TEST SETUP PHOTOGRAPHS
Back of Handheld PC with 0.5cm Separation Distance

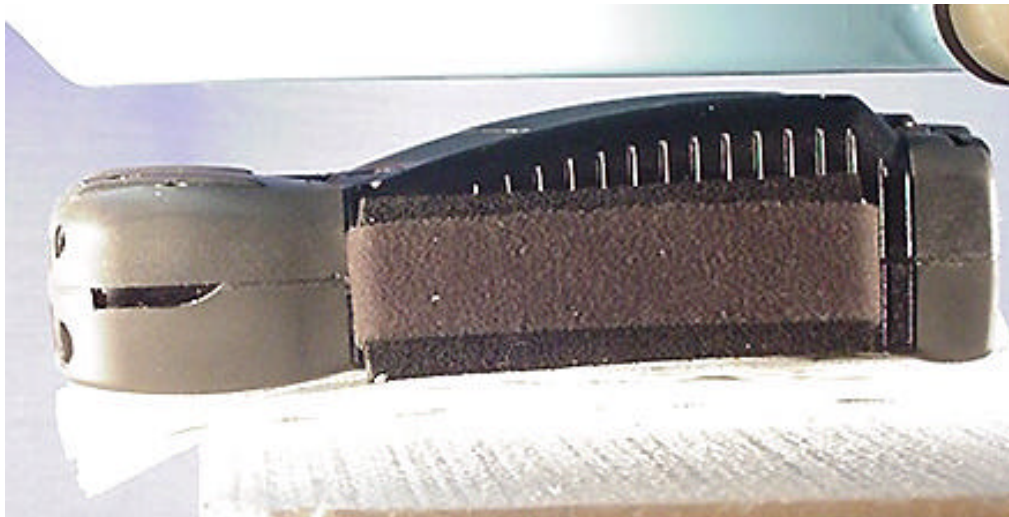

HAND & BODY SAR TEST SETUP PHOTOGRAPHS
Left Side of Handheld PC with 0.0cm Separation Distance
(permanent hand-strap touching phantom surface)



HAND & BODY SAR TEST SETUP PHOTOGRAPHS
Right Side of Handheld PC with 0.0cm Separation Distance

