

Appendix A

Detailed System Check Results

1. System Performance Check
System Performance Check 13 MHz Head
System Performance Check 835 MHz Head
System Performance Check 1750 MHz Head
System Performance Check 1900 MHz Head
System Performance Check 2450 MHz Head
System Performance Check 2600 MHz Head
System Performance Check 3500 MHz Head
System Performance Check 3700 MHz Head
System Performance Check 3900 MHz Head
System Performance Check 5250 MHz Head
System Performance Check 5600 MHz Head
System Performance Check 5750 MHz Head

Test Laboratory: SGS-SAR Lab

System Check_Head_13MHz

DUT: CLA-13; Type: CLA-13; Serial: 1032

Communication System: UID 0, CW (0); Frequency: 13 MHz; Duty Cycle: 1:1

Medium: HSL_13; Medium parameters used: $f = 13 \text{ MHz}$; $\sigma = 0.736 \text{ S/m}$; $\epsilon_r = 54.1$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN3793; ConvF(15.3, 15.3, 15.3); Calibrated: 2022-09-30
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1324; Calibrated: 2022-10-17
- Phantom: SAR 8-2; Type: EL4; Serial: TP:1143
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Configuration/Pin=250mW/Area Scan (8x8x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$
Maximum value of SAR (measured) = 0.153 W/kg


Configuration/Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 15.11 V/m ; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 0.202 W/kg

SAR(1 g) = 0.114 W/kg ; SAR(10 g) = 0.072 W/kg

Maximum value of SAR (measured) = 0.165 W/kg

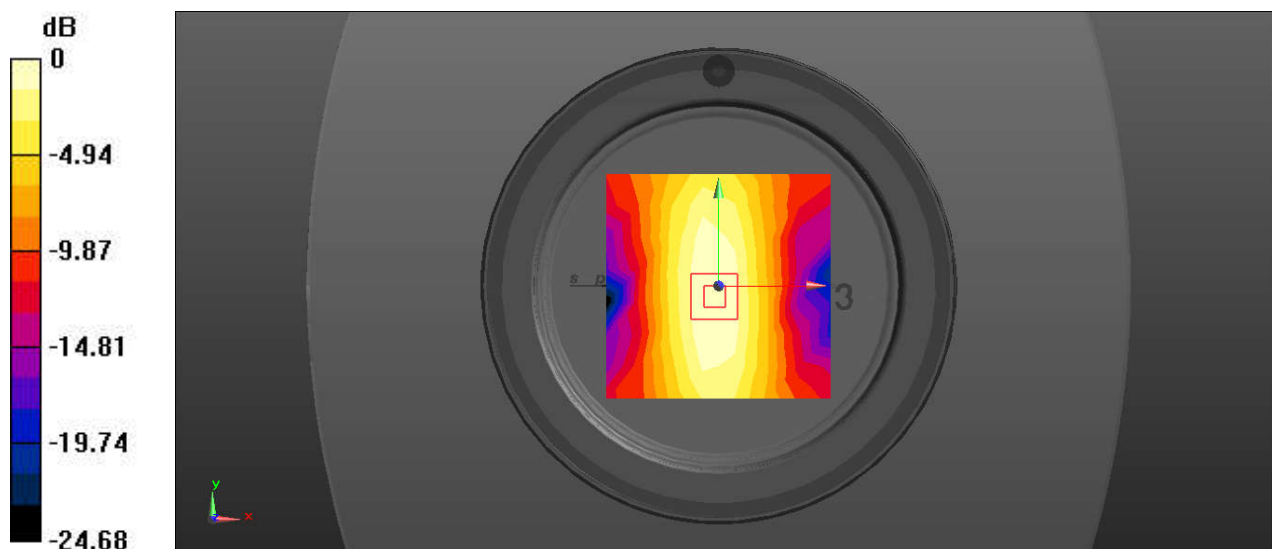

Measurement Report for Device, , , CW, Channel 0 (835.0 MHz)

Communication System: ; Frequency: 835.0

Medium: HSL. Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 43.1$

DASY8 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(10.29, 10.29, 10.29); Calibrated: 2023-01-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.39 W/kg; SAR (10g) = 1.57 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.14 dB

SAR (1g) = 2.30 W/kg; SAR (10g) = 1.49 W/kg;

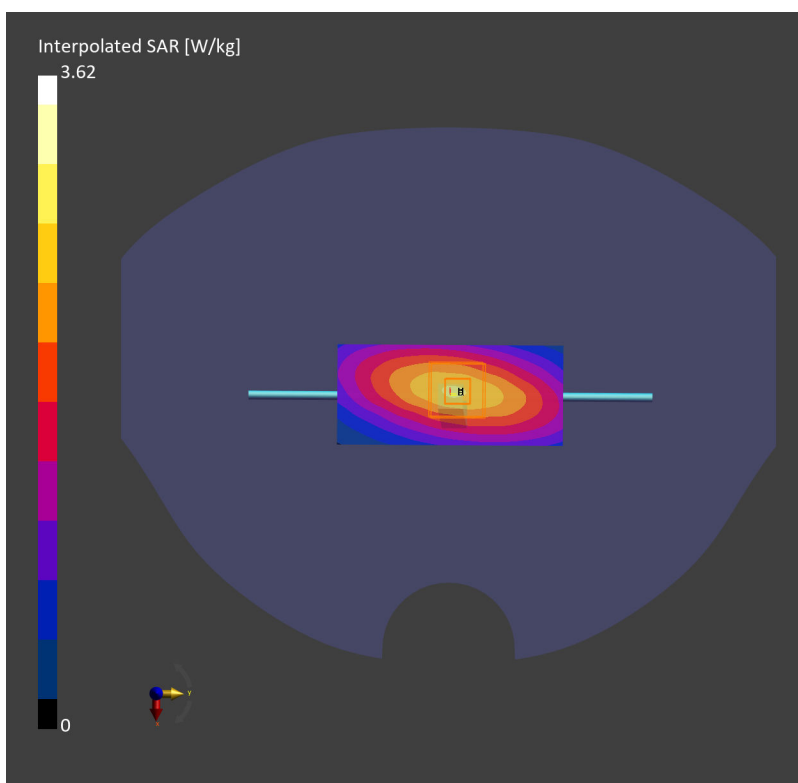

Measurement Report for Device, , , CW, Channel 0 (835.0 MHz)

Communication System: ; Frequency: 835.0

Medium: HSL. Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.930$ S/m; $\epsilon_r = 43.0$

DASY8 Configuration:

- Probe: EX3DV4 - SN7636; ConvF(10.4, 10.4, 10.4); Calibrated: 2023-06-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.51 W/kg; SAR (10g) = 1.65 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.08 dB

SAR (1g) = 2.41 W/kg; SAR (10g) = 1.57 W/kg;

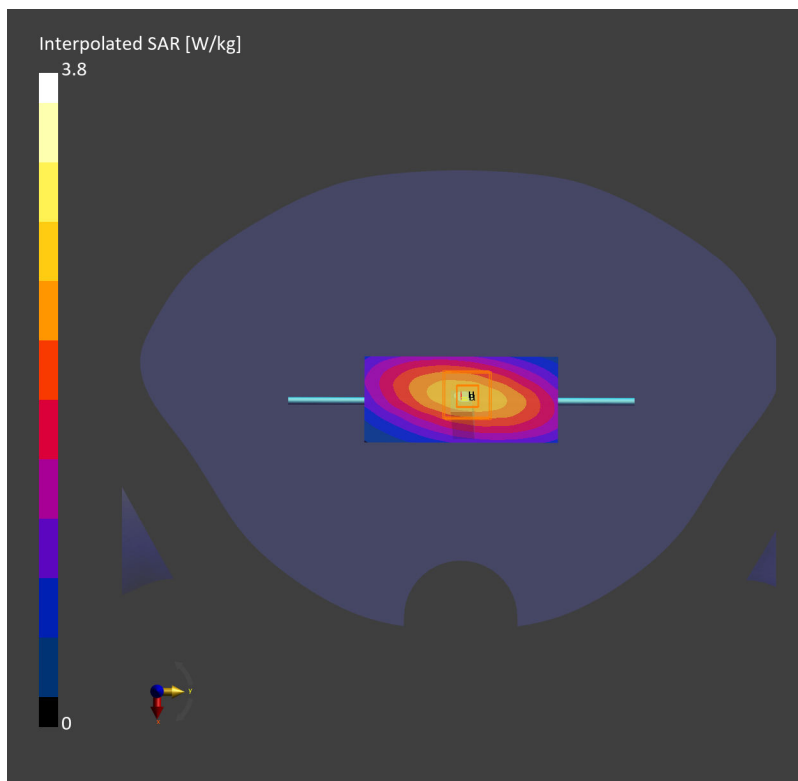

Measurement Report for Device, , CW, Channel 0 (1750.0 MHz)

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 40.4$

DASY8 Configuration:

- Probe: EX3DV4 - SN3793; ConvF(8.17, 8.17, 8.17); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.46 W/kg; SAR (10g) = 5.07 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.18 dB

SAR (1g) = 9.16 W/kg; SAR (10g) = 4.89 W/kg;

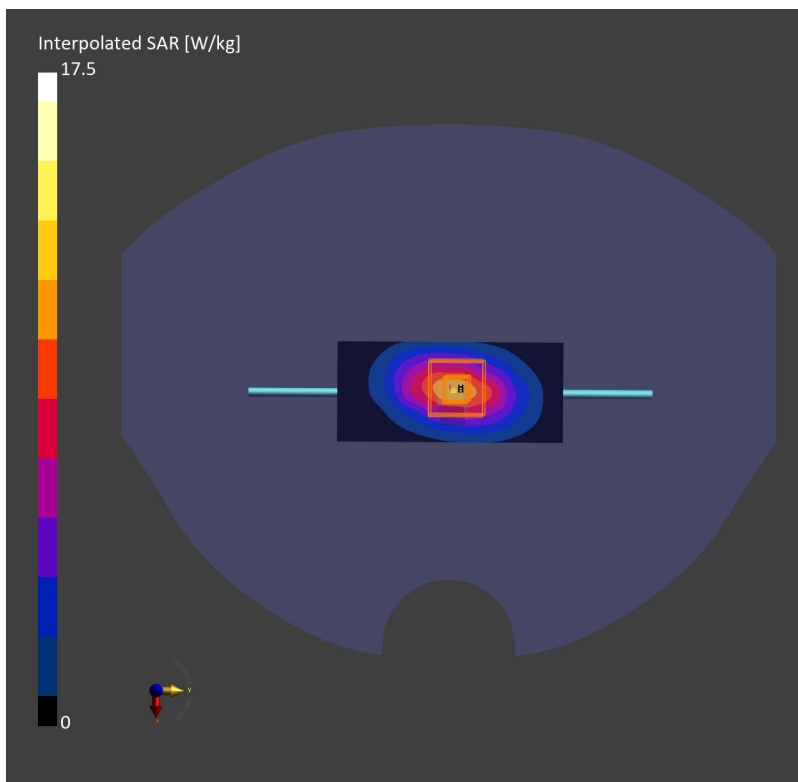

Measurement Report for Device, , CW, Channel 0 (1750.0 MHz)

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 40.5$

DASY8 Configuration:

- Probe: EX3DV4 - SN3793; ConvF(8.17, 8.17, 8.17); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.04 W/kg; SAR (10g) = 4.73 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 9.01 W/kg; SAR (10g) = 4.68 W/kg;

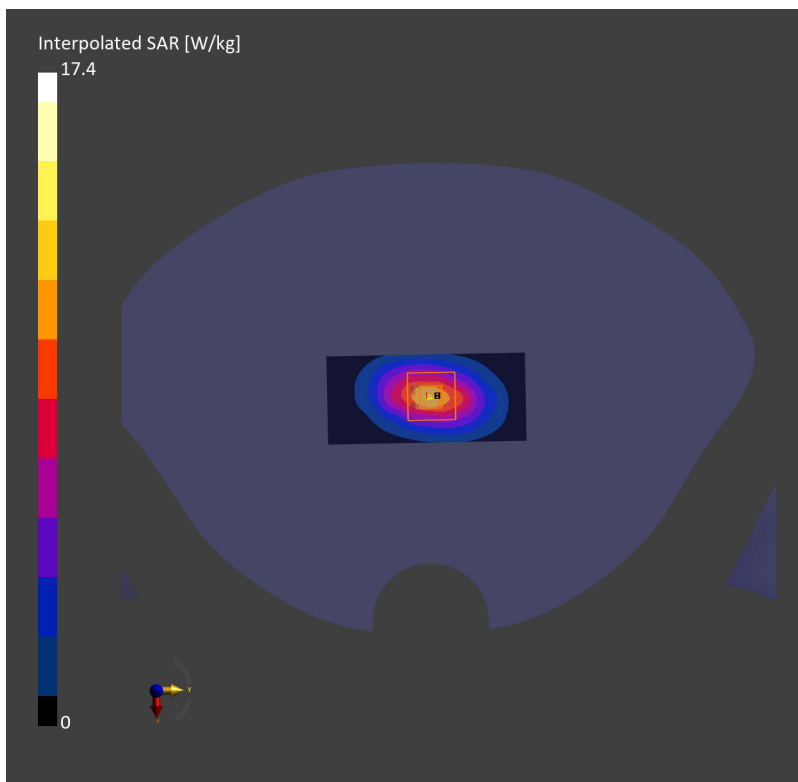

Measurement Report for Device, , , CW, Channel 0 (1750.0 MHz)

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.33$ S/m; $\epsilon_r = 39.6$

DASY8 Configuration:

- Probe: EX3DV4 - SN7636; ConvF(8.89, 8.89, 8.89); Calibrated: 2023-06-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.36 W/kg; SAR (10g) = 5.02 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 9.06 W/kg; SAR (10g) = 4.83 W/kg;

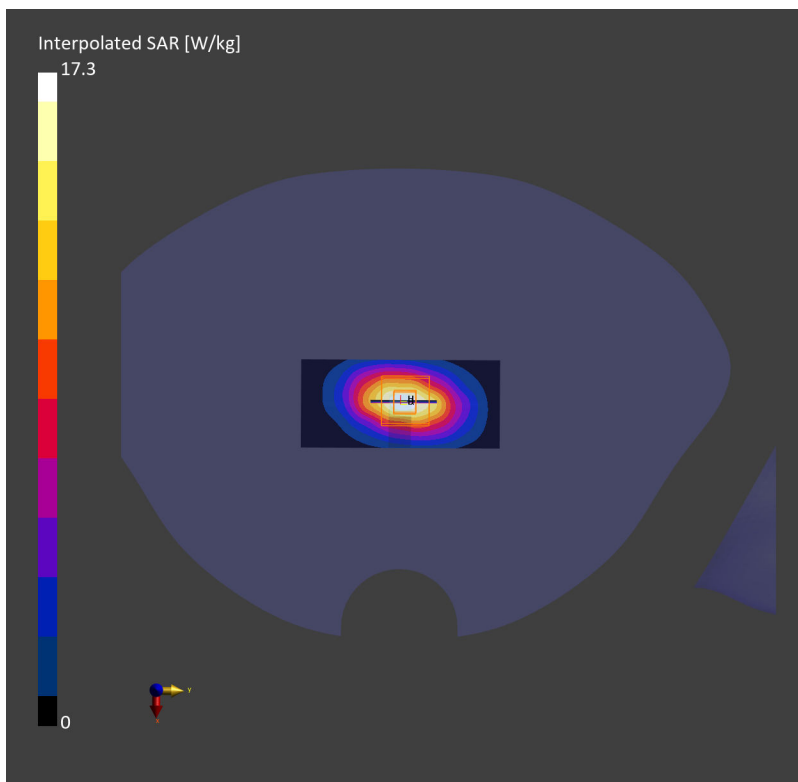

Measurement Report for Device, , , CW, Channel 0 (1900.0 MHz)

Communication System: ; Frequency: 1900.0

Medium: HSL. Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 40.4$

DASY8 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(8.49, 8.49, 8.49); Calibrated: 2023-01-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.62 W/kg; SAR (10g) = 4.95 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.04 dB

SAR (1g) = 9.30 W/kg; SAR (10g) = 4.82 W/kg;

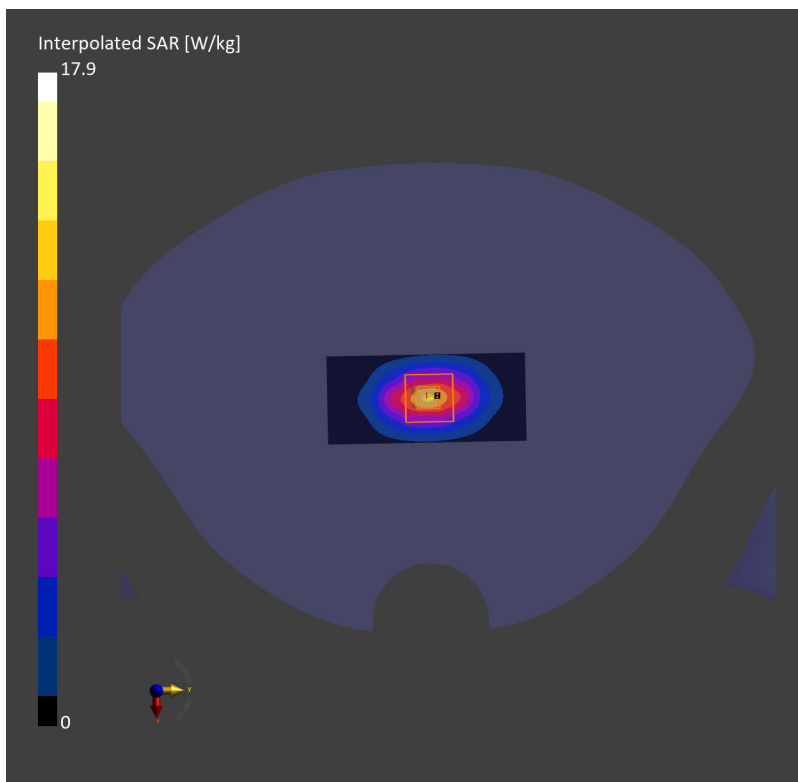

Measurement Report for Device, , , CW, Channel 0 (1900.0 MHz)

Communication System: ; Frequency: 1900.0

Medium: HSL. Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 40.3$

DASY8 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(8.49, 8.49, 8.49); Calibrated: 2023-01-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 9.53 W/kg; SAR (10g) = 4.94 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.17 dB

SAR (1g) = 9.25 W/kg; SAR (10g) = 4.75 W/kg;

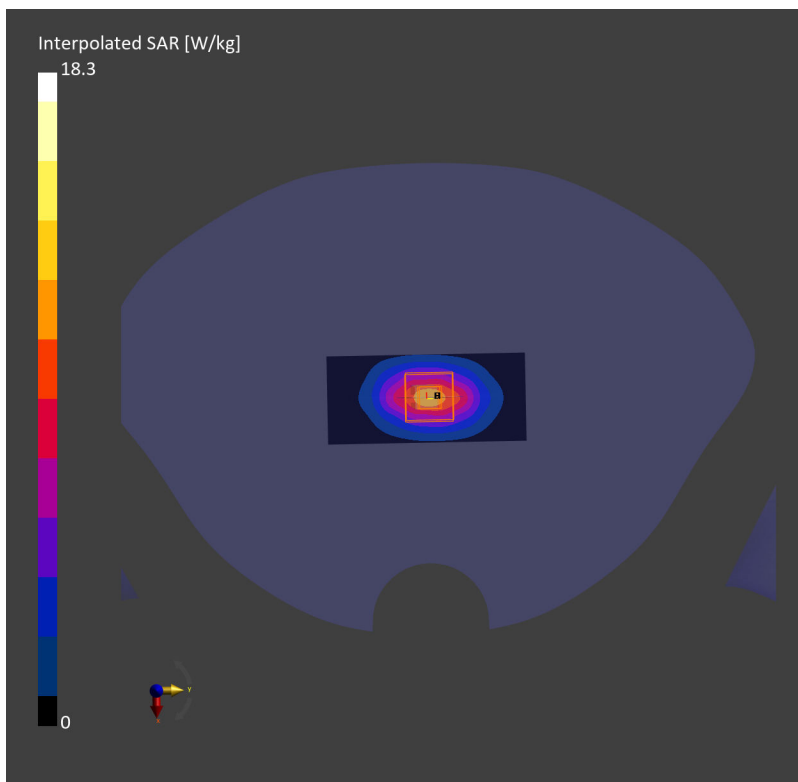

Measurement Report for Device, , CW, Channel 0 (2600.0 MHz)

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.96$ S/m; $\epsilon_r = 37.8$

DASY8 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(7.71, 7.71, 7.71); Calibrated: 2023-01-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (100.0 mm x 140.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 14.0 W/kg; SAR (10g) = 6.34 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 13.8 W/kg; SAR (10g) = 6.44 W/kg;

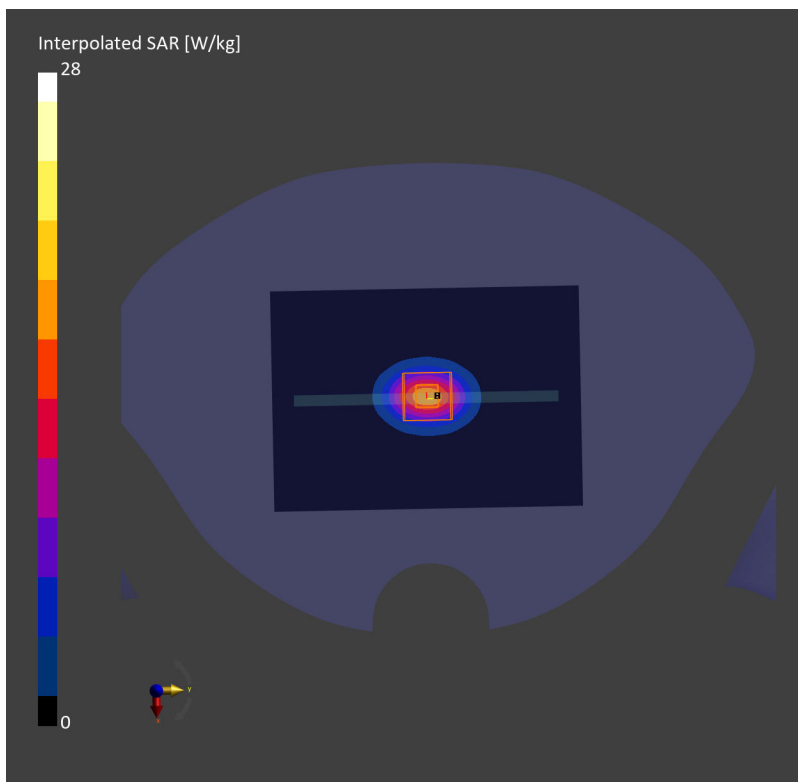

Test Laboratory: SGS-SAR Lab

System Performance Check 2450MHz Head

DUT: D2450V2; Type: Dipole; Serial: 922

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL2450; Medium parameters used: $f = 2450$ MHz; $\sigma = 1.808$ S/m; $\epsilon_r = 39.205$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(7.9, 7.9, 7.9); Calibrated: 2023-01-06
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1374; Calibrated: 2023-06-05
- Phantom: SAM 3; Type: QD000P40CD; Serial: TP:1770
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=250mW/Area Scan (9x10x1): Measurement grid: dx=12mm, dy=12mm
Maximum value of SAR (measured) = 19.3 W/kg


Body/d=10mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 99.74 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 27.1 W/kg

SAR(1 g) = 12.5 W/kg; SAR(10 g) = 5.75 W/kg

Maximum value of SAR (measured) = 21.6 W/kg

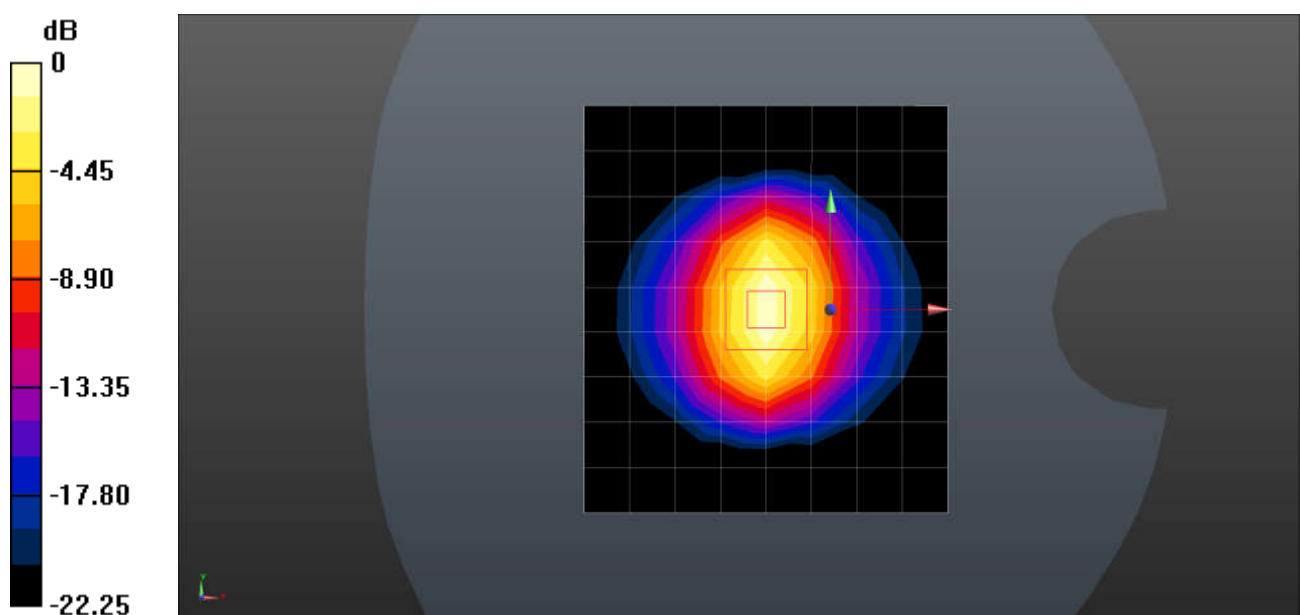

0 dB = 21.6 W/kg = 13.34 dBW/kg

Measurement Report for Device, , , CW, Channel 0 (2600.0 MHz)

Communication System: ; Frequency: 2600.0

Medium: HSL. Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.89$ S/m; $\epsilon_r = 37.1$

DASY8 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(7.71, 7.71, 7.71); Calibrated: 2023-01-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.6 W/kg; SAR (10g) = 6.70 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.17 dB

SAR (1g) = 14.7 W/kg; SAR (10g) = 6.66 W/kg;

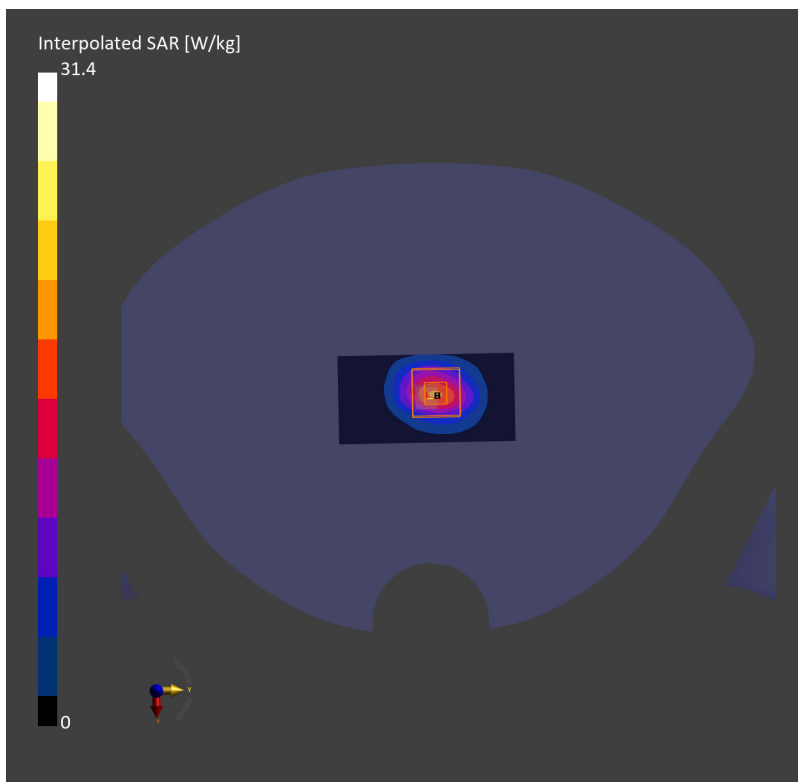

Measurement Report for Device, , , CW, Channel 0 (3500.0 MHz)

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used: $f = 3500.0$ MHz; $\sigma = 3.01$ S/m; $\epsilon_r = 38.0$

DASY8 Configuration:

- Probe: EX3DV4 - SN3793; ConvF(6.77, 6.77, 6.77); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.11 W/kg; SAR (10g) = 2.37 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.09 dB

SAR (1g) = 6.06 W/kg; SAR (10g) = 2.33 W/kg;

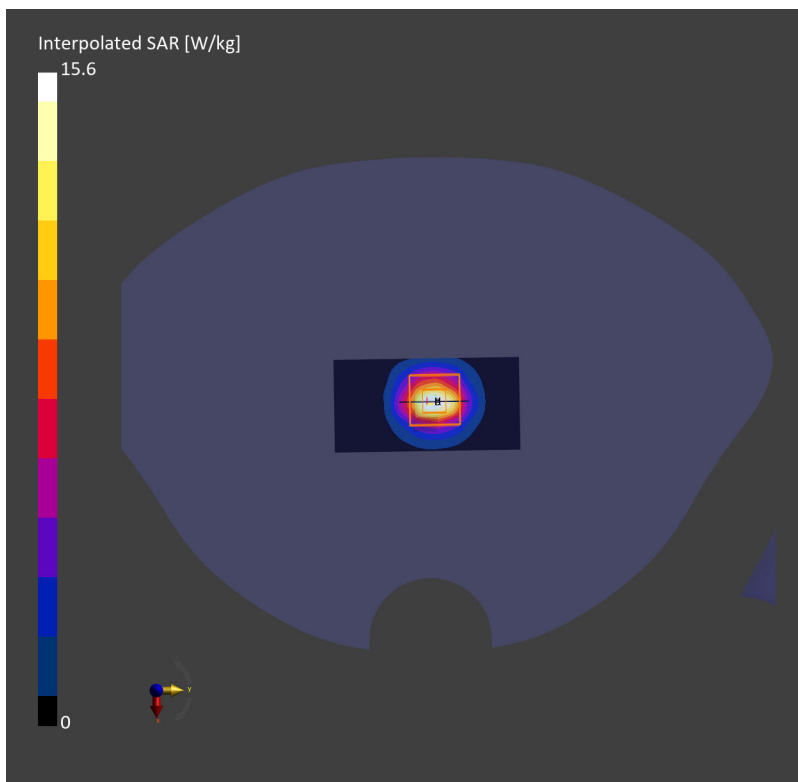

Measurement Report for Device, , , CW, Channel 0 (3500.0 MHz)

Communication System: ; Frequency: 3500.0

Medium: HSL. Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.99$ S/m; $\epsilon_r = 38.6$

DASY8 Configuration:

- Probe: EX3DV4 - SN7636; ConvF(7.20, 7.20, 7.20); Calibrated: 2023-06-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.07 W/kg; SAR (10g) = 2.35 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.11 dB

SAR (1g) = 6.14 W/kg; SAR (10g) = 2.36 W/kg;

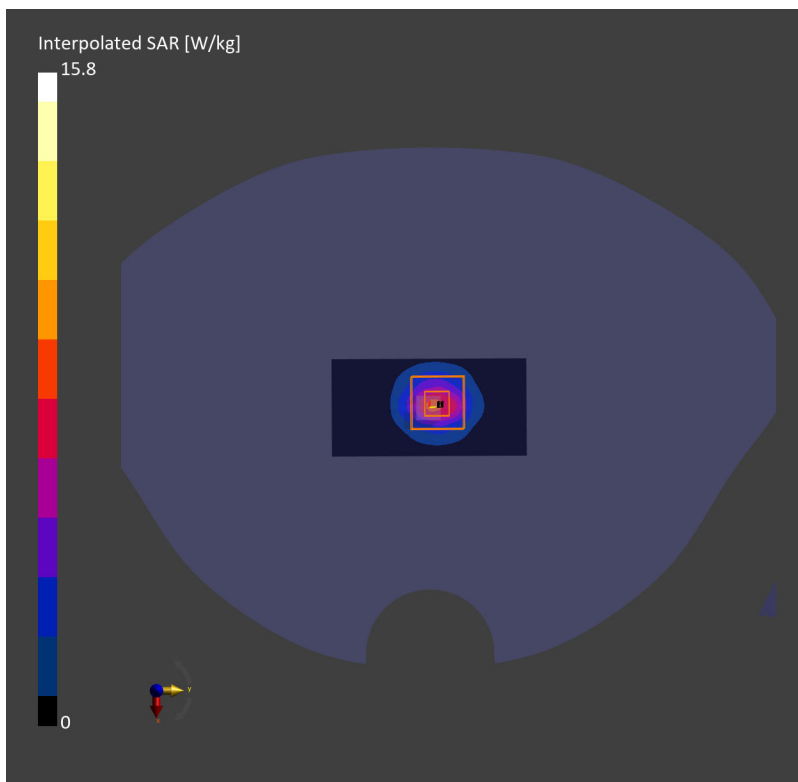

Measurement Report for Device, , , CW, Channel 0 (3700.0 MHz)

Communication System: ; Frequency: 3700.0

Medium: HSL. Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.06$ S/m; $\epsilon_r = 39.4$

DASY8 Configuration:

- Probe: EX3DV4 - SN3793; ConvF(6.48, 6.48, 6.48); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.15 W/kg; SAR (10g) = 2.22 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.11 dB

SAR (1g) = 6.33 W/kg; SAR (10g) = 2.36 W/kg;

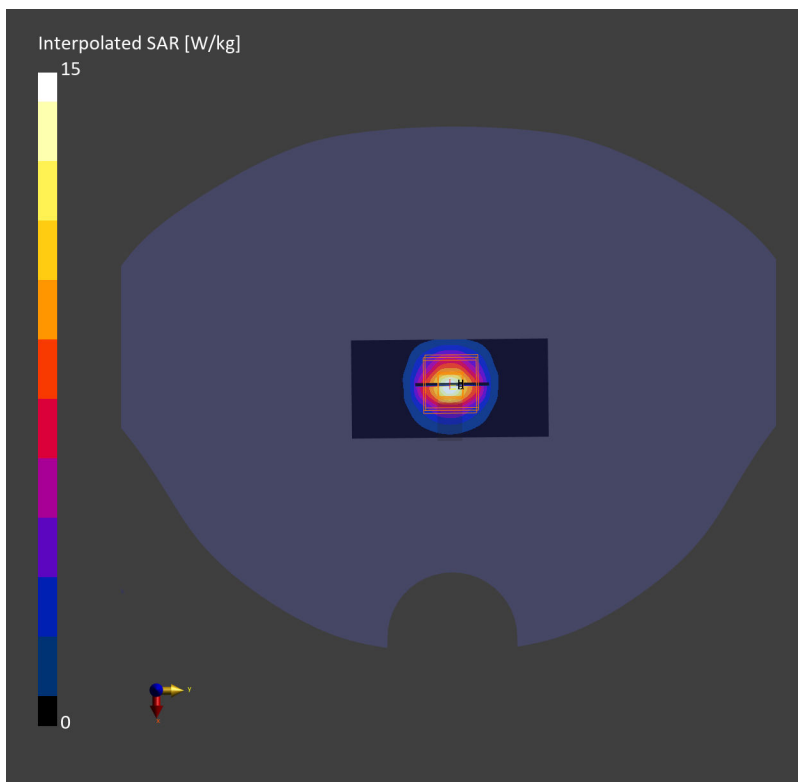

Measurement Report for Device, , , CW, Channel 0 (3700.0 MHz)

Communication System: ; Frequency: 3700.0

Medium: HSL. Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.25$ S/m; $\epsilon_r = 38.4$

DASY8 Configuration:

- Probe: EX3DV4 - SN7636; ConvF(7.00, 7.00, 7.00); Calibrated: 2023-06-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.73 W/kg; SAR (10g) = 2.39 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 6.88 W/kg; SAR (10g) = 2.45 W/kg;

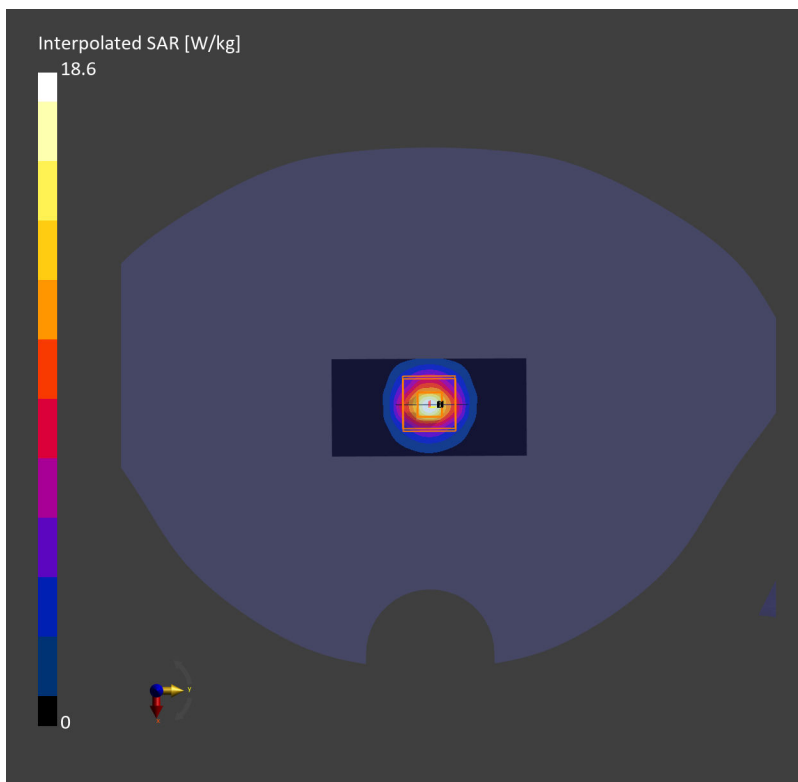

Measurement Report for Device, , , CW, Channel 0 (3900.0 MHz)

Communication System: ; Frequency: 3900.0

Medium: HSL. Medium parameters used: $f = 3900.0$ MHz; $\sigma = 3.28$ S/m; $\epsilon_r = 39.1$

DASY8 Configuration:

- Probe: EX3DV4 - SN3793; ConvF(6.19, 6.19, 6.19); Calibrated: 2022-09-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1484; Calibrated: 2023-06-05
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2103
- Measurement Software: cDASY8 V16.2.0.1425


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.40 W/kg; SAR (10g) = 2.27 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 6.54 W/kg; SAR (10g) = 2.33 W/kg;

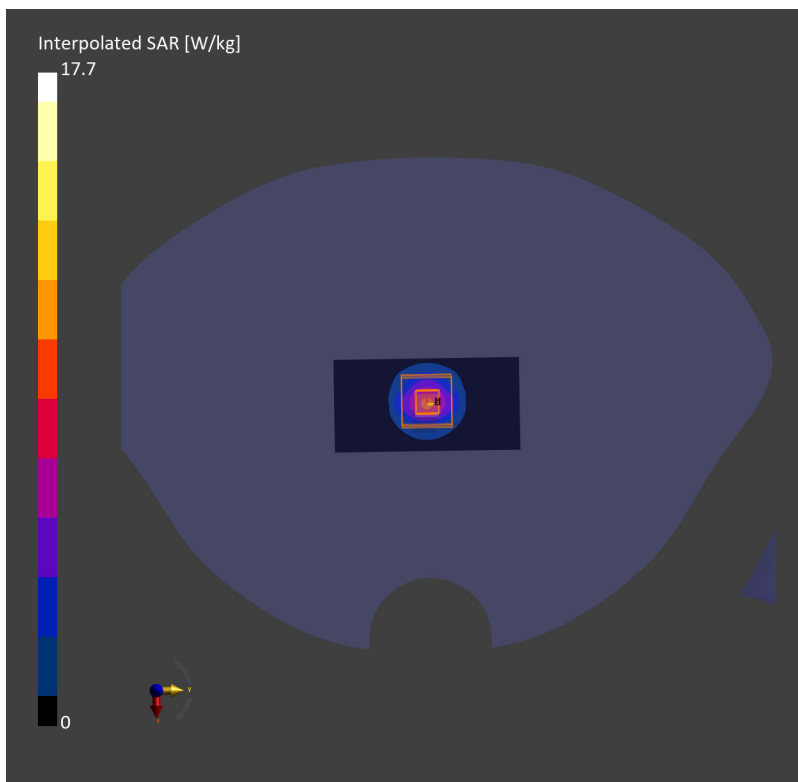

Test Laboratory: SGS-SAR Lab

System Performance Check 5.25GHz Head

DUT: D5GHzV2; Type: Dipole; Serial: 1313

Communication System: UID 0, CW (0); Frequency: 5250 MHz; Duty Cycle: 1:1

Medium: HSL5G; Medium parameters used: $f = 5250$ MHz; $\sigma = 4.59$ S/m; $\epsilon_r = 35.818$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(5.65, 5.65, 5.65); Calibrated: 2023-01-06
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1374; Calibrated: 2023-06-05
- Phantom: SAM 3; Type: QD000P40CD; Serial: TP:1770
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=100mW, f=5250 MHz/Area Scan (8x8x1): Measurement grid:

dx=10mm, dy=10mm

Maximum value of SAR (measured) = 15.5 W/kg

Body/d=10mm, Pin=100mW, f=5250 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement


grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 73.69 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 33.8 W/kg

SAR(1 g) = 7.24 W/kg; SAR(10 g) = 2.08 W/kg

Maximum value of SAR (measured) = 19.8 W/kg

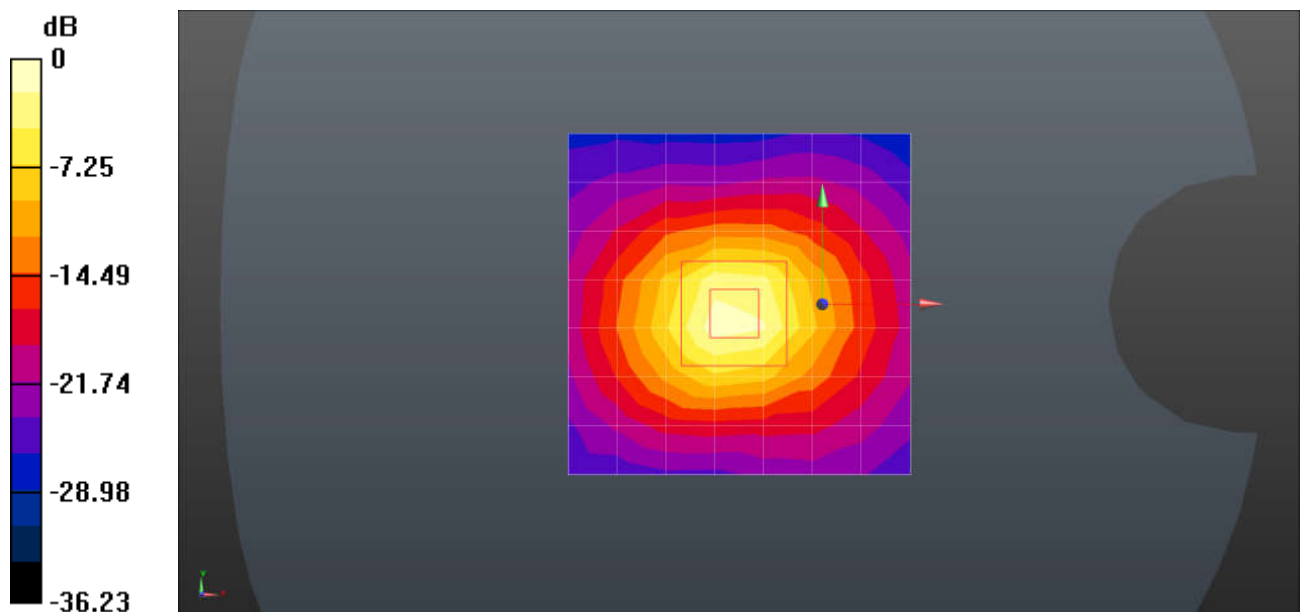

0 dB = 19.8 W/kg = 12.97 dBW/kg

Test Laboratory: SGS-SAR Lab

System Performance Check 5.6GHz Head

DUT: D5GHzV2; Type: Dipole; Serial: 1313

Communication System: UID 0, CW (0); Frequency: 5600 MHz; Duty Cycle: 1:1

Medium: HSL5G; Medium parameters used: $f = 5600$ MHz; $\sigma = 5.055$ S/m; $\epsilon_r = 35.146$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(5.05, 5.05, 5.05); Calibrated: 2023-01-06
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1374; Calibrated: 2023-06-05
- Phantom: SAM 3; Type: QD000P40CD; Serial: TP:1770
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=100mW, f=5600 MHz/Area Scan (8x8x1): Measurement grid:

dx=10mm, dy=10mm

Maximum value of SAR (measured) = 15.6 W/kg

Body/d=10mm, Pin=100mW, f=5600 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement


grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.74 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 35.4 W/kg

SAR(1 g) = 7.24 W/kg; SAR(10 g) = 2.07 W/kg

Maximum value of SAR (measured) = 20.1 W/kg

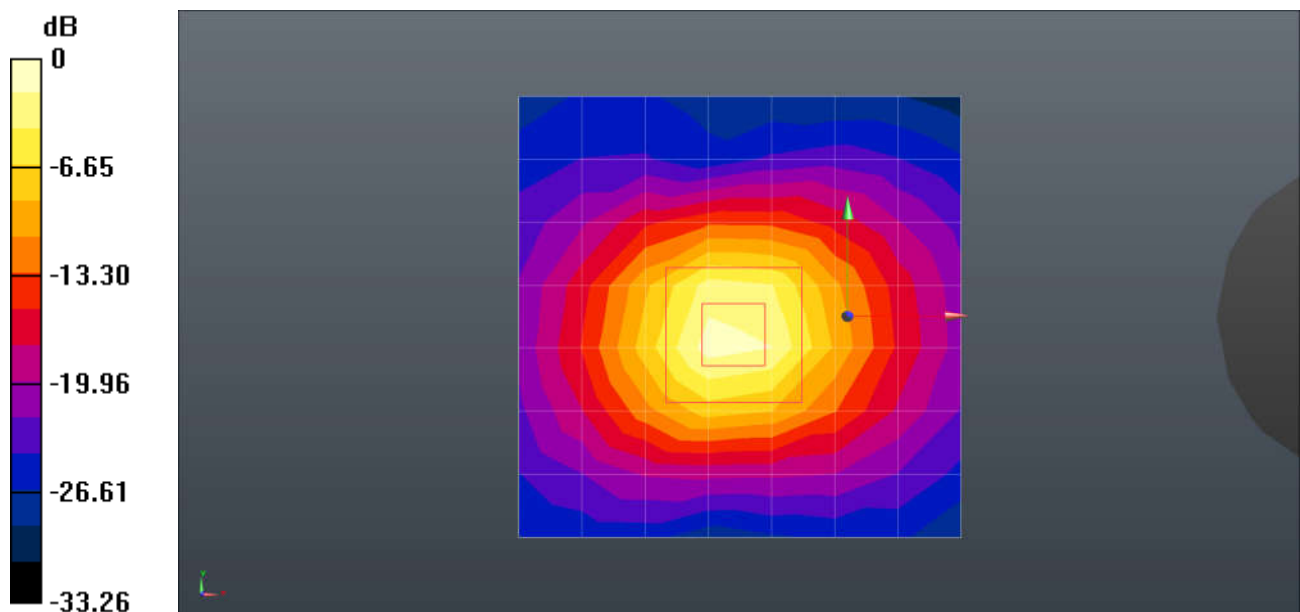

0 dB = 20.1 W/kg = 13.03 dBW/kg

Test Laboratory: SGS-SAR Lab

System Performance Check 5.75GHz Head

DUT: D5GHzV2; Type: Dipole; Serial: 1313

Communication System: UID 0, CW (0); Frequency: 5750 MHz; Duty Cycle: 1:1

Medium: HSL5G; Medium parameters used: $f = 5750$ MHz; $\sigma = 5.235$ S/m; $\epsilon_r = 34.774$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY 5 Configuration:

- Probe: EX3DV4 - SN3982; ConvF(5.15, 5.15, 5.15); Calibrated: 2023-01-06
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1374; Calibrated: 2023-06-05
- Phantom: SAM 3; Type: QD000P40CD; Serial: TP:1770
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Body/d=10mm, Pin=100mW, f=5750 MHz/Area Scan (8x8x1): Measurement grid:

dx=10mm, dy=10mm

Maximum value of SAR (measured) = 15.1 W/kg

Body/d=10mm, Pin=100mW, f=5750 MHz/Zoom Scan (7x7x7)/Cube 0: Measurement


grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 63.61 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 35.6 W/kg

SAR(1 g) = 7.13 W/kg; SAR(10 g) = 2.03 W/kg

Maximum value of SAR (measured) = 19.8 W/kg

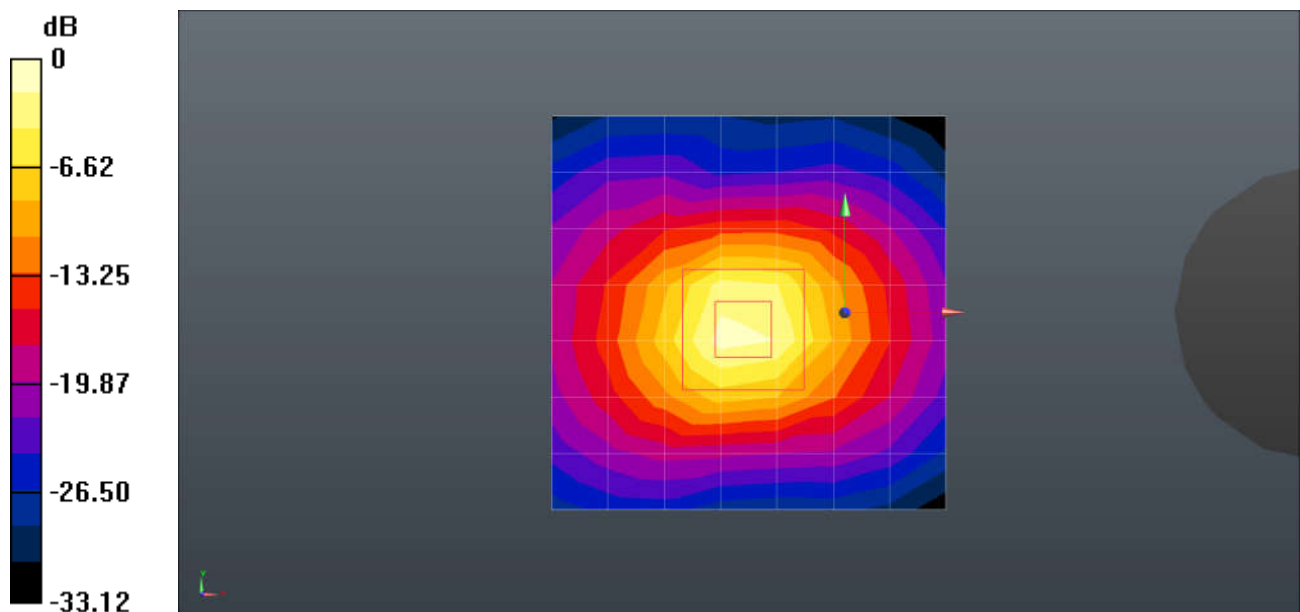

0 dB = 19.8 W/kg = 12.97 dBW/kg